


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110419\
Data File : VN059072.D
Acq On : 4 Nov 2019 8:39
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110119W.M
Title : SW846 8260
Last Update : Sat Nov 02 05:43:23 2019

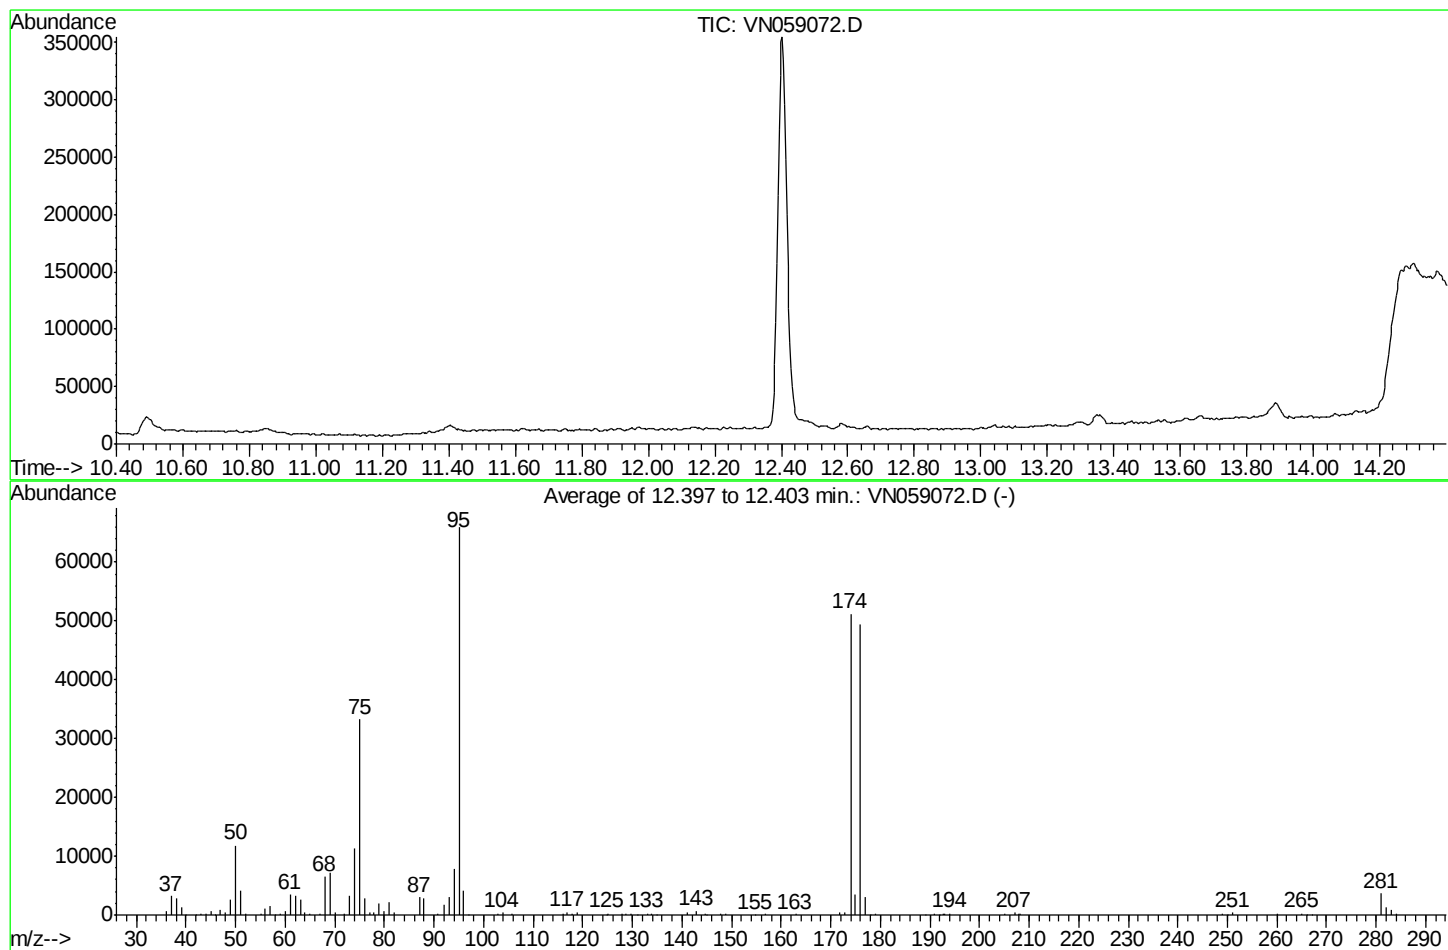

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	11838	PASS
75	95	30	60	50.5	33303	PASS
95	95	100	100	100.0	65946	PASS
96	95	5	9	6.4	4224	PASS
173	174	0.00	2	0.8	388	PASS
174	95	50	100	77.6	51176	PASS
175	174	5	9	7.0	3599	PASS
176	174	95	101	96.6	49429	PASS
177	176	5	9	6.4	3151	PASS