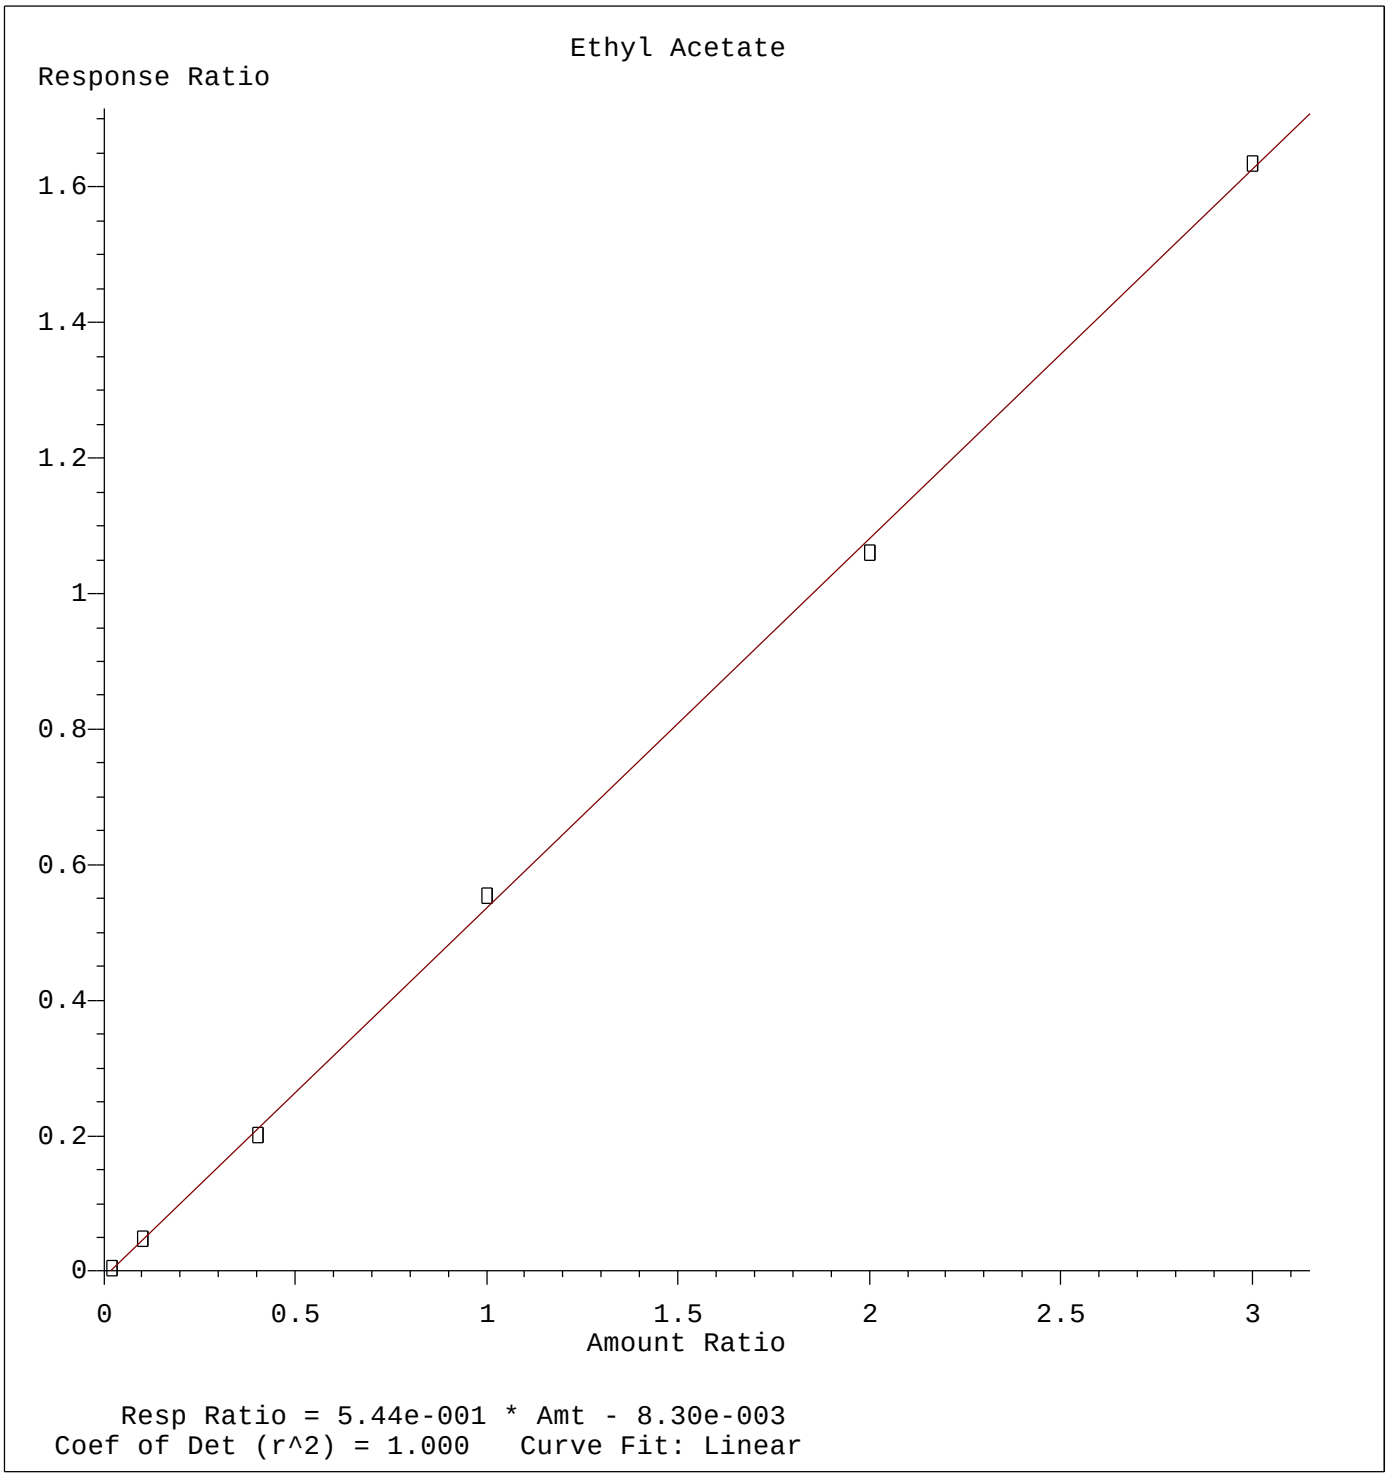

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
Calibration Table Last Updated: Wed Nov 04 12:09:03 2020

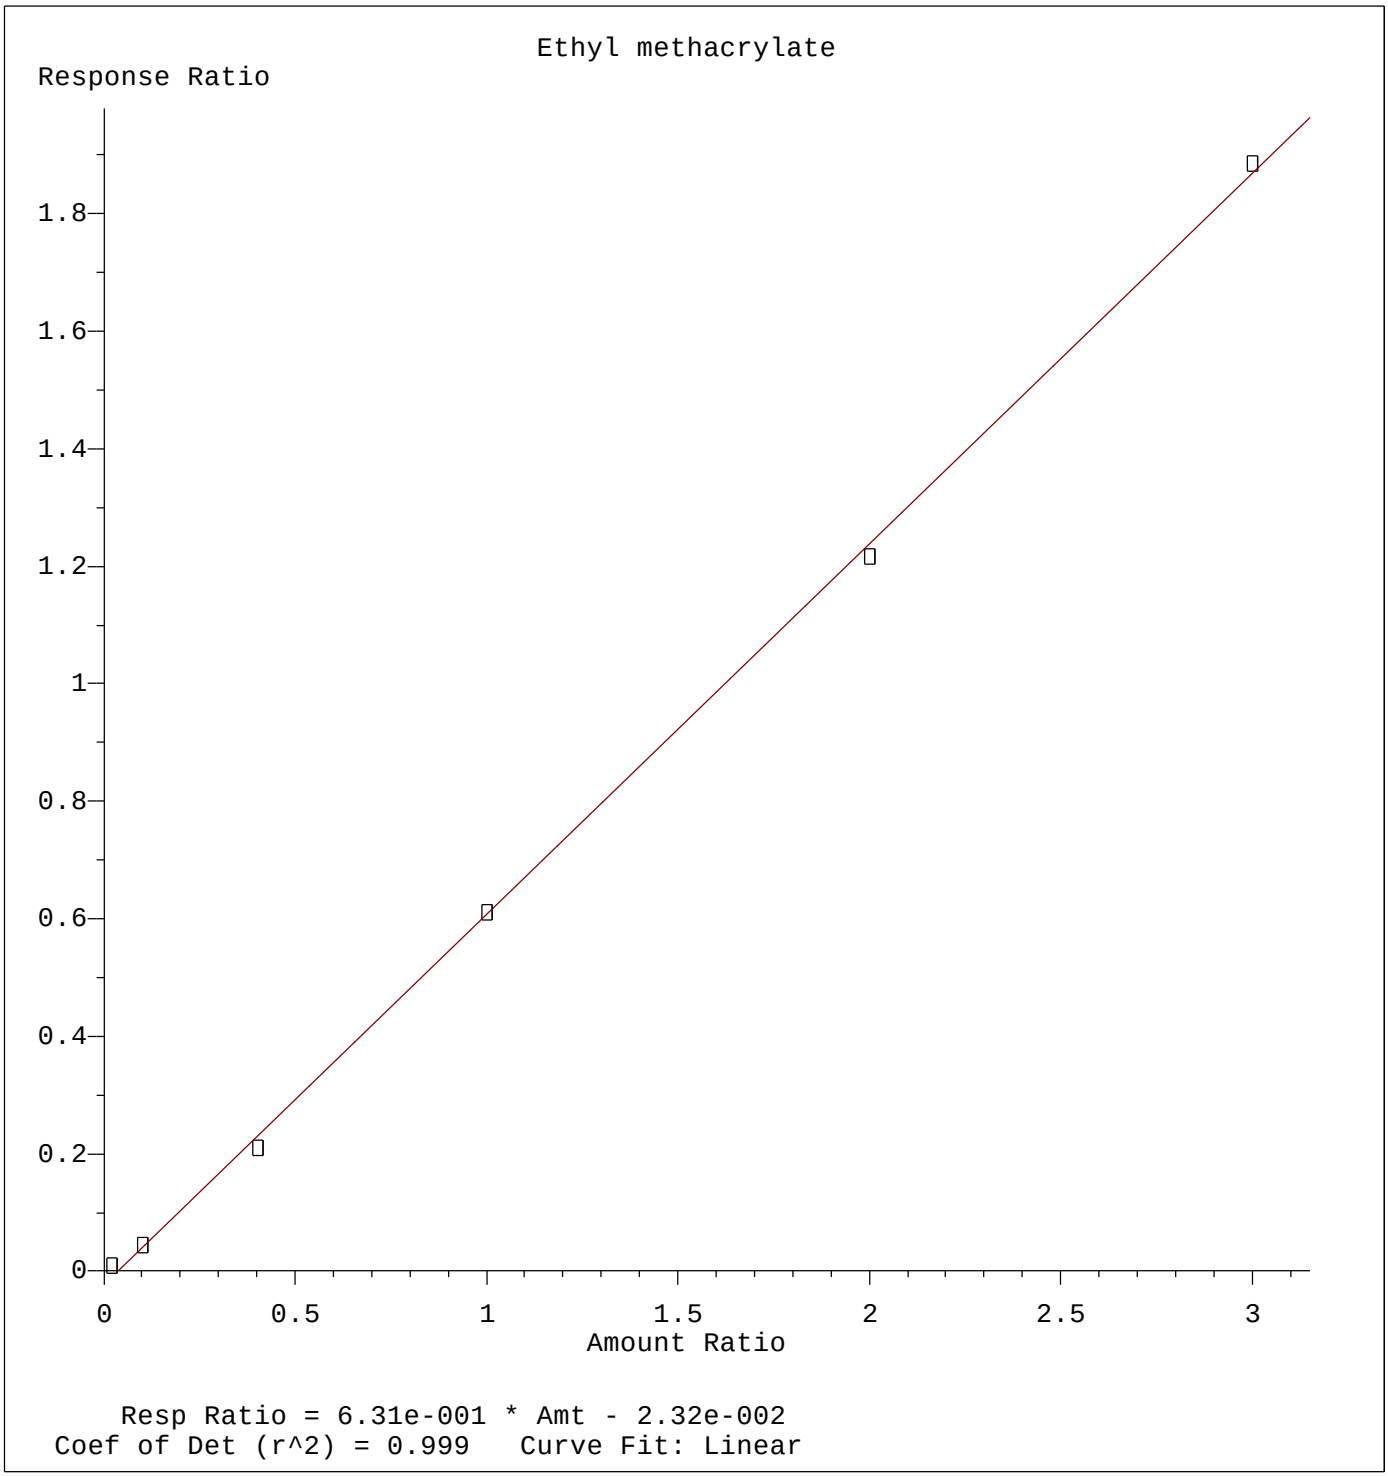

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
Calibration Table Last Updated: Wed Nov 04 12:09:03 2020

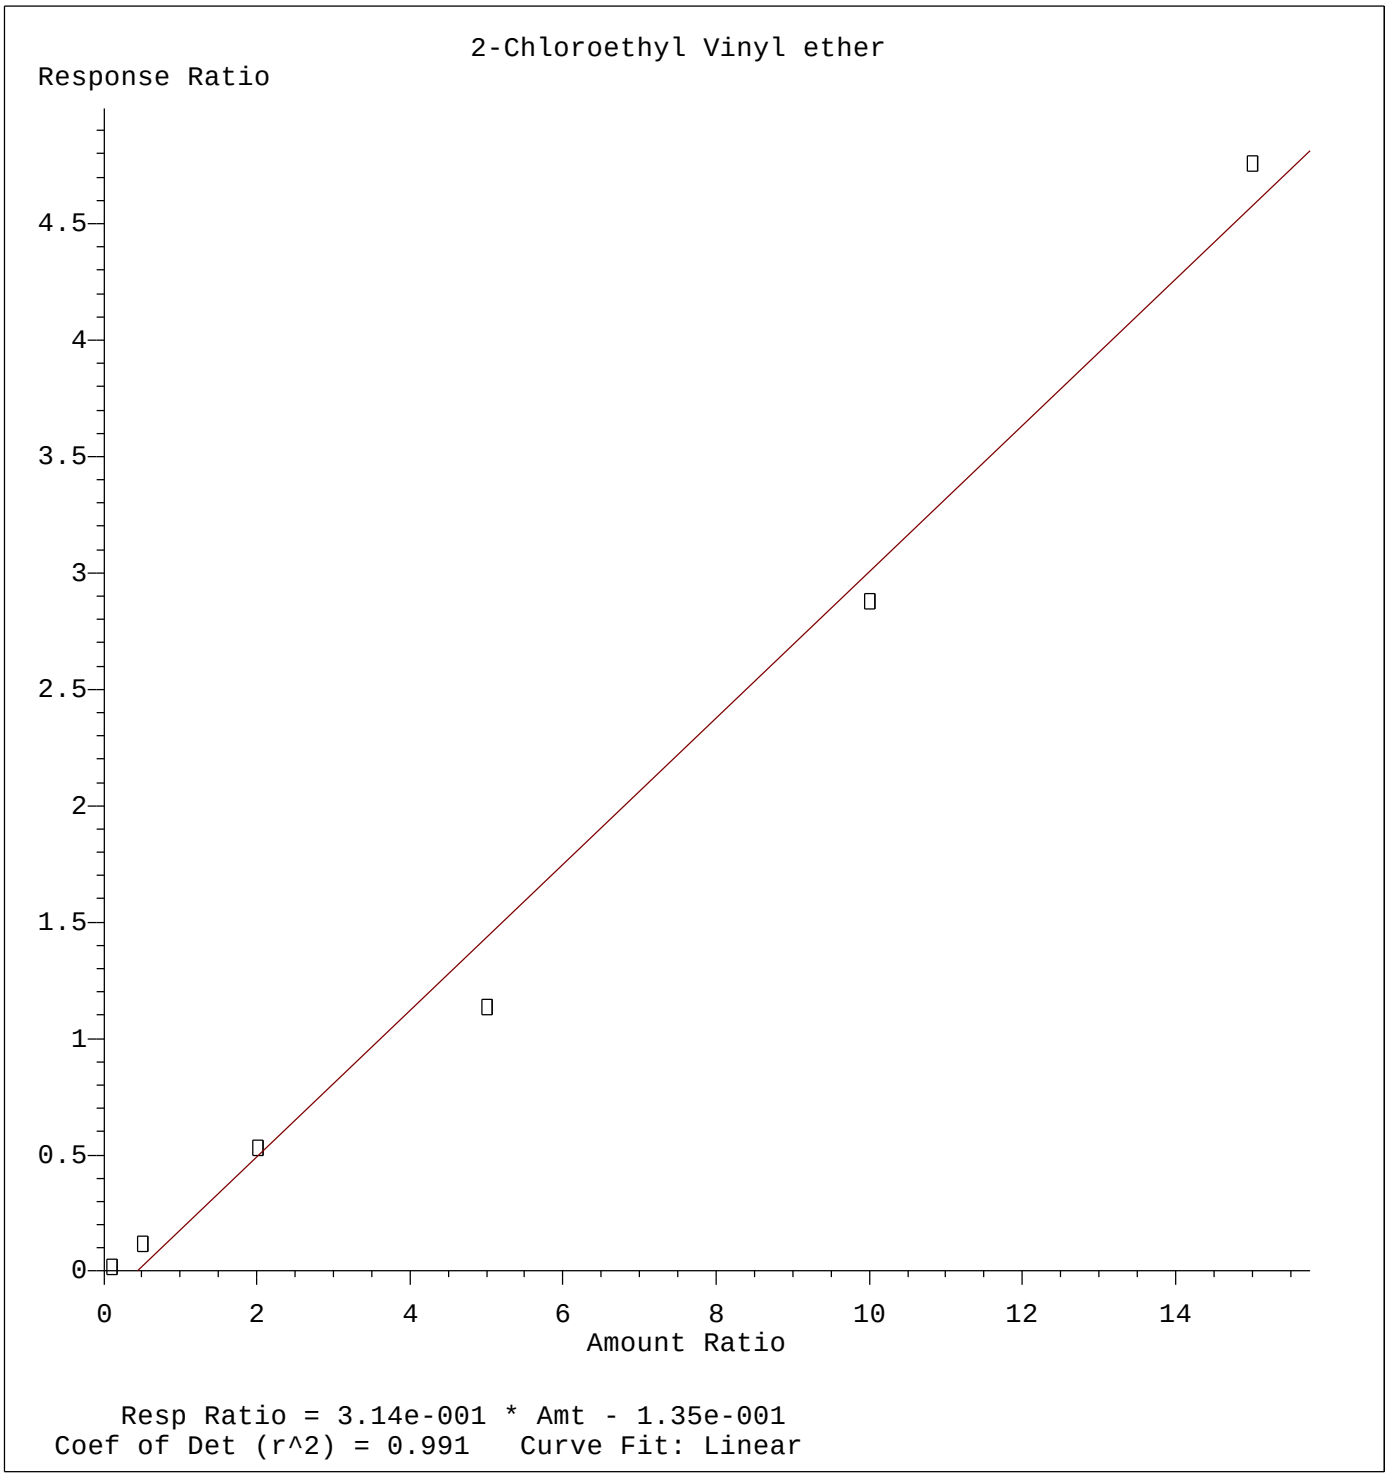

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
Calibration Table Last Updated: Wed Nov 04 12:09:03 2020

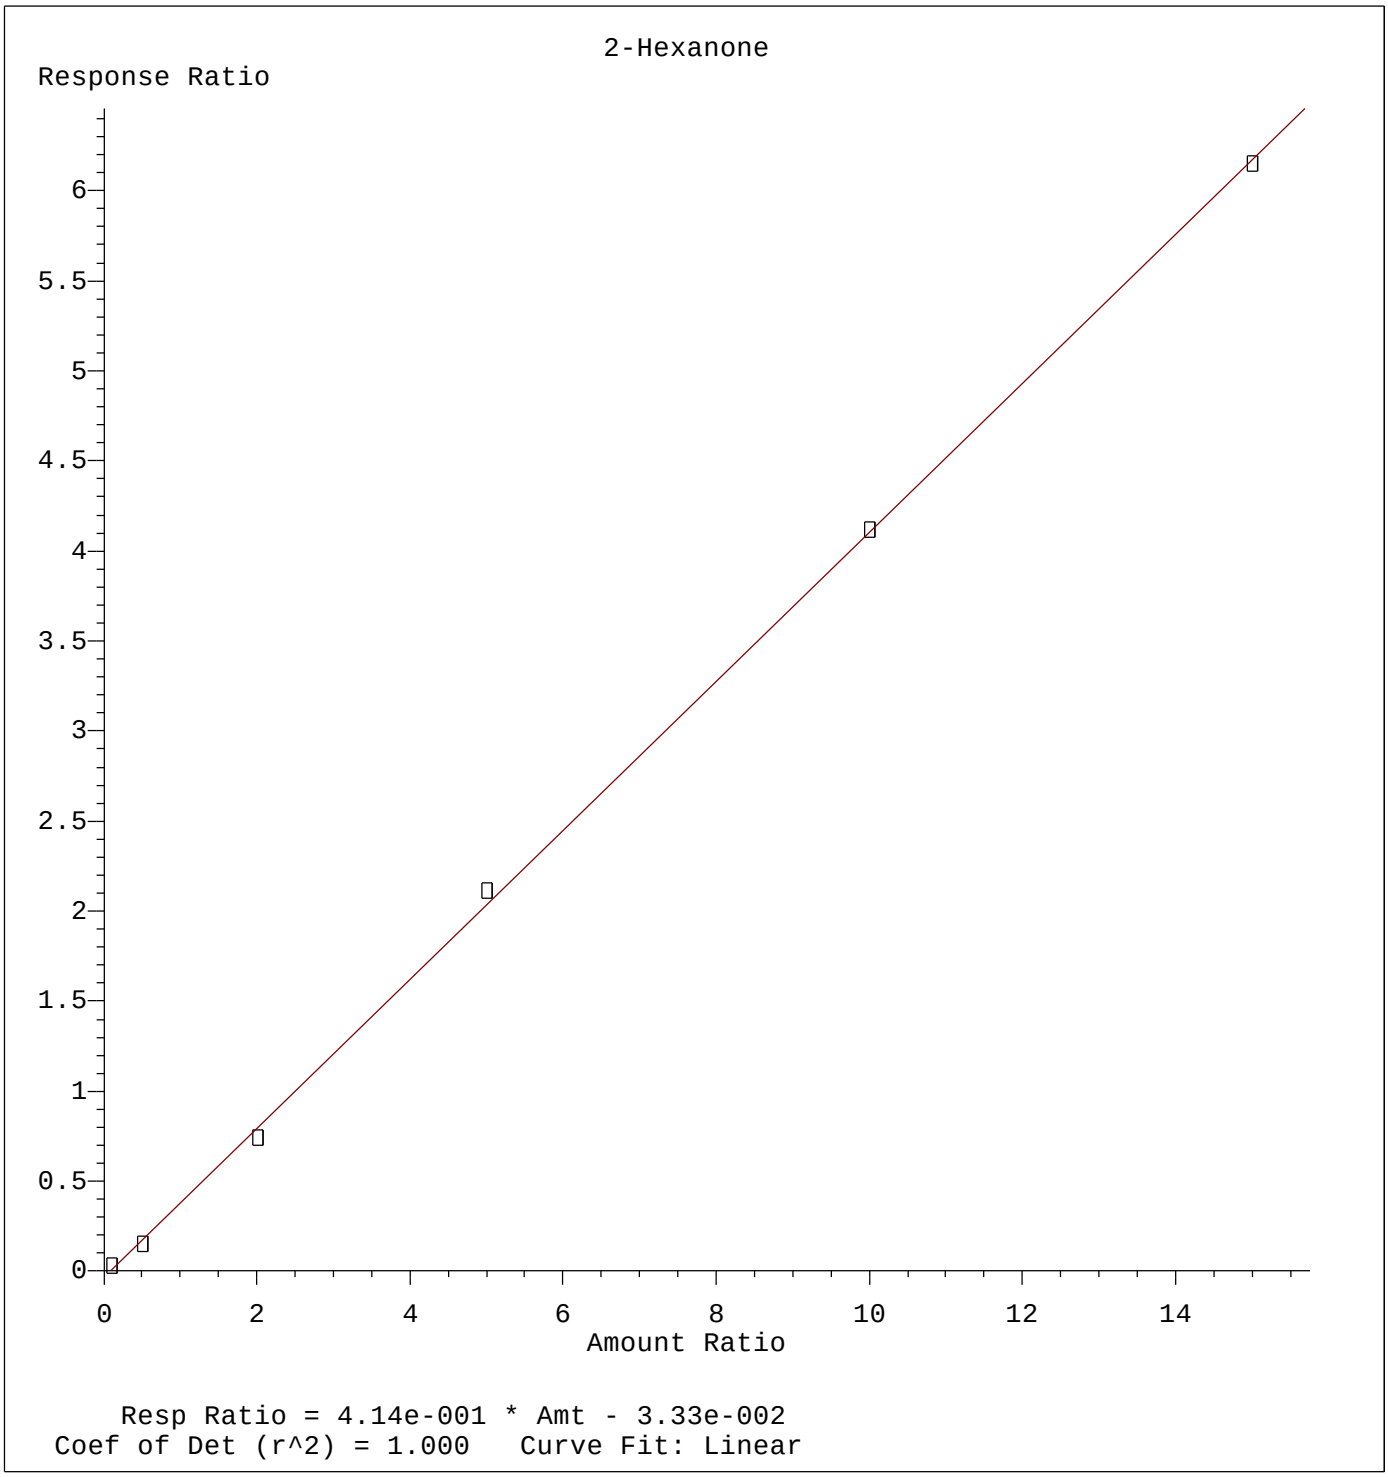

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
Calibration Table Last Updated: Wed Nov 04 12:09:03 2020

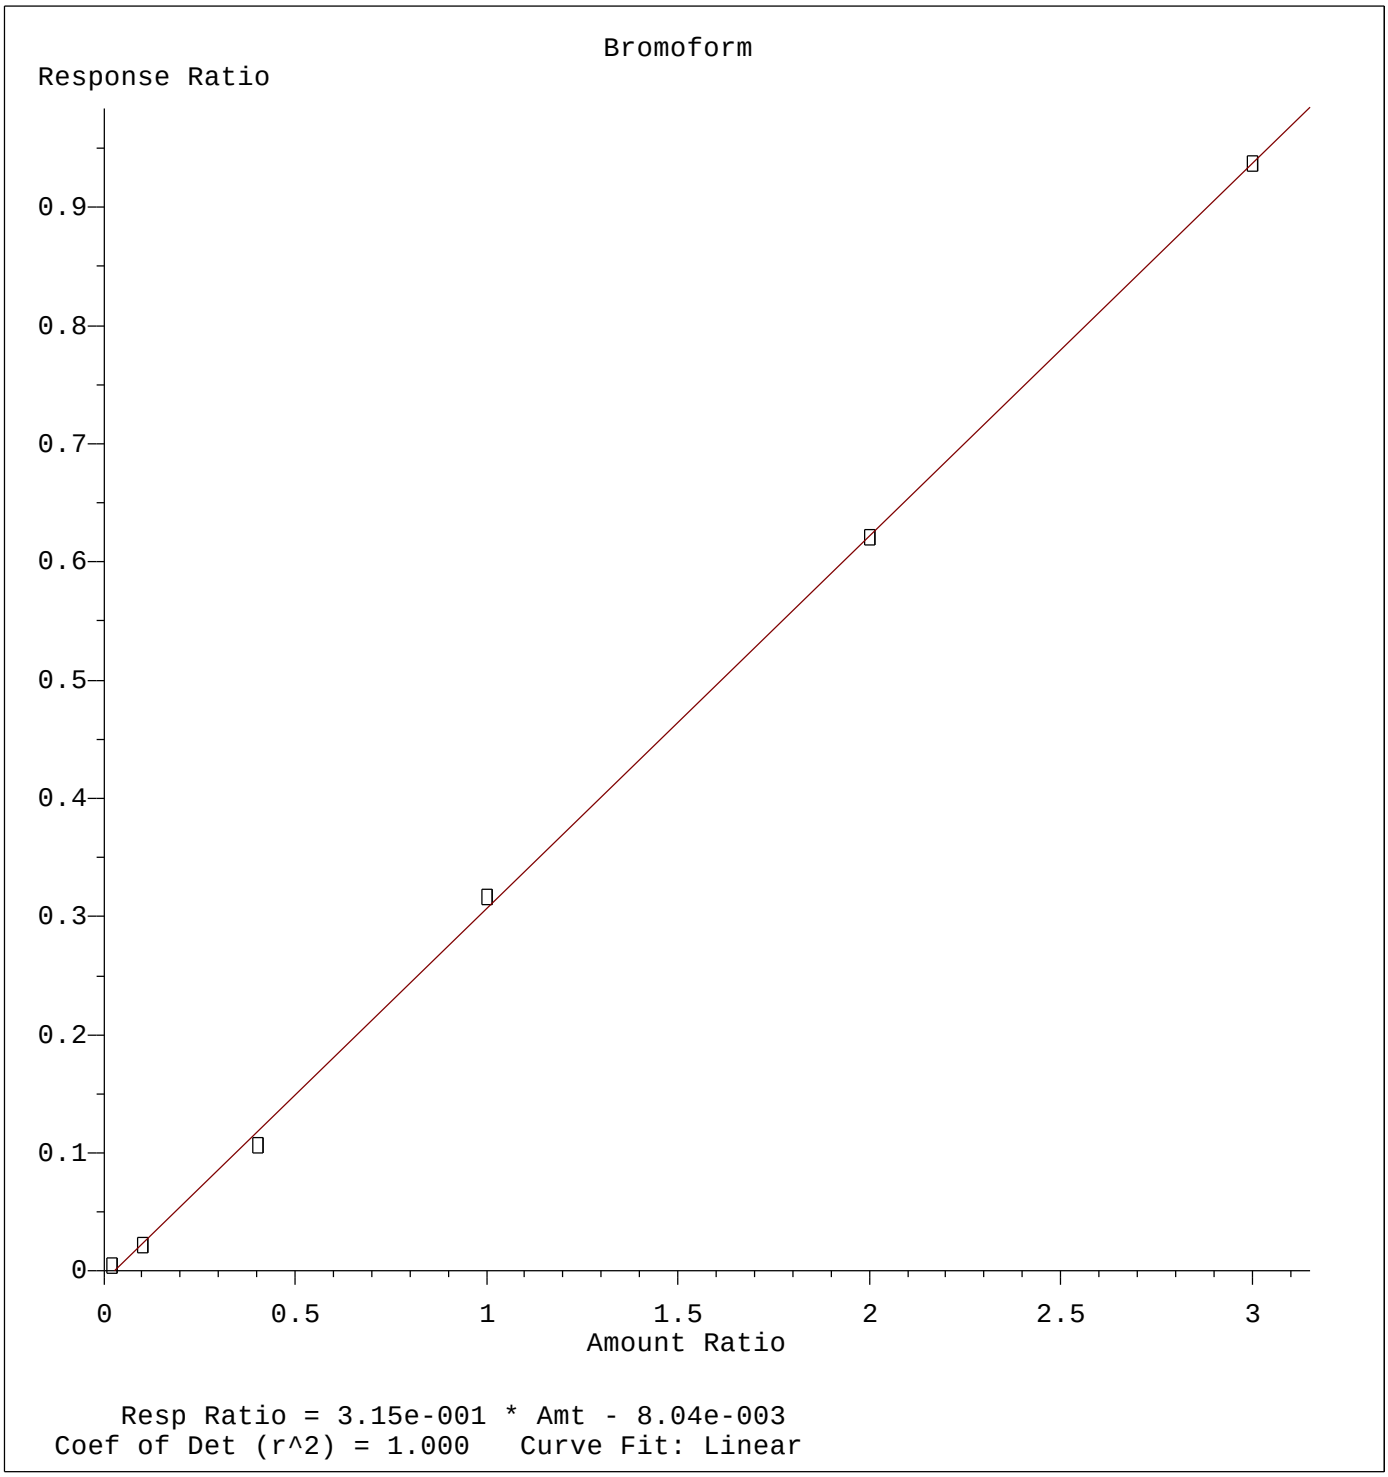

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
Calibration Table Last Updated: Wed Nov 04 12:09:03 2020

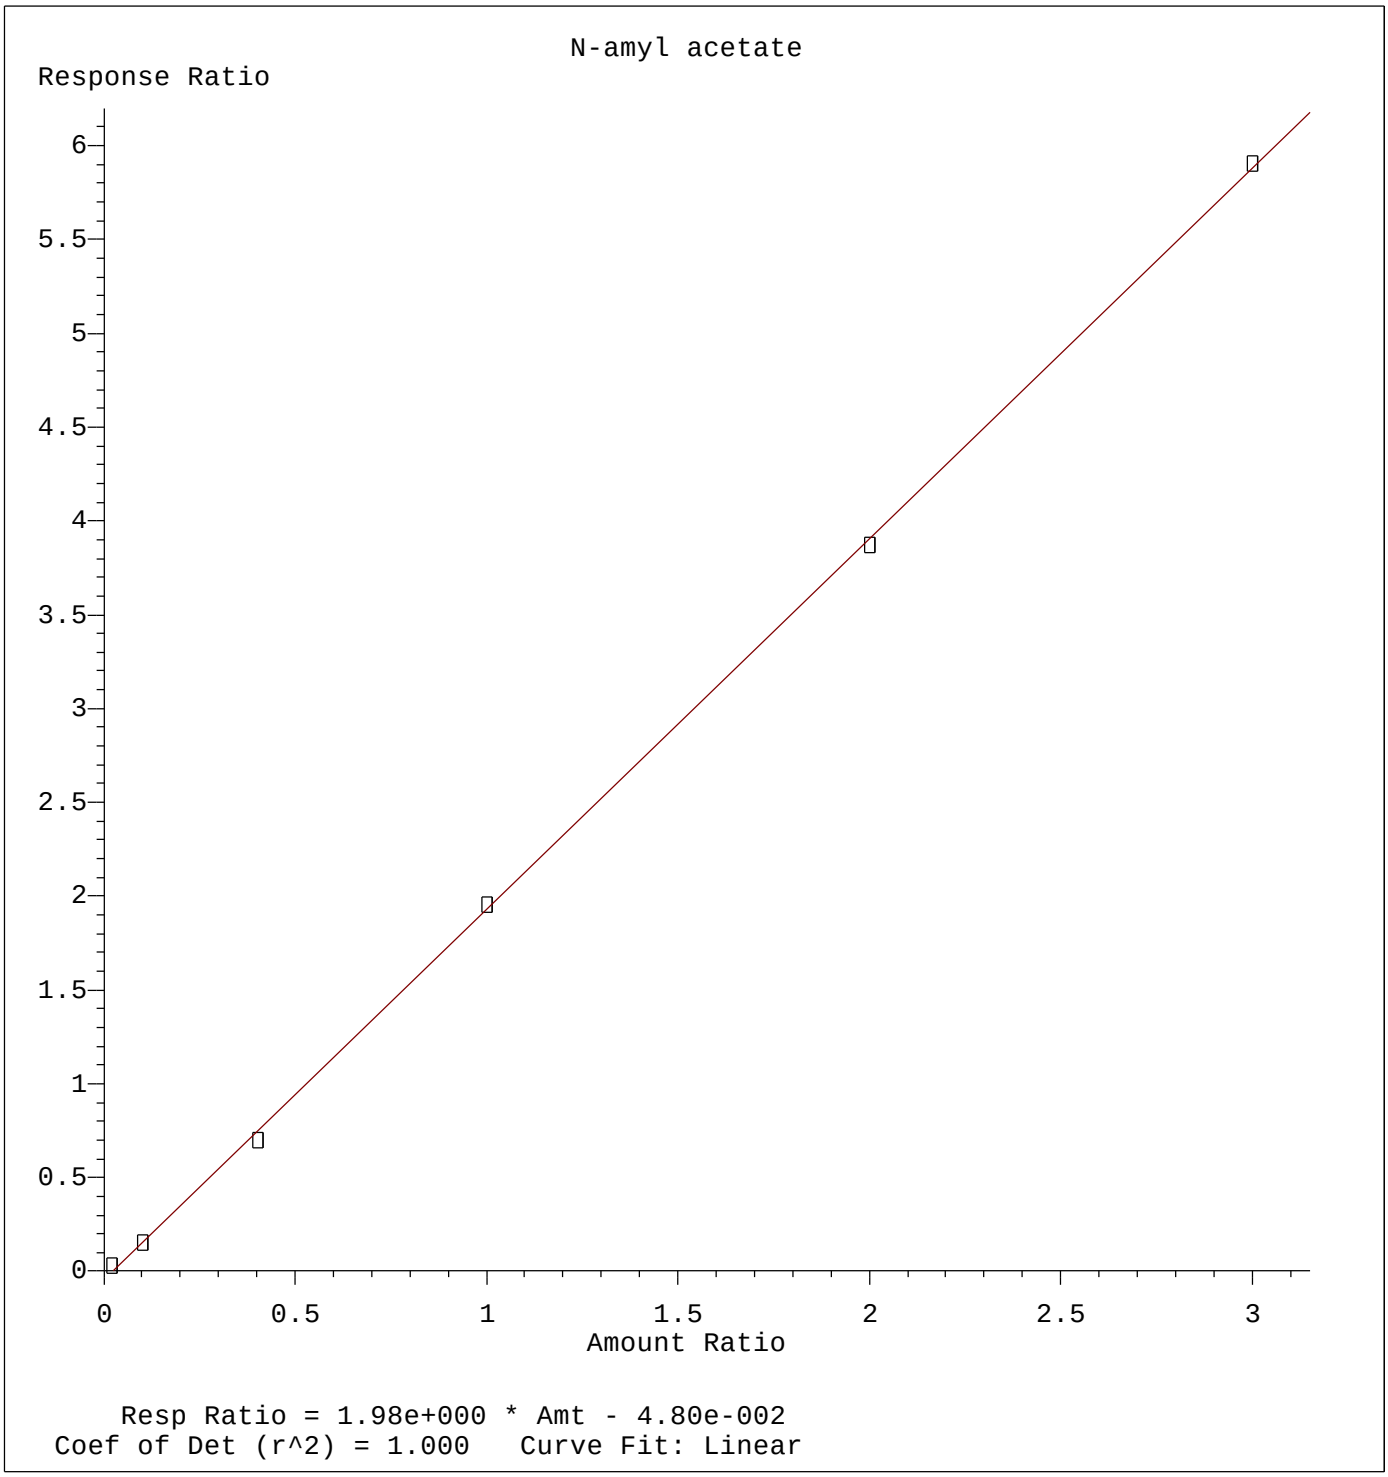

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
Calibration Table Last Updated: Wed Nov 04 12:09:03 2020

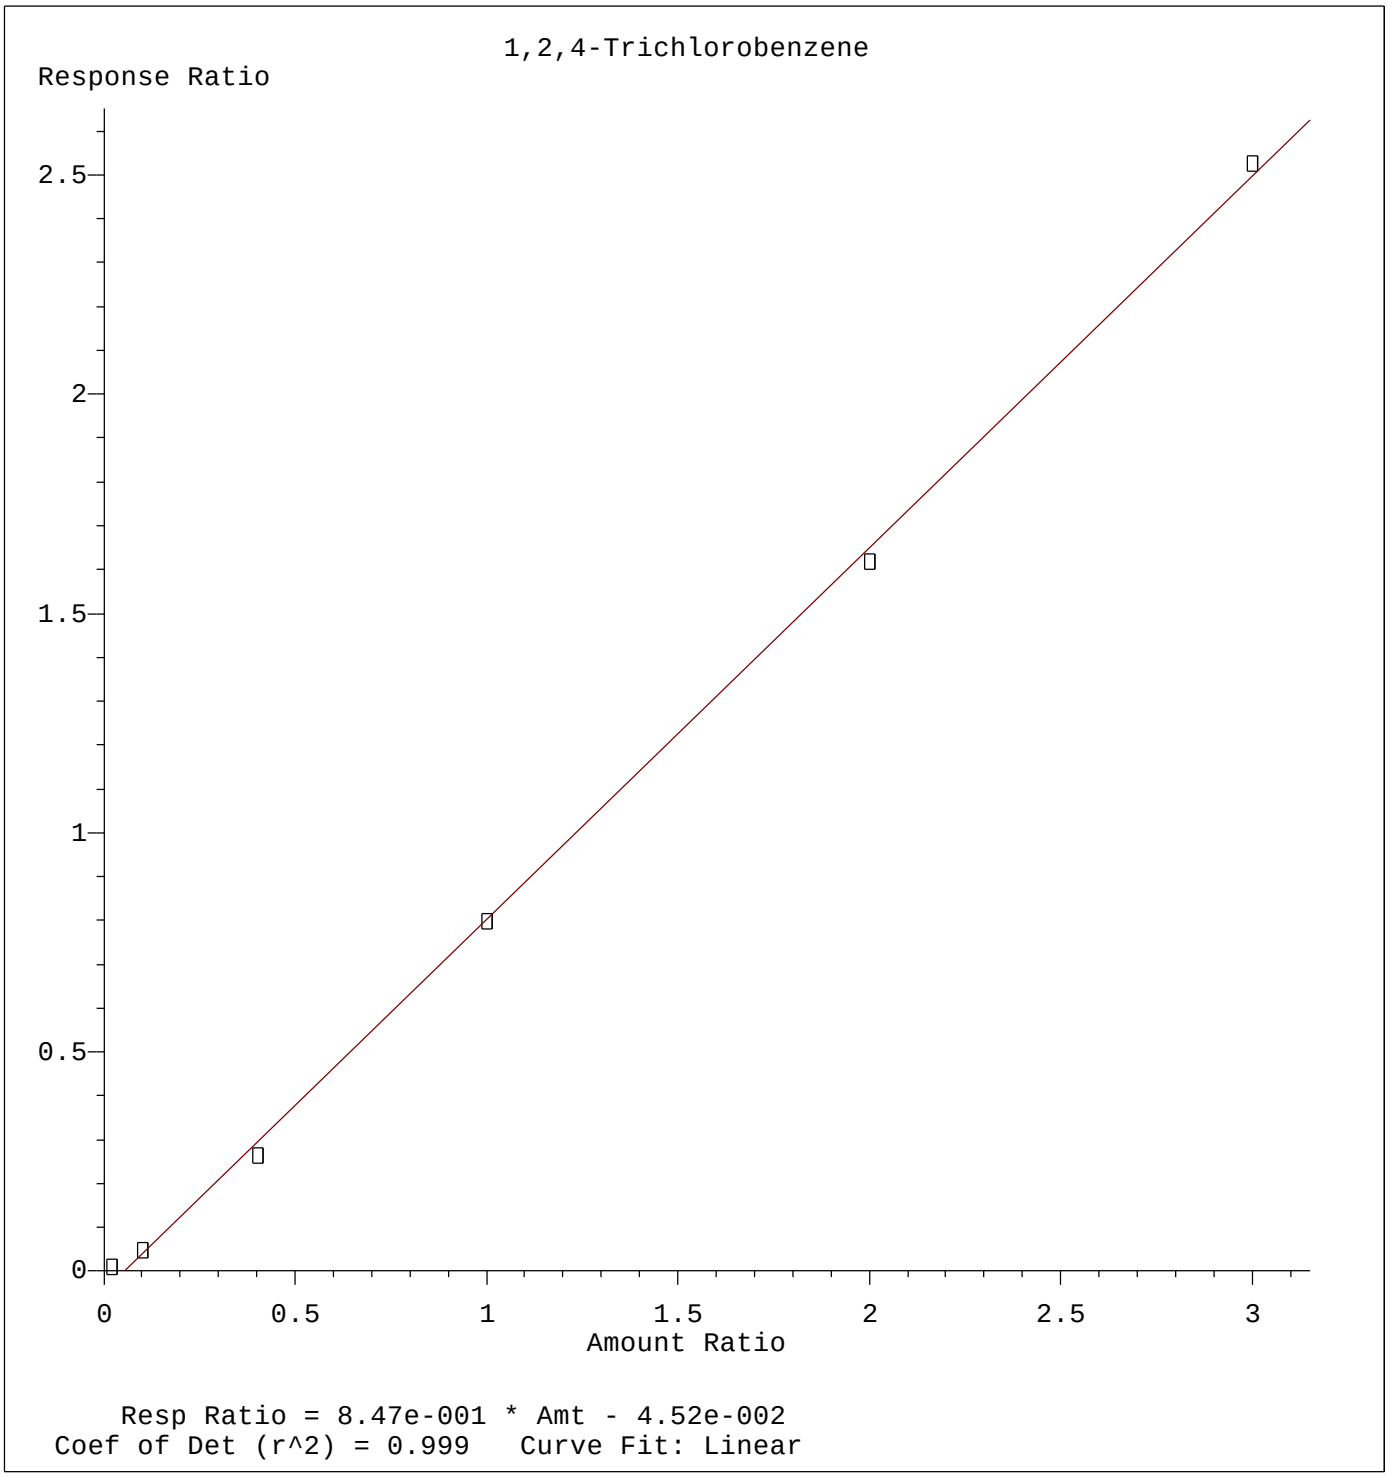

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
Calibration Table Last Updated: Wed Nov 04 12:09:03 2020

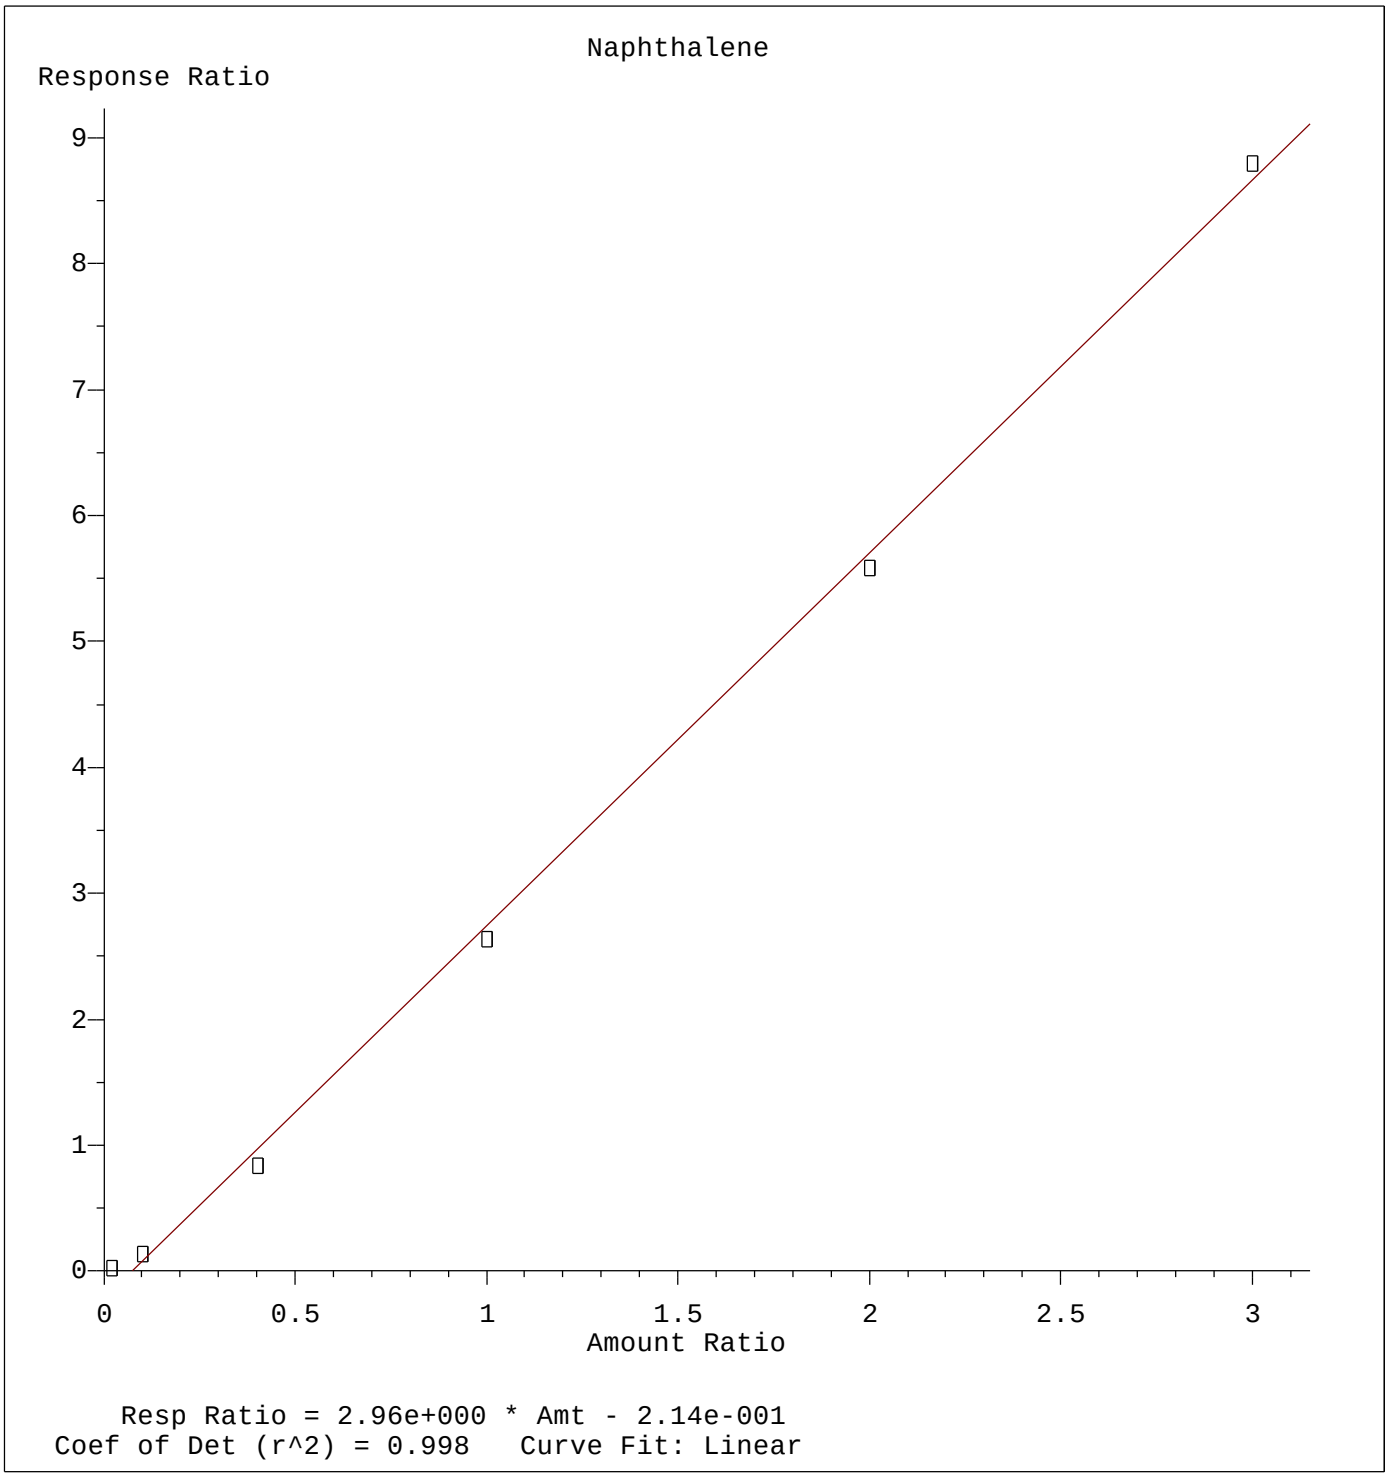

Resp Ratio = 2.96e+000 * Amt - 2.14e-001
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
Calibration Table Last Updated: Wed Nov 04 12:09:03 2020

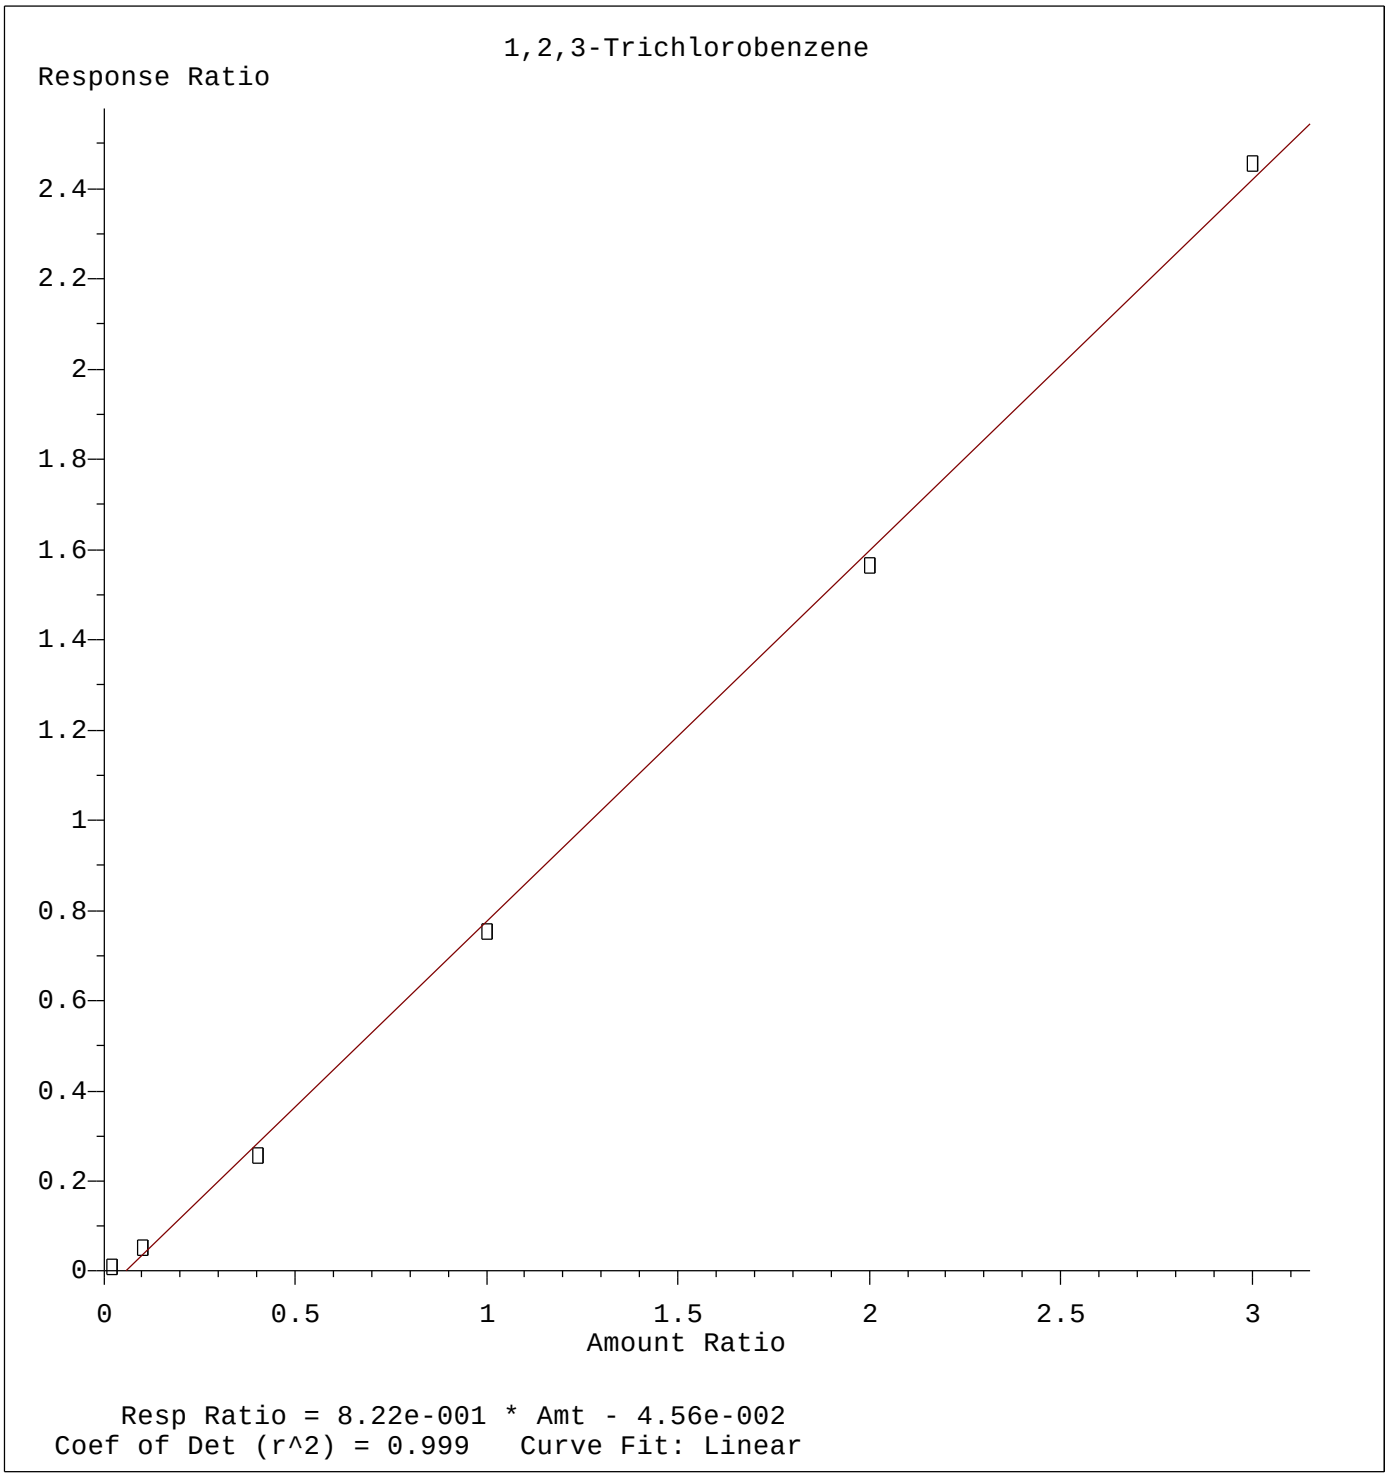

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
Calibration Table Last Updated: Wed Nov 04 12:09:03 2020