


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN110420\
 Data File : VN064424.D
 Acq On : 4 Nov 2020 9:02
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
 Title : SW846 8260
 Last Update : Wed Nov 04 12:09:03 2020

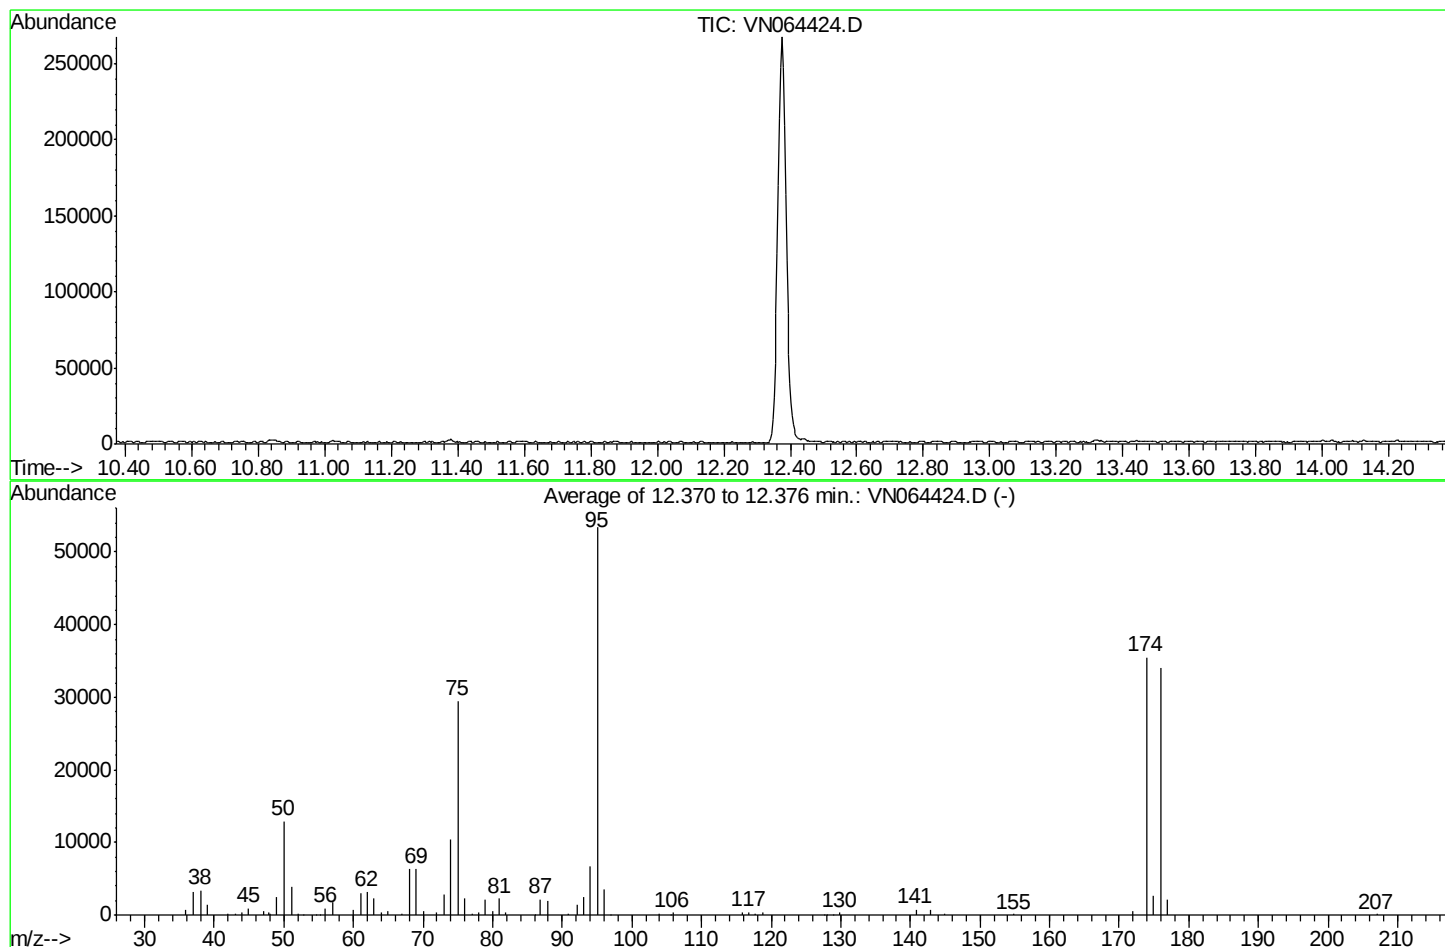

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.2	12899	PASS
75	95	30	60	55.3	29533	PASS
95	95	100	100	100.0	53408	PASS
96	95	5	9	6.7	3563	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	66.5	35504	PASS
175	174	5	9	7.4	2626	PASS
176	174	95	101	95.8	34000	PASS
177	176	5	9	6.2	2093	PASS