

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110422\
 Data File : VN075169.D
 Acq On : 04 Nov 2022 12:57
 Operator : JC\MD
 Sample : N5418-11RE
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-M

Quant Time: Nov 05 06:57:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 09:48:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	111890	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	220977	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	205979	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	80498	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	89624	59.449	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	118.900%
35) Dibromofluoromethane	8.171	113	68734	52.985	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	105.960%
50) Toluene-d8	10.565	98	271313	53.907	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	107.820%
62) 4-Bromofluorobenzene	12.853	95	87124	49.279	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	98.560%
Target Compounds						
					Qvalue	
3) Chloromethane	2.301	50	454	0.294	ug/l #	42
5) Bromomethane	2.918	94	473	Below Cal		94
6) Chloroethane	2.995	64	702	0.444	ug/l #	45
11) Tert butyl alcohol	5.500	59	2816	8.010	ug/l #	72
16) Acetone	4.453	43	12775	20.013	ug/l #	85
18) Methyl Acetate	5.047	43	1943	0.932	ug/l #	63
20) Methylene Chloride	5.277	84	11947	8.394	ug/l	92
25) 2-Butanone	7.500	43	2051	2.043	ug/l	91
29) Tetrahydrofuran	7.847	42	311	0.479	ug/l #	26
31) Cyclohexane	8.224	56	3007	1.341	ug/l #	53
36) 1,1-Dichloropropene	8.224	75	10332	5.144	ug/l #	49
37) Ethyl Acetate	7.571	43	16152	7.333	ug/l	98
38) Carbon Tetrachloride	8.230	117	13223	5.985	ug/l #	14
43) Isopropyl Acetate	8.694	43	71553	20.944	ug/l #	91
45) 1,2-Dichloropropane	9.741	63	859	0.587	ug/l #	42
48) Methyl methacrylate	9.671	41	2076	1.325	ug/l #	41
51) 4-Methyl-2-Pentanone	10.453	43	3591	1.629	ug/l #	81
54) cis-1,3-Dichloropropene	10.359	75	27551	11.146	ug/l #	67
56) Ethyl methacrylate	10.988	69	686	0.276	ug/l #	1
57) 1,3-Dichloropropane	11.206	76	3794	1.398	ug/l #	42
58) 2-Chloroethyl Vinyl ether	10.165	63	348	0.362	ug/l #	44
59) 2-Hexanone	11.171	43	57000	34.066	ug/l #	21
71) Bromoform	12.853	173	646	0.529	ug/l #	1
74) N-amyl acetate	12.482	43	732	0.306	ug/l #	38
76) 1,2,3-Trichloropropane	12.847	75	48088	28.135	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	48088	72.222	ug/l #	10
93) 1,2,4-Trichlorobenzene	15.394	180	496	0.416	ug/l #	84
95) Naphthalene	15.635	128	3365	0.734	ug/l #	72
96) 1,2,3-Trichlorobenzene	15.847	180	486	0.410	ug/l #	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110422\
Data File : VN075169.D
Acq On : 04 Nov 2022 12:57
Operator : JC\MD
Sample : N5418-11RE
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP-M

Quant Time: Nov 05 06:57:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 09:48:49 2022
Response via : Initial Calibration




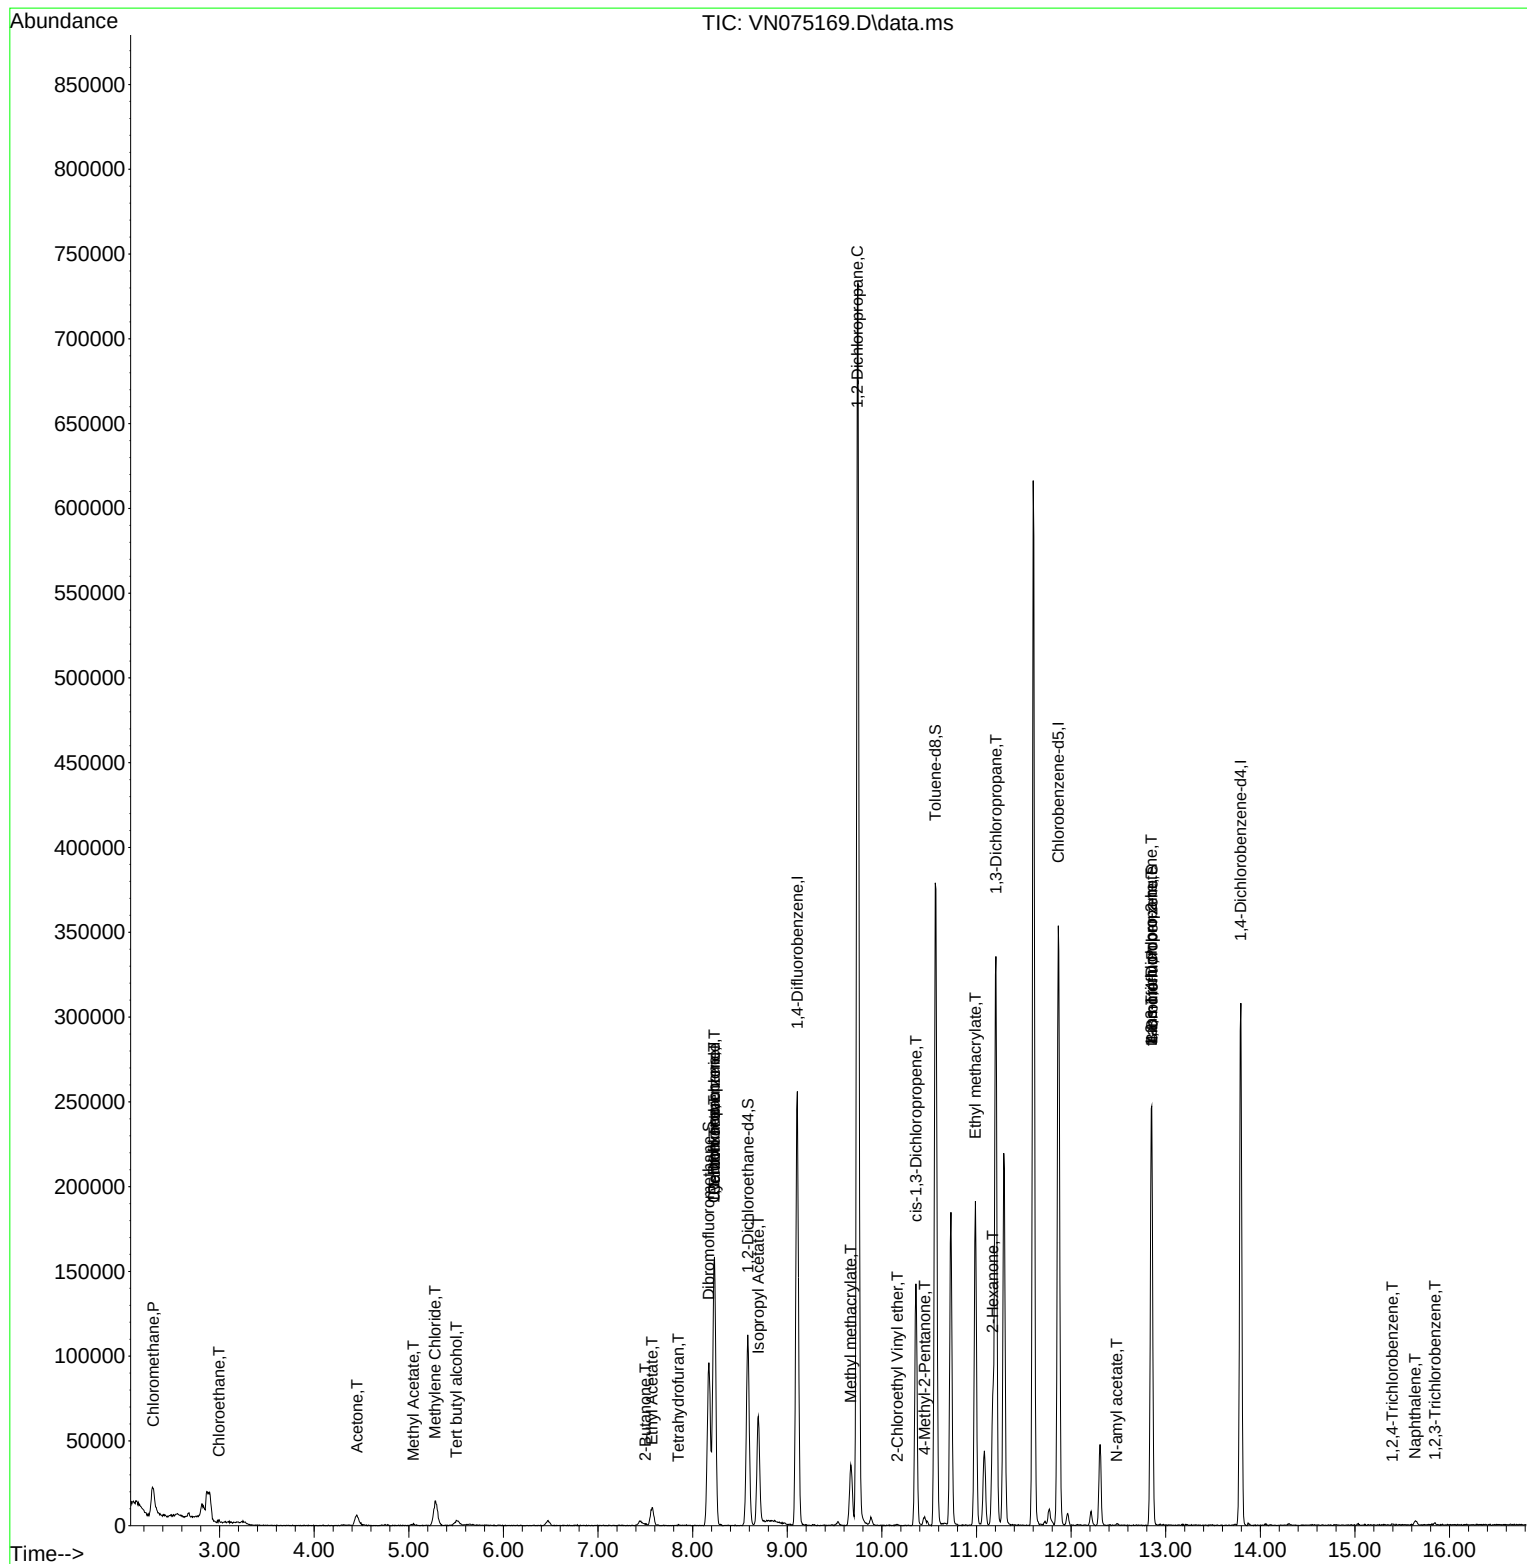




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57




Instrument :
MSVOA_N
ClientSampleId :
TP-M


Tgt Ion:168 Resp: 111890
Ion Ratio Lower Upper
168 100
99 62.4 51.6 77.4

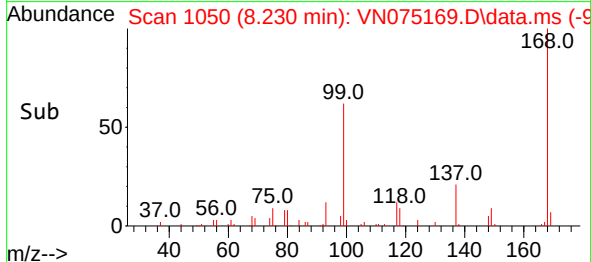

#3
Chloromethane
Concen: 0.294 ug/l
RT: 2.301 min Scan# 42
Delta R.T. -0.070 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57

Tgt Ion: 50 Resp: 454
Ion Ratio Lower Upper
50 100
52 0.0 25.8 38.6#


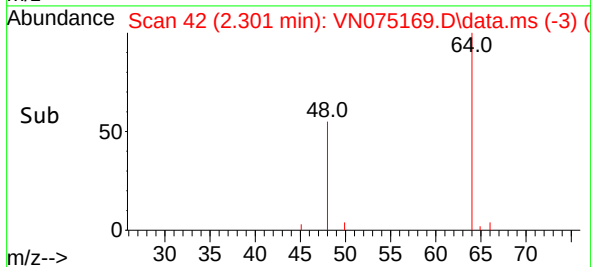

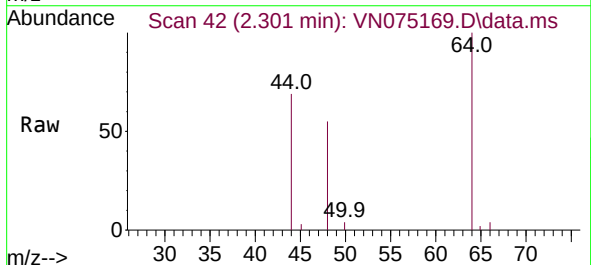


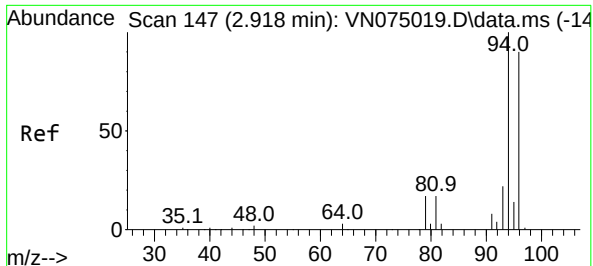

#5
Bromomethane
Concen: Below Cal
RT: 2.918 min Scan# 147
Delta R.T. 0.000 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57



Instrument :
MSVOA_N
ClientSampleId :
TP-M


Tgt Ion: 94 Resp: 473
Ion Ratio Lower Upper
94 100
96 84.0 71.8 107.6

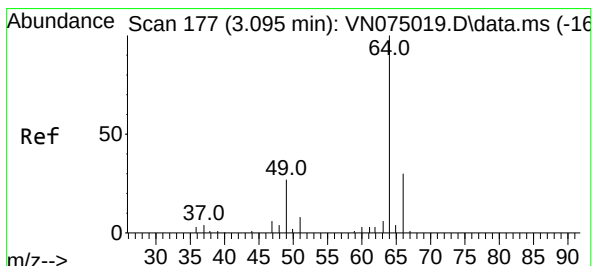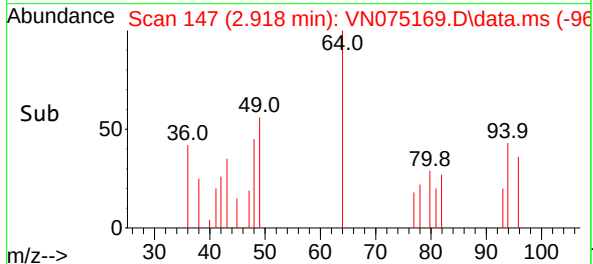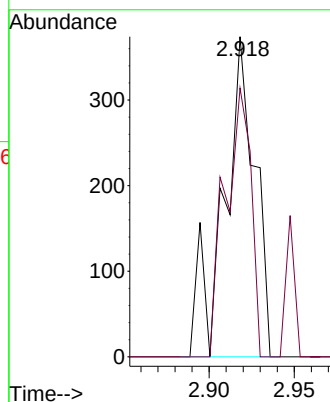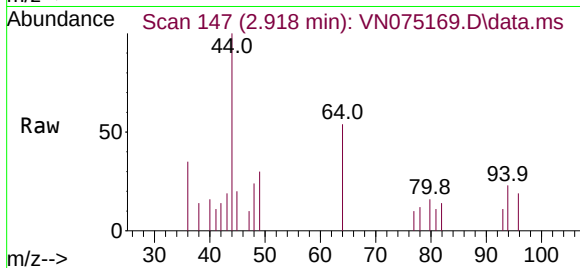

#6
Chloroethane
Concen: 0.444 ug/l
RT: 2.995 min Scan# 160
Delta R.T. -0.100 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57

Tgt Ion: 64 Resp: 702
Ion Ratio Lower Upper
64 100
66 0.0 23.8 35.8#



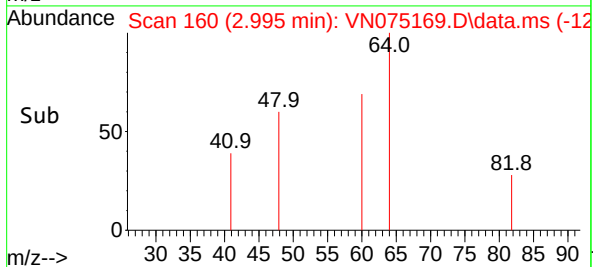
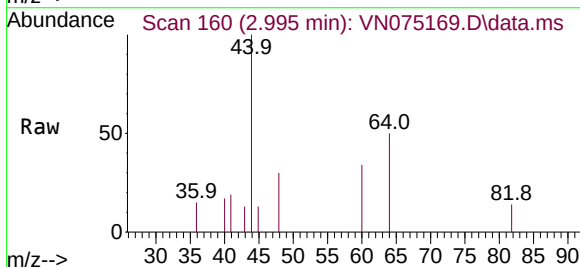




#11
Tert butyl alcohol
Concen: 8.010 ug/l
RT: 5.500 min Scan# 51
Delta R.T. -0.042 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57




Instrument :
MSVOA_N
ClientSampleId :
TP-M


Tgt Ion: 59 Resp: 2816
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#

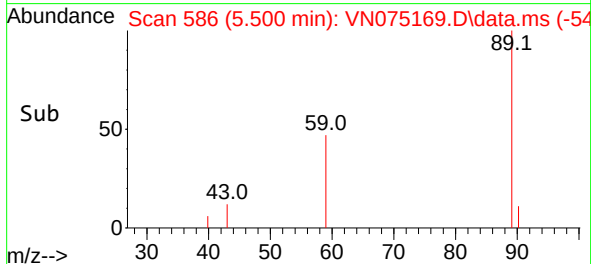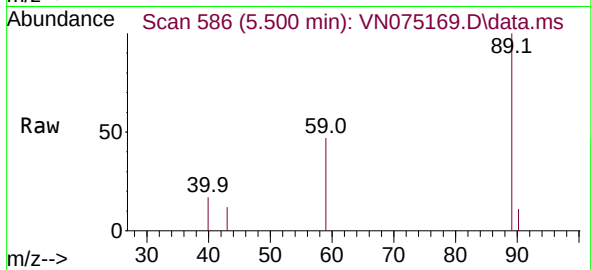

#16
Acetone
Concen: 20.013 ug/l
RT: 4.453 min Scan# 408
Delta R.T. 0.011 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57

Tgt Ion: 43 Resp: 12775
Ion Ratio Lower Upper
43 100
58 40.1 25.5 38.3#




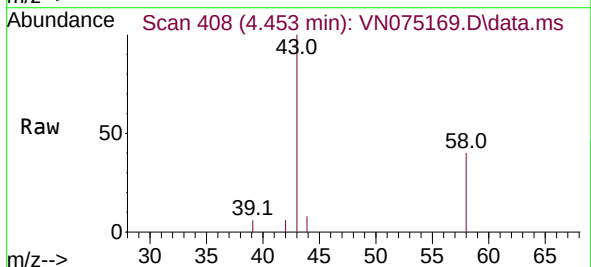




#18
Methyl Acetate
Concen: 0.932 ug/l
RT: 5.047 min Scan# 508
Delta R.T. 0.005 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57




Instrument :
MSVOA_N
ClientSampleId :
TP-M


Tgt Ion: 43 Resp: 1943
Ion Ratio Lower Upper
43 100
74 8.4 22.0 33.0#

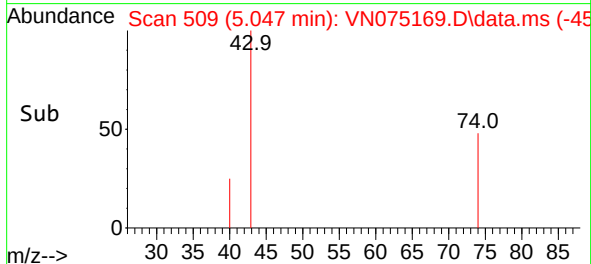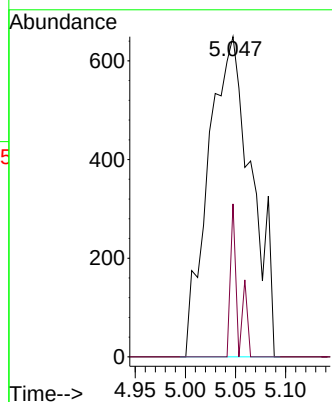

#20
Methylene Chloride
Concen: 8.394 ug/l
RT: 5.277 min Scan# 548
Delta R.T. -0.006 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57

Tgt Ion: 84 Resp: 11947
Ion Ratio Lower Upper
84 100
49 108.5 94.9 142.3
51 32.8 26.8 40.2
86 58.8 53.7 80.5

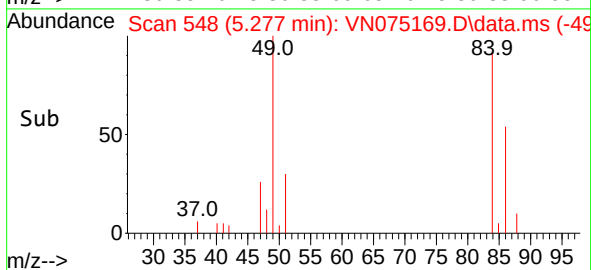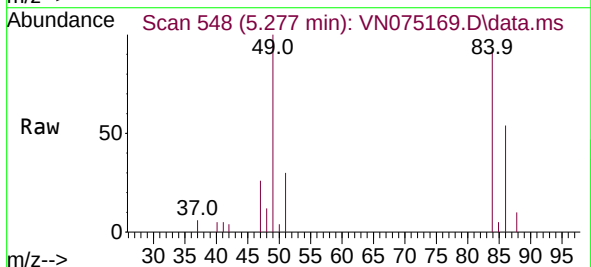

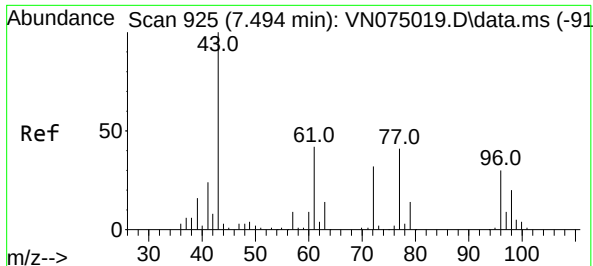

#25

2-Butanone

Concen: 2.043 ug/l

RT: 7.500 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN075169.D

Acq: 04 Nov 2022 12:57

Instrument :

MSVOA_N

ClientSampleId :





TP-M

Tgt Ion: 43 Resp: 2051

Ion Ratio Lower Upper

43 100

72 26.8 25.5 38.3

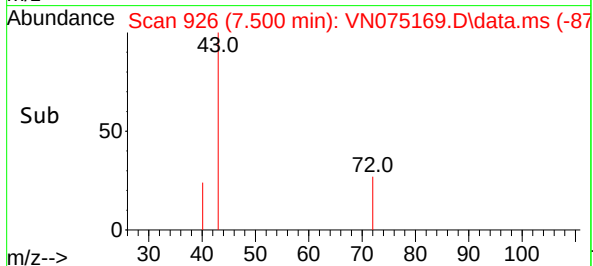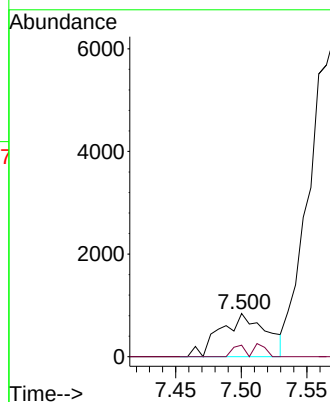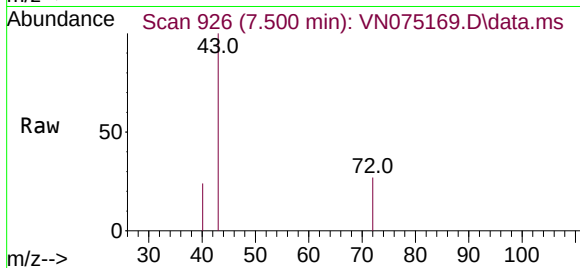

#29

Tetrahydrofuran

Concen: 0.479 ug/l

RT: 7.847 min Scan# 985

Delta R.T. 0.000 min

Lab File: VN075169.D

Acq: 04 Nov 2022 12:57




Tgt Ion: 42 Resp: 311


Ion Ratio Lower Upper

42 100

72 0.0 43.0 64.6#

71 0.0 39.9 59.9#


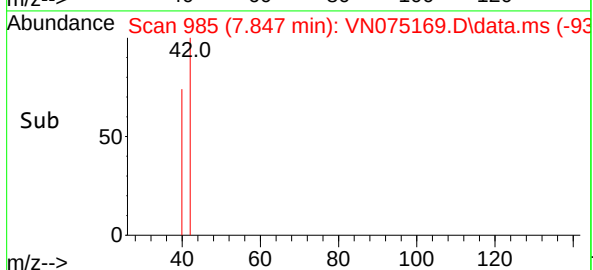

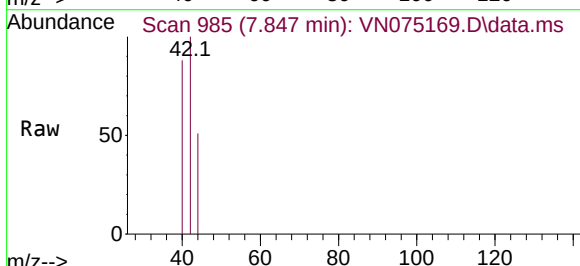




#31
Cyclohexane
Concen: 1.341 ug/l
RT: 8.224 min Scan# 1049
Delta R.T. -0.035 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57




Instrument :
MSVOA_N
ClientSampleId :
TP-M


Tgt Ion: 56 Resp: 3007
Ion Ratio Lower Upper
56 100
69 130.6 25.2 37.8#
84 102.0 77.8 116.8

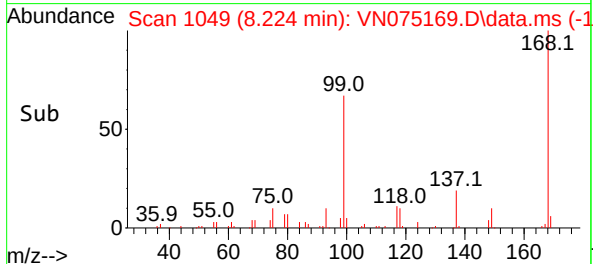

#33
1,2-Dichloroethane-d4
Concen: 59.449 ug/l
RT: 8.582 min Scan# 1110
Delta R.T. -0.005 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57

Tgt Ion: 65 Resp: 89624
Ion Ratio Lower Upper
65 100
67 51.1 0.0 102.0

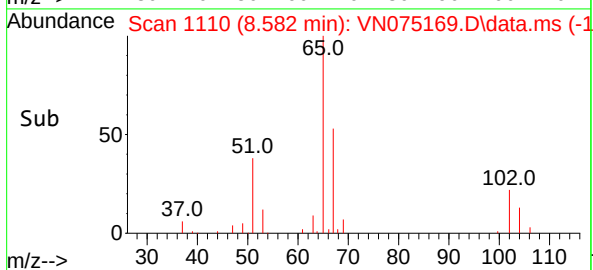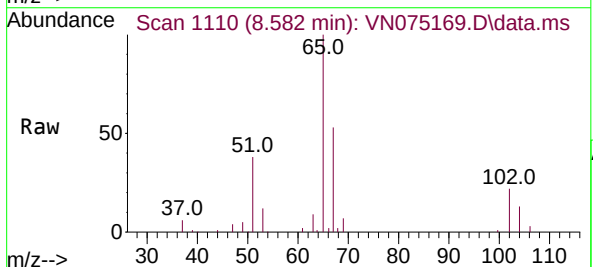

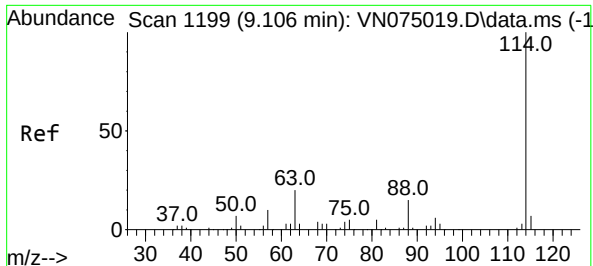

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN075169.D

Acq: 04 Nov 2022 12:57

Instrument :

MSVOA_N

ClientSampleId :

TP-M





Tgt Ion:114 Resp: 220977

Ion Ratio Lower Upper

114 100

63 20.2 0.0 39.6

88 14.7 0.0 29.0

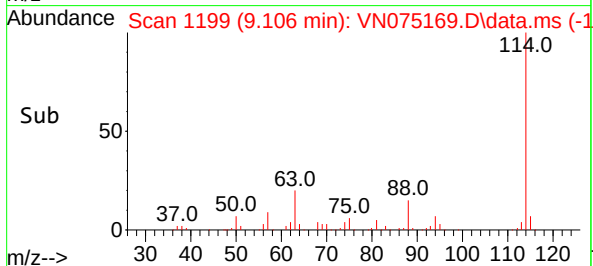

#35

Dibromofluoromethane

Concen: 52.985 ug/l

RT: 8.171 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VN075169.D

Acq: 04 Nov 2022 12:57




Tgt Ion:113 Resp: 68734


Ion Ratio Lower Upper

113 100

111 103.5 80.5 120.7

192 16.4 13.2 19.8

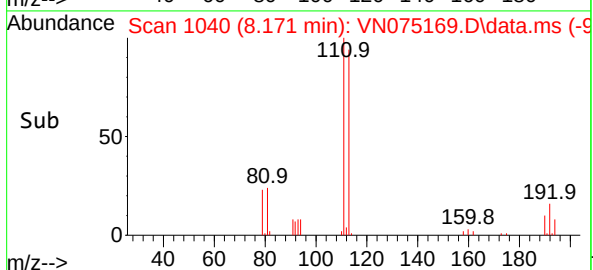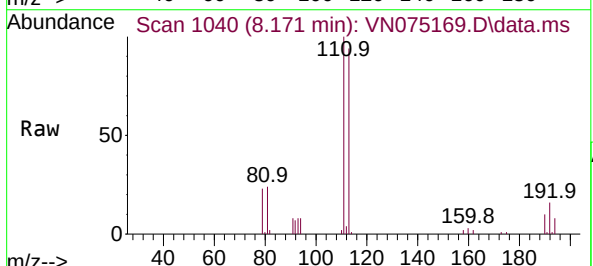



#36

1,1-Dichloropropene

Concen: 5.144 ug/l

RT: 8.224 min Scan# 1049

Delta R.T. -0.153 min

Lab File: VN075169.D

Acq: 04 Nov 2022 12:57

Instrument :

MSVOA_N

ClientSampleId :

TP-M





Tgt Ion: 75 Resp: 10332

Ion Ratio Lower Upper

75 100

110 8.0 17.8 53.3#

77 0.0 24.6 37.0#

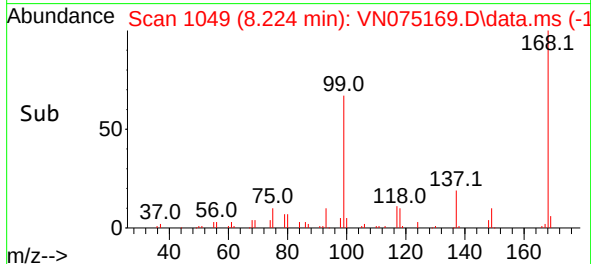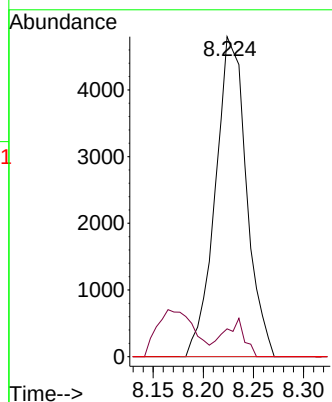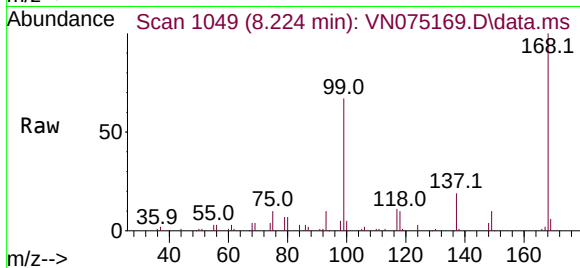

#37

Ethyl Acetate

Concen: 7.333 ug/l

RT: 7.571 min Scan# 938

Delta R.T. -0.000 min

Lab File: VN075169.D

Acq: 04 Nov 2022 12:57




Tgt Ion: 43 Resp: 16152


Ion Ratio Lower Upper

43 100

61 15.1 12.2 18.4


70 9.9 9.4 14.2

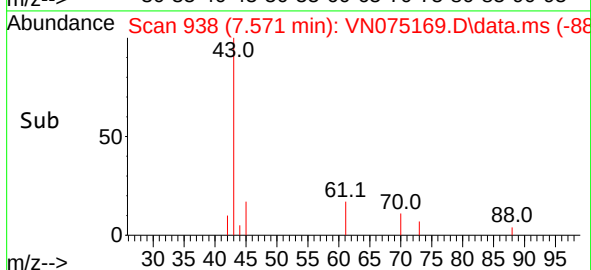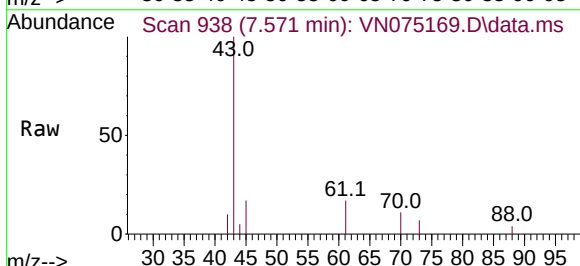






#38
Carbon Tetrachloride
Concen: 5.985 ug/l
RT: 8.230 min Scan# 1074
Delta R.T. -0.141 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57

Instrument :
MSVOA_N
ClientSampleId :
TP-M







Tgt Ion:117 Resp: 13223
Ion Ratio Lower Upper
117 100
119 3.0 76.7 115.1#
121 0.0 23.9 35.9#

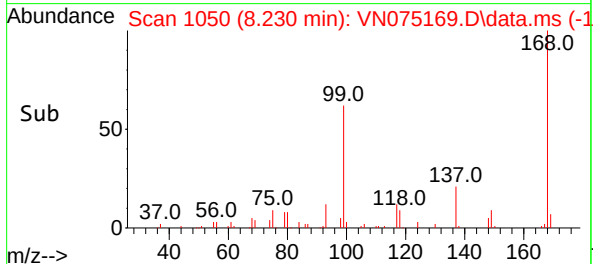

#43
Isopropyl Acetate
Concen: 20.944 ug/l
RT: 8.694 min Scan# 1129
Delta R.T. 0.000 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57

Tgt Ion: 43 Resp: 71553
Ion Ratio Lower Upper
43 100
61 20.7 22.4 33.6#
87 16.1 12.5 18.7

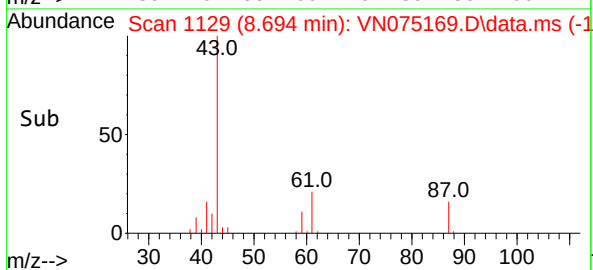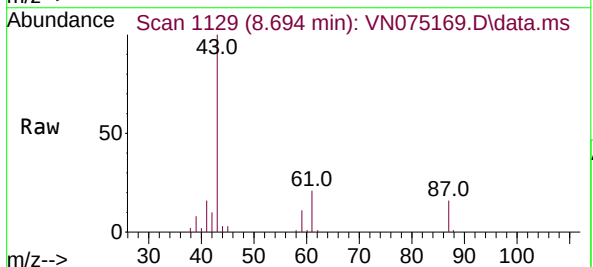

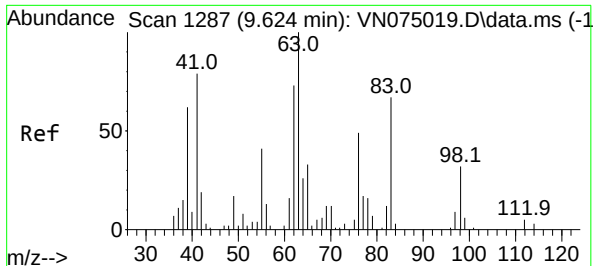

#45

1,2-Dichloropropane

Concen: 0.587 ug/l

RT: 9.741 min Scan# 11

Delta R.T. 0.117 min

Lab File: VN075169.D

Acq: 04 Nov 2022 12:57

Instrument :

MSVOA_N

ClientSampleId :





TP-M

Tgt Ion: 63 Resp: 859

Ion Ratio Lower Upper

63 100

65 0.0 26.1 39.1#

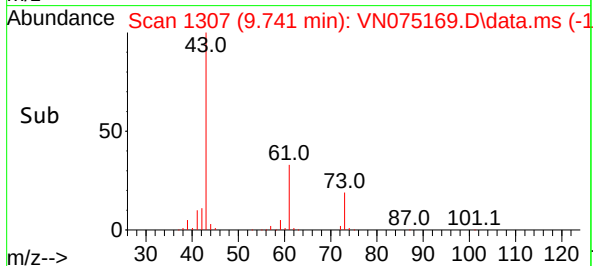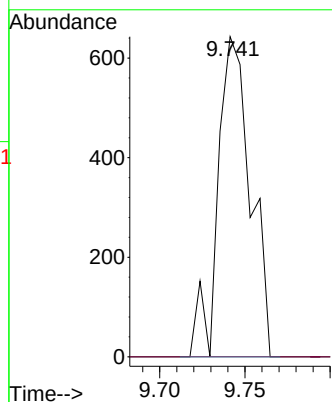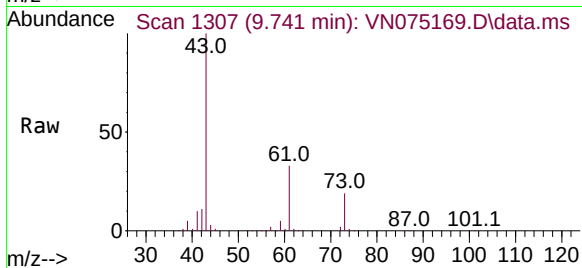

#48

Methyl methacrylate

Concen: 1.325 ug/l

RT: 9.671 min Scan# 1295

Delta R.T. -0.011 min

Lab File: VN075169.D

Acq: 04 Nov 2022 12:57




Tgt Ion: 41 Resp: 2076


Ion Ratio Lower Upper

41 100

69 0.0 80.2 120.2#

39 70.4 56.2 84.2

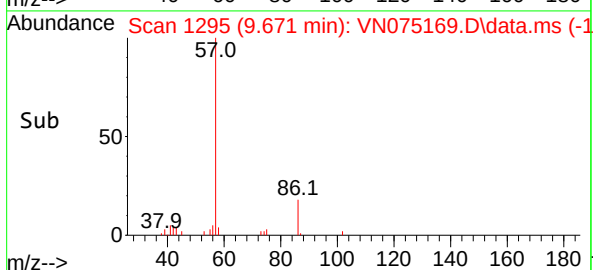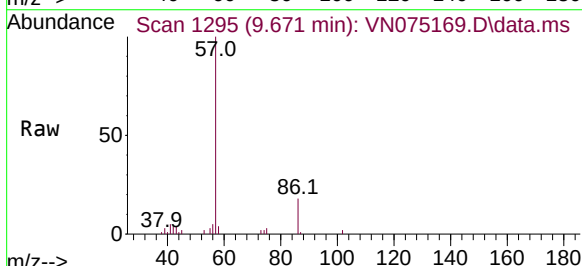



#50

Toluene-d8

Concen: 53.907 ug/l

RT: 10.565 min Scan# 1447

Delta R.T. -0.006 min

Lab File: VN075169.D

Acq: 04 Nov 2022 12:57

Instrument :

MSVOA_N

ClientSampleId :





TP-M

Tgt Ion: 98 Resp: 271313

Ion Ratio Lower Upper

98 100

100 65.0 53.0 79.6

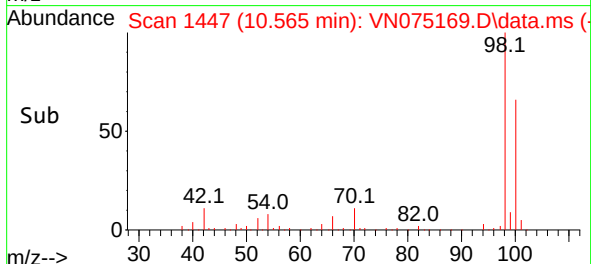

#51

4-Methyl-2-Pentanone

Concen: 1.629 ug/l

RT: 10.453 min Scan# 1428

Delta R.T. 0.006 min

Lab File: VN075169.D




Acq: 04 Nov 2022 12:57


Tgt Ion: 43 Resp: 3591

Ion Ratio Lower Upper

43 100

58 29.8 33.6 50.4#


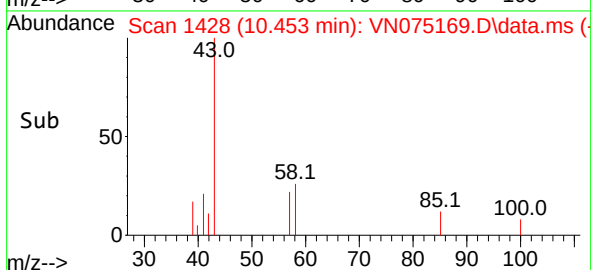




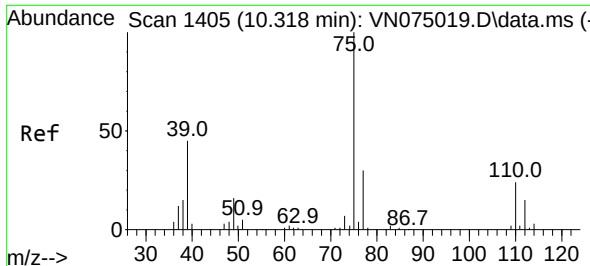

#54
 cis-1,3-Dichloropropene
 Concen: 11.146 ug/l
 RT: 10.359 min Scan# 1412
 Delta R.T. 0.041 min
 Lab File: VN075169.D
 Acq: 04 Nov 2022 12:57




Instrument :
 MSVOA_N
 ClientSampleId :
 TP-M


Tgt Ion: 75 Resp: 27551
 Ion Ratio Lower Upper
 75 100
 77 0.0 23.7 35.5#
 39 32.6 35.8 53.6#

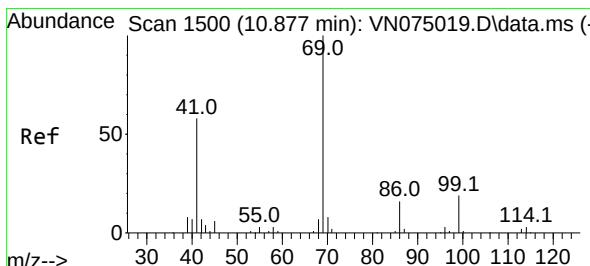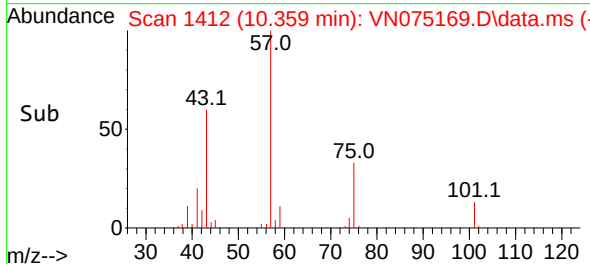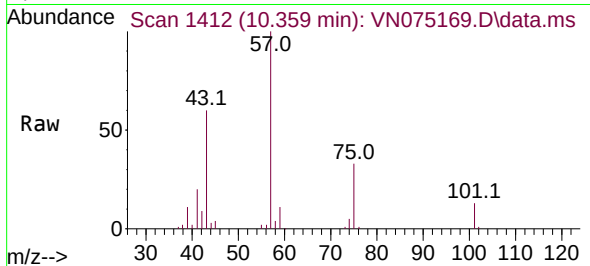

#56
 Ethyl methacrylate
 Concen: 0.276 ug/l
 RT: 10.988 min Scan# 1519
 Delta R.T. 0.111 min
 Lab File: VN075169.D
 Acq: 04 Nov 2022 12:57

Tgt Ion: 69 Resp: 686
 Ion Ratio Lower Upper
 69 100
 41 5274.8 45.6 68.4#
 39 2476.4 28.5 42.7#

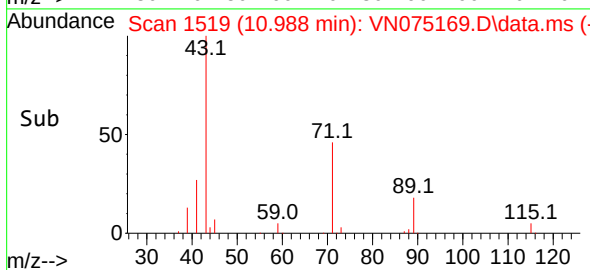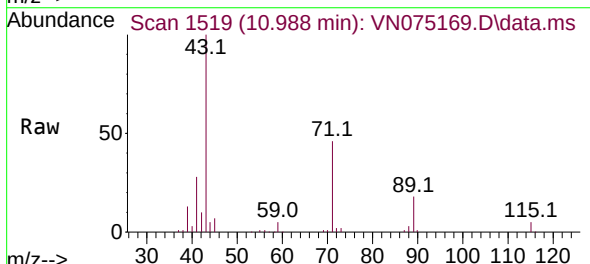



#57

1,3-Dichloropropane

Concen: 1.398 ug/l

RT: 11.206 min Scan# 11

Delta R.T. 0.041 min

Lab File: VN075169.D

Acq: 04 Nov 2022 12:57

Instrument :

MSVOA_N

ClientSampleId :





TP-M

Tgt Ion: 76 Resp: 3794

Ion Ratio Lower Upper

76 100

78 0.0 25.8 38.6#

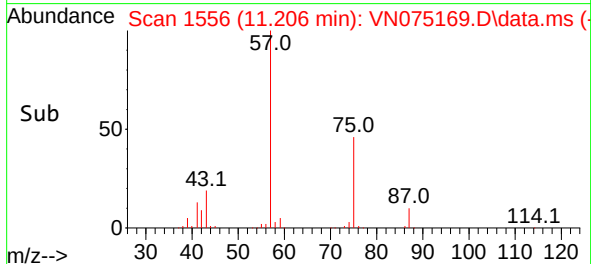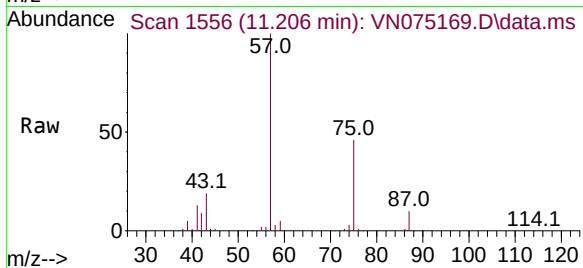

#58

2-Chloroethyl Vinyl ether

Concen: 0.362 ug/l

RT: 10.165 min Scan# 1379

Delta R.T. -0.000 min

Lab File: VN075169.D




Acq: 04 Nov 2022 12:57


Tgt Ion: 63 Resp: 348

Ion Ratio Lower Upper

63 100

106 0.0 24.8 37.2#


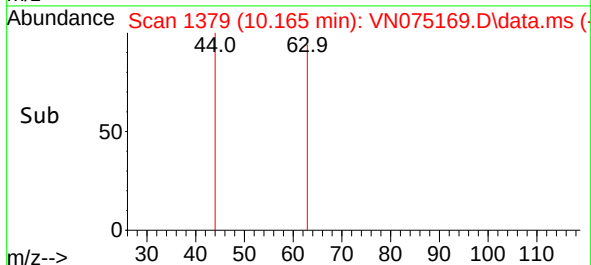
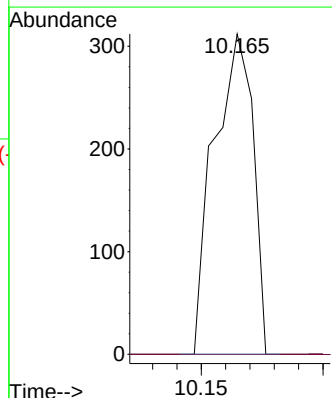
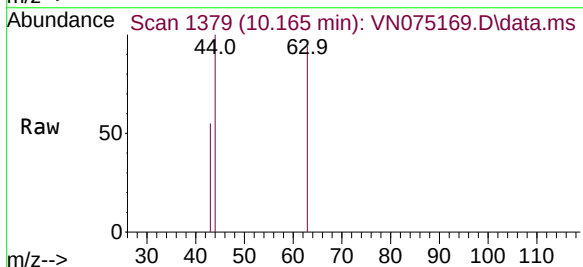




#59
2-Hexanone
Concen: 34.066 ug/l
RT: 11.171 min Scan# 111
Delta R.T. -0.029 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57




Instrument :
MSVOA_N
ClientSampleId :
TP-M


Tgt Ion: 43 Resp: 57000
Ion Ratio Lower Upper
43 100
58 0.0 29.6 88.8#

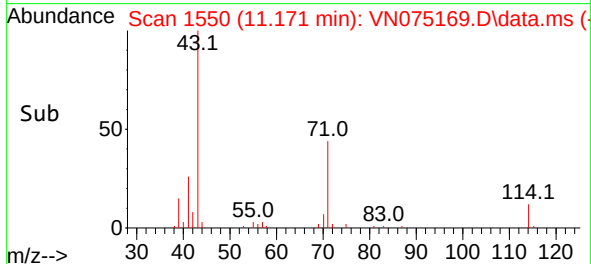

#62
4-Bromofluorobenzene
Concen: 49.279 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57

Tgt Ion: 95 Resp: 87124
Ion Ratio Lower Upper
95 100
174 73.3 0.0 147.4
176 70.0 0.0 142.2


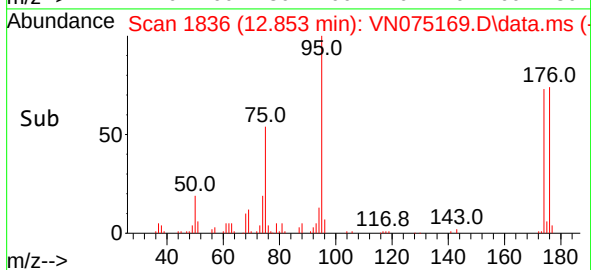

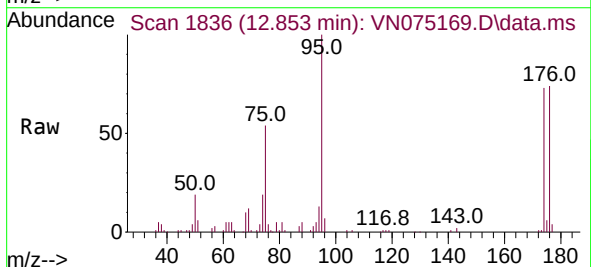




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57




Instrument :
MSVOA_N
ClientSampleId :
TP-M


Tgt Ion:117 Resp: 205979
Ion Ratio Lower Upper
117 100
82 56.0 43.1 64.7
119 31.1 25.5 38.3

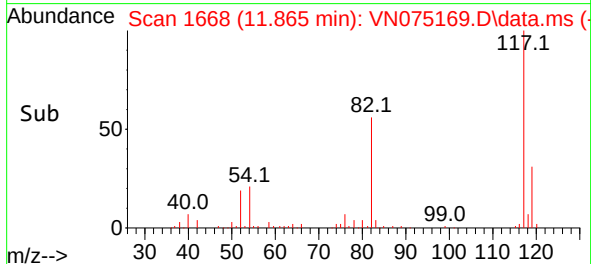

#71
Bromoform
Concen: 0.529 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.271 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57

Tgt Ion:173 Resp: 646
Ion Ratio Lower Upper
173 100
175 674.1 24.6 74.0#
254 0.0 0.0 0.0


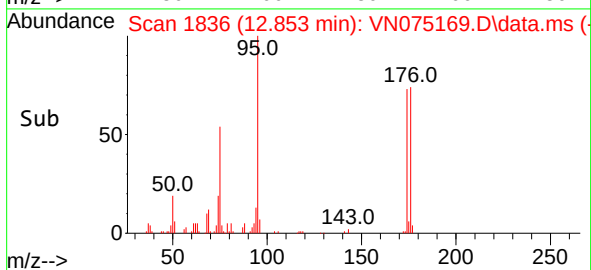

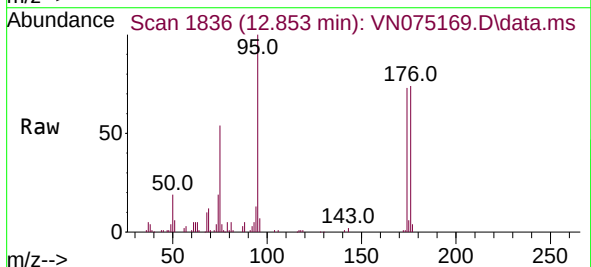




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57




Instrument :
MSVOA_N
ClientSampleId :
TP-M


Tgt Ion:152 Resp: 80498
Ion Ratio Lower Upper
152 100
115 61.6 30.2 90.6
150 157.3 0.0 348.4

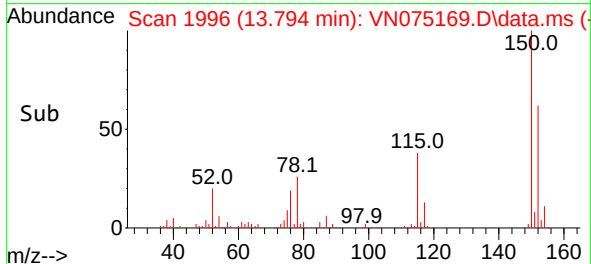

#74
N-ethyl acetate
Concen: 0.306 ug/l
RT: 12.482 min Scan# 1773
Delta R.T. -0.012 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57

Tgt Ion: 43 Resp: 732
Ion Ratio Lower Upper
43 100
70 0.0 39.8 59.8#
55 0.0 19.9 29.9#
61 0.0 21.7 32.5#


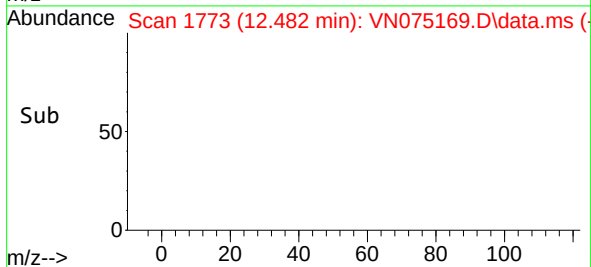

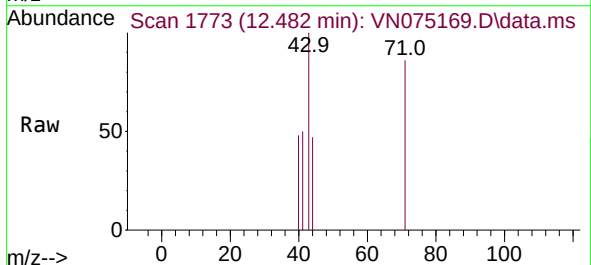




#76
1,2,3-Trichloropropane
Concen: 28.135 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. -0.147 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57




Instrument :
MSVOA_N
ClientSampleId :
TP-M


Tgt Ion: 75 Resp: 48088
Ion Ratio Lower Upper
75 100
77 1.2 75.6 226.8#

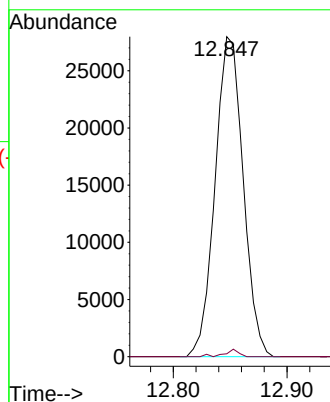

#81
trans-1,4-Dichloro-2-butene
Concen: 72.222 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. 0.106 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57

Tgt Ion: 75 Resp: 48088
Ion Ratio Lower Upper
75 100
53 0.0 78.5 117.7#
89 0.0 37.7 56.5#


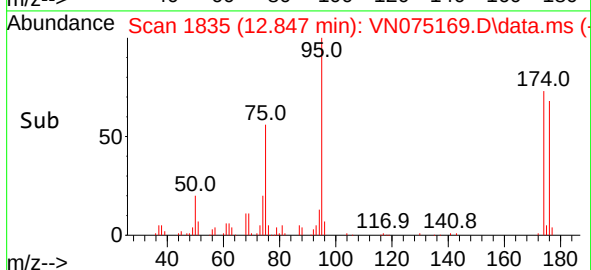






#93
1,2,4-Trichlorobenzene
Concen: 0.416 ug/l
RT: 15.394 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57




Instrument :
MSVOA_N
ClientSampleId :
TP-M


Tgt Ion:180 Resp: 496
Ion Ratio Lower Upper
180 100
182 95.2 47.8 143.4
145 0.0 16.8 50.3#

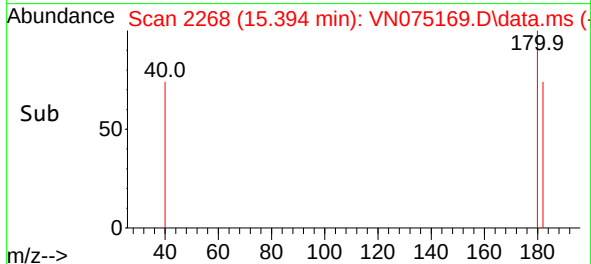

#95
Naphthalene
Concen: 0.734 ug/l
RT: 15.635 min Scan# 2309
Delta R.T. -0.006 min
Lab File: VN075169.D
Acq: 04 Nov 2022 12:57


Tgt Ion:128 Resp: 3365
Ion Ratio Lower Upper
128 100
127 0.0 10.4 15.6#
129 2.6 8.6 12.8#

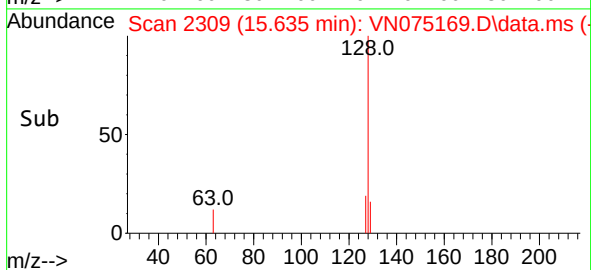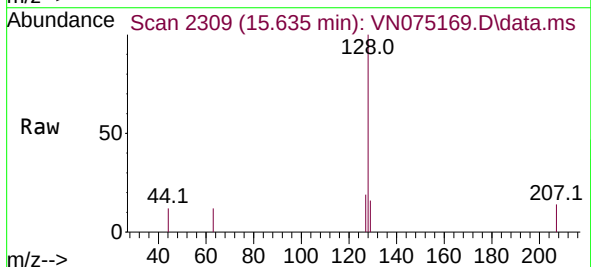



#96
 1,2,3-Trichlorobenzene
 Concen: 0.410 ug/l
 RT: 15.847 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VN075169.D
 Acq: 04 Nov 2022 12:57

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-M

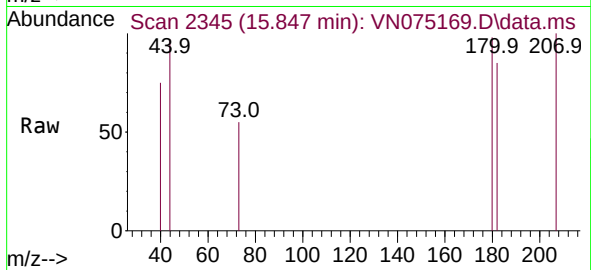

Tgt Ion	Ratio	Lower	Upper
180	100		
182	101.2	47.3	141.8
145	0.0	17.6	52.9#

