

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110422\
 Data File : VN075180.D
 Acq On : 04 Nov 2022 17:41
 Operator : JC\MD
 Sample : N5482-02 100X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FLOOR-DRAIN-WATER

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M

Title : SW846 8260

Signal : TIC: VN075180.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.301	37	42	49	rBV2	5335	12548	2.81%	0.518%
2	2.818	124	130	133	rBV2	7157	14534	3.25%	0.599%
3	2.895	140	143	151	rVB4	19084	41799	9.36%	1.724%
4	5.289	540	550	556	rBV4	1930	5588	1.25%	0.230%
5	8.171	1031	1040	1044	rBV2	64387	149908	33.56%	6.183%
6	8.230	1044	1050	1061	rVB2	113900	256732	57.48%	10.590%
7	8.583	1101	1110	1119	rBV	75108	167315	37.46%	6.901%
8	8.718	1124	1133	1135	rBV3	6283	15013	3.36%	0.619%
9	9.106	1190	1199	1210	rVB	172064	345060	77.26%	14.233%
10	10.571	1439	1448	1458	rBV	246491	446621	100.00%	18.422%
11	11.871	1660	1669	1679	rVB	213325	385070	86.22%	15.883%
12	12.853	1829	1836	1844	rVB	157597	260682	58.37%	10.753%
13	13.794	1987	1996	2005	rVB	191636	323495	72.43%	13.343%




Sum of corrected areas: 2424365

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110422\
Data File : VN075180.D
Acq On : 04 Nov 2022 17:41
Operator : JC\MD
Sample : N5482-02 100X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAIN-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

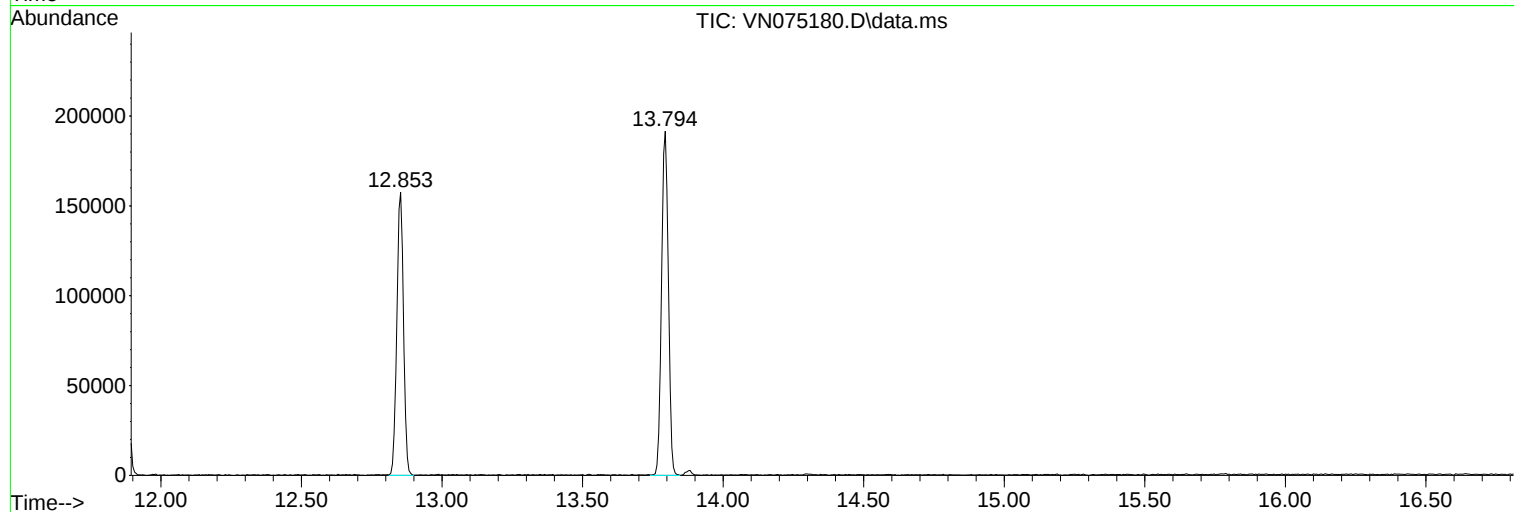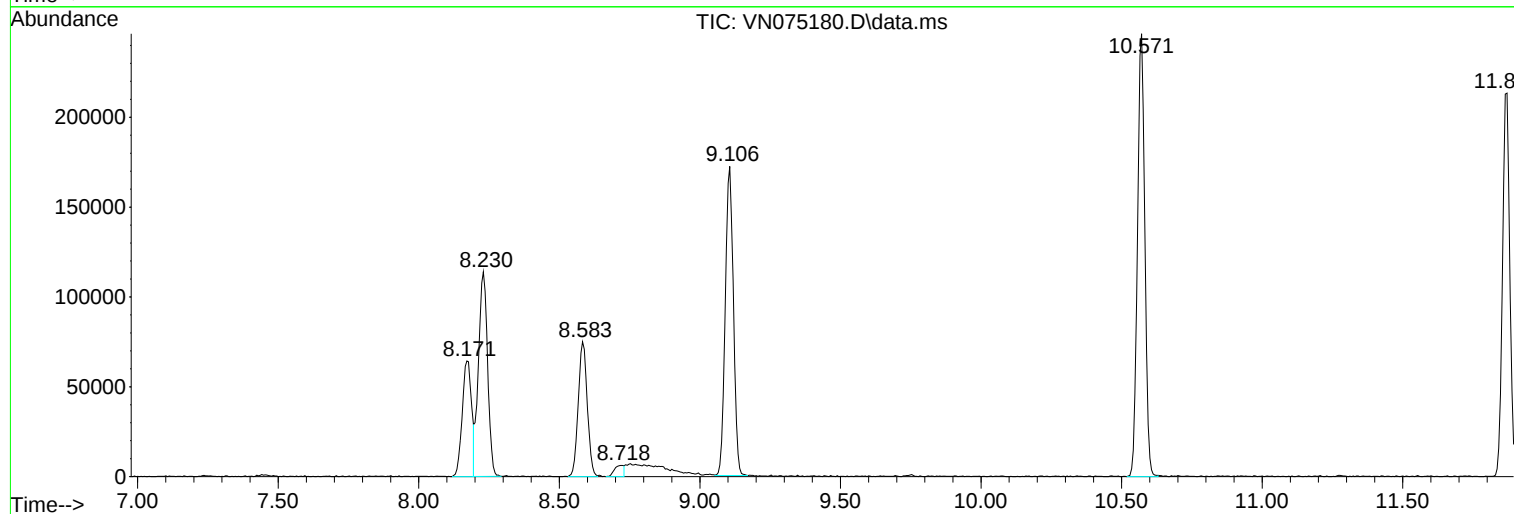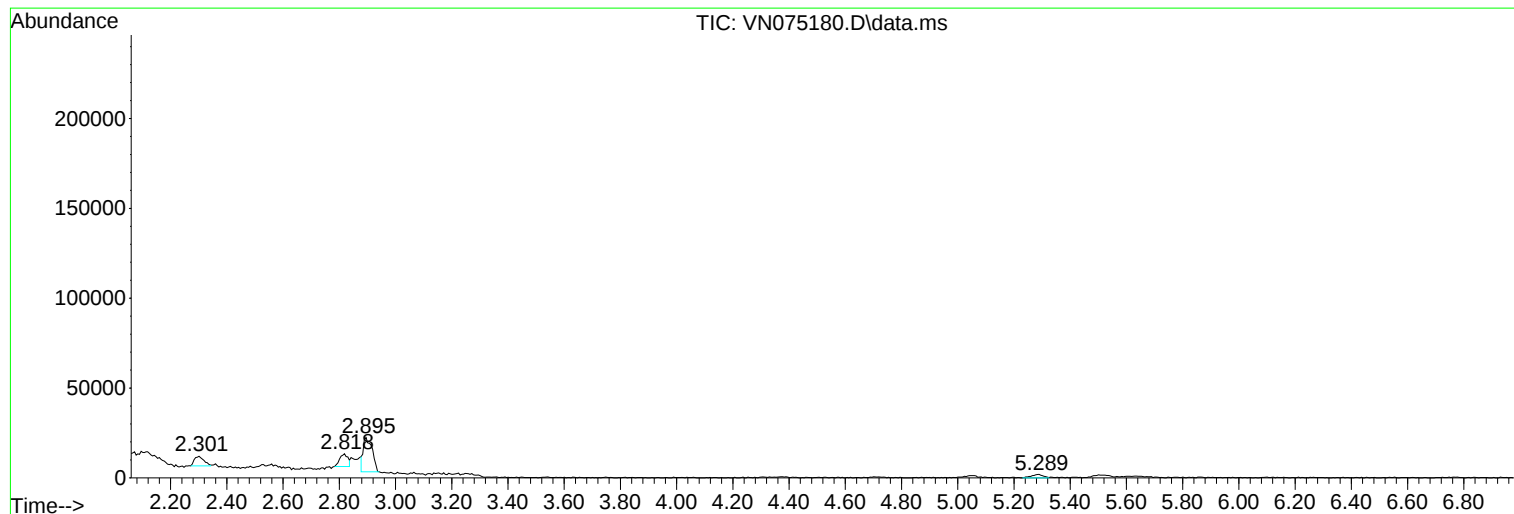

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110422\
Data File : VN075180.D
Acq On : 04 Nov 2022 17:41
Operator : JC\MD
Sample : N5482-02 100X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAIN-WATER










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Aminomethanesulfonic acid Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.895	8.14 ug/l	41799	Pentafluorobenzene	8.230

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
2			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	64
3			Sulfur dioxide	64	O2S	007446-09-5	64
4			Ethyl Chloride	64	C2H5Cl	000075-00-3	56
5			2-Aminoethyl hydrogen sulfate	141	C2H7NO4S	000926-39-6	9

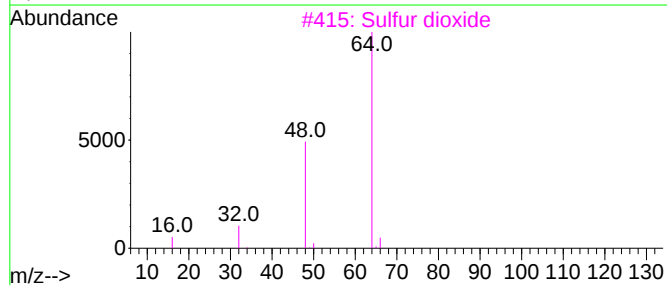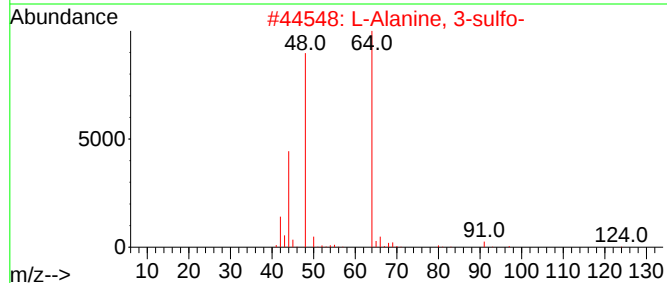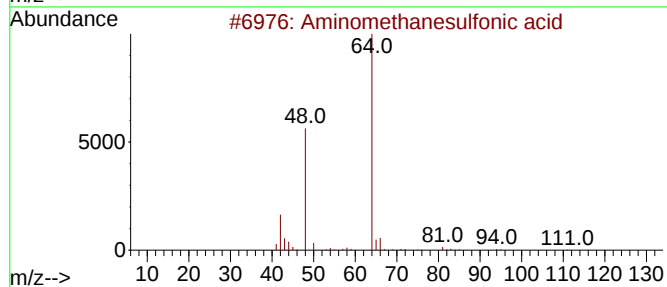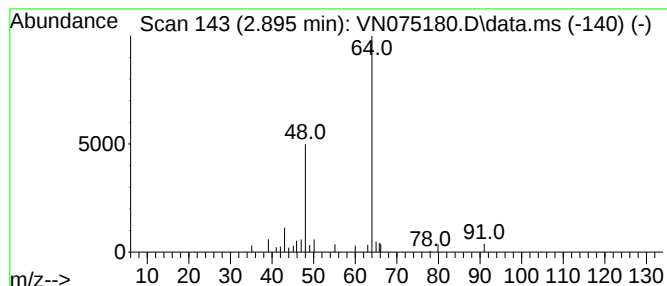

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110422\
Data File : VN075180.D
Acq On : 04 Nov 2022 17:41
Operator : JC\MD
Sample : N5482-02 100X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAIN-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Aminomethanesul...	2.895	8.1	ug/l	41799	1	8.230	256732	50.0