
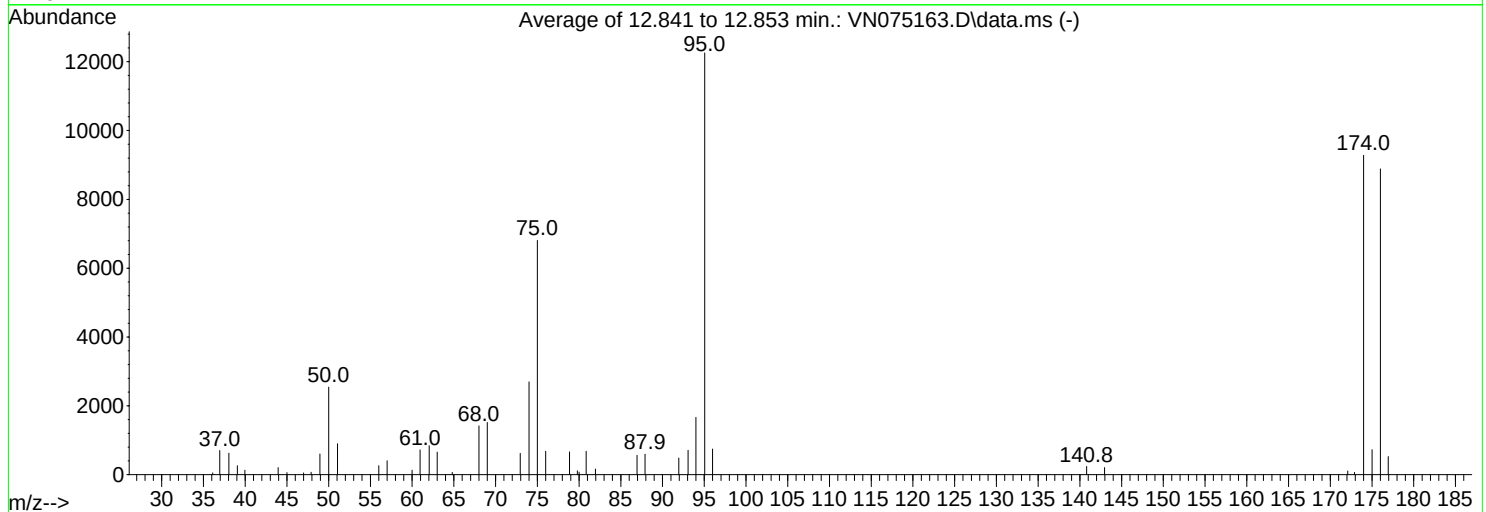


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110422\
 Data File : VN075163.D
 Acq On : 04 Nov 2022 08:35
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
 Title : SW846 8260
 Last Update : Thu Oct 27 09:48:49 2022

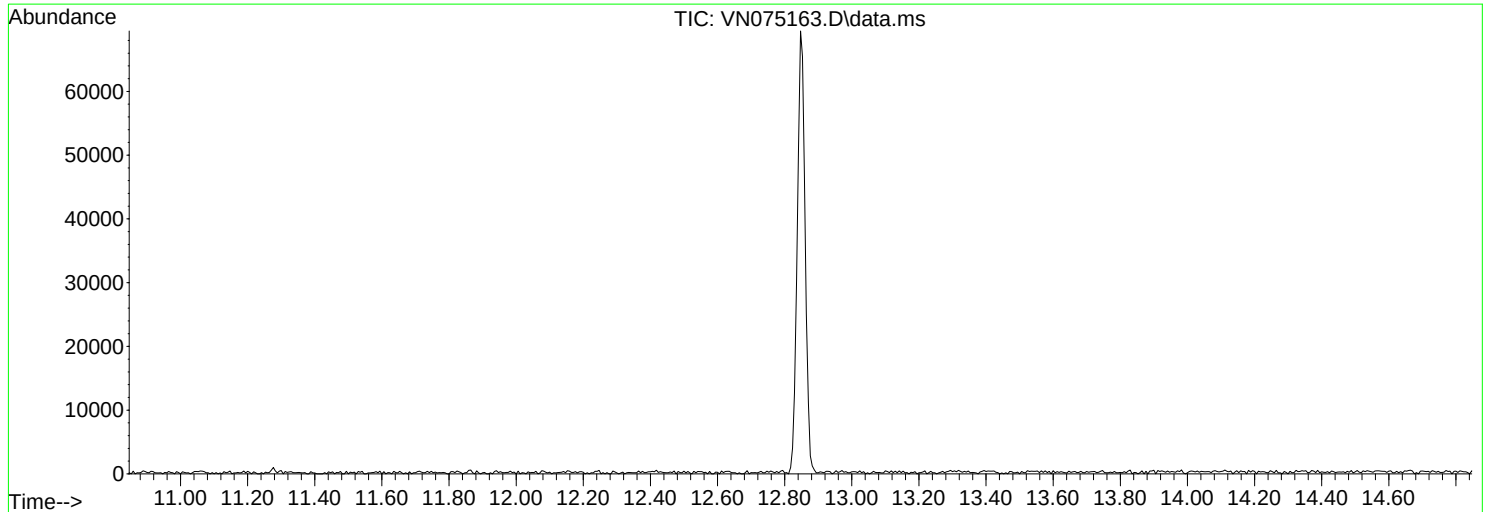

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	2542	PASS
75	95	30	60	55.5	6809	PASS
95	95	100	100	100.0	12258	PASS
96	95	5	9	6.1	745	PASS
173	174	0.00	2	0.7	63	PASS
174	95	50	100	75.7	9282	PASS
175	174	5	9	7.8	727	PASS
176	174	95	101	95.7	8885	PASS
177	176	5	9	5.9	525	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	53	51.05	896	74.00	2695	93.05	70
36.95	700	56.00	262	75.00	6809	94.00	166
38.05	621	57.00	403	76.00	677	95.05	1225
39.05	260	60.00	129	78.85	659	96.00	74
39.95	131	60.95	719	79.80	110	140.80	237
43.95	207	62.05	844	80.00	73	142.95	204
45.00	61	63.00	654	80.85	680	172.10	106
47.00	50	64.80	66	81.95	164	172.90	63
47.90	68	68.00	1417	86.95	564	174.00	9282
48.95	601	69.00	1516	87.90	597	175.00	727
50.00	2542	72.95	619	91.95	486	176.00	8885

Average of 12.841 to 12.853 min.: VN075163.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.95	525						

Instrument :

MSVOA_N

ClientSampleId :

BFB