
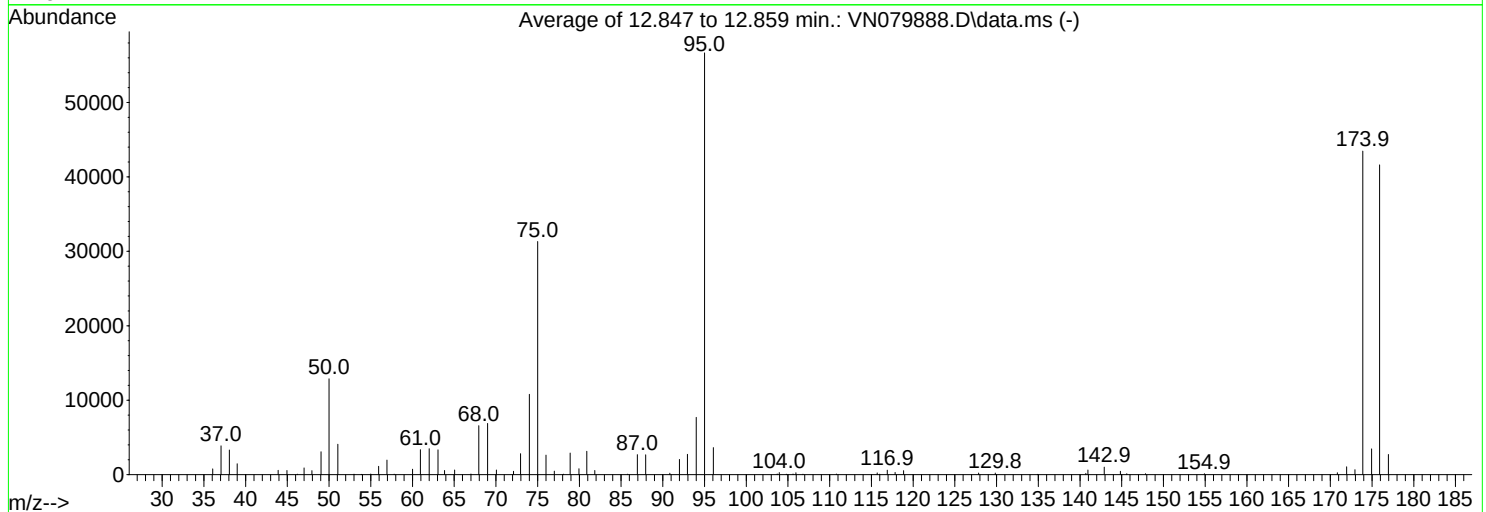


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110423\
Data File : VN079888.D
Acq On : 04 Nov 2023 12:07
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Title : SW846 8260
Last Update : Thu Nov 02 05:49:08 2023

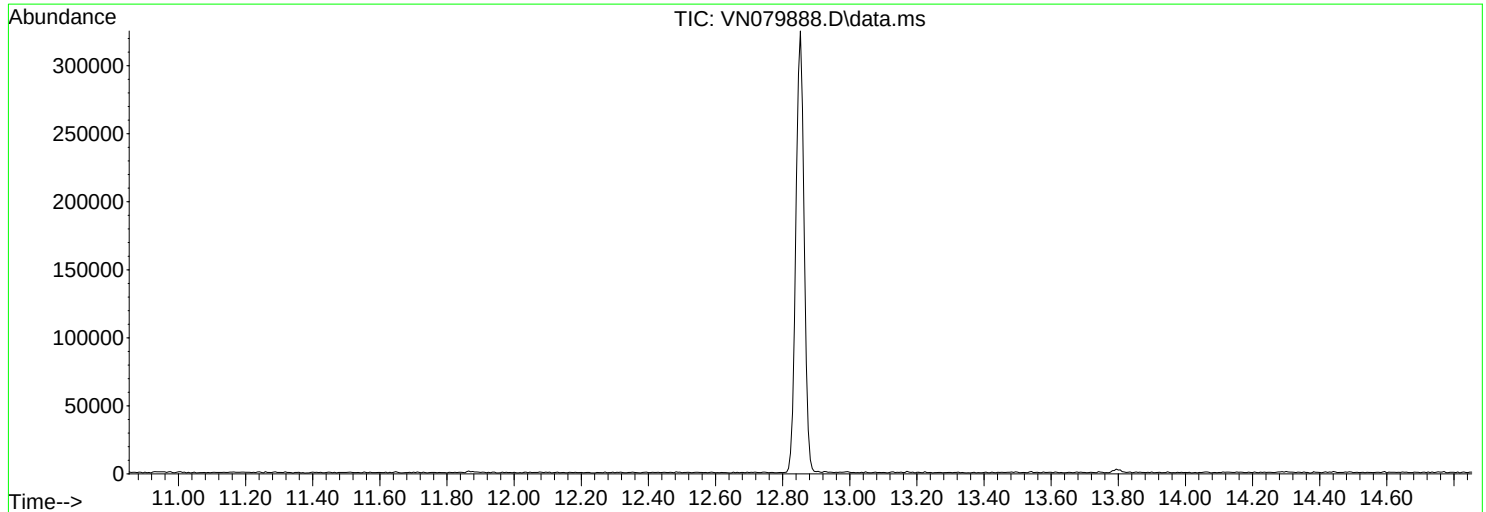

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	12886	PASS
75	95	30	60	55.3	31323	PASS
95	95	100	100	100.0	56664	PASS
96	95	5	9	6.4	3624	PASS
173	174	0.00	2	1.5	658	PASS
174	95	50	100	76.7	43472	PASS
175	174	5	9	7.9	3452	PASS
176	174	95	101	95.7	41621	PASS
177	176	5	9	6.5	2711	PASS

Average of 12.847 to 12.859 min.: VN079888.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	771	50.00	12886	63.05	3337	76.00	2621
37.05	3868	51.05	4085	63.85	557	77.00	461
38.05	3317	53.00	67	65.05	615	78.10	61
39.00	1456	53.90	55	67.00	79	78.90	289
40.00	18	55.00	81	67.95	6568	79.95	803
43.90	590	55.95	1120	69.00	6872	80.90	3138
44.95	550	56.95	1951	70.05	632	81.85	550
46.20	61	57.80	69	72.10	446	85.80	61
47.00	900	60.00	740	72.95	2813	86.95	2696
47.95	535	60.95	3344	74.00	10787	87.95	2664
49.05	3071	62.00	3480	75.00	31323	90.85	193

Average of 12.847 to 12.859 min.: VN079888.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.00	2041	110.80	88	142.90	1004	176.95	2711
92.95	2723	115.70	233	144.85	463		
94.00	7686	116.00	75	145.60	122		
95.00	56664	116.90	609	147.85	136		
96.05	3624	117.85	299	154.90	131		
103.70	84	118.85	537	170.85	254		
103.95	272	127.85	209	171.95	1051		
104.80	60	129.85	215	172.95	658		
105.60	80	134.90	54	173.90	43472		
105.95	250	140.70	173	174.95	3452		
106.80	56	140.95	619	175.90	41621		

Instrument :

MSVOA_N

ClientSampleId :

BFB