


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN110518\
Data File : VN052141.D
Acq On : 5 Nov 2018 11:02
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110518W.M
Title : SW846 8260
Last Update : Mon Nov 05 22:32:25 2018

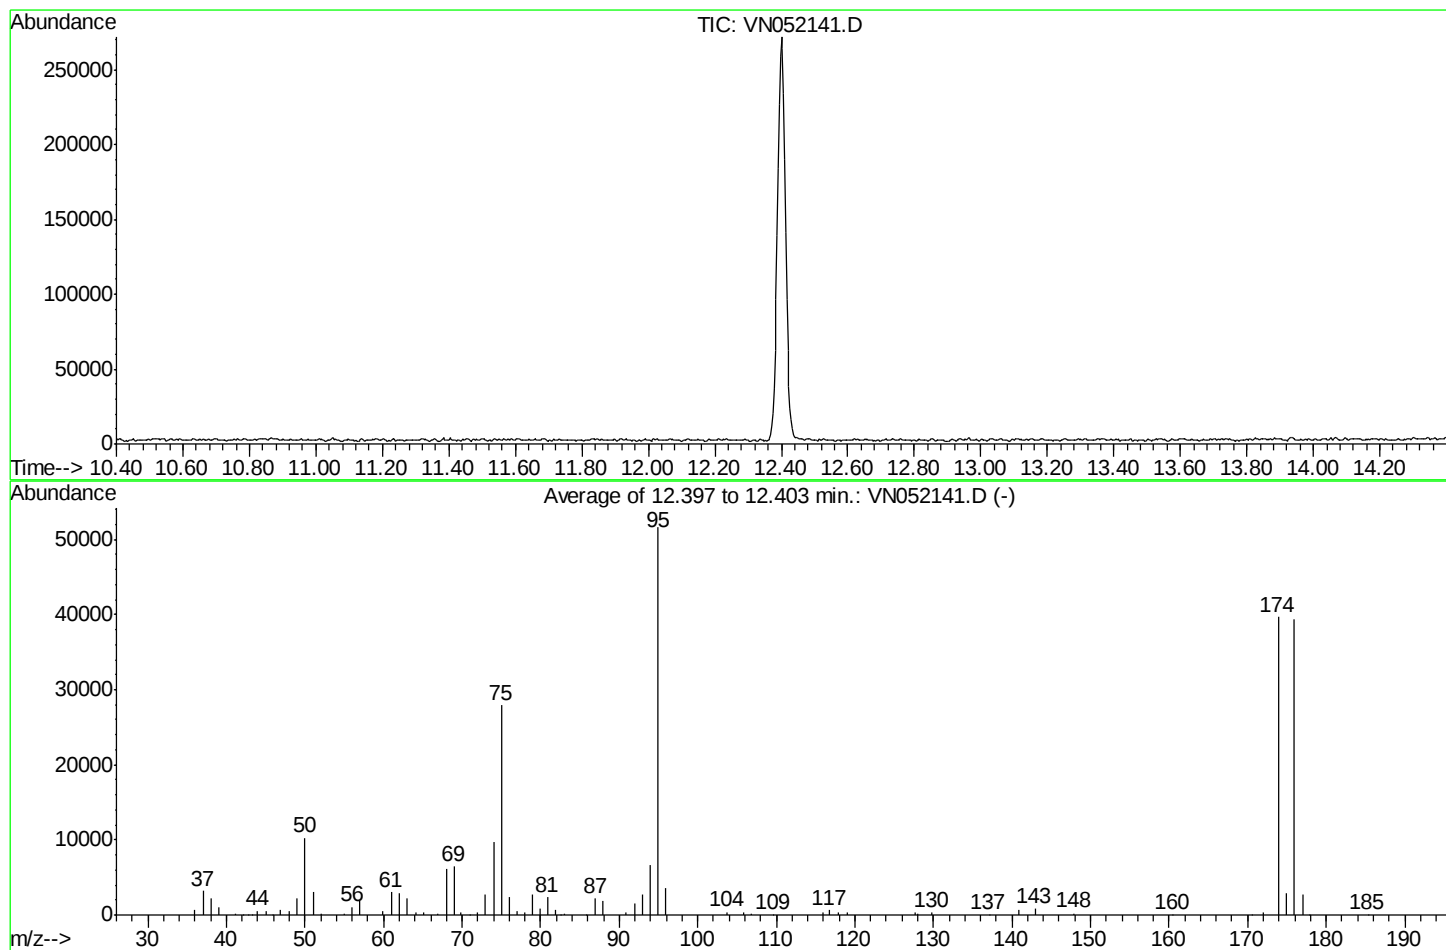

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	10288	PASS
75	95	30	60	54.1	27914	PASS
95	95	100	100	100.0	51624	PASS
96	95	5	9	7.0	3594	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.8	39645	PASS
175	174	5	9	7.4	2951	PASS
176	174	95	101	99.2	39312	PASS
177	176	5	9	7.0	2747	PASS