


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN110518\
 Data File : VN052150.D
 Acq On : 5 Nov 2018 15:56
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 10 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110518W.M
 Title : SW846 8260
 Last Update : Mon Nov 05 22:32:25 2018

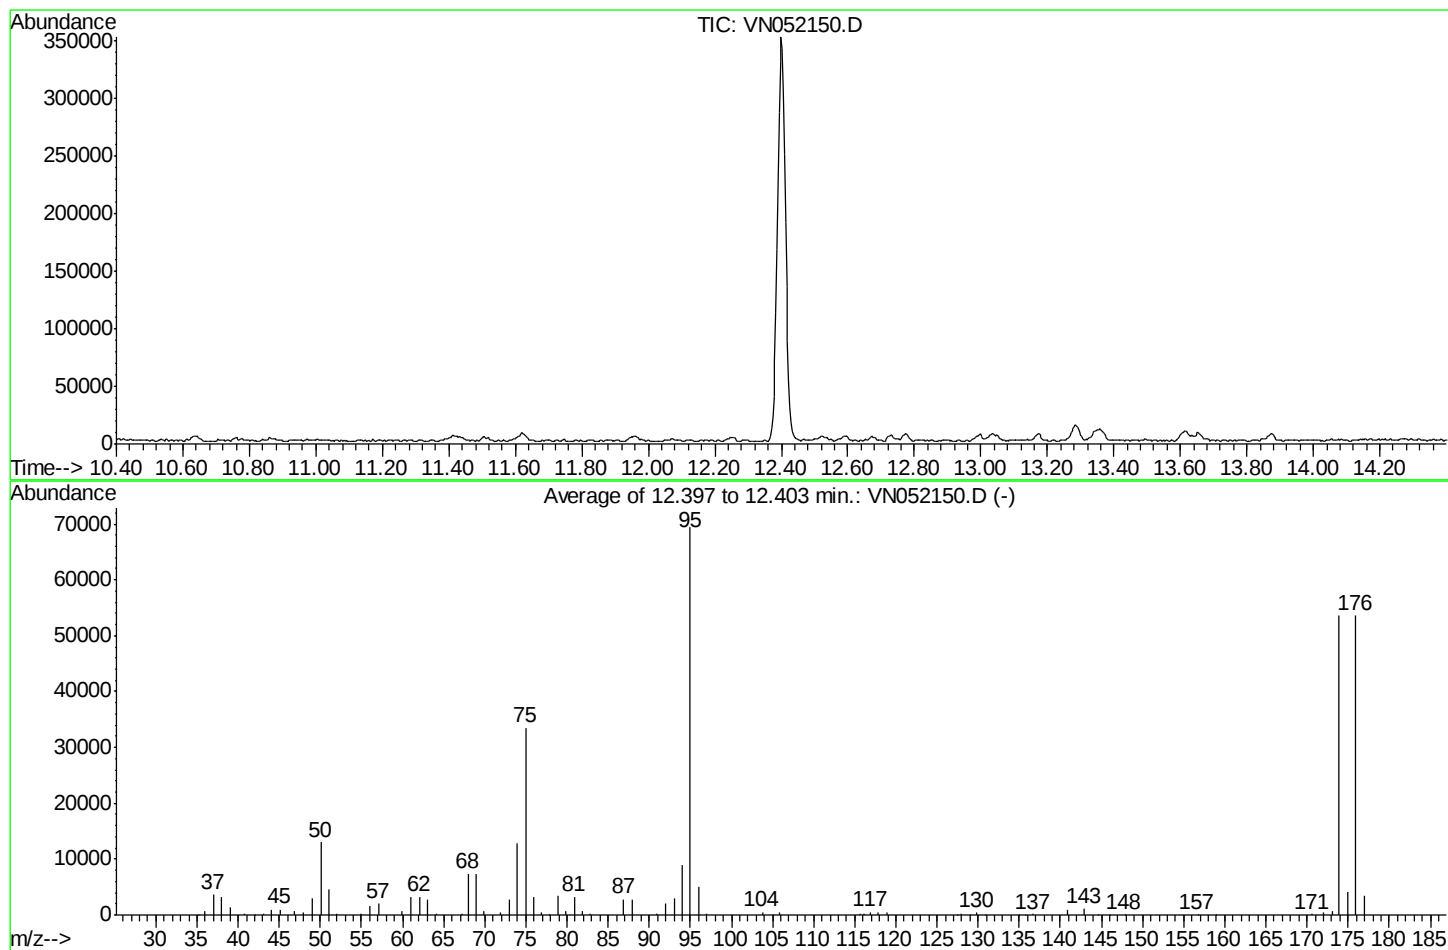

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	13044	PASS
75	95	30	60	48.2	33485	PASS
95	95	100	100	100.0	69402	PASS
96	95	5	9	7.3	5051	PASS
173	174	0.00	2	1.5	807	PASS
174	95	50	100	77.2	53544	PASS
175	174	5	9	7.8	4189	PASS
176	174	95	101	100.0	53546	PASS
177	176	5	9	6.5	3498	PASS