


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN110519\
Data File : VN059082.D
Acq On : 5 Nov 2019 9:41
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110119W.M
Title : SW846 8260
Last Update : Sat Nov 02 05:43:23 2019

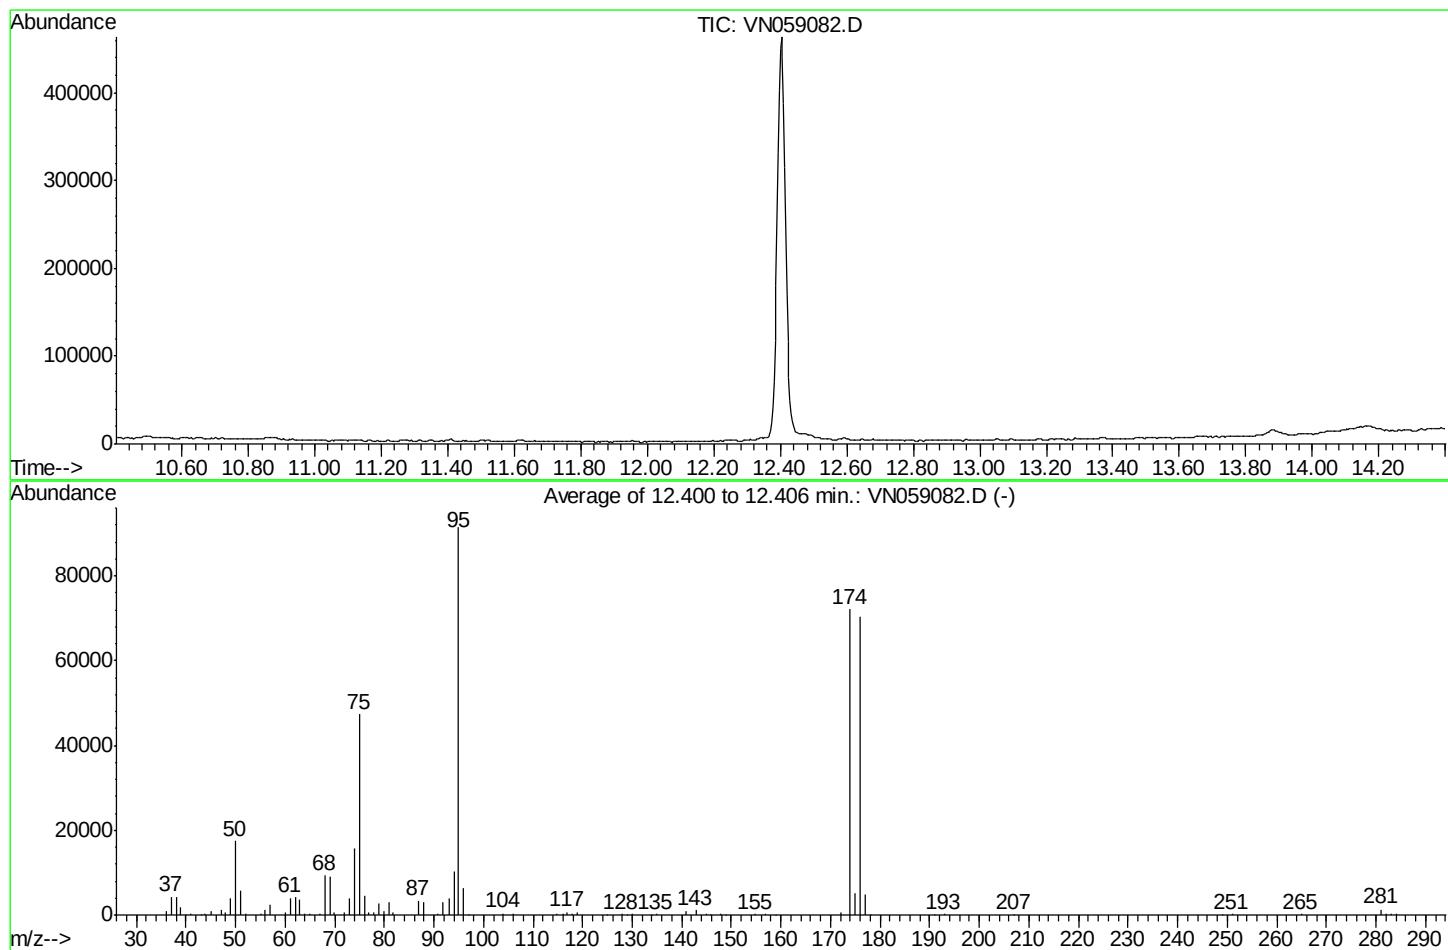

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	17448	PASS
75	95	30	60	51.8	47320	PASS
95	95	100	100	100.0	91434	PASS
96	95	5	9	6.9	6312	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.9	72101	PASS
175	174	5	9	7.0	5067	PASS
176	174	95	101	97.6	70336	PASS
177	176	5	9	6.7	4712	PASS