

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN110520\
 Data File : VN064453.D
 Acq On : 5 Nov 2020 11:51
 Operator : JC/MD
 Sample : VN1105WBL01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1105WBL01

Quant Time: Nov 06 03:00:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 04 12:09:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	248824	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	499734	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	518311	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	190281	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	240377	55.46	ug/l	0.00
Spiked Amount 50.000			Recovery	=	110.92%	
35) Dibromofluoromethane	7.55	113	173472	50.98	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.96%	
50) Toluene-d8	10.06	98	643667	48.95	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.90%	
62) 4-Bromofluorobenzene	12.38	95	245148	49.29	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.58%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN110520\
Data File : VN064453.D
Acq On : 5 Nov 2020 11:51
Operator : JC/MD
Sample : VN1105WBL01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1105WBL01

Quant Time: Nov 06 03:00:03 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 04 12:09:03 2020
Response via : Initial Calibration

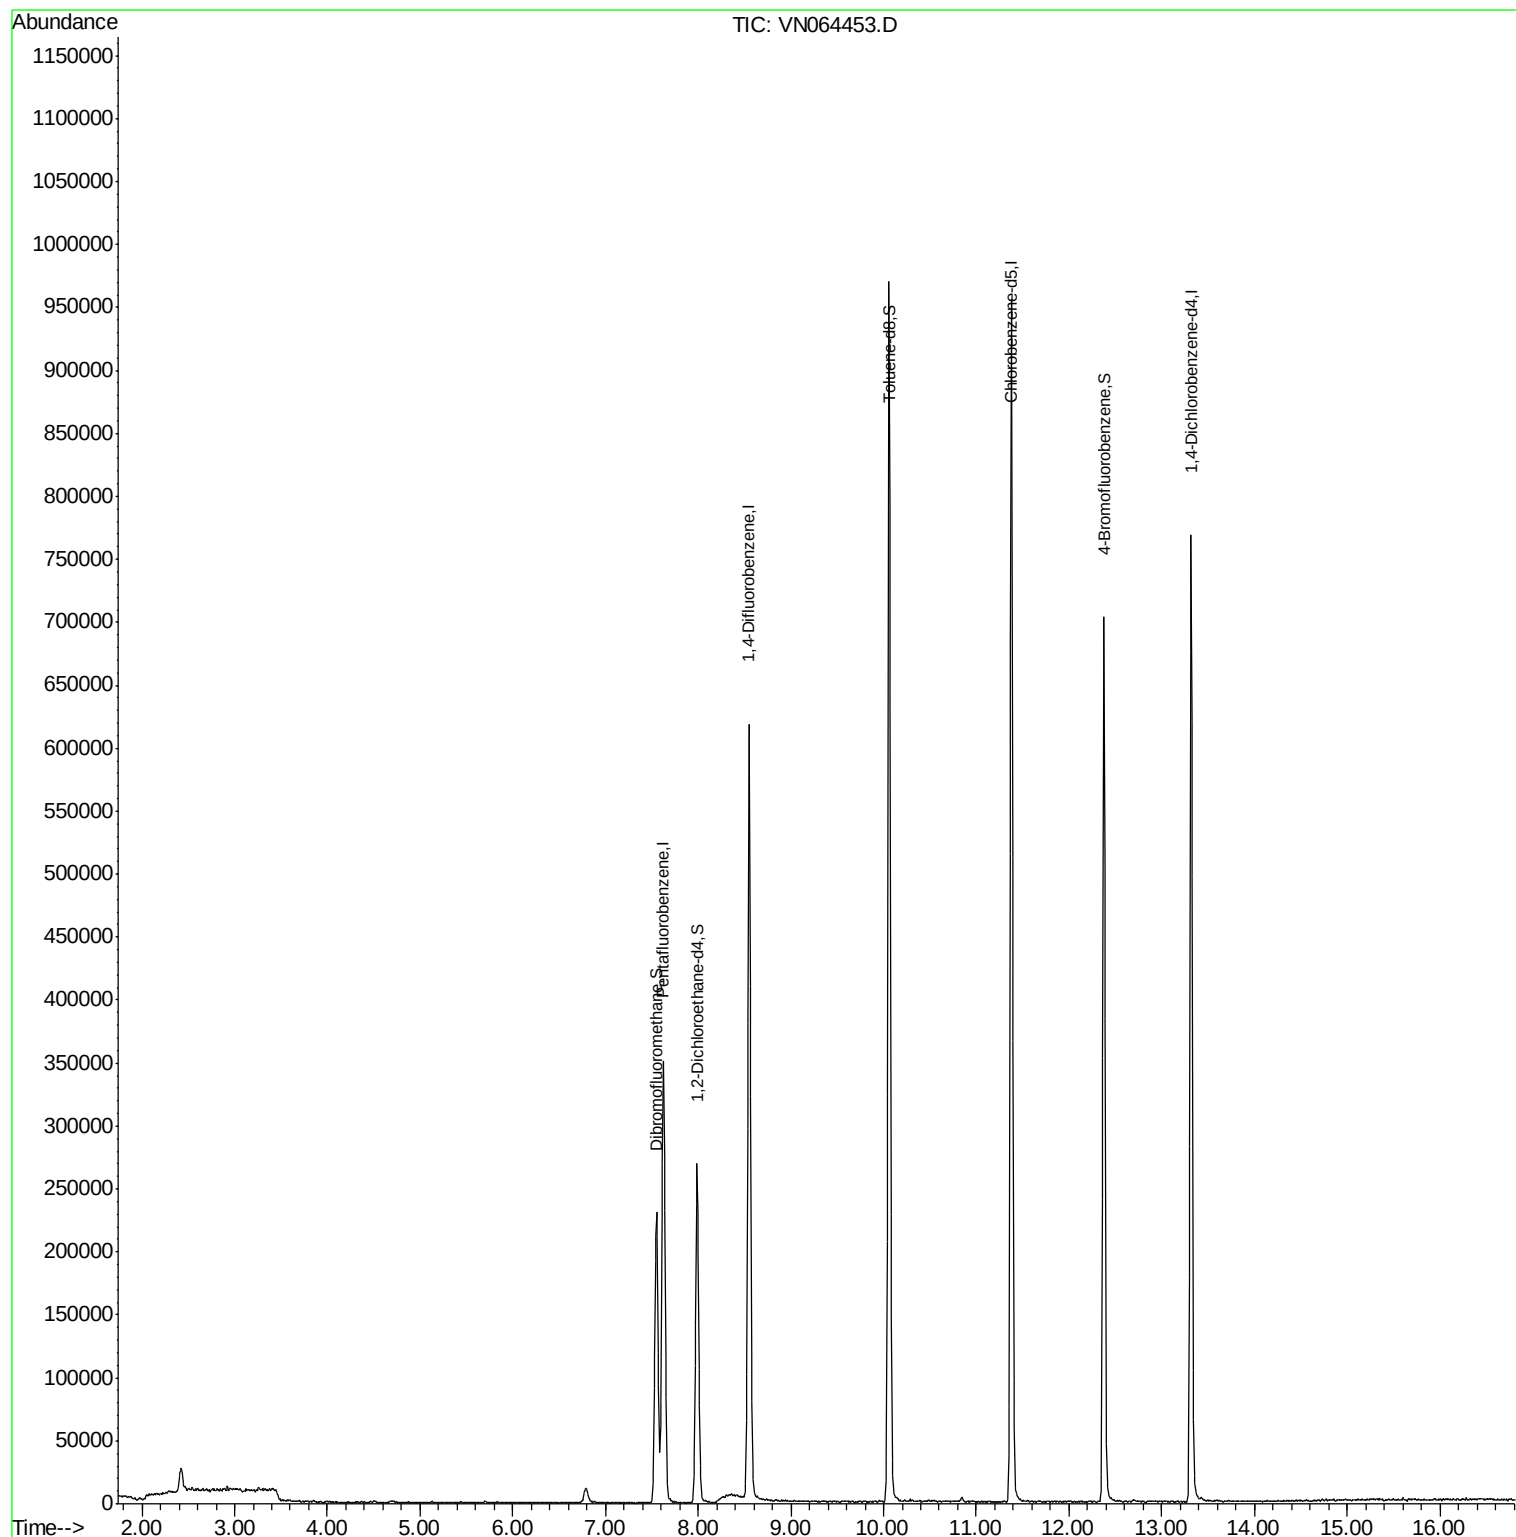

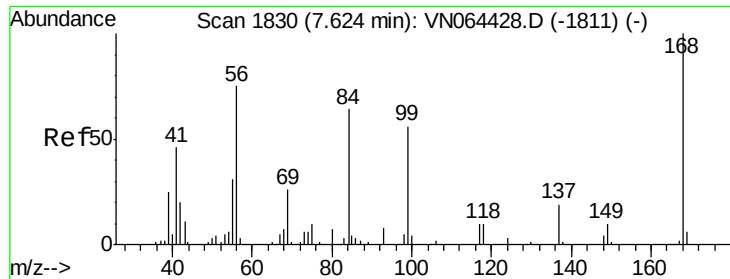

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064453.D

Acq: 5 Nov 2020 11:51

Instrument :

MSVOA_N

ClientSampleId :


VN1105WBL01

Tot Ion:168 Resp: 248824

Ion Ratio Lower Upper

168 100

99 66.6 53.4 80.2

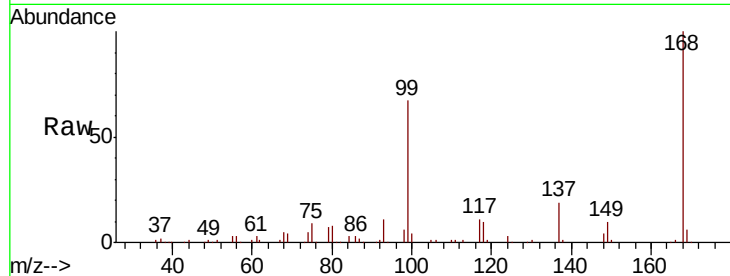

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.63

120000

100000

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70

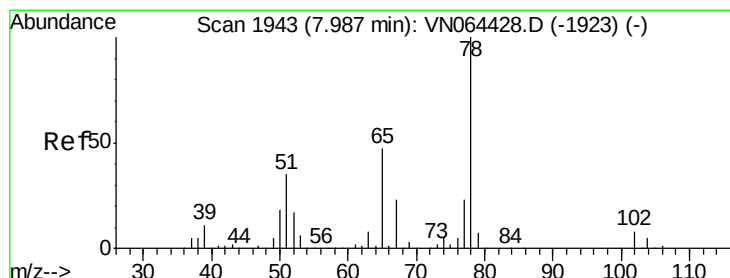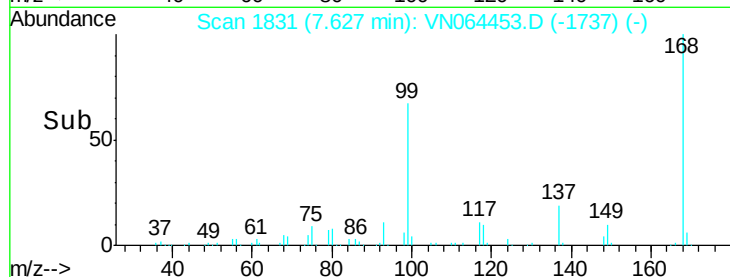

#33

1,2-Dichloroethane-d4

Concen: 55.461 ug/l

RT: 7.99 min Scan# 1943

Delta R.T. -0.00 min

Lab File: VN064453.D


Acq: 5 Nov 2020 11:51

Tgt Ion: 65 Resp: 240377

Ion Ratio Lower Upper

65 100

67 50.1 0.0 101.6

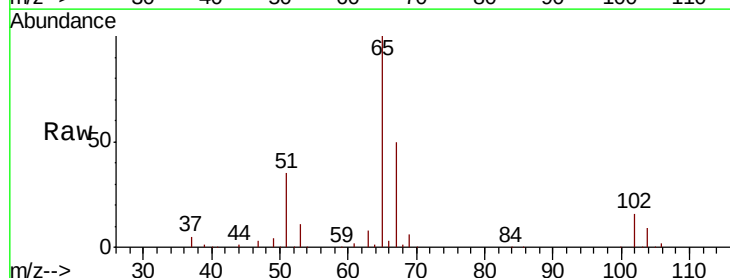

Abundance Ion 64.90 (64.60 to 65.60): VN

Ion 66.90 (66.60 to 67.60): VN

7.99

120000

100000

80000


60000


40000

20000

0

Time--> 7.90 8.00 8.10

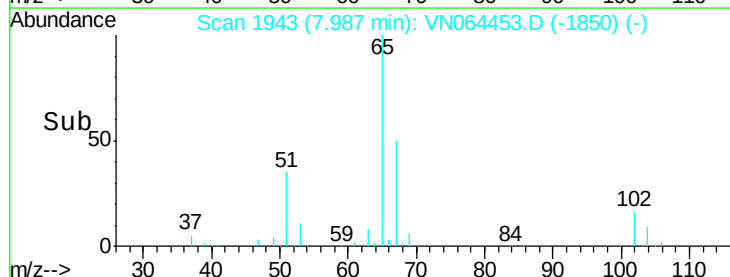


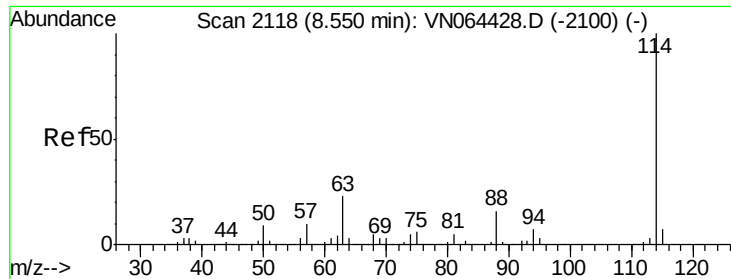




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.55 min Scan# 2118
Delta R.T. -0.00 min
Lab File: VN064453.D
Acq: 5 Nov 2020 11:51

Instrument :
MSVOA_N
ClientSampleId :
VN1105WBL01

Tot Ion:114 Resp: 499734
Ion Ratio Lower Upper
114 100
63 24.1 0.0 45.6
88 16.5 0.0 32.8

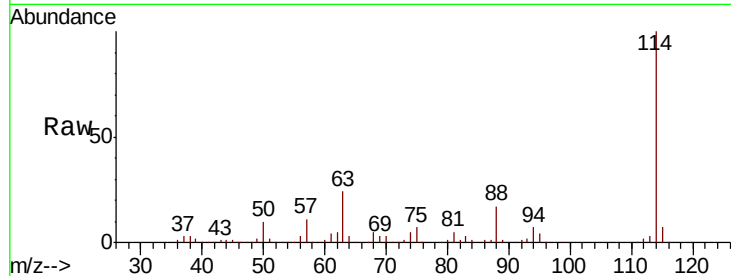


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VN
Ion 87.90 (87.60 to 88.60): VN

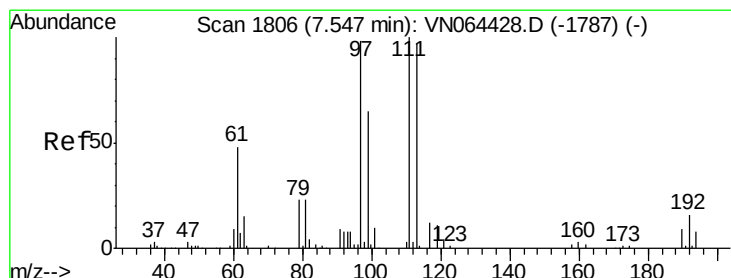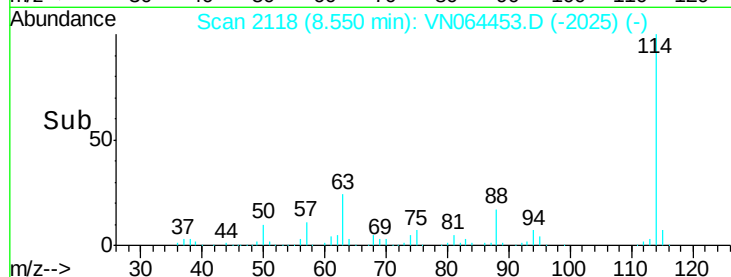
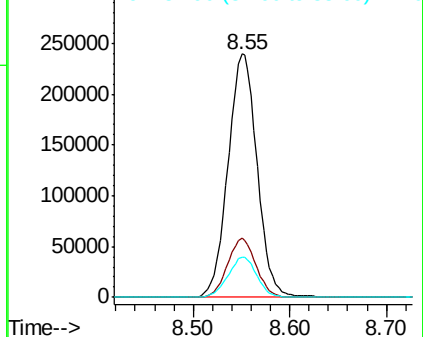



#35
Dibromofluoromethane
Concen: 50.984 ug/l
RT: 7.55 min Scan# 1807
Delta R.T. 0.00 min
Lab File: VN064453.D
Acq: 5 Nov 2020 11:51

Tgt Ion:113 Resp: 173472
Ion Ratio Lower Upper
113 100
111 102.3 81.1 121.7
192 15.7 12.8 19.2

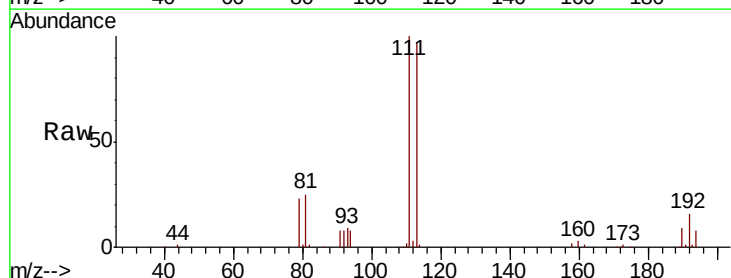

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

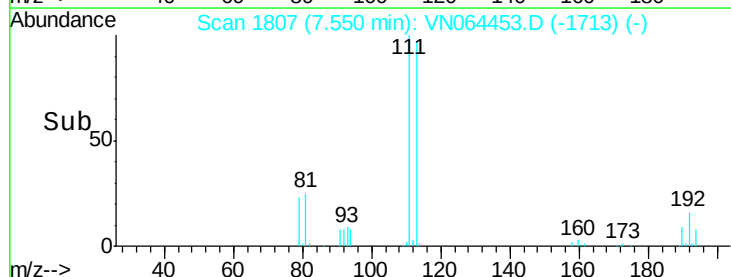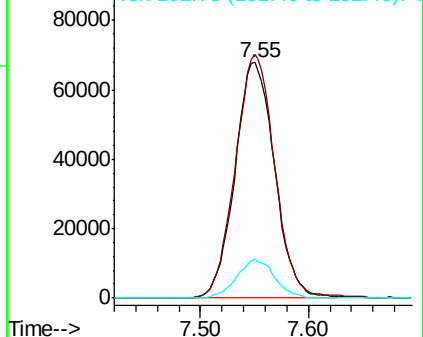

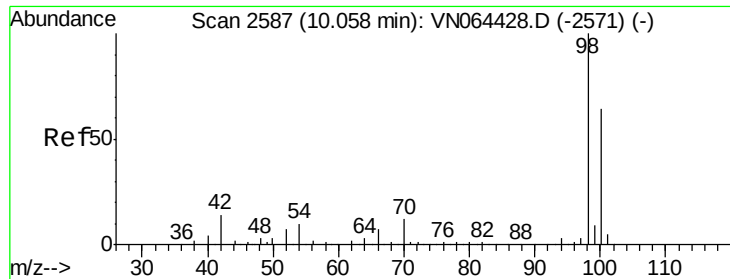

#50

Toluene-d8

Concen: 48.945 ug/l

RT: 10.06 min Scan# 2588

Delta R.T. 0.00 min

Lab File: VN064453.D

Acq: 5 Nov 2020 11:51

Instrument :

MSVOA_N

ClientSampleId :


VN1105WBL01

Tot Ion: 98 Resp: 643667

Ion Ratio Lower Upper

98 100

100 64.2 50.7 76.1

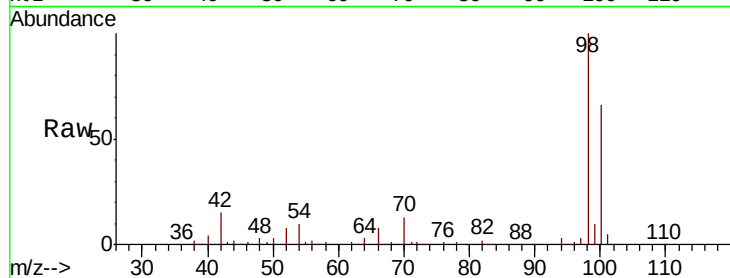

Abundance Ion 98.00 (97.70 to 98.70): VN064428.D (-2571) (-)

Ion 100.00 (99.70 to 100.70): VN064428.D (-2571) (-)

10.06



300000

200000

100000

0

Time-->

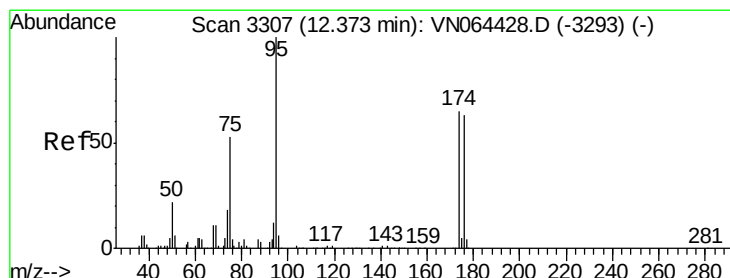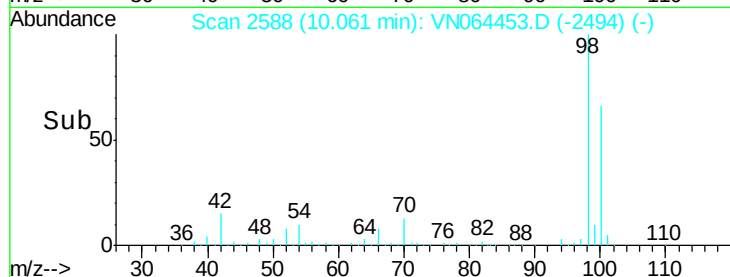

#62

4-Bromofluorobenzene

Concen: 49.292 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.00 min

Lab File: VN064453.D

Acq: 5 Nov 2020 11:51


Tgt Ion: 95 Resp: 245148

Ion Ratio Lower Upper

95 100

174 68.8 0.0 132.6

176 66.8 0.0 129.2

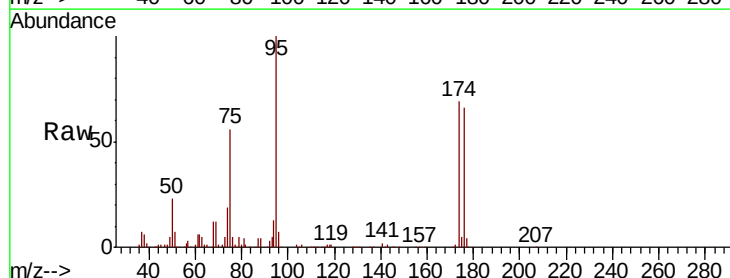

Abundance Ion 94.90 (94.60 to 95.60): VN064428.D (-3293) (-)

Ion 173.80 (173.50 to 174.50): VN064428.D (-3293) (-)

Ion 175.80 (175.50 to 176.50): VN064428.D (-3293) (-)

12.38


150000


100000

50000

0

Time-->

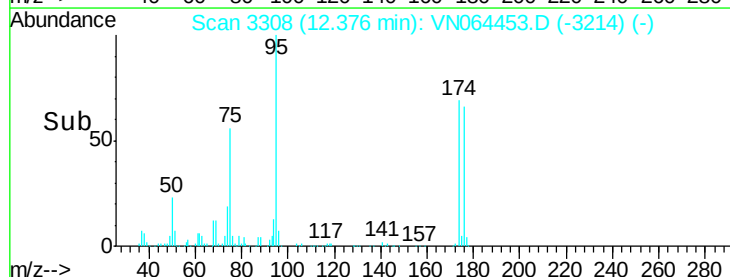


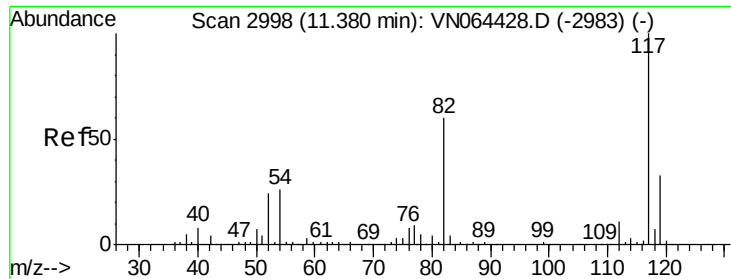




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. -0.00 min
Lab File: VN064453.D
Acq: 5 Nov 2020 11:51

Instrument :
MSVOA_N
ClientSampleId :
VN1105WBL01

Tot Ion:117 Resp: 518311
Ion Ratio Lower Upper
117 100
82 57.9 48.1 72.1
119 32.3 26.2 39.4

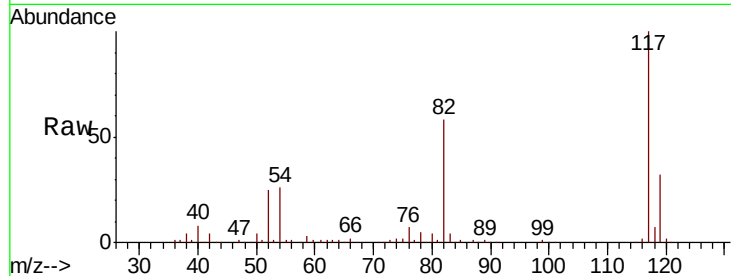


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VN
Ion 118.90 (118.60 to 119.60): V

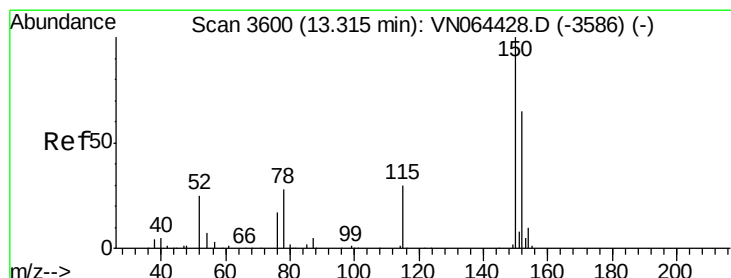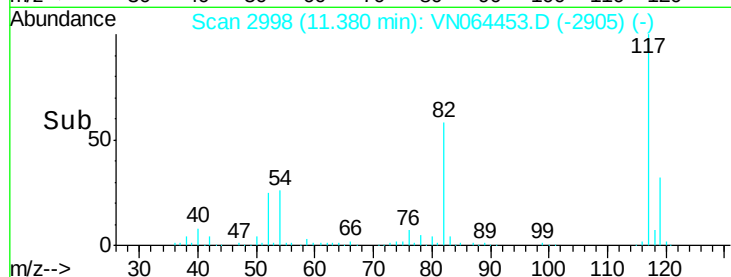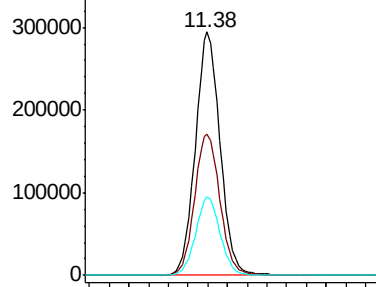

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN064453.D
Acq: 5 Nov 2020 11:51

Tgt Ion:152 Resp: 190281
Ion Ratio Lower Upper
152 100
115 65.6 32.0 96.0
150 156.0 0.0 353.8

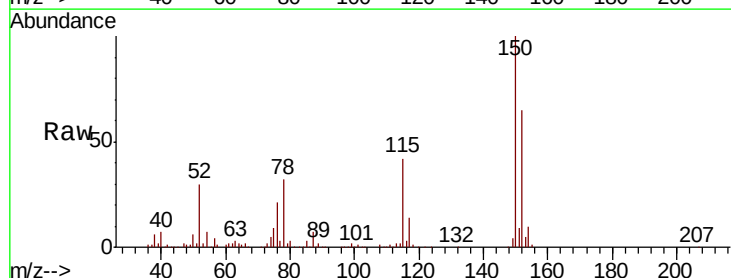

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

