
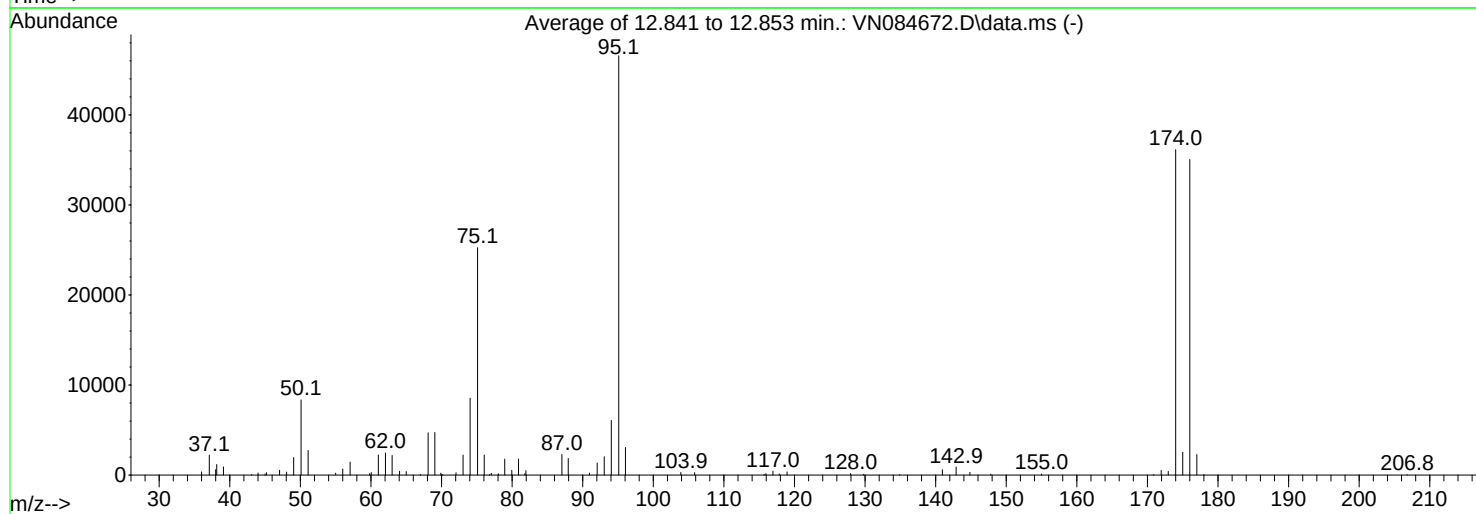


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110524\
Data File : VN084672.D
Acq On : 05 Nov 2024 08:06
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Title : SW846 8260
Last Update : Thu Oct 31 18:45:38 2024

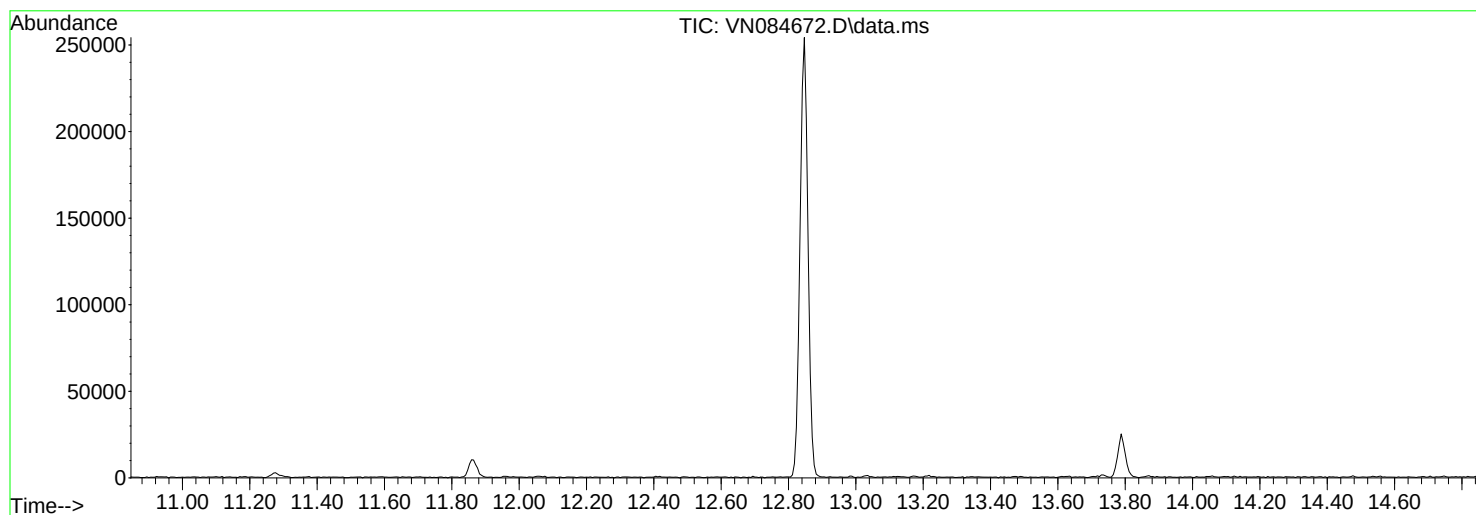

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	8351	PASS
75	95	30	60	54.3	25267	PASS
95	95	100	100	100.0	46573	PASS
96	95	5	9	6.6	3060	PASS
173	174	0.00	2	1.1	408	PASS
174	95	50	100	77.6	36147	PASS
175	174	5	9	7.0	2541	PASS
176	174	95	101	96.9	35043	PASS
177	176	5	9	6.5	2283	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	353	49.05	1954	64.05	424	76.05	2222
37.10	2223	50.10	8351	65.00	390	76.80	60
38.00	613	51.10	2734	67.00	67	77.05	202
38.15	1173	55.00	215	68.10	4691	78.05	153
39.10	909	56.00	675	69.05	4733	78.95	1769
43.10	54	57.05	1451	69.90	221	79.95	527
44.00	243	59.80	170	70.10	68	80.90	1790
45.00	123	60.05	276	72.05	263	81.80	151
45.20	273	61.05	2230	73.05	2222	81.95	498
47.05	540	62.05	2461	74.05	8535	87.05	2288
48.05	332	63.00	2182	75.10	25267	87.95	1845

Average of 12.841 to 12.853 min.: VN084672.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.95	226	117.85	123	171.95	530		
92.05	1334	118.95	360	172.95	408		
93.05	2034	127.95	167	174.00	36147		
94.05	6069	129.80	92	175.00	2541		
95.10	46573	134.90	50	176.00	35043		
96.05	3060	140.95	593	177.00	2283		
103.90	299	142.90	888	178.00	59		
105.85	277	144.85	312	206.80	53		
115.70	55	147.80	107				
115.95	165	155.00	123				
116.95	439	170.90	62				

Instrument :

MSVOA_N

ClientSampleId :

BFB