



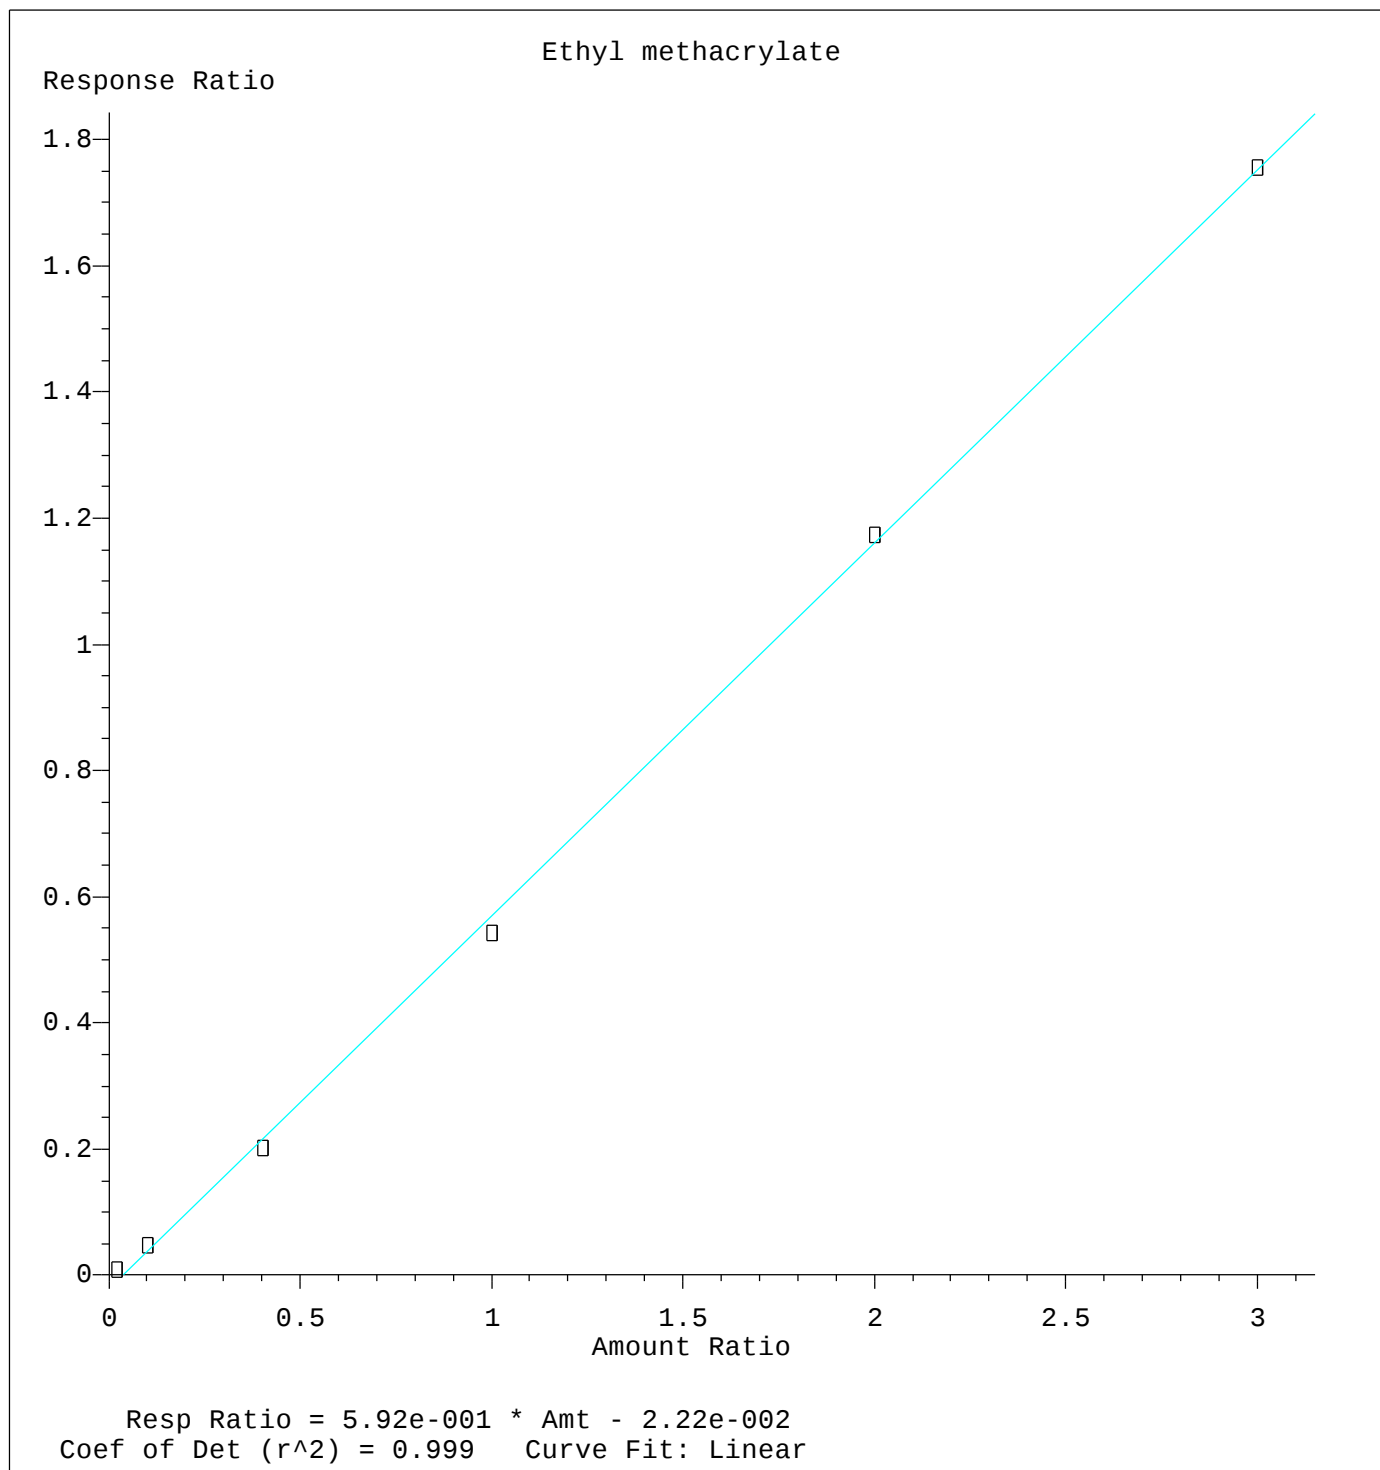

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110619W.M
Calibration Table Last Updated: Thu Nov 07 04:00:41 2019

1,2-Dibromo-3-Chloropropane

Response Ratio

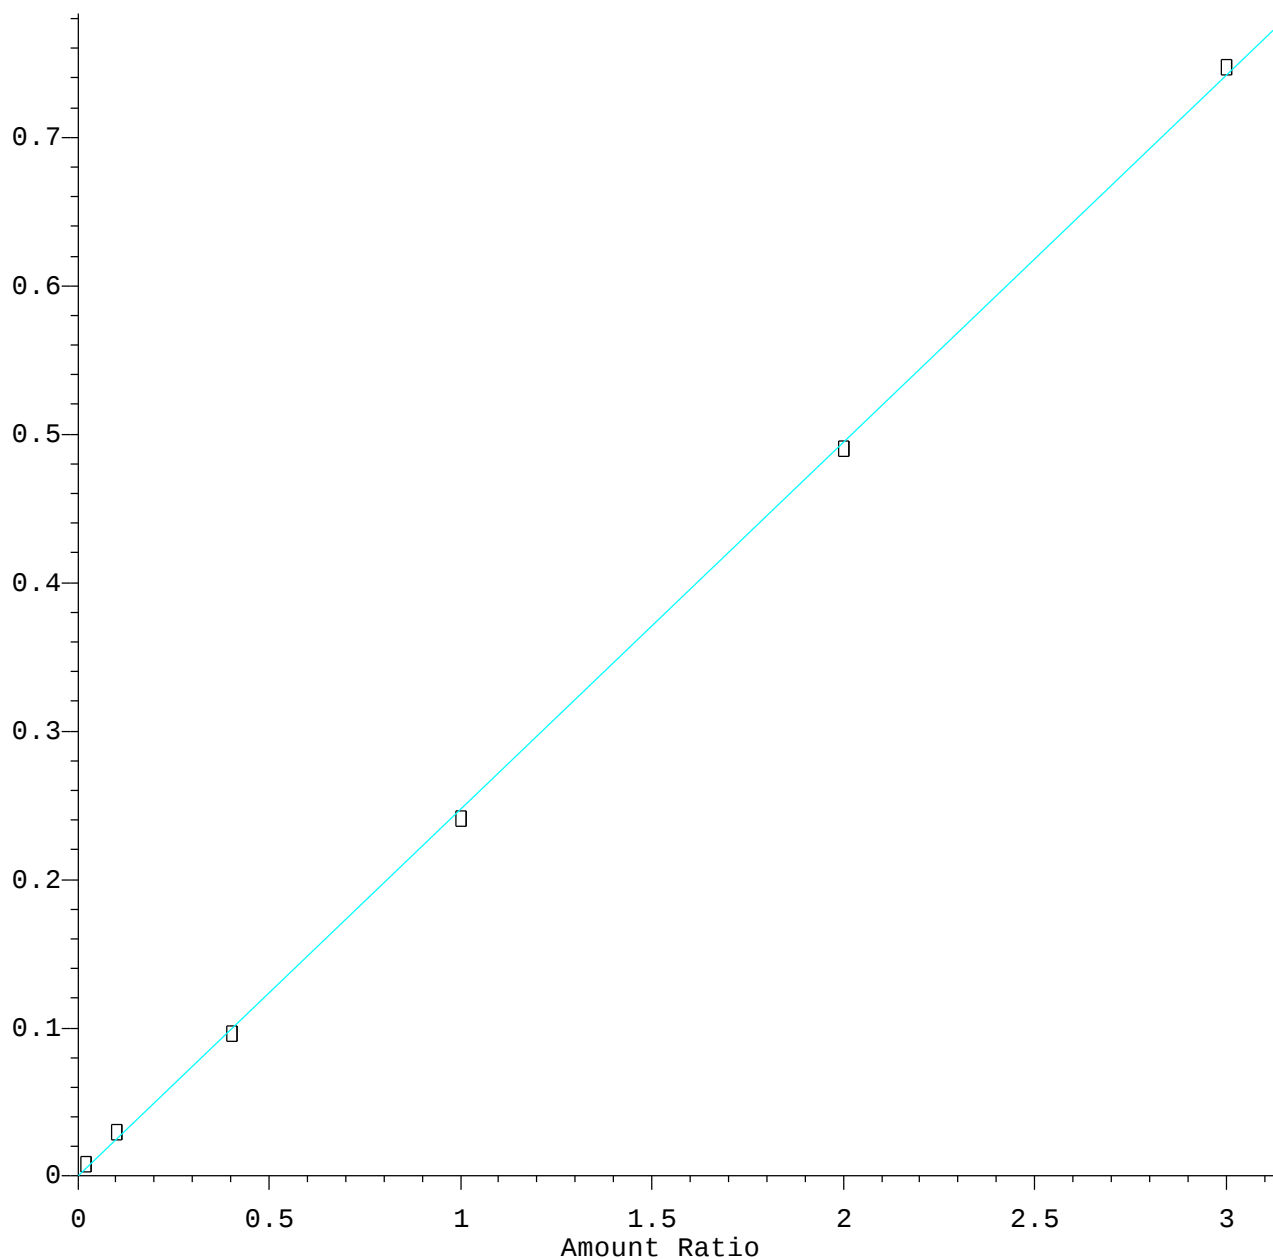


Resp Ratio = 2.47e-001 * Amt - 1.30e-004
Coef of Det (r²) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110619W.M
Calibration Table Last Updated: Thu Nov 07 04:00:41 2019


1,2,4-Trichlorobenzene

Response Ratio

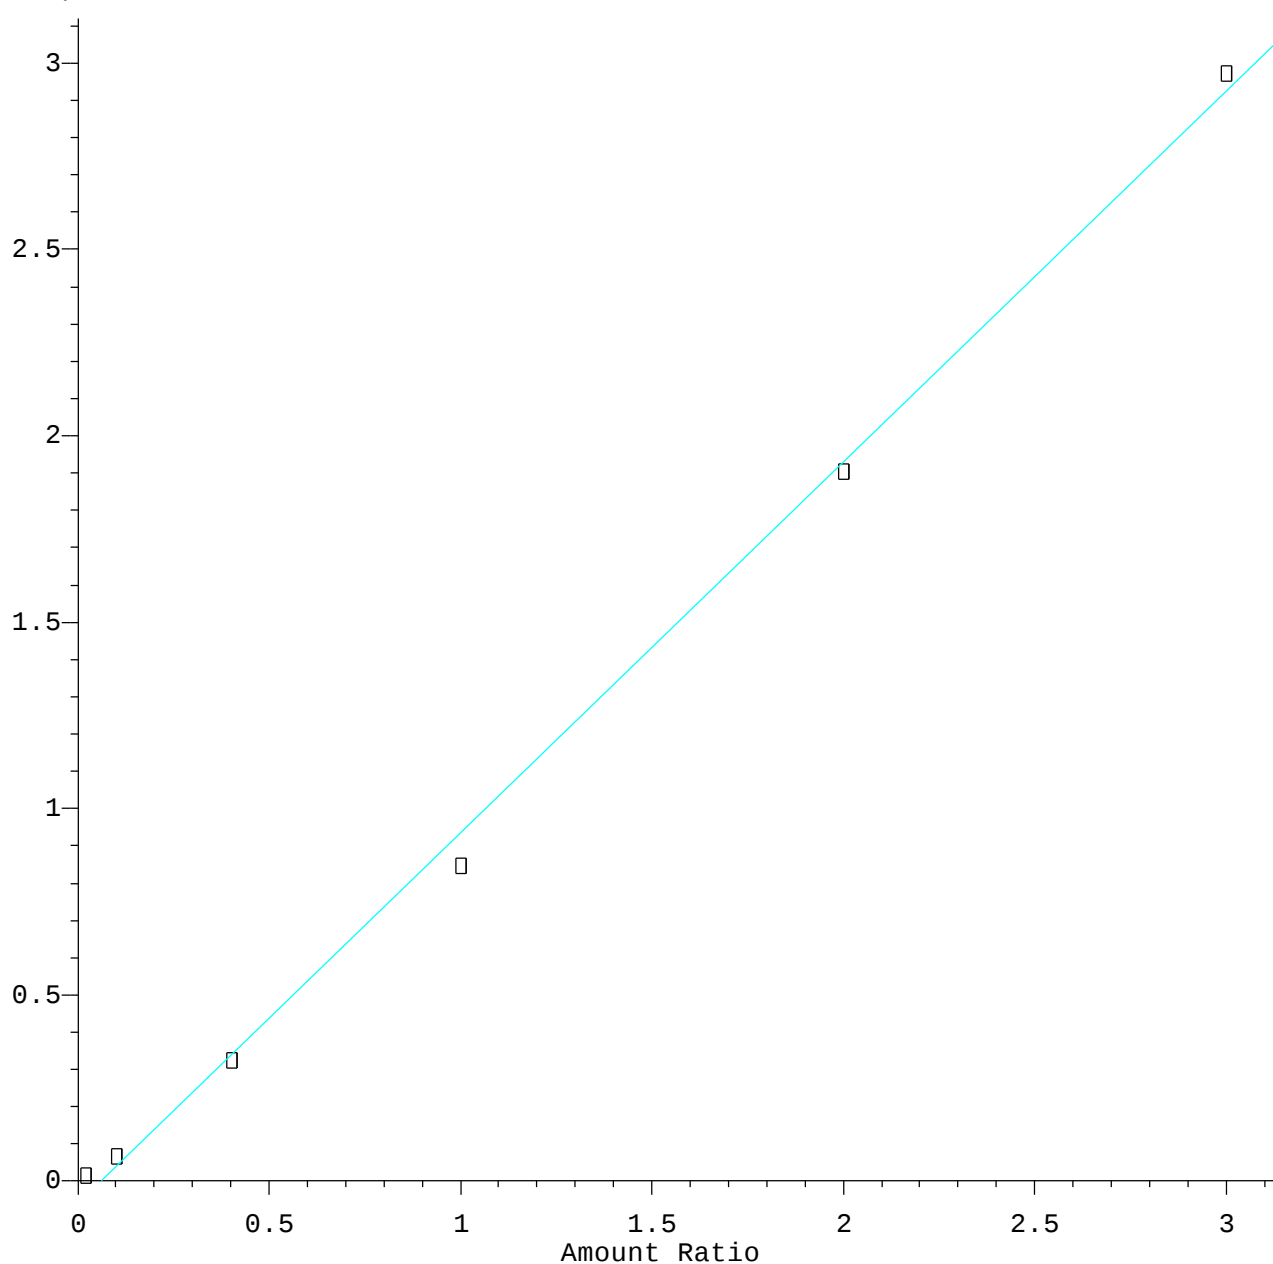

Resp Ratio = 9.94×10^{-1} * Amt - 6.06×10^{-2}
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110619W.M
Calibration Table Last Updated: Thu Nov 07 04:00:41 2019

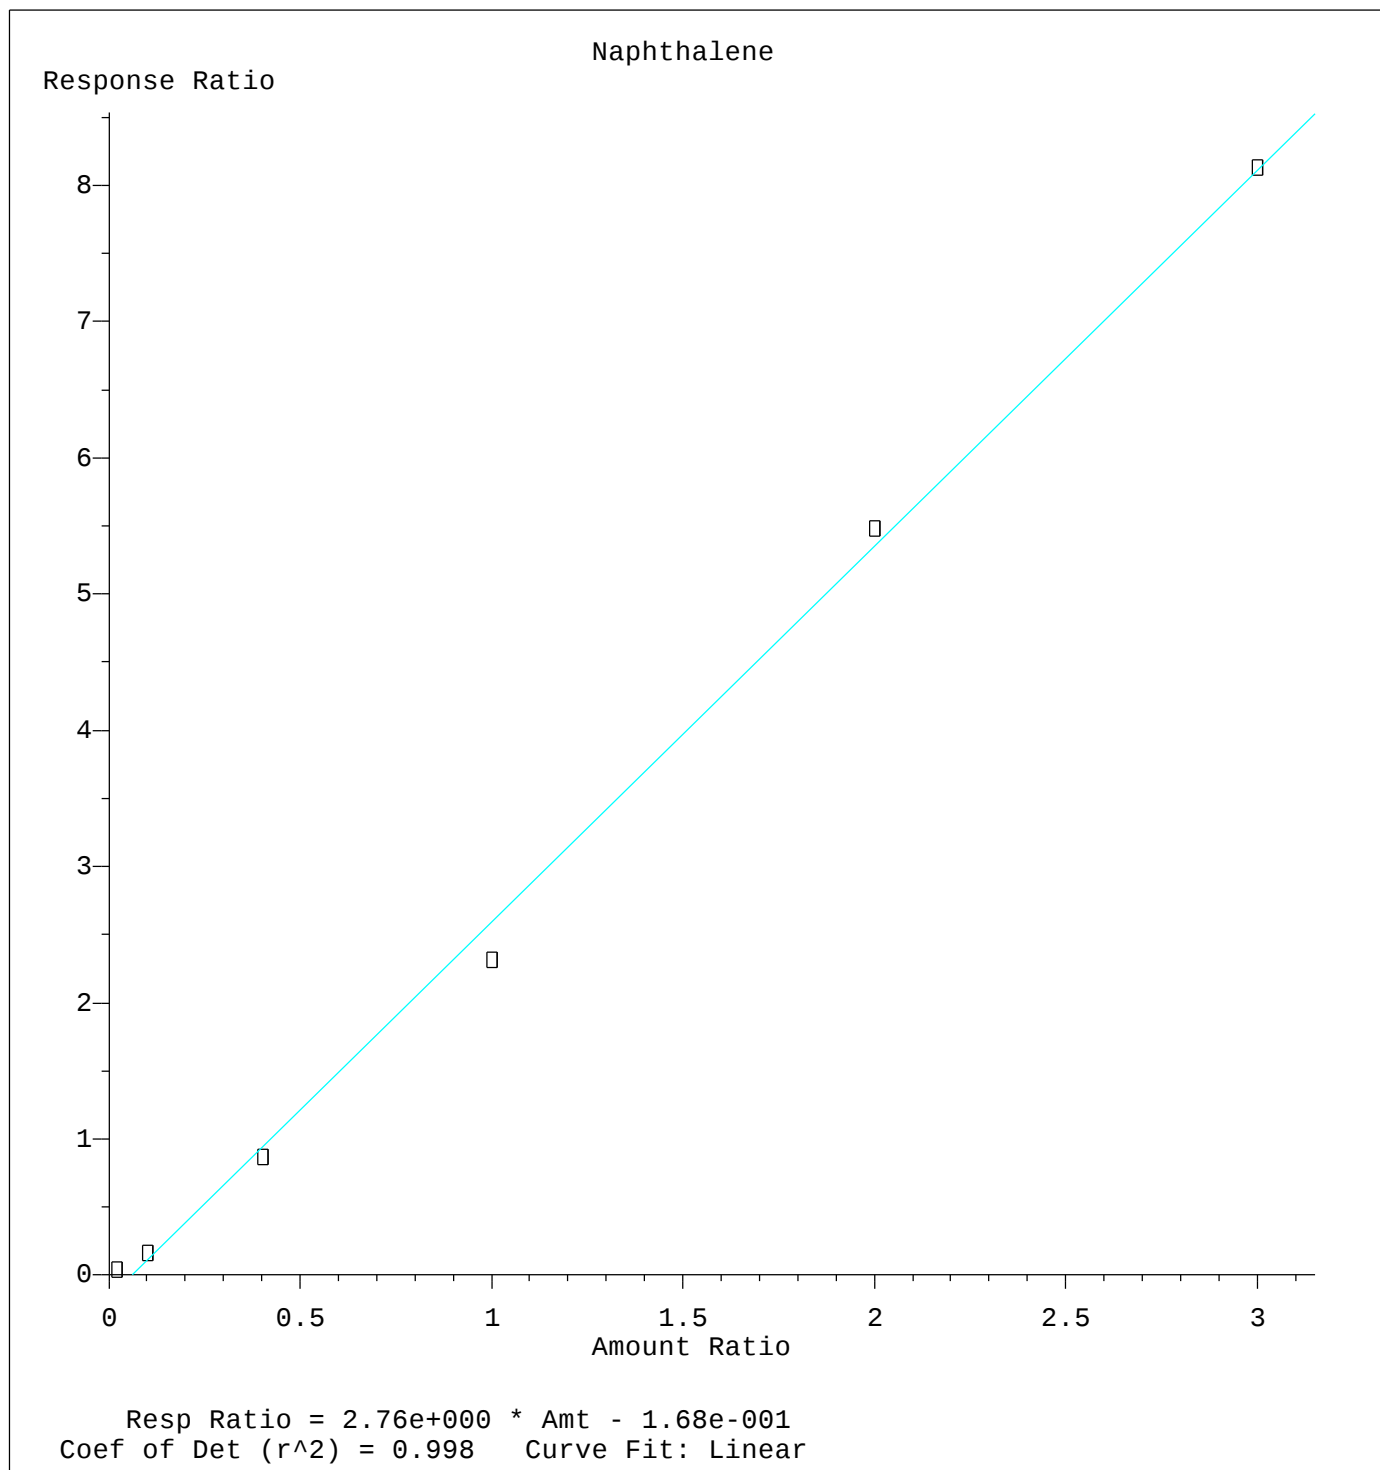

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110619W.M
Calibration Table Last Updated: Thu Nov 07 04:00:41 2019