

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN110619\
 Data File : VN059100.D
 Acq On : 6 Nov 2019 12:29
 Operator : JC/SP
 Sample : VN1106WBL01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1106WBL01

Quant Time: Nov 07 04:14:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110619W.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 07 04:00:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	463590	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.57	114	723498	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	627504	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	225638	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.00	65	288930	50.70	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.40%	
35) Dibromofluoromethane	7.57	113	225447	52.19	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.38%	
50) Toluene-d8	10.08	98	874356	51.38	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.76%	
62) 4-Bromofluorobenzene	12.40	95	279443	45.55	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.10%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN110619\
Data File : VN059100.D
Acq On : 6 Nov 2019 12:29
Operator : JC/SP
Sample : VN1106WBL01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1106WBL01

Quant Time: Nov 07 04:14:35 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N110619W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 07 04:00:41 2019
Response via : Initial Calibration

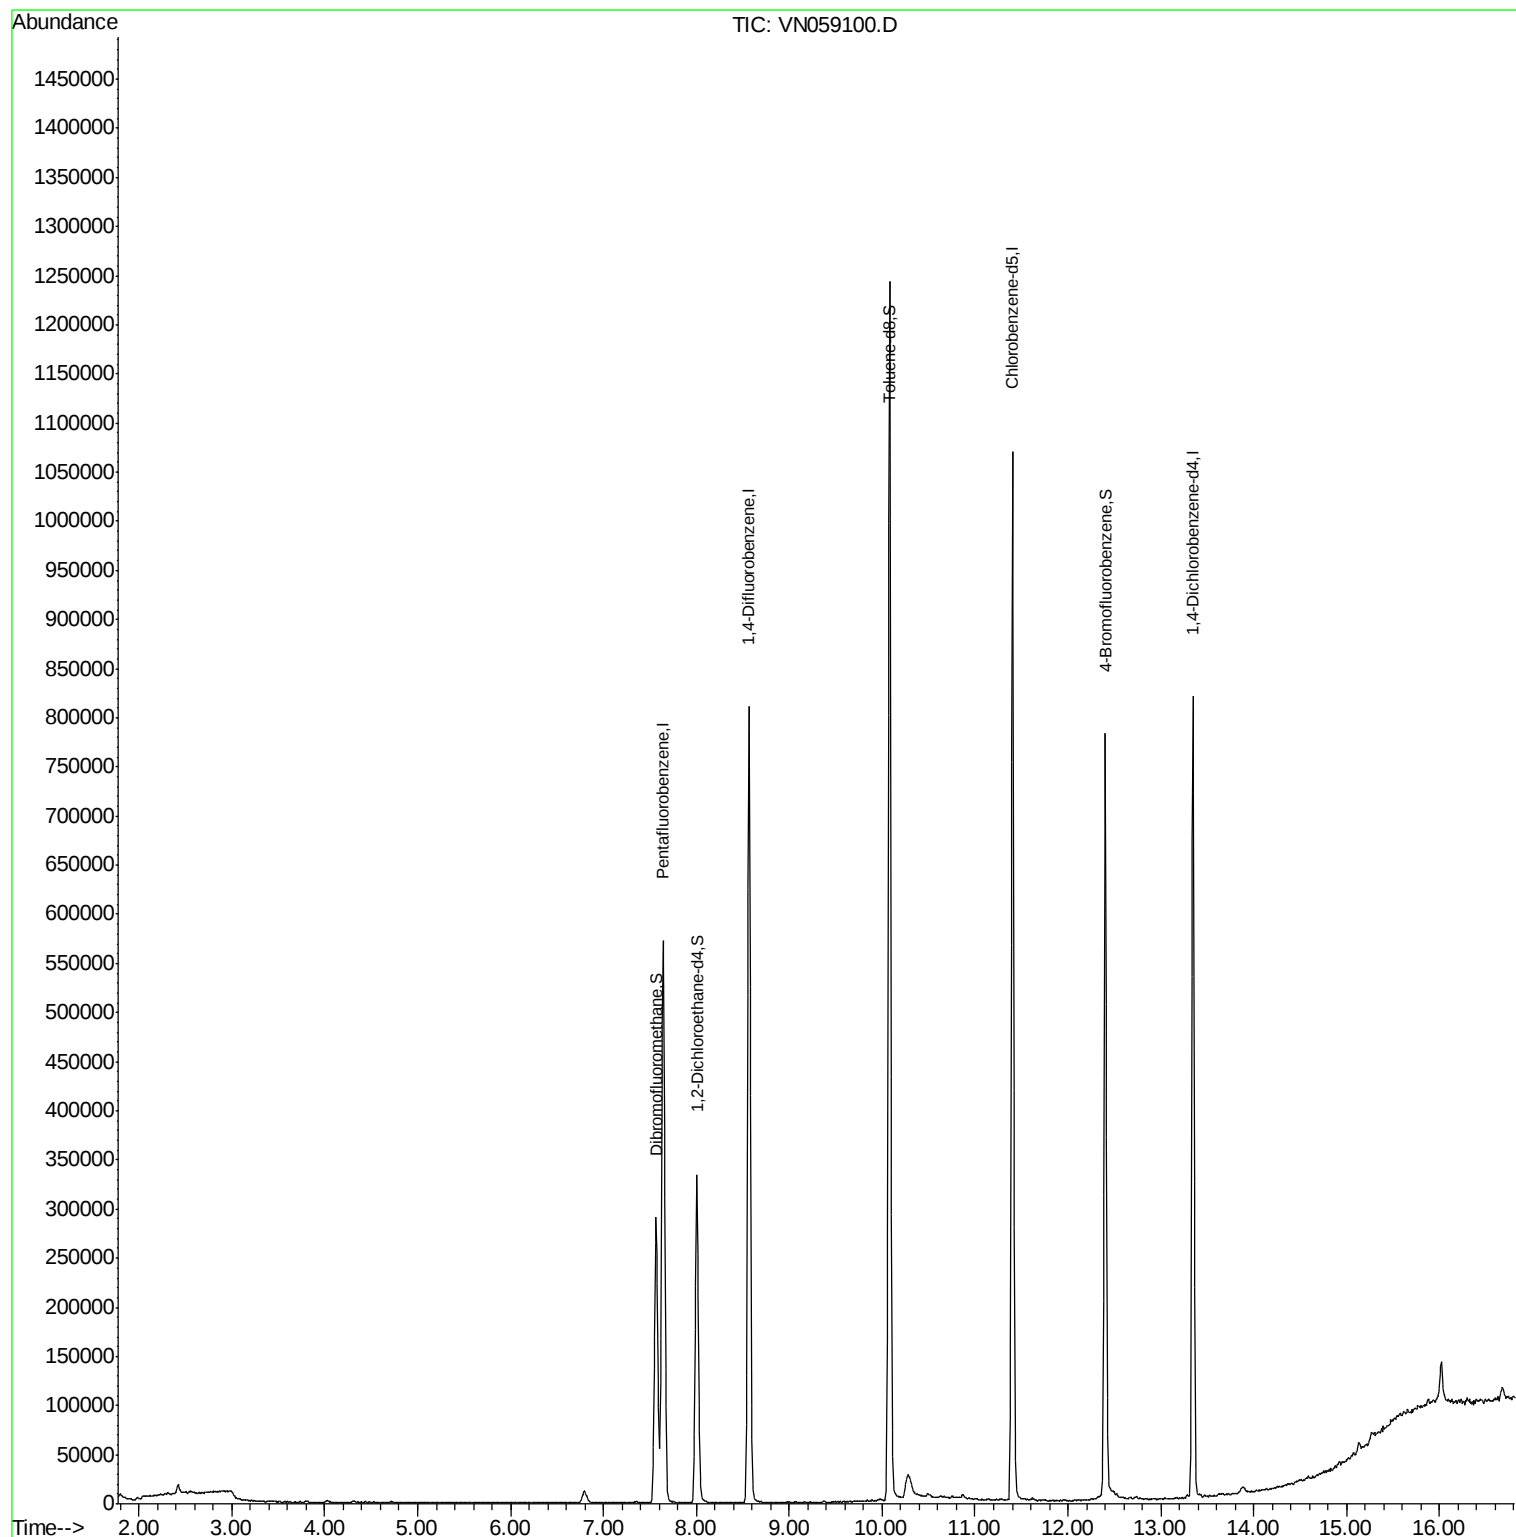



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.64 min Scan# 1826

Delta R.T. -0.00 min

Lab File: VN059100.D

Acq: 6 Nov 2019 12:29

Instrument :

MSVOA_N

ClientSampleId :


VN1106WBL01

Tgt Ion:168 Resp: 463590

Ion Ratio Lower Upper

168 100

99 56.2 45.7 68.5

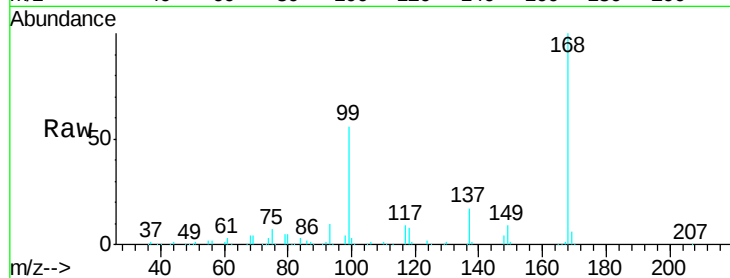

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.64

200000



150000

100000

50000

0

Time--> 7.50 7.60 7.70

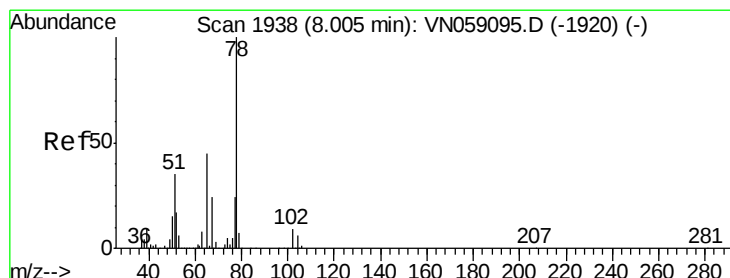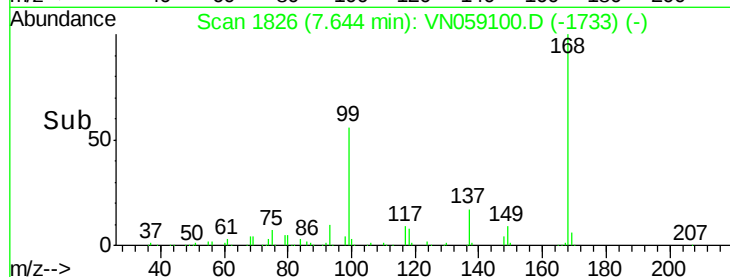

#33

1,2-Dichloroethane-d4

Concen: 50.701 ug/l

RT: 8.00 min Scan# 1938

Delta R.T. -0.00 min

Lab File: VN059100.D


Acq: 6 Nov 2019 12:29

Tgt Ion: 65 Resp: 288930

Ion Ratio Lower Upper

65 100

67 53.7 0.0 107.4

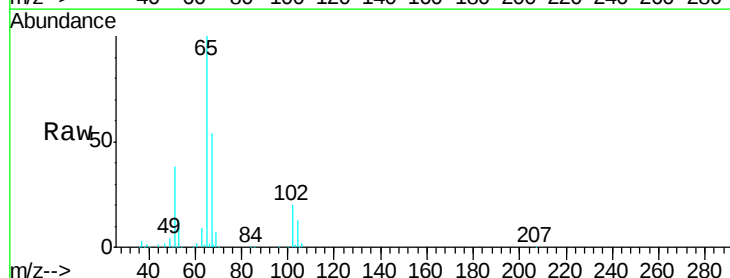

Abundance Ion 64.90 (64.60 to 65.60): VN

Ion 66.90 (66.60 to 67.60): VN


8.00


100000

50000

0

Time--> 7.90 8.00 8.10

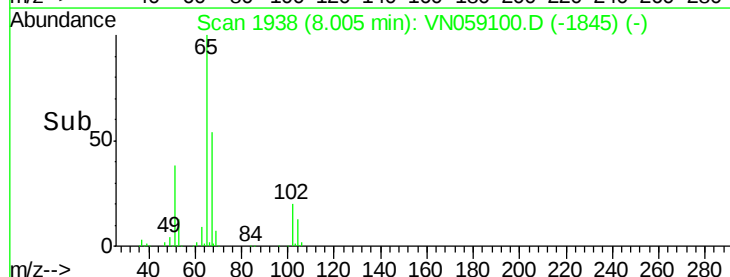

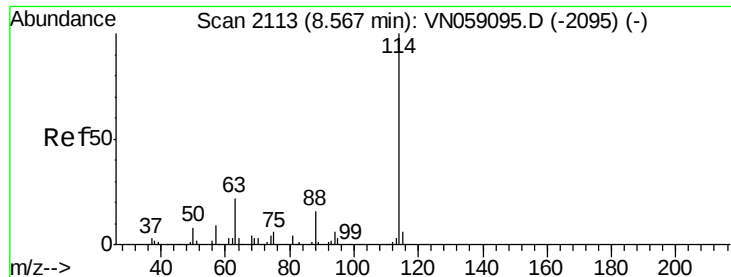

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.57 min Scan# 2113

Delta R.T. -0.00 min

Lab File: VN059100.D

Acq: 6 Nov 2019 12:29

Instrument :

MSVOA_N

ClientSampleId :

VN1106WBL01


Tgt Ion:114 Resp: 723498

Ion Ratio Lower Upper

114 100

63 21.4 0.0 43.4




88 16.0 0.0 32.2

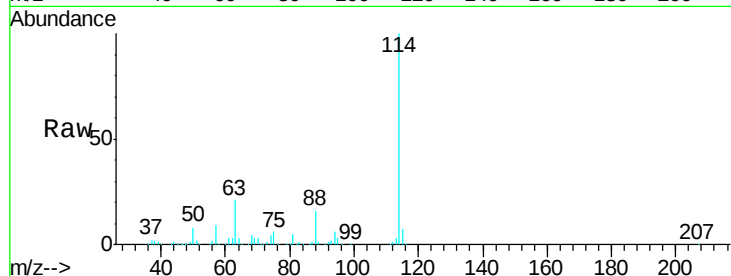

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

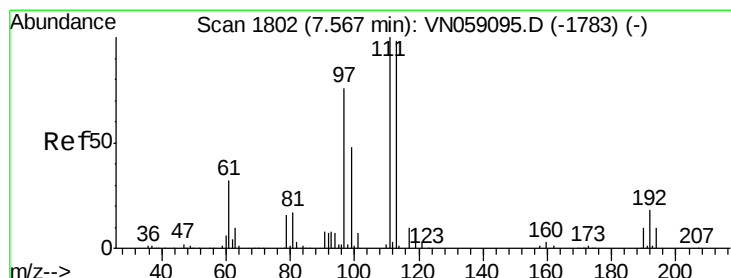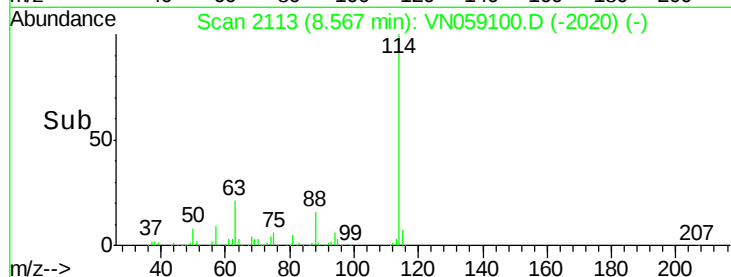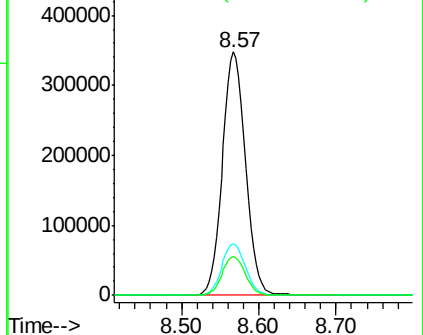

#35

Dibromofluoromethane

Concen: 52.187 ug/l

RT: 7.57 min Scan# 1802

Delta R.T. -0.00 min

Lab File: VN059100.D

Acq: 6 Nov 2019 12:29


Tgt Ion:113 Resp: 225447

Ion Ratio Lower Upper

113 100

111 101.4 82.8 124.2



192 19.4 16.1 24.1

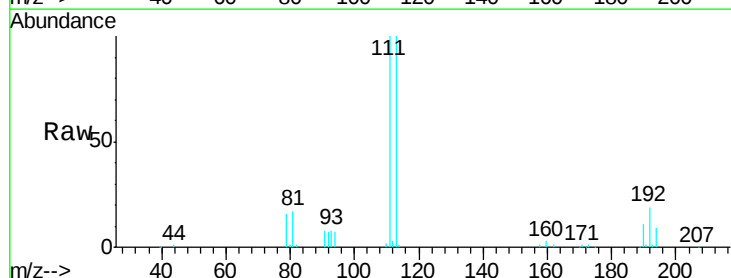


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

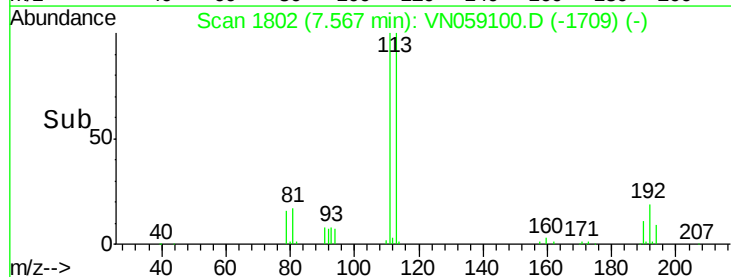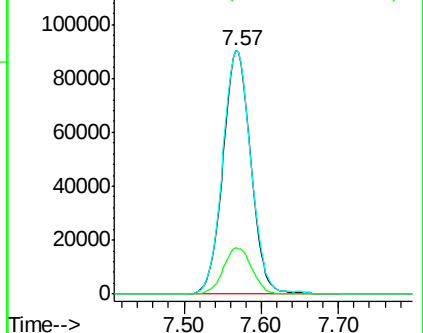

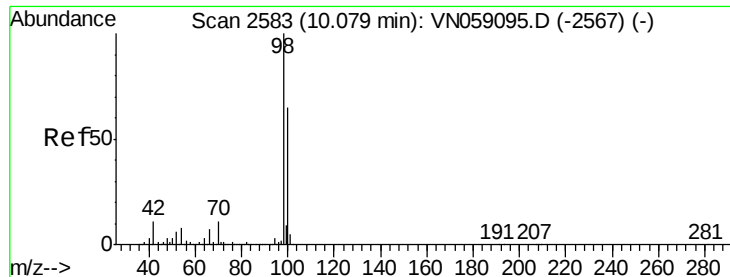

#50

Toluene-d8

Concen: 51.384 ug/l

RT: 10.08 min Scan# 2584

Delta R.T. 0.00 min

Lab File: VN059100.D

Acq: 6 Nov 2019 12:29

Instrument :

MSVOA_N

ClientSampled :





VN1106WBL01

Tgt Ion: 98 Resp: 874356

Ion Ratio Lower Upper

98 100

100 64.4 52.2 78.2

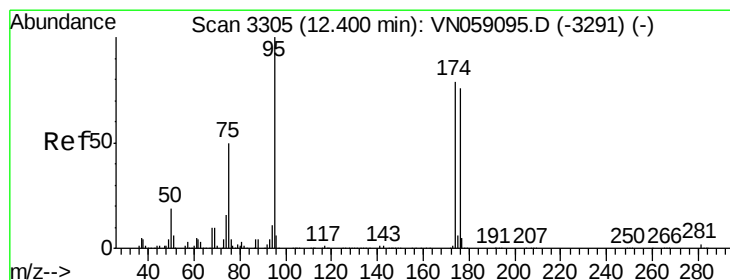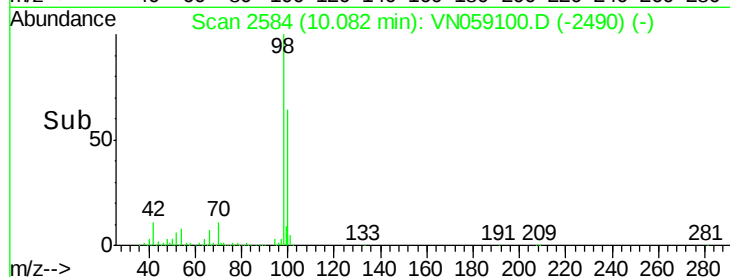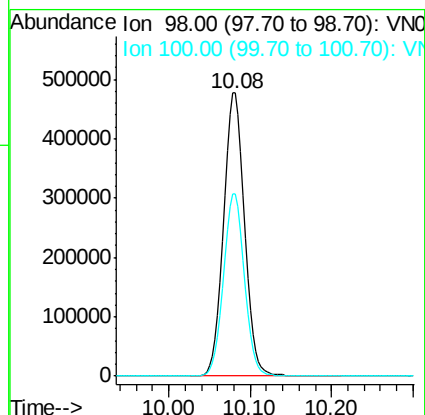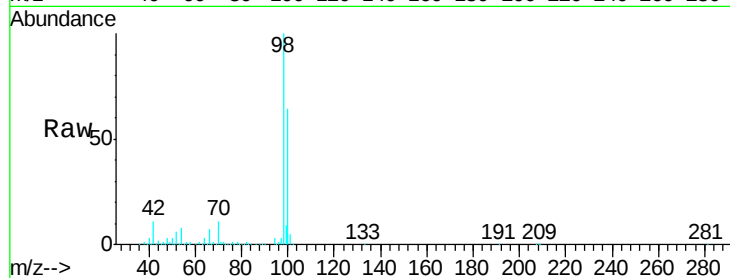

#62

4-Bromofluorobenzene

Concen: 45.546 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN059100.D

Acq: 6 Nov 2019 12:29




Tgt Ion: 95 Resp: 279443


Ion Ratio Lower Upper

95 100

174 77.5 0.0 158.2

176 75.3 0.0 151.8

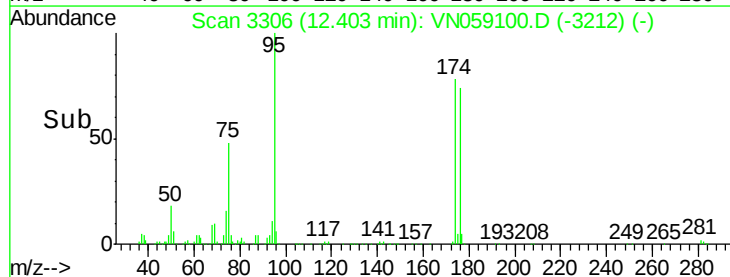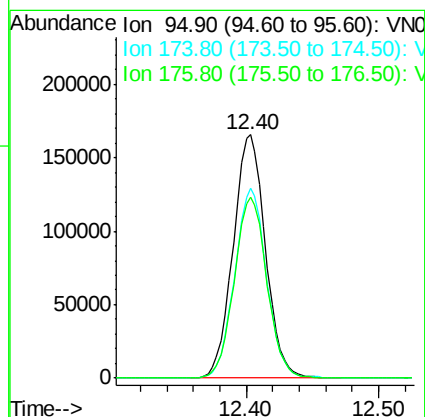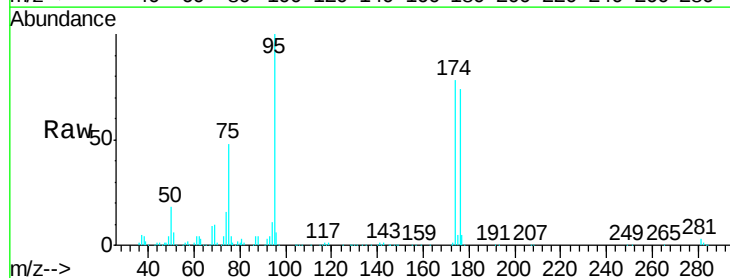

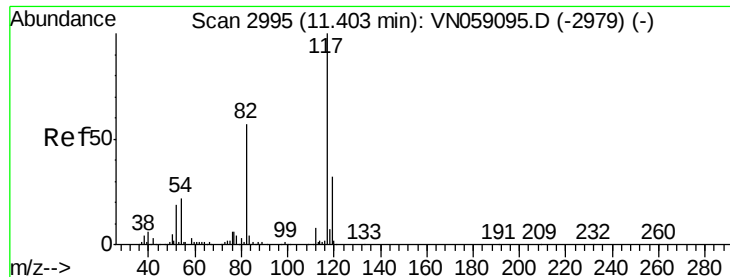

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.40 min Scan# 2995

Delta R.T. -0.00 min

Lab File: VN059100.D

Acq: 6 Nov 2019 12:29

Instrument :

MSVOA_N

ClientSampleId :

VN1106WBL01


Tgt Ion:117 Resp: 627504

Ion Ratio Lower Upper

117 100

82 57.4 45.8 68.8




119 31.7 25.8 38.6

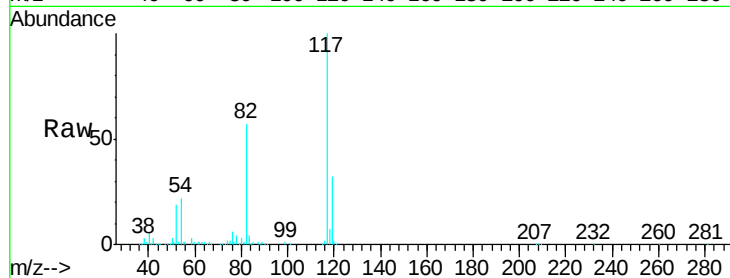

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

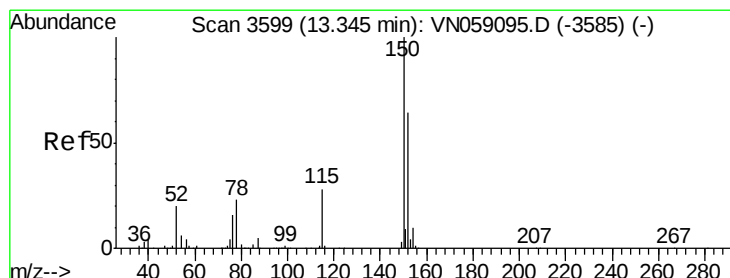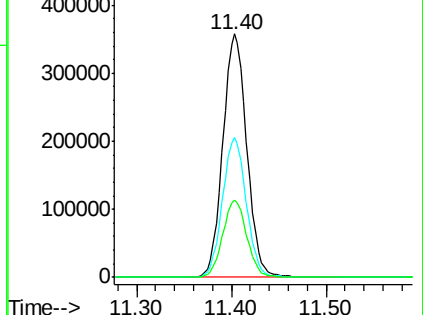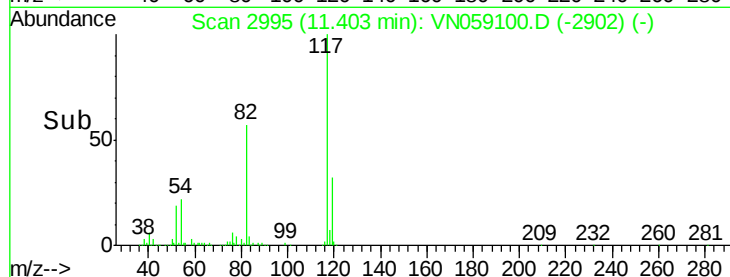

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3599

Delta R.T. -0.00 min

Lab File: VN059100.D

Acq: 6 Nov 2019 12:29


Tgt Ion:152 Resp: 225638

Ion Ratio Lower Upper

152 100

115 58.9 29.4 88.2

150 157.8 0.0 345.8

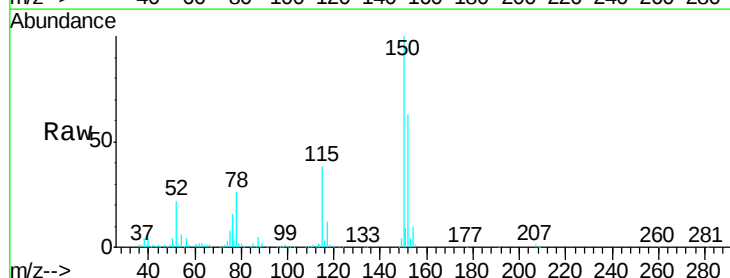

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

