

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN110620\
 Data File : VN064496.D
 Acq On : 6 Nov 2020 20:28
 Operator : JC/MD
 Sample : L4657-04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PAV-B49-110520-17-18

Quant Time: Nov 07 03:53:52 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 04 12:09:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	243385	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	510341	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	547628	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	200512	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	240790	56.80	ug/l	0.00
Spiked Amount			Recovery	=	113.60%	
35) Dibromofluoromethane	7.55	113	174081	50.10	ug/l	0.00
Spiked Amount			Recovery	=	100.20%	
50) Toluene-d8	10.06	98	669170	49.83	ug/l	0.00
Spiked Amount			Recovery	=	99.66%	
62) 4-Bromofluorobenzene	12.38	95	259133	51.02	ug/l	0.00
Spiked Amount			Recovery	=	102.04%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acrolein	3.45	56	125	0.431	ug/l #	48
16) Acetone	3.78	43	13652	8.454	ug/l	96
18) Methyl Acetate	4.30	43	5439	1.713	ug/l #	75
20) Methylene Chloride	4.50	84	13857	4.325	ug/l	97
25) 2-Butanone	6.81	43	2074	1.008	ug/l #	52
29) Tetrahydrofuran	7.16	42	484	0.383	ug/l #	55
31) Cyclohexane	7.63	56	7286	1.414	ug/l #	53
36) 1,1-Dichloropropene	7.62	75	23805	4.415	ug/l #	50
37) Ethyl Acetate	6.89	43	350	0.825	ug/l #	71
38) Carbon Tetrachloride	7.63	117	28875	5.011	ug/l #	18
43) Isopropyl Acetate	8.13	43	98550	11.279	ug/l	99
45) 1,2-Dichloropropane	9.23	63	1826	0.432	ug/l #	45
48) Methyl methacrylate	9.14	41	6545	1.485	ug/l #	15
49) 1,4-Dioxane	9.24	88	139	2.394	ug/l #	1
51) 4-Methyl-2-Pentanone	9.96	43	8152	1.600	ug/l	98
54) cis-1,3-Dichloropropene	9.87	75	38960	5.744	ug/l #	66
56) Ethyl methacrylate	10.52	69	3039	2.313	ug/l #	1
57) 1,3-Dichloropropane	10.74	76	6876	1.045	ug/l #	42
59) 2-Hexanone	10.74	43	115526	31.385	ug/l #	53
71) Bromoform	12.38	173	422	1.397	ug/l #	1
74) N-amyl acetate	12.00	43	2803	1.568	ug/l #	48
76) 1,2,3-Trichloropropane	12.38	75	143404	29.518	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.38	75	143404	82.417	ug/l #	8
95) Naphthalene	15.12	128	111	3.632	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN110620\
Data File : VN064496.D
Acq On : 6 Nov 2020 20:28
Operator : JC/MD
Sample : L4657-04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PAV-B49-110520-17-18

Quant Time: Nov 07 03:53:52 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 04 12:09:03 2020
Response via : Initial Calibration

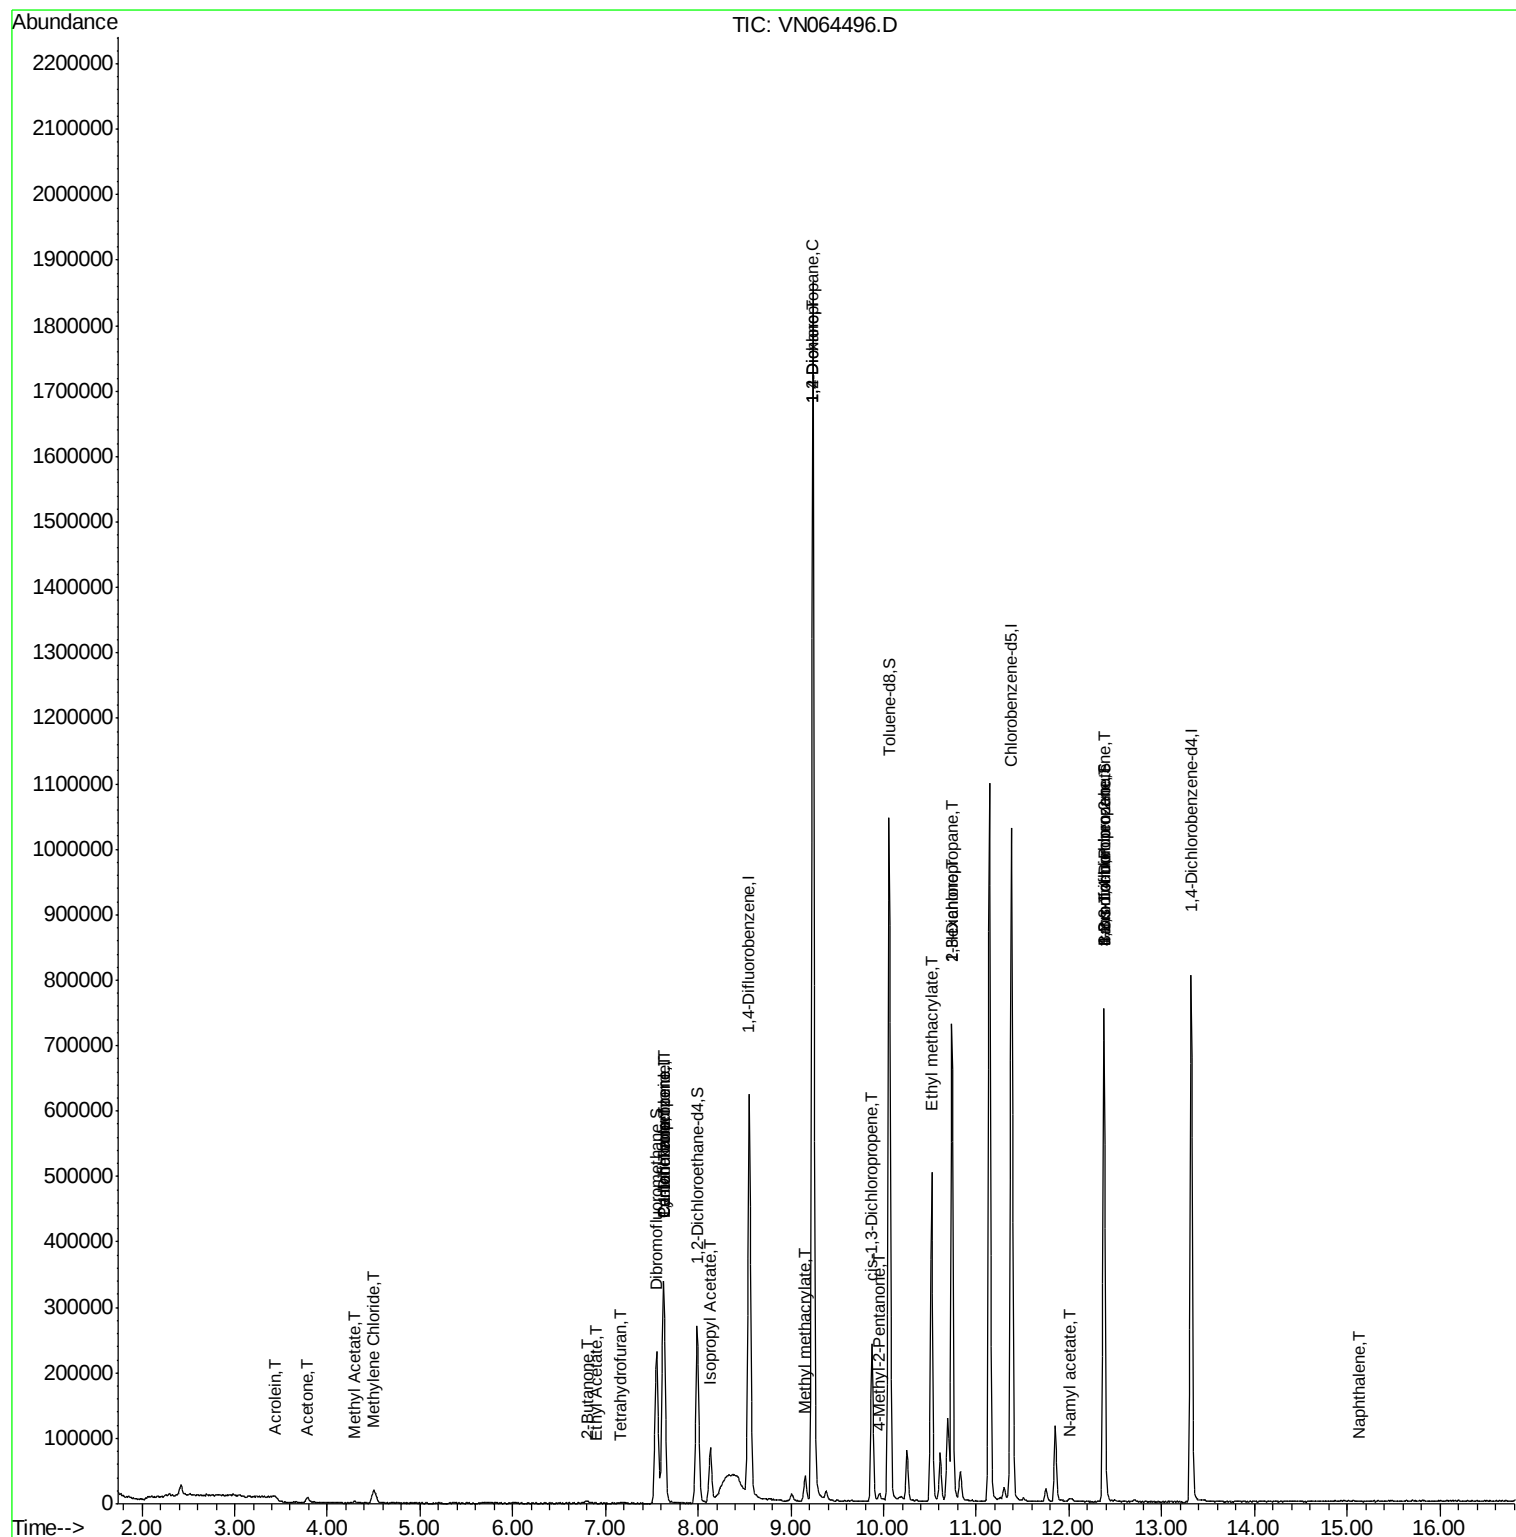



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064496.D

Acq: 6 Nov 2020 20:28

Instrument :

MSVOA_N

ClientSampleId :


PAV-B49-110520-17-18

Tot Ion:168 Resp: 243385

Ion Ratio Lower Upper

168 100

99 68.7 53.4 80.2



Abundance Ion 167.90 (167.60 to 168.60): VN064428.D (-1811) (-)

Ion 98.90 (98.60 to 99.60): VN064428.D (-1811) (-)

7.63

100000

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70



#13

Acrolein

Concen: 0.431 ug/l

RT: 3.45 min Scan# 532

Delta R.T. -0.12 min

Lab File: VN064496.D


Acq: 6 Nov 2020 20:28

Tgt Ion: 56 Resp: 125

Ion Ratio Lower Upper

56 100

55 112.8 55.9 83.9#



Abundance Ion 56.00 (55.70 to 56.70): VN064428.D (-548) (-)

Ion 55.00 (54.70 to 55.70): VN064428.D (-548) (-)

3.45

400


300


200

100

0

Time--> 3.44 3.45 3.46









#16
Acetone
Concen: 8.454 ug/l
RT: 3.78 min Scan# 634
Delta R.T. 0.00 min
Lab File: VN064496.D
Acq: 6 Nov 2020 20:28




Instrument :
MSVOA_N
ClientSampleId :
PAV-B49-110520-17-18


Tot Ion: 43 Resp: 13652
Ion Ratio Lower Upper
43 100
58 24.8 21.4 32.0

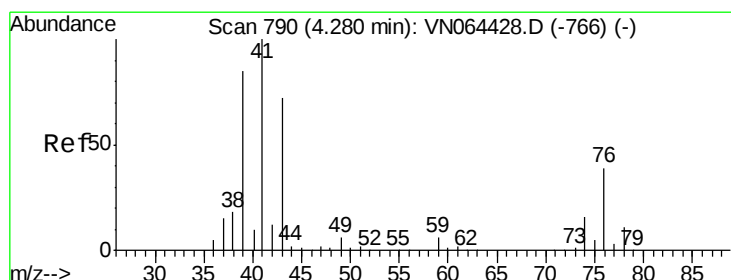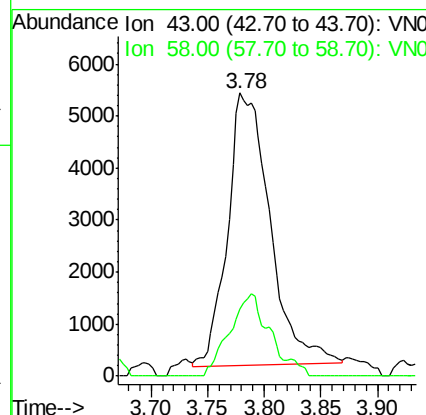

#18
Methyl Acetate
Concen: 1.713 ug/l
RT: 4.30 min Scan# 795
Delta R.T. 0.02 min
Lab File: VN064496.D
Acq: 6 Nov 2020 20:28

Tgt Ion: 43 Resp: 5439
Ion Ratio Lower Upper
43 100
74 9.2 17.0 25.4#


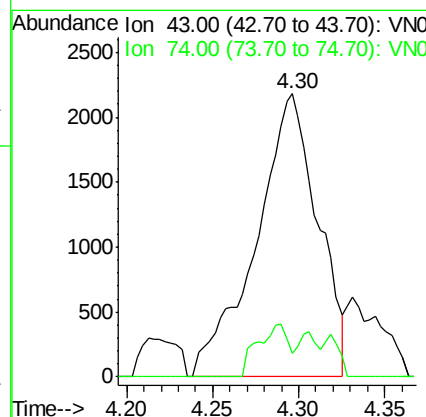






#20
Methvlene Chloride
Concen: 4.325 ug/l
RT: 4.50 min Scan# 859
Delta R.T. -0.00 min
Lab File: VN064496.D
Acq: 6 Nov 2020 20:28




Instrument :
MSVOA_N
ClientSampleId :
PAV-B49-110520-17-18


Tot Ion:	84	Resp:	13857
Ion	Ratio	Lower	Upper
84	100		
49	142.3	110.1	165.1
51	42.3	33.6	50.4
86	62.8	52.1	78.1

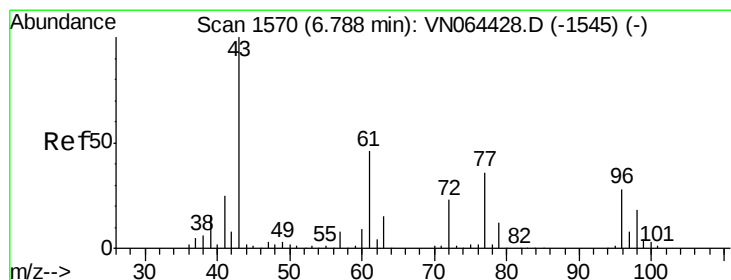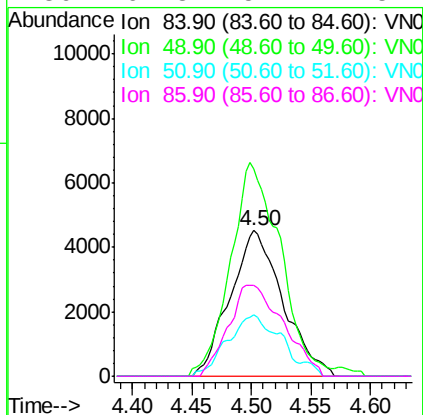

#25
2-Butanone
Concen: 1.008 ug/l
RT: 6.81 min Scan# 1577
Delta R.T. 0.02 min
Lab File: VN064496.D
Acq: 6 Nov 2020 20:28

Tgt Ion:	43	Resp:	2074
Ion	Ratio	Lower	Upper
43	100		
72	0.0	18.5	27.7#

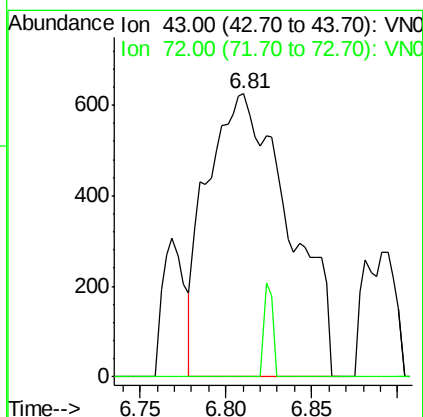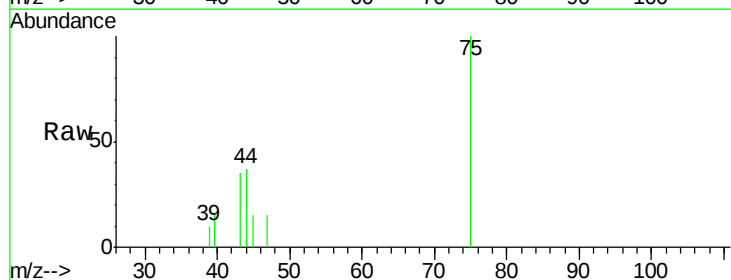



#29

Tetrahydrofuran

Concen: 0.383 ug/l

RT: 7.16 min Scan# 1687

Delta R.T. -0.00 min

Lab File: VN064496.D

Acq: 6 Nov 2020 20:28

Instrument :

MSVOA_N

ClientSampleId :

PAV-B49-110520-17-18





Tot Ion: 42 Resp: 484

Ion Ratio Lower Upper

42 100

72 22.3 31.7 47.5#

71 0.0 29.8 44.6#

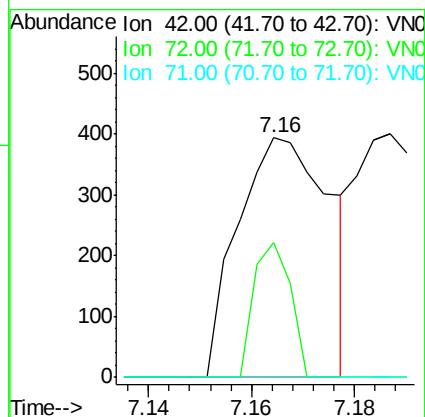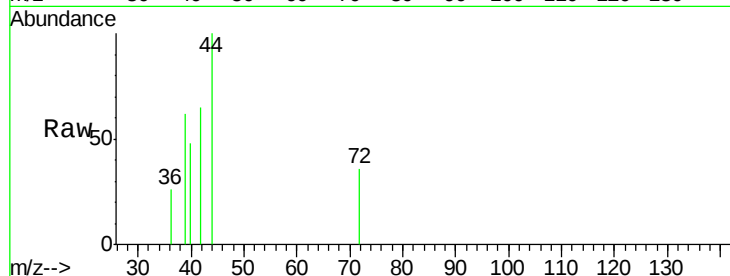

#31

Cyclohexane

Concen: 1.414 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.02 min

Lab File: VN064496.D

Acq: 6 Nov 2020 20:28




Tgt Ion: 56 Resp: 7286


Ion Ratio Lower Upper

56 100

69 122.1 25.6 38.4#

84 79.6 63.0 94.6

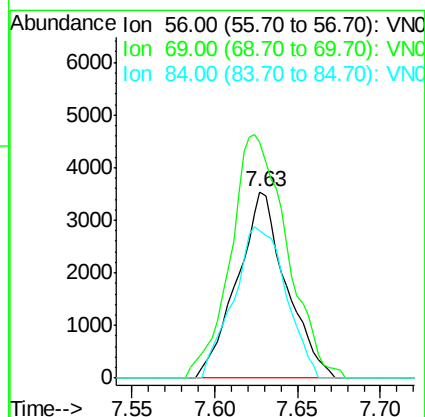



#33

1,2-Dichloroethane-d4

Concen: 56.798 ug/l

RT: 7.99 min Scan# 1944

Delta R.T. 0.00 min

Lab File: VN064496.D

Acq: 6 Nov 2020 20:28

Instrument :

MSVOA_N

ClientSampleId :


PAV-B49-110520-17-18

Tot Ion: 65 Resp: 240790

Ion Ratio Lower Upper




65 100

67 50.6 0.0 101.6



Abundance Ion 64.90 (64.60 to 65.60): VN064496.D (-1850) (-)

Ion 66.90 (66.60 to 67.60): VN064496.D (-1850) (-)

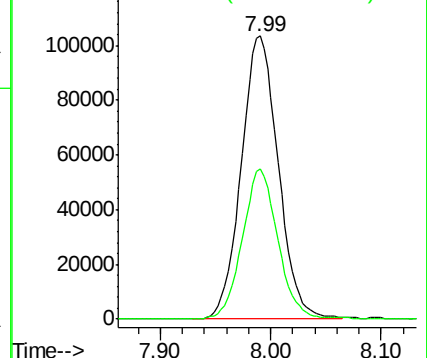

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2118

Delta R.T. -0.00 min

Lab File: VN064496.D

Acq: 6 Nov 2020 20:28


Tgt Ion: 114 Resp: 510341

Ion Ratio Lower Upper

114 100

63 23.1 0.0 45.6



88 16.1 0.0 32.8




Abundance Ion 113.90 (113.60 to 114.60): VN064496.D (-2025) (-)

Ion 63.00 (62.70 to 63.70): VN064496.D (-2025) (-)

Ion 87.90 (87.60 to 88.60): VN064496.D (-2025) (-)




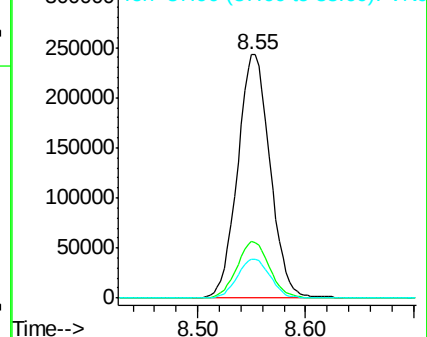




#35
 Dibromofluoromethane
 Concen: 50.099 ug/l
 RT: 7.55 min Scan# 1807
 Delta R.T. 0.00 min
 Lab File: VN064496.D
 Acq: 6 Nov 2020 20:28




Instrument :
 MSVOA_N
 ClientSampleId :
 PAV-B49-110520-17-18

Tot Ion	Ratio	Lower	Upper
113	100		
111	102.2	81.1	121.7
192	16.4	12.8	19.2

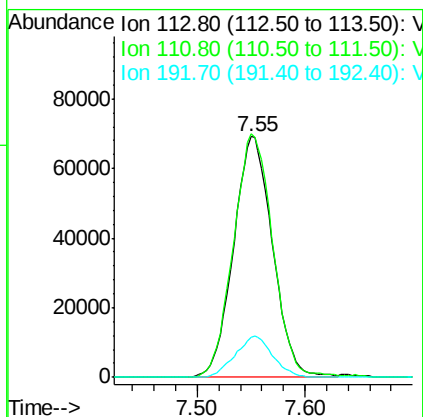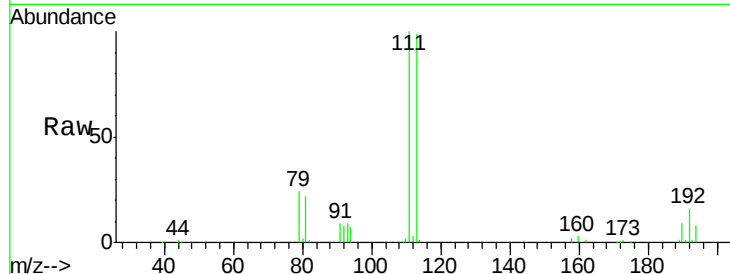

#36
 1,1-Dichloropropene
 Concen: 4.415 ug/l
 RT: 7.62 min Scan# 1830
 Delta R.T. -0.13 min
 Lab File: VN064496.D
 Acq: 6 Nov 2020 20:28

Tgt Ion	Ratio	Lower	Upper
75	100		
110	7.3	16.0	48.0#
77	0.0	24.0	36.0#



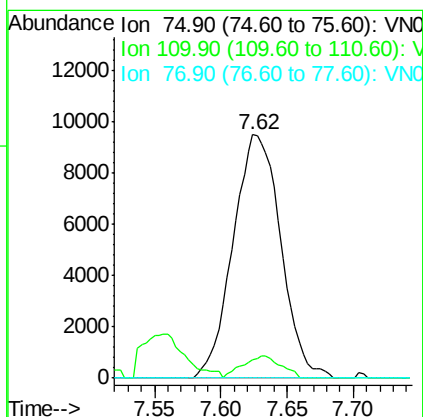
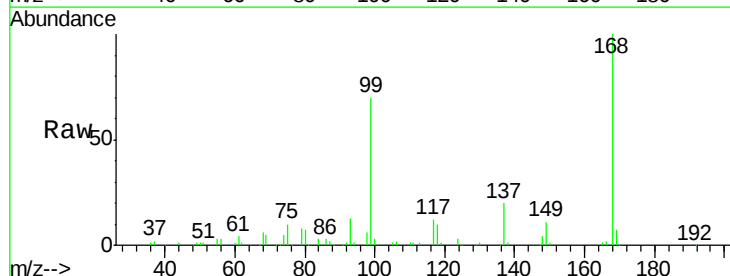




#37
Ethyl Acetate
Concen: 0.825 ug/l
RT: 6.89 min Scan# 1602
Delta R.T. 0.01 min
Lab File: VN064496.D
Acq: 6 Nov 2020 20:28




Instrument :
MSVOA_N
ClientSampleId :
PAV-B49-110520-17-18


Tot Ion: 43 Resp: 350
Ion Ratio Lower Upper
43 100
61 0.0 10.0 15.0#
70 0.0 7.1 10.7#

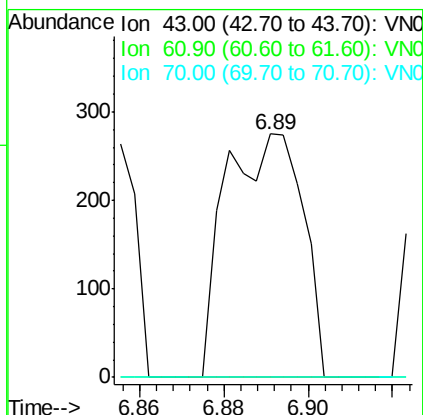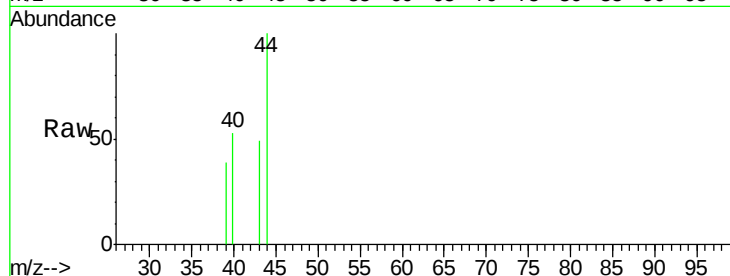

#38
Carbon Tetrachloride
Concen: 5.011 ug/l
RT: 7.63 min Scan# 1832
Delta R.T. -0.10 min
Lab File: VN064496.D
Acq: 6 Nov 2020 20:28

Tgt Ion: 117 Resp: 28875
Ion Ratio Lower Upper
117 100
119 6.9 75.5 113.3#
121 0.0 24.4 36.6#

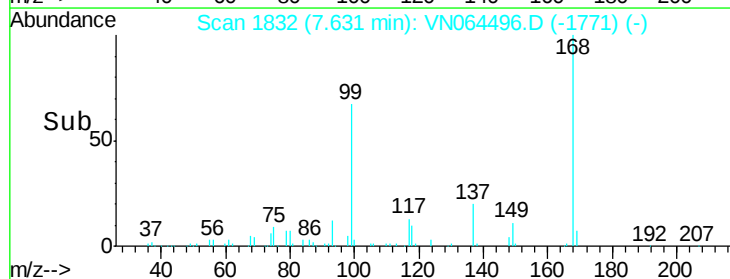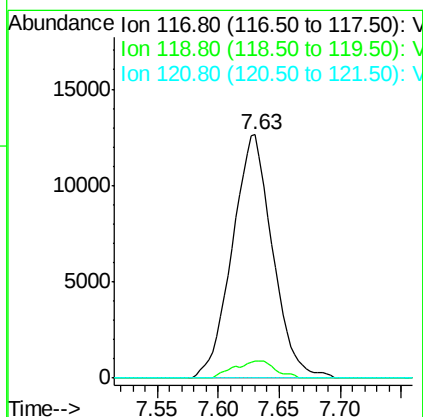



#43

Isopropyl Acetate

Concen: 11.279 ug/l

RT: 8.13 min Scan# 1988

Delta R.T. 0.01 min

Lab File: VN064496.D

Acq: 6 Nov 2020 20:28

Instrument :

MSVOA_N

ClientSampleId :

PAV-B49-110520-17-18


Tot Ion: 43 Resp: 98550

Ion Ratio Lower Upper

43 100

61 16.9 14.0 21.0




87 11.7 9.1 13.7



Abundance Ion 43.00 (42.70 to 43.70): VN064428.D (-1966) (-)

Ion 61.00 (60.70 to 61.70): VN064428.D (-1966) (-)

Ion 87.00 (86.70 to 87.70): VN064428.D (-1966) (-)

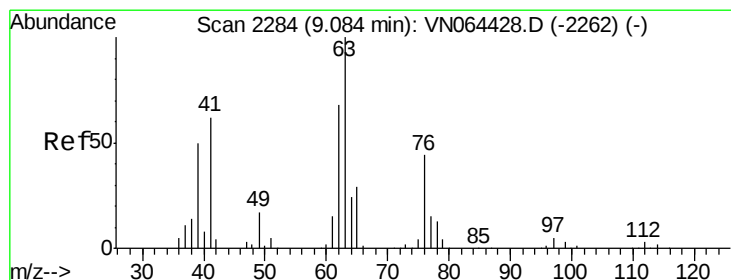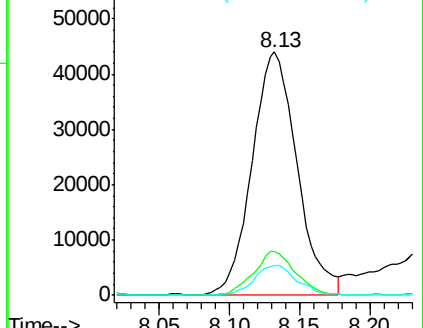

#45

1,2-Dichloropropane

Concen: 0.432 ug/l

RT: 9.23 min Scan# 2331

Delta R.T. 0.15 min

Lab File: VN064496.D


Acq: 6 Nov 2020 20:28

Tgt Ion: 63 Resp: 1826

Ion Ratio Lower Upper



63 100


65 0.0 23.6 35.4#



Abundance Ion 62.90 (62.60 to 63.60): VN064428.D (-2262) (-)

Ion 64.90 (64.60 to 65.60): VN064428.D (-2262) (-)




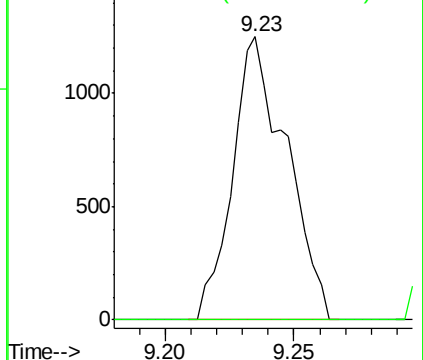


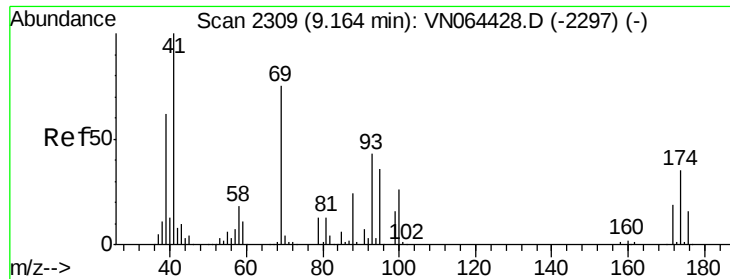

#48
Methyl methacrylate
Concen: 1.485 ug/l
RT: 9.14 min Scan# 2303
Delta R.T. -0.02 min
Lab File: VN064496.D
Acq: 6 Nov 2020 20:28




Instrument :
MSVOA_N
ClientSampleId :
PAV-B49-110520-17-18


Tot Ion: 41 Resp: 6545
Ion Ratio Lower Upper
41 100
69 0.0 60.4 90.6#
39 0.0 51.2 76.8#

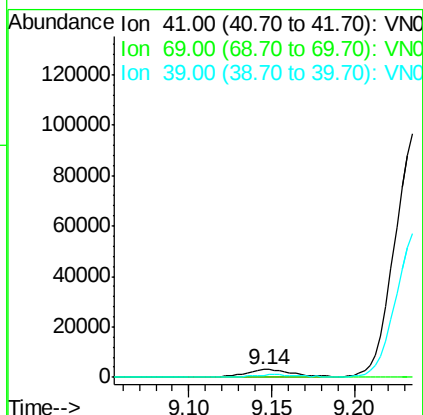

#49
1,4-Dioxane
Concen: 2.394 ug/l
RT: 9.24 min Scan# 2334
Delta R.T. 0.08 min
Lab File: VN064496.D
Acq: 6 Nov 2020 20:28

Tgt Ion: 88 Resp: 139
Ion Ratio Lower Upper
88 100
43 1322515.1 31.0 46.6#
58 6773.4 58.4 87.6#

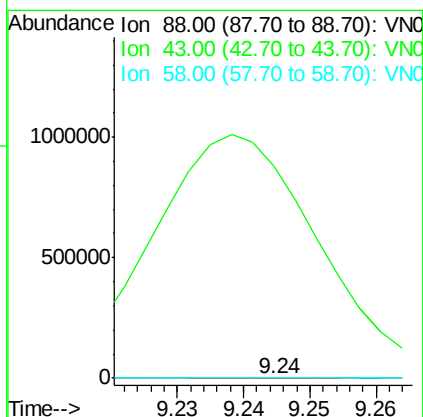



#50

Toluene-d8

Concen: 49.827 ug/l

RT: 10.06 min Scan# 2588

Delta R.T. 0.00 min

Lab File: VN064496.D

Acq: 6 Nov 2020 20:28

Instrument :

MSVOA_N

ClientSampleId :


PAV-B49-110520-17-18

Tot Ion: 98 Resp: 669170

Ion Ratio Lower Upper




98 100

100 64.3 50.7 76.1



Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN

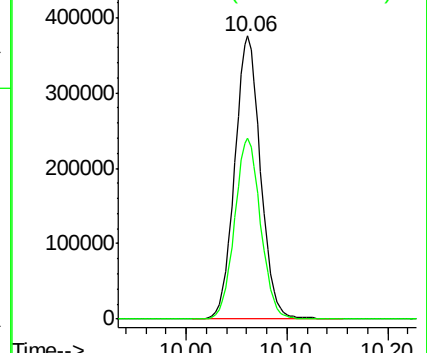

#51

4-Methyl-2-Pentanone

Concen: 1.600 ug/l

RT: 9.96 min Scan# 2555

Delta R.T. 0.00 min

Lab File: VN064496.D


Acq: 6 Nov 2020 20:28

Tgt Ion: 43 Resp: 8152

Ion Ratio Lower Upper



43 100


58 34.5 28.4 42.6



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

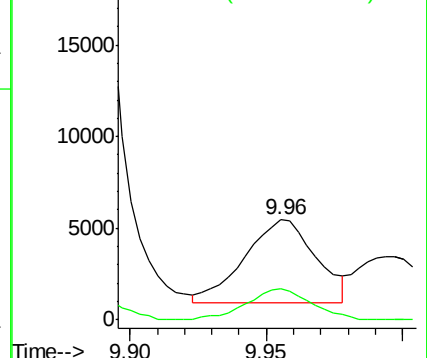



#54

cis-1,3-Dichloropropene

Concen: 5.744 ug/l

RT: 9.87 min Scan# 2530

Delta R.T. 0.07 min

Lab File: VN064496.D

Acq: 6 Nov 2020 20:28

Instrument :

MSVOA_N

ClientSampleId :

PAV-B49-110520-17-18





Tot Ion: 75 Resp: 38960

Ion Ratio Lower Upper

75 100

77 0.0 24.9 37.3#

39 42.0 47.1 70.7#

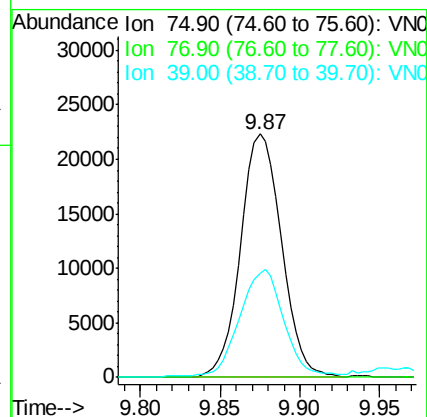

#56

Ethyl methacrylate

Concen: 2.313 ug/l

RT: 10.52 min Scan# 2730

Delta R.T. 0.12 min

Lab File: VN064496.D

Acq: 6 Nov 2020 20:28




Tgt Ion: 69 Resp: 3039


Ion Ratio Lower Upper

69 100

41 3438.3 59.3 88.9#

39 1599.2 35.4 53.0#



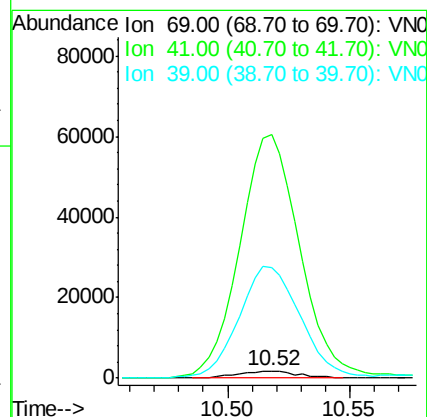





#57
 1,3-Dichloropropane
 Concen: 1.045 ug/l
 RT: 10.74 min Scan# 2798
 Delta R.T. 0.06 min
 Lab File: VN064496.D
 Acq: 6 Nov 2020 20:28




Instrument :
 MSVOA_N
 ClientSampleId :
 PAV-B49-110520-17-18


Tot Ion: 76 Resp: 6876
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.8 38.6#

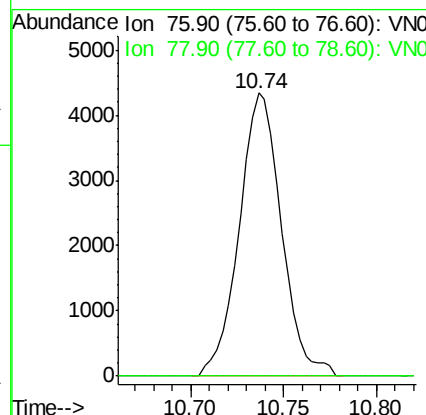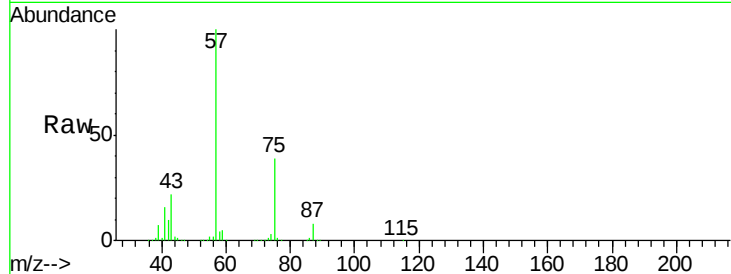

#59
 2-Hexanone
 Concen: 31.385 ug/l
 RT: 10.74 min Scan# 2798
 Delta R.T. 0.02 min
 Lab File: VN064496.D
 Acq: 6 Nov 2020 20:28

Tgt Ion: 43 Resp: 115526
 Ion Ratio Lower Upper
 43 100
 58 17.2 24.7 74.1#

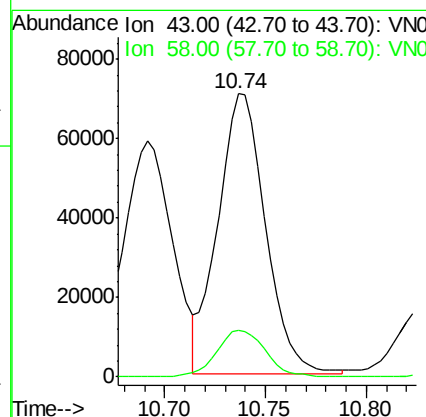



#62

4-Bromofluorobenzene

Concen: 51.021 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.00 min

Lab File: VN064496.D

Acq: 6 Nov 2020 20:28

Instrument :

MSVOA_N

ClientSampleId :

PAV-B49-110520-17-18


Tot Ion: 95 Resp: 259133

Ion Ratio Lower Upper

95 100

174 68.8 0.0 132.6

176 65.1 0.0 129.2






Abundance Ion 94.90 (94.60 to 95.60): VN064428.D (-3293) (-)

Ion 173.80 (173.50 to 174.50): VN064428.D (-3293) (-)

Ion 175.80 (175.50 to 176.50): VN064428.D (-3293) (-)

12.38

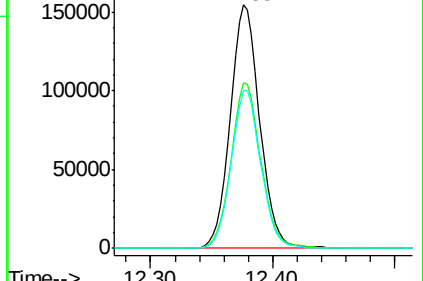

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.38 min Scan# 2998

Delta R.T. -0.00 min

Lab File: VN064496.D

Acq: 6 Nov 2020 20:28


Tgt Ion: 117 Resp: 547628

Ion Ratio Lower Upper

117 100

82 58.3 48.1 72.1

119 32.1 26.2 39.4






Abundance Ion 116.90 (116.60 to 117.60): VN064428.D (-2983) (-)

Ion 82.00 (81.70 to 82.70): VN064428.D (-2983) (-)

Ion 118.90 (118.60 to 119.60): VN064428.D (-2983) (-)

11.38

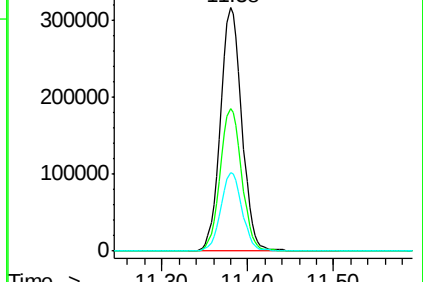



#71

Bromoform

Concen: 1.397 ug/l

RT: 12.38 min Scan# 3310

Delta R.T. 0.28 min

Lab File: VN064496.D

Acq: 6 Nov 2020 20:28

Instrument :

MSVOA_N

ClientSampleId :

PAV-B49-110520-17-18


Tot Ion:173 Resp: 422

Ion Ratio Lower Upper

173 100

175 2623.7 23.7 71.1#




254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

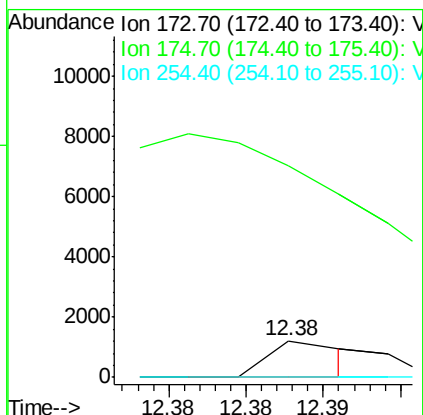

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3601

Delta R.T. 0.00 min

Lab File: VN064496.D

Acq: 6 Nov 2020 20:28


Tgt Ion:152 Resp: 200512

Ion Ratio Lower Upper

152 100

115 63.3 32.0 96.0



150 153.8 0.0 353.8




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V



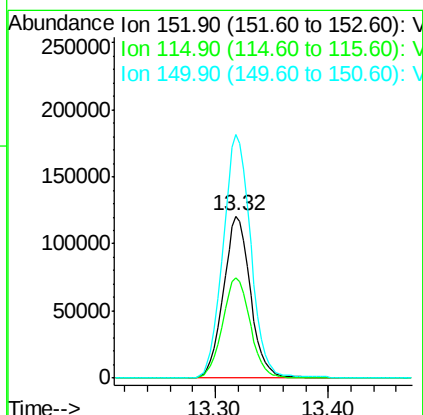





#74
N-amyl acetate
Concen: 1.568 ug/l
RT: 12.00 min Scan# 3192
Delta R.T. -0.04 min
Lab File: VN064496.D
Acq: 6 Nov 2020 20:28




Instrument :
MSVOA_N
ClientSampleId :
PAV-B49-110520-17-18


Tot Ion: 43 Resp: 2803
Ion Ratio Lower Upper
43 100
70 0.0 29.6 44.4#
55 3.5 18.4 27.6#
61 0.0 17.8 26.6#

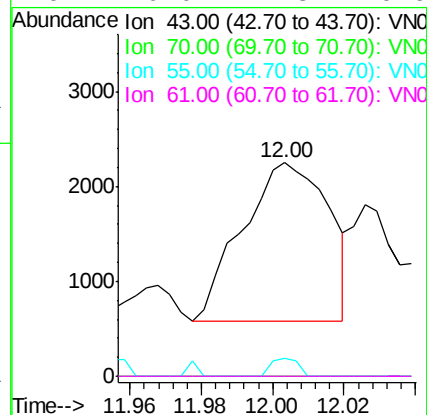

#76
1,2,3-Trichloropropane
Concen: 29.518 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. -0.15 min
Lab File: VN064496.D
Acq: 6 Nov 2020 20:28

Tgt Ion: 75 Resp: 143404
Ion Ratio Lower Upper
75 100
77 0.7 0.0 0.0#

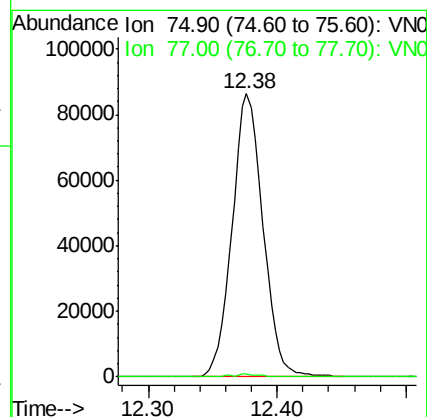



#81

trans-1,4-Dichloro-2-butene

Concen: 82.417 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.10 min

Lab File: VN064496.D

Acq: 6 Nov 2020 20:28

Instrument :

MSVOA_N

ClientSampleId :

PAV-B49-110520-17-18


Tot Ion: 75 Resp: 143404

Ion Ratio Lower Upper

75 100

53 0.1 84.0 126.0#




89 0.0 36.3 54.5#



Abundance Ion 74.90 (74.60 to 75.60): VN064428.D (-3266) (-)

Ion 53.00 (52.70 to 53.70): VN064428.D (-3266) (-)

Ion 88.90 (88.60 to 89.60): VN064428.D (-3266) (-)

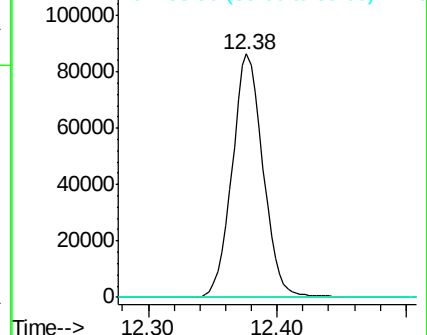

#95

Naphthalene

Concen: 3.632 ug/l

RT: 15.12 min Scan# 4161

Delta R.T. 0.02 min

Lab File: VN064496.D

Acq: 6 Nov 2020 20:28


Tgt Ion: 128 Resp: 111

Ion Ratio Lower Upper

128 100

127 0.0 10.5 15.7#

129 0.0 8.8 13.2#



Abundance Ion 128.00 (127.70 to 128.70): VN064428.D (-4139) (-)

Ion 127.00 (126.70 to 127.70): VN064428.D (-4139) (-)

Ion 129.00 (128.70 to 129.70): VN064428.D (-4139) (-)

