

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN110620\
 Data File : VN064498.D
 Acq On : 6 Nov 2020 21:17
 Operator : JC/MD
 Sample : L4625-19
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 CONTAINER-002-1B

Quant Time: Nov 07 04:50:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 04 12:09:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	240253	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	513059	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	539978	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	191504	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.99	65	238774	57.06	ug/l	0.00
Spiked Amount 50.000			Recovery	=	114.12%	
35) Dibromofluoromethane	7.55	113	171631	49.13	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.26%	
50) Toluene-d8	10.06	98	663938	49.18	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.36%	
62) 4-Bromofluorobenzene	12.38	95	251682	49.29	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.58%	
Target Compounds						
16) Acetone	3.79	43	22726	14.256	ug/l	94
18) Methyl Acetate	4.29	43	6271	2.001	ug/l #	74
20) Methylene Chloride	4.51	84	8842	2.796	ug/l #	92
43) Isopropyl Acetate	8.13	43	100108	11.397	ug/l	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN110620\
Data File : VN064498.D
Acq On : 6 Nov 2020 21:17
Operator : JC/MD
Sample : L4625-19
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
CONTAINER-002-1B

Quant Time: Nov 07 04:50:16 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 04 12:09:03 2020
Response via : Initial Calibration

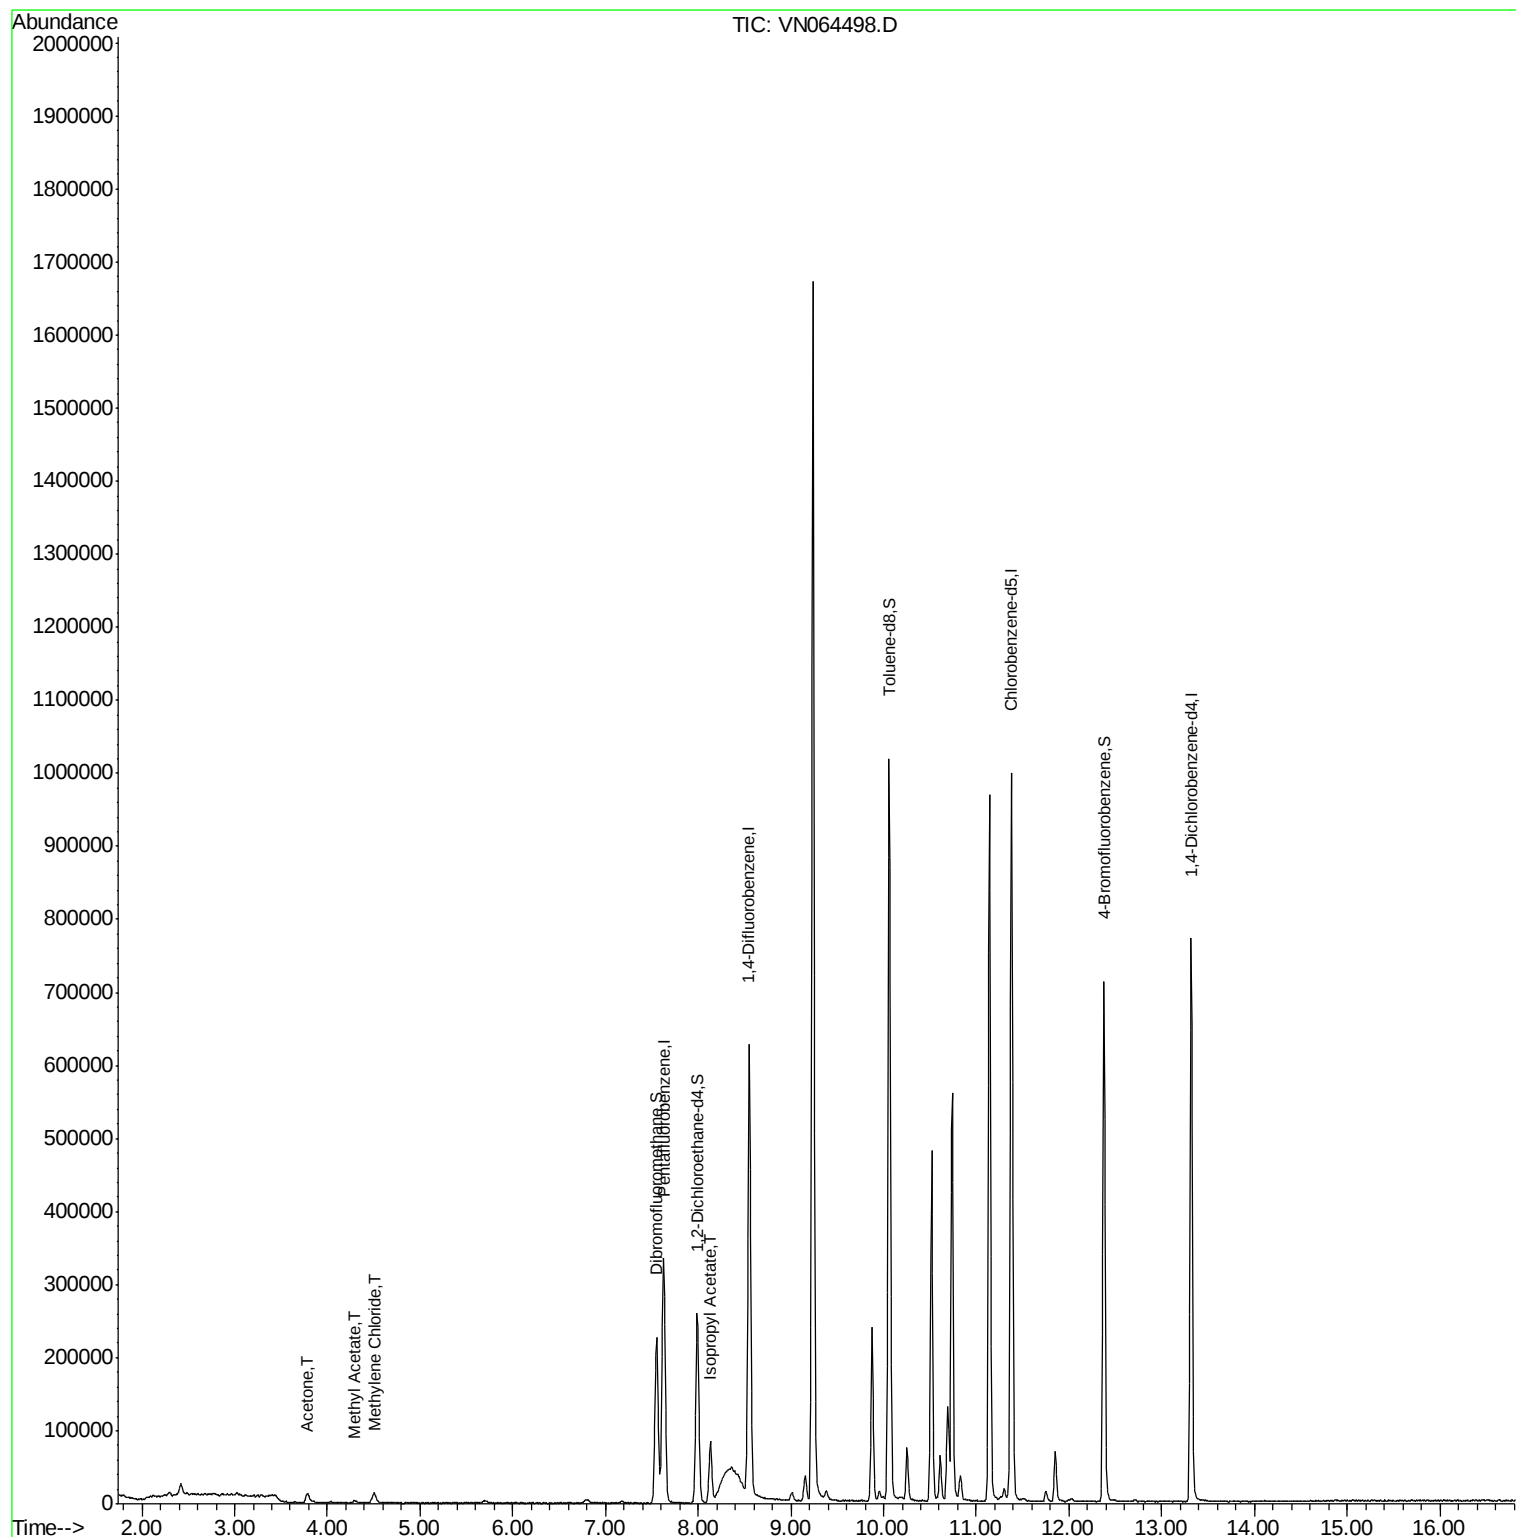



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064498.D

Acq: 6 Nov 2020 21:17

Instrument :

MSVOA_N

ClientSampleId :


CONTAINER-002-1B

Tot Ion:168 Resp: 240253

Ion Ratio Lower Upper

168 100

99 66.9 53.4 80.2

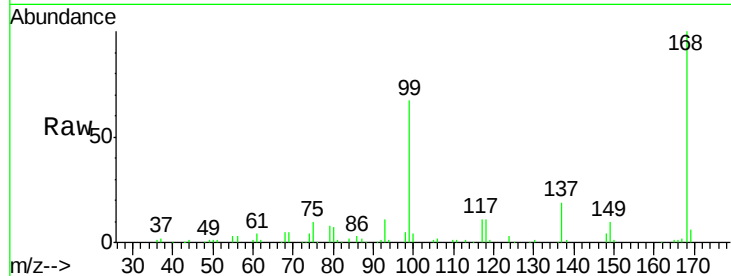

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.63

100000

80000



60000

40000

20000

0

Time-->

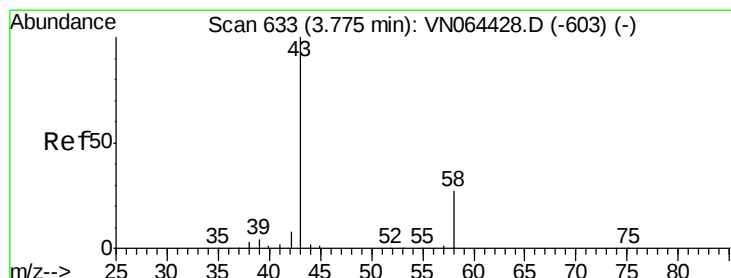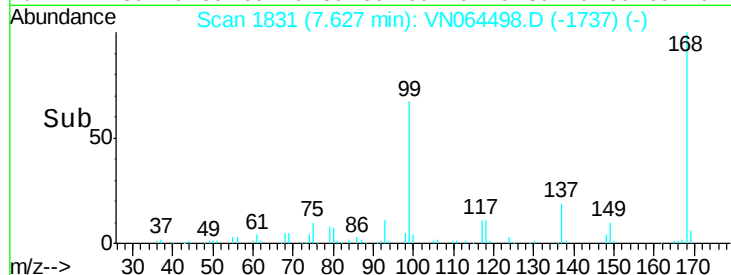

#16

Acetone

Concen: 14.256 ug/l

RT: 3.79 min Scan# 636

Delta R.T. 0.01 min

Lab File: VN064498.D


Acq: 6 Nov 2020 21:17

Tgt Ion: 43 Resp: 22726

Ion Ratio Lower Upper

43 100

58 23.4 21.4 32.0

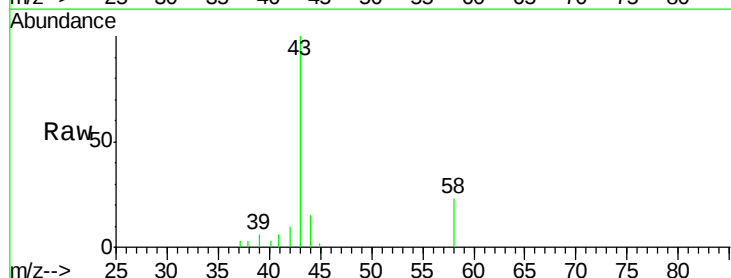

Abundance Ion 43.00 (42.70 to 43.70): VN

Ion 58.00 (57.70 to 58.70): VN

3.79

10000

8000


6000


4000

2000

0

Time-->




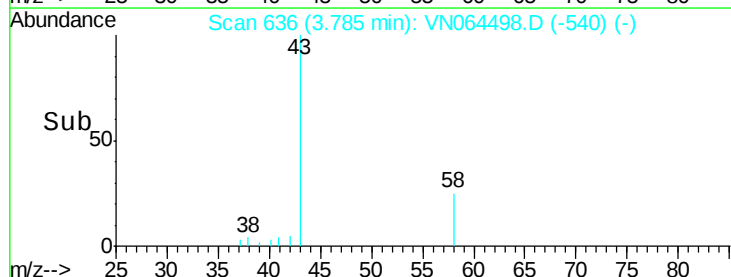


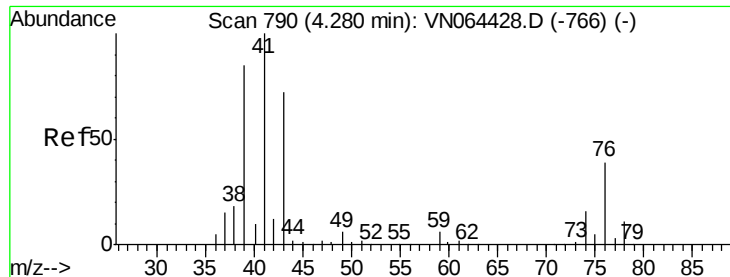

#18
Methyl Acetate
Concen: 2.001 ug/l
RT: 4.29 min Scan# 793
Delta R.T. 0.01 min
Lab File: VN064498.D
Acq: 6 Nov 2020 21:17




Instrument :
MSVOA_N
ClientSampleId :
CONTAINER-002-1B

Tot Ion: 43 Resp: 6271
Ion Ratio Lower Upper
43 100
74 9.1 17.0 25.4#

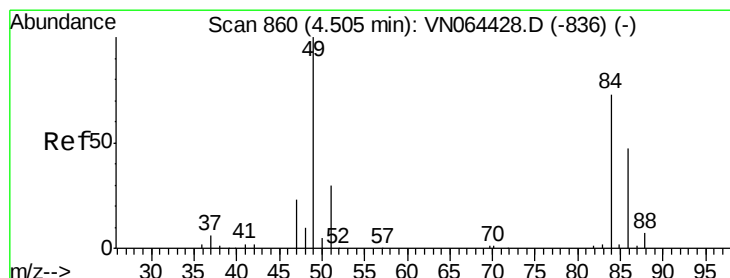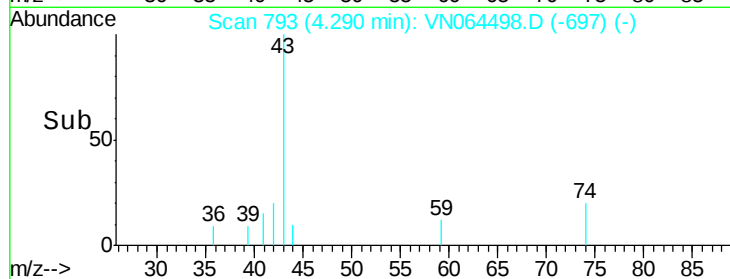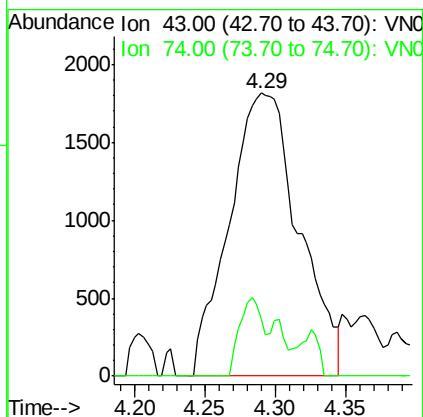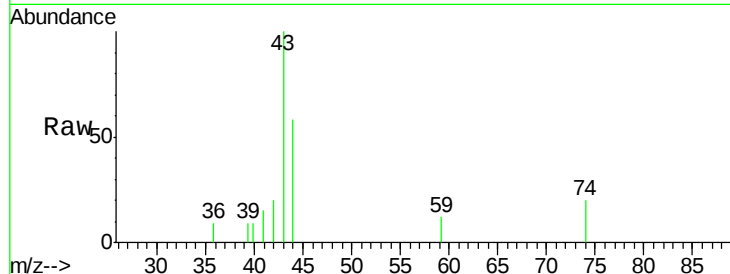

#20
Methylene Chloride
Concen: 2.796 ug/l
RT: 4.51 min Scan# 860
Delta R.T. -0.00 min
Lab File: VN064498.D
Acq: 6 Nov 2020 21:17

Tgt Ion: 84 Resp: 8842
Ion Ratio Lower Upper
84 100
49 134.3 110.1 165.1
51 54.5 33.6 50.4#
86 72.8 52.1 78.1


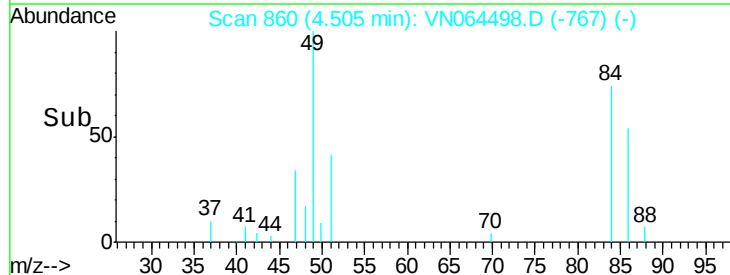
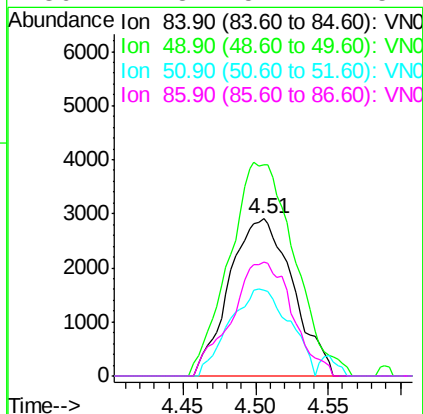
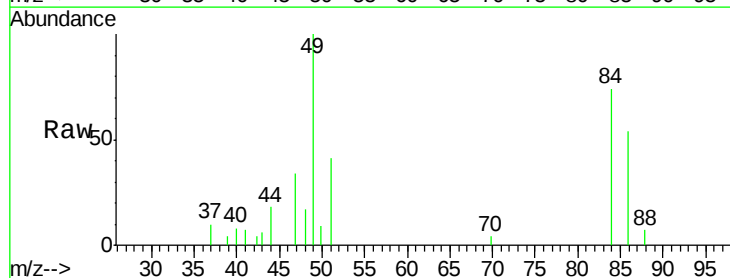




#33
 1,2-Dichloroethane-d4
 Concen: 57.057 ug/l
 RT: 7.99 min Scan# 1944
 Delta R.T. 0.00 min
 Lab File: VN064498.D
 Acq: 6 Nov 2020 21:17




Instrument :
 MSVOA_N
 ClientSampleId :
 CONTAINER-002-1B

Tot Ion: 65 Resp: 238774
 Ion Ratio Lower Upper
 65 100
 67 49.7 0.0 101.6

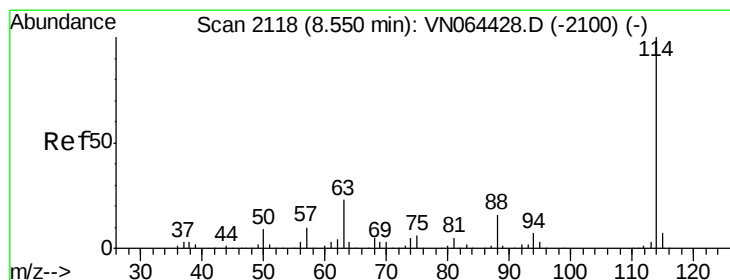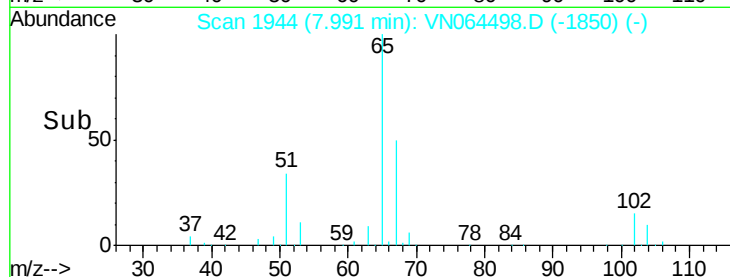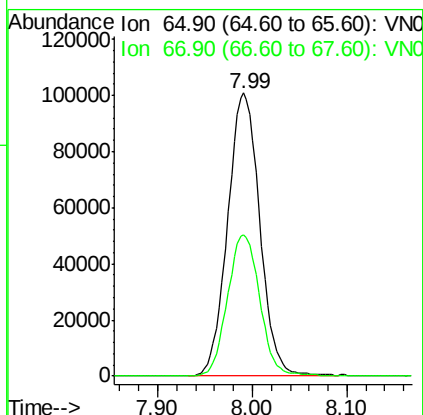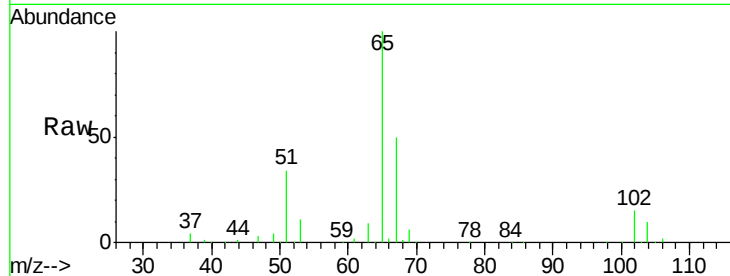

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN064498.D
 Acq: 6 Nov 2020 21:17

Tgt Ion: 114 Resp: 513059
 Ion Ratio Lower Upper
 114 100
 63 22.5 0.0 45.6
 88 16.5 0.0 32.8


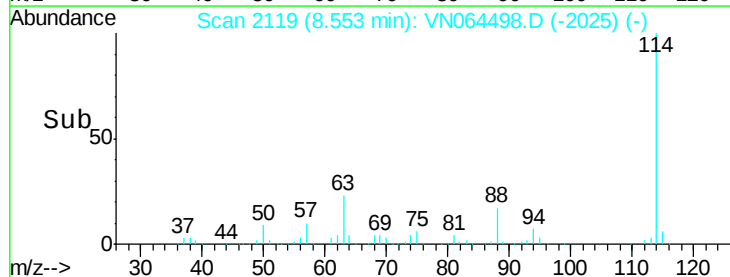
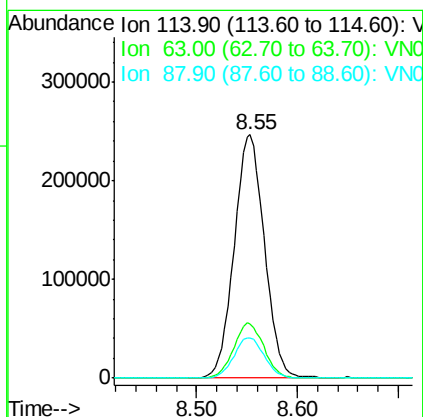
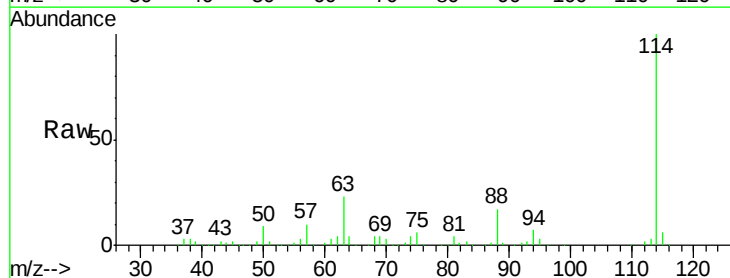




#35
 Dibromofluoromethane
 Concen: 49.133 ug/l
 RT: 7.55 min Scan# 1807
 Delta R.T. 0.00 min
 Lab File: VN064498.D
 Acq: 6 Nov 2020 21:17




Instrument :
 MSVOA_N
 ClientSampleId :
 CONTAINER-002-1B


Tot Ion:113 Resp: 171631
 Ion Ratio Lower Upper
 113 100
 111 103.3 81.1 121.7
 192 16.2 12.8 19.2

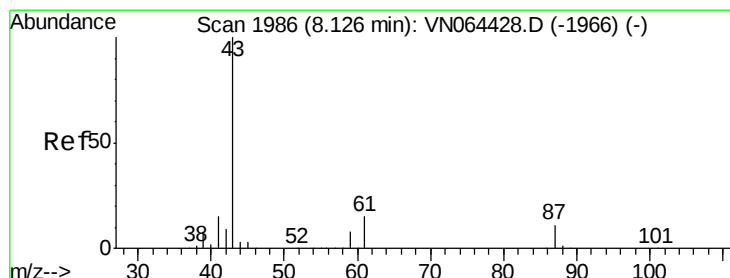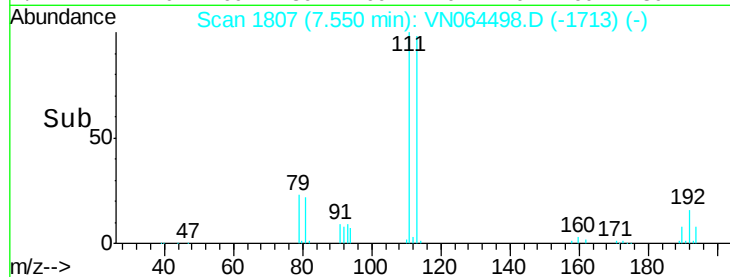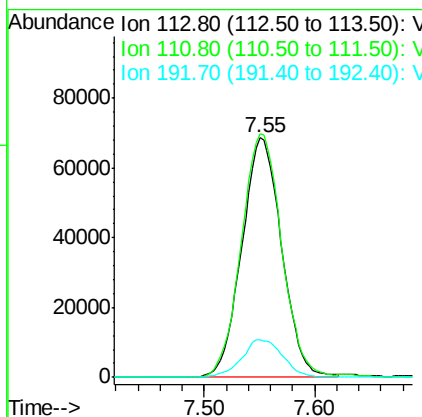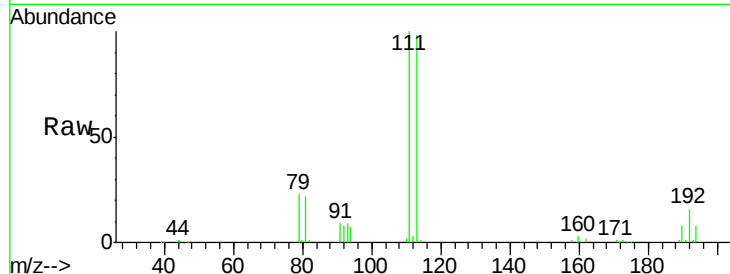

#43
 Isopropyl Acetate
 Concen: 11.397 ug/l
 RT: 8.13 min Scan# 1988
 Delta R.T. 0.01 min
 Lab File: VN064498.D
 Acq: 6 Nov 2020 21:17

Tgt Ion: 43 Resp: 100108
 Ion Ratio Lower Upper
 43 100
 61 17.4 14.0 21.0
 87 11.2 9.1 13.7

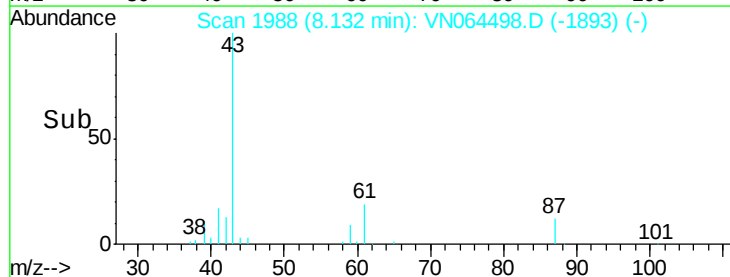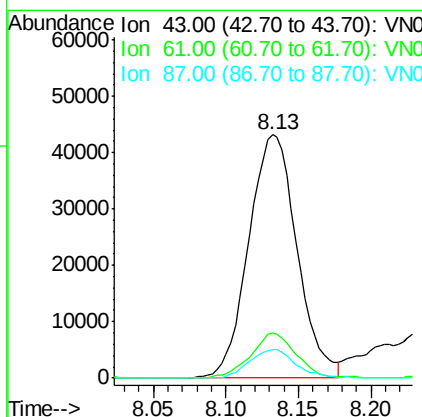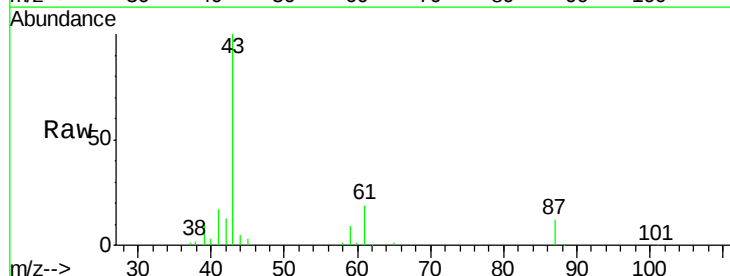

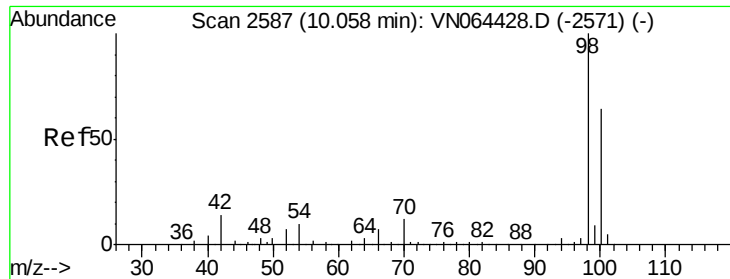

#50

Toluene-d8

Concen: 49.176 ug/l

RT: 10.06 min Scan# 2588

Delta R.T. 0.00 min

Lab File: VN064498.D

Acq: 6 Nov 2020 21:17

Instrument :

MSVOA_N

ClientSampleId :


CONTAINER-002-1B

Tot Ion: 98 Resp: 663938

Ion Ratio Lower Upper

98 100

100 62.6 50.7 76.1

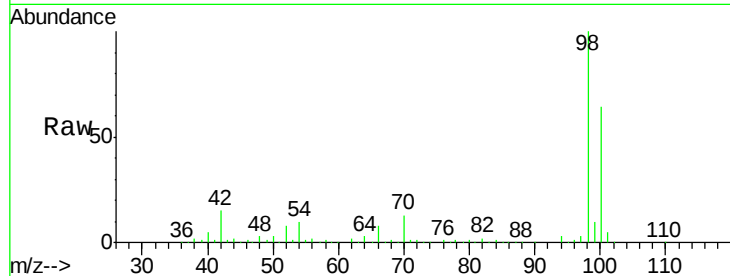

Abundance Ion 98.00 (97.70 to 98.70): VN064428.D (-2571) (-)

Ion 100.00 (99.70 to 100.70): VN064428.D (-2571) (-)

10.06

400000



300000

200000

100000

0

Time-->

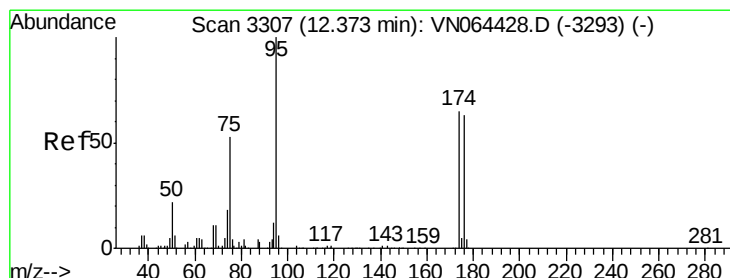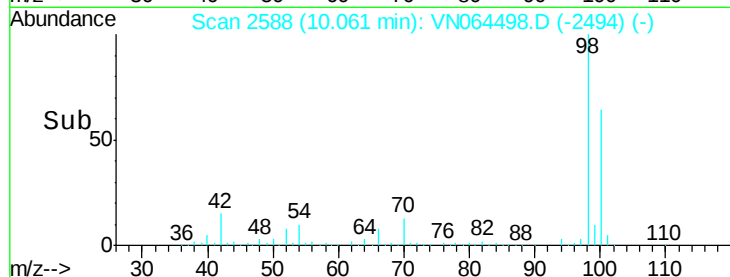

#62

4-Bromofluorobenzene

Concen: 49.291 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.00 min

Lab File: VN064498.D

Acq: 6 Nov 2020 21:17


Tgt Ion: 95 Resp: 251682

Ion Ratio Lower Upper

95 100

174 68.1 0.0 132.6

176 64.4 0.0 129.2

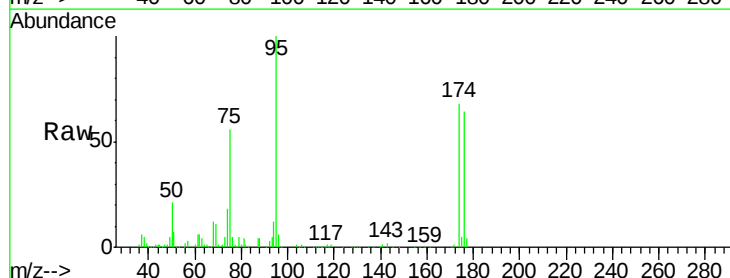

Abundance Ion 94.90 (94.60 to 95.60): VN064428.D (-3293) (-)

Ion 173.80 (173.50 to 174.50): VN064428.D (-3293) (-)

Ion 175.80 (175.50 to 176.50): VN064428.D (-3293) (-)

12.38

200000


150000


100000

50000

0

Time-->

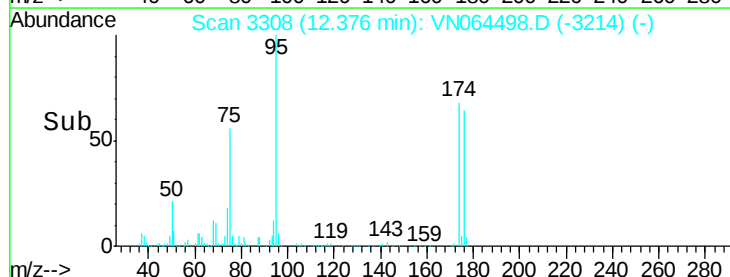


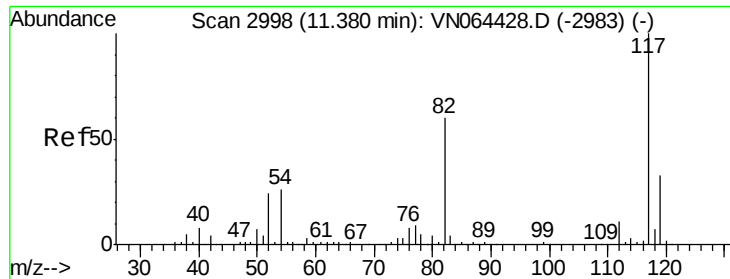




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. -0.00 min
Lab File: VN064498.D
Acq: 6 Nov 2020 21:17

Instrument :
MSVOA_N
ClientSampleId :
CONTAINER-002-1B

Tot Ion:117 Resp: 539978
Ion Ratio Lower Upper
117 100
82 60.2 48.1 72.1
119 31.4 26.2 39.4

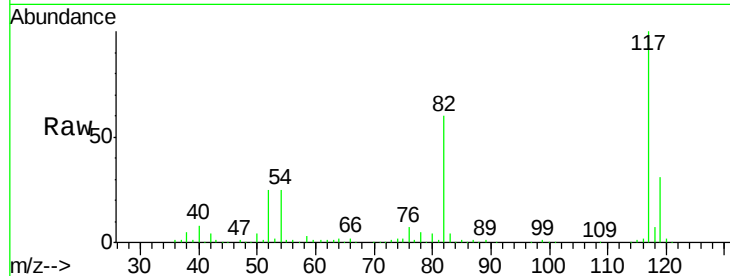


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

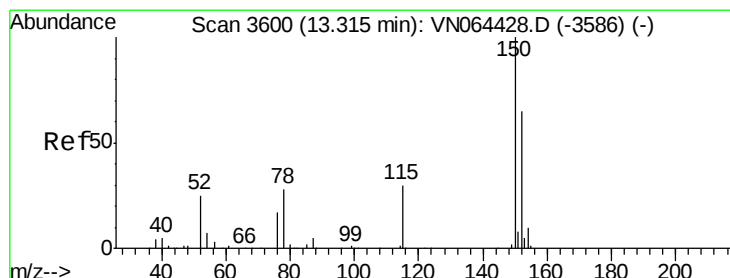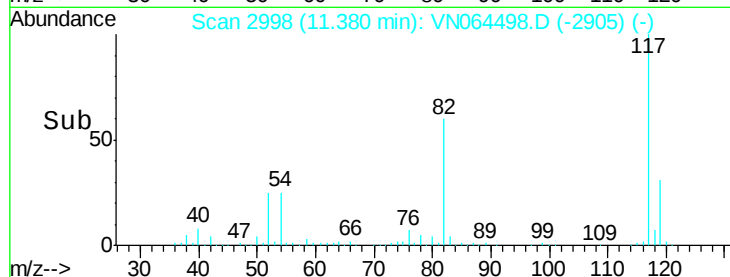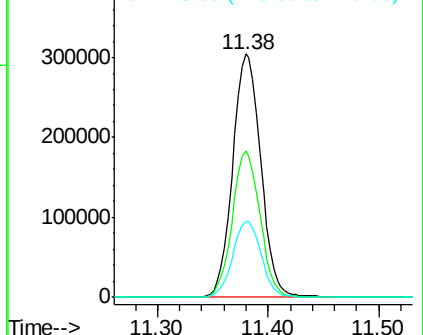

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN064498.D
Acq: 6 Nov 2020 21:17

Tgt Ion:152 Resp: 191504
Ion Ratio Lower Upper
152 100
115 65.4 32.0 96.0
150 156.0 0.0 353.8

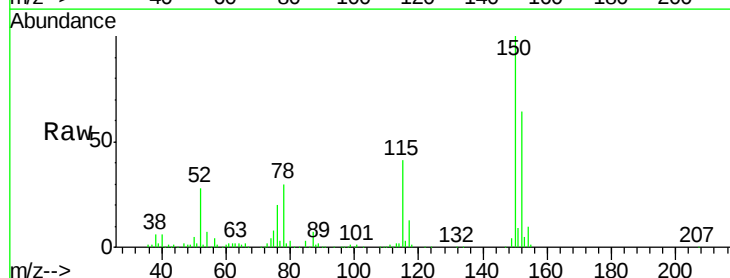

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

