

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110623\
 Data File : VN079952.D
 Acq On : 07 Nov 2023 07:41
 Operator : JC\MD
 Sample : 05107-35
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 07 12:31:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 02 05:49:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	268850	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	579036	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	631439	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	244533	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	245244	59.874	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 119.740%			
35) Dibromofluoromethane	8.171	113	200961	49.037	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 98.080%			
50) Toluene-d8	10.571	98	773108	51.244	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 102.480%			
62) 4-Bromofluorobenzene	12.853	95	266631	53.288	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 106.580%			
Target Compounds						
					Qvalue	
3) Chloromethane	2.359	50	1470	Below Cal		90
11) Tert butyl alcohol	5.518	59	4689	8.968	ug/l #	77
13) Acrolein	4.195	56	310	3.199	ug/l #	49
16) Acetone	4.436	43	90859	63.151	ug/l	98
17) Carbon Disulfide	4.712	76	2543	0.305	ug/l #	75
18) Methyl Acetate	5.042	43	13601	1.976	ug/l #	61
20) Methylene Chloride	5.283	84	29613	8.157	ug/l #	80
25) 2-Butanone	7.506	43	11877	5.637	ug/l #	75
26) 2,2-Dichloropropane	7.436	77	1067	0.207	ug/l #	53
29) Tetrahydrofuran	7.859	42	852	0.622	ug/l #	57
31) Cyclohexane	8.224	56	7260	1.341	ug/l #	40
36) 1,1-Dichloropropene	8.224	75	26237	4.484	ug/l #	47
37) Ethyl Acetate	7.577	43	4549	0.848	ug/l #	77
38) Carbon Tetrachloride	8.236	117	30141	5.111	ug/l #	15
40) Benzene	8.612	78	4620	0.264	ug/l	98
42) 1,2-Dichloroethane	8.688	62	1365	0.223	ug/l #	73
43) Isopropyl Acetate	8.694	43	209193	22.228	ug/l #	75
48) Methyl methacrylate	9.677	41	7676	1.862	ug/l #	31
51) 4-Methyl-2-Pentanone	10.447	43	484667	91.473	ug/l	88
52) Toluene	10.630	92	4294	0.413	ug/l	83
54) cis-1,3-Dichloropropene	10.365	75	74136	10.638	ug/l #	73
56) Ethyl methacrylate	10.794	69	2090	0.351	ug/l #	32
57) 1,3-Dichloropropane	11.206	76	6799	0.923	ug/l #	42
59) 2-Hexanone	11.171	43	212671	52.468	ug/l #	19
67) Ethyl Benzene	11.965	91	14729	0.617	ug/l	95
68) m/p-Xylenes	12.071	106	19082	2.147	ug/l	95
69) o-Xylene	12.400	106	119014	13.903	ug/l	89
70) Styrene	12.400	104	8056	0.586	ug/l #	1
74) N-amyl acetate	12.465	43	6888	0.850	ug/l #	37
76) 1,2,3-Trichloropropane	12.853	75	146654	25.545	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	146654	69.503	ug/l #	15
84) 1,2,4-Trimethylbenzene	13.506	105	9098	0.640	ug/l #	32
85) sec-Butylbenzene	13.506	105	9098	0.556	ug/l #	57
95) Naphthalene	15.641	128	16301	1.267	ug/l #	93

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110623\
Data File : VN079952.D
Acq On : 07 Nov 2023 07:41
Operator : JC\MD
Sample : 05107-35
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 46 Sample Multiplier: 1


Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Nov 07 12:31:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 02 05:49:08 2023
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed						


Quant Time: Nov 07 12:31:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 02 05:49:08 2023
Response via : Initial Calibration

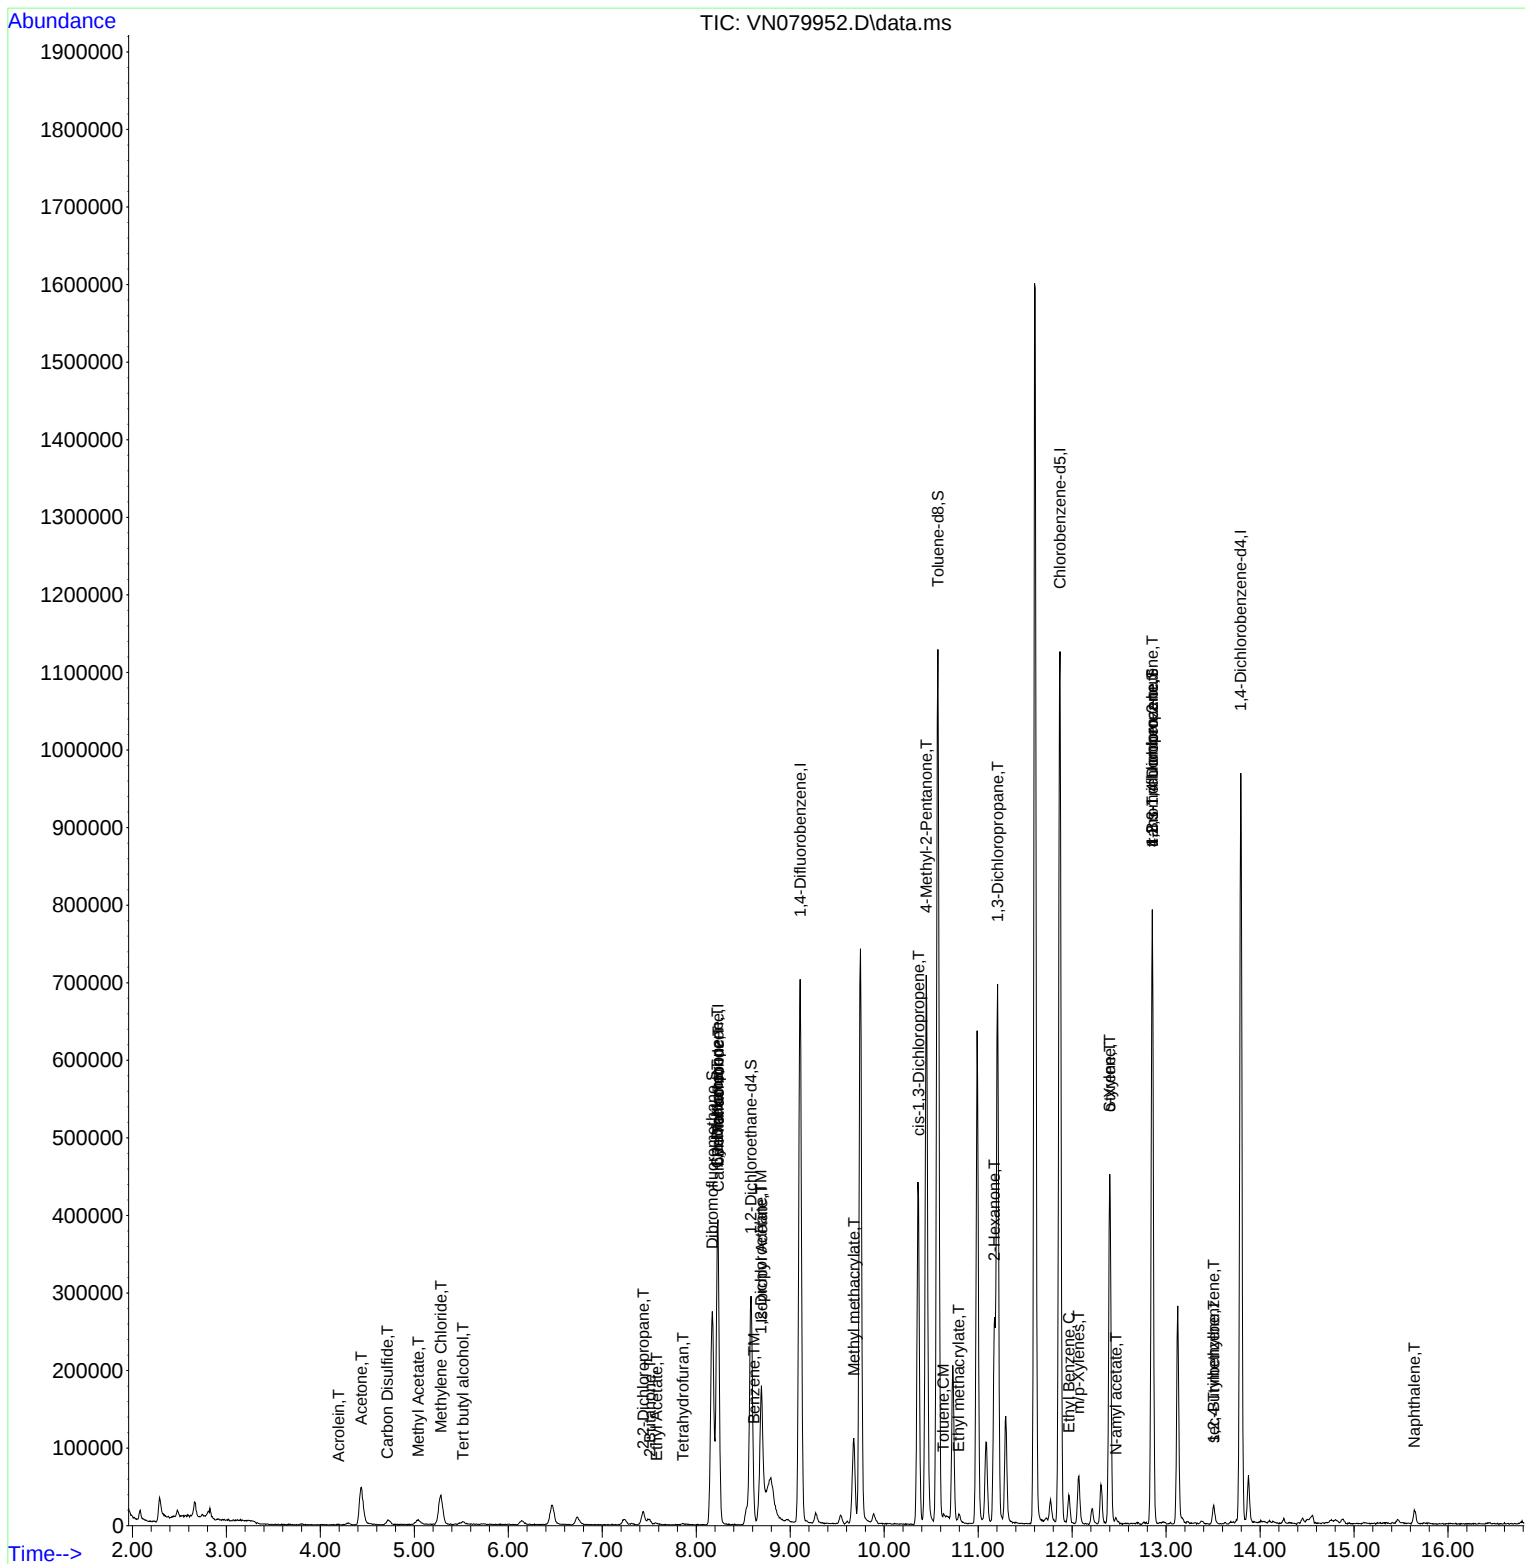






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 10
Delta R.T. 0.001 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:168 Resp: 268850
Ion Ratio Lower Upper
168 100
99 63.9 53.0 79.6

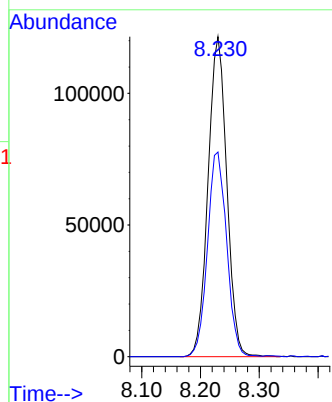

#3
Chloromethane
Concen: Below Cal
RT: 2.359 min Scan# 69
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Tgt Ion: 50 Resp: 1470
Ion Ratio Lower Upper
50 100
52 38.7 26.5 39.7



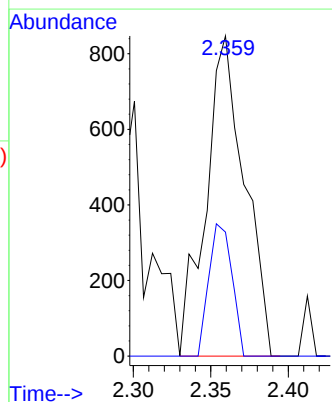





#11
Tert butyl alcohol
Concen: 8.968 ug/l
RT: 5.518 min Scan# 607
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 59 Resp: 4689
Ion Ratio Lower Upper
59 100
57 1.6 8.2 12.4#



#13
Acrolein
Concen: 3.199 ug/l
RT: 4.195 min Scan# 381
Delta R.T. 0.012 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Tgt Ion: 56 Resp: 310
Ion Ratio Lower Upper
56 100
55 27.1 54.5 81.7#


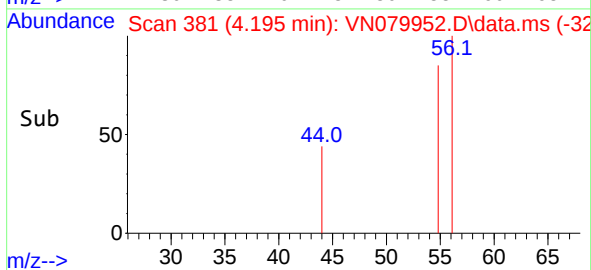






#16
Acetone
Concen: 63.151 ug/l
RT: 4.436 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 90859
Ion Ratio Lower Upper
43 100
58 36.2 28.0 42.0



#17
Carbon Disulfide
Concen: 0.305 ug/l
RT: 4.712 min Scan# 469
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Tgt Ion: 76 Resp: 2543
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.0#





#18

Methyl Acetate

Concen: 1.976 ug/l

RT: 5.042 min Scan# 51

Delta R.T. 0.018 min

Lab File: VN079952.D

Acq: 07 Nov 2023 07:41

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 13601

Ion Ratio Lower Upper

43 100

74 10.7 26.2 39.4#

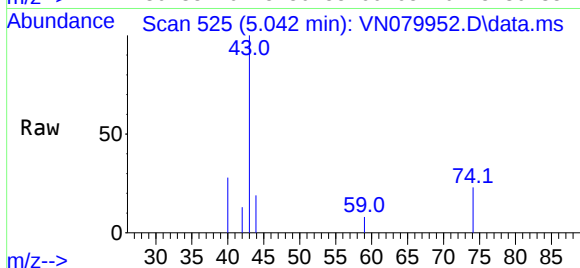

#20

Methylene Chloride

Concen: 8.157 ug/l

RT: 5.283 min Scan# 566

Delta R.T. 0.012 min

Lab File: VN079952.D

Acq: 07 Nov 2023 07:41

Tgt Ion: 84 Resp: 29613




Ion Ratio Lower Upper


84 100

49 133.1 79.7 119.5#

51 35.9 25.2 37.8

86 62.9 53.3 79.9

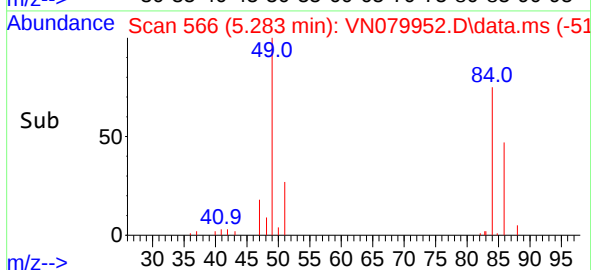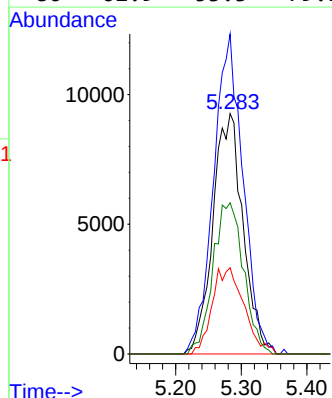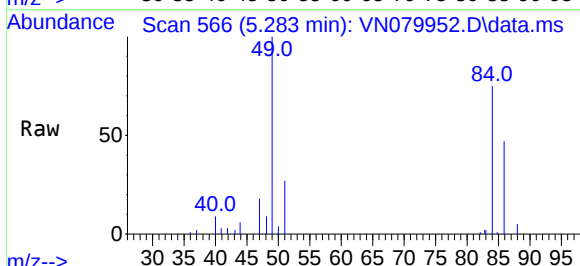



#25

2-Butanone

Concen: 5.637 ug/l

RT: 7.506 min Scan# 94

Delta R.T. 0.018 min

Lab File: VN079952.D

Acq: 07 Nov 2023 07:41

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 11877

Ion Ratio Lower Upper

43 100

72 22.8 30.2 45.2#

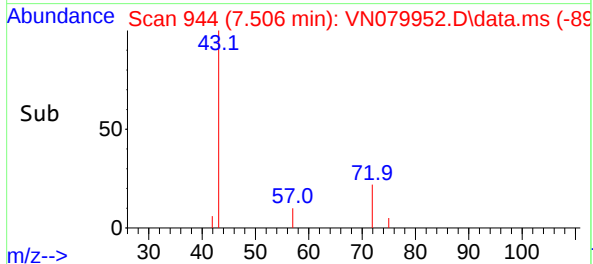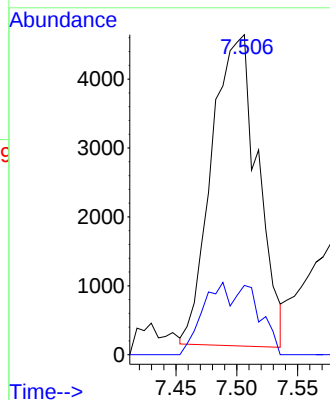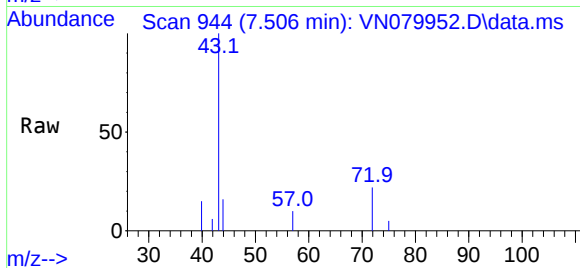

#26

2,2-Dichloropropane

Concen: 0.207 ug/l

RT: 7.436 min Scan# 932

Delta R.T. -0.053 min

Lab File: VN079952.D




Acq: 07 Nov 2023 07:41


Tgt Ion: 77 Resp: 1067

Ion Ratio Lower Upper

77 100

97 0.0 11.2 33.6#


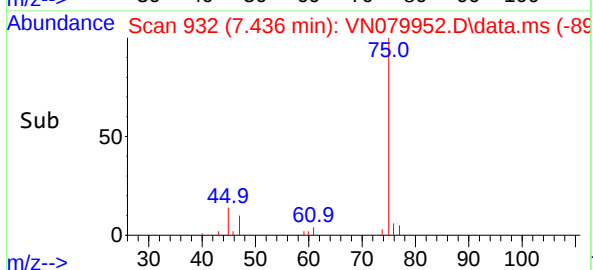
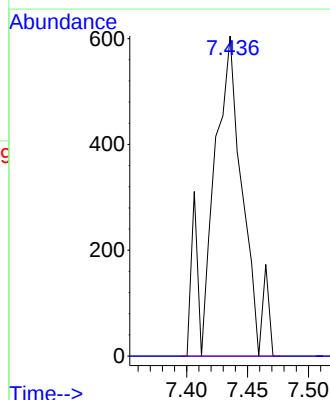
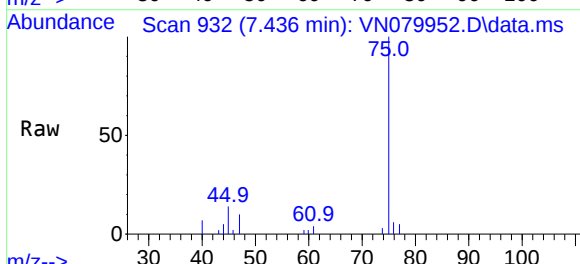


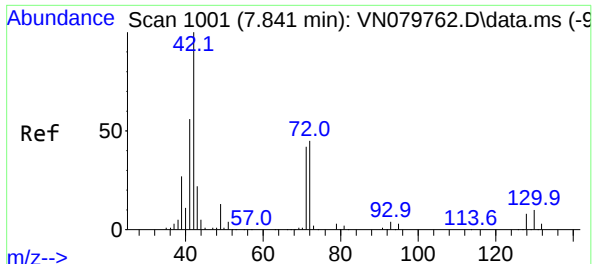

#29
Tetrahydrofuran
Concen: 0.622 ug/l
RT: 7.859 min Scan# 1066
Delta R.T. 0.018 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 42 Resp: 852
Ion Ratio Lower Upper
42 100
72 40.6 49.8 74.6#
71 14.9 47.4 71.2#

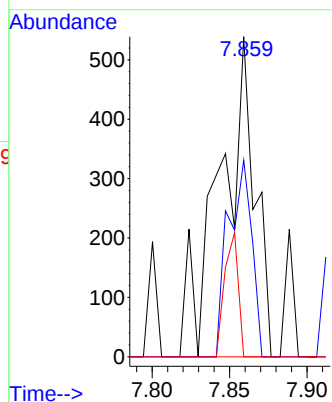

#31
Cyclohexane
Concen: 1.341 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.035 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Tgt Ion: 56 Resp: 7260
Ion Ratio Lower Upper
56 100
69 114.7 26.8 40.2#
84 135.1 81.8 122.6#


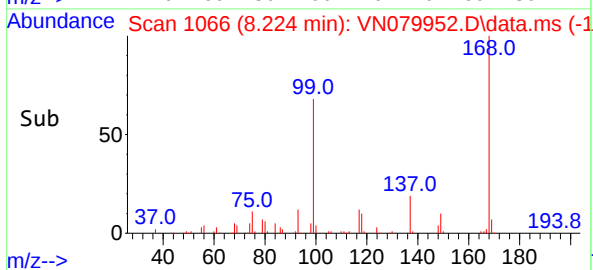

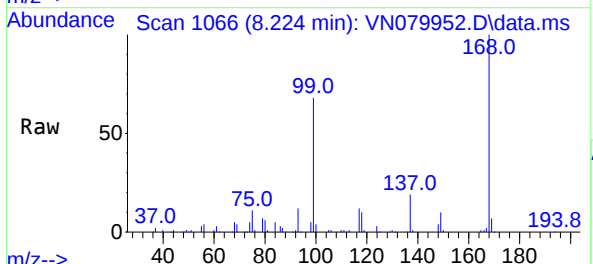




#33
1,2-Dichloroethane-d4
Concen: 59.874 ug/l
RT: 8.583 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 65 Resp: 245244
Ion Ratio Lower Upper
65 100
67 51.1 0.0 106.6

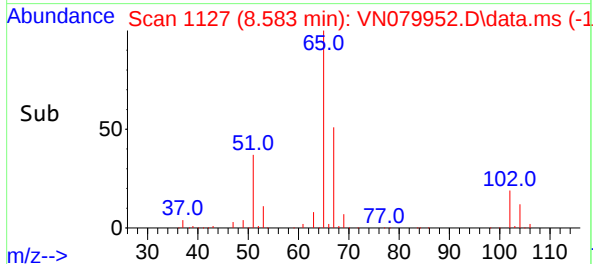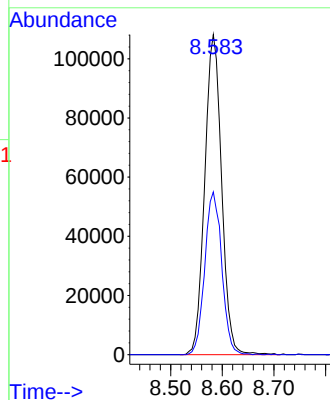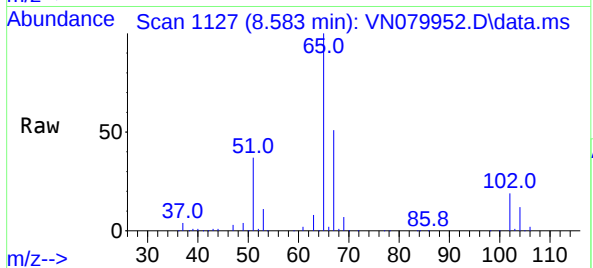

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 1216
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41


Tgt Ion: 114 Resp: 579036
Ion Ratio Lower Upper
114 100
63 22.7 0.0 36.4
88 16.7 0.0 30.6

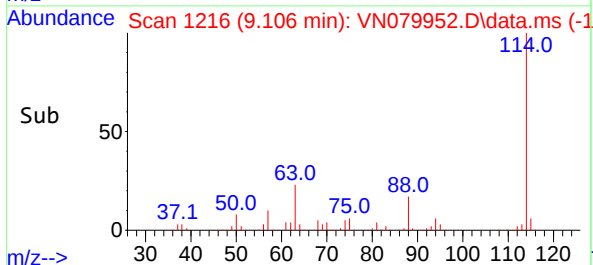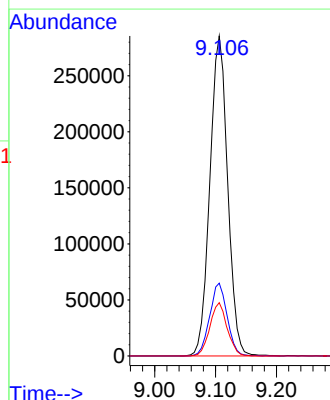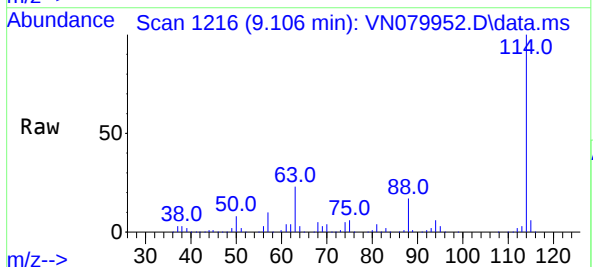



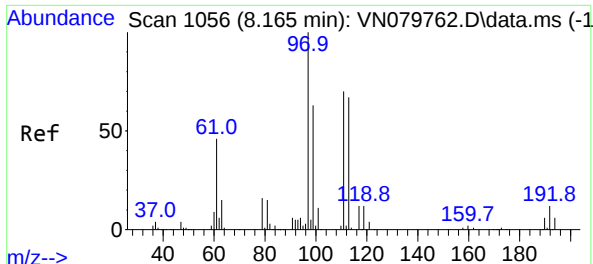


#35
Dibromofluoromethane
Concen: 49.037 ug/l
RT: 8.171 min Scan# 1056
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Instrument :
MSVOA_N
ClientSampleId :



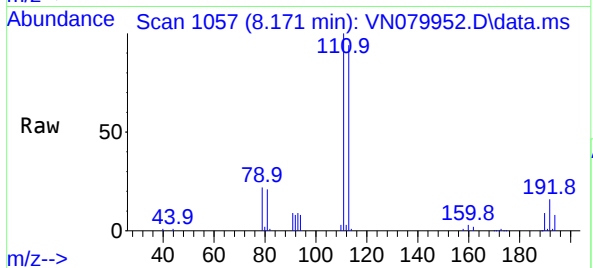



Tgt Ion:113 Resp: 200961
Ion Ratio Lower Upper
113 100
111 104.2 82.6 123.8
192 16.8 12.7 19.1

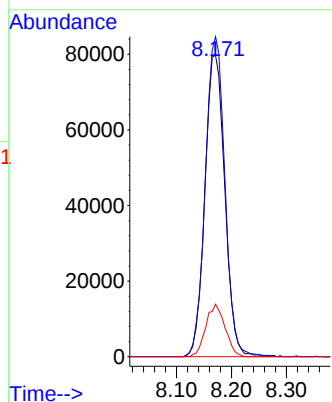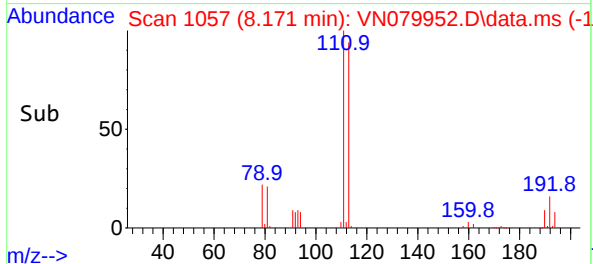

#36
1,1-Dichloropropene
Concen: 4.484 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.153 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41


Tgt Ion: 75 Resp: 26237
Ion Ratio Lower Upper
75 100
110 7.5 19.1 57.3#
77 0.0 25.0 37.4#

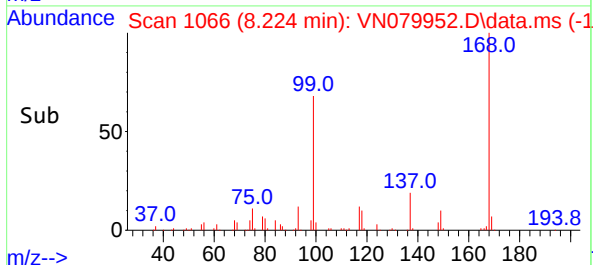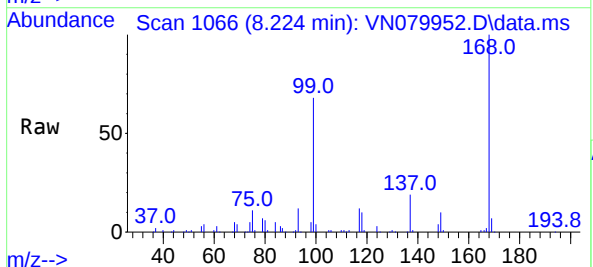





#37
Ethyl Acetate
Concen: 0.848 ug/l
RT: 7.577 min Scan# 91
Delta R.T. 0.012 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 4549
Ion Ratio Lower Upper
43 100
61 3.4 13.2 19.8#
70 8.4 11.3 16.9#

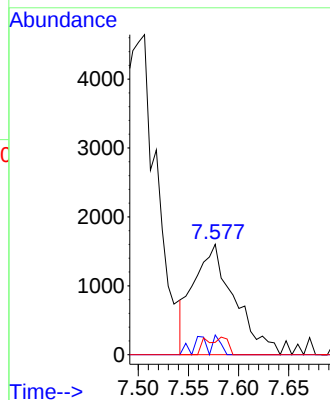

#38
Carbon Tetrachloride
Concen: 5.111 ug/l
RT: 8.236 min Scan# 1068
Delta R.T. -0.123 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Tgt Ion: 117 Resp: 30141
Ion Ratio Lower Upper
117 100
119 4.7 77.3 115.9#
121 0.0 23.3 34.9#



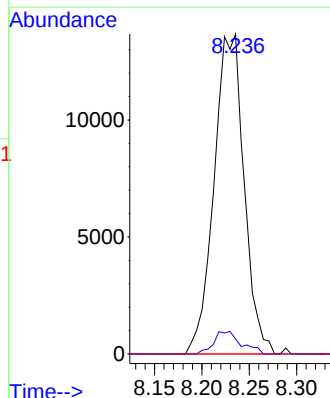





#40
Benzene
Concen: 0.264 ug/l
RT: 8.612 min Scan# 1132
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 78 Resp: 4620
Ion Ratio Lower Upper
78 100
77 22.6 19.0 28.6

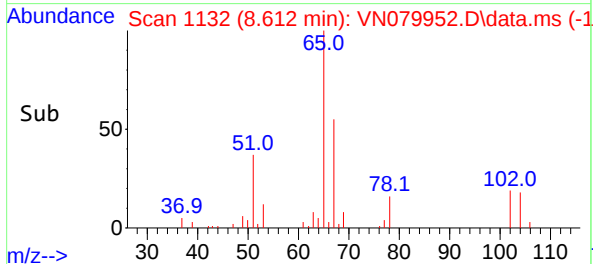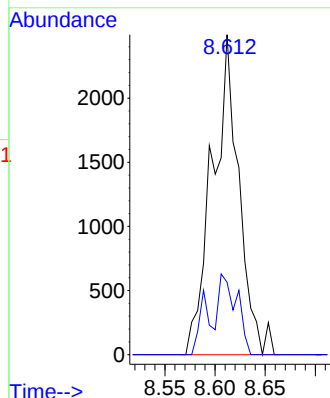

#42
1,2-Dichloroethane
Concen: 0.223 ug/l
RT: 8.688 min Scan# 1145
Delta R.T. 0.018 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41


Tgt Ion: 62 Resp: 1365
Ion Ratio Lower Upper
62 100
98 0.0 0.0 19.8

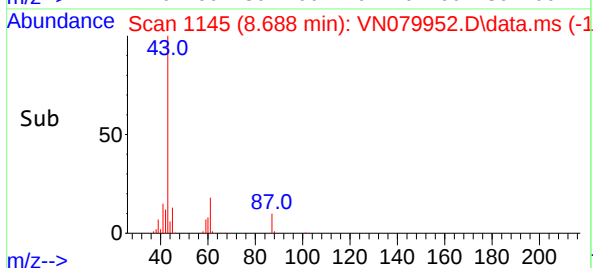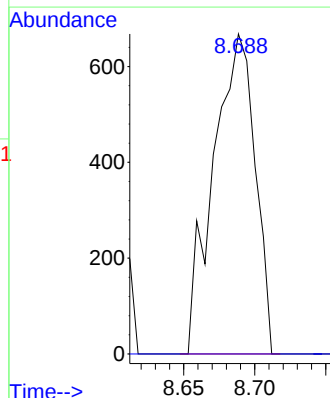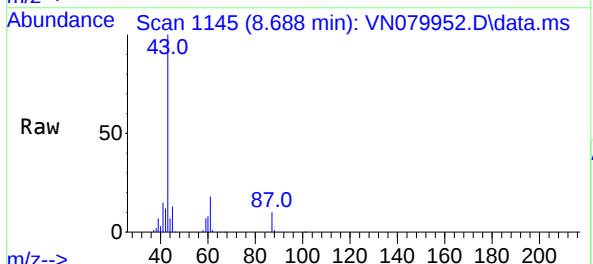






#43
Isopropyl Acetate
Concen: 22.228 ug/l
RT: 8.694 min Scan# 1145
Delta R.T. 0.006 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Instrument :
MSVOA_N
ClientSampleId :



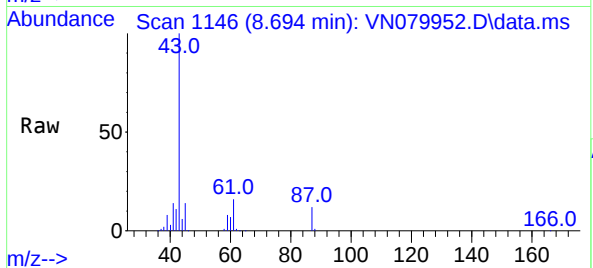



Tgt Ion: 43 Resp: 209193
Ion Ratio Lower Upper
43 100
61 15.2 24.7 37.1#
87 9.7 14.6 21.8#

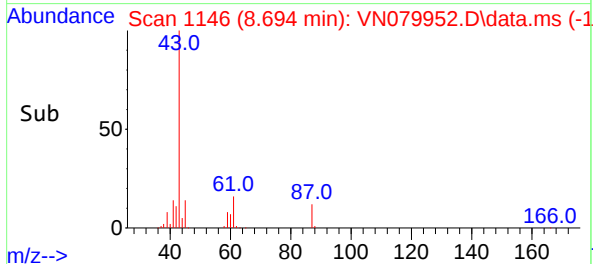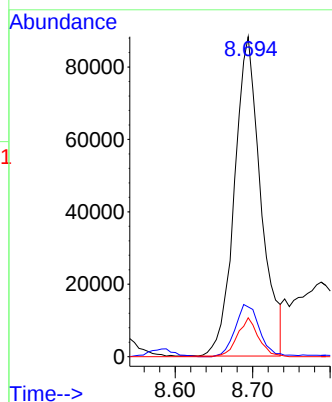

#48
Methyl methacrylate
Concen: 1.862 ug/l
RT: 9.677 min Scan# 1313
Delta R.T. -0.006 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Tgt Ion: 41 Resp: 7676
Ion Ratio Lower Upper
41 100
69 0.0 90.4 135.6#
39 62.1 54.6 81.8


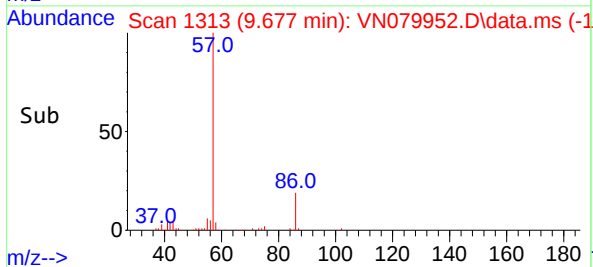
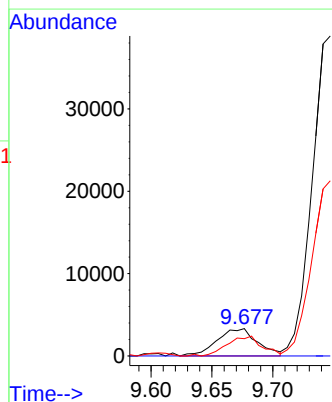
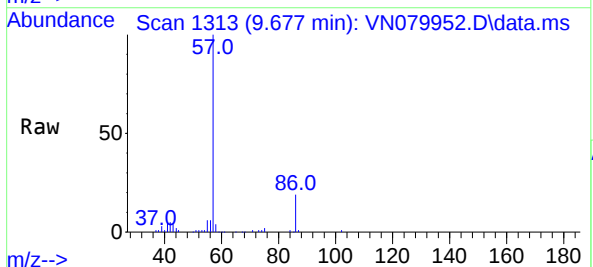




#50
Toluene-d8
Concen: 51.244 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 773108
Ion Ratio Lower Upper
98 100
100 64.6 52.0 78.0

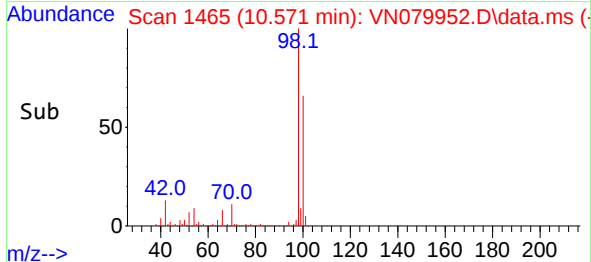

#51
4-Methyl-2-Pentanone
Concen: 91.473 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Tgt Ion: 43 Resp: 484667
Ion Ratio Lower Upper
43 100
58 37.6 36.6 54.8


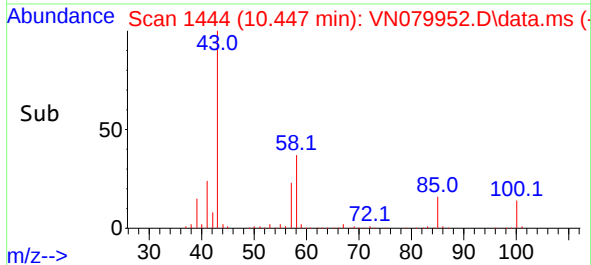






#52
Toluene
Concen: 0.413 ug/l
RT: 10.630 min Scan# 1476
Delta R.T. -0.006 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 92 Resp: 4294
Ion Ratio Lower Upper
92 100
91 148.1 137.4 206.0



#54
cis-1,3-Dichloropropene
Concen: 10.638 ug/l
RT: 10.365 min Scan# 1430
Delta R.T. 0.047 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Tgt Ion: 75 Resp: 74136
Ion Ratio Lower Upper
75 100
77 0.4 26.1 39.1#
39 38.7 31.6 47.4


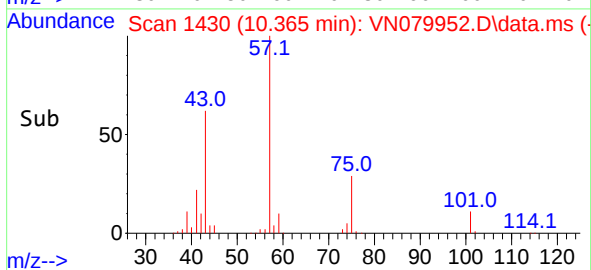






#56
Ethyl methacrylate
Concen: 0.351 ug/l
RT: 10.794 min Scan# 11
Delta R.T. -0.082 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 69 Resp: 2090
Ion Ratio Lower Upper
69 100
41 0.0 39.6 59.4#
39 0.0 28.6 43.0#



#57
1,3-Dichloropropane
Concen: 0.923 ug/l
RT: 11.206 min Scan# 1573
Delta R.T. 0.041 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Tgt Ion: 76 Resp: 6799
Ion Ratio Lower Upper
76 100
78 0.0 26.1 39.1#


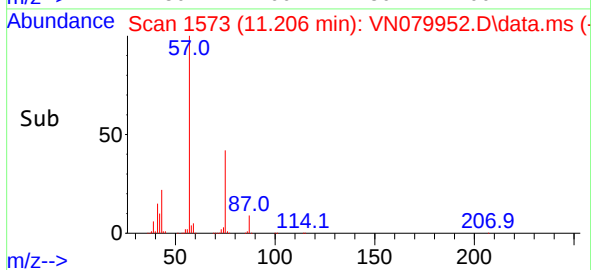






#59
2-Hexanone
Concen: 52.468 ug/l
RT: 11.171 min Scan# 111
Delta R.T. -0.029 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 212671
Ion Ratio Lower Upper
43 100
58 0.0 31.7 95.1#

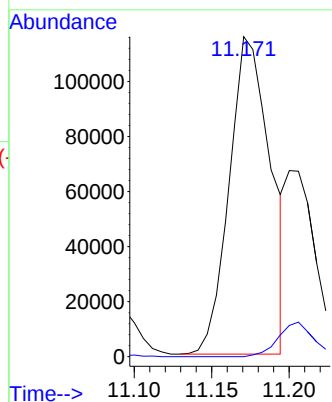

#62
4-Bromofluorobenzene
Concen: 53.288 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Tgt Ion: 95 Resp: 266631
Ion Ratio Lower Upper
95 100
174 72.4 0.0 143.8
176 70.0 0.0 135.8


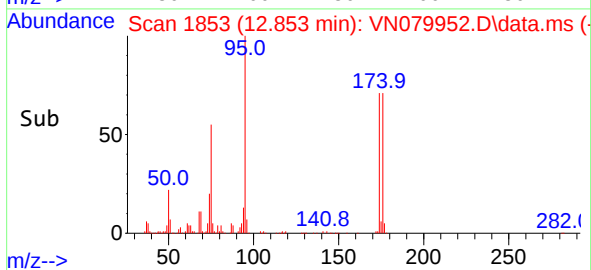






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 631439
Ion Ratio Lower Upper
117 100
82 57.6 44.0 66.0
119 32.6 25.6 38.4

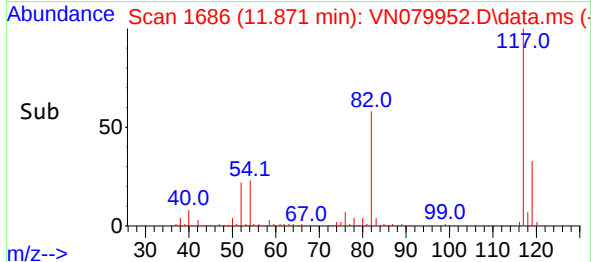

#67
Ethyl Benzene
Concen: 0.617 ug/l
RT: 11.965 min Scan# 1702
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Tgt Ion: 91 Resp: 14729
Ion Ratio Lower Upper
91 100
106 29.1 25.6 38.4









#68
m/p-Xylenes
Concen: 2.147 ug/l
RT: 12.071 min Scan# 1720
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 19082
Ion Ratio Lower Upper
106 100
91 192.3 159.6 239.4

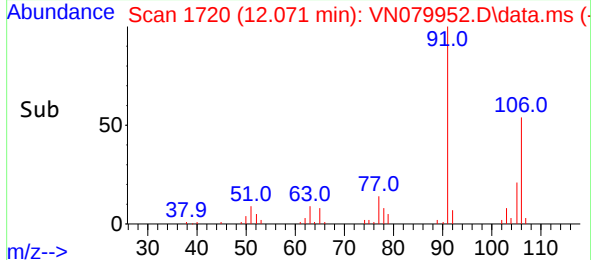

#69
o-Xylene
Concen: 13.903 ug/l
RT: 12.400 min Scan# 1776
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Tgt Ion:106 Resp: 119014
Ion Ratio Lower Upper
106 100
91 227.5 105.2 315.5


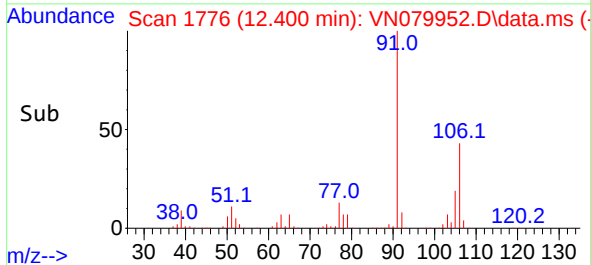






#70
Styrene
Concen: 0.586 ug/l
RT: 12.400 min Scan# 11
Delta R.T. -0.012 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:	104	Resp:	8056
Ion Ratio	Lower	Upper	
104	100		
78	256.6	39.5	59.3#
103	230.2	43.2	64.8#

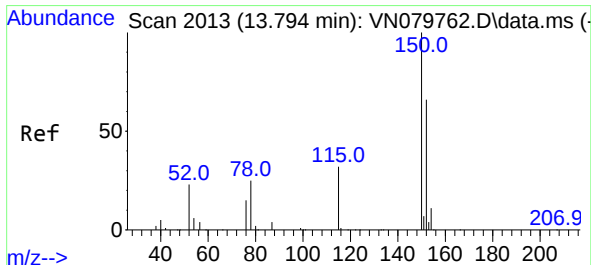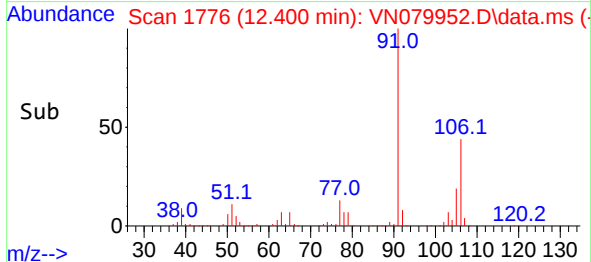

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Tgt Ion:	152	Resp:	244533
Ion Ratio	Lower	Upper	
152	100		
115	63.8	32.3	96.8
150	161.1	0.0	355.8




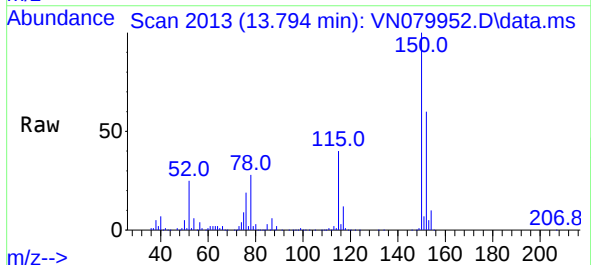




#74
N-amy1 acetate
Concen: 0.850 ug/l
RT: 12.465 min Scan# 11
Delta R.T. -0.029 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43	Resp: 6888
Ion Ratio	Lower Upper
43 100	
70 0.0	43.4 65.2#
55 3.3	21.4 32.0#
61 0.0	22.8 34.2#

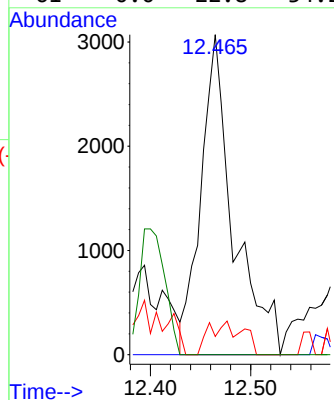

#76
1,2,3-Trichloropropane
Concen: 25.545 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.141 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41


Tgt Ion: 75	Resp: 146654
Ion Ratio	Lower Upper
75 100	
77 1.6	84.5 253.5#

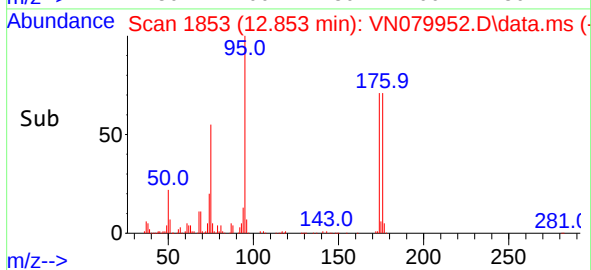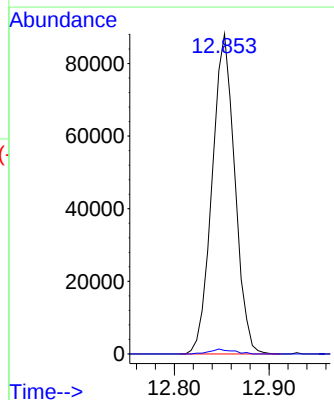



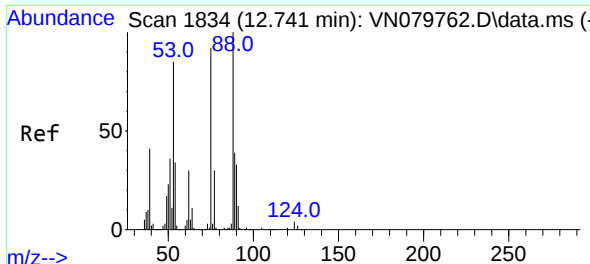


#81
trans-1,4-Dichloro-2-butene
Concen: 69.503 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.118 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Instrument :
MSVOA_N
ClientSampleId :



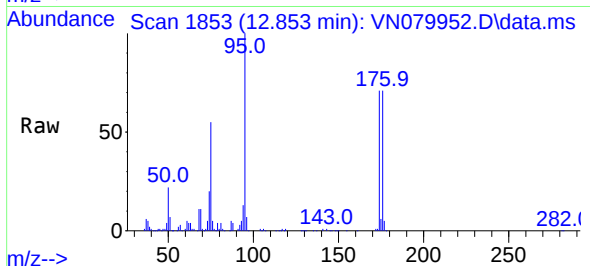



Tgt Ion: 75 Resp: 146654
Ion Ratio Lower Upper
75 100
53 0.3 67.4 101.2#
89 0.0 38.8 58.2#

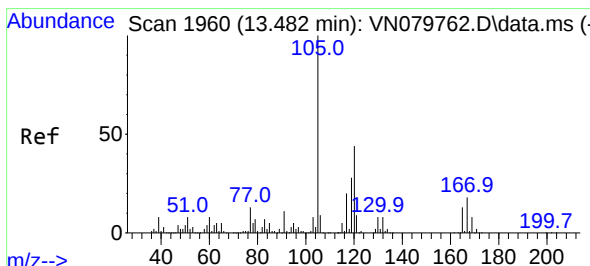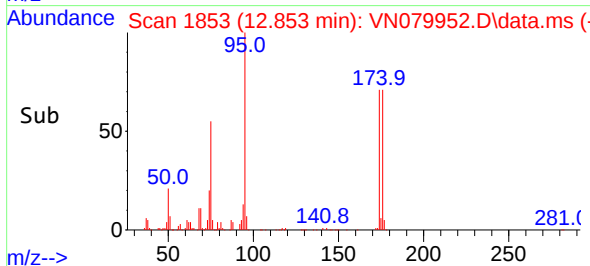

#84
1,2,4-Trimethylbenzene
Concen: 0.640 ug/l
RT: 13.506 min Scan# 1964
Delta R.T. 0.024 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Tgt Ion: 105 Resp: 9098
Ion Ratio Lower Upper
105 100
120 0.0 22.0 66.0#


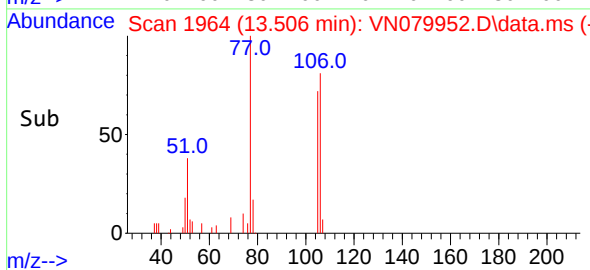

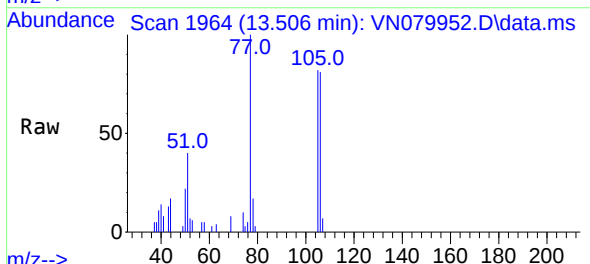




#85
sec-Butylbenzene
Concen: 0.556 ug/l
RT: 13.506 min Scan# 1964
Delta R.T. -0.112 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:105 Resp: 9098
Ion Ratio Lower Upper
105 100
134 0.0 9.8 29.3#

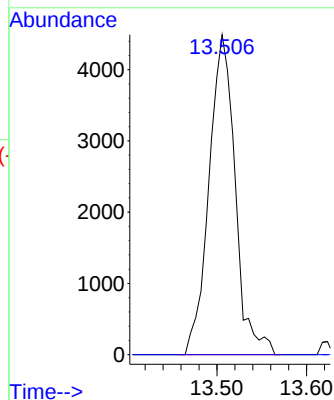

#95
Naphthalene
Concen: 1.267 ug/l
RT: 15.641 min Scan# 2327
Delta R.T. 0.000 min
Lab File: VN079952.D
Acq: 07 Nov 2023 07:41

Tgt Ion:128 Resp: 16301
Ion Ratio Lower Upper
128 100
127 13.1 10.0 15.0
129 5.5 8.7 13.1#

