
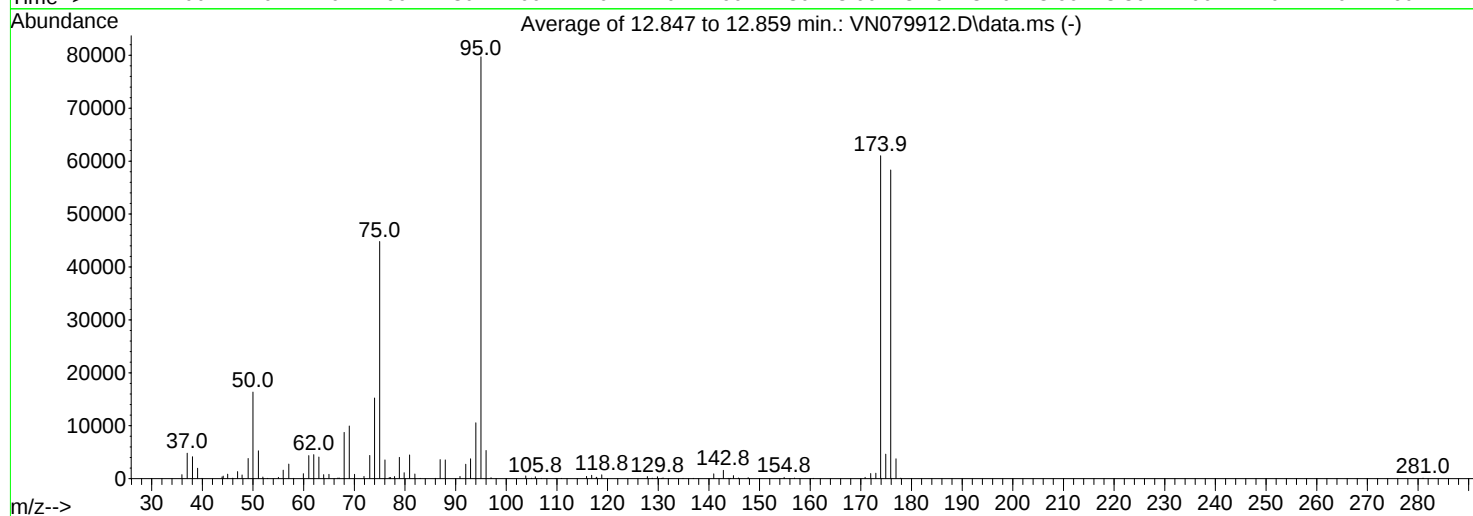


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110623\
Data File : VN079912.D
Acq On : 06 Nov 2023 09:53
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Title : SW846 8260
Last Update : Thu Nov 02 05:49:08 2023

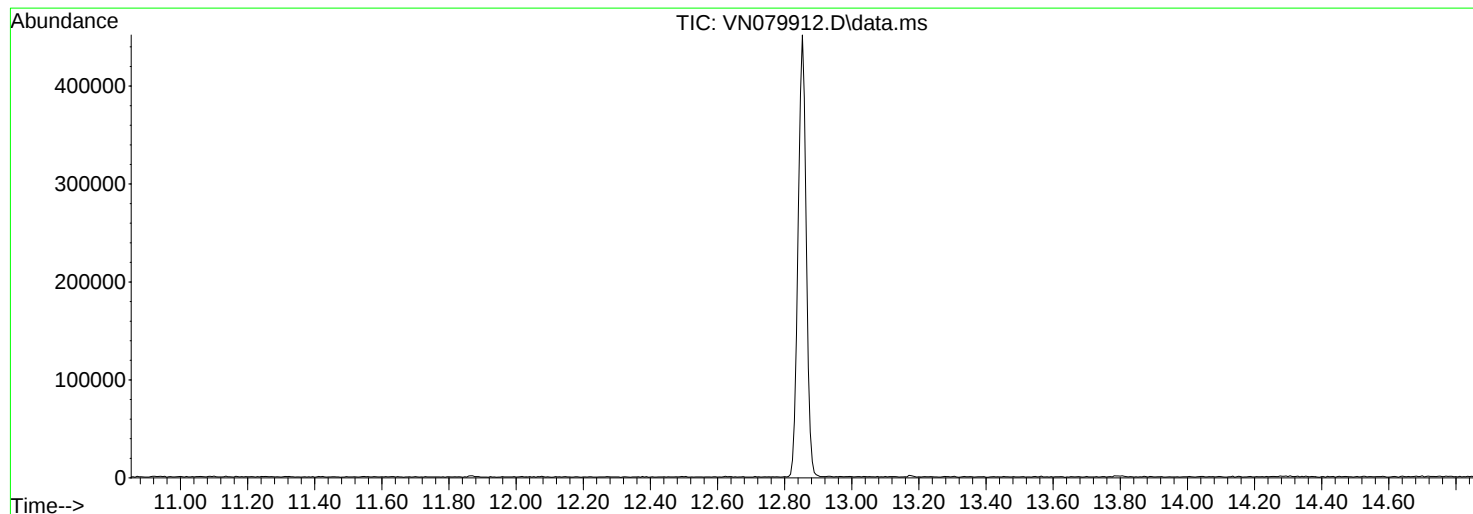

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	16369	PASS
75	95	30	60	56.2	44821	PASS
95	95	100	100	100.0	79709	PASS
96	95	5	9	6.7	5328	PASS
173	174	0.00	2	1.7	1019	PASS
174	95	50	100	76.5	61013	PASS
175	174	5	9	7.6	4621	PASS
176	174	95	101	95.6	58320	PASS
177	176	5	9	6.4	3741	PASS

Average of 12.847 to 12.859 min.: VN079912.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	754	49.05	3821	62.00	4551	74.00	1523
37.00	4804	50.00	16369	63.00	4088	75.00	4482
38.05	4144	51.05	5265	63.95	755	76.05	355
39.05	1971	51.95	314	65.00	822	76.90	21
39.90	66	52.90	62	66.75	124	77.15	223
43.90	320	55.00	239	67.00	113	77.95	411
44.10	488	55.95	1604	68.00	8728	78.90	4030
45.00	850	57.05	2758	69.00	9949	79.85	1132
46.00	97	58.00	74	70.05	804	80.90	4467
46.95	1345	59.95	924	71.90	414	81.95	880
47.85	708	61.00	4370	73.05	4398	83.00	67

Average of 12.847 to 12.859 min.: VN079912.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.00	61	105.00	84	128.80	93	145.85	118
86.95	3602	105.75	361	129.85	356	147.75	191
87.95	3545	106.90	57	130.70	69	154.85	248
90.85	436	109.80	58	130.95	142	156.90	124
92.00	2717	110.90	56	134.90	68	160.60	57
92.95	3745	115.85	422	136.90	71	170.85	256
94.00	10546	116.85	632	140.95	923	171.95	966
95.00	79709	117.70	139	142.85	1589	172.95	1019
96.00	5328	117.85	285	143.80	54	173.90	61013
97.00	186	118.85	715	144.20	51	174.90	4621
103.85	502	127.85	410	144.85	584	175.90	58320

Average of 12.847 to 12.859 min.: VN079912.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.95	3741						
177.90	80						
281.00	83						

Instrument :

MSVOA_N

ClientSampleId :

BFB