
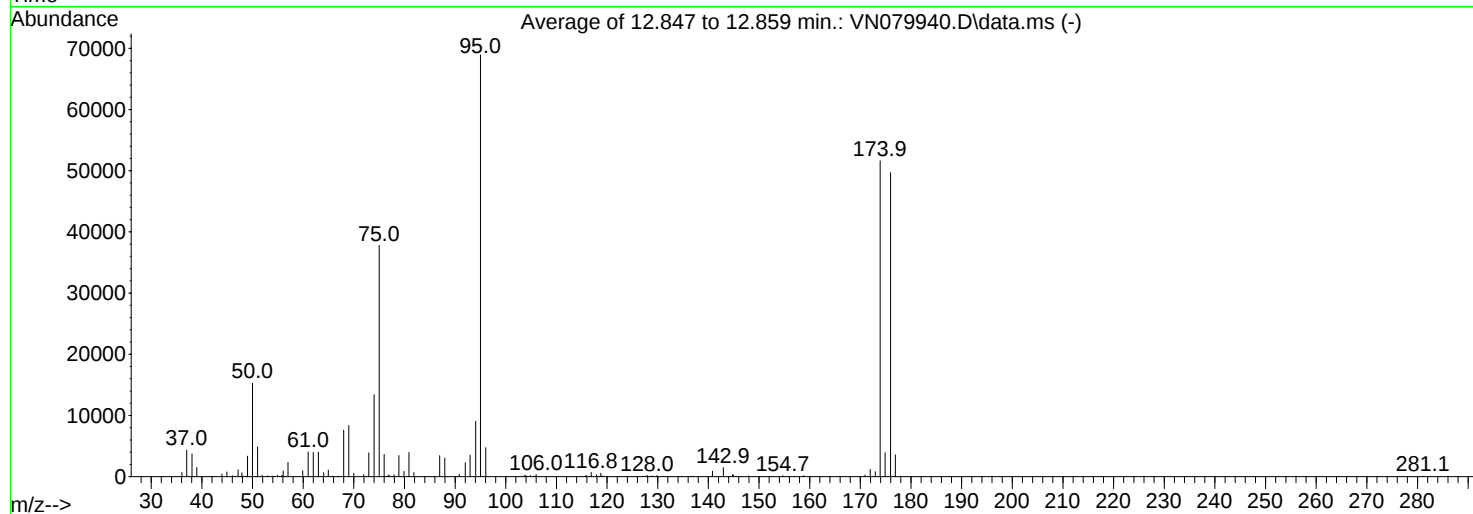


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110623\
Data File : VN079940.D
Acq On : 07 Nov 2023 01:29
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Title : SW846 8260
Last Update : Thu Nov 02 05:49:08 2023

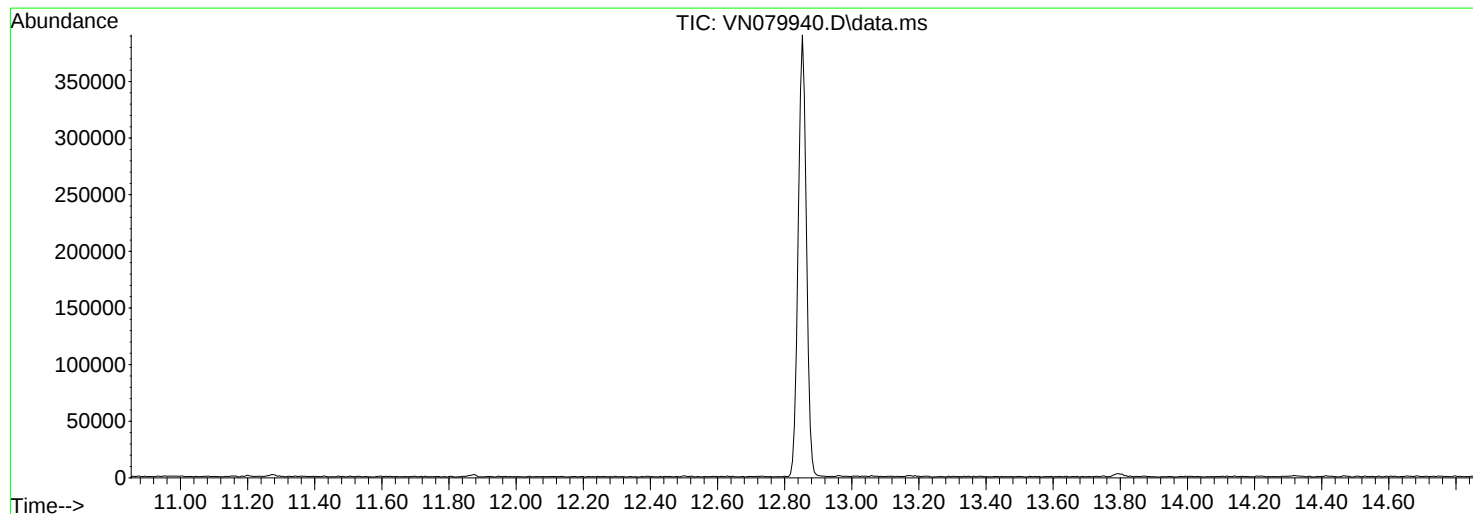

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	15283	PASS
75	95	30	60	54.8	37781	PASS
95	95	100	100	100.0	68939	PASS
96	95	5	9	6.9	4743	PASS
173	174	0.00	2	1.6	812	PASS
174	95	50	100	74.9	51621	PASS
175	174	5	9	7.5	3897	PASS
176	174	95	101	96.3	49699	PASS
177	176	5	9	7.2	3554	PASS

Average of 12.847 to 12.859 min.: VN079940.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	688	51.00	4894	63.00	4009	74.00	1338
37.00	4345	51.90	224	64.05	661	75.00	3778
38.05	3705	52.95	136	64.95	1078	76.00	363
39.00	1517	53.90	76	65.80	81	76.80	22
43.95	444	54.95	202	66.80	59	76.95	301
44.95	771	55.80	219	67.00	54	77.95	318
46.05	159	56.05	919	68.00	7615	78.90	3449
47.15	1118	57.00	2358	69.00	8356	79.90	877
47.90	642	59.90	968	70.00	550	80.90	3950
49.00	3348	61.00	4058	71.95	338	81.85	695
50.00	15283	62.00	3964	72.95	3899	85.90	63

Average of 12.847 to 12.859 min.: VN079940.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.95	3417	104.85	177	128.90	131	154.90	50
87.95	3042	105.60	79	129.85	175	156.90	60
90.80	394	106.00	339	134.70	86	158.70	57
92.00	2275	115.70	103	136.60	54	158.85	150
92.95	3516	115.85	194	137.00	61	170.90	274
94.05	9046	116.85	673	140.80	888	171.95	1190
95.00	68939	117.90	280	142.95	1477	172.95	812
96.05	4743	118.75	551	144.75	321	173.90	51621
103.60	137	119.00	144	144.95	226	174.90	3897
103.85	247	127.80	114	147.90	135	175.95	49699
104.10	91	127.95	189	154.70	152	176.90	3554

Average of 12.847 to 12.859 min.: VN079940.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
177.90	74						
281.10	71						

Instrument :

MSVOA_N

ClientSampleId :

BFB