

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN110718\
 Data File : VN052209.D
 Acq On : 7 Nov 2018 16:05
 Operator : MD\SY
 Sample : J5844-04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 15 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 MH-C

Quant Time: Nov 07 16:26:57 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110518W.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 05 22:32:25 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	434996	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	713993	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	586787	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	199366	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	252838	49.02	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.04%	
35) Dibromofluoromethane	7.59	113	226183	51.02	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.04%	
50) Toluene-d8	10.09	98	863989	50.41	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.82%	
62) 4-Bromofluorobenzene	12.40	95	248584	44.18	ug/l	0.00
Spiked Amount	50.000		Recovery	=	88.36%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN110718\
Data File : VN052209.D
Acq On : 7 Nov 2018 16:05
Operator : MD\SY
Sample : J5844-04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 15 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
MH-C

Quant Time: Nov 07 16:26:57 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N110518W.M
Quant Title : SW846 8260
QLast Update : Mon Nov 05 22:32:25 2018
Response via : Initial Calibration

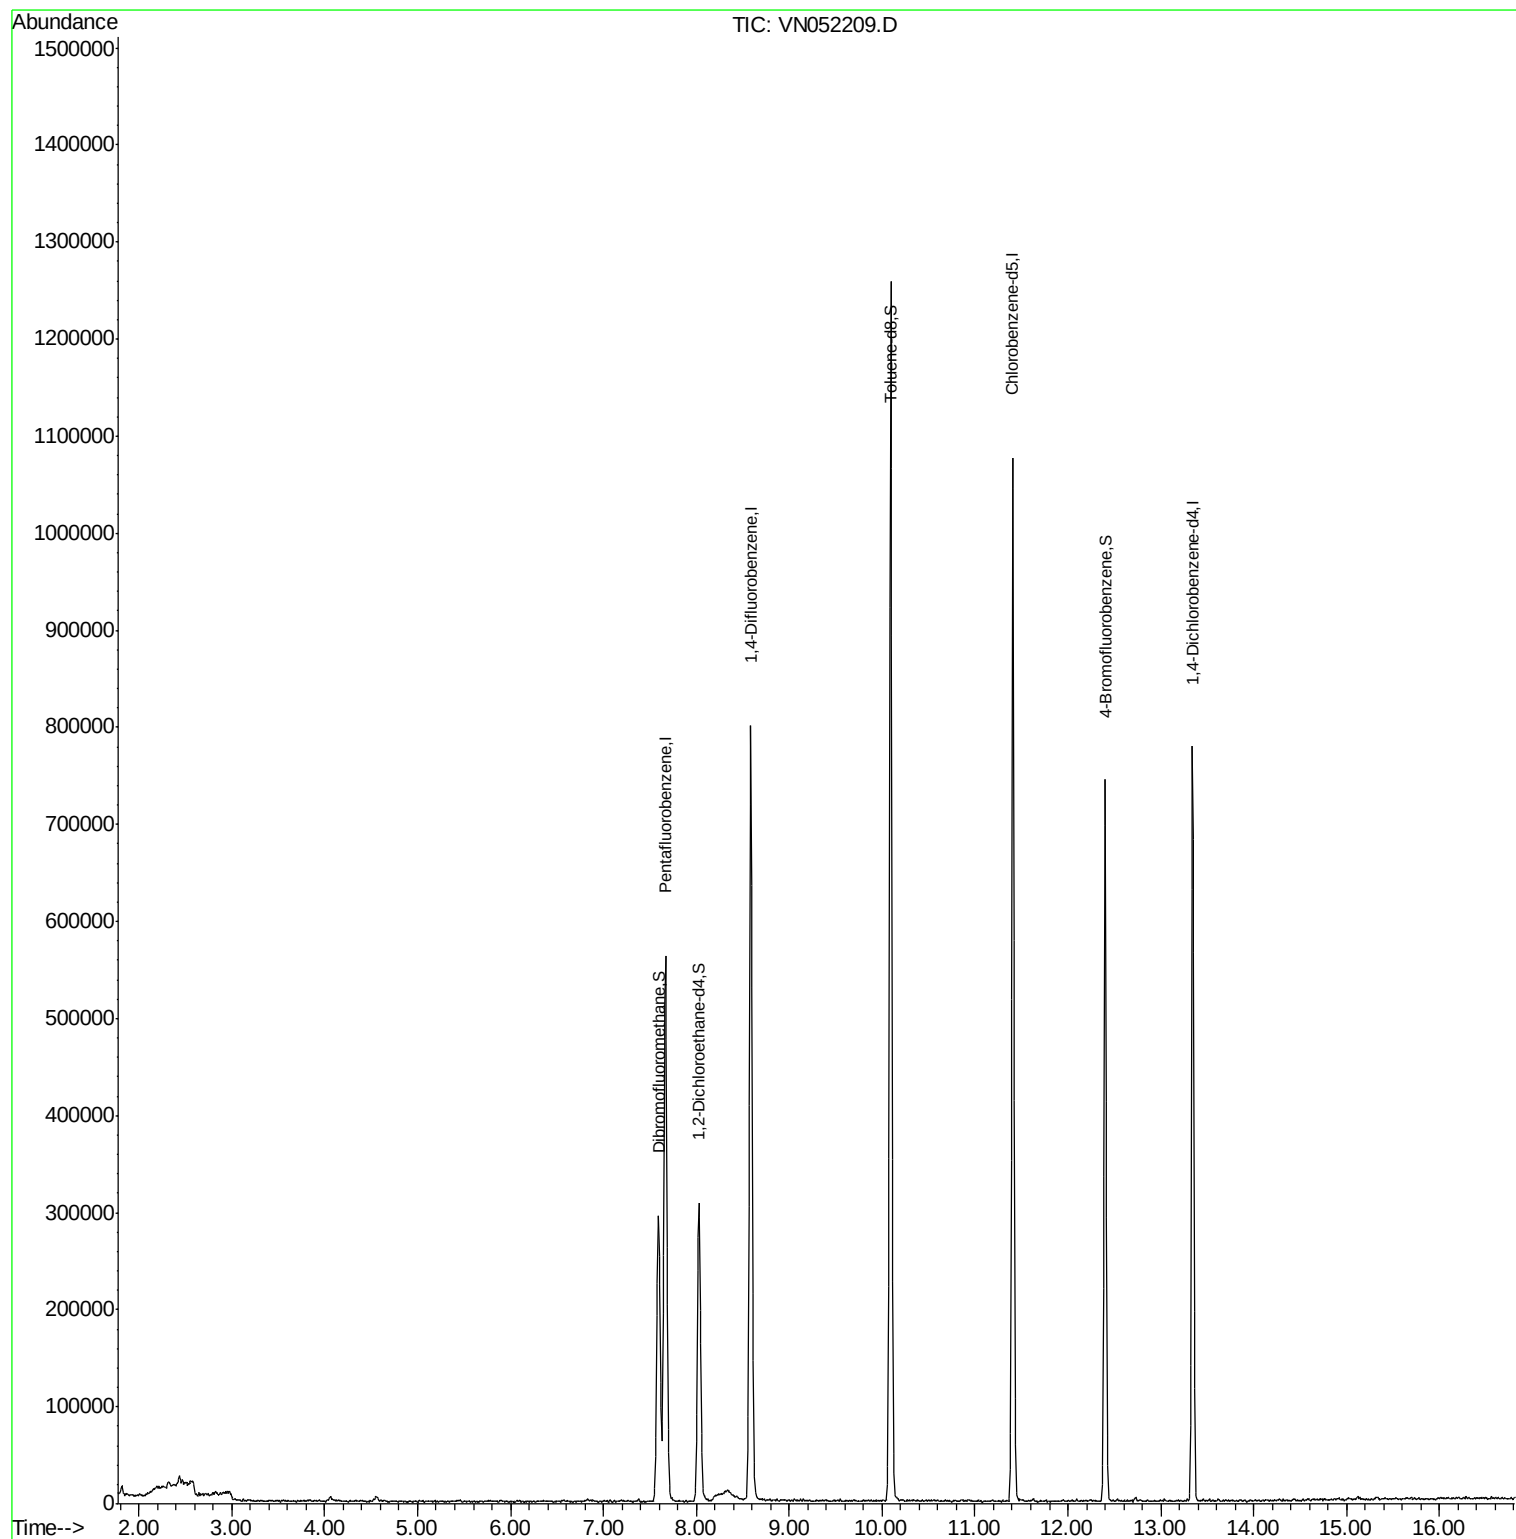

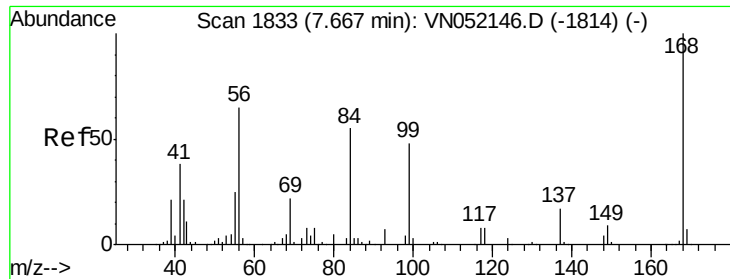

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1834

Delta R.T. 0.00 min

Lab File: VN052209.D

Acq: 7 Nov 2018 16:05

Instrument :

MSVOA_N

ClientSampled :


MH-C

Tot Ion:168 Resp: 434996

Ion Ratio Lower Upper

168 100

99 57.9 45.4 68.2

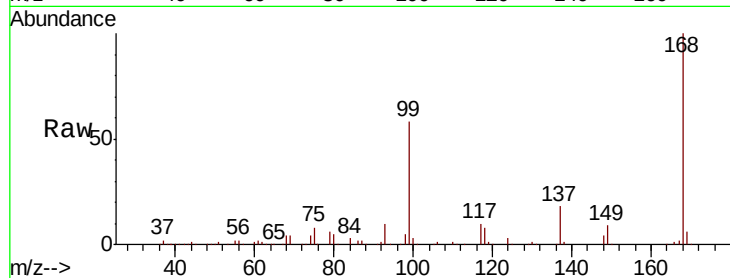

Abundance Ion 167.90 (167.60 to 168.60): VN052209.D (-1740) (-)

Ion 98.90 (98.60 to 99.60): VN052209.D (-1740) (-)

7.67

200000



150000

100000

50000

0

Time-->

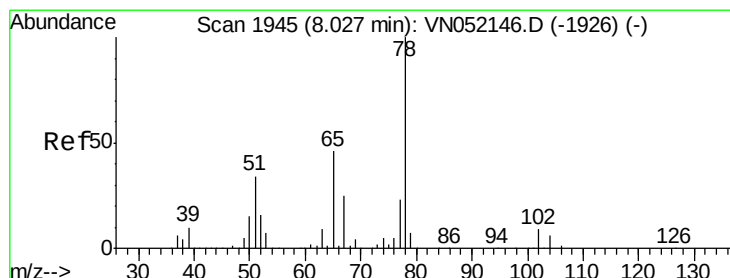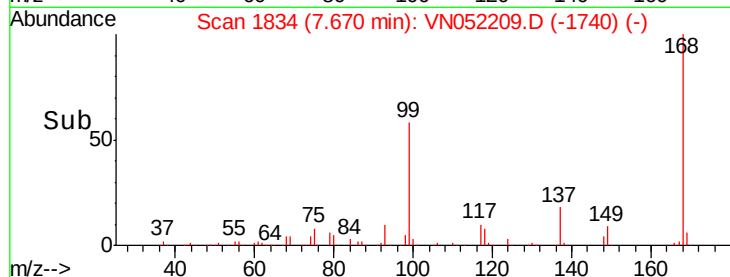

#33

1,2-Dichloroethane-d4

Concen: Below ug/l

RT: 8.03 min Scan# 1945

Delta R.T. 0.00 min

Lab File: VN052209.D


Acq: 7 Nov 2018 16:05

Tgt Ion: 65 Resp: 252838

Ion Ratio Lower Upper

65 100

67 53.8 0.0 107.6

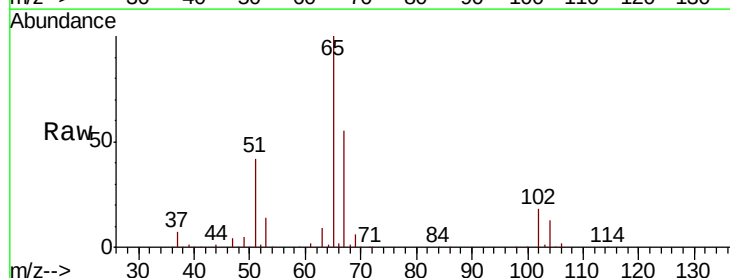

Abundance Ion 64.90 (64.60 to 65.60): VN052209.D (-1852) (-)

Ion 66.90 (66.60 to 67.60): VN052209.D (-1852) (-)

8.03

120000

100000

80000


60000


40000

20000

0

Time-->




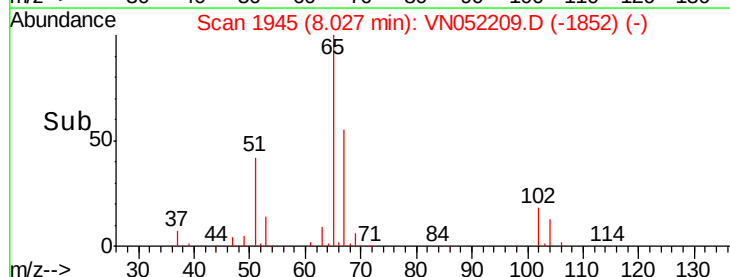


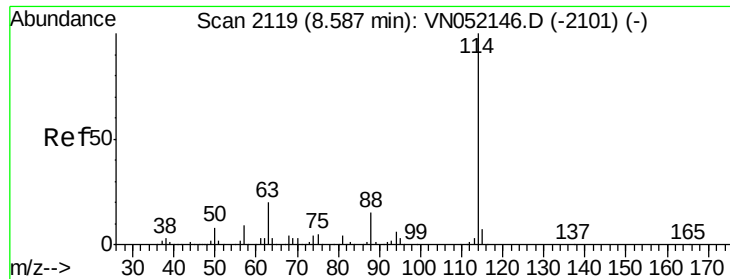

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN052209.D
 Acq: 7 Nov 2018 16:05




Instrument :
 MSVOA_N
 ClientSampleId :
 MH-C


Tot Ion:114 Resp: 713993
 Ion Ratio Lower Upper
 114 100
 63 21.4 0.0 40.0
 88 15.3 0.0 31.0

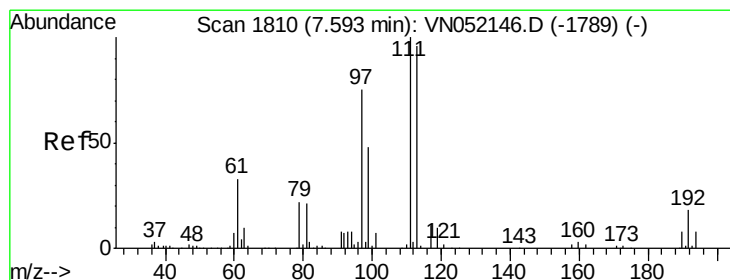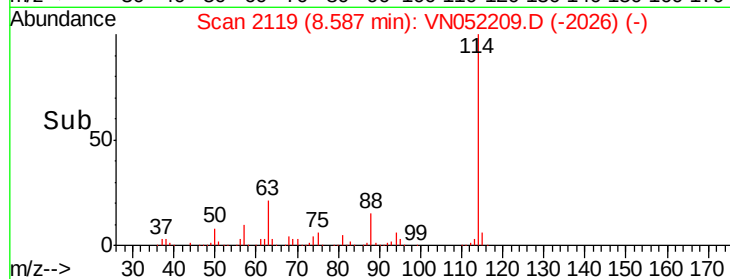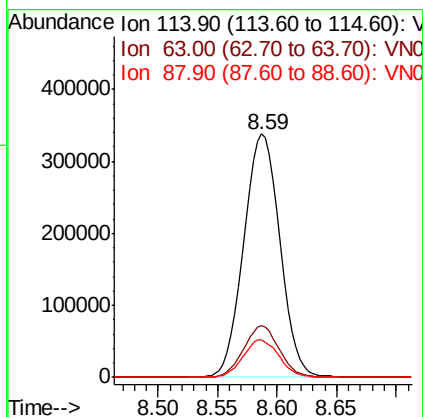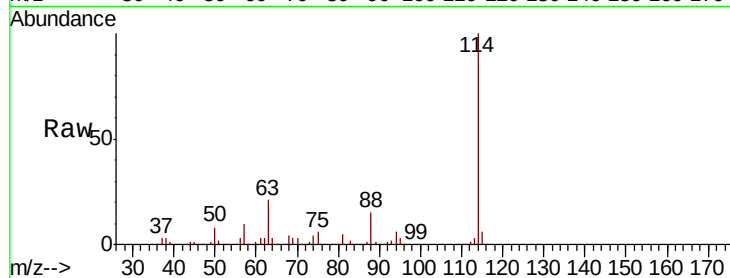

#35
 Dibromofluoromethane
 Concen: 50.000 ug/l
 RT: 7.59 min Scan# 1810
 Delta R.T. 0.00 min
 Lab File: VN052209.D
 Acq: 7 Nov 2018 16:05

Tgt Ion:113 Resp: 226183
 Ion Ratio Lower Upper
 113 100
 111 102.8 81.7 122.5
 192 17.8 14.2 21.4

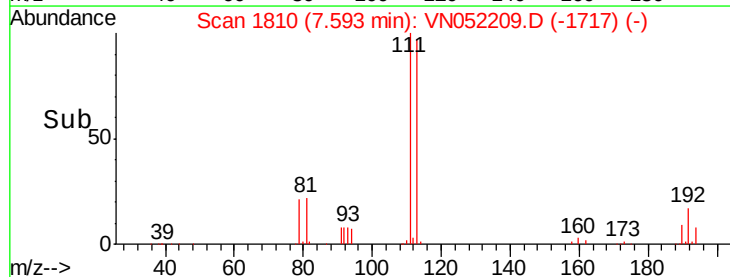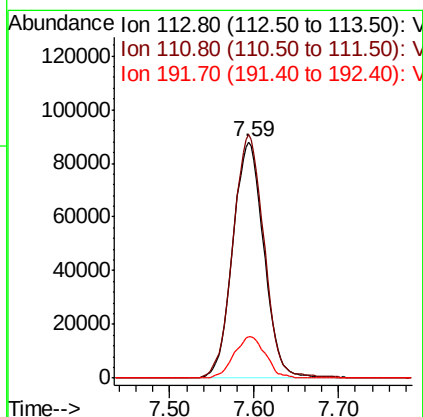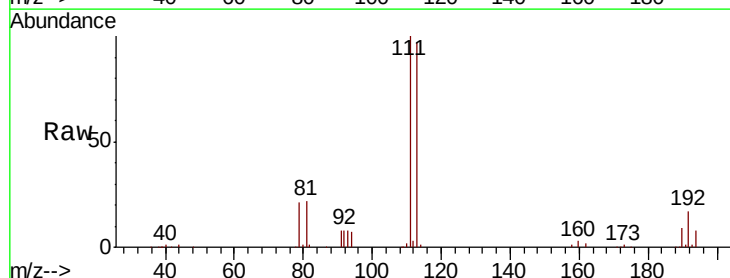

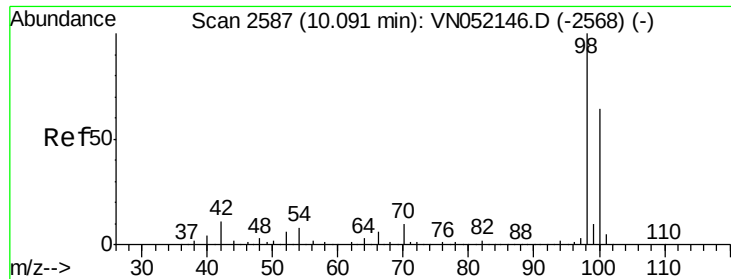

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.09 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN052209.D

Acq: 7 Nov 2018 16:05

Instrument :

MSVOA_N

ClientSampled :


MH-C

Tot Ion: 98 Resp: 863989

Ion Ratio Lower Upper




98 100

100 63.5 50.5 75.7

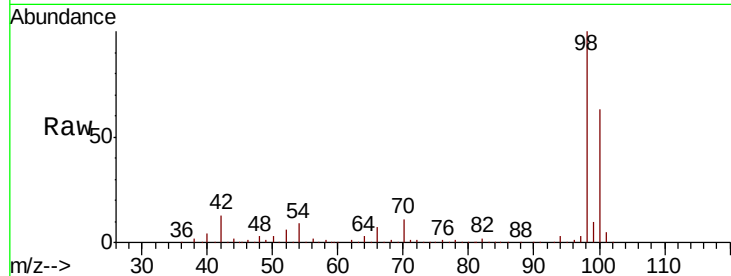

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN

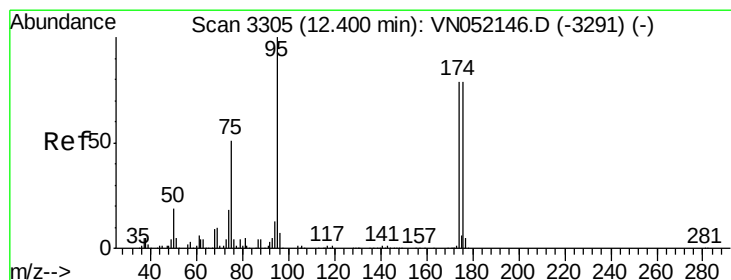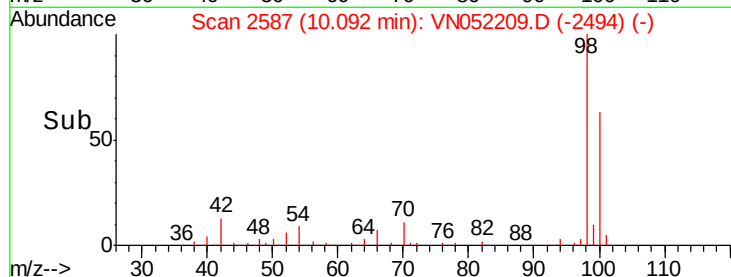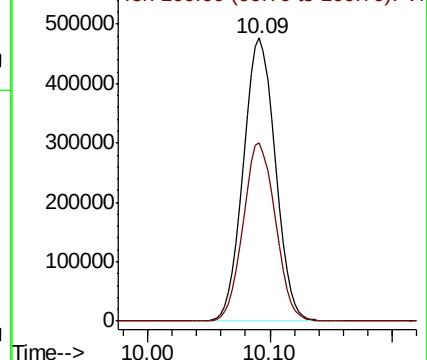

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.40 min Scan# 3305

Delta R.T. 0.00 min

Lab File: VN052209.D

Acq: 7 Nov 2018 16:05


Tgt Ion: 95 Resp: 248584

Ion Ratio Lower Upper

95 100

174 78.5 0.0 162.6



176 75.8 0.0 155.4

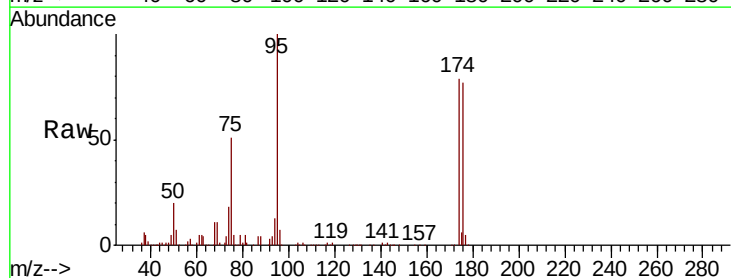


Abundance Ion 94.90 (94.60 to 95.60): VN0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V



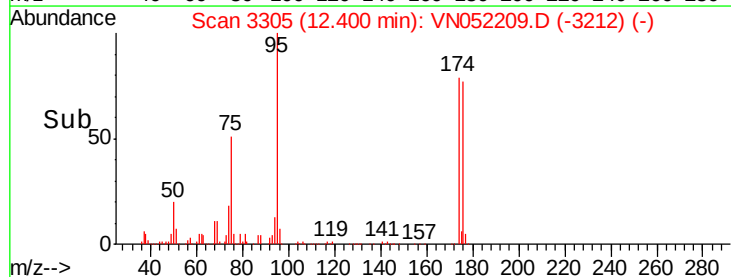
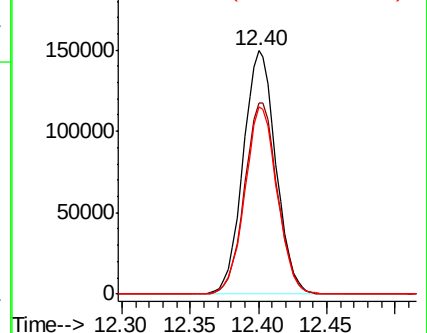


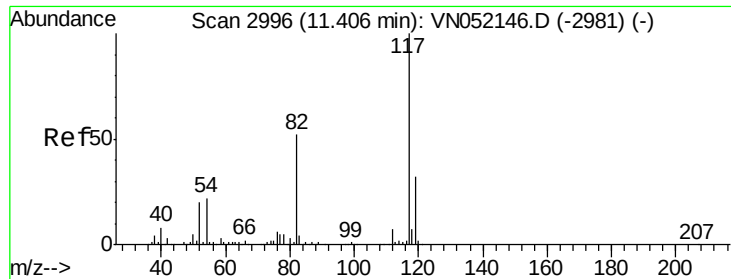

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. 0.00 min
Lab File: VN052209.D
Acq: 7 Nov 2018 16:05

Instrument :
MSVOA_N
ClientSampled :
MH-C

Tot Ion	Ratio	Lower	Upper
117	100		
82	55.3	41.9	62.9
119	32.5	25.7	38.5

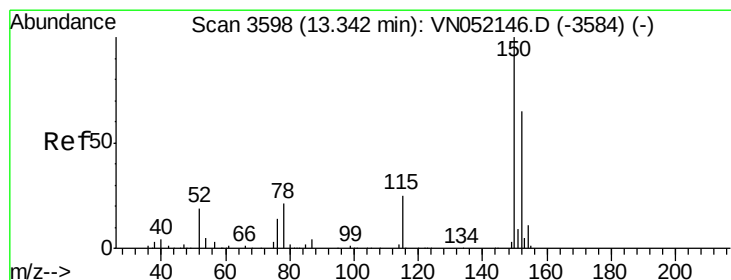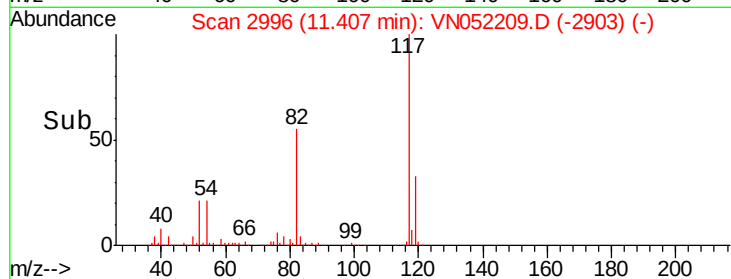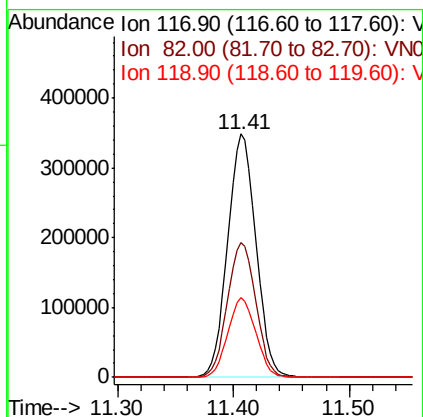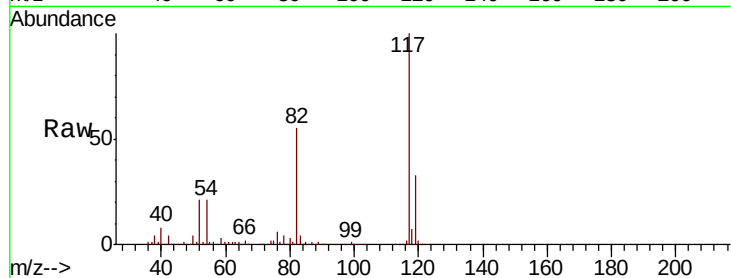

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. 0.00 min
Lab File: VN052209.D
Acq: 7 Nov 2018 16:05

Tgt Ion	Ratio	Lower	Upper
152	100		
115	60.1	28.5	85.5
150	155.3	0.0	348.6

