


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN110718\
 Data File : VN052195.D
 Acq On : 7 Nov 2018 8:22
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110518W.M
 Title : SW846 8260
 Last Update : Mon Nov 05 22:32:25 2018

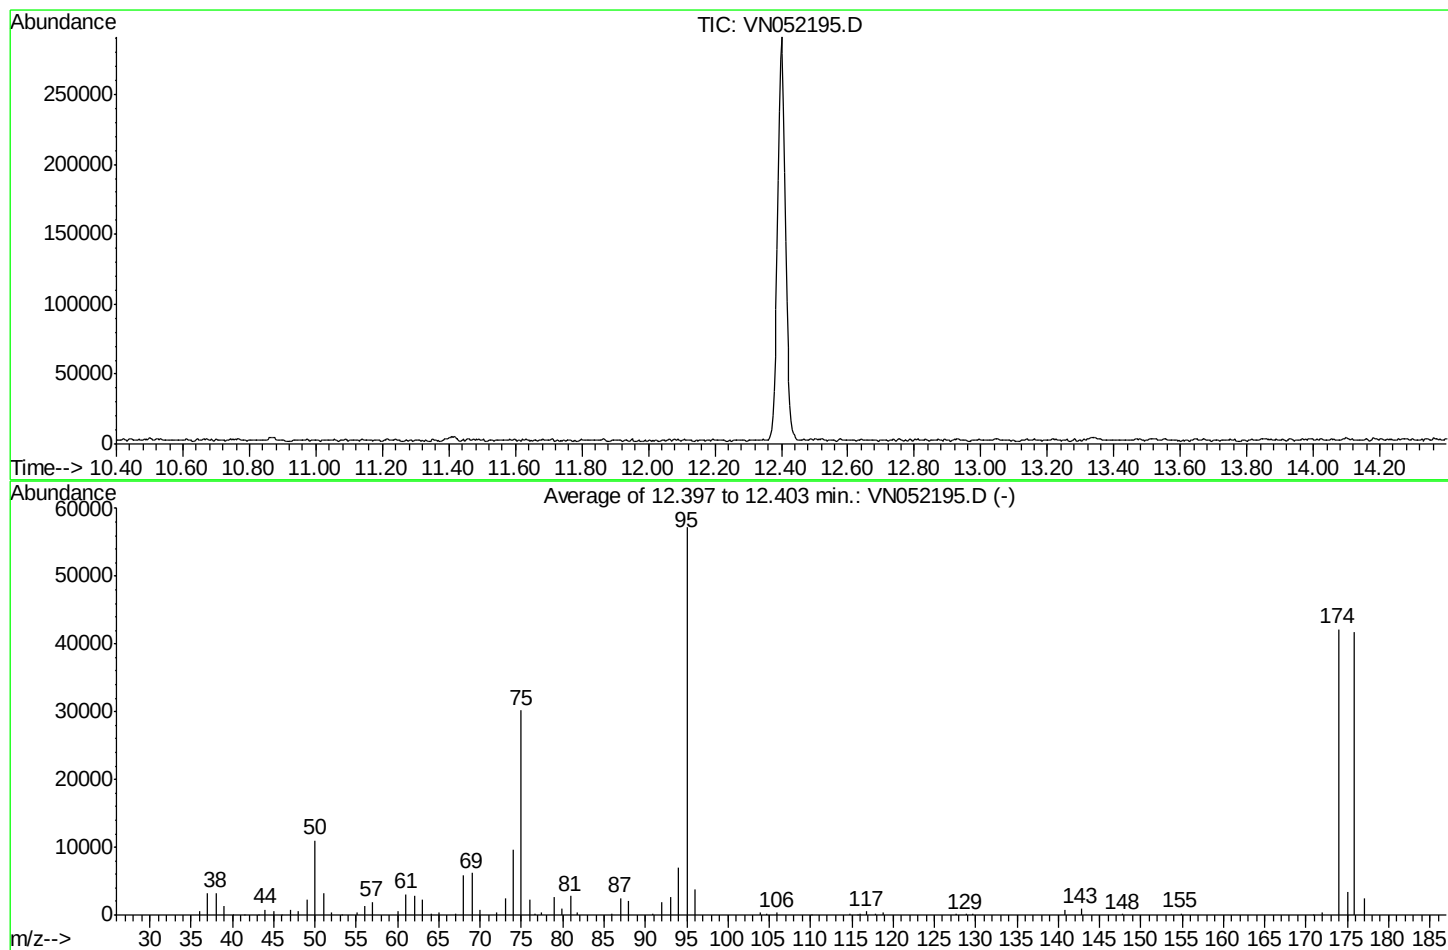

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	11053	PASS
75	95	30	60	52.8	30192	PASS
95	95	100	100	100.0	57224	PASS
96	95	5	9	6.6	3765	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.7	42194	PASS
175	174	5	9	8.2	3470	PASS
176	174	95	101	99.1	41818	PASS
177	176	5	9	6.0	2513	PASS