

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110722\
 Data File : VN075188.D
 Acq On : 07 Nov 2022 15:21
 Operator : JC\MD
 Sample : PB148848TB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB148848TB

Quant Time: Nov 08 01:10:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 09:48:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.229	168	95522	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	191723	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.864	117	175912	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	70505	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	75614	58.750	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 117.500%			
35) Dibromofluoromethane	8.171	113	61210	54.384	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 108.760%			
50) Toluene-d8	10.570	98	229695	52.602	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 105.200%			
62) 4-Bromofluorobenzene	12.853	95	74515	48.578	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 97.160%			
Target Compounds						Qvalue
5) Bromomethane	2.924	94	433	Below Cal		84
6) Chloroethane	3.089	64	631	0.467 ug/l #		45
11) Tert butyl alcohol	5.518	59	2145	7.147 ug/l #		72
16) Acetone	4.447	43	9605	17.625 ug/l		97
18) Methyl Acetate	5.041	43	957	0.538 ug/l #		56
20) Methylene Chloride	5.283	84	13026	10.720 ug/l #		93
25) 2-Butanone	7.494	43	2622	3.059 ug/l		92
29) Tetrahydrofuran	7.853	42	160	0.289 ug/l #		52
31) Cyclohexane	8.235	56	2315	1.209 ug/l #		10
36) 1,1-Dichloropropene	8.229	75	8580	4.924 ug/l #		48
37) Ethyl Acetate	7.577	43	18545	9.705 ug/l #		89
38) Carbon Tetrachloride	8.229	117	10800	5.635 ug/l #		17
42) 1,2-Dichloroethane	8.682	62	544	0.280 ug/l #		75
43) Isopropyl Acetate	8.694	43	80075	27.015 ug/l #		89
45) 1,2-Dichloropropane	9.741	63	992	0.781 ug/l #		42
48) Methyl methacrylate	9.665	41	2268	1.668 ug/l #		35
51) 4-Methyl-2-Pentanone	10.453	43	5823	3.044 ug/l #		72
53) t-1,3-Dichloropropene	10.723	75	628	0.311 ug/l		95
54) cis-1,3-Dichloropropene	10.359	75	29214	13.622 ug/l #		65
56) Ethyl methacrylate	10.994	69	914	0.424 ug/l #		1
57) 1,3-Dichloropropane	11.206	76	4346	1.845 ug/l #		42
59) 2-Hexanone	11.176	43	60267	41.514 ug/l #		21
71) Bromoform	12.853	173	551	0.528 ug/l #		1
74) N-amyl acetate	12.494	43	568	0.271 ug/l #		46
76) 1,2,3-Trichloropropane	12.853	75	40826	27.272 ug/l #		1
81) trans-1,4-Dichloro-2-b...	12.853	75	40826	70.006 ug/l #		10
93) 1,2,4-Trichlorobenzene	15.394	180	361	0.346 ug/l #		80
95) Naphthalene	15.641	128	3279	0.817 ug/l #		87
96) 1,2,3-Trichlorobenzene	15.835	180	595	0.574 ug/l #		80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110722\
Data File : VN075188.D
Acq On : 07 Nov 2022 15:21
Operator : JC\MD
Sample : PB148848TB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB148848TB

Quant Time: Nov 08 01:10:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 09:48:49 2022
Response via : Initial Calibration




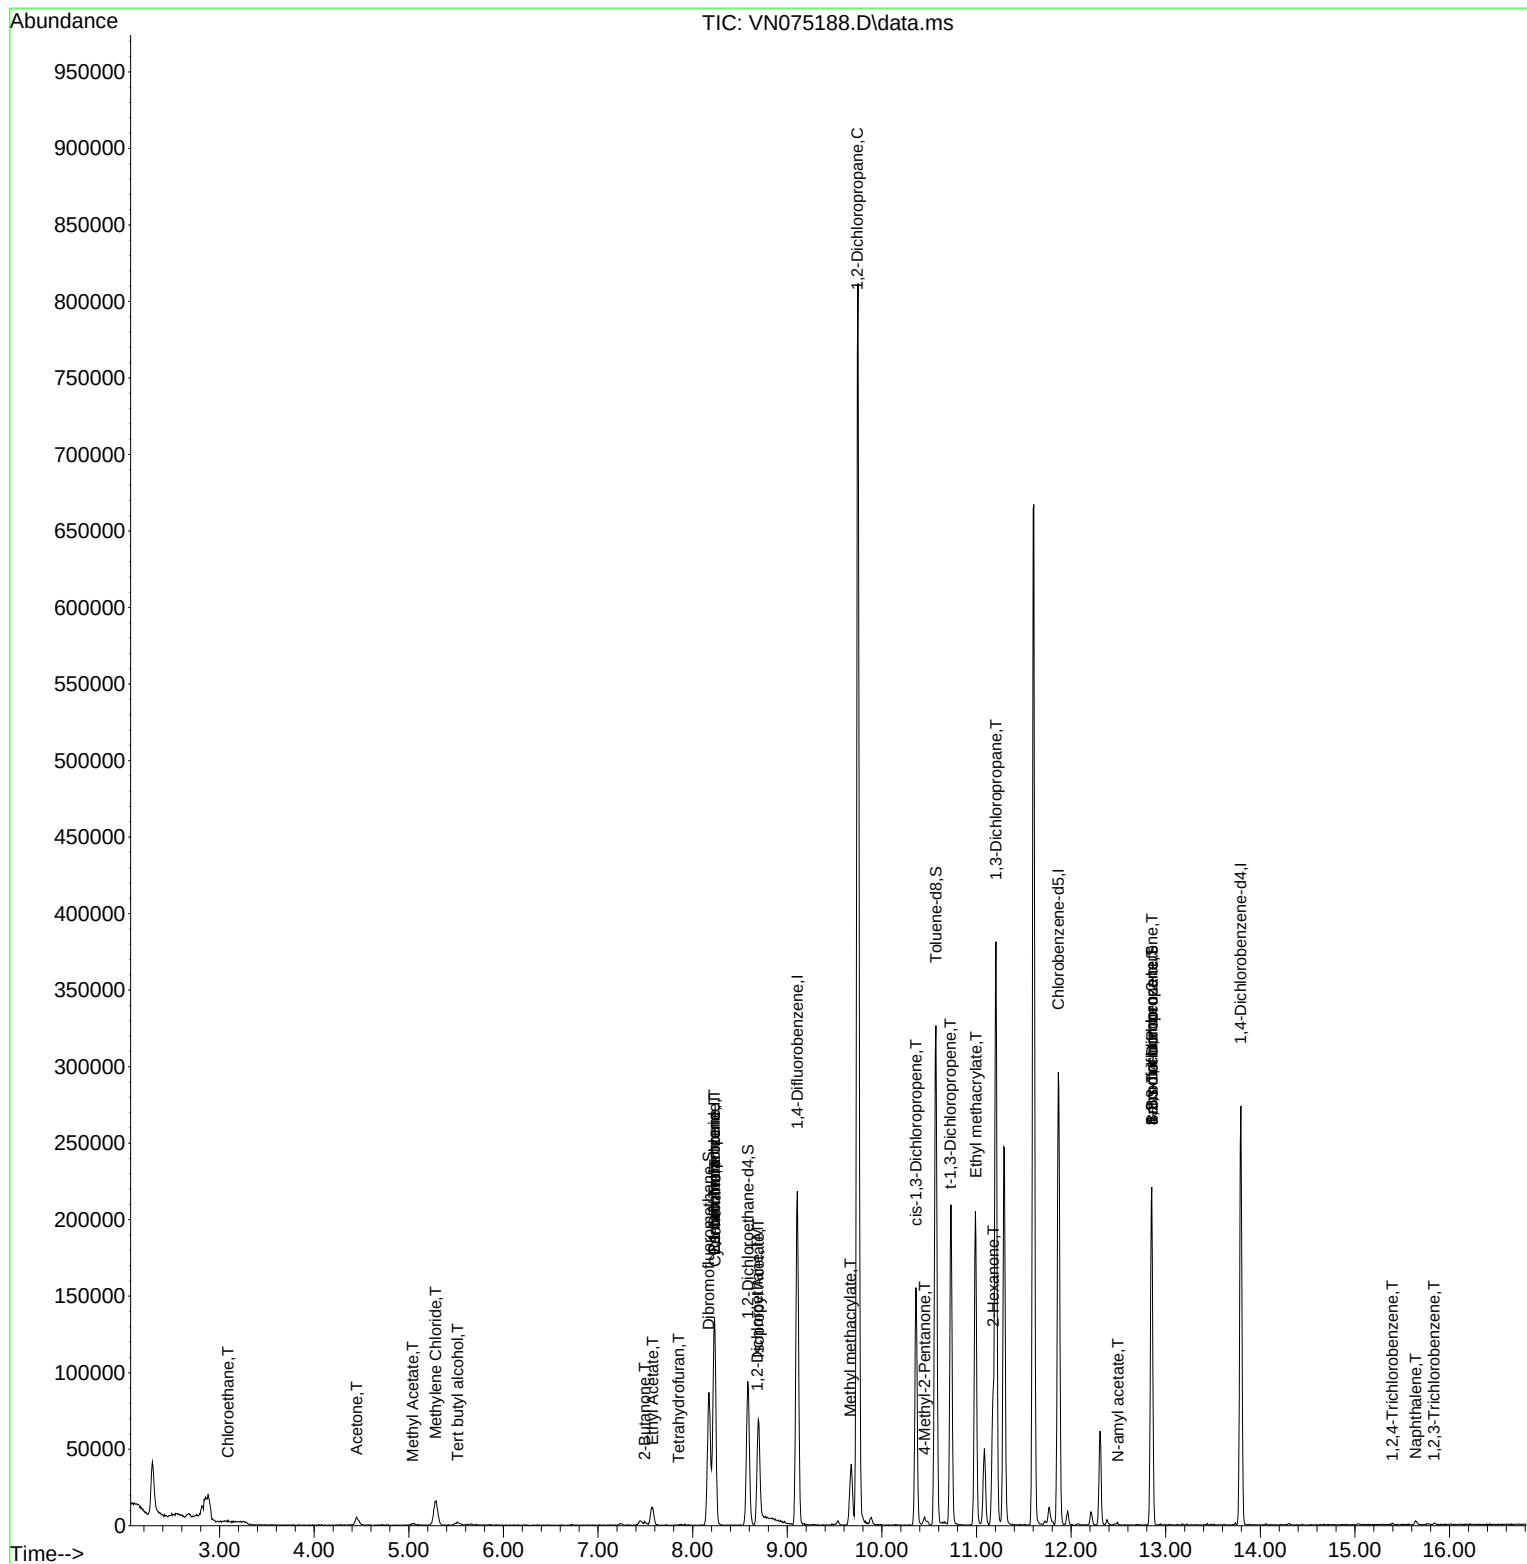


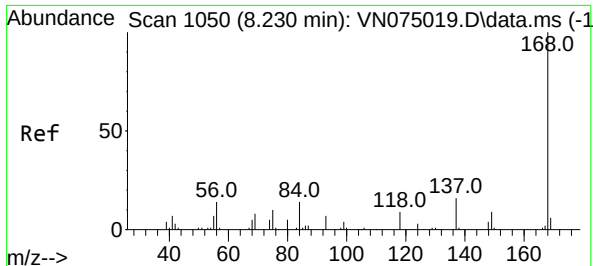

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 10
Delta R.T. -0.001 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21




Instrument :
MSVOA_N
ClientSampleId :
PB148848TB


Tgt Ion:168 Resp: 95522
Ion Ratio Lower Upper
168 100
99 64.6 51.6 77.4

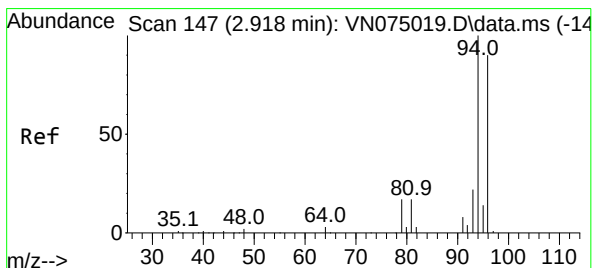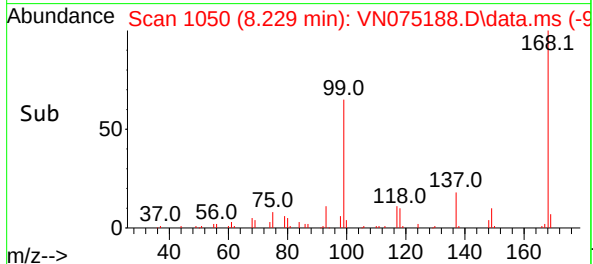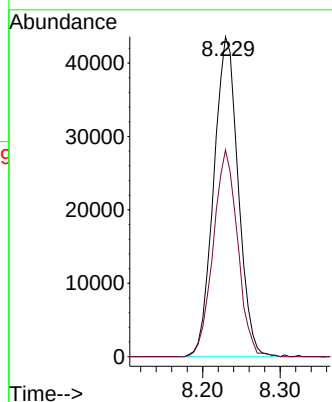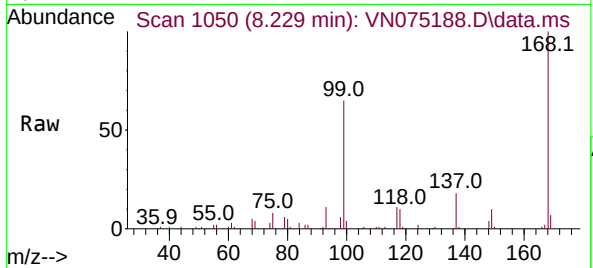

#5
Bromomethane
Concen: Below Cal
RT: 2.924 min Scan# 148
Delta R.T. 0.006 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21

Tgt Ion: 94 Resp: 433
Ion Ratio Lower Upper
94 100
96 74.7 71.8 107.6


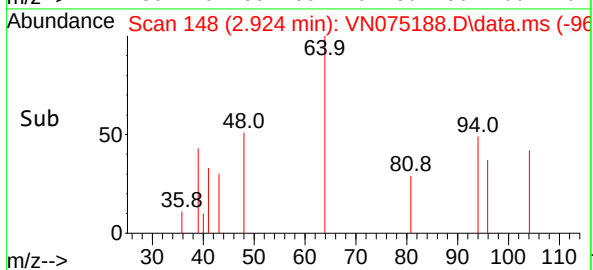
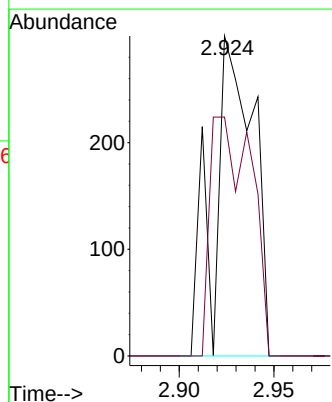
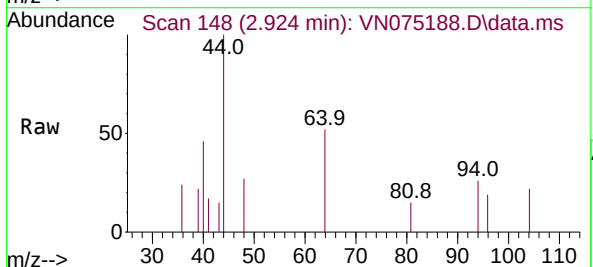




#6
Chloroethane
Concen: 0.467 ug/l
RT: 3.089 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21




Instrument :
MSVOA_N
ClientSampleId :
PB148848TB


Tgt Ion: 64 Resp: 631
Ion Ratio Lower Upper
64 100
66 0.0 23.8 35.8#



#11
Tert butyl alcohol
Concen: 7.147 ug/l
RT: 5.518 min Scan# 589
Delta R.T. -0.024 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21

Tgt Ion: 59 Resp: 2145
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#









#16
Acetone
Concen: 17.625 ug/l
RT: 4.447 min Scan# 406
Delta R.T. 0.005 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21




Instrument :
MSVOA_N
ClientSampleId :
PB148848TB


Tgt Ion: 43 Resp: 9605
Ion Ratio Lower Upper
43 100
58 30.1 25.5 38.3

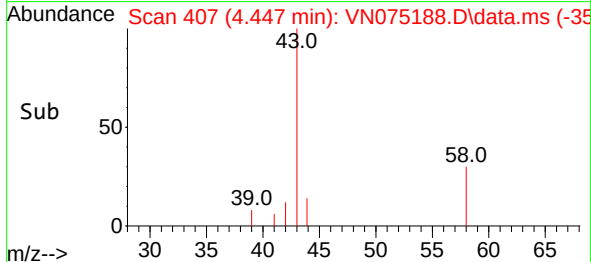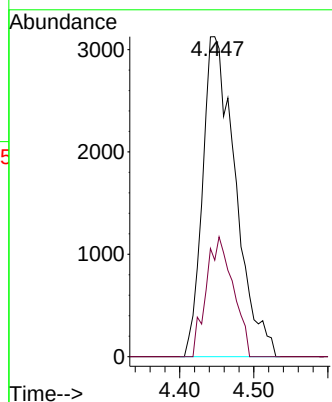

#18
Methyl Acetate
Concen: 0.538 ug/l
RT: 5.041 min Scan# 508
Delta R.T. -0.001 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21

Tgt Ion: 43 Resp: 957
Ion Ratio Lower Upper
43 100
74 50.4 22.0 33.0#


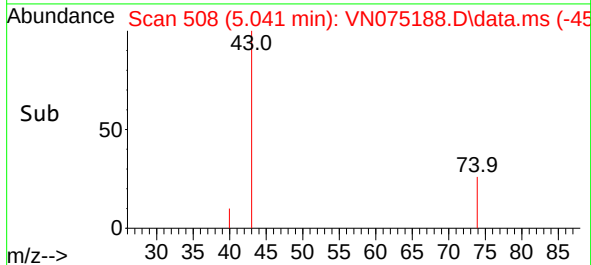
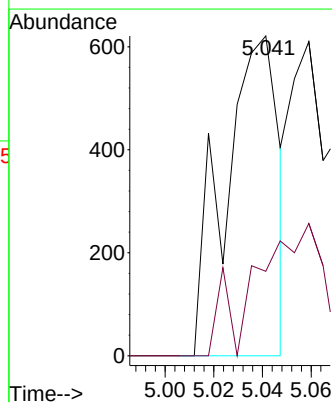
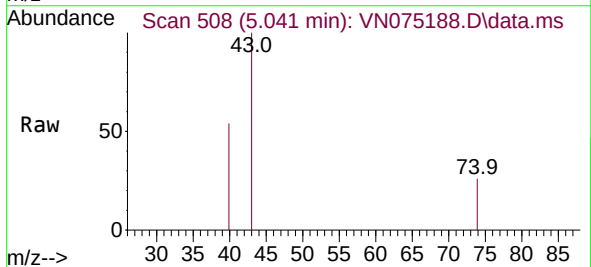




#20
Methylene Chloride
Concen: 10.720 ug/l
RT: 5.283 min Scan# 549
Delta R.T. -0.000 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21




Instrument :
MSVOA_N
ClientSampleId :
PB148848TB


Tgt Ion:	84	Resp:	13026
Ion	Ratio	Lower	Upper
84	100		
49	122.4	94.9	142.3
51	34.8	26.8	40.2
86	53.6	53.7	80.5



#25
2-Butanone
Concen: 3.059 ug/l
RT: 7.494 min Scan# 925
Delta R.T. 0.000 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21

Tgt Ion:	43	Resp:	2622
Ion	Ratio	Lower	Upper
43	100		
72	27.7	25.5	38.3

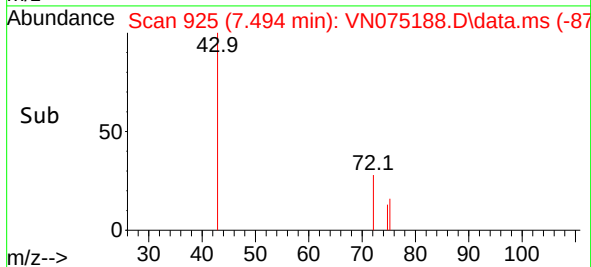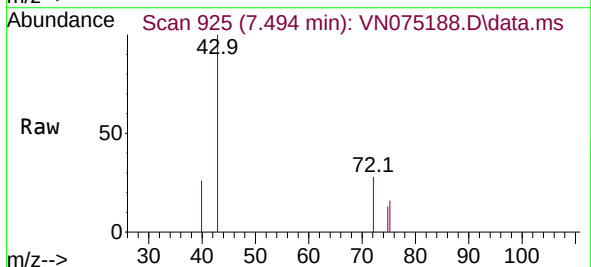



#29

Tetrahydrofuran

Concen: 0.289 ug/l

RT: 7.853 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN075188.D

Acq: 07 Nov 2022 15:21

Instrument :

MSVOA_N

ClientSampleId :

PB148848TB





Tgt Ion: 42 Resp: 160

Ion Ratio Lower Upper

42 100

72 0.0 43.0 64.6#

71 36.9 39.9 59.9#

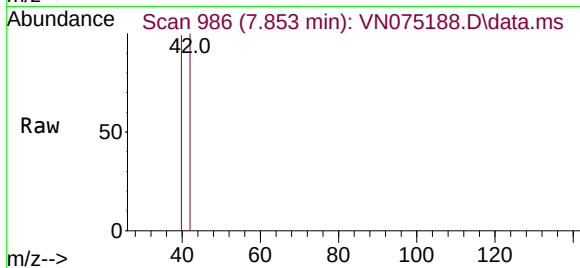

#31

Cyclohexane

Concen: 1.209 ug/l

RT: 8.235 min Scan# 1051

Delta R.T. -0.024 min

Lab File: VN075188.D

Acq: 07 Nov 2022 15:21




Tgt Ion: 56 Resp: 2315


Ion Ratio Lower Upper

56 100

69 153.6 25.2 37.8#

84 144.0 77.8 116.8#

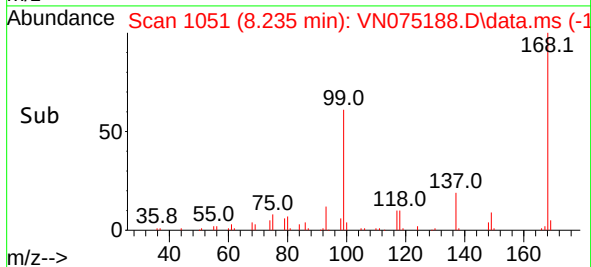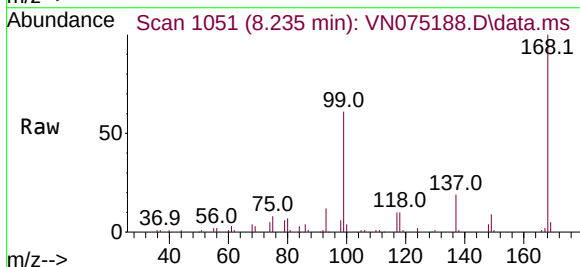

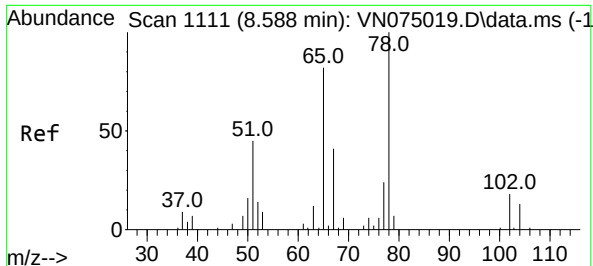

#33

1,2-Dichloroethane-d4

Concen: 58.750 ug/l

RT: 8.582 min Scan# 1111

Delta R.T. -0.006 min

Lab File: VN075188.D

Acq: 07 Nov 2022 15:21

Instrument :

MSVOA_N

ClientSampleId :





PB148848TB

Tgt Ion: 65 Resp: 75614

Ion Ratio Lower Upper

65 100

67 53.1 0.0 102.0

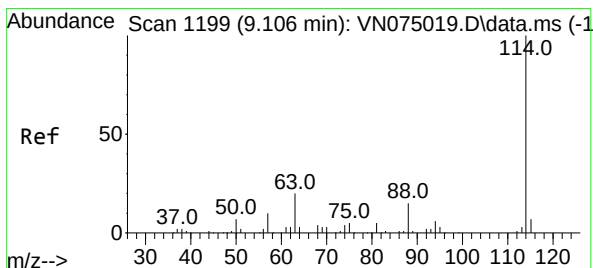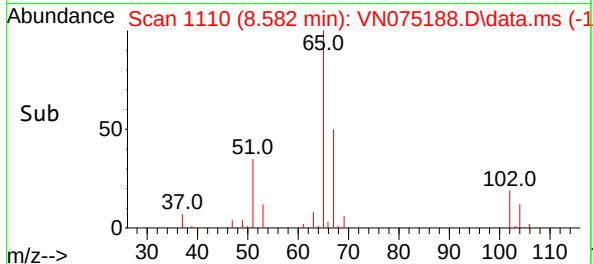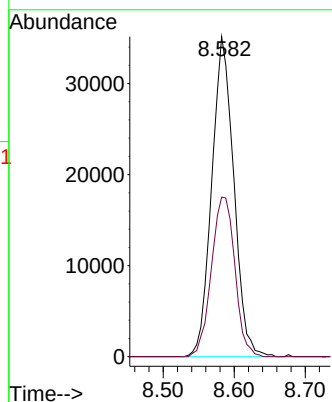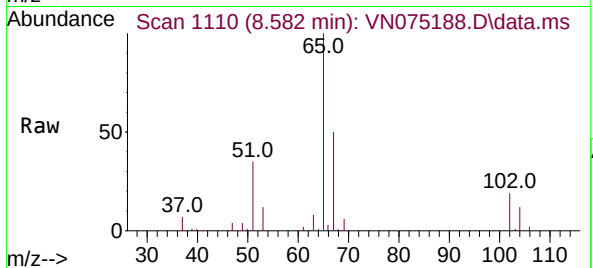

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. -0.000 min

Lab File: VN075188.D

Acq: 07 Nov 2022 15:21




Tgt Ion: 114 Resp: 191723


Ion Ratio Lower Upper

114 100

63 19.4 0.0 39.6

88 14.3 0.0 29.0


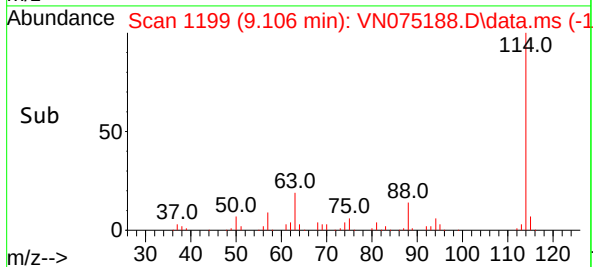

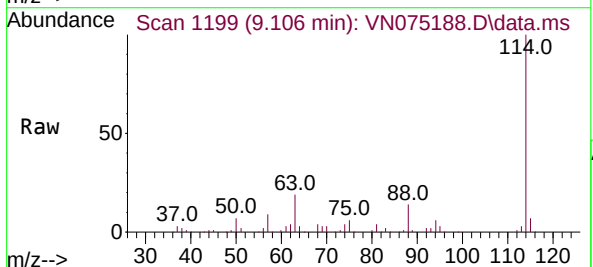


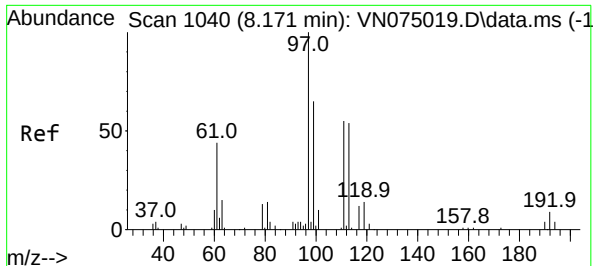

#35
Dibromofluoromethane
Concen: 54.384 ug/l
RT: 8.171 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21




Instrument :
MSVOA_N
ClientSampleId :
PB148848TB


Tgt Ion:113 Resp: 61210
Ion Ratio Lower Upper
113 100
111 101.8 80.5 120.7
192 15.8 13.2 19.8

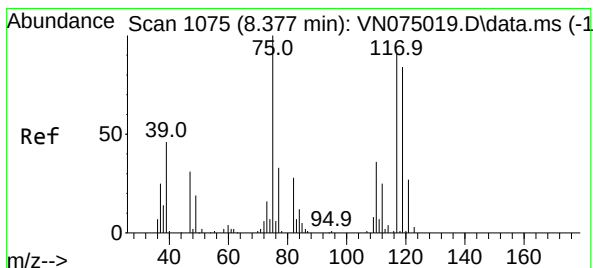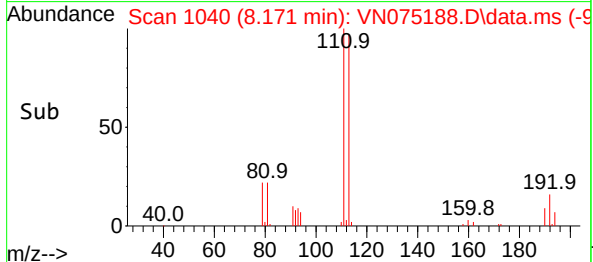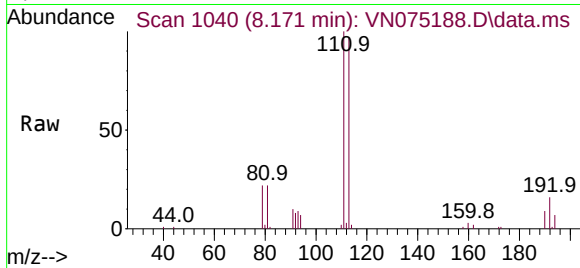

#36
1,1-Dichloropropene
Concen: 4.924 ug/l
RT: 8.229 min Scan# 1050
Delta R.T. -0.148 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21

Tgt Ion: 75 Resp: 8580
Ion Ratio Lower Upper
75 100
110 7.6 17.8 53.3#
77 0.0 24.6 37.0#

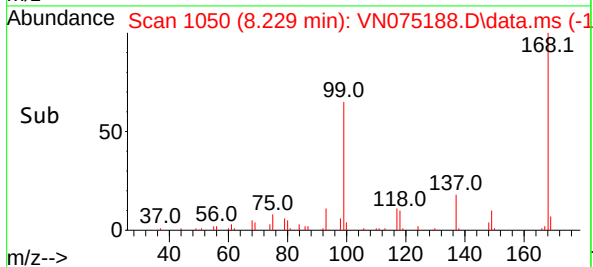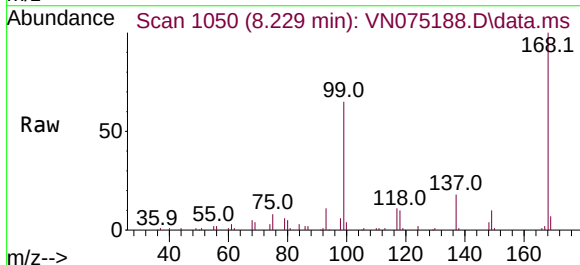



#37

Ethyl Acetate

Concen: 9.705 ug/l

RT: 7.577 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN075188.D


Acq: 07 Nov 2022 15:21

Instrument :




MSVOA_N

ClientSampleId :

PB148848TB

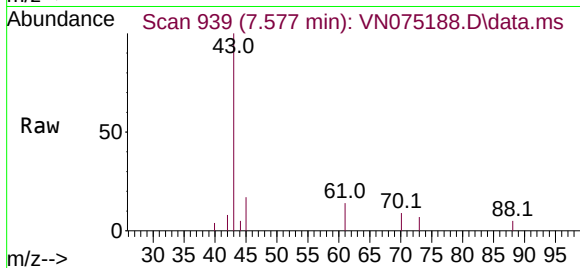

Tgt Ion:	43	Resp:	18545
Ion	Ratio	Lower	Upper
43	100		
61	7.1	12.2	18.4#
70	11.8	9.4	14.2

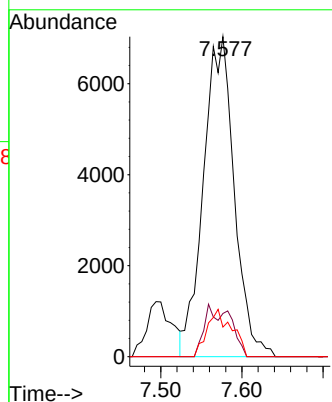

#38

Carbon Tetrachloride

Concen: 5.635 ug/l




RT: 8.229 min Scan# 1050


Delta R.T. -0.142 min

Lab File: VN075188.D

Acq: 07 Nov 2022 15:21

Tgt Ion:	117	Resp:	10800
Ion	Ratio	Lower	Upper
117	100		
119	6.6	76.7	115.1#
121	0.0	23.9	35.9#

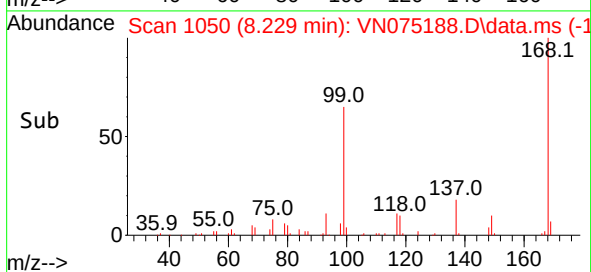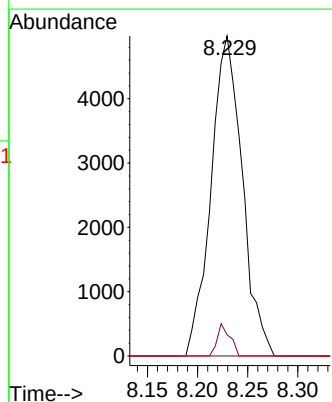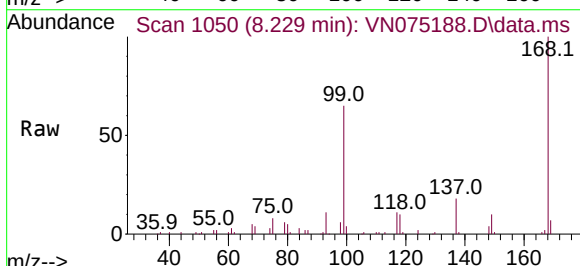

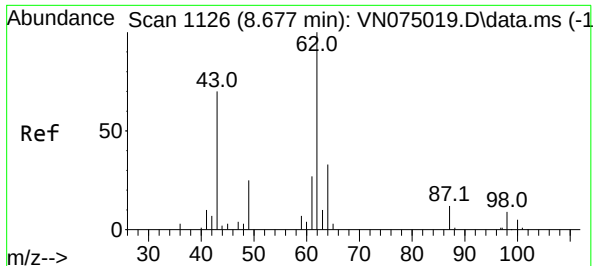

#42

1,2-Dichloroethane

Concen: 0.280 ug/l

RT: 8.682 min Scan# 1127

Delta R.T. 0.005 min

Lab File: VN075188.D

Acq: 07 Nov 2022 15:21

Instrument :

MSVOA_N

ClientSampleId :





PB148848TB

Tgt Ion: 62 Resp: 544

Ion Ratio Lower Upper

62 100

98 0.0 0.0 18.2

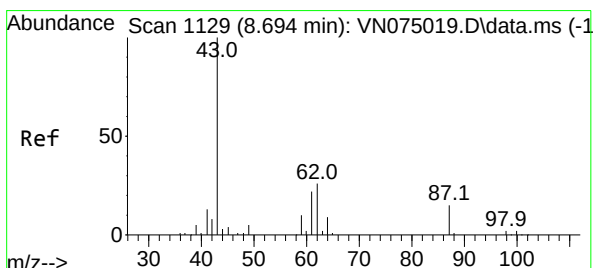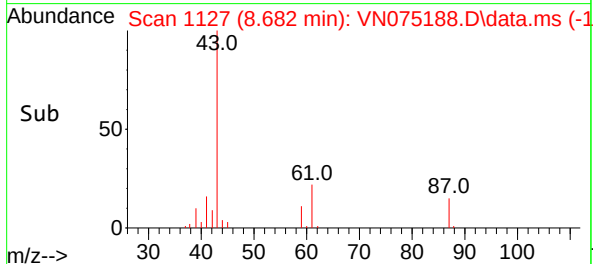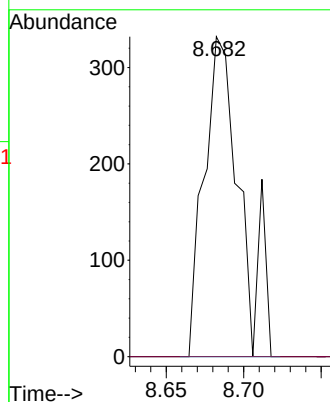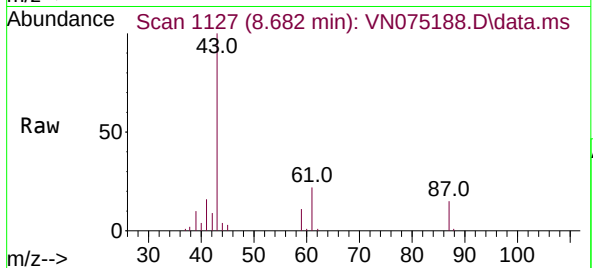

#43

Isopropyl Acetate

Concen: 27.015 ug/l

RT: 8.694 min Scan# 1129

Delta R.T. 0.000 min

Lab File: VN075188.D

Acq: 07 Nov 2022 15:21




Tgt Ion: 43 Resp: 80075


Ion Ratio Lower Upper

43 100

61 19.8 22.4 33.6

87 14.6 12.5 18.7

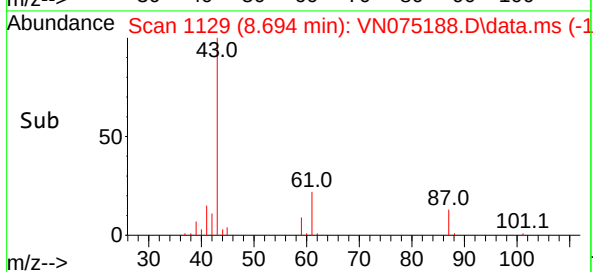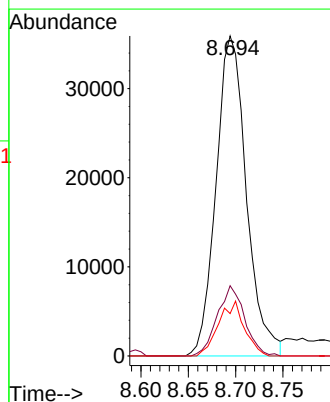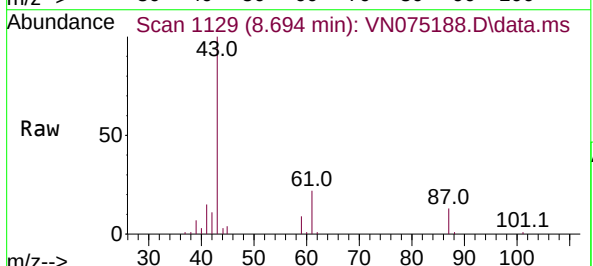

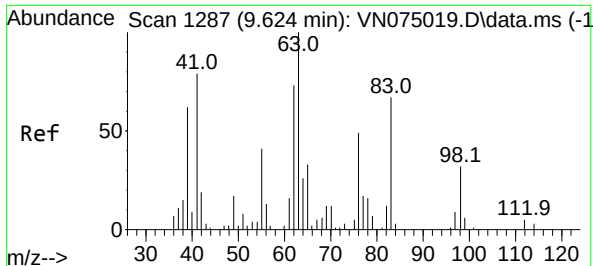

#45

1,2-Dichloropropane

Concen: 0.781 ug/l

RT: 9.741 min Scan# 11

Delta R.T. 0.117 min

Lab File: VN075188.D

Acq: 07 Nov 2022 15:21

Instrument :

MSVOA_N

ClientSampleId :





PB148848TB

Tgt Ion: 63 Resp: 992

Ion Ratio Lower Upper

63 100

65 0.0 26.1 39.1#

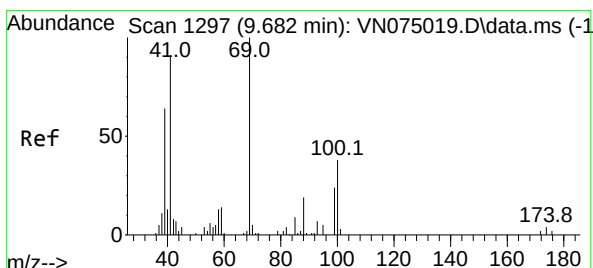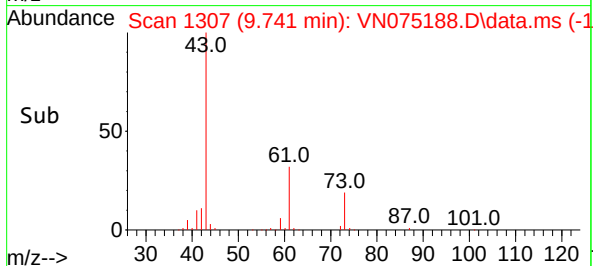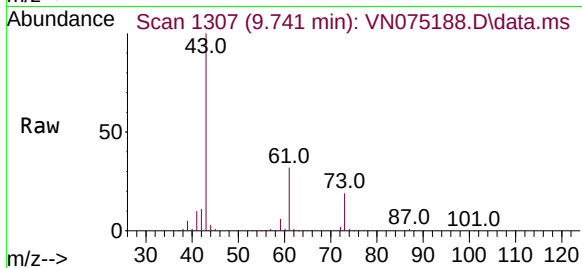

#48

Methyl methacrylate

Concen: 1.668 ug/l

RT: 9.665 min Scan# 1294

Delta R.T. -0.017 min

Lab File: VN075188.D

Acq: 07 Nov 2022 15:21




Tgt Ion: 41 Resp: 2268


Ion Ratio Lower Upper

41 100

69 0.0 80.2 120.2#

39 58.9 56.2 84.2


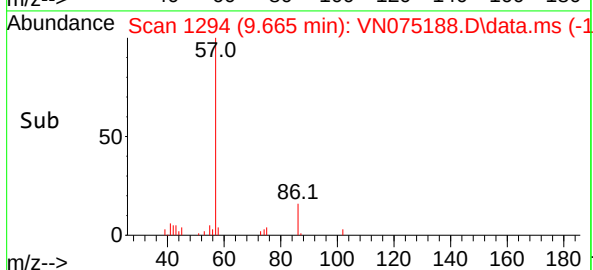

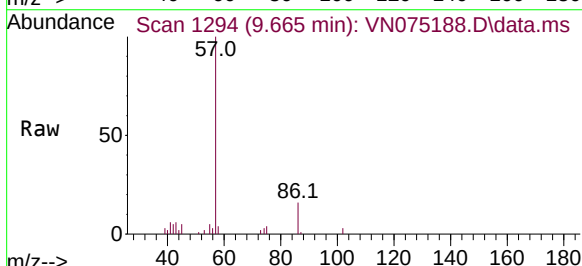




#50
Toluene-d8
Concen: 52.602 ug/l
RT: 10.570 min Scan# 1448
Delta R.T. -0.001 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21




Instrument :
MSVOA_N
ClientSampleId :
PB148848TB


Tgt Ion: 98 Resp: 229695
Ion Ratio Lower Upper
98 100
100 64.6 53.0 79.6

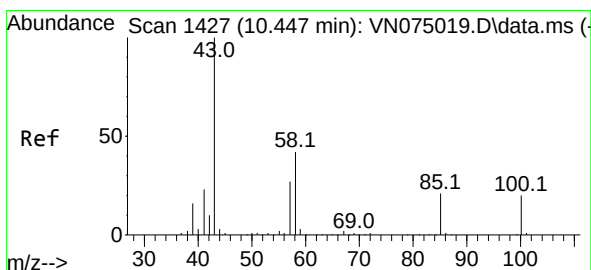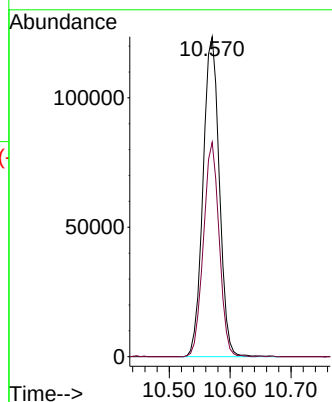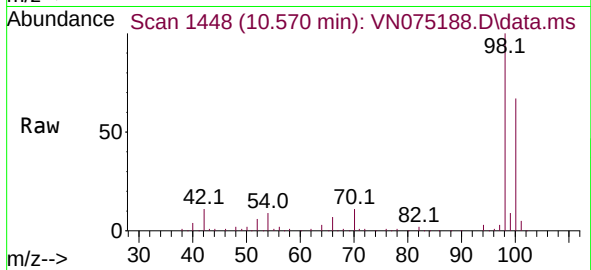

#51
4-Methyl-2-Pentanone
Concen: 3.044 ug/l
RT: 10.453 min Scan# 1428
Delta R.T. 0.006 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21

Tgt Ion: 43 Resp: 5823
Ion Ratio Lower Upper
43 100
58 24.3 33.6 50.4#


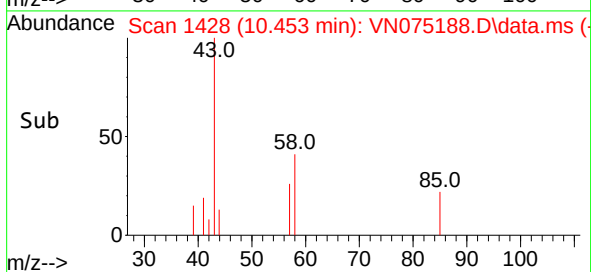
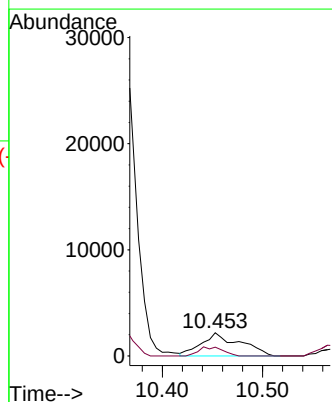
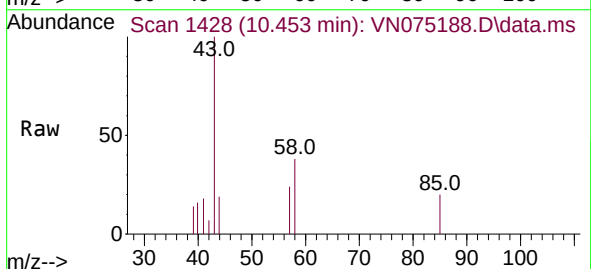




#53
 t-1,3-Dichloropropene
 Concen: 0.311 ug/l
 RT: 10.723 min Scan# 1412
 Delta R.T. -0.118 min
 Lab File: VN075188.D
 Acq: 07 Nov 2022 15:21




Instrument :
 MSVOA_N
 ClientSampleId :
 PB148848TB


Tgt Ion: 75 Resp: 628
 Ion Ratio Lower Upper
 75 100
 77 34.4 25.4 38.2

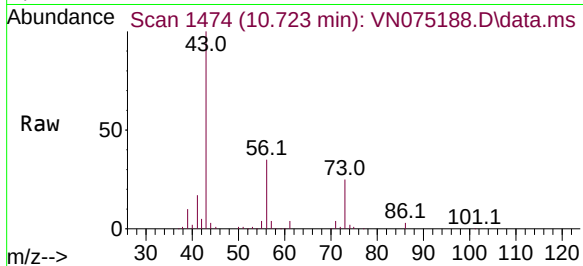

#54
 cis-1,3-Dichloropropene
 Concen: 13.622 ug/l
 RT: 10.359 min Scan# 1412
 Delta R.T. 0.041 min
 Lab File: VN075188.D
 Acq: 07 Nov 2022 15:21

Tgt Ion: 75 Resp: 29214
 Ion Ratio Lower Upper
 75 100
 77 0.0 23.7 35.5#
 39 31.0 35.8 53.6#


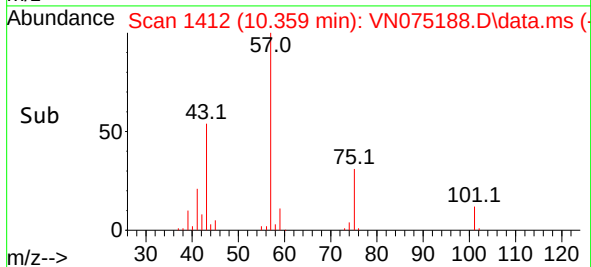

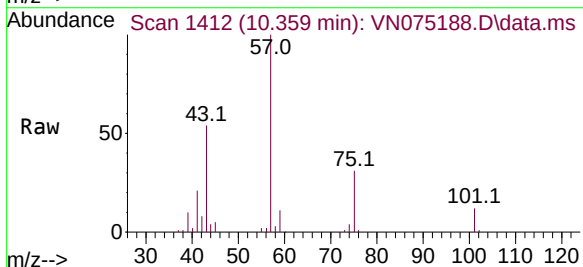




#56
Ethyl methacrylate
Concen: 0.424 ug/l
RT: 10.994 min Scan# 11
Delta R.T. 0.117 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21




Instrument :
MSVOA_N
ClientSampleId :
PB148848TB


Tgt Ion: 69 Resp: 914
Ion Ratio Lower Upper
69 100
41 4191.5 45.6 68.4#
39 1928.7 28.5 42.7#



#57
1,3-Dichloropropane
Concen: 1.845 ug/l
RT: 11.206 min Scan# 1556
Delta R.T. 0.041 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21

Tgt Ion: 76 Resp: 4346
Ion Ratio Lower Upper
76 100
78 0.0 25.8 38.6#


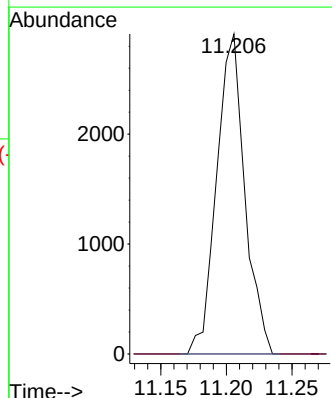

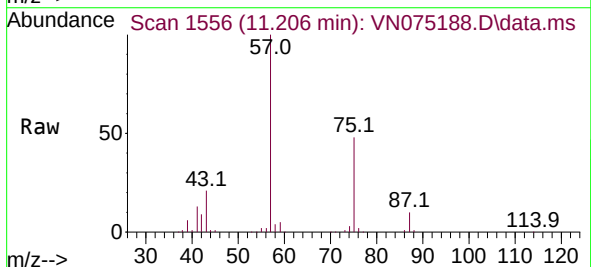




#59
2-Hexanone
Concen: 41.514 ug/l
RT: 11.176 min Scan# 11
Delta R.T. -0.024 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21




Instrument :
MSVOA_N
ClientSampleId :
PB148848TB


Tgt Ion: 43 Resp: 60267
Ion Ratio Lower Upper
43 100
58 0.0 29.6 88.8#

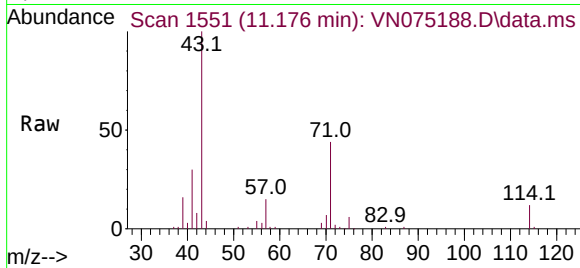

#62
4-Bromofluorobenzene
Concen: 48.578 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21

Tgt Ion: 95 Resp: 74515
Ion Ratio Lower Upper
95 100
174 74.9 0.0 147.4
176 72.7 0.0 142.2


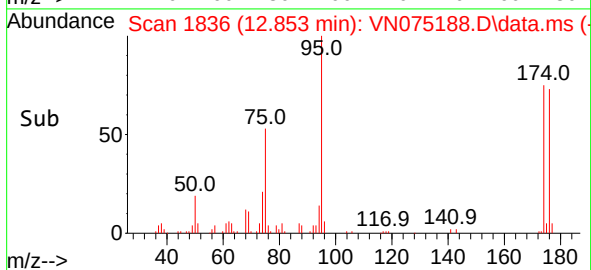

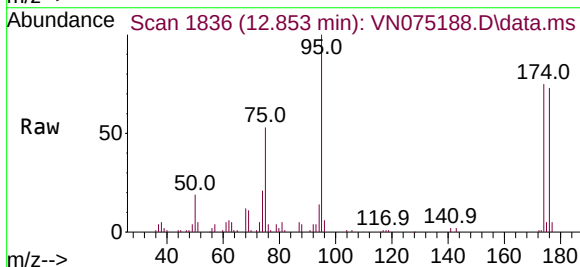




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.864 min Scan# 117
Delta R.T. -0.007 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21




Instrument :
MSVOA_N
ClientSampleId :
PB148848TB


Tgt Ion:117 Resp: 175912
Ion Ratio Lower Upper
117 100
82 56.6 43.1 64.7
119 32.2 25.5 38.3

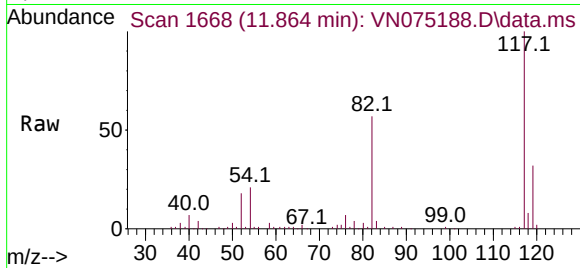

#71
Bromoform
Concen: 0.528 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.271 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21

Tgt Ion:173 Resp: 551
Ion Ratio Lower Upper
173 100
175 611.8 24.6 74.0#
254 0.0 0.0 0.0


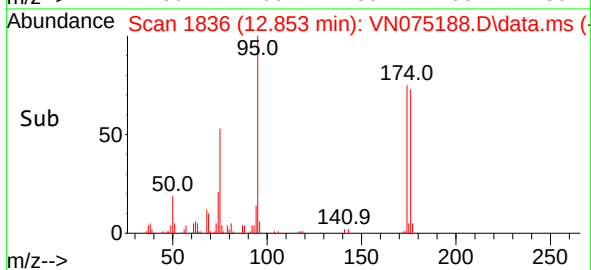

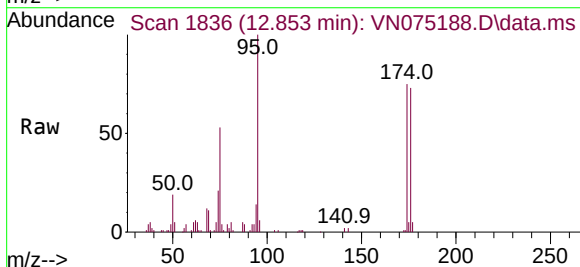




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21




Instrument :
MSVOA_N
ClientSampleId :
PB148848TB


Tgt Ion:152 Resp: 70505
Ion Ratio Lower Upper
152 100
115 61.8 30.2 90.6
150 157.6 0.0 348.4

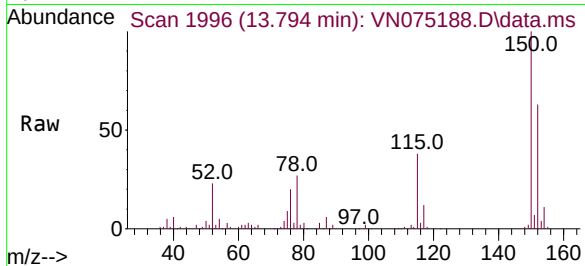

#74
N-ethyl acetate
Concen: 0.271 ug/l
RT: 12.494 min Scan# 1775
Delta R.T. -0.000 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21

Tgt Ion: 43 Resp: 568
Ion Ratio Lower Upper
43 100
70 10.0 39.8 59.8#
55 0.0 19.9 29.9#
61 0.0 21.7 32.5#


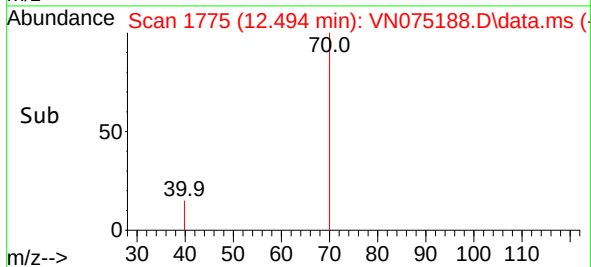

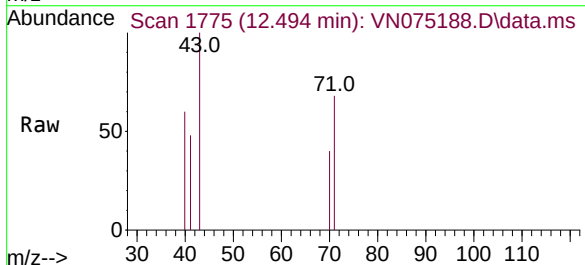




#76
1,2,3-Trichloropropane
Concen: 27.272 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21




Instrument :
MSVOA_N
ClientSampleId :
PB148848TB


Tgt Ion: 75 Resp: 40826
Ion Ratio Lower Upper
75 100
77 0.8 75.6 226.8#



#81
trans-1,4-Dichloro-2-butene
Concen: 70.006 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.112 min
Lab File: VN075188.D
Acq: 07 Nov 2022 15:21

Tgt Ion: 75 Resp: 40826
Ion Ratio Lower Upper
75 100
53 0.0 78.5 117.7#
89 0.0 37.7 56.5#


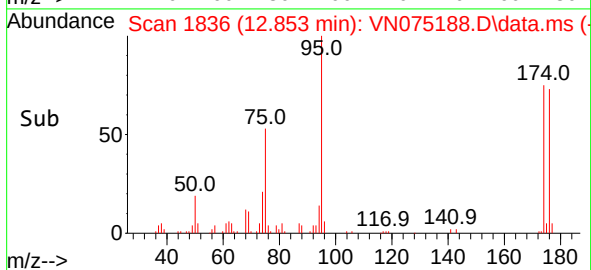






#93
 1,2,4-Trichlorobenzene
 Concen: 0.346 ug/l
 RT: 15.394 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN075188.D
 Acq: 07 Nov 2022 15:21




Instrument :
 MSVOA_N
 ClientSampleId :
 PB148848TB


Tgt Ion:180 Resp: 361
 Ion Ratio Lower Upper
 180 100
 182 88.9 47.8 143.4
 145 0.0 16.8 50.3#



#95
 Naphthalene
 Concen: 0.817 ug/l
 RT: 15.641 min Scan# 2310
 Delta R.T. -0.000 min
 Lab File: VN075188.D
 Acq: 07 Nov 2022 15:21


Tgt Ion:128 Resp: 3279
 Ion Ratio Lower Upper
 128 100
 127 6.8 10.4 15.6#
 129 6.8 8.6 12.8#

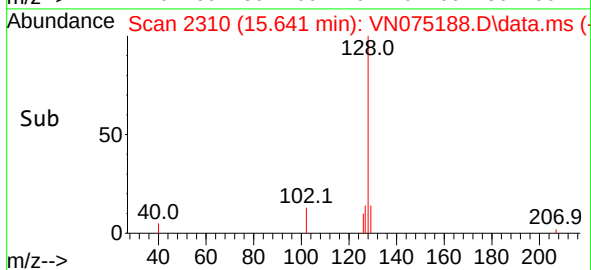



#96
 1,2,3-Trichlorobenzene
 Concen: 0.574 ug/l
 RT: 15.835 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VN075188.D
 Acq: 07 Nov 2022 15:21

Instrument :
 MSVOA_N
 ClientSampleId :
 PB148848TB



Tgt Ion:180 Resp: 595
 Ion Ratio Lower Upper
 180 100
 182 90.4 47.3 141.8
 145 0.0 17.6 52.9#

