
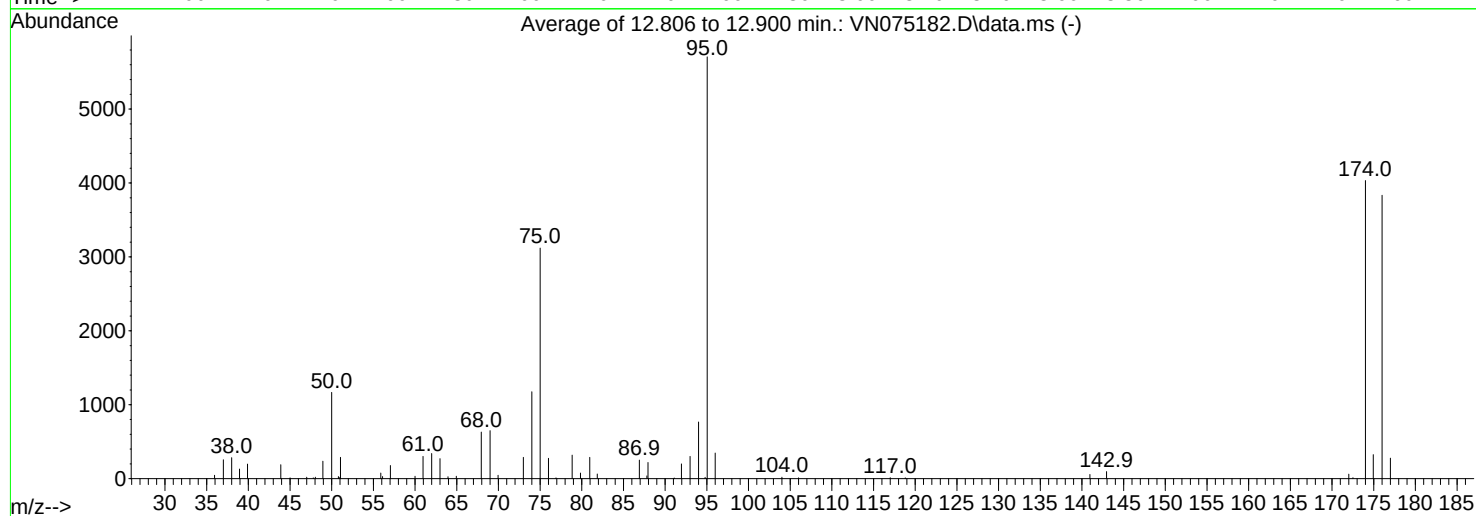


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110722\
 Data File : VN075182.D
 Acq On : 07 Nov 2022 11:46
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
 Title : SW846 8260
 Last Update : Thu Oct 27 09:48:49 2022

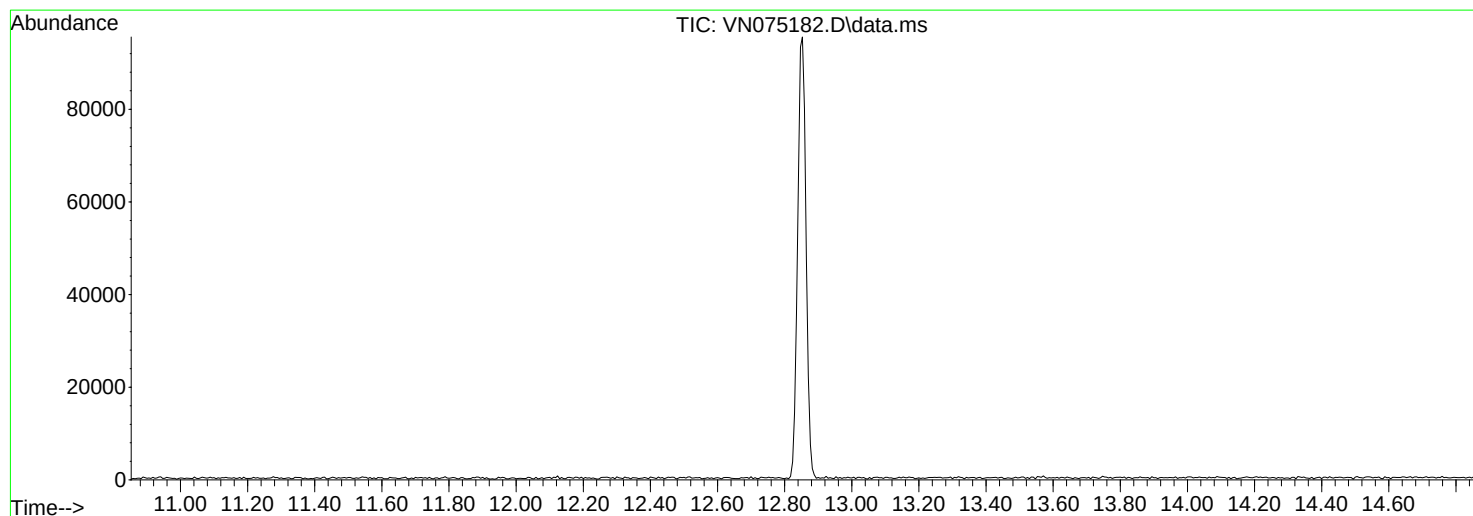

AutoFind: Averaged scan 1828 to 1844; Bkg corrected with scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	1166	PASS
75	95	30	60	54.7	3119	PASS
95	95	100	100	100.0	5707	PASS
96	95	5	9	6.1	347	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.7	4034	PASS
175	174	5	9	8.1	325	PASS
176	174	95	101	95.0	3833	PASS
177	176	5	9	7.2	277	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	46	50.00	1166	63.95	26	79.85	7
37.00	255	50.80	29	64.95	32	80.95	28
38.00	284	50.90	17	67.95	631	81.85	6
38.95	130	51.05	289	69.00	649	86.90	25
39.90	197	55.90	76	69.95	45	87.80	37
43.90	189	56.10	28	73.00	287	87.95	219
45.00	11	57.05	178	74.00	1175	91.10	9
47.00	19	60.00	33	75.00	3119	91.95	199
47.80	11	60.95	302	76.00	275	93.00	301
48.05	20	62.00	341	76.90	10	94.00	767
48.95	237	63.00	270	78.85	319	94.80	18

Average of 12.806 to 12.900 min.: VN075182.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.05	5707	174.95	325				
96.00	347	176.00	3833				
104.00	20	177.00	277				
106.00	10						
117.00	12						
118.80	11						
140.95	56						
142.95	95						
172.00	61						
172.50	13						
174.00	4034						

Instrument :

MSVOA_N

ClientSampleId :

BFB