

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110723\
 Data File : VN079973.D
 Acq On : 07 Nov 2023 18:34
 Operator : JC\MD
 Sample : 05107-29 20X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 1076

Quant Time: Nov 08 04:33:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 02 05:49:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.229	168	282047	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	574687	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	603545	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	251854	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	242796	56.503	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 113.000%			
35) Dibromofluoromethane	8.171	113	199037	48.935	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 97.860%			
50) Toluene-d8	10.570	98	726343	48.508	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 97.020%			
62) 4-Bromofluorobenzene	12.853	95	271784	54.729	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 109.460%			
Target Compounds						Qvalue
3) Chloromethane	2.371	50	950	Below Cal	#	42
5) Bromomethane	2.965	94	554	0.205	ug/l #	60
11) Tert butyl alcohol	5.512	59	329	0.600	ug/l #	72
16) Acetone	4.441	43	17165	11.372	ug/l #	88
18) Methyl Acetate	5.041	43	3646	0.505	ug/l #	74
20) Methylene Chloride	5.277	84	1584	0.416	ug/l #	75
25) 2-Butanone	7.494	43	4423	2.001	ug/l	99
30) Chloroform	7.965	83	1552	0.218	ug/l #	68
31) Cyclohexane	8.224	56	8011	1.411	ug/l #	38
36) 1,1-Dichloropropene	8.229	75	25737	4.432	ug/l #	46
38) Carbon Tetrachloride	8.229	117	30035	5.132	ug/l #	15
40) Benzene	8.612	78	557895	32.073	ug/l	100
43) Isopropyl Acetate	8.700	43	11130	1.192	ug/l #	78
48) Methyl methacrylate	9.659	41	1177	0.288	ug/l #	13
51) 4-Methyl-2-Pentanone	10.453	43	4205	0.800	ug/l #	64
52) Toluene	10.635	92	218642	21.202	ug/l	100
53) t-1,3-Dichloropropene	10.641	75	2837	0.447	ug/l #	1
54) cis-1,3-Dichloropropene	10.365	75	1789	0.259	ug/l #	72
55) 1,1,2-Trichloroethane	10.888	97	2064	0.498	ug/l #	30
59) 2-Hexanone	11.176	43	4951	1.231	ug/l #	19
67) Ethyl Benzene	11.964	91	19906	0.873	ug/l	90
68) m/p-Xylenes	12.070	106	32732	3.852	ug/l	86
69) o-Xylene	12.406	106	23776	2.906	ug/l	92
70) Styrene	12.412	104	5994	0.456	ug/l #	27
76) 1,2,3-Trichloropropane	12.853	75	147415	24.932	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.176	105	5915	0.398	ug/l	91
81) trans-1,4-Dichloro-2-b...	12.853	75	147415	67.833	ug/l #	15
84) 1,2,4-Trimethylbenzene	13.494	105	20065	1.371	ug/l	79
85) sec-Butylbenzene	13.494	105	20065	1.190	ug/l #	57
95) Naphthalene	15.647	128	266490	20.110	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110723\
Data File : VN079973.D
Acq On : 07 Nov 2023 18:34
Operator : JC\MD
Sample : 05107-29 20X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
1076

Quant Time: Nov 08 04:33:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 02 05:49:08 2023
Response via : Initial Calibration

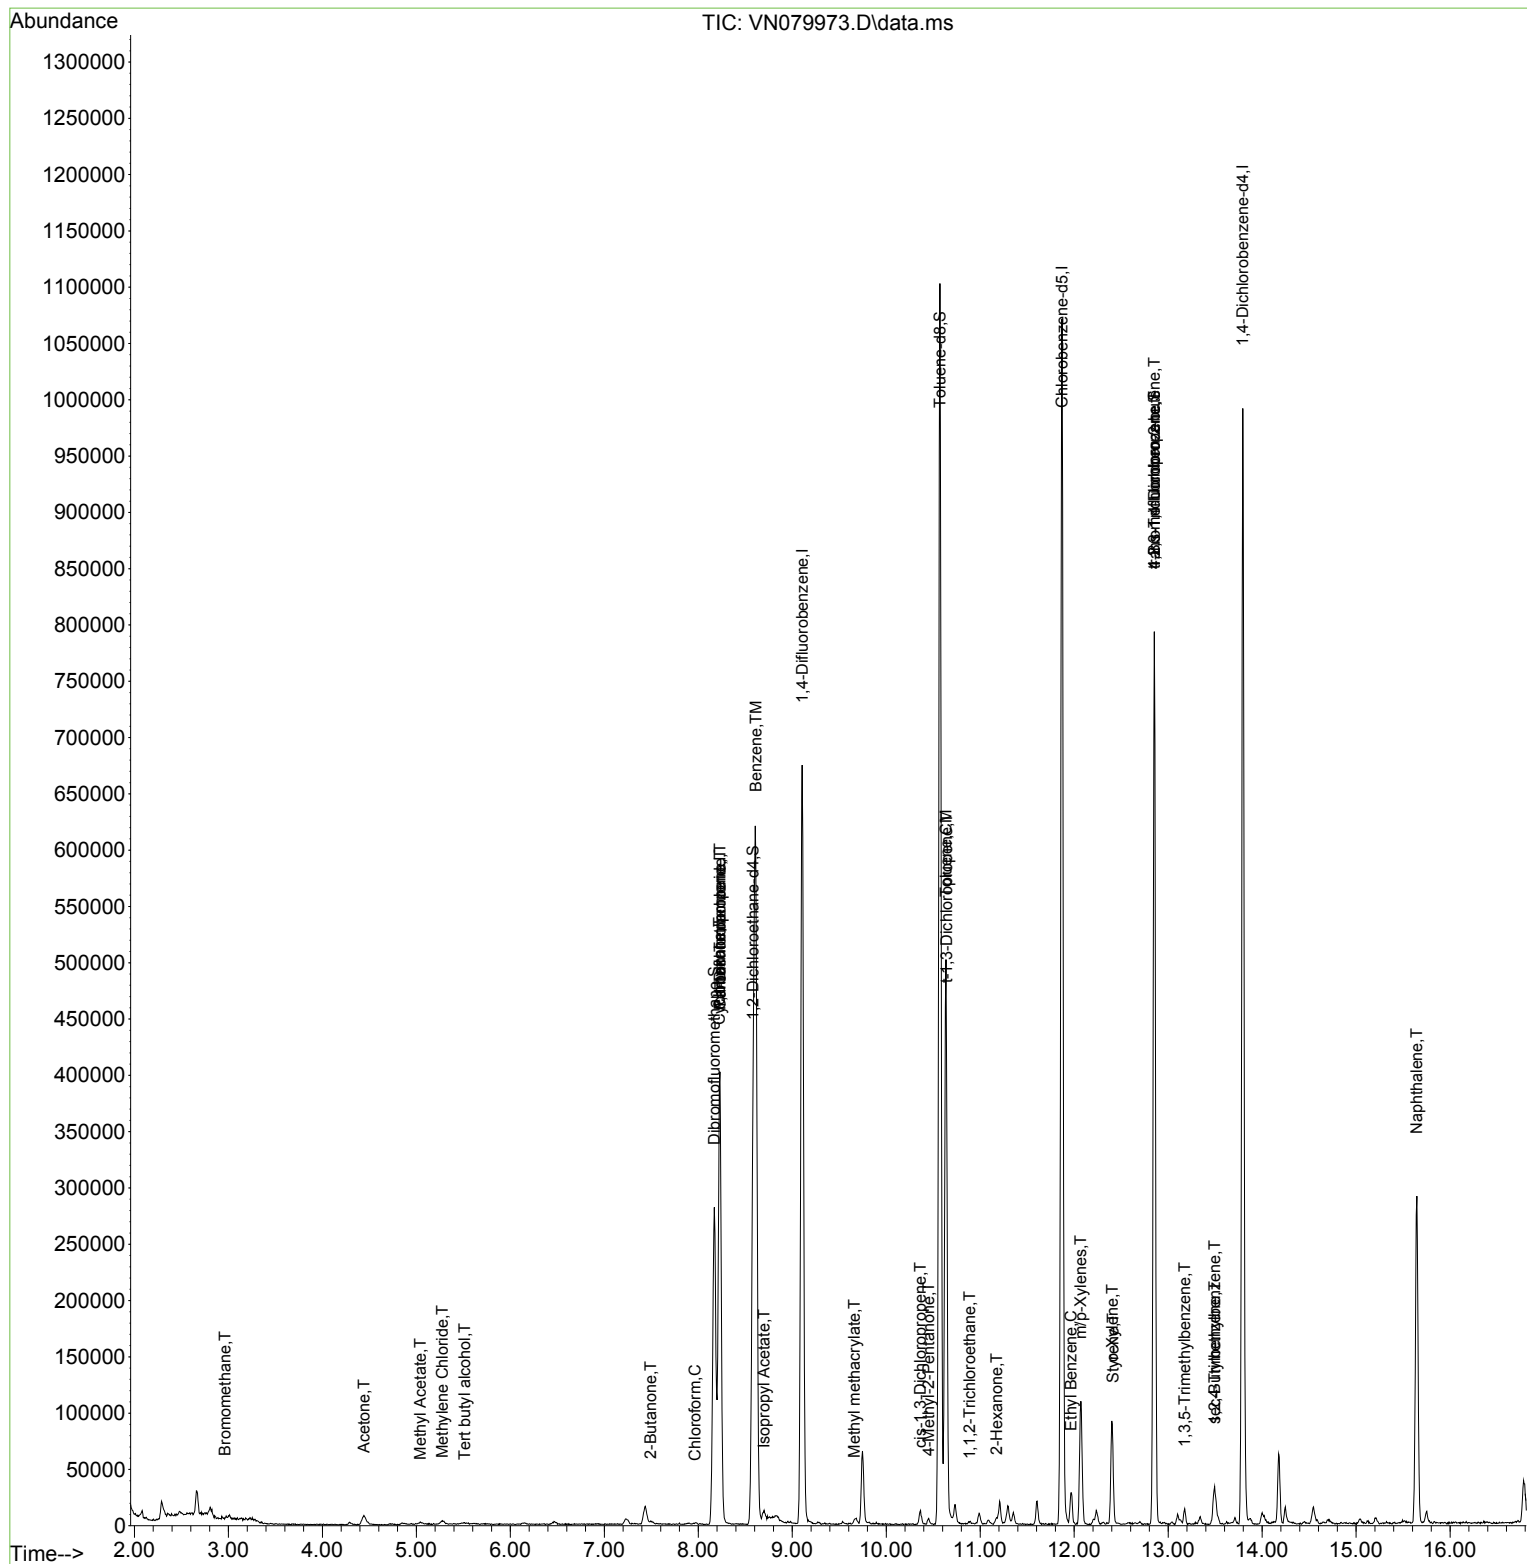



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.229 min Scan# 1067

Delta R.T. 0.000 min

Lab File: VN079973.D

Acq: 07 Nov 2023 18:34

Instrument :

MSVOA_N

ClientSampleId :





1076

Tgt Ion:168 Resp: 282047

Ion Ratio Lower Upper

168 100

99 62.7 53.0 79.6

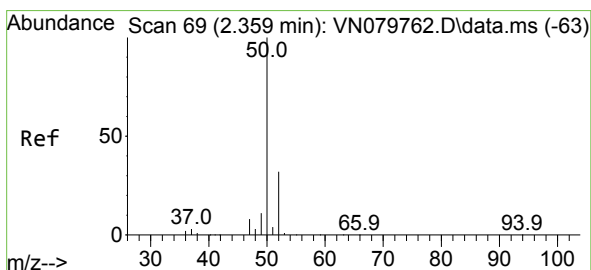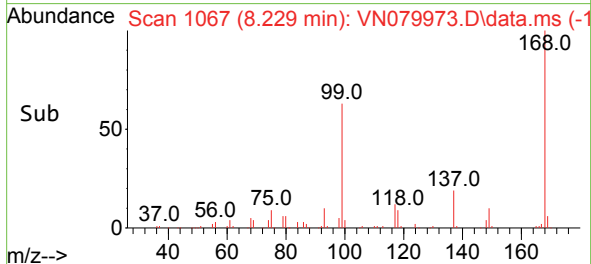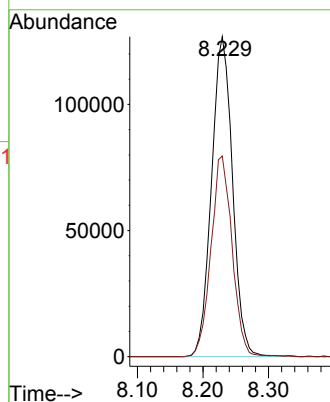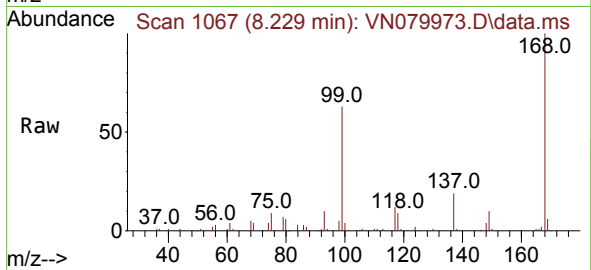

#3

Chloromethane

Concen: Below Cal

RT: 2.371 min Scan# 71

Delta R.T. 0.012 min

Lab File: VN079973.D




Acq: 07 Nov 2023 18:34


Tgt Ion: 50 Resp: 950

Ion Ratio Lower Upper

50 100

52 0.0 26.5 39.7#



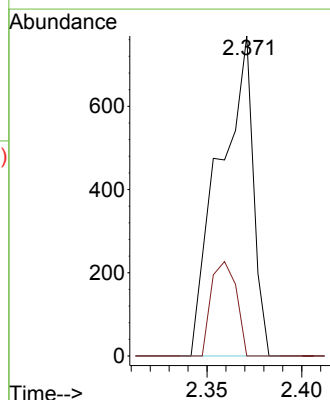





#5
Bromomethane
Concen: 0.205 ug/l
RT: 2.965 min Scan# 11
Delta R.T. 0.012 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34




Instrument :
MSVOA_N
ClientSampleId :
1076


Tgt Ion: 94 Resp: 554
Ion Ratio Lower Upper
94 100
96 53.2 73.1 109.7#

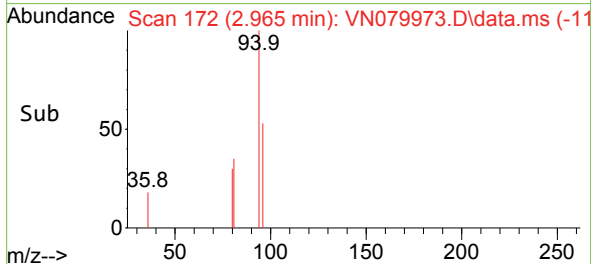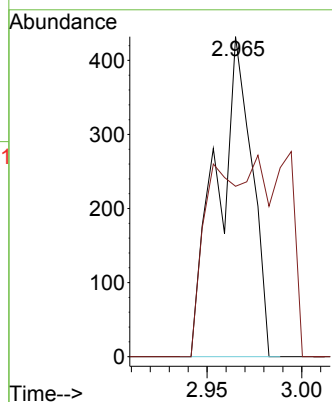

#11
Tert butyl alcohol
Concen: 0.600 ug/l
RT: 5.512 min Scan# 605
Delta R.T. -0.006 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34

Tgt Ion: 59 Resp: 329
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#



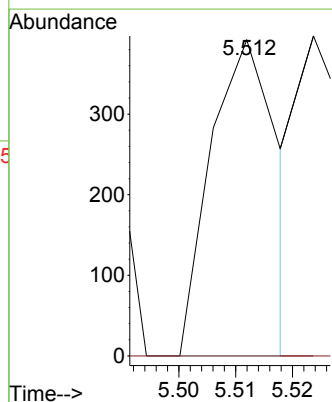





#16
Acetone
Concen: 11.372 ug/l
RT: 4.441 min Scan# 41
Delta R.T. 0.012 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34




Instrument :
MSVOA_N
ClientSampleId :
1076


Tgt Ion: 43 Resp: 17165
Ion Ratio Lower Upper
43 100
58 27.8 28.0 42.0#

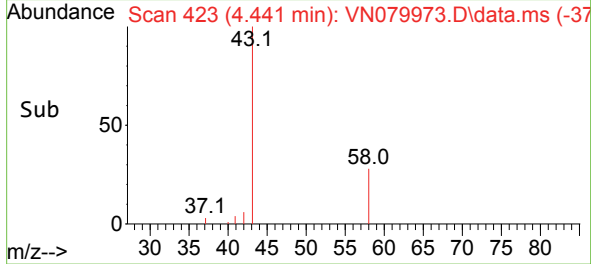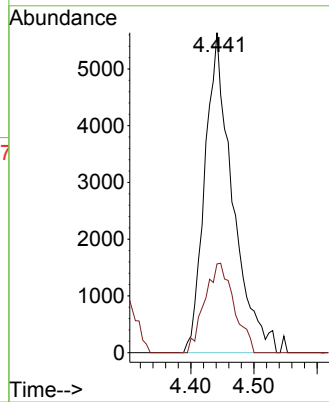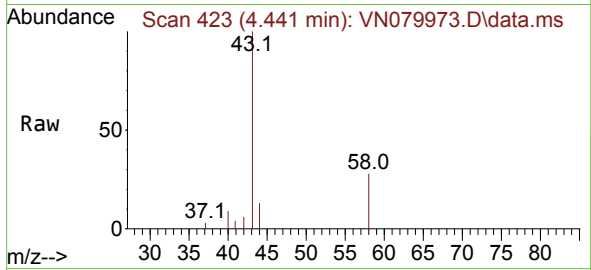

#18
Methyl Acetate
Concen: 0.505 ug/l
RT: 5.041 min Scan# 525
Delta R.T. 0.018 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34

Tgt Ion: 43 Resp: 3646
Ion Ratio Lower Upper
43 100
74 18.1 26.2 39.4#


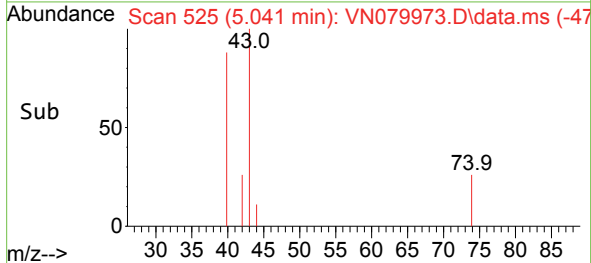
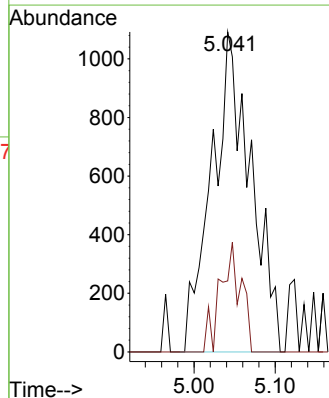





#20
Methylene Chloride
Concen: 0.416 ug/l
RT: 5.277 min Scan# 510
Delta R.T. 0.006 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34




Instrument :
MSVOA_N
ClientSampleId :
1076


Tgt Ion: 84	Resp: 1584
Ion Ratio	Lower Upper
84 100	
49 118.1	79.7 119.5
51 64.9	25.2 37.8#
86 81.7	53.3 79.9#



#25
2-Butanone
Concen: 2.001 ug/l
RT: 7.494 min Scan# 942
Delta R.T. 0.006 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34

Tgt Ion: 43	Resp: 4423		
Ion Ratio	Lower	Upper	
43 100			
72 38.5	30.2	45.2	


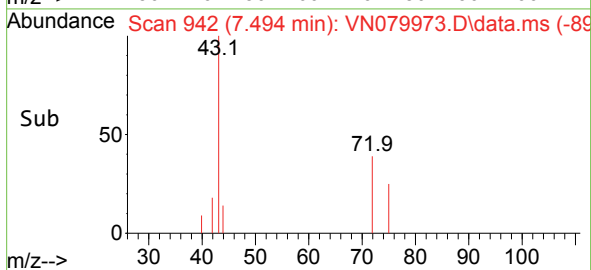






#30
Chloroform
Concen: 0.218 ug/l
RT: 7.965 min Scan# 1076
Delta R.T. -0.006 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34




Instrument :
MSVOA_N
ClientSampleId :
1076


Tgt Ion: 83 Resp: 1552
Ion Ratio Lower Upper
83 100
85 42.8 55.4 83.0#

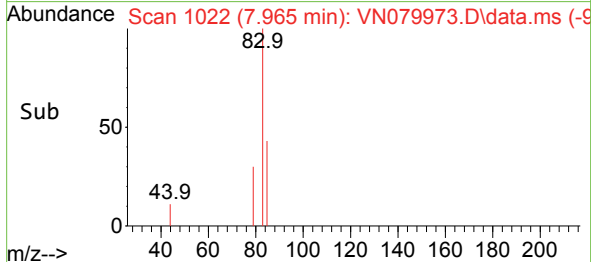

#31
Cyclohexane
Concen: 1.411 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.035 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34

Tgt Ion: 56 Resp: 8011
Ion Ratio Lower Upper
56 100
69 143.5 26.8 40.2#
84 83.2 81.8 122.6




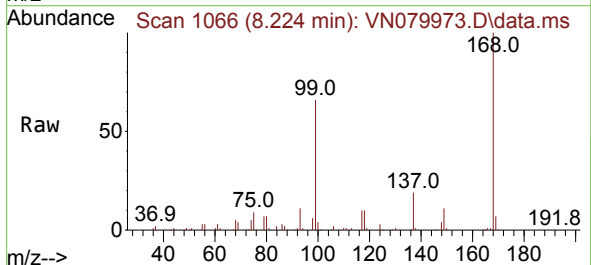




#33
 1,2-Dichloroethane-d4
 Concen: 56.503 ug/l
 RT: 8.582 min Scan# 1127
 Delta R.T. -0.000 min
 Lab File: VN079973.D
 Acq: 07 Nov 2023 18:34




Instrument :
 MSVOA_N
 ClientSampleId :
 1076


Tgt Ion: 65 Resp: 242796
 Ion Ratio Lower Upper
 65 100
 67 52.1 0.0 106.6

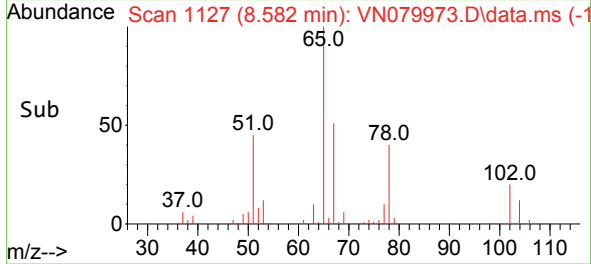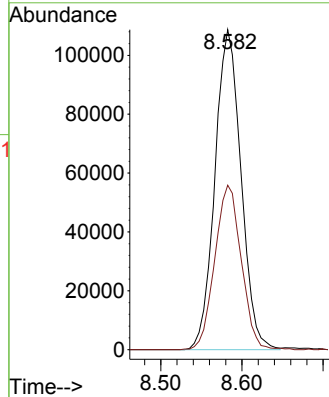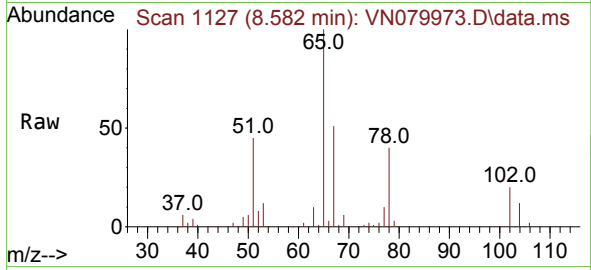

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 9.106 min Scan# 1216
 Delta R.T. -0.000 min
 Lab File: VN079973.D
 Acq: 07 Nov 2023 18:34

Tgt Ion: 114 Resp: 574687
 Ion Ratio Lower Upper
 114 100
 63 22.1 0.0 36.4
 88 16.3 0.0 30.6



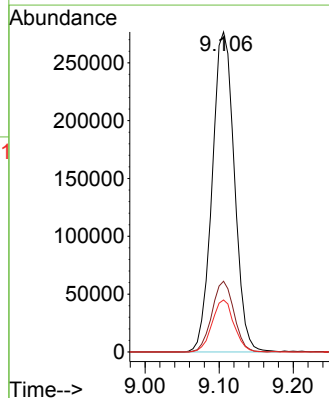





#35
Dibromofluoromethane
Concen: 48.935 ug/l
RT: 8.171 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34




Instrument :
MSVOA_N
ClientSampleId :
1076


Tgt Ion:113 Resp: 199037
Ion Ratio Lower Upper
113 100
111 104.1 82.6 123.8
192 17.7 12.7 19.1

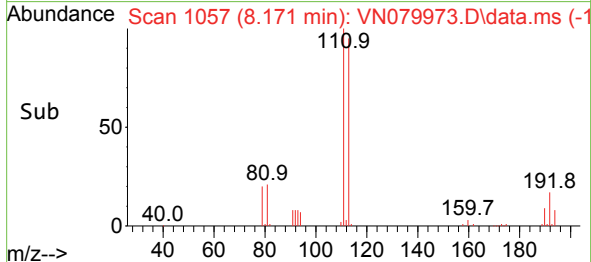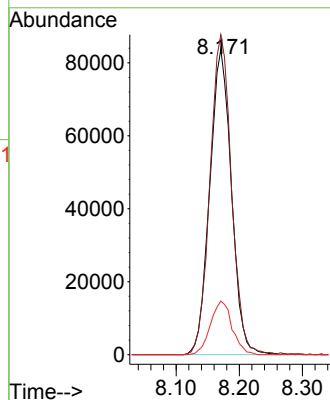

#36
1,1-Dichloropropene
Concen: 4.432 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34

Tgt Ion: 75 Resp: 25737
Ion Ratio Lower Upper
75 100
110 7.3 19.1 57.3#
77 0.0 25.0 37.4#

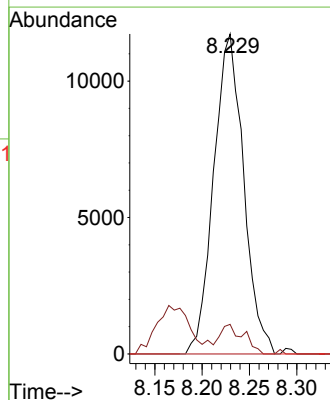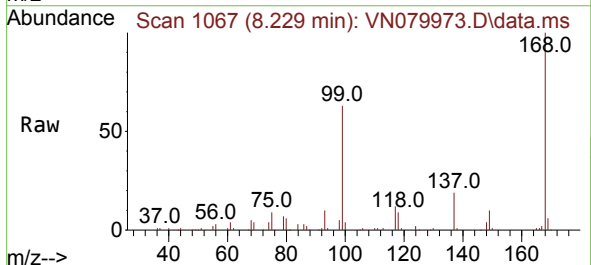



#38

Carbon Tetrachloride

Concen: 5.132 ug/l

RT: 8.229 min Scan# 1067

Delta R.T. -0.129 min

Lab File: VN079973.D


Acq: 07 Nov 2023 18:34

Instrument :

MSVOA_N

ClientSampleId :

1076






Tgt Ion:117 Resp: 30035

Ion Ratio Lower Upper

117 100

119 4.6 77.3 115.9#

121 0.0 23.3 34.9#

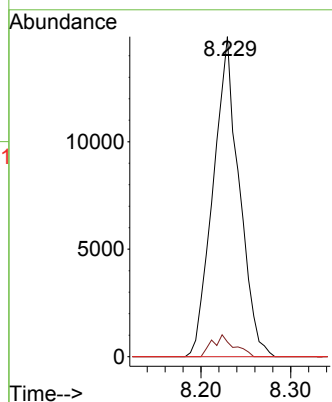

#40

Benzene

Concen: 32.073 ug/l

RT: 8.612 min Scan# 1132

Delta R.T. -0.000 min

Lab File: VN079973.D




Acq: 07 Nov 2023 18:34


Tgt Ion: 78 Resp: 557895

Ion Ratio Lower Upper

78 100

77 24.0 19.0 28.6


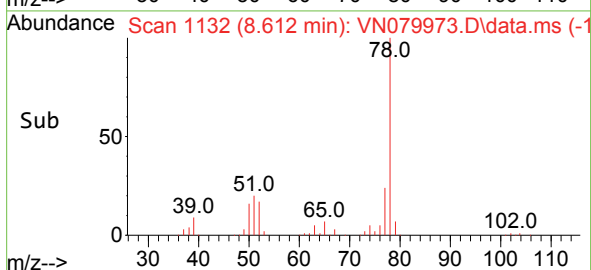






#43
Isopropyl Acetate
Concen: 1.192 ug/l
RT: 8.700 min Scan# 1145
Delta R.T. 0.012 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34




Instrument :
MSVOA_N
ClientSampleId :
1076


Tgt Ion: 43 Resp: 11130
Ion Ratio Lower Upper
43 100
61 16.9 24.7 37.1#
87 10.5 14.6 21.8#

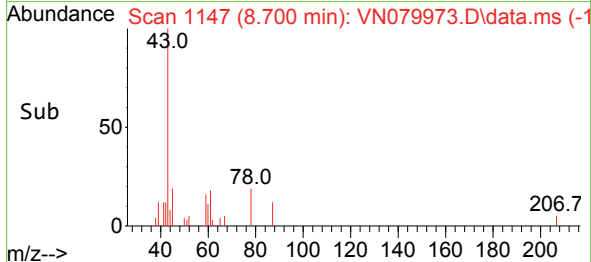

#48
Methyl methacrylate
Concen: 0.288 ug/l
RT: 9.659 min Scan# 1310
Delta R.T. -0.024 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34

Tgt Ion: 41 Resp: 1177
Ion Ratio Lower Upper
41 100
69 0.0 90.4 135.6#
39 22.9 54.6 81.8#


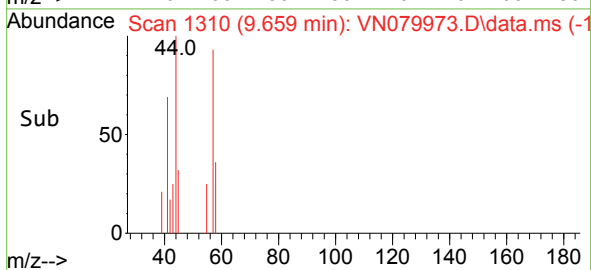

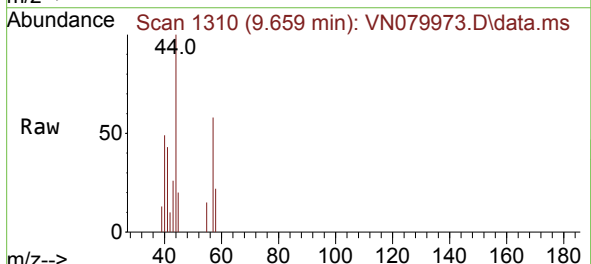


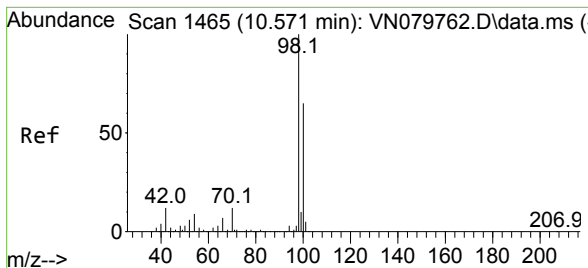

#50
Toluene-d8
Concen: 48.508 ug/l
RT: 10.570 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34




Instrument :
MSVOA_N
ClientSampleId :
1076


Tgt Ion: 98 Resp: 726343
Ion Ratio Lower Upper
98 100
100 64.6 52.0 78.0

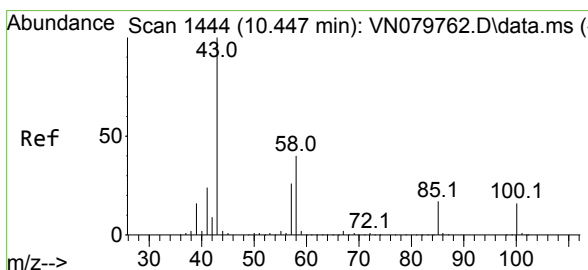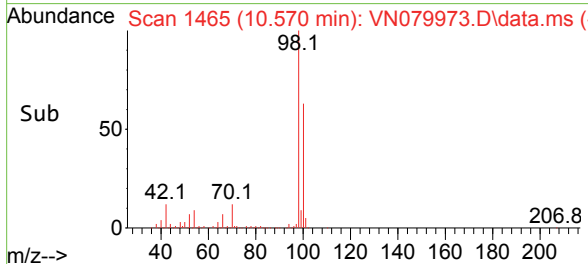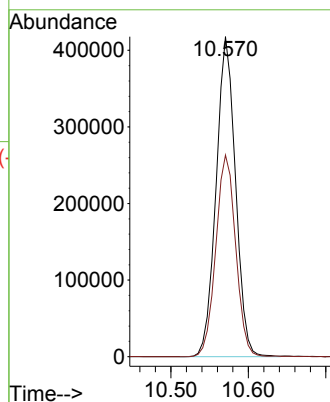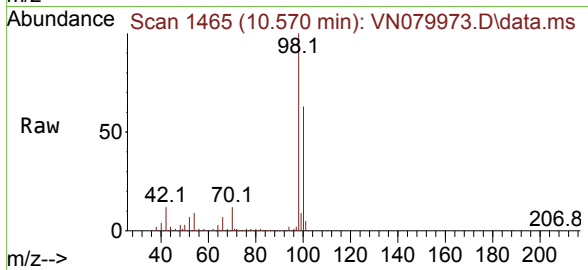

#51
4-Methyl-2-Pentanone
Concen: 0.800 ug/l
RT: 10.453 min Scan# 1445
Delta R.T. 0.006 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34

Tgt Ion: 43 Resp: 4205
Ion Ratio Lower Upper
43 100
58 22.0 36.6 54.8#

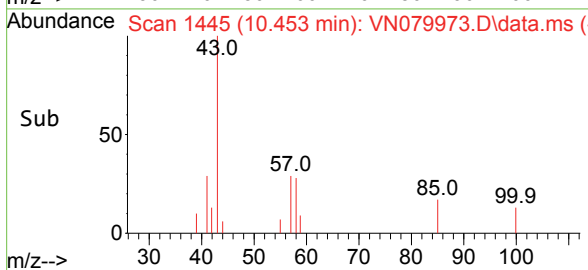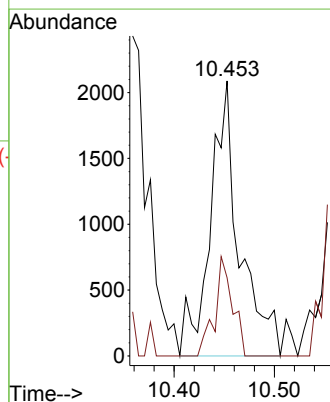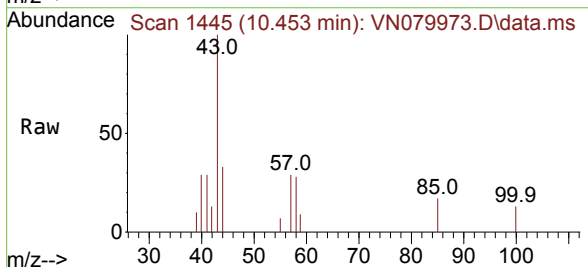

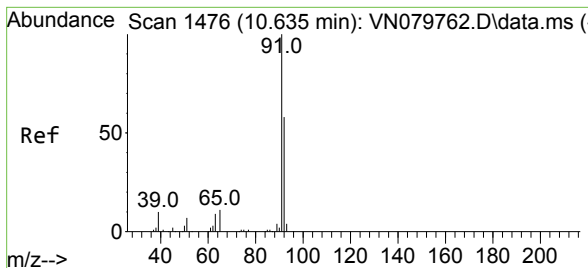

#52

Toluene

Concen: 21.202 ug/l

RT: 10.635 min Scan# 1476

Delta R.T. -0.000 min

Lab File: VN079973.D

Acq: 07 Nov 2023 18:34

Instrument :

MSVOA_N

ClientSampleId :





1076

Tgt Ion: 92 Resp: 218642

Ion Ratio Lower Upper

92 100

91 172.2 137.4 206.0

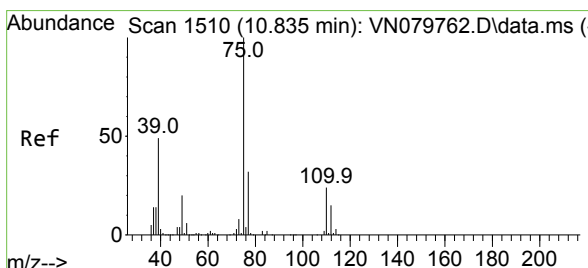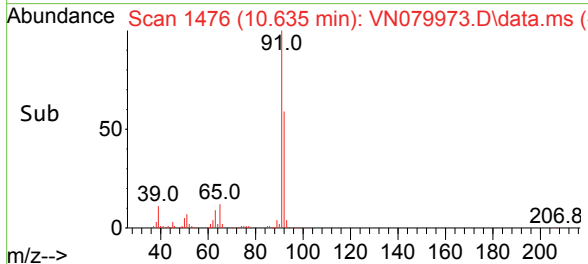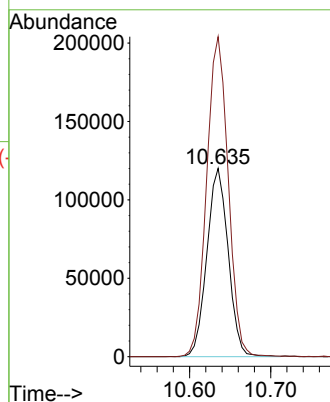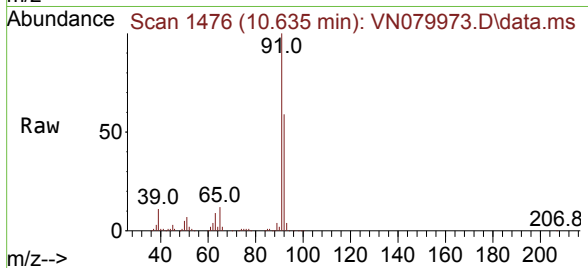

#53

t-1,3-Dichloropropene

Concen: 0.447 ug/l

RT: 10.641 min Scan# 1477

Delta R.T. -0.200 min

Lab File: VN079973.D




Acq: 07 Nov 2023 18:34


Tgt Ion: 75 Resp: 2837

Ion Ratio Lower Upper

75 100

77 160.9 25.4 38.0#


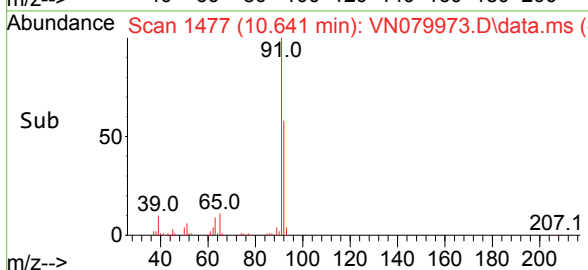
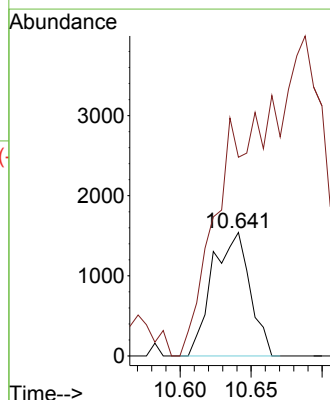
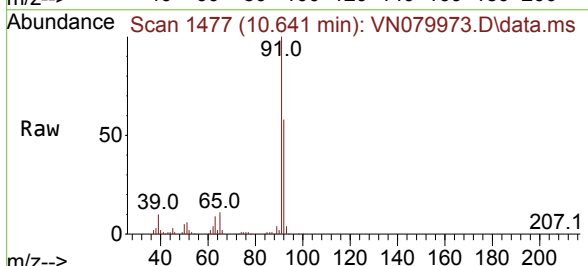


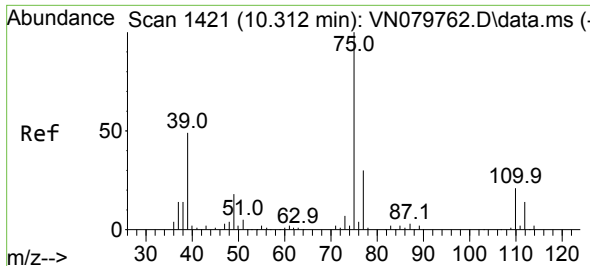

#54
 cis-1,3-Dichloropropene
 Concen: 0.259 ug/l
 RT: 10.365 min Scan# 1421
 Delta R.T. 0.047 min
 Lab File: VN079973.D
 Acq: 07 Nov 2023 18:34




Instrument :
 MSVOA_N
 ClientSampleId :
 1076


Tgt Ion: 75 Resp: 1789
 Ion Ratio Lower Upper
 75 100
 77 0.0 26.1 39.1#
 39 41.0 31.6 47.4

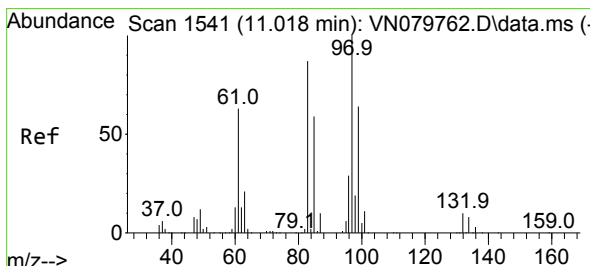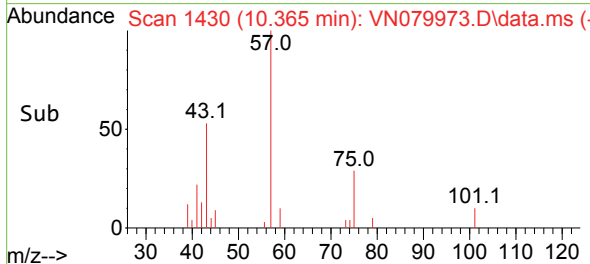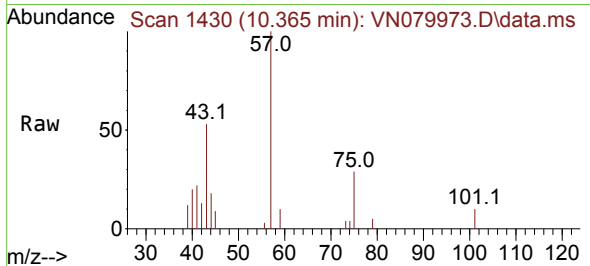

#55
 1,1,2-Trichloroethane
 Concen: 0.498 ug/l
 RT: 10.888 min Scan# 1519
 Delta R.T. -0.129 min
 Lab File: VN079973.D
 Acq: 07 Nov 2023 18:34

Tgt Ion: 97 Resp: 2064
 Ion Ratio Lower Upper
 97 100
 83 0.0 65.1 97.7#
 85 0.0 43.4 65.2#
 99 34.1 49.2 73.8#


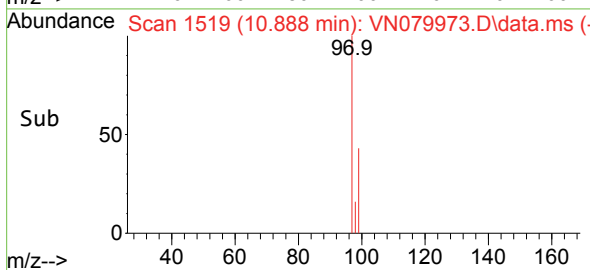

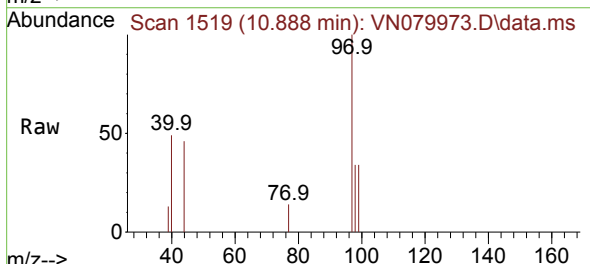




#59
2-Hexanone
Concen: 1.231 ug/l
RT: 11.176 min Scan# 11076
Delta R.T. -0.024 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34




Instrument :
MSVOA_N
ClientSampleId :
1076


Tgt Ion: 43 Resp: 4951
Ion Ratio Lower Upper
43 100
58 0.0 31.7 95.1#

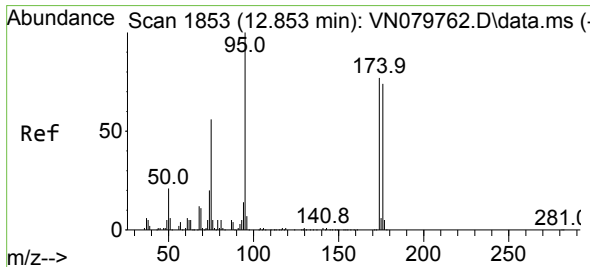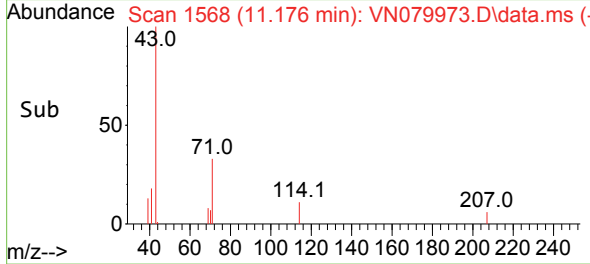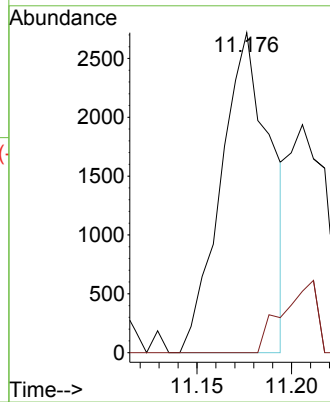

#62
4-Bromofluorobenzene
Concen: 54.729 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34

Tgt Ion: 95 Resp: 271784
Ion Ratio Lower Upper
95 100
174 73.6 0.0 143.8
176 68.7 0.0 135.8


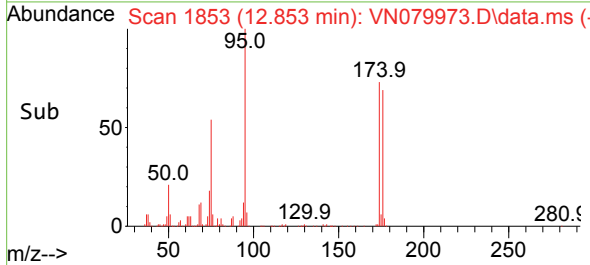
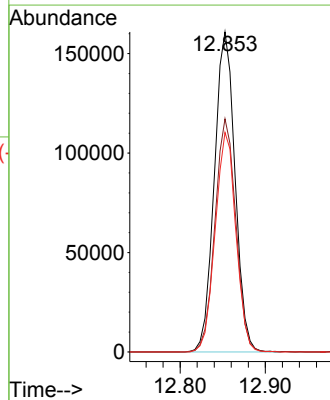
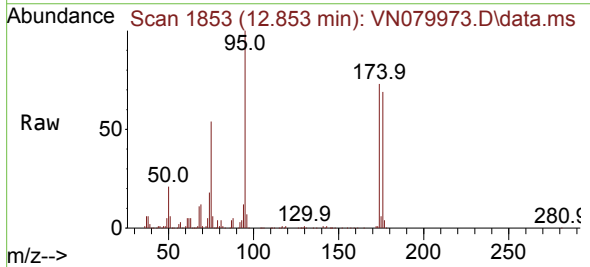


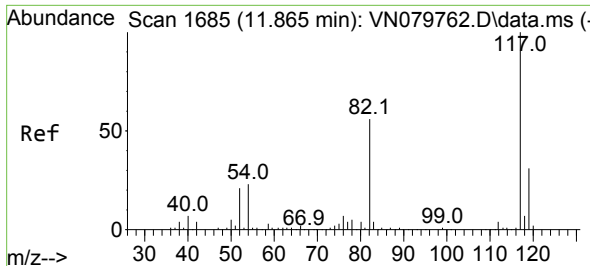

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1176
Delta R.T. -0.000 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34




Instrument :
MSVOA_N
ClientSampleId :
1076


Tgt Ion:117 Resp: 603545
Ion Ratio Lower Upper
117 100
82 57.3 44.0 66.0
119 30.8 25.6 38.4

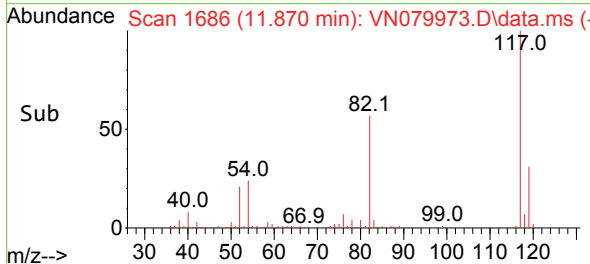

#67
Ethyl Benzene
Concen: 0.873 ug/l
RT: 11.964 min Scan# 1702
Delta R.T. -0.000 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34

Tgt Ion: 91 Resp: 19906
Ion Ratio Lower Upper
91 100
106 37.3 25.6 38.4


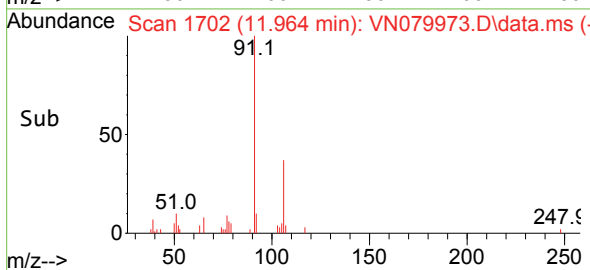

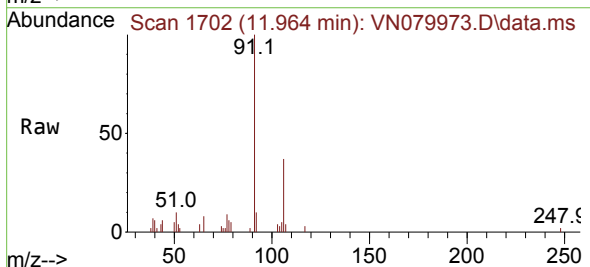




#68
m/p-Xylenes
Concen: 3.852 ug/l
RT: 12.070 min Scan# 11076
Delta R.T. -0.000 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34




Instrument :
MSVOA_N
ClientSampleId :
1076


Tgt Ion:106 Resp: 32732
Ion Ratio Lower Upper
106 100
91 220.1 159.6 239.4

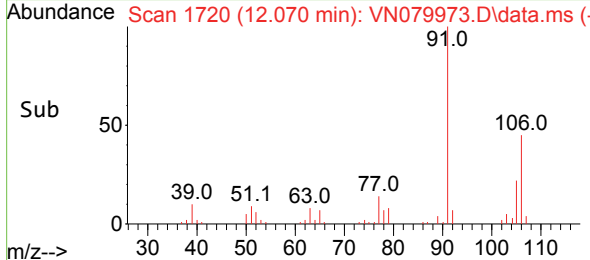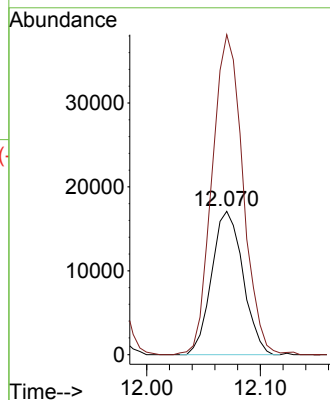

#69
o-Xylene
Concen: 2.906 ug/l
RT: 12.406 min Scan# 1777
Delta R.T. 0.006 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34

Tgt Ion:106 Resp: 23776
Ion Ratio Lower Upper
106 100
91 223.4 105.2 315.5

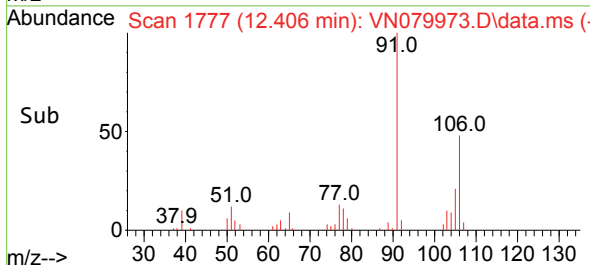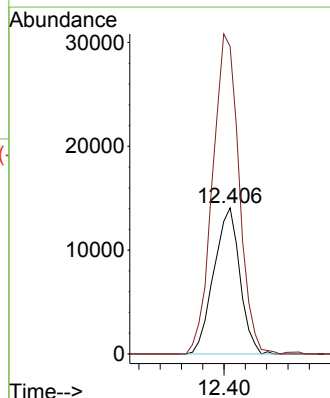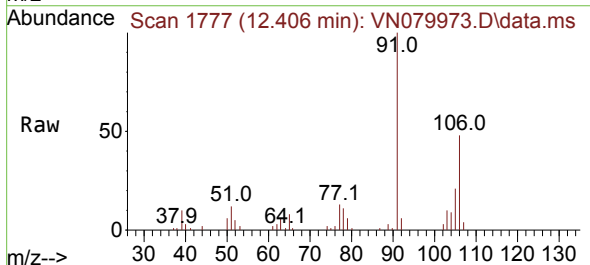



#70

Styrene

Concen: 0.456 ug/l

RT: 12.412 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN079973.D

Acq: 07 Nov 2023 18:34

Instrument :

MSVOA_N

ClientSampleId :

1076





Tgt Ion:104 Resp: 5994

Ion Ratio Lower Upper

104 100

78 105.0 39.5 59.3#

103 101.6 43.2 64.8#

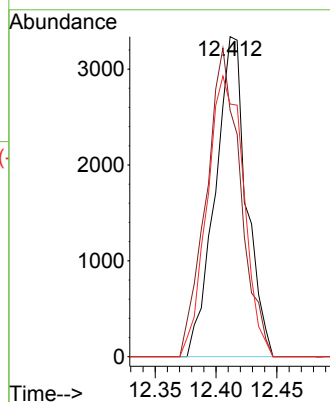

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. -0.000 min

Lab File: VN079973.D

Acq: 07 Nov 2023 18:34




Tgt Ion:152 Resp: 251854


Ion Ratio Lower Upper

152 100

115 63.6 32.3 96.8

150 157.9 0.0 355.8


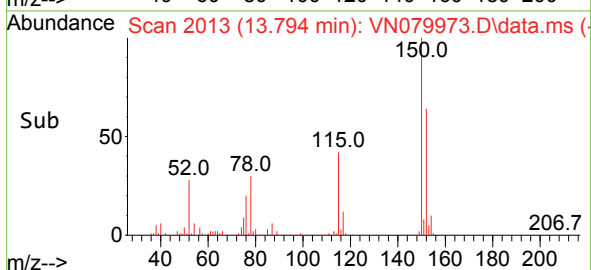
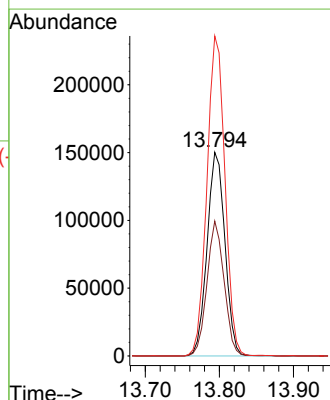





#76
 1,2,3-Trichloropropane
 Concen: 24.932 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. -0.141 min
 Lab File: VN079973.D
 Acq: 07 Nov 2023 18:34




Instrument :
 MSVOA_N
 ClientSampleId :
 1076


Tgt Ion: 75 Resp: 147415
 Ion Ratio Lower Upper
 75 100
 77 1.2 84.5 253.5#

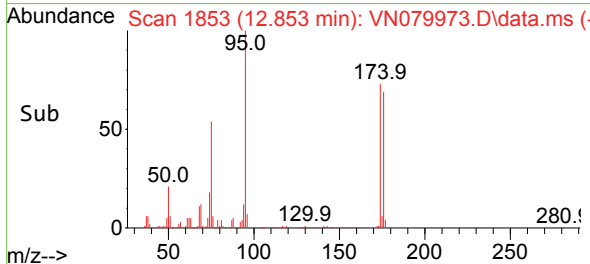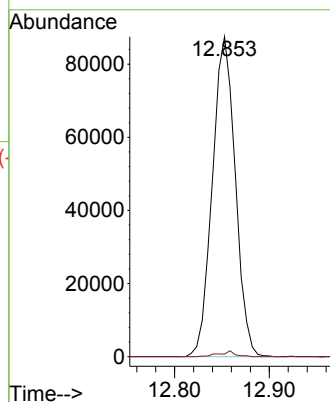

#80
 1,3,5-Trimethylbenzene
 Concen: 0.398 ug/l
 RT: 13.176 min Scan# 1908
 Delta R.T. -0.000 min
 Lab File: VN079973.D
 Acq: 07 Nov 2023 18:34

Tgt Ion:105 Resp: 5915
 Ion Ratio Lower Upper
 105 100
 120 54.2 24.1 72.3


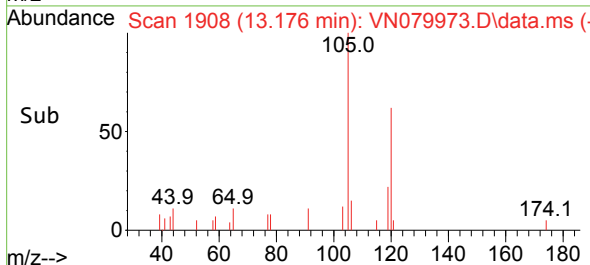
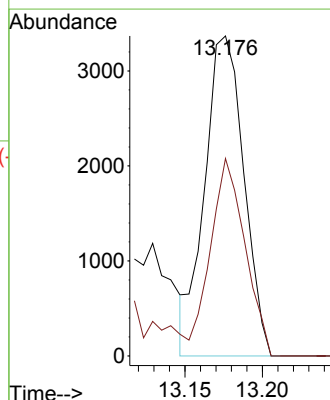
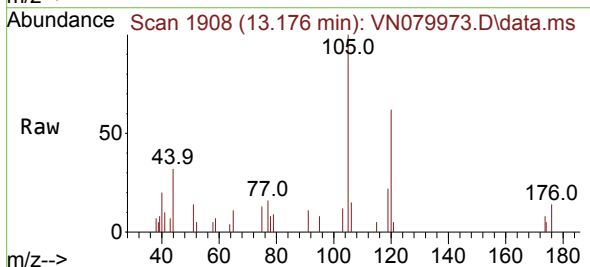




#81
trans-1,4-Dichloro-2-butene
Concen: 67.833 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.118 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34




Instrument :
MSVOA_N
ClientSampleId :
1076


Tgt Ion: 75 Resp: 147415
Ion Ratio Lower Upper
75 100
53 0.4 67.4 101.2#
89 0.0 38.8 58.2#

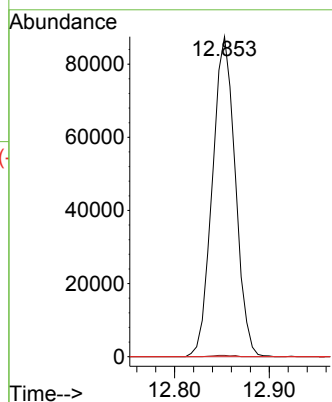

#84
1,2,4-Trimethylbenzene
Concen: 1.371 ug/l
RT: 13.494 min Scan# 1962
Delta R.T. 0.012 min
Lab File: VN079973.D
Acq: 07 Nov 2023 18:34

Tgt Ion: 105 Resp: 20065
Ion Ratio Lower Upper
105 100
120 30.3 22.0 66.0


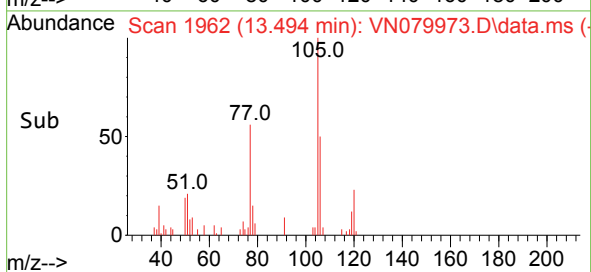
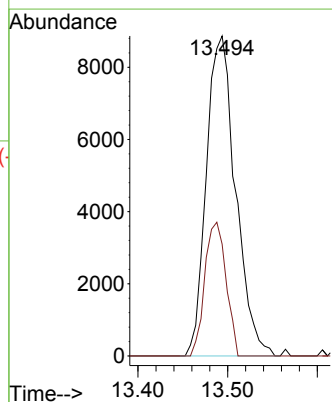
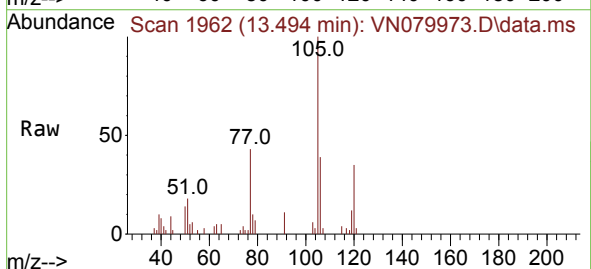




#85
 sec-Butylbenzene
 Concen: 1.190 ug/l
 RT: 13.494 min Scan# 1962
 Delta R.T. -0.124 min
 Lab File: VN079973.D
 Acq: 07 Nov 2023 18:34

Instrument :
 MSVOA_N
 ClientSampleId :
 1076

Tgt Ion:105 Resp: 20065
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.8 29.3#

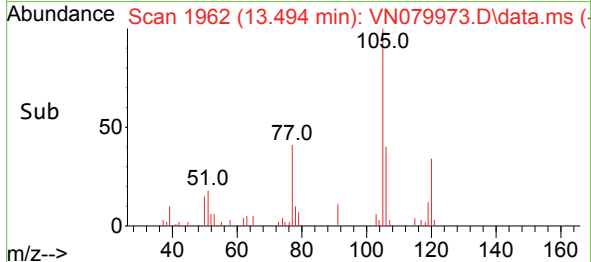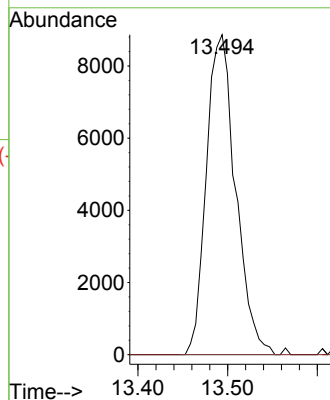

#95
 Naphthalene
 Concen: 20.110 ug/l
 RT: 15.647 min Scan# 2328
 Delta R.T. 0.006 min
 Lab File: VN079973.D
 Acq: 07 Nov 2023 18:34

Tgt Ion:128 Resp: 266490
 Ion Ratio Lower Upper
 128 100
 127 13.1 10.0 15.0
 129 11.1 8.7 13.1

