
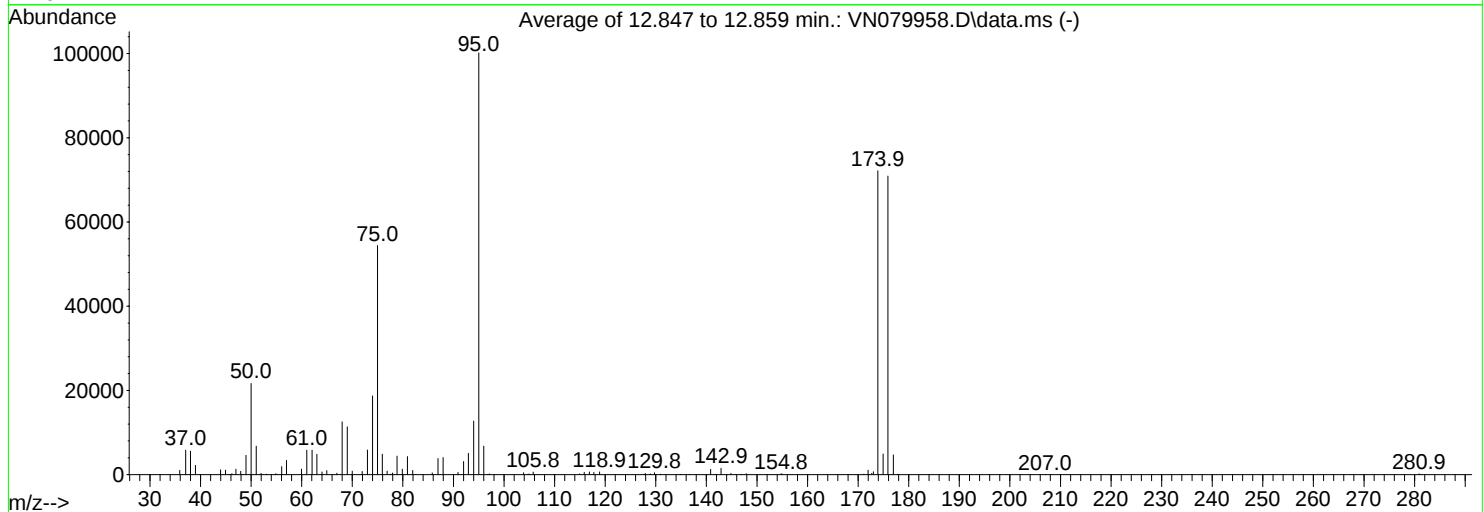


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110723\
Data File : VN079958.D
Acq On : 07 Nov 2023 10:43
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Title : SW846 8260
Last Update : Thu Nov 02 05:49:08 2023

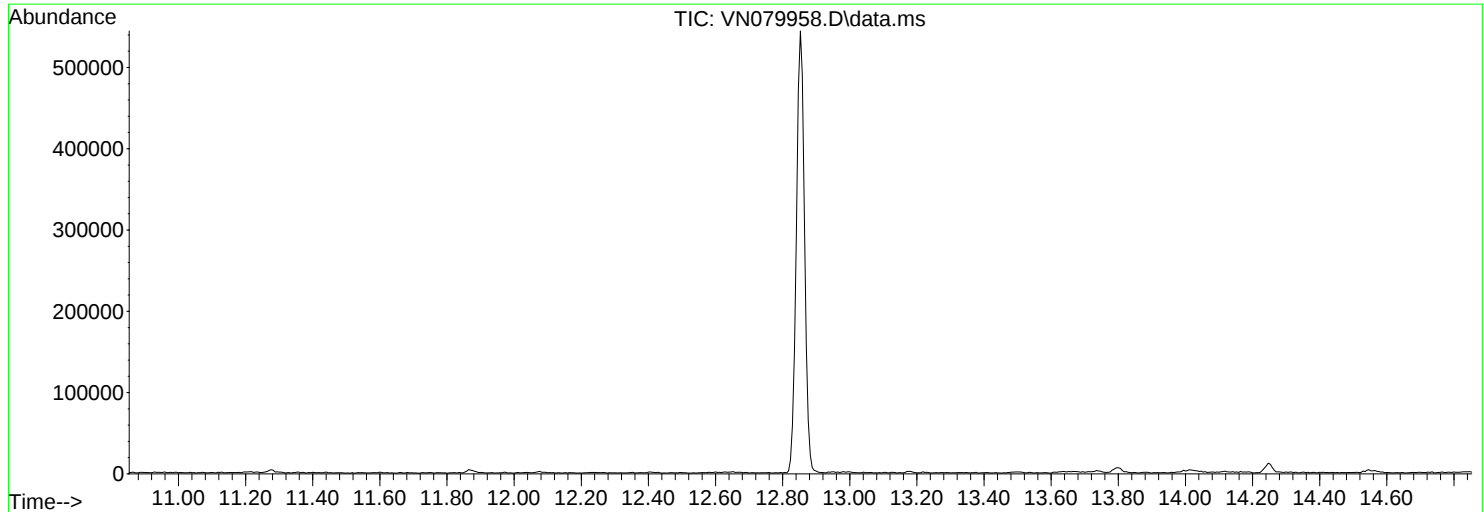

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.6	21661	PASS
75	95	30	60	54.3	54408	PASS
95	95	100	100	100.0	100168	PASS
96	95	5	9	6.7	6750	PASS
173	174	0.00	2	1.0	706	PASS
174	95	50	100	72.0	72160	PASS
175	174	5	9	6.8	4913	PASS
176	174	95	101	98.3	70907	PASS
177	176	5	9	6.6	4681	PASS

Average of 12.847 to 12.859 min.: VN079958.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	1035	50.00	21661	62.05	5796	75.00	5440
37.05	5835	51.00	6762	63.00	4832	75.95	487
38.00	5570	51.95	300	64.00	646	76.90	84
39.00	2218	53.05	109	64.95	961	77.60	11
43.95	1129	54.85	211	66.95	358	77.95	383
44.95	1057	55.10	111	68.00	12550	78.85	4416
45.80	56	56.05	1901	69.00	11375	79.90	1297
46.20	220	57.00	3401	70.00	855	80.90	4307
47.00	1309	58.00	55	71.95	754	81.95	985
47.95	791	59.95	1303	73.00	5860	85.80	429
49.00	4603	61.00	5807	74.00	18683	86.95	3856

Average of 12.847 to 12.859 min.: VN079958.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.95	4074	104.95	174	129.75	441	146.90	72
90.90	550	105.75	611	130.90	122	147.85	218
92.00	3122	109.80	57	134.80	84	154.80	212
92.95	5071	114.90	183	135.00	57	155.00	119
94.00	12741	115.85	530	136.70	84	171.15	127
95.00	100168	116.85	652	140.85	1255	171.95	1055
96.00	6750	117.75	550	141.70	64	172.70	291
96.80	86	118.90	660	142.90	1541	173.00	706
97.10	136	127.70	120	144.10	52	173.90	72160
103.85	460	127.95	274	144.85	303	174.95	4913
104.70	58	128.95	160	145.80	52	175.90	70907

Average of 12.847 to 12.859 min.: VN079958.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.95	4681						
177.80	65						
207.00	62						
280.90	201						
281.30	72						

Instrument :

MSVOA_N

ClientSampleId :

BFB