

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110725\
 Data File : VN088223.D
 Acq On : 07 Nov 2025 10:39
 Operator : JC\MD
 Sample : VN1107MBL01
 Misc : 5.00g/10mL/100uL/5.0mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1107MBL01

Quant Time: Nov 08 01:53:17 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 03 01:16:06 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.206	168	226952	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.082	114	504591	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.841	117	469491	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	213204	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.559	65	227748	58.033	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	116.060%
35) Dibromofluoromethane	8.147	113	173465	51.172	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.340%
50) Toluene-d8	10.541	98	645304	49.404	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	98.800%
62) 4-Bromofluorobenzene	12.829	95	238473	51.697	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	103.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110725\
Data File : VN088223.D
Acq On : 07 Nov 2025 10:39
Operator : JC\MD
Sample : VN1107MBL01
Misc : 5.00g/10mL/100uL/5.0mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1107MBL01

Quant Time: Nov 08 01:53:17 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Quant Title : SW846 8260
QLast Update : Mon Nov 03 01:16:06 2025
Response via : Initial Calibration




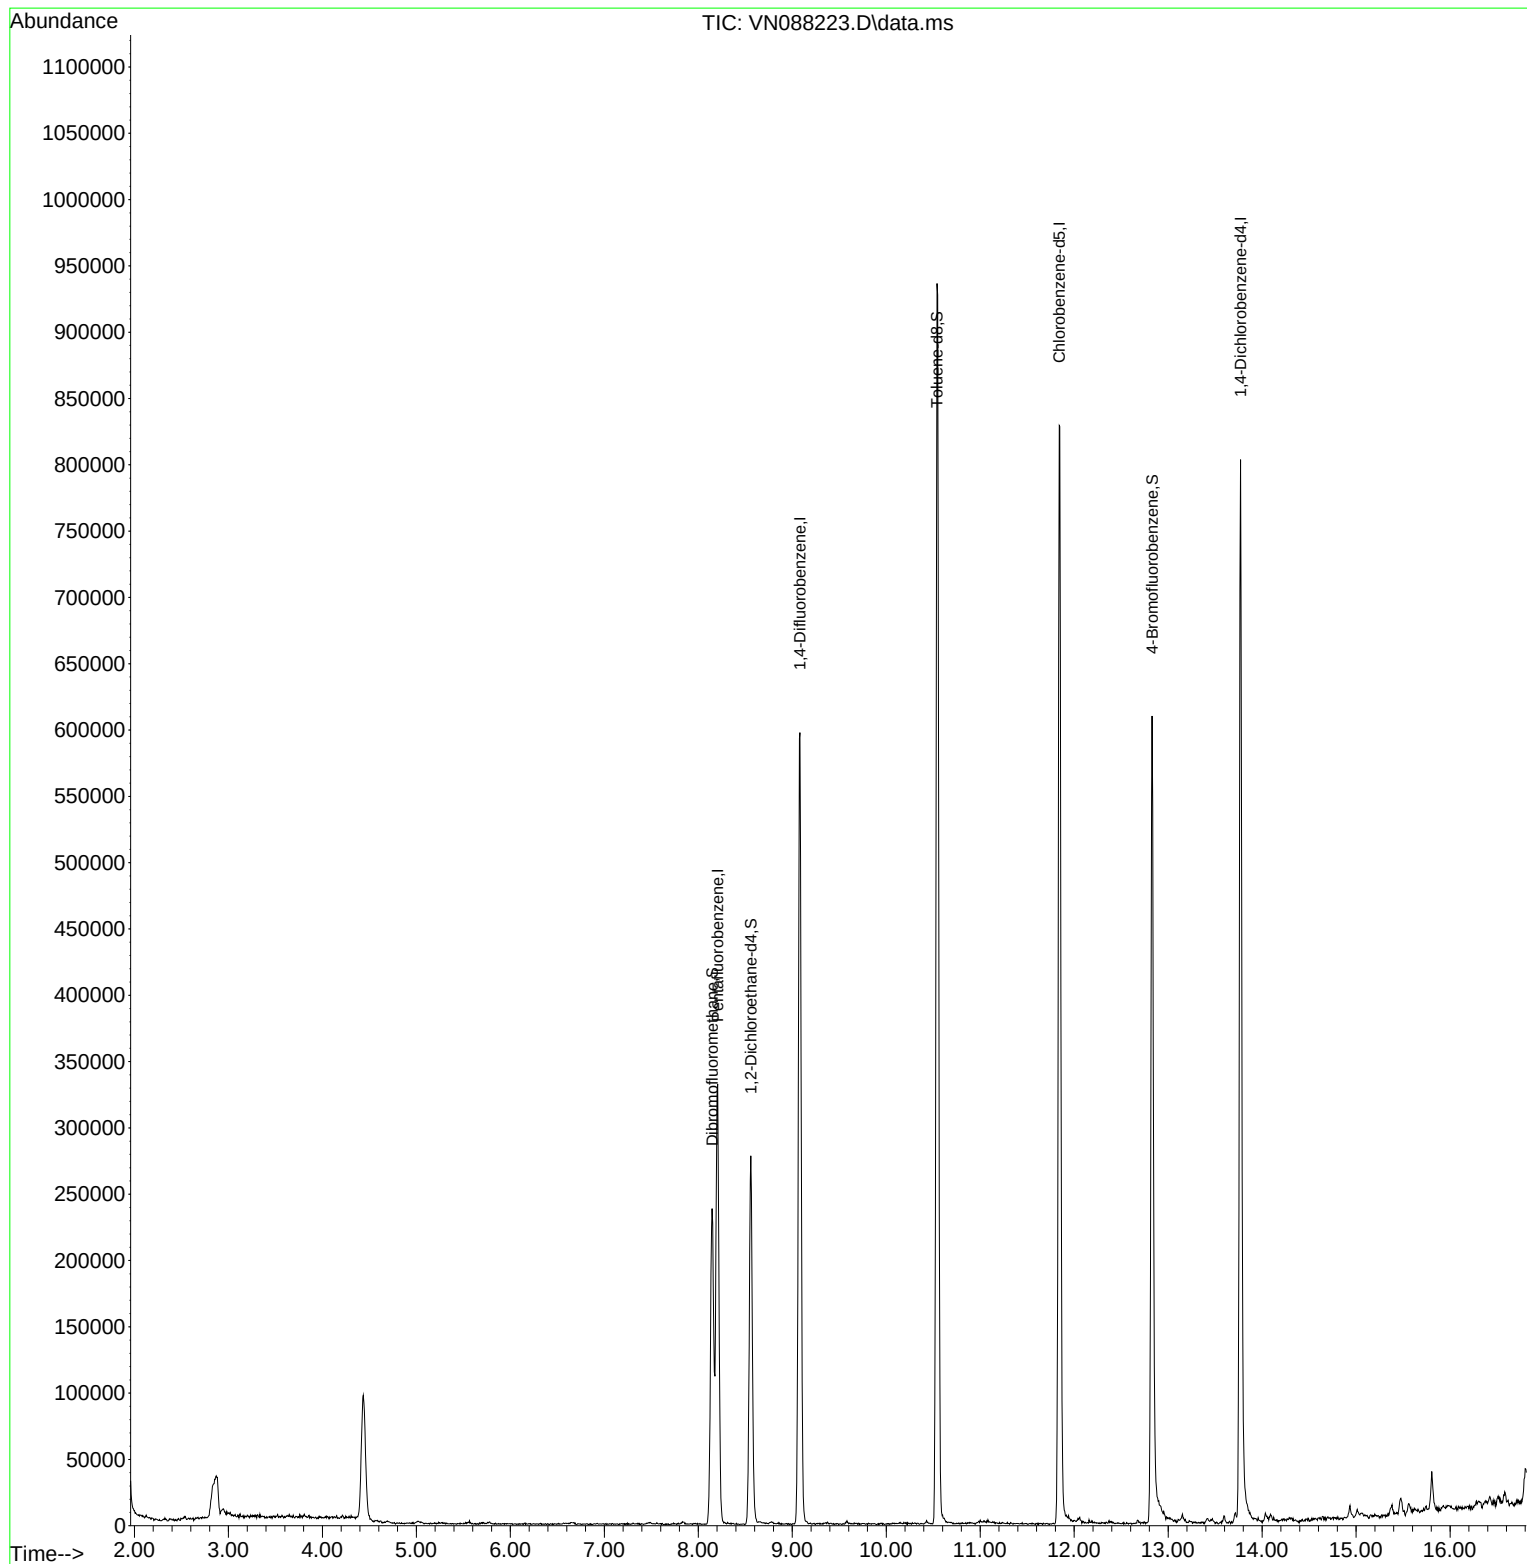


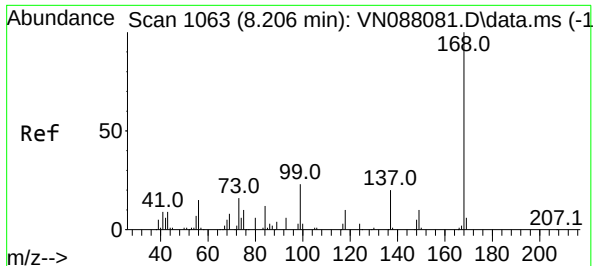

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.206 min Scan# 1063
Delta R.T. -0.000 min
Lab File: VN088223.D
Acq: 07 Nov 2025 10:39




Instrument :
MSVOA_N
ClientSampleId :
VN1107MBL01


Tgt Ion:168 Resp: 226952
Ion Ratio Lower Upper
168 100
99 67.0 57.2 85.8

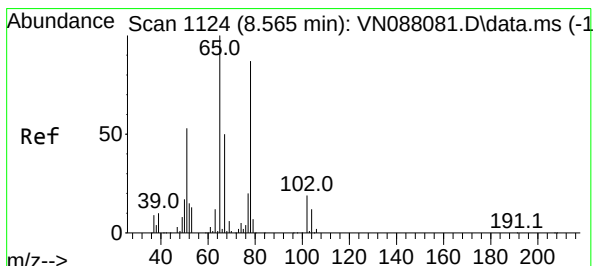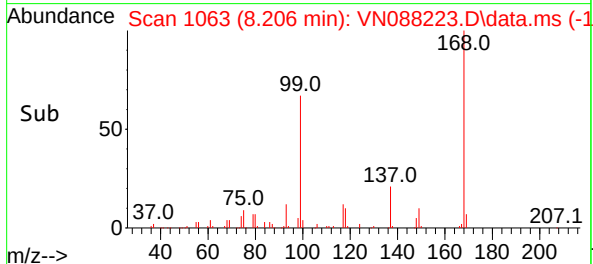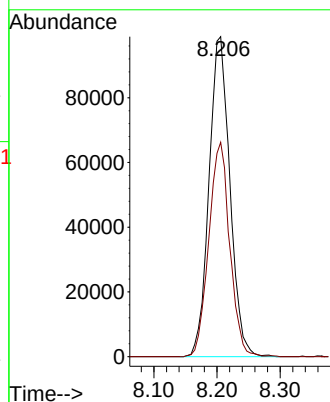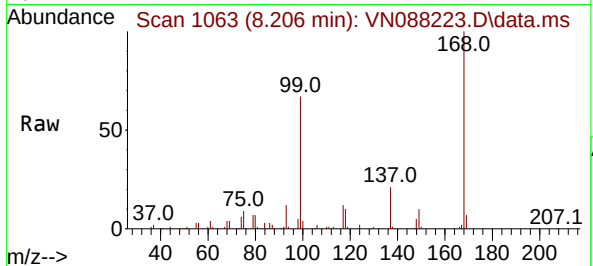

#33
1,2-Dichloroethane-d4
Concen: 58.033 ug/l
RT: 8.559 min Scan# 1123
Delta R.T. -0.000 min
Lab File: VN088223.D
Acq: 07 Nov 2025 10:39

Tgt Ion: 65 Resp: 227748
Ion Ratio Lower Upper
65 100
67 51.7 0.0 100.0

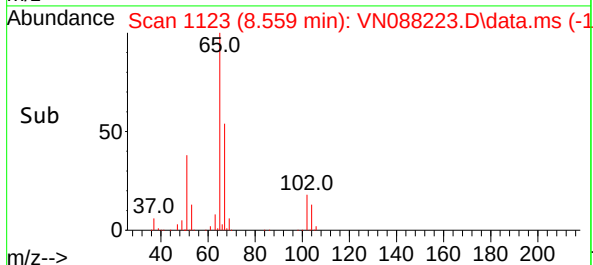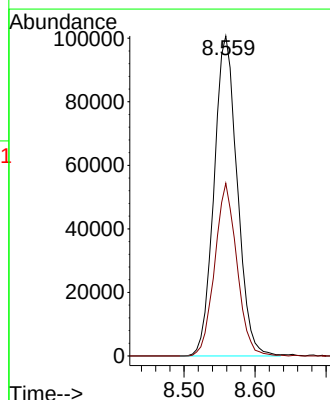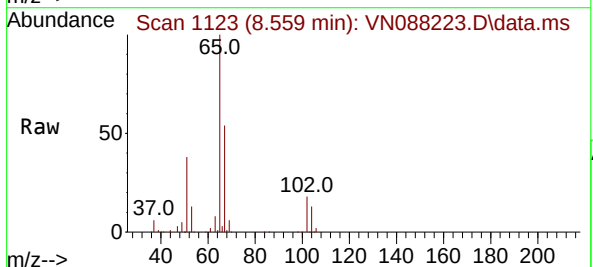

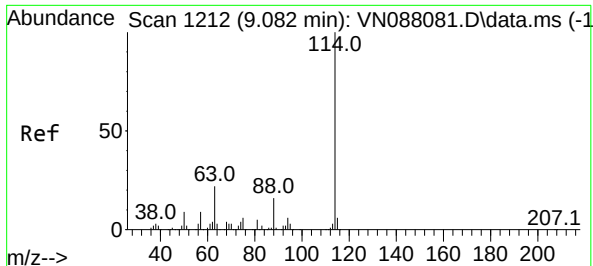

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.082 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN088223.D

Acq: 07 Nov 2025 10:39

Instrument :

MSVOA_N

ClientSampleId :

VN1107MBL01





Tgt Ion:114 Resp: 504591

Ion Ratio Lower Upper

114 100

63 23.2 0.0 45.2

88 15.7 0.0 33.4

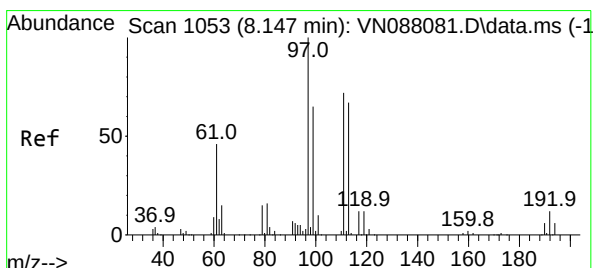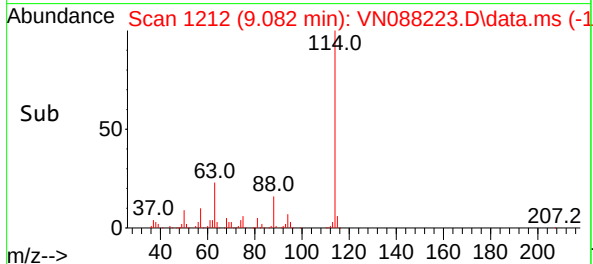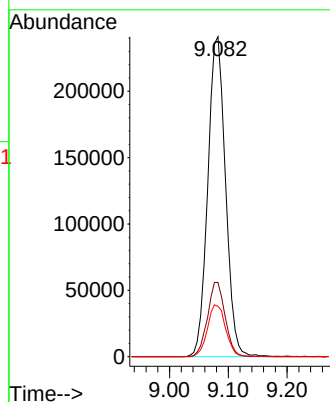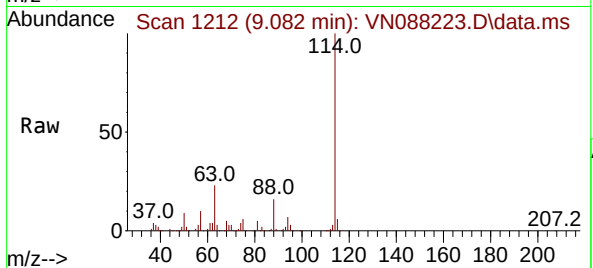

#35

Dibromofluoromethane

Concen: 51.172 ug/l

RT: 8.147 min Scan# 1053

Delta R.T. -0.006 min

Lab File: VN088223.D

Acq: 07 Nov 2025 10:39




Tgt Ion:113 Resp: 173465


Ion Ratio Lower Upper

113 100

111 102.3 82.8 124.2

192 16.7 12.8 19.2


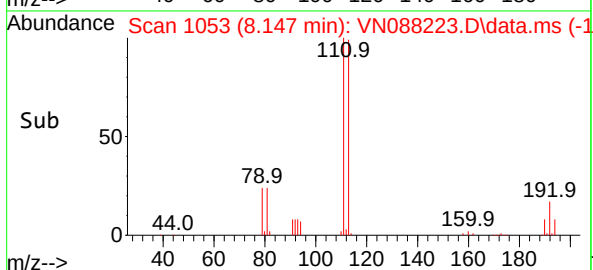
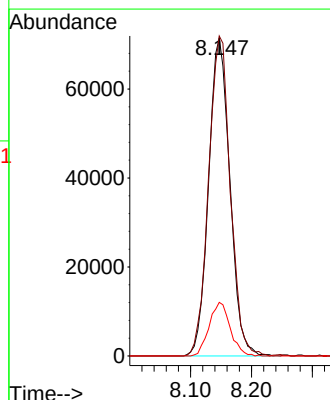
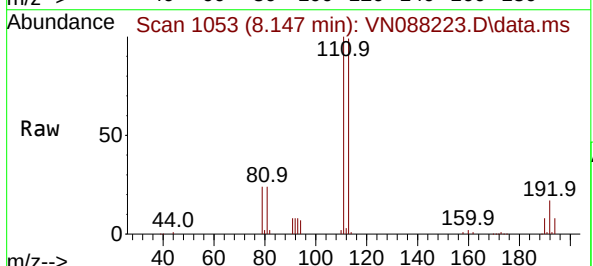


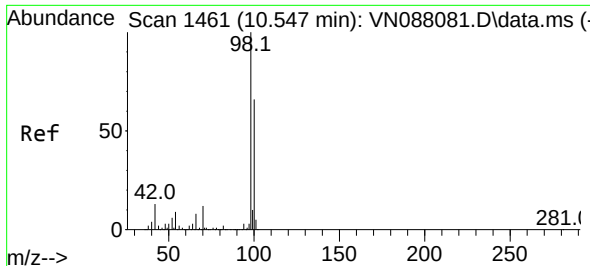

#50
Toluene-d8
Concen: 49.404 ug/l
RT: 10.541 min Scan# 1461
Delta R.T. -0.006 min
Lab File: VN088223.D
Acq: 07 Nov 2025 10:39




Instrument :
MSVOA_N
ClientSampleId :
VN1107MBL01


Tgt Ion: 98 Resp: 645304
Ion Ratio Lower Upper
98 100
100 65.0 52.8 79.2

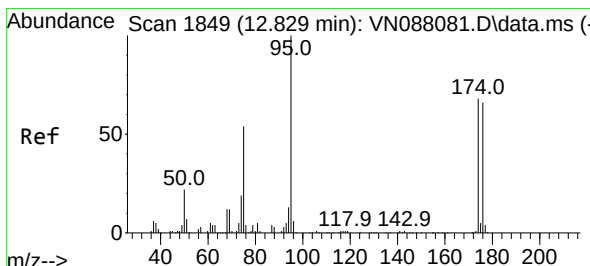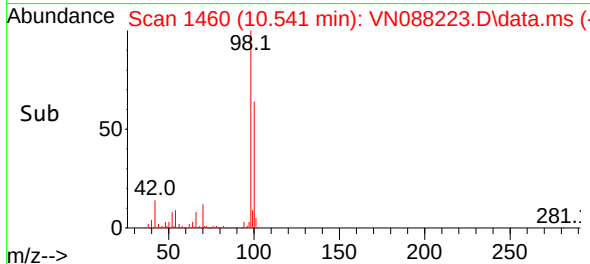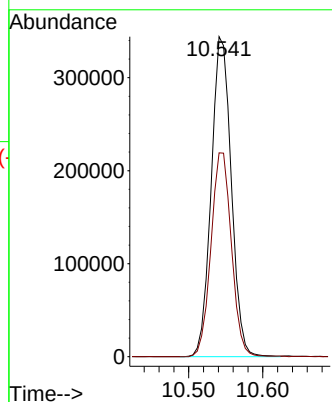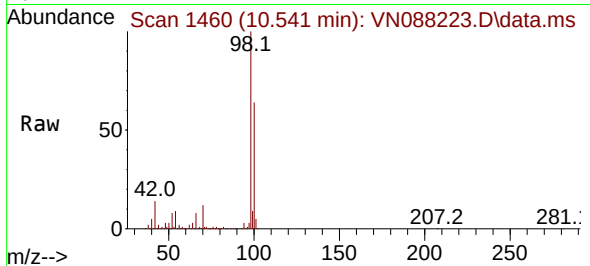

#62
4-Bromofluorobenzene
Concen: 51.697 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.006 min
Lab File: VN088223.D
Acq: 07 Nov 2025 10:39

Tgt Ion: 95 Resp: 238473
Ion Ratio Lower Upper
95 100
174 67.7 0.0 138.4
176 63.7 0.0 132.6


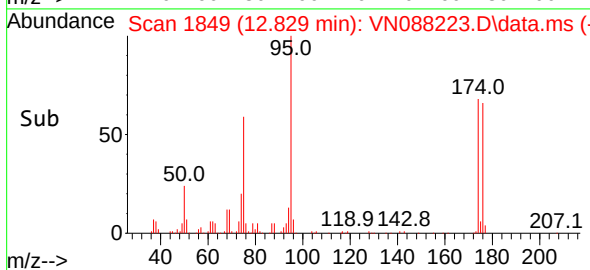
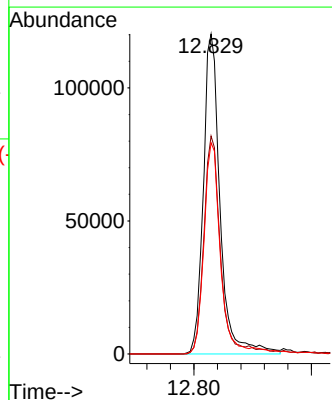
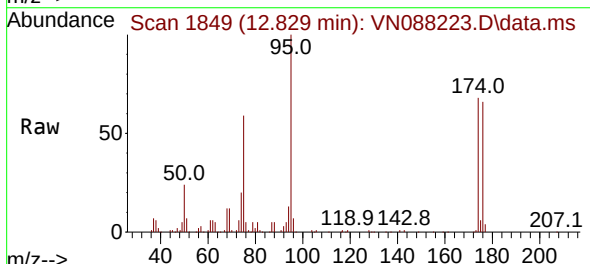


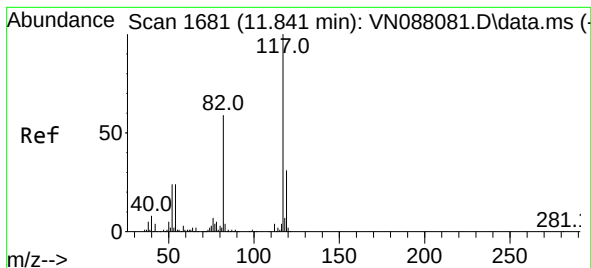

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.841 min Scan# 1
Delta R.T. -0.000 min
Lab File: VN088223.D
Acq: 07 Nov 2025 10:39

Instrument :
MSVOA_N
ClientSampleId :
VN1107MBL01

Tgt Ion:117 Resp: 469491
Ion Ratio Lower Upper
117 100
82 61.8 47.4 71.2
119 30.8 24.3 36.5

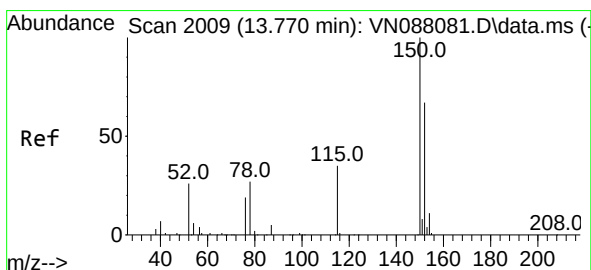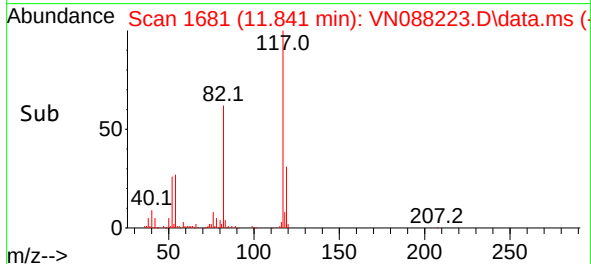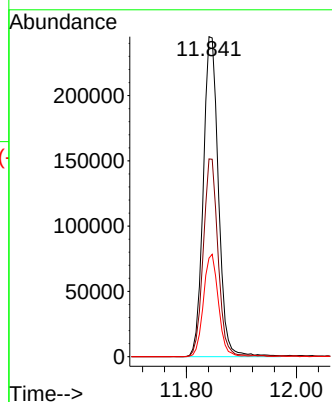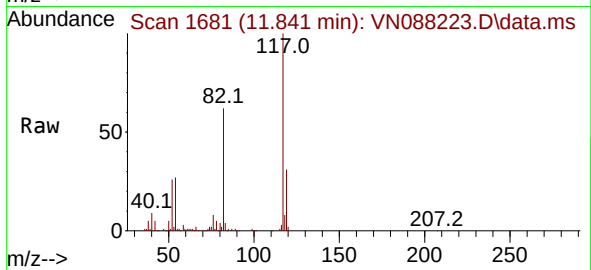

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.770 min Scan# 2009
Delta R.T. 0.006 min
Lab File: VN088223.D
Acq: 07 Nov 2025 10:39

Tgt Ion:152 Resp: 213204
Ion Ratio Lower Upper
152 100
115 66.9 32.3 96.8
150 161.2 0.0 351.0

