


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN110818\
Data File : VN052212.D
Acq On : 8 Nov 2018 9:12
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N110118W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Nov 02 05:39:38 2018

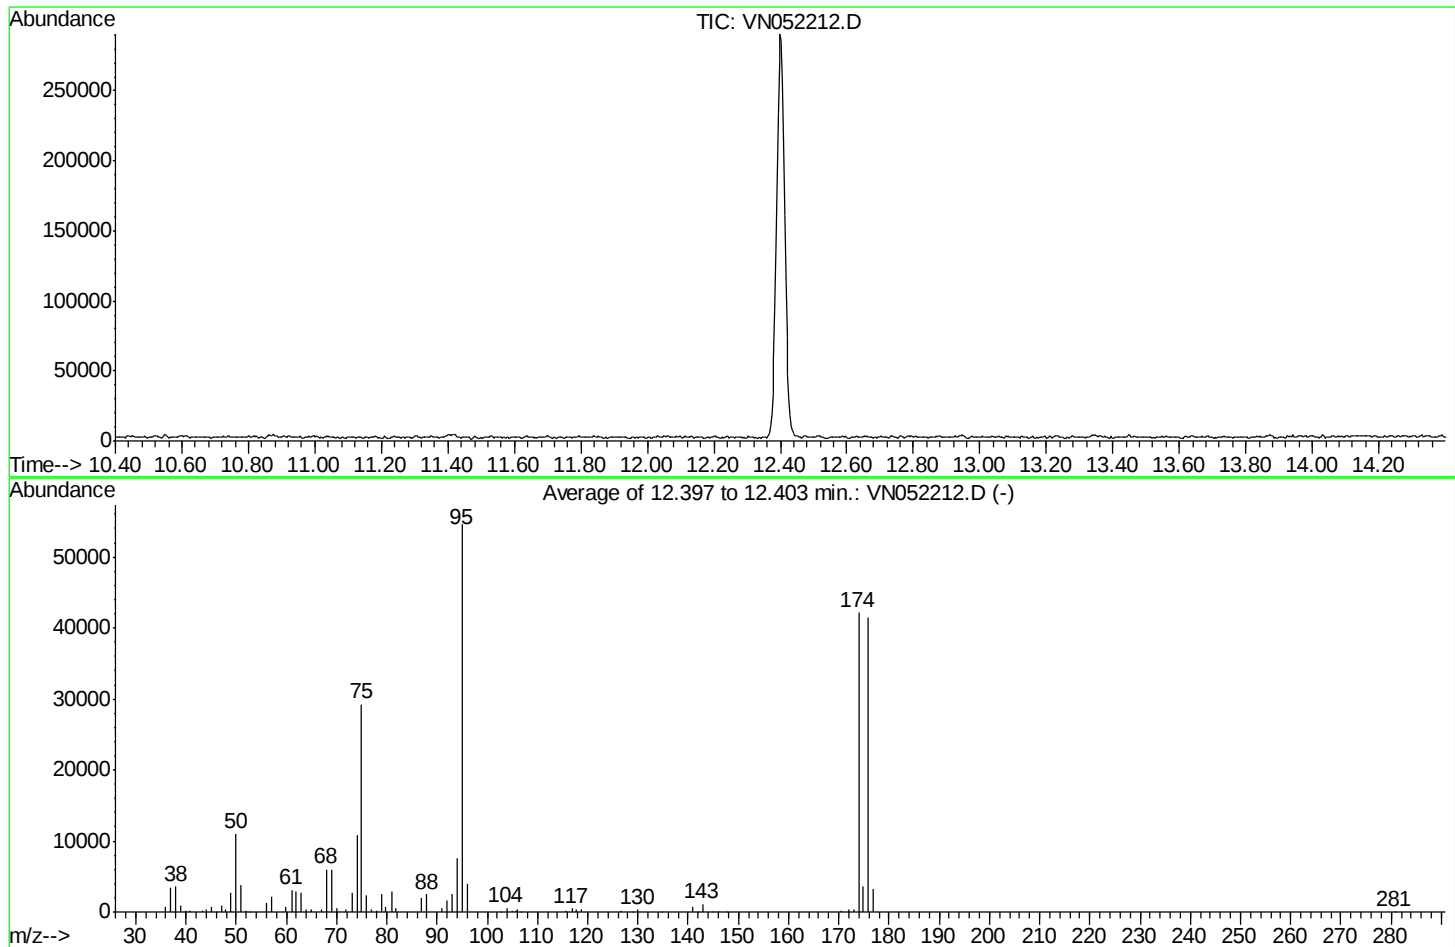

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	11030	PASS
75	95	30	60	53.6	29274	PASS
95	95	100	100	100.0	54592	PASS
96	95	5	9	7.4	4016	PASS
173	174	0.00	2	0.7	307	PASS
174	95	50	100	77.2	42144	PASS
175	174	5	9	8.5	3583	PASS
176	174	95	101	98.6	41552	PASS
177	176	5	9	7.9	3277	PASS