
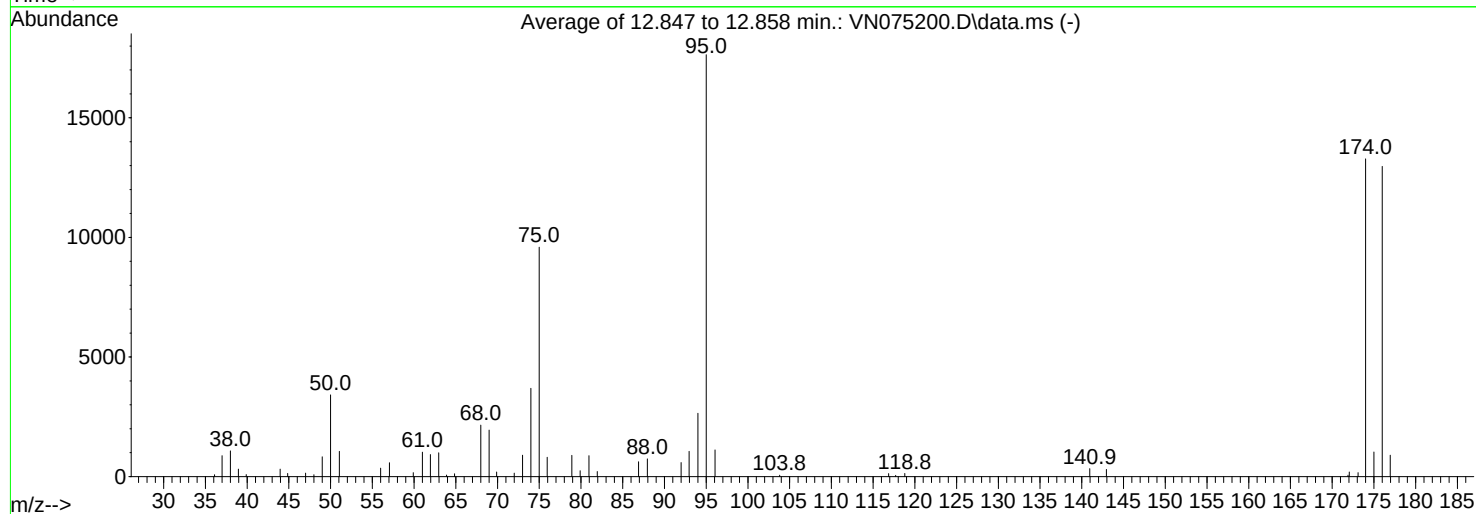


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110822\
Data File : VN075200.D
Acq On : 08 Nov 2022 09:33
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Title : SW846 8260
Last Update : Thu Oct 27 09:48:49 2022

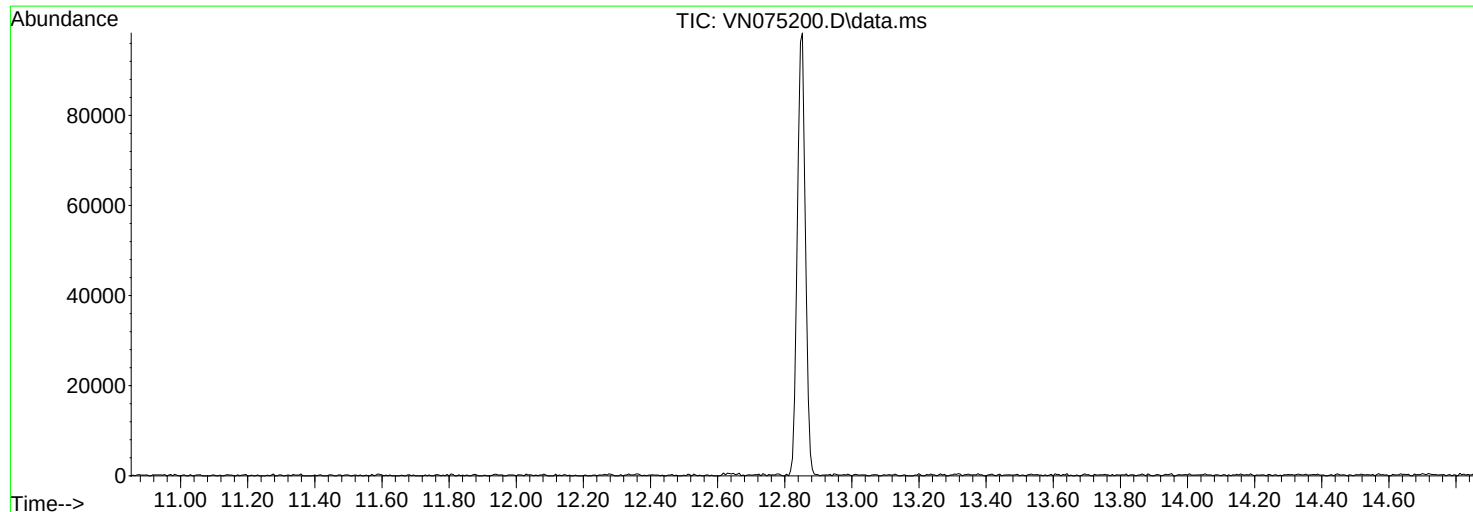

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	3415	PASS
75	95	30	60	54.4	9591	PASS
95	95	100	100	100.0	17633	PASS
96	95	5	9	6.3	1116	PASS
173	174	0.00	2	1.2	165	PASS
174	95	50	100	75.3	13278	PASS
175	174	5	9	7.7	1024	PASS
176	174	95	101	97.7	12966	PASS
177	176	5	9	6.9	892	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	78	51.05	1057	69.90	190	87.95	737
37.00	872	56.00	349	72.00	141	92.00	583
38.00	1077	57.05	577	73.00	893	92.95	1052
38.95	313	59.90	165	74.00	3688	94.00	2645
39.90	83	61.00	1020	75.00	9591	95.00	17633
43.95	309	61.95	919	75.95	807	96.05	1116
44.85	132	62.95	994	78.90	886	103.80	55
47.00	142	63.90	65	79.90	243	116.85	121
48.00	77	64.85	119	80.95	871	117.70	50
49.00	825	68.00	2148	81.95	208	118.80	133
50.00	3415	69.00	1941	86.90	621	140.95	334

Average of 12.847 to 12.858 min.: VN075200.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
142.95	299						
171.90	55						
172.05	194						
173.10	165						
174.00	13278						
175.00	1024						
176.00	12966						
176.95	892						

Instrument :

MSVOA_N

ClientSampleId :

BFB