

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110823\
 Data File : VN080011.D
 Acq On : 08 Nov 2023 23:31
 Operator : JC\MD
 Sample : 05283-04 10X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 14B-4

Quant Time: Nov 09 04:31:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N110823W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Thu Nov 09 04:02:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.818	128	67530	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.106	114	313884	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.870	117	296150	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.582	65	172181	30.374	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	101.233%
60) 4-Bromofluorobenzene	12.853	95	114497	24.176	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	80.600%
63) Toluene-d8	10.570	98	402826	28.707	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	95.700%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110823\
Data File : VN080011.D
Acq On : 08 Nov 2023 23:31
Operator : JC\MD
Sample : 05283-04 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
14B-4

Quant Time: Nov 09 04:31:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N110823W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Thu Nov 09 04:02:05 2023
Response via : Initial Calibration




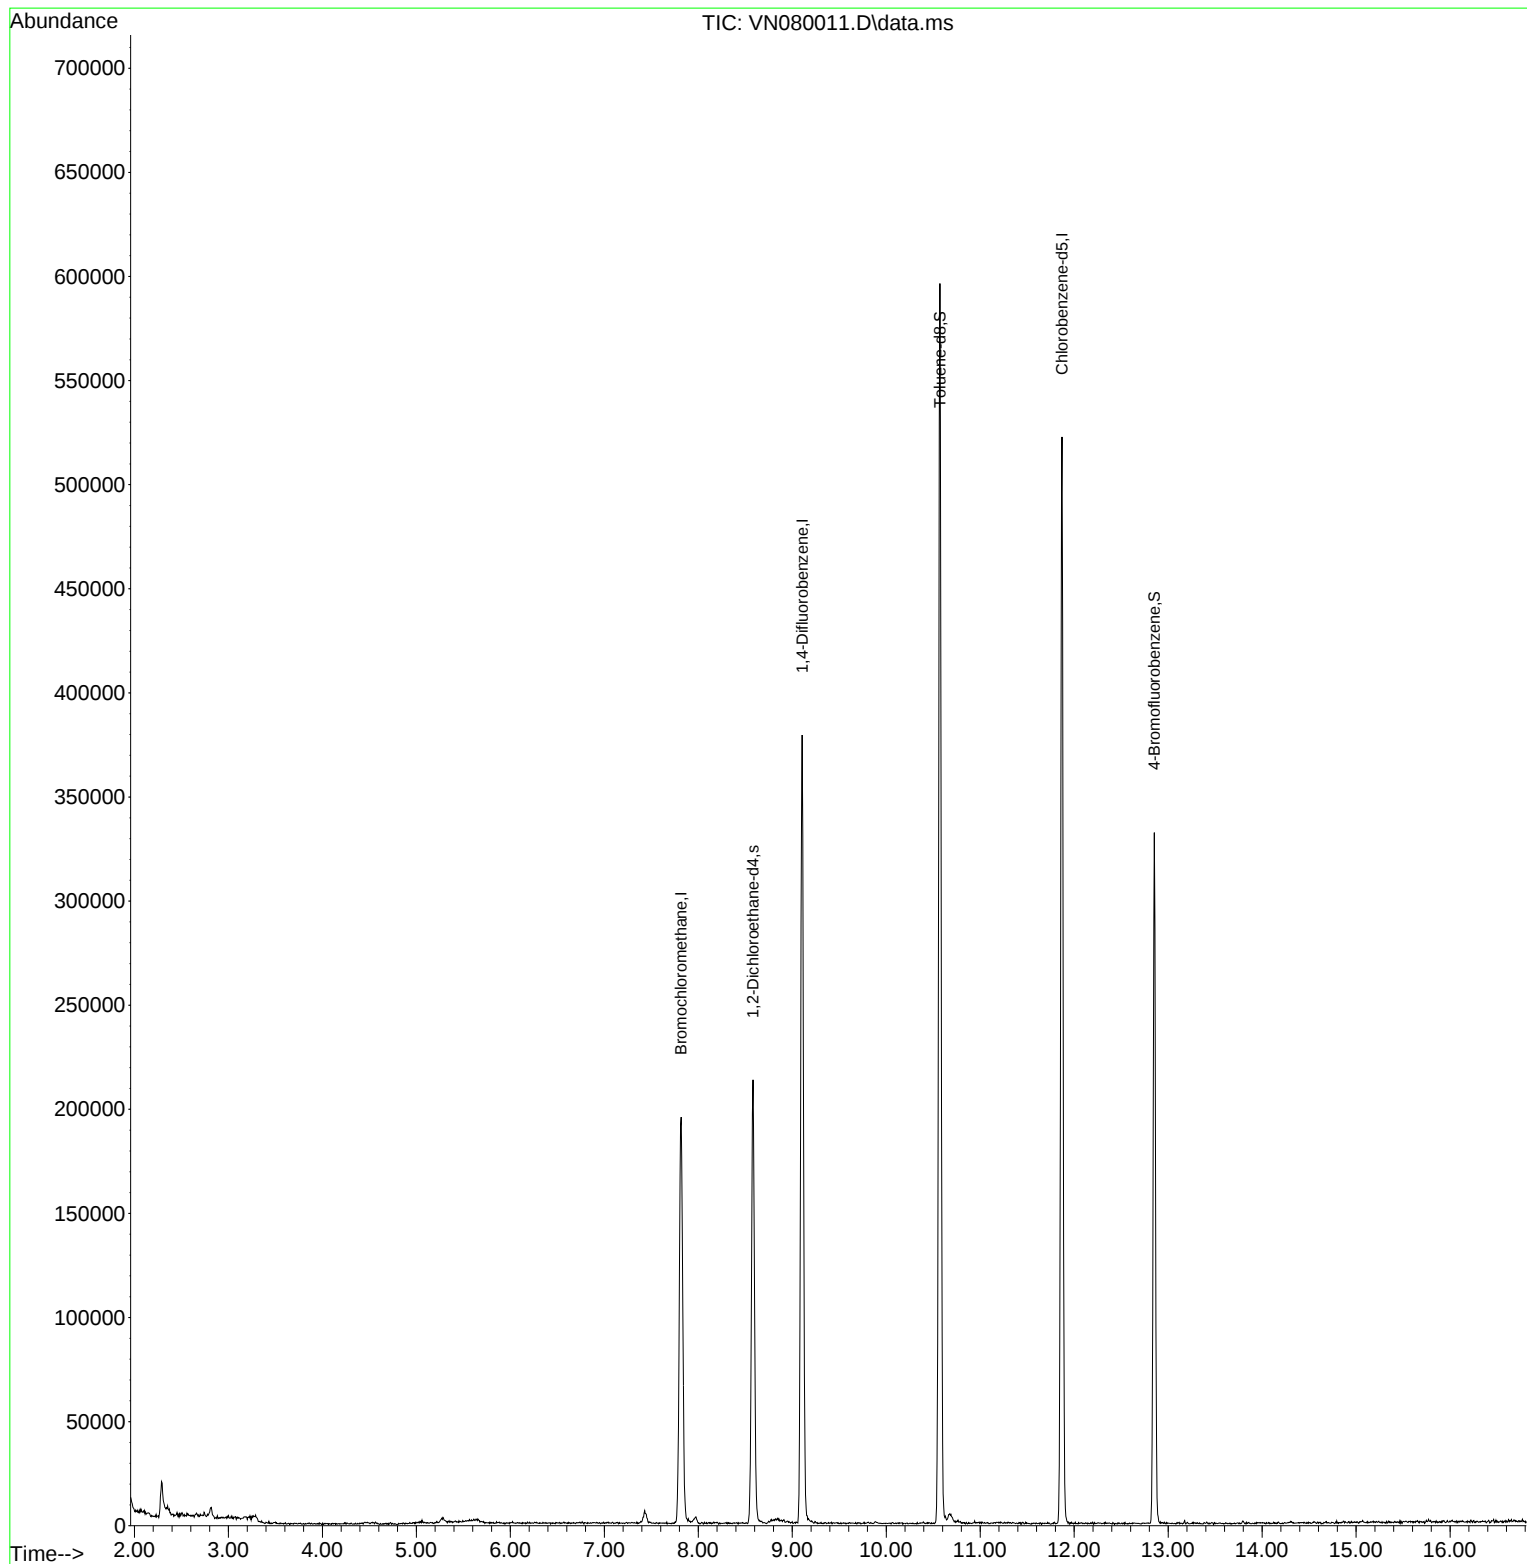


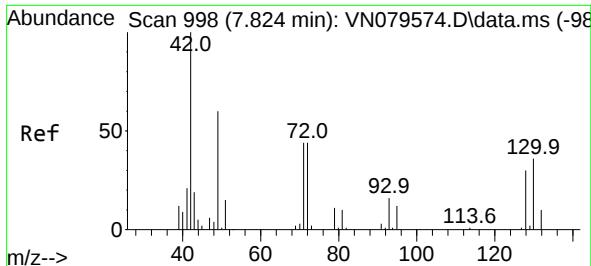

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.818 min Scan# 997
Delta R.T. -0.006 min
Lab File: VN080011.D
Acq: 08 Nov 2023 23:31




Instrument :
MSVOA_N
ClientSampleId :
14B-4


Tgt Ion:128 Resp: 67530
Ion Ratio Lower Upper
128 100
49 178.8 0.0 468.5
130 130.1 0.0 320.7

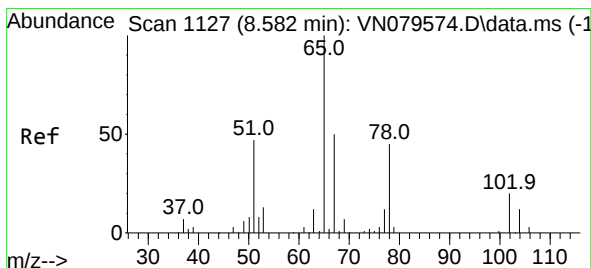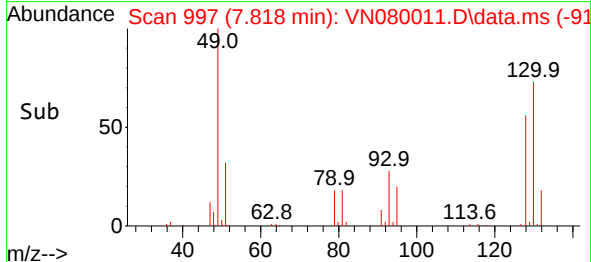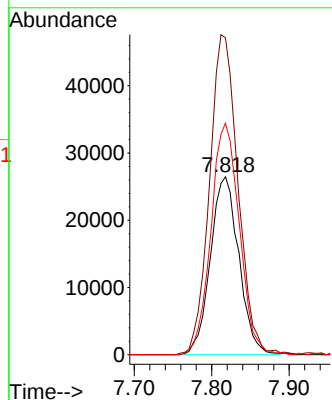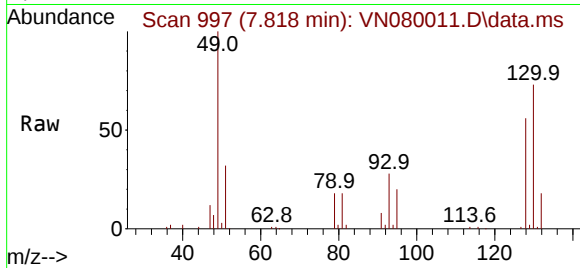

#27
1,2-Dichloroethane-d4
Concen: 30.374 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VN080011.D
Acq: 08 Nov 2023 23:31

Tgt Ion: 65 Resp: 172181
Ion Ratio Lower Upper
65 100
67 51.3 42.1 63.1

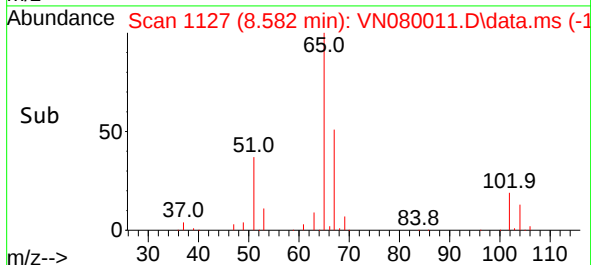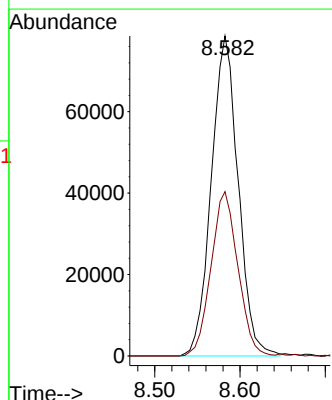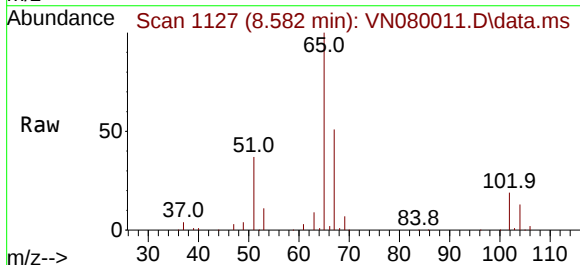

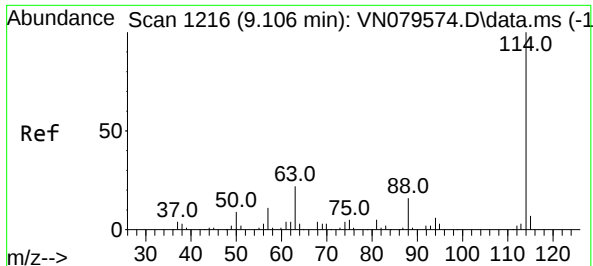

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 9.106 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN080011.D

Acq: 08 Nov 2023 23:31

Instrument :

MSVOA_N

ClientSampleId :

14B-4





Tgt Ion:114 Resp: 313884

Ion Ratio Lower Upper

114 100

63 22.2 18.1 27.1

88 16.3 12.2 18.2

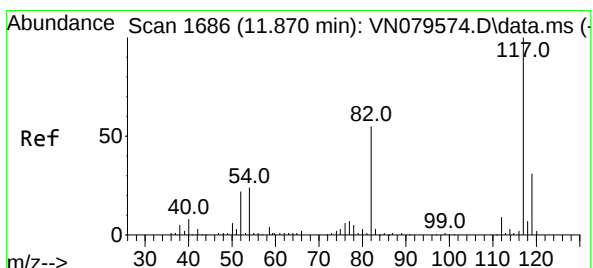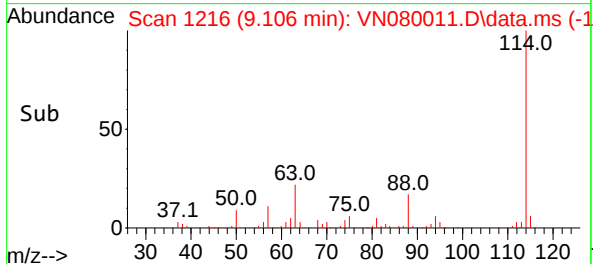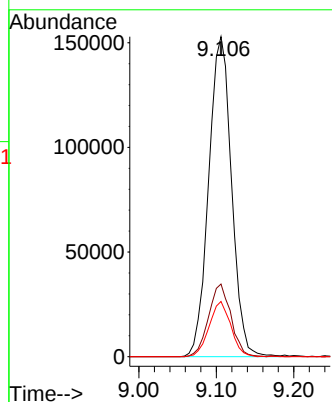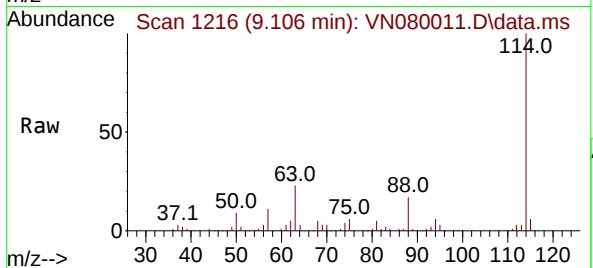

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 11.870 min Scan# 1686

Delta R.T. 0.000 min

Lab File: VN080011.D

Acq: 08 Nov 2023 23:31




Tgt Ion:117 Resp: 296150


Ion Ratio Lower Upper

117 100

82 58.4 46.2 69.2

119 32.0 25.2 37.8


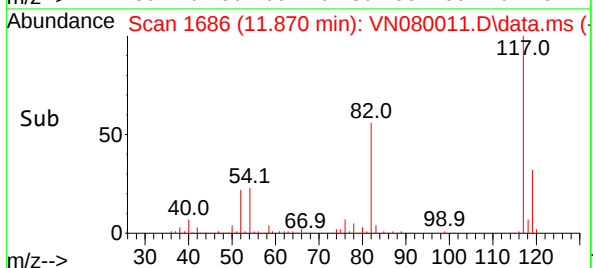
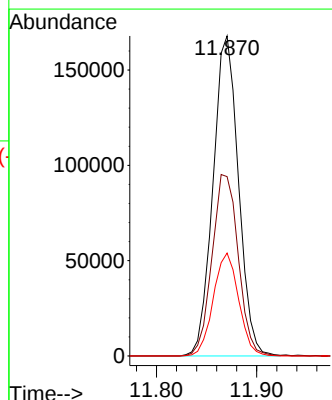
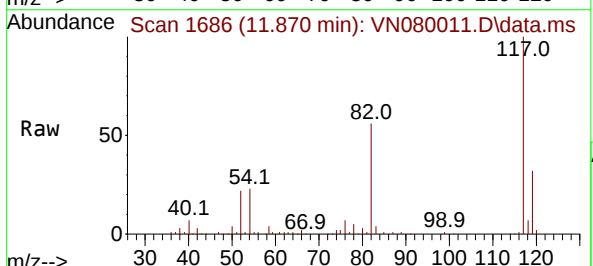


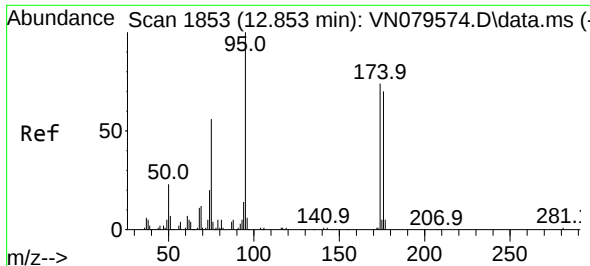

#60
4-Bromofluorobenzene
Concen: 24.176 ug/l
RT: 12.853 min Scan# 114497
Delta R.T. -0.000 min
Lab File: VN080011.D
Acq: 08 Nov 2023 23:31

Instrument :
MSVOA_N
ClientSampleId :
14B-4

Tgt Ion: 95 Resp: 114497
Ion Ratio Lower Upper
95 100
174 72.1 60.5 90.7
176 69.5 57.2 85.8

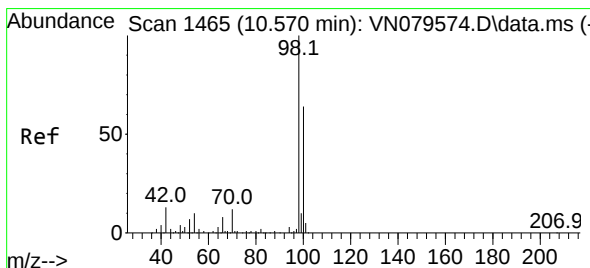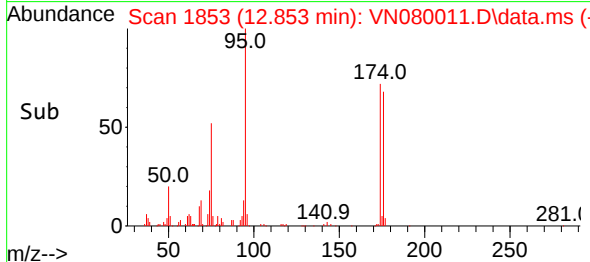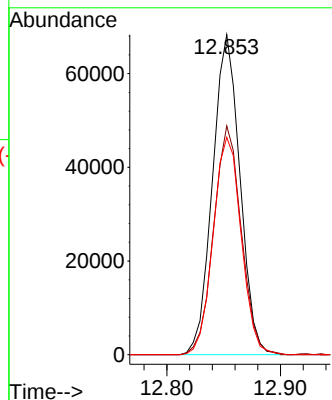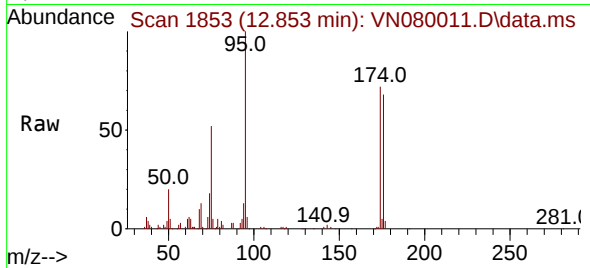

#63
Toluene-d8
Concen: 28.707 ug/l
RT: 10.570 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN080011.D
Acq: 08 Nov 2023 23:31

Tgt Ion: 98 Resp: 402826
Ion Ratio Lower Upper
98 100
100 64.0 51.6 77.4

