


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110823\
 Data File : VN079994.D
 Acq On : 08 Nov 2023 16:26
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N110823W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Nov 09 04:02:05 2023

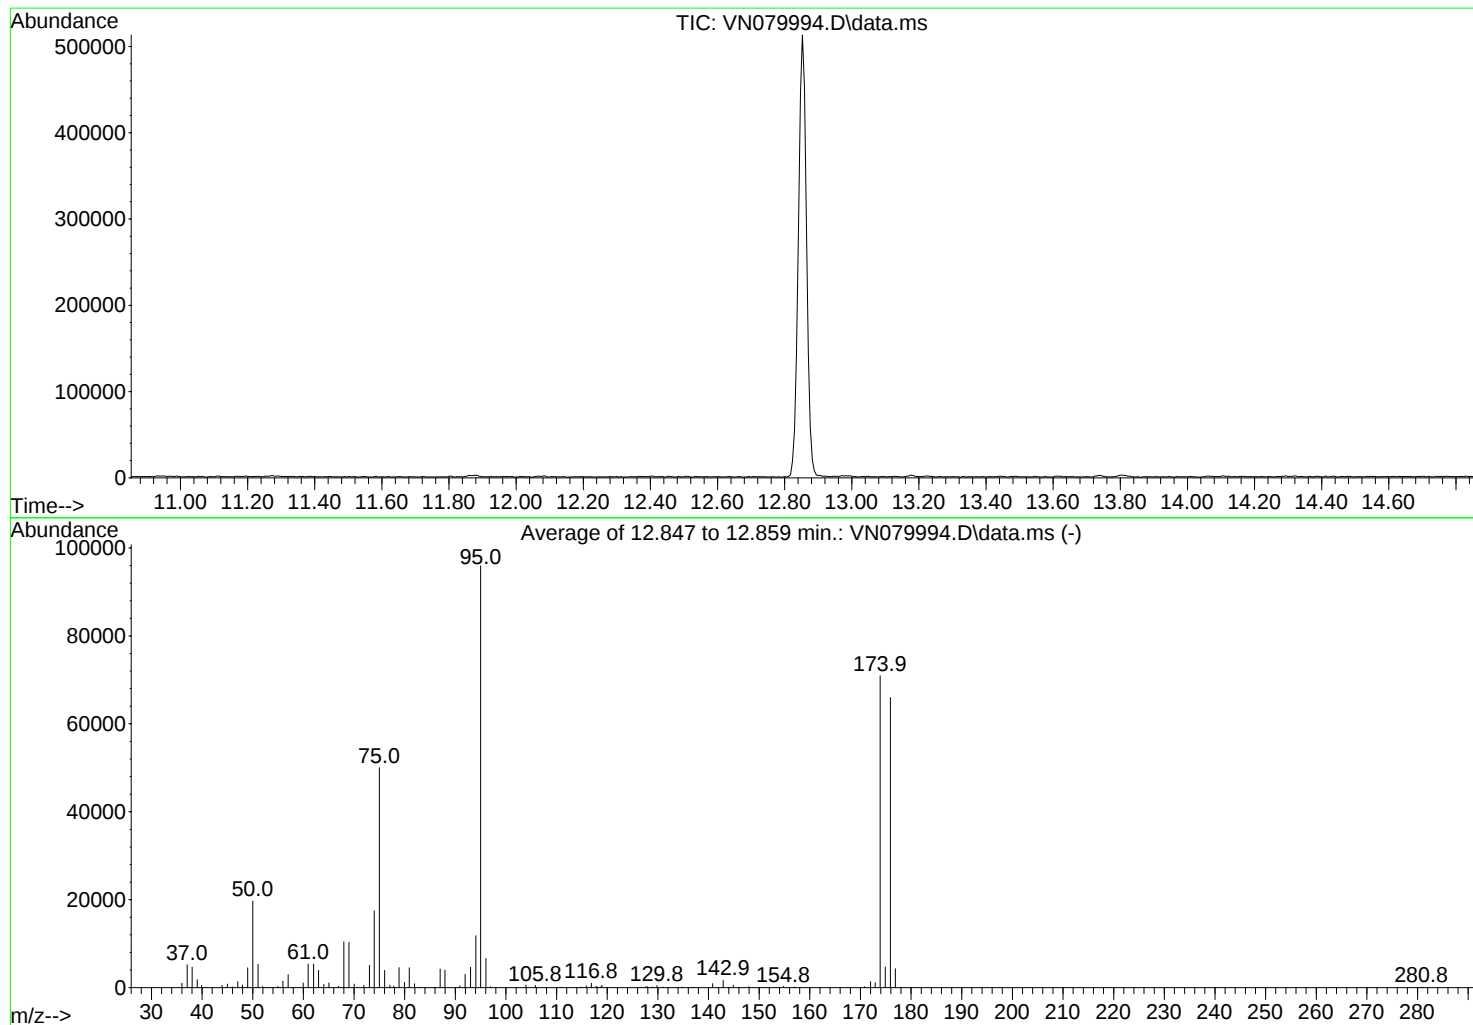

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	19704	PASS
75	95	30	60	52.1	50029	PASS
95	95	100	100	100.0	95933	PASS
96	95	5	9	6.9	6636	PASS
173	174	0.00	2	1.6	1123	PASS
174	95	50	100	73.9	70931	PASS
175	174	5	9	6.6	4697	PASS
176	174	95	101	93.0	65963	FAIL*
177	176	5	9	6.5	4300	PASS