

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110824\
 Data File : VN084739.D
 Acq On : 08 Nov 2024 10:44
 Operator : JC\MD
 Sample : VN1108WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1108WBL01

Quant Time: Nov 08 22:26:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 31 18:45:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.218	168	170398	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	297081	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	255691	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	113797	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	119910	48.722	ug/l	0.00
Spiked Amount	50.000	Range 74 - 125	Recovery	=	97.440%	
35) Dibromofluoromethane	8.159	113	98292	48.880	ug/l	0.00
Spiked Amount	50.000	Range 75 - 124	Recovery	=	97.760%	
50) Toluene-d8	10.565	98	337837	45.608	ug/l	0.00
Spiked Amount	50.000	Range 86 - 113	Recovery	=	91.220%	
62) 4-Bromofluorobenzene	12.847	95	127156	45.931	ug/l	0.00
Spiked Amount	50.000	Range 77 - 121	Recovery	=	91.860%	


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110824\
Data File : VN084739.D
Acq On : 08 Nov 2024 10:44
Operator : JC\MD
Sample : VN1108WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1108WBL01


Quant Time: Nov 08 22:26:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 31 18:45:38 2024
Response via : Initial Calibration

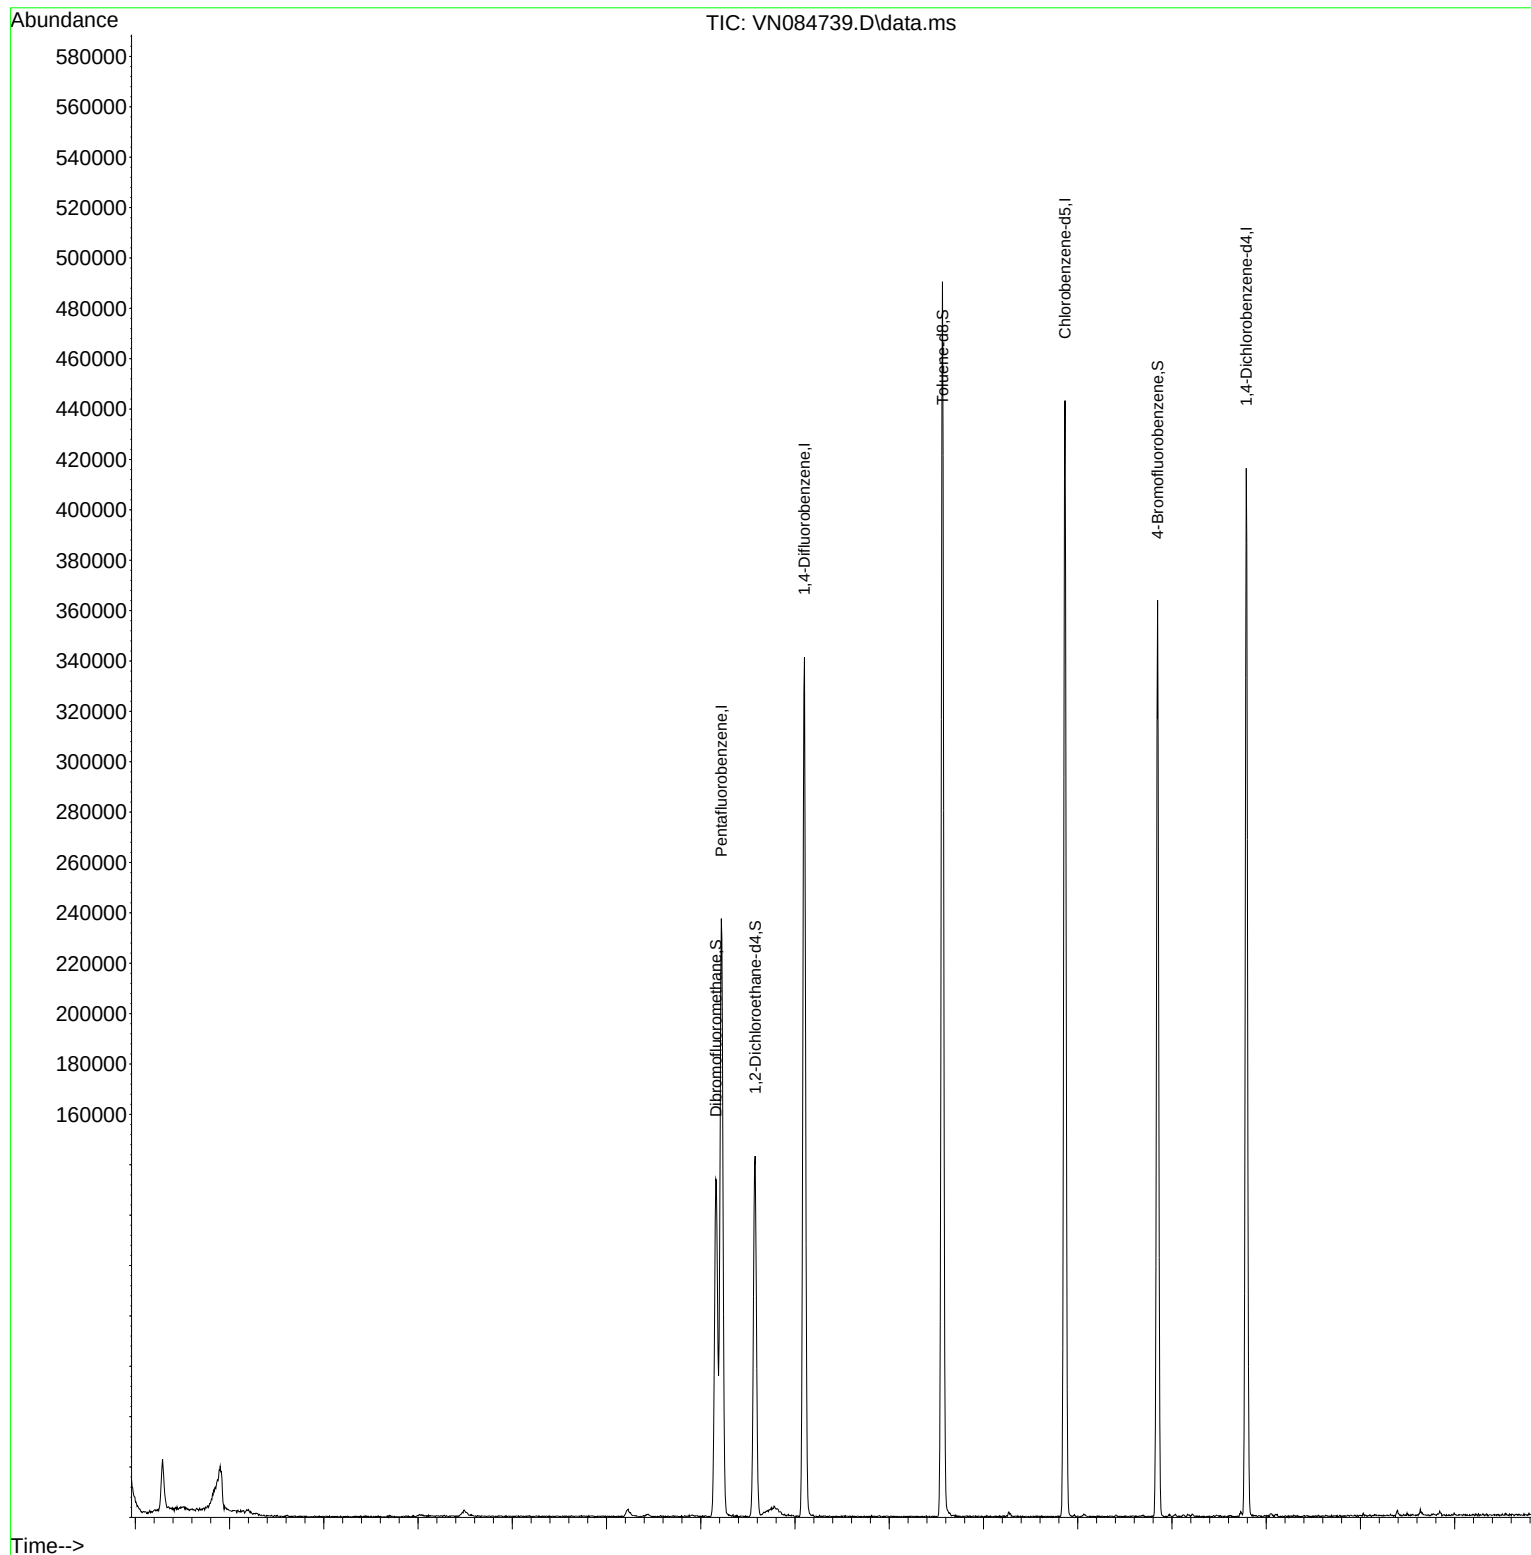



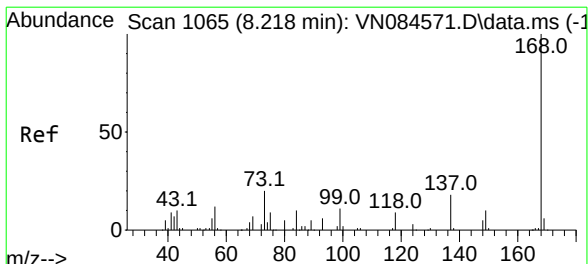


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.006 min
Lab File: VN084739.D
Acq: 08 Nov 2024 10:44

Instrument :
MSVOA_N
ClientSampleId :
VN1108WBL01



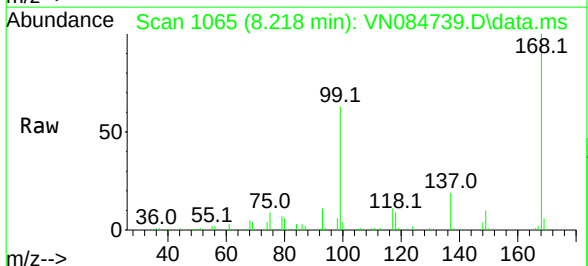



Tgt Ion:168 Resp: 170398
Ion Ratio Lower Upper
168 100
99 63.3 54.2 81.2

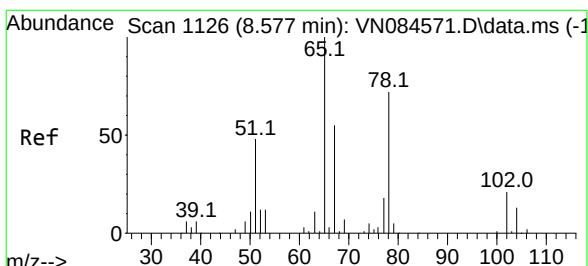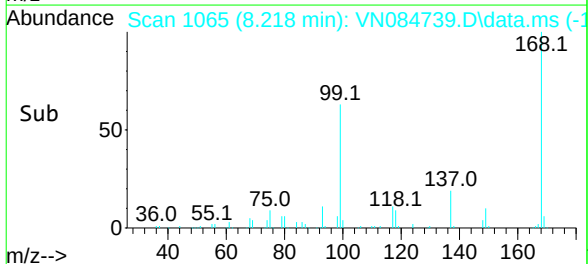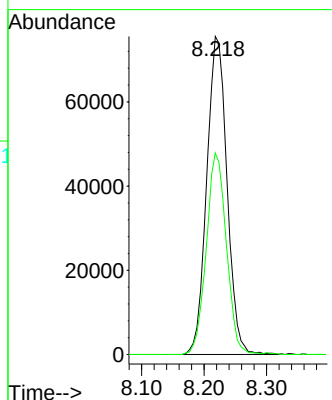

#33
1,2-Dichloroethane-d4
Concen: 48.722 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN084739.D
Acq: 08 Nov 2024 10:44

Tgt Ion: 65 Resp: 119910
Ion Ratio Lower Upper
65 100
67 51.4 0.0 102.0


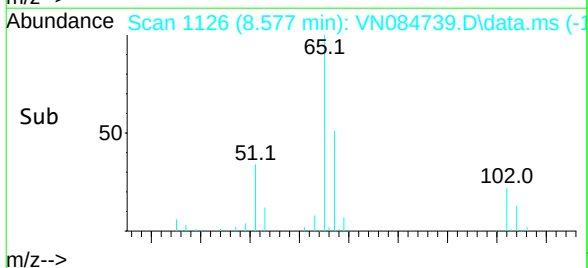
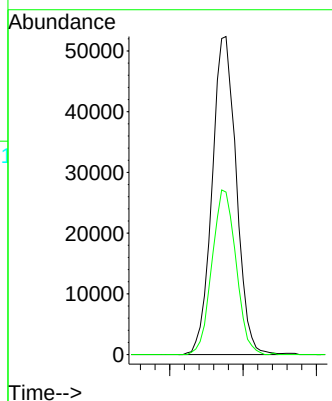
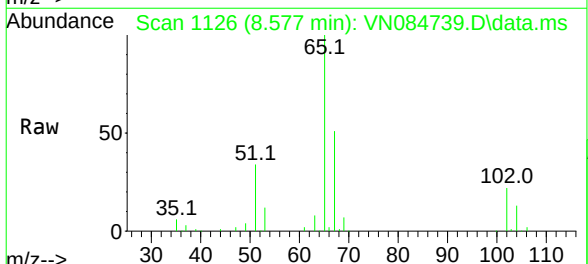


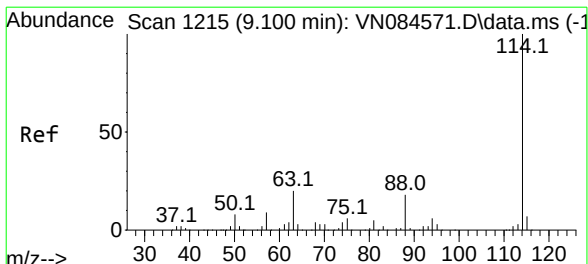

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 9.100 min Scan# 12
 Delta R.T. 0.000 min
 Lab File: VN084739.D
 Acq: 08 Nov 2024 10:44




Instrument :
 MSVOA_N
 ClientSampleId :
 VN1108WBL01


Tgt Ion:	114	Resp:	297081
Ion	Ratio	Lower	Upper
114	100		
63	19.2	0.0	43.8
88	15.3	0.0	31.6

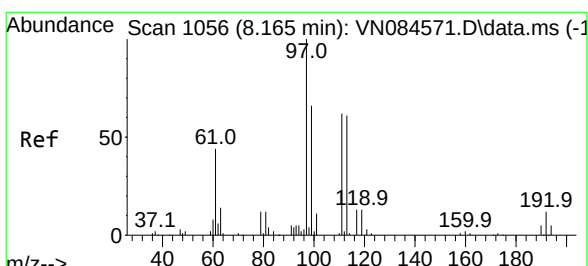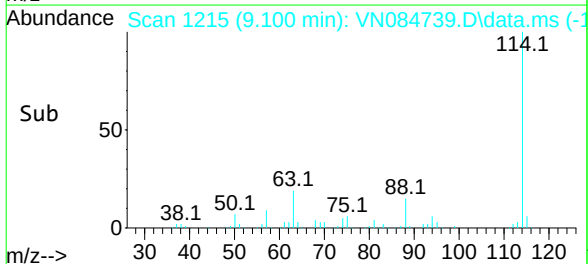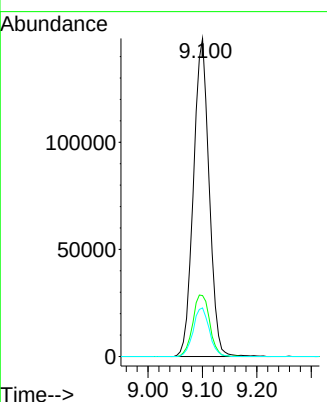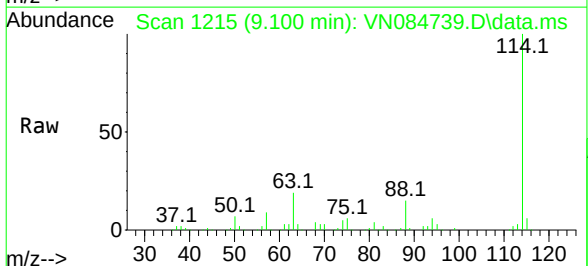

#35
 Dibromofluoromethane
 Concen: 48.880 ug/l
 RT: 8.159 min Scan# 1055
 Delta R.T. -0.006 min
 Lab File: VN084739.D
 Acq: 08 Nov 2024 10:44

Tgt Ion:	113	Resp:	98292
Ion	Ratio	Lower	Upper
113	100		
111	101.9	83.3	124.9
192	18.7	13.5	20.3

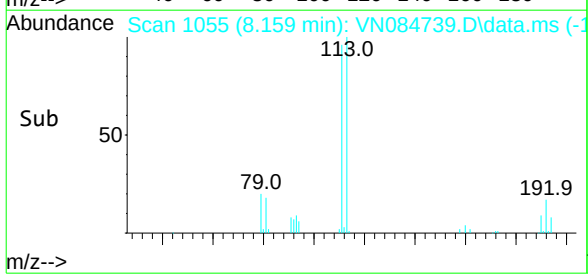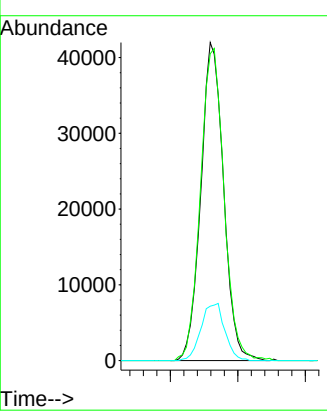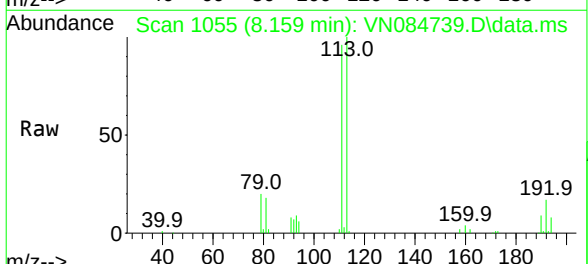

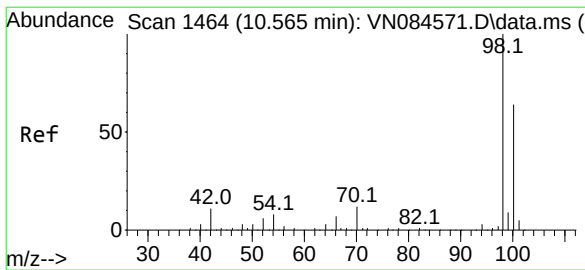

#50

Toluene-d8

Concen: 45.608 ug/l

RT: 10.565 min Scan# 1464

Delta R.T. -0.000 min

Lab File: VN084739.D

Acq: 08 Nov 2024 10:44

Instrument :

MSVOA_N

ClientSampleId :





VN1108WBL01

Tgt Ion: 98 Resp: 337837

Ion Ratio Lower Upper

98 100

100 64.9 52.7 79.1

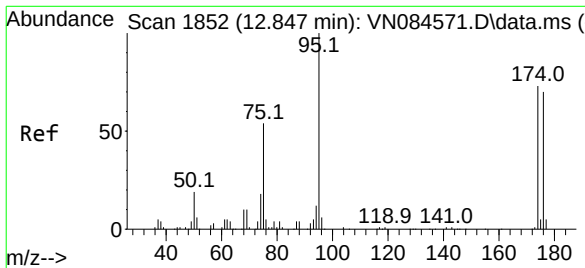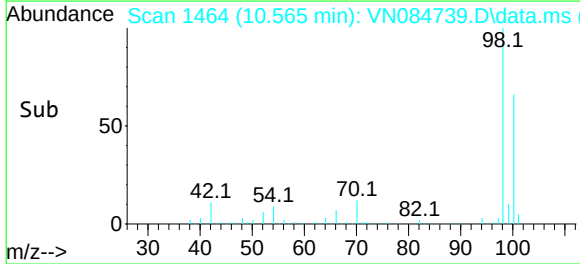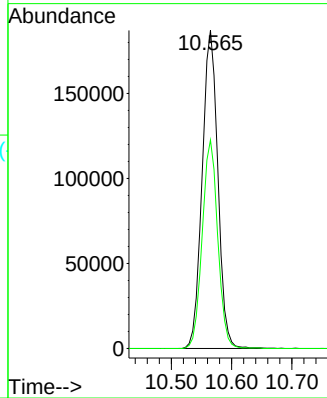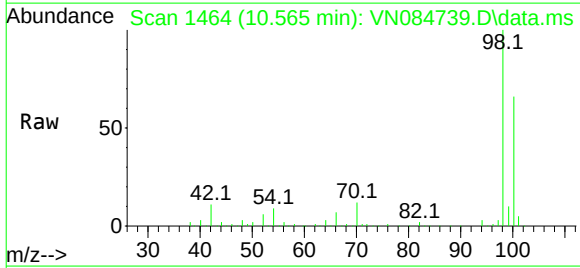

#62

4-Bromofluorobenzene

Concen: 45.931 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. 0.000 min

Lab File: VN084739.D

Acq: 08 Nov 2024 10:44




Tgt Ion: 95 Resp: 127156


Ion Ratio Lower Upper

95 100

174 76.6 0.0 145.2

176 70.9 0.0 140.0


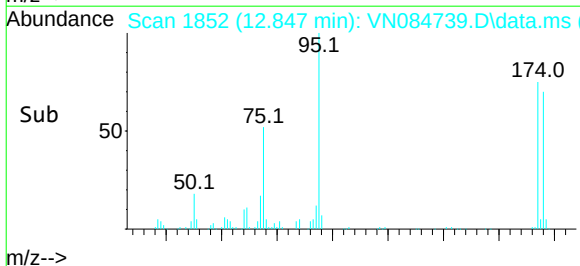
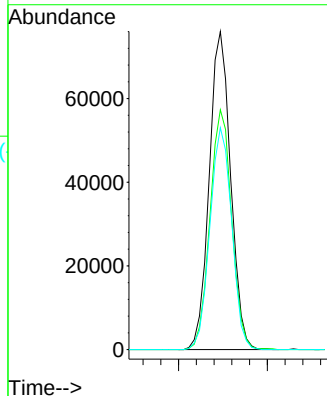
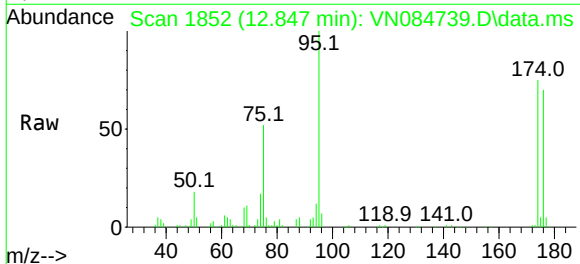


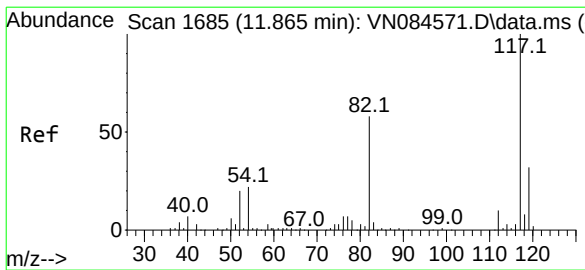

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN084739.D
Acq: 08 Nov 2024 10:44

Instrument :
MSVOA_N
ClientSampleId :
VN1108WBL01

Tgt Ion:	117	Resp:	255691
Ion	Ratio	Lower	Upper
117	100		
82	55.2	47.2	70.8
119	32.5	25.4	38.0

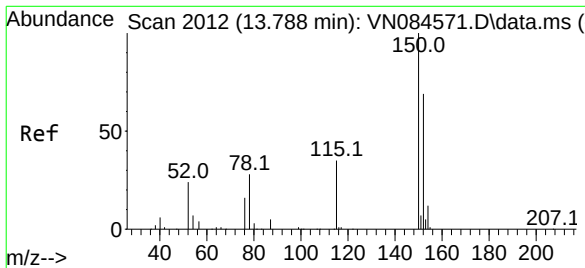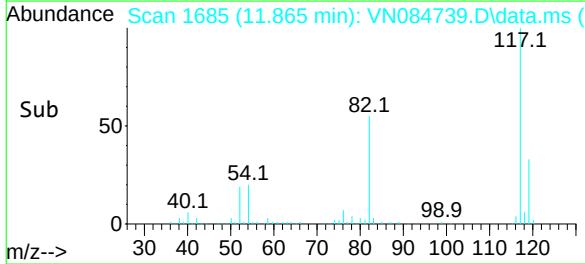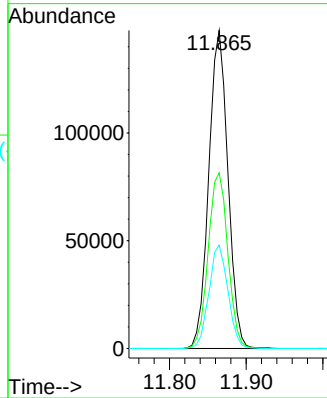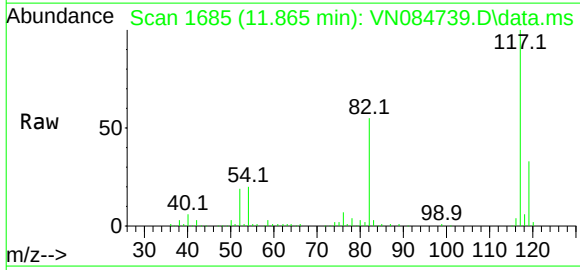

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. 0.000 min
Lab File: VN084739.D
Acq: 08 Nov 2024 10:44

Tgt Ion:	152	Resp:	113797
Ion	Ratio	Lower	Upper
152	100		
115	61.9	31.3	93.9
150	158.3	0.0	349.8

