


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN110918\
Data File : VN052223.D
Acq On : 9 Nov 2018 13:01
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110918W.M
Title : SW846 8260
Last Update : Mon Nov 12 00:34:27 2018

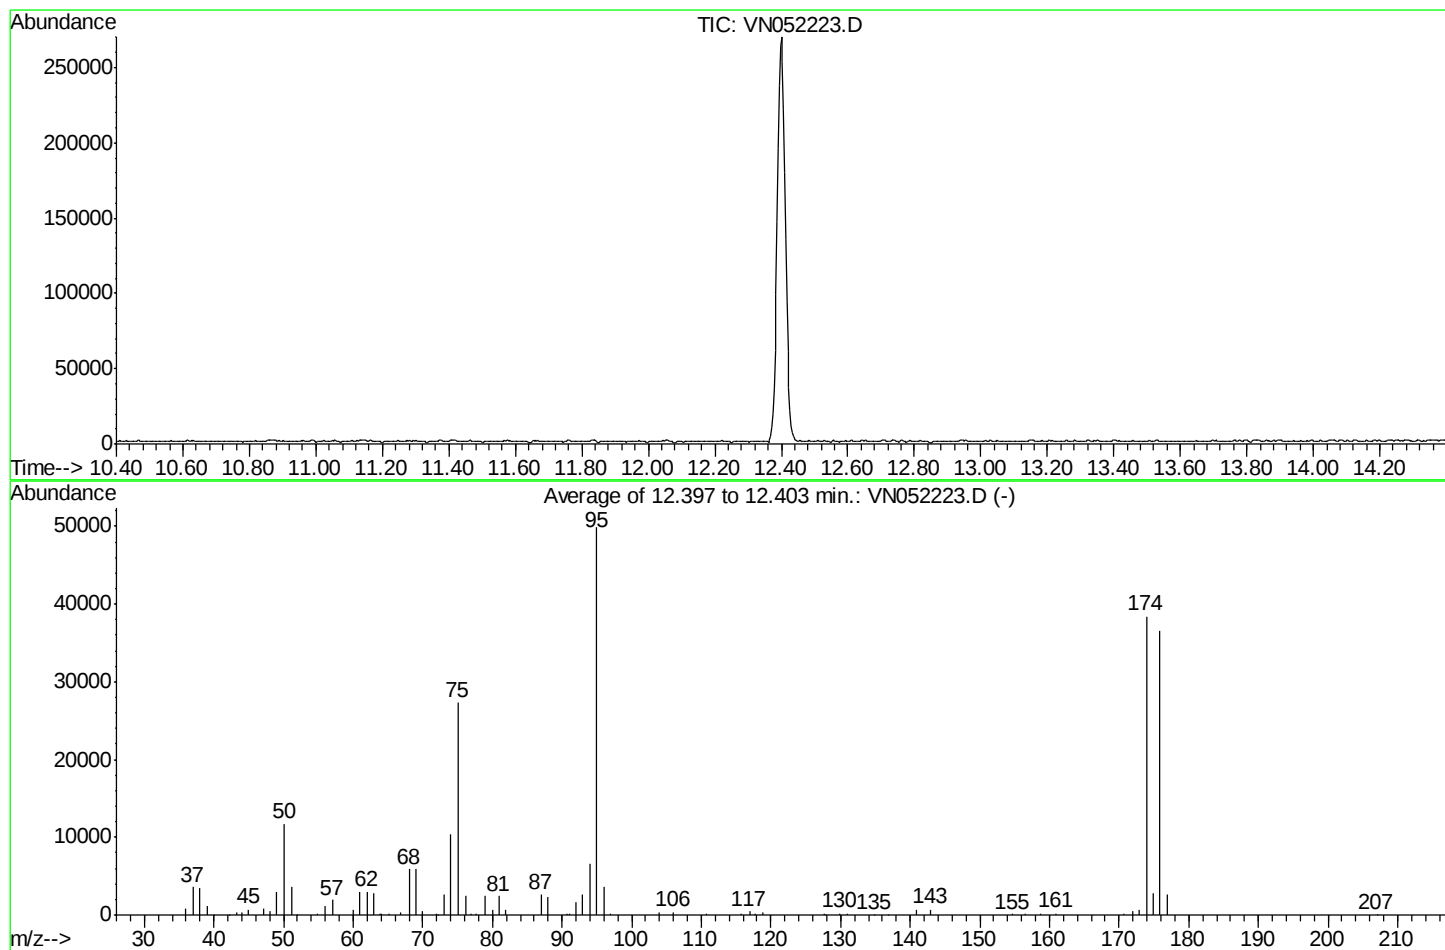

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	11722	PASS
75	95	30	60	54.7	27280	PASS
95	95	100	100	100.0	49882	PASS
96	95	5	9	7.1	3557	PASS
173	174	0.00	2	1.6	626	PASS
174	95	50	100	77.1	38442	PASS
175	174	5	9	7.3	2792	PASS
176	174	95	101	95.3	36645	PASS
177	176	5	9	7.3	2676	PASS