


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN110920\
Data File : VN064502.D
Acq On : 9 Nov 2020 9:35
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N110920W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Mon Nov 09 13:16:36 2020

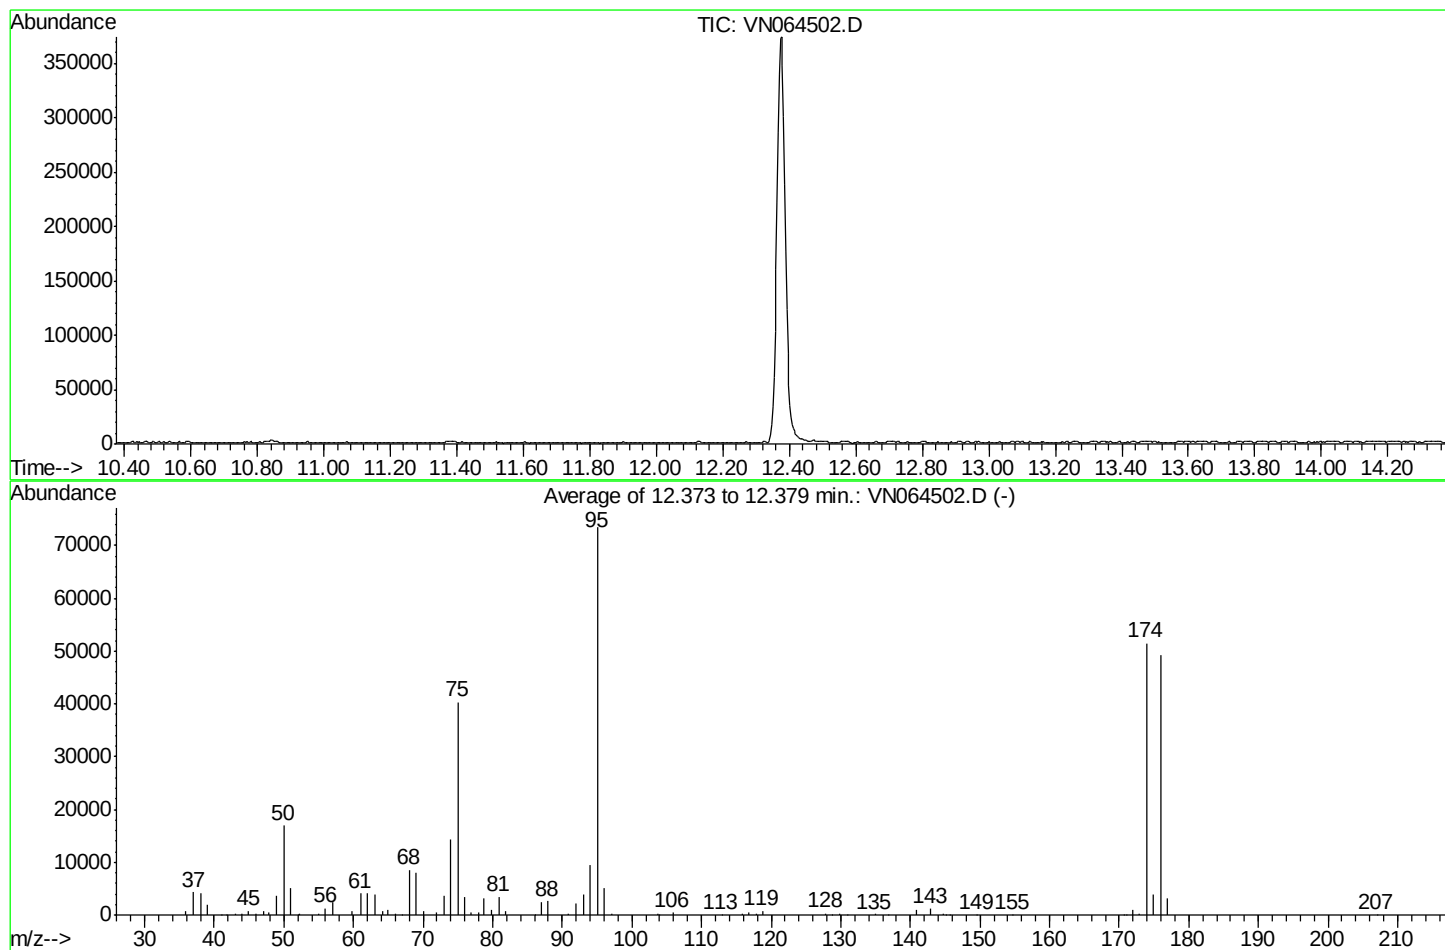

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	16973	PASS
75	95	30	60	54.8	40288	PASS
95	95	100	100	100.0	73472	PASS
96	95	5	9	6.9	5035	PASS
173	174	0.00	2	0.5	280	PASS
174	95	50	100	70.0	51445	PASS
175	174	5	9	7.6	3912	PASS
176	174	95	101	95.6	49162	PASS
177	176	5	9	6.7	3274	PASS