


Dibromochloromethane

Response Ratio

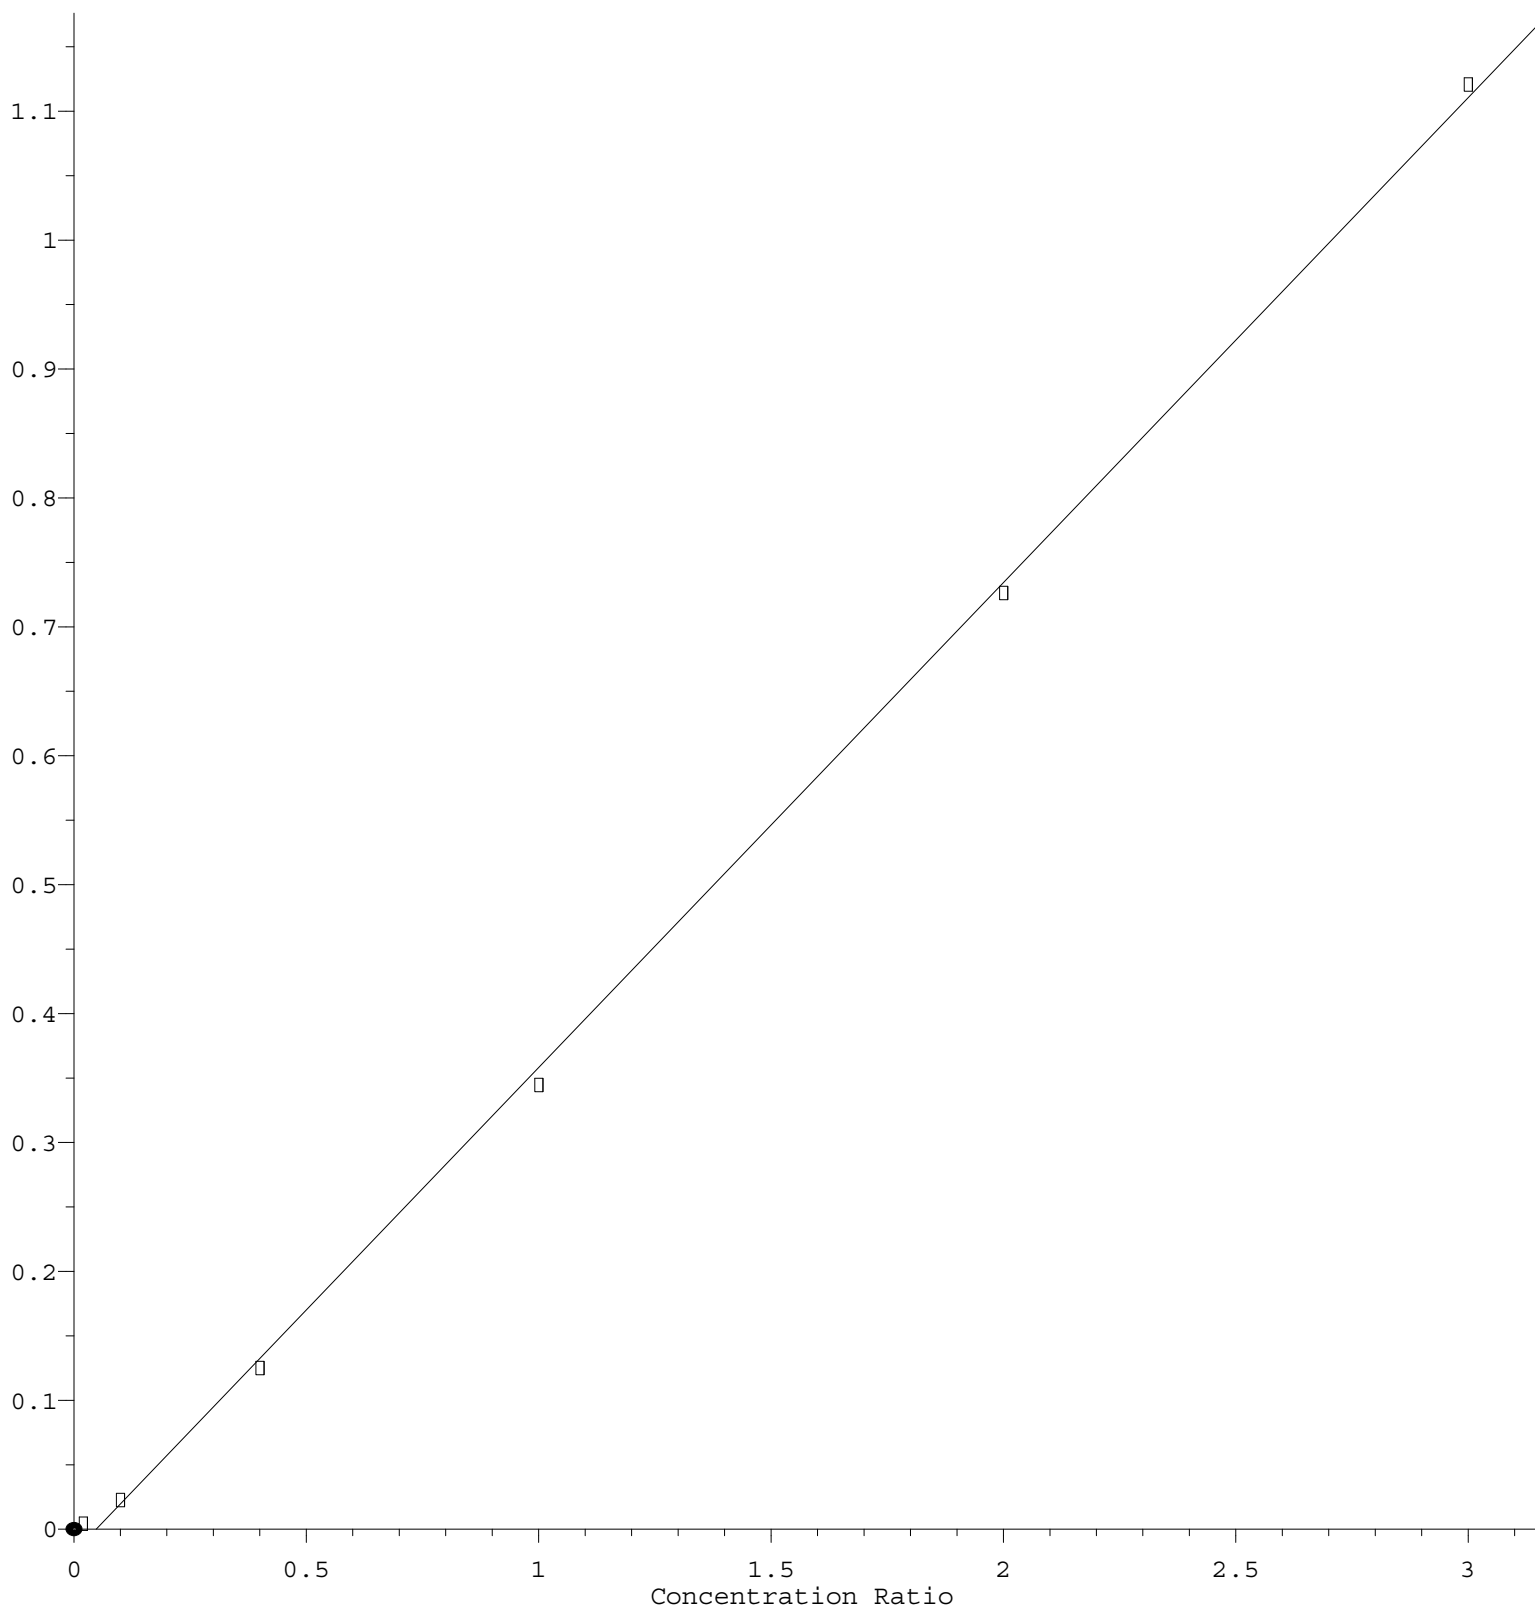

$$\text{Response} = 3.761\text{e-}001 * \text{Amt} - 1.818\text{e-}002$$


Coef of Det (r^2) = 0.999368 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M

Calibration Table Last Updated: Tue Nov 09 18:18:22 2021

Hexachloroethane

Response Ratio

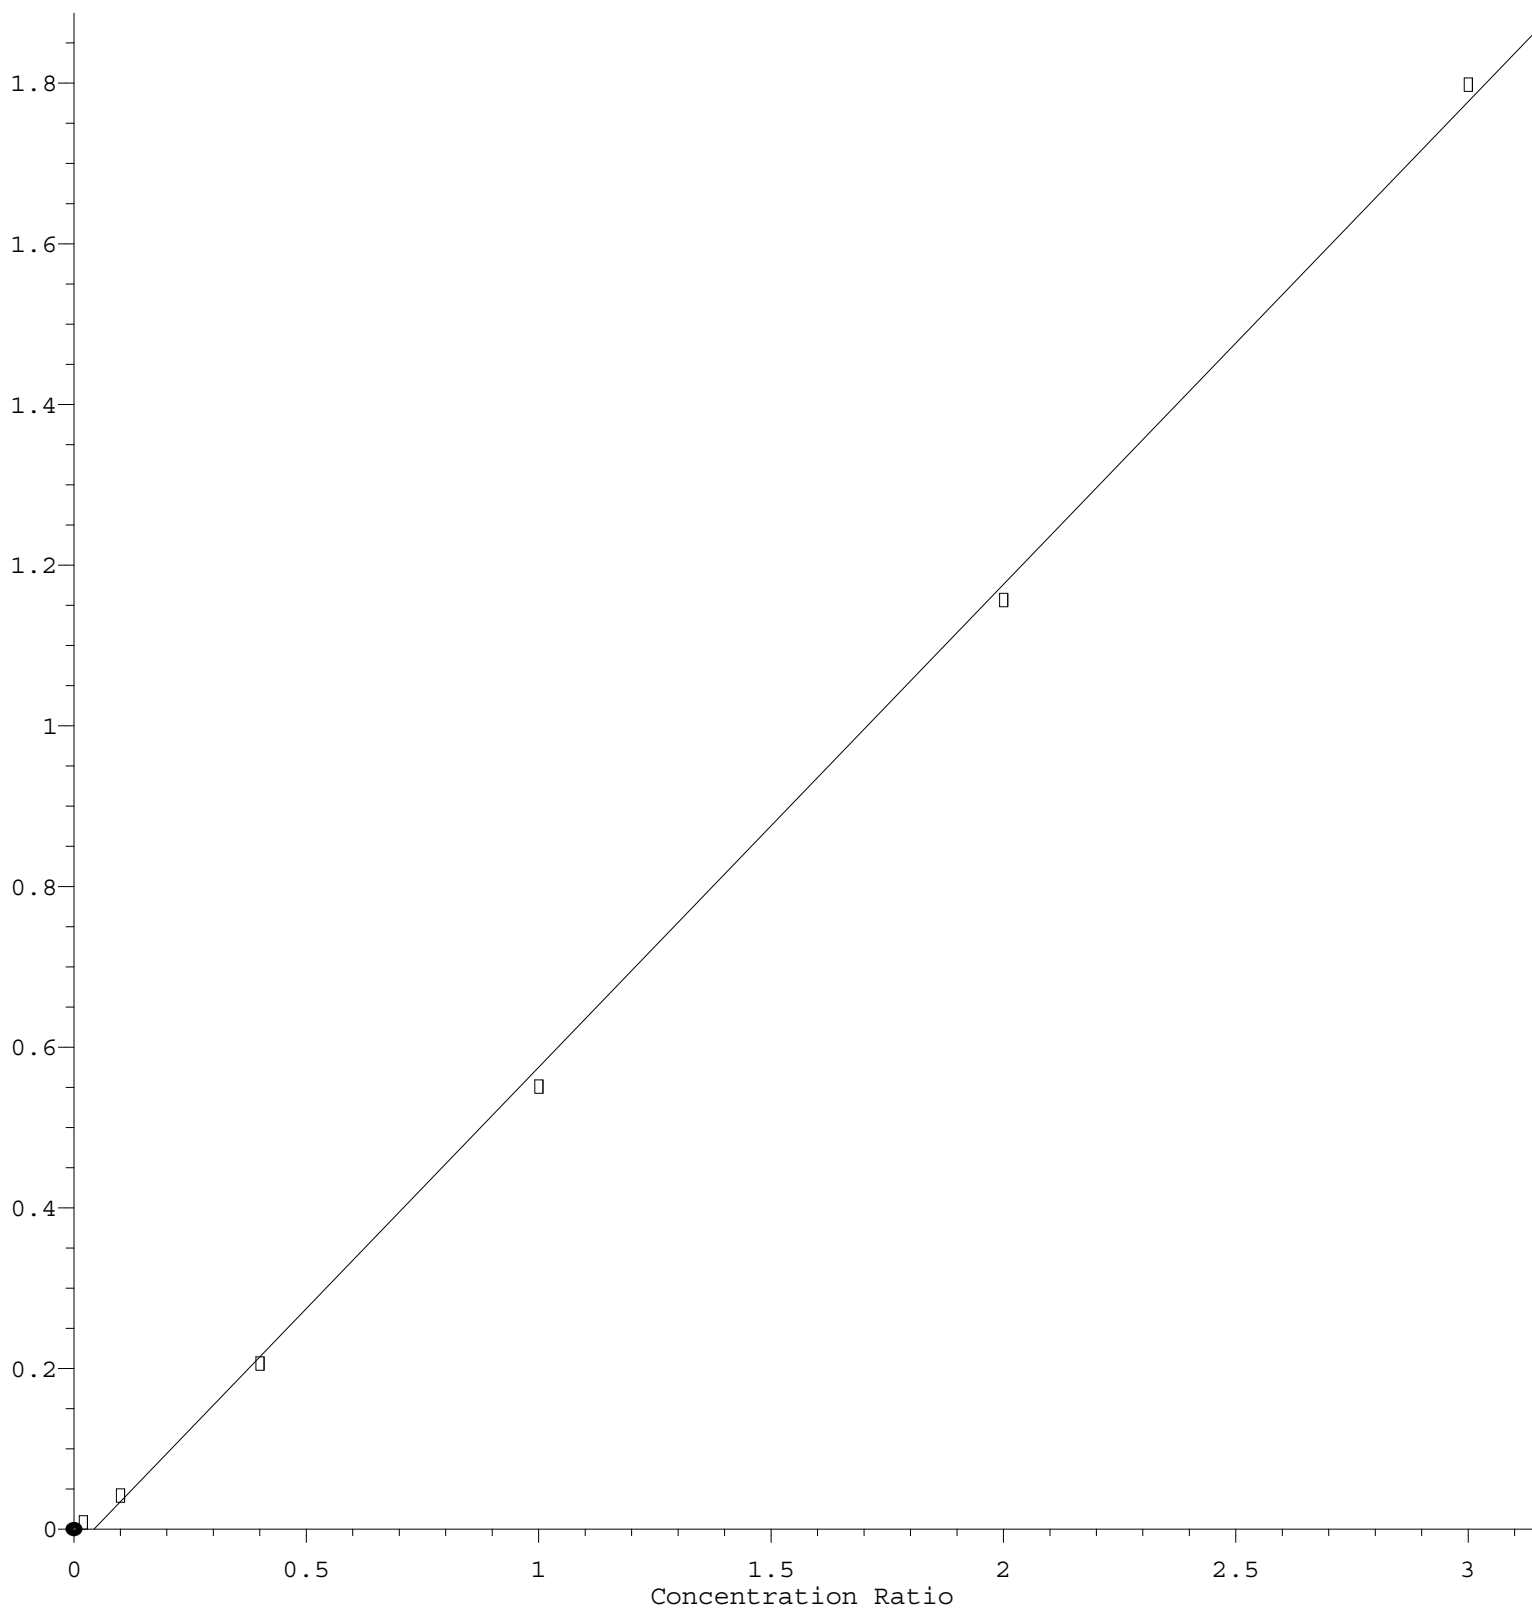

$$\text{Response} = 6.008\text{e-}001 * \text{Amt} - 2.598\text{e-}002$$


Coef of Det (r^2) = 0.999207 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M

Calibration Table Last Updated: Tue Nov 09 18:18:22 2021

1,2-Dibromoethane

Response Ratio

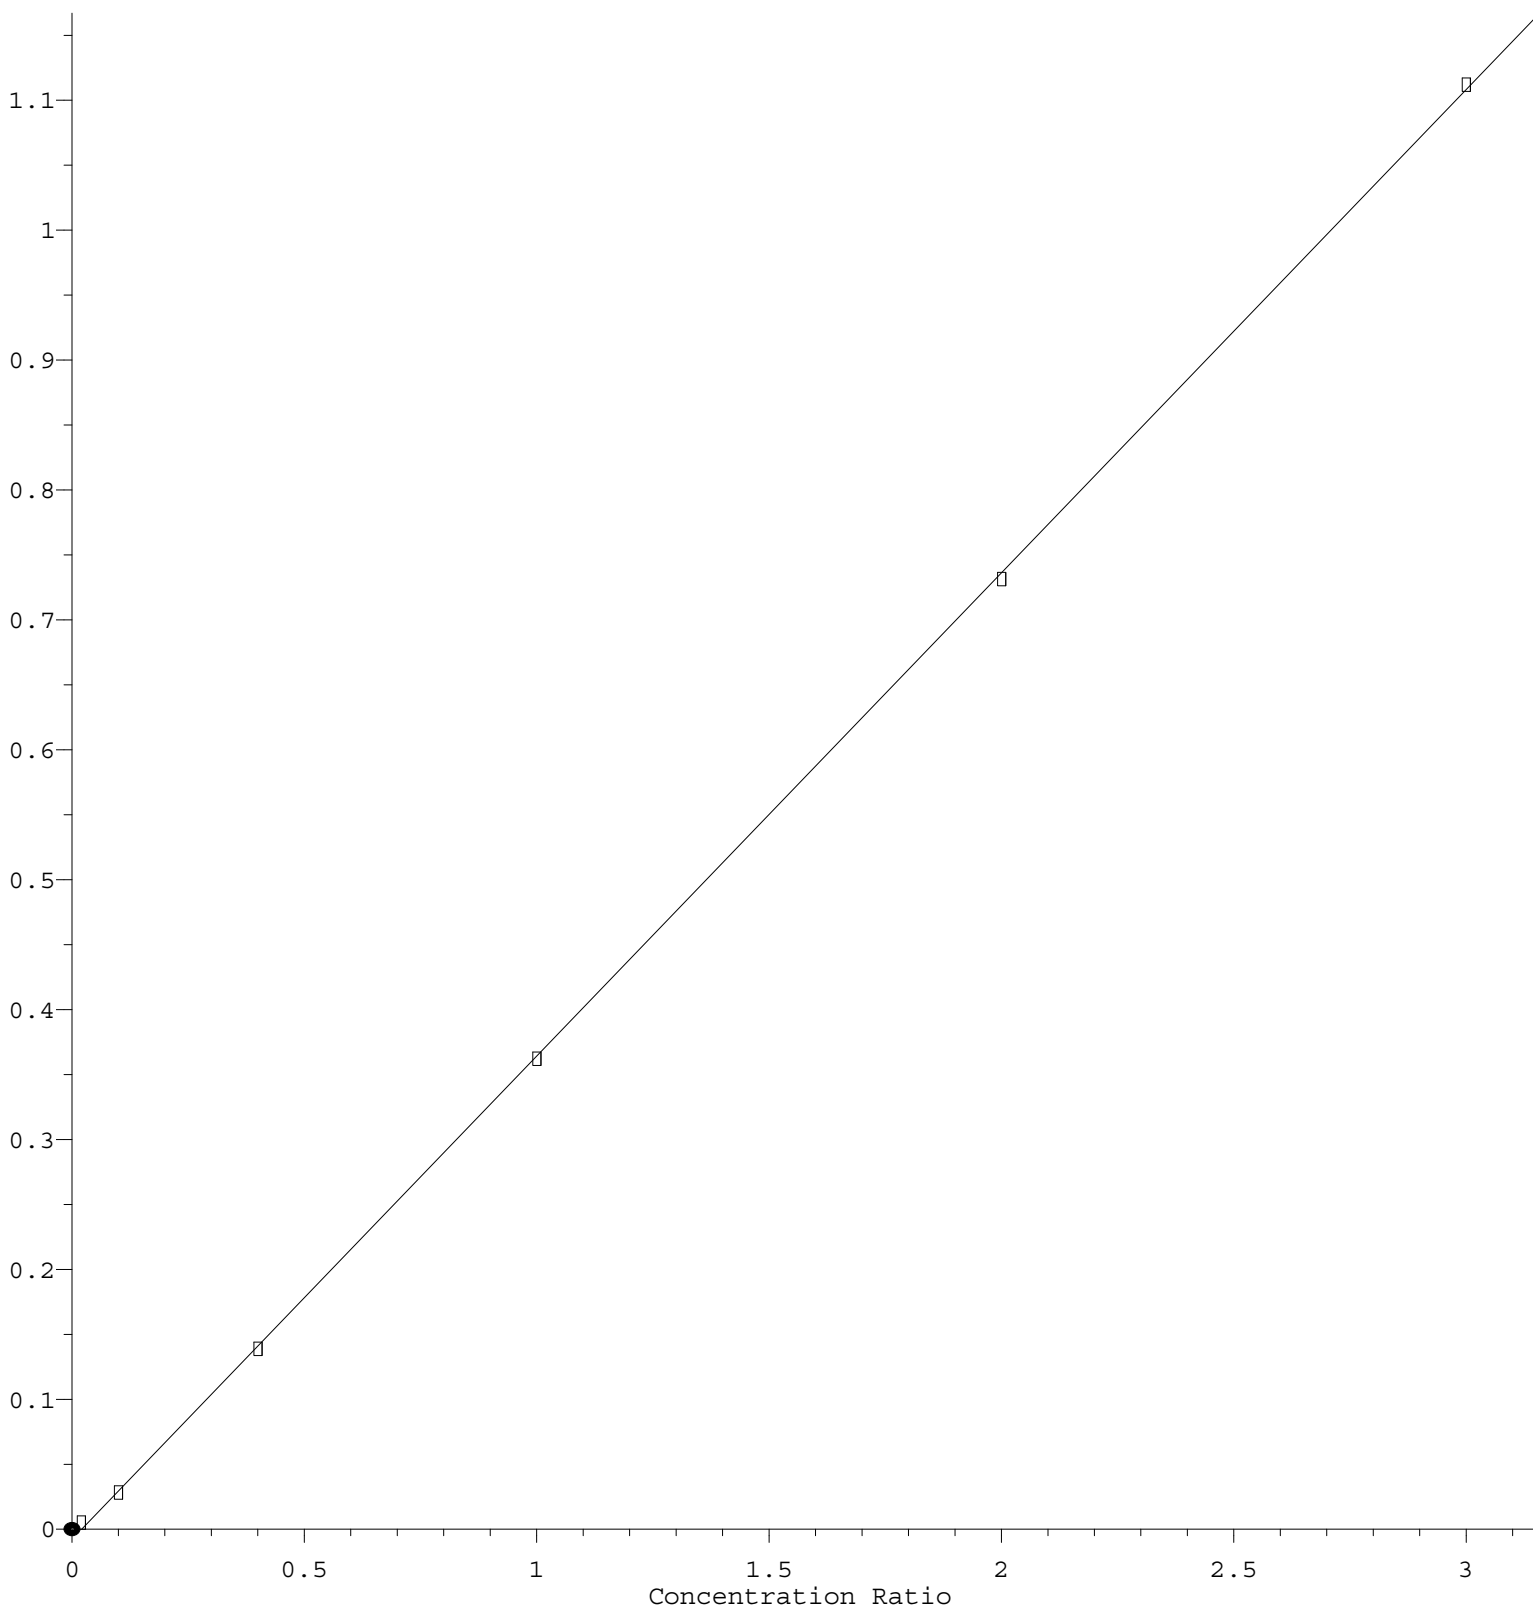

$$\text{Response} = 3.720\text{e-}001 * \text{Amt} - 7.968\text{e-}003$$


Coef of Det (r^2) = 0.999922 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M

Calibration Table Last Updated: Tue Nov 09 18:18:22 2021

Styrene


Response Ratio

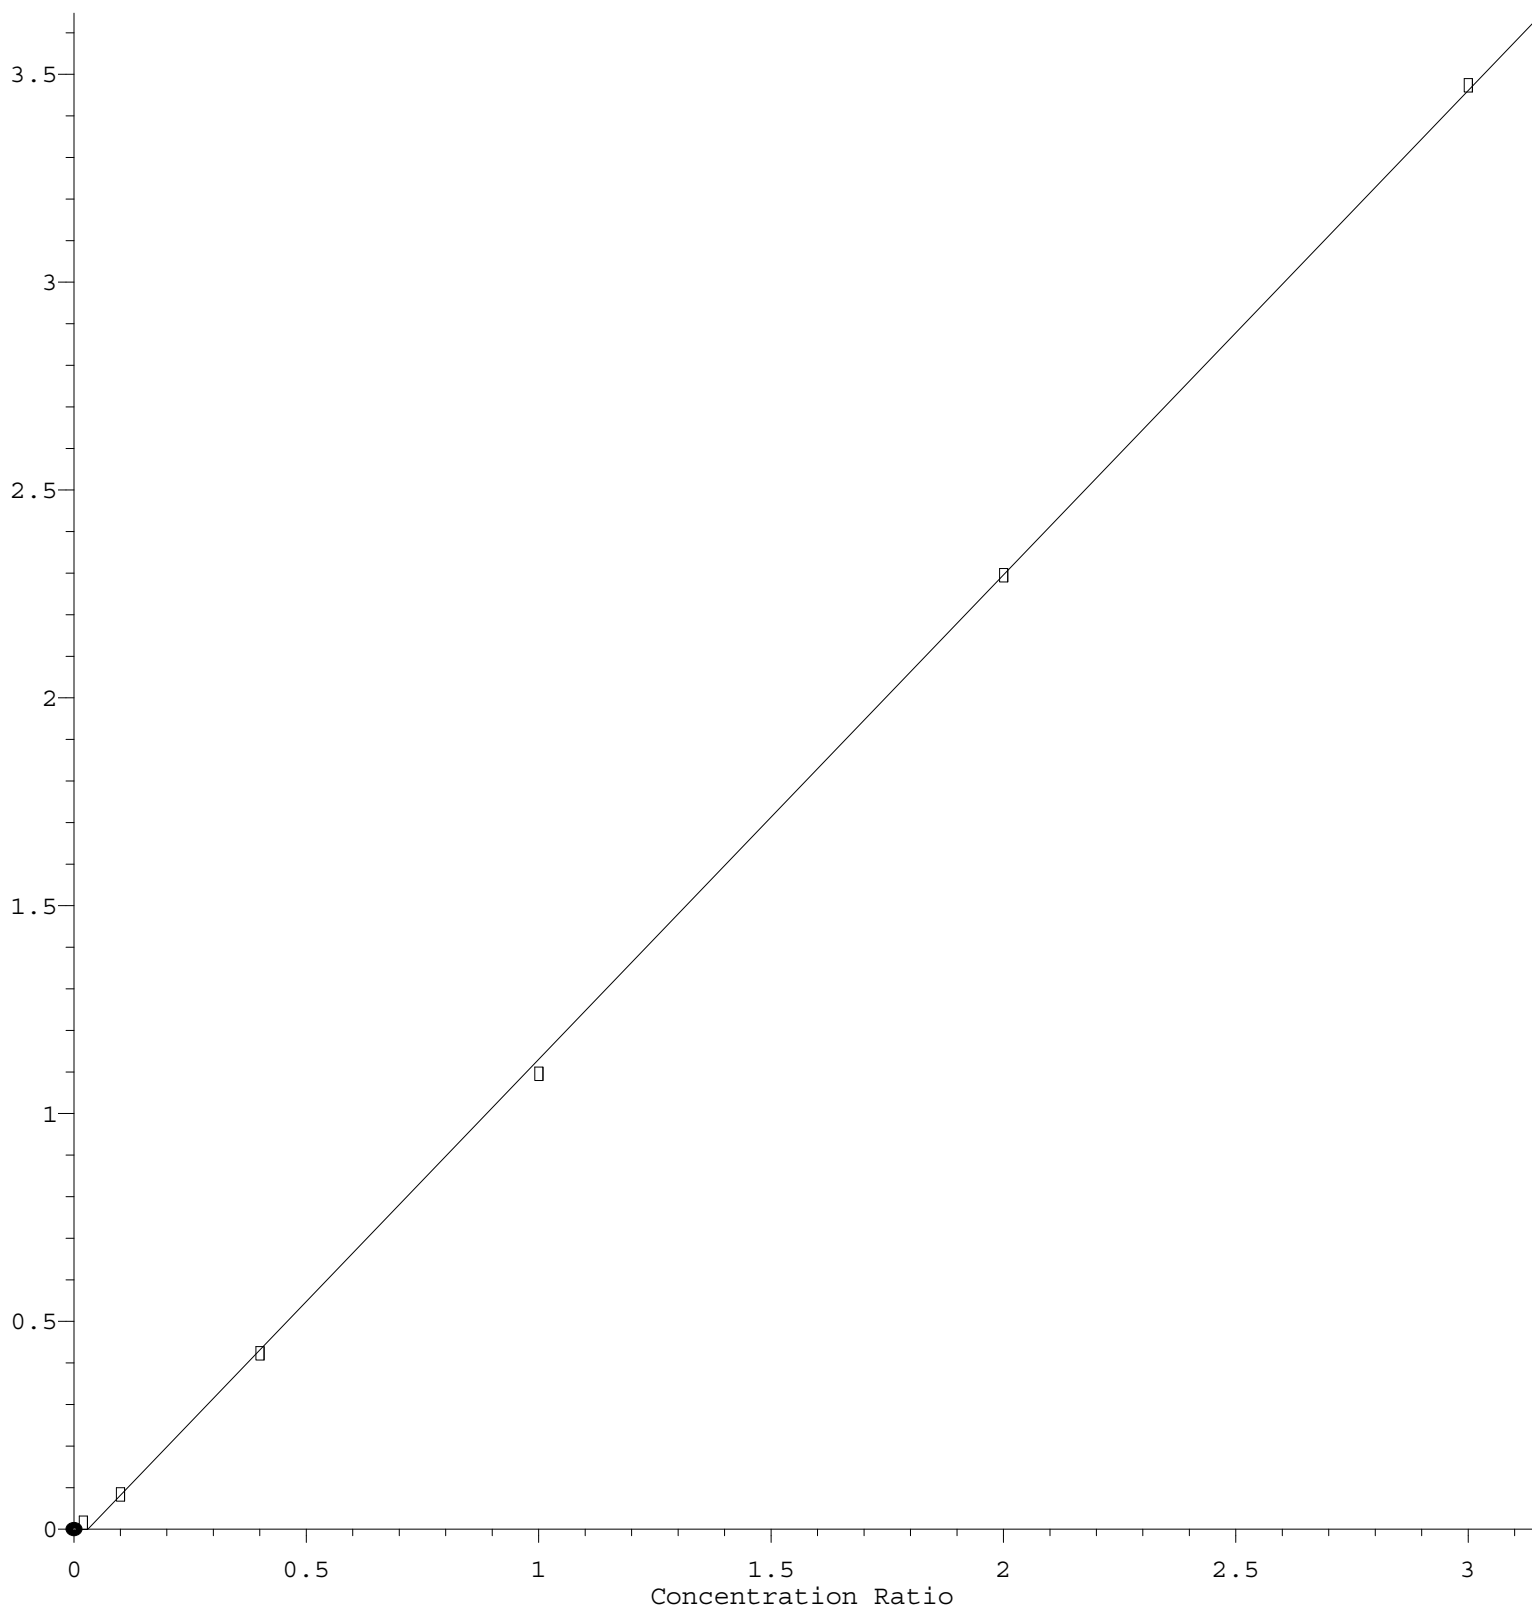

Response = 1.165e+000 * Amt - 3.544e-002
Coef of Det (r^2) = 0.999774 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M
Calibration Table Last Updated: Tue Nov 09 18:18:22 2021

Naphthalene


Response Ratio

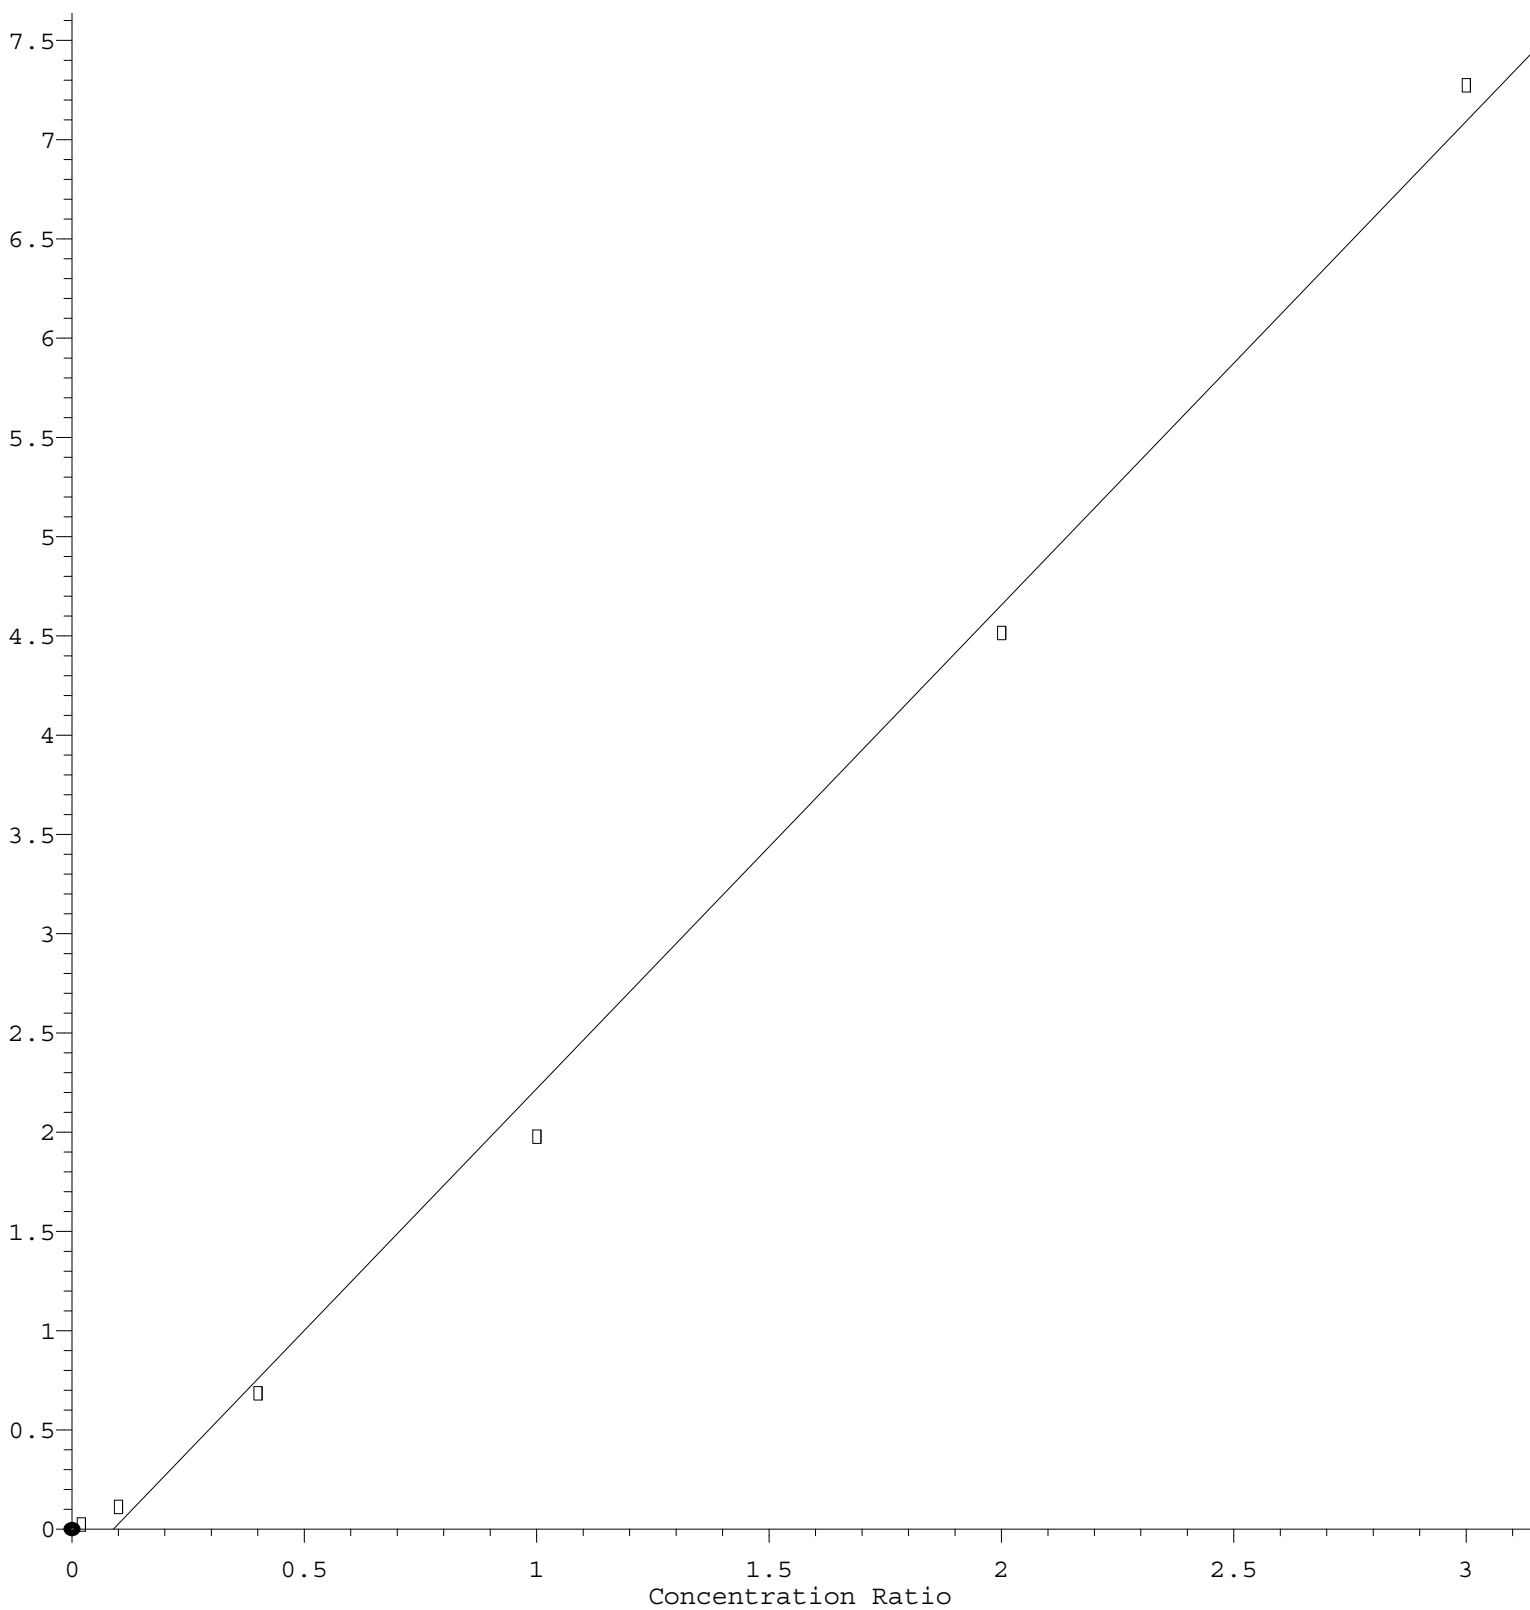

Response = 2.437e+000 * Amt - 2.169e-001
 Coef of Det (r^2) = 0.996191 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M
 Calibration Table Last Updated: Tue Nov 09 18:18:22 2021

cis-1,3-Dichloropropene

Response Ratio

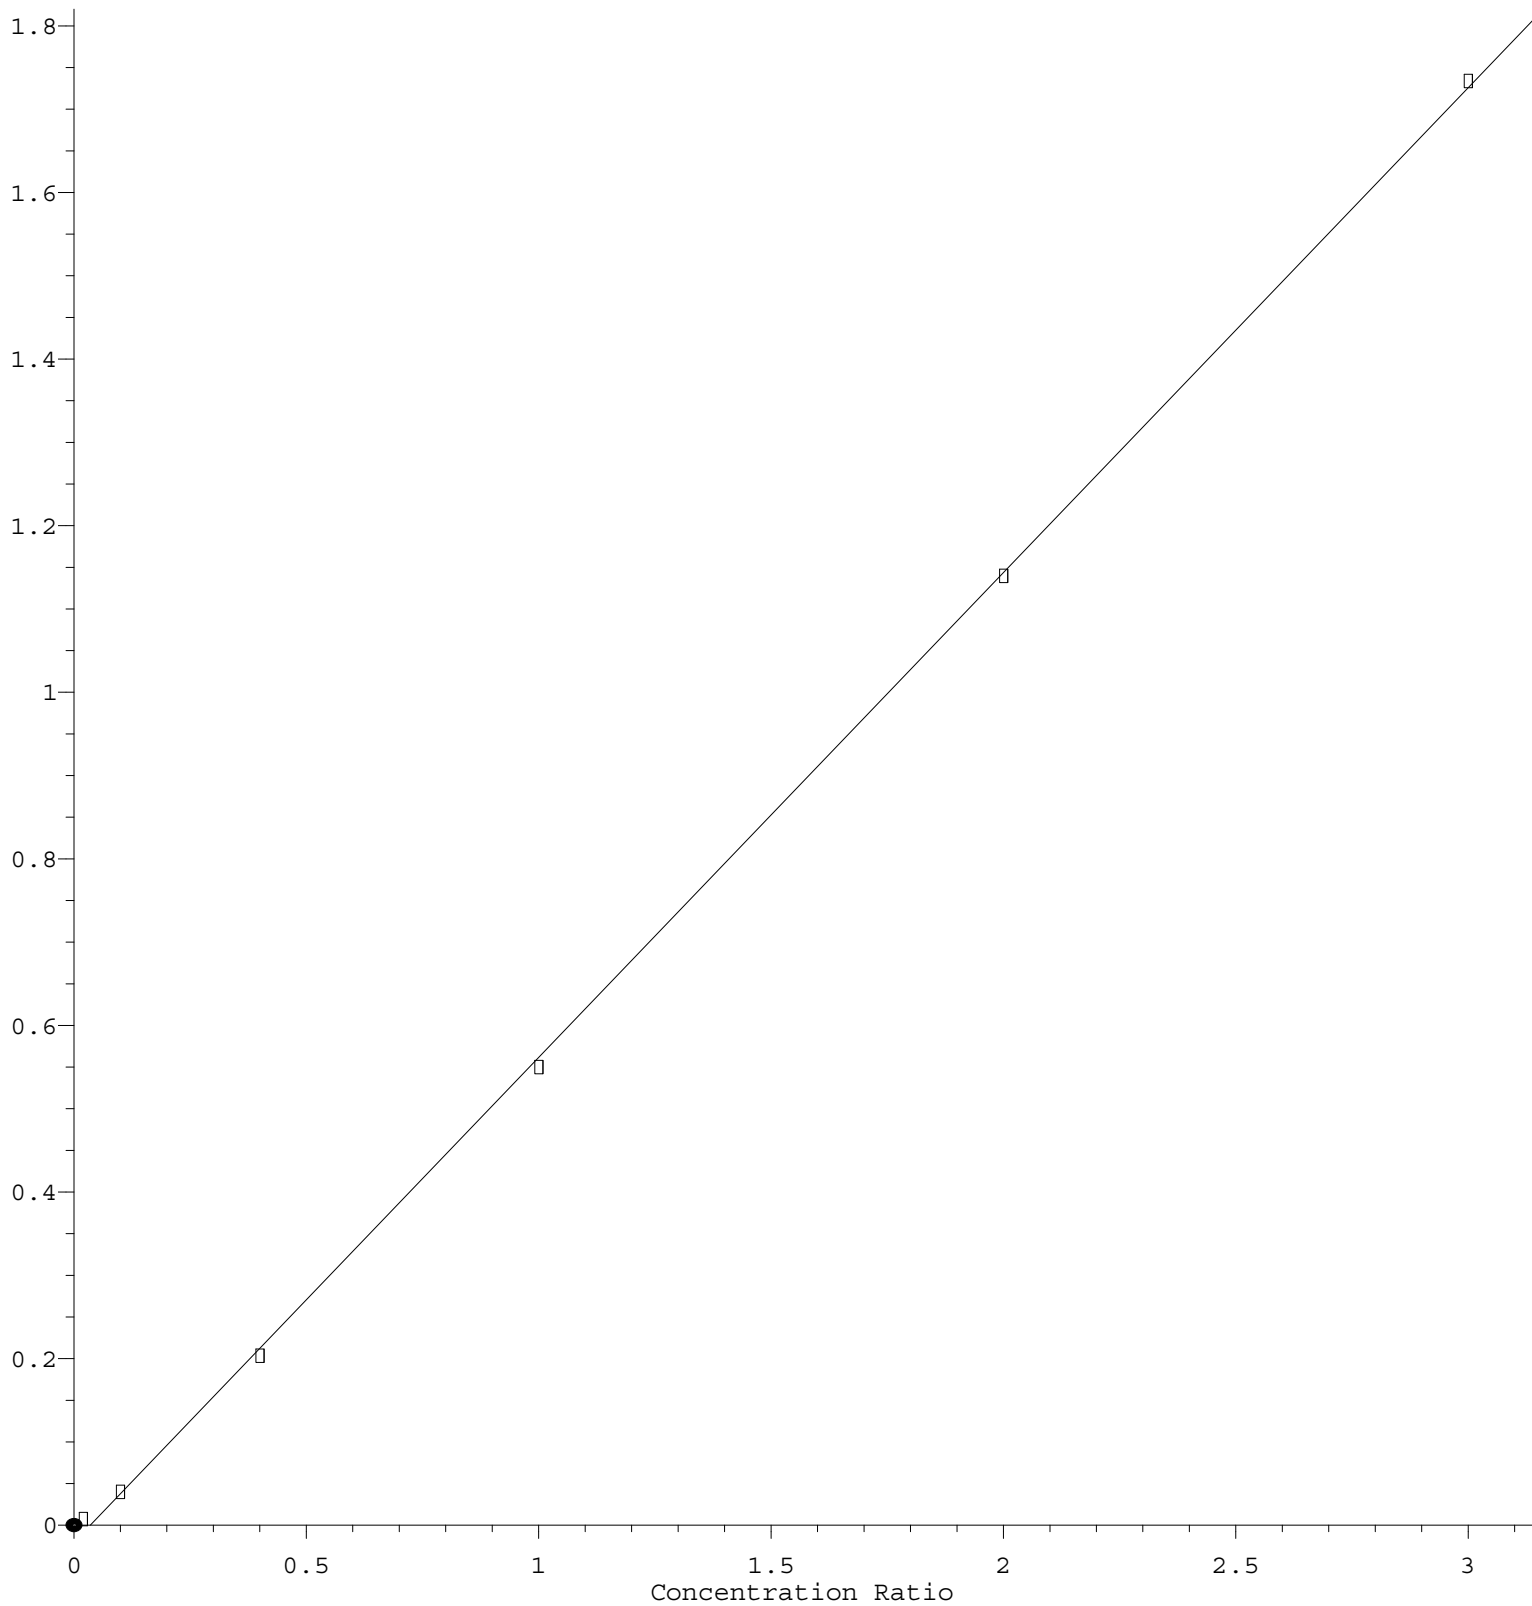

$$\text{Response} = 5.820\text{e-}001 * \text{Amt} - 2.017\text{e-}002$$


Coef of Det (r^2) = 0.999766 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M

Calibration Table Last Updated: Tue Nov 09 18:18:22 2021

trans-1,4-Dichloro-2-butene

Response Ratio

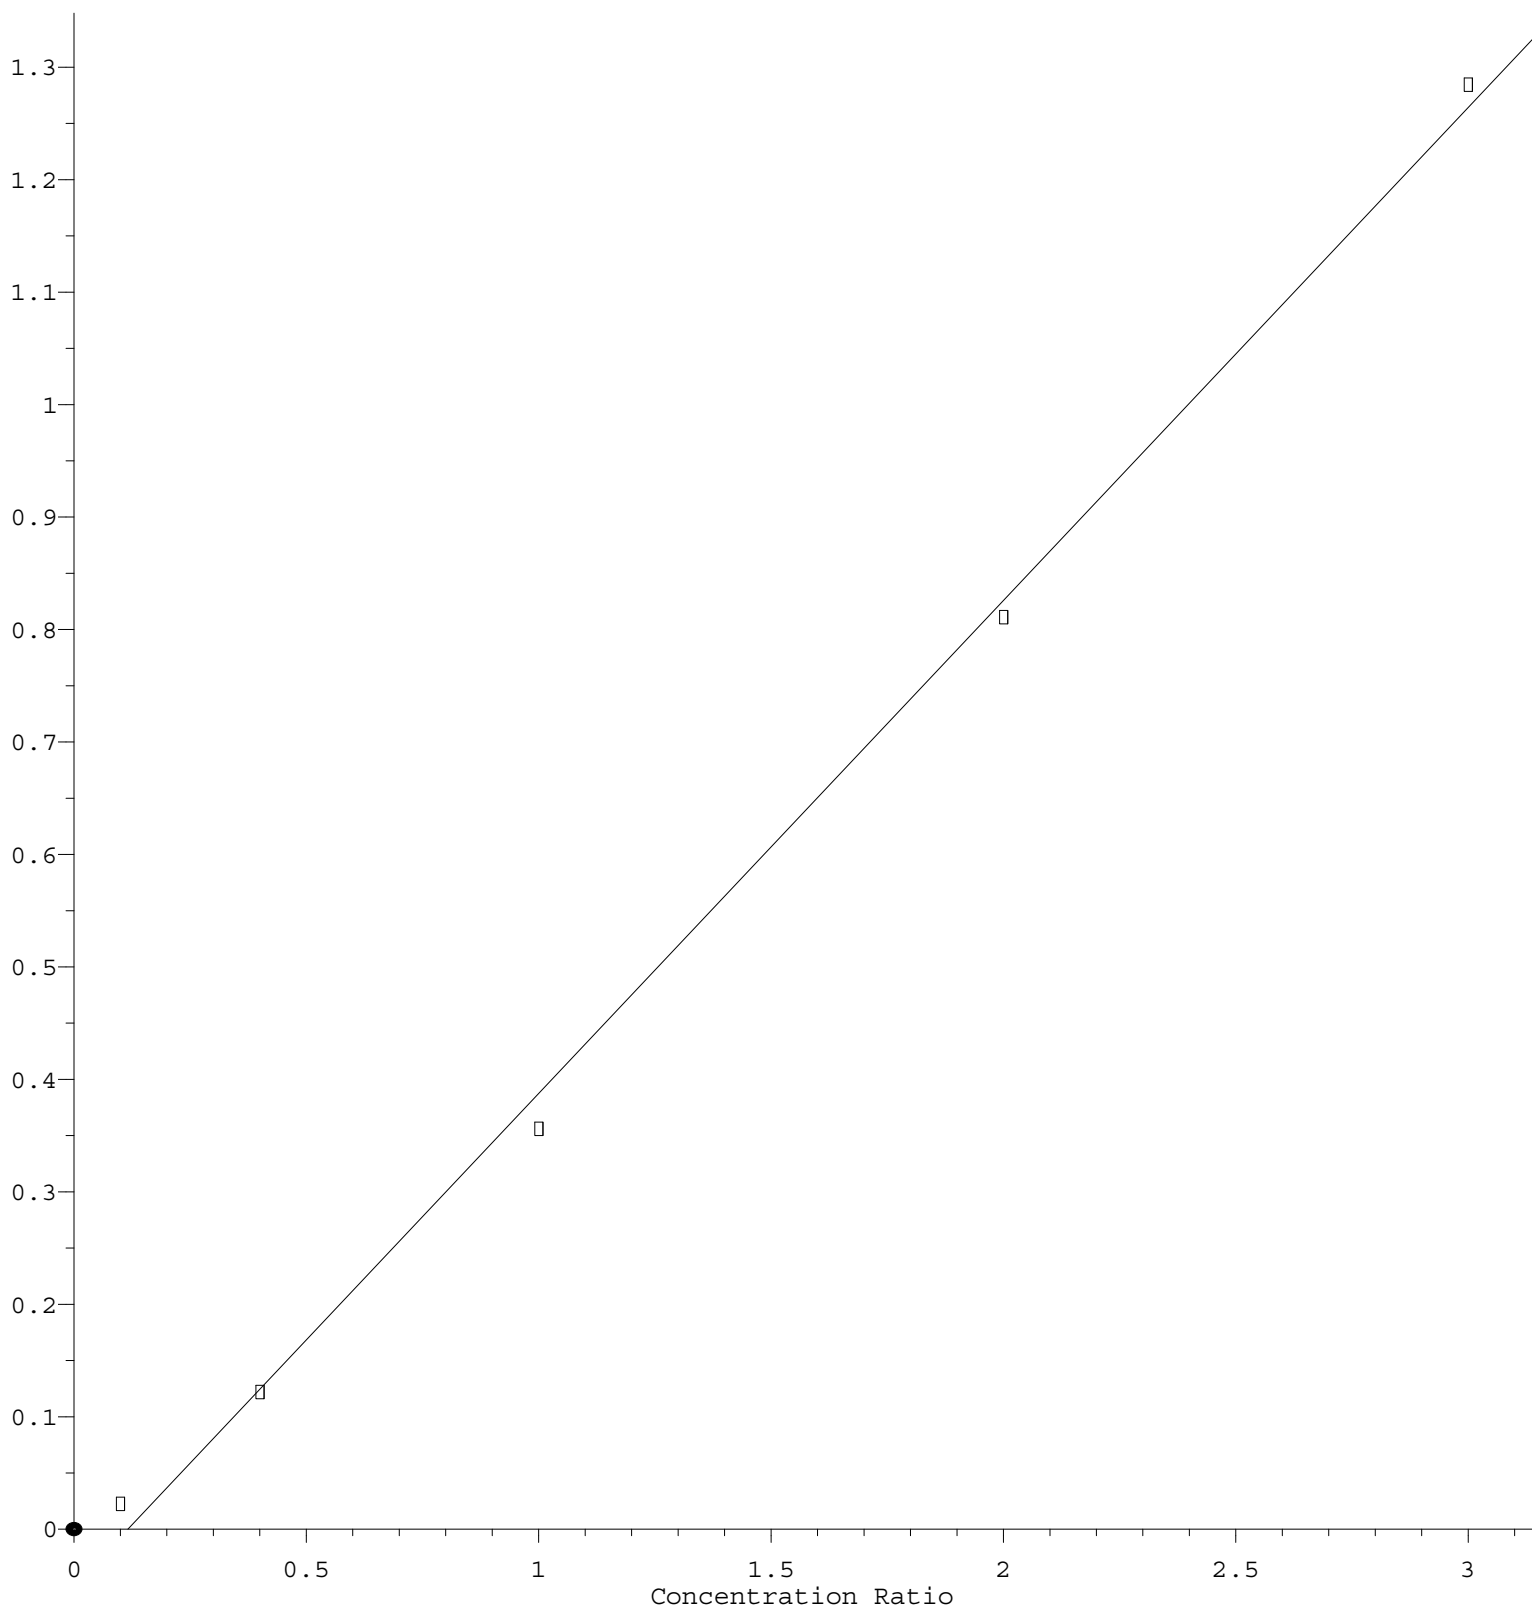


$$\text{Response} = 4.384\text{e-}001 * \text{Amt} - 5.074\text{e-}002$$

Coef of Det (r^2) = 0.997732 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M

Calibration Table Last Updated: Tue Nov 09 18:18:22 2021


1,2-Dibromo-3-Chloropropane

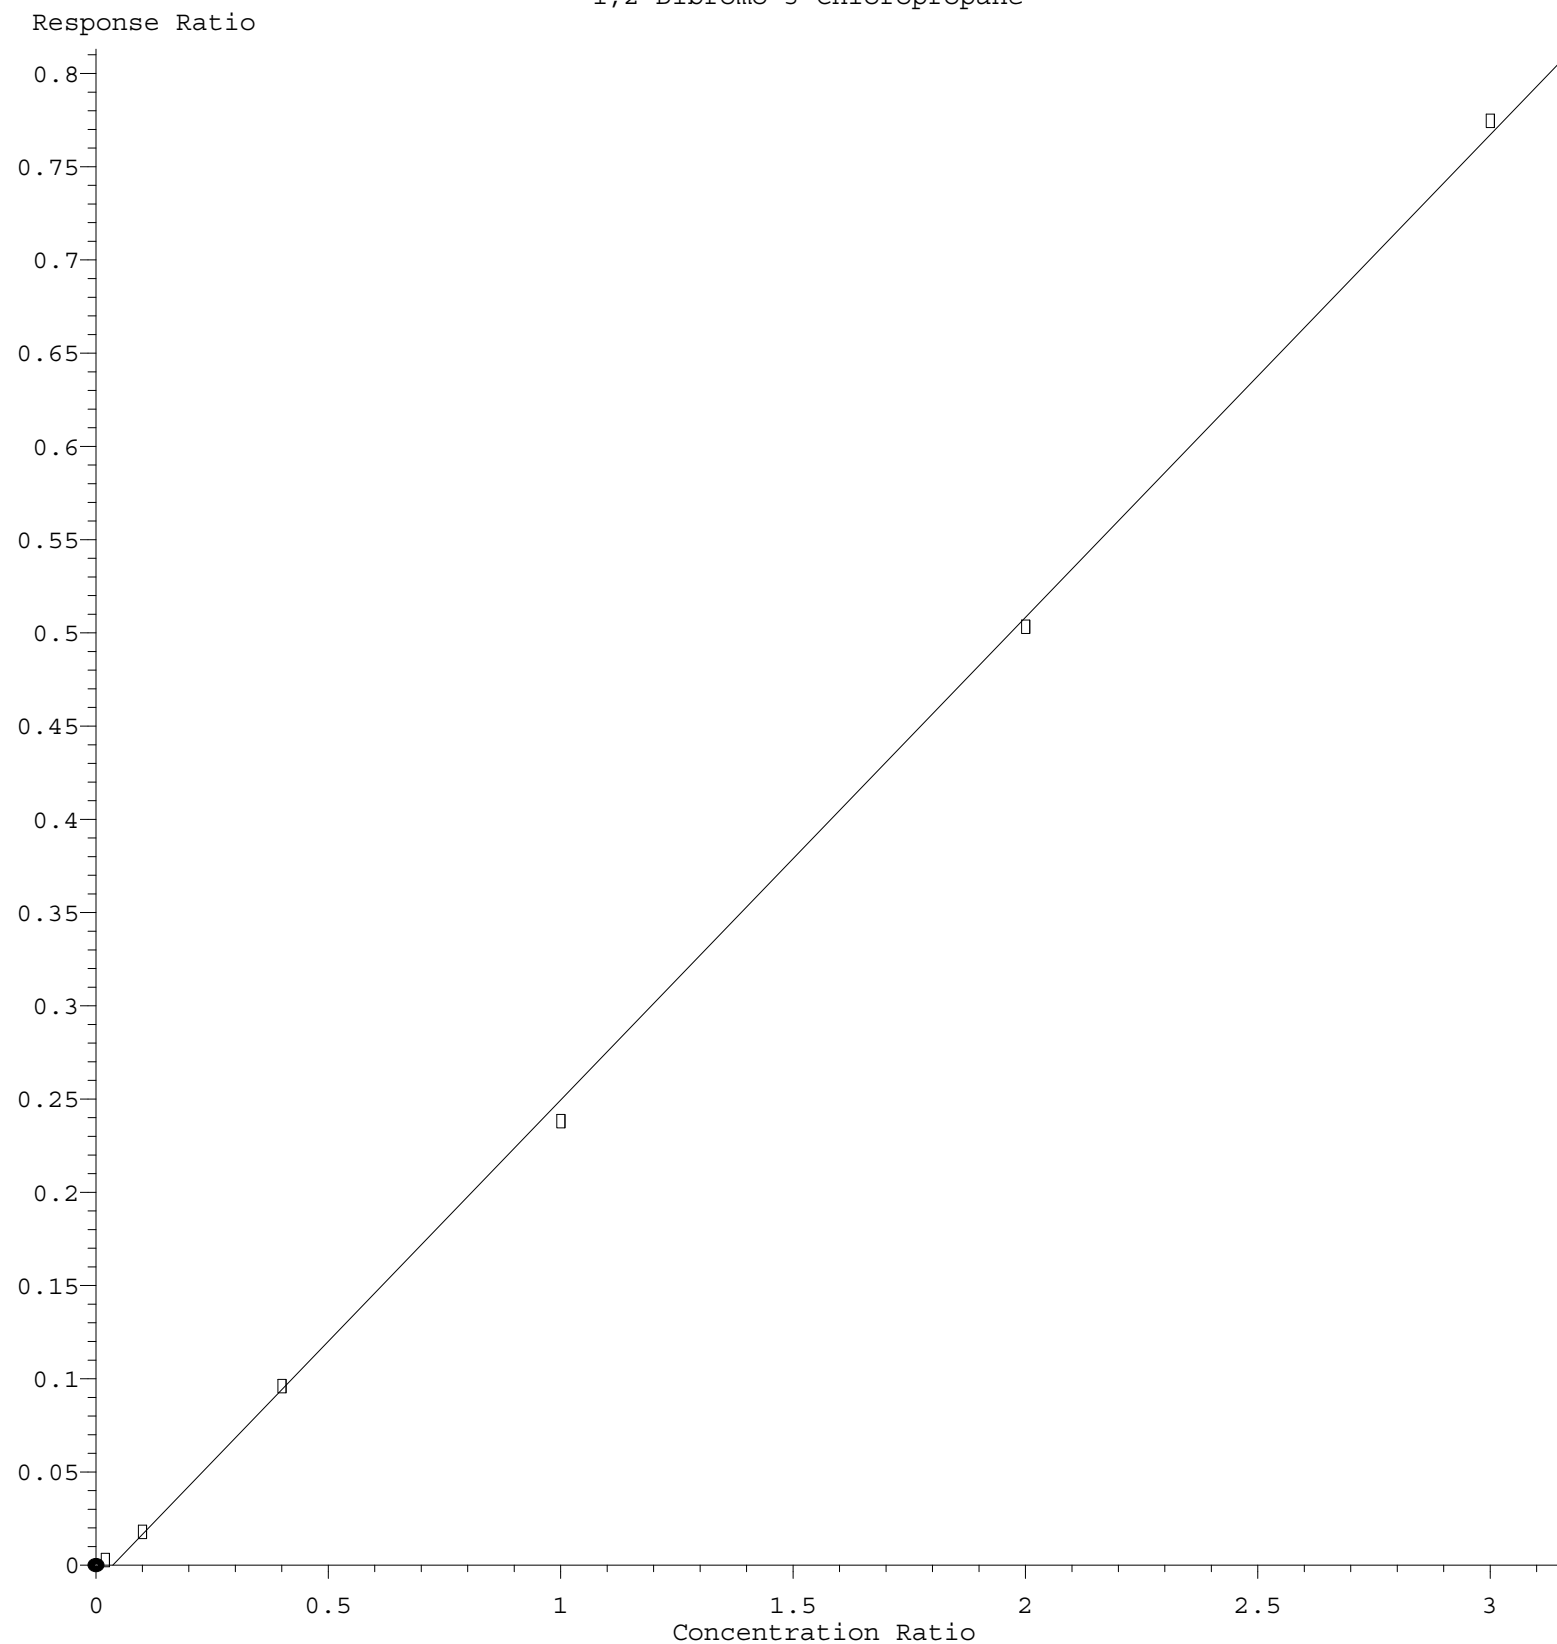

Response = 2.589e-001 * Amt - 9.306e-003
 Coef of Det (r^2) = 0.999448 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M
 Calibration Table Last Updated: Tue Nov 09 18:18:22 2021

1,2,3-Trichlorobenzene

Response Ratio

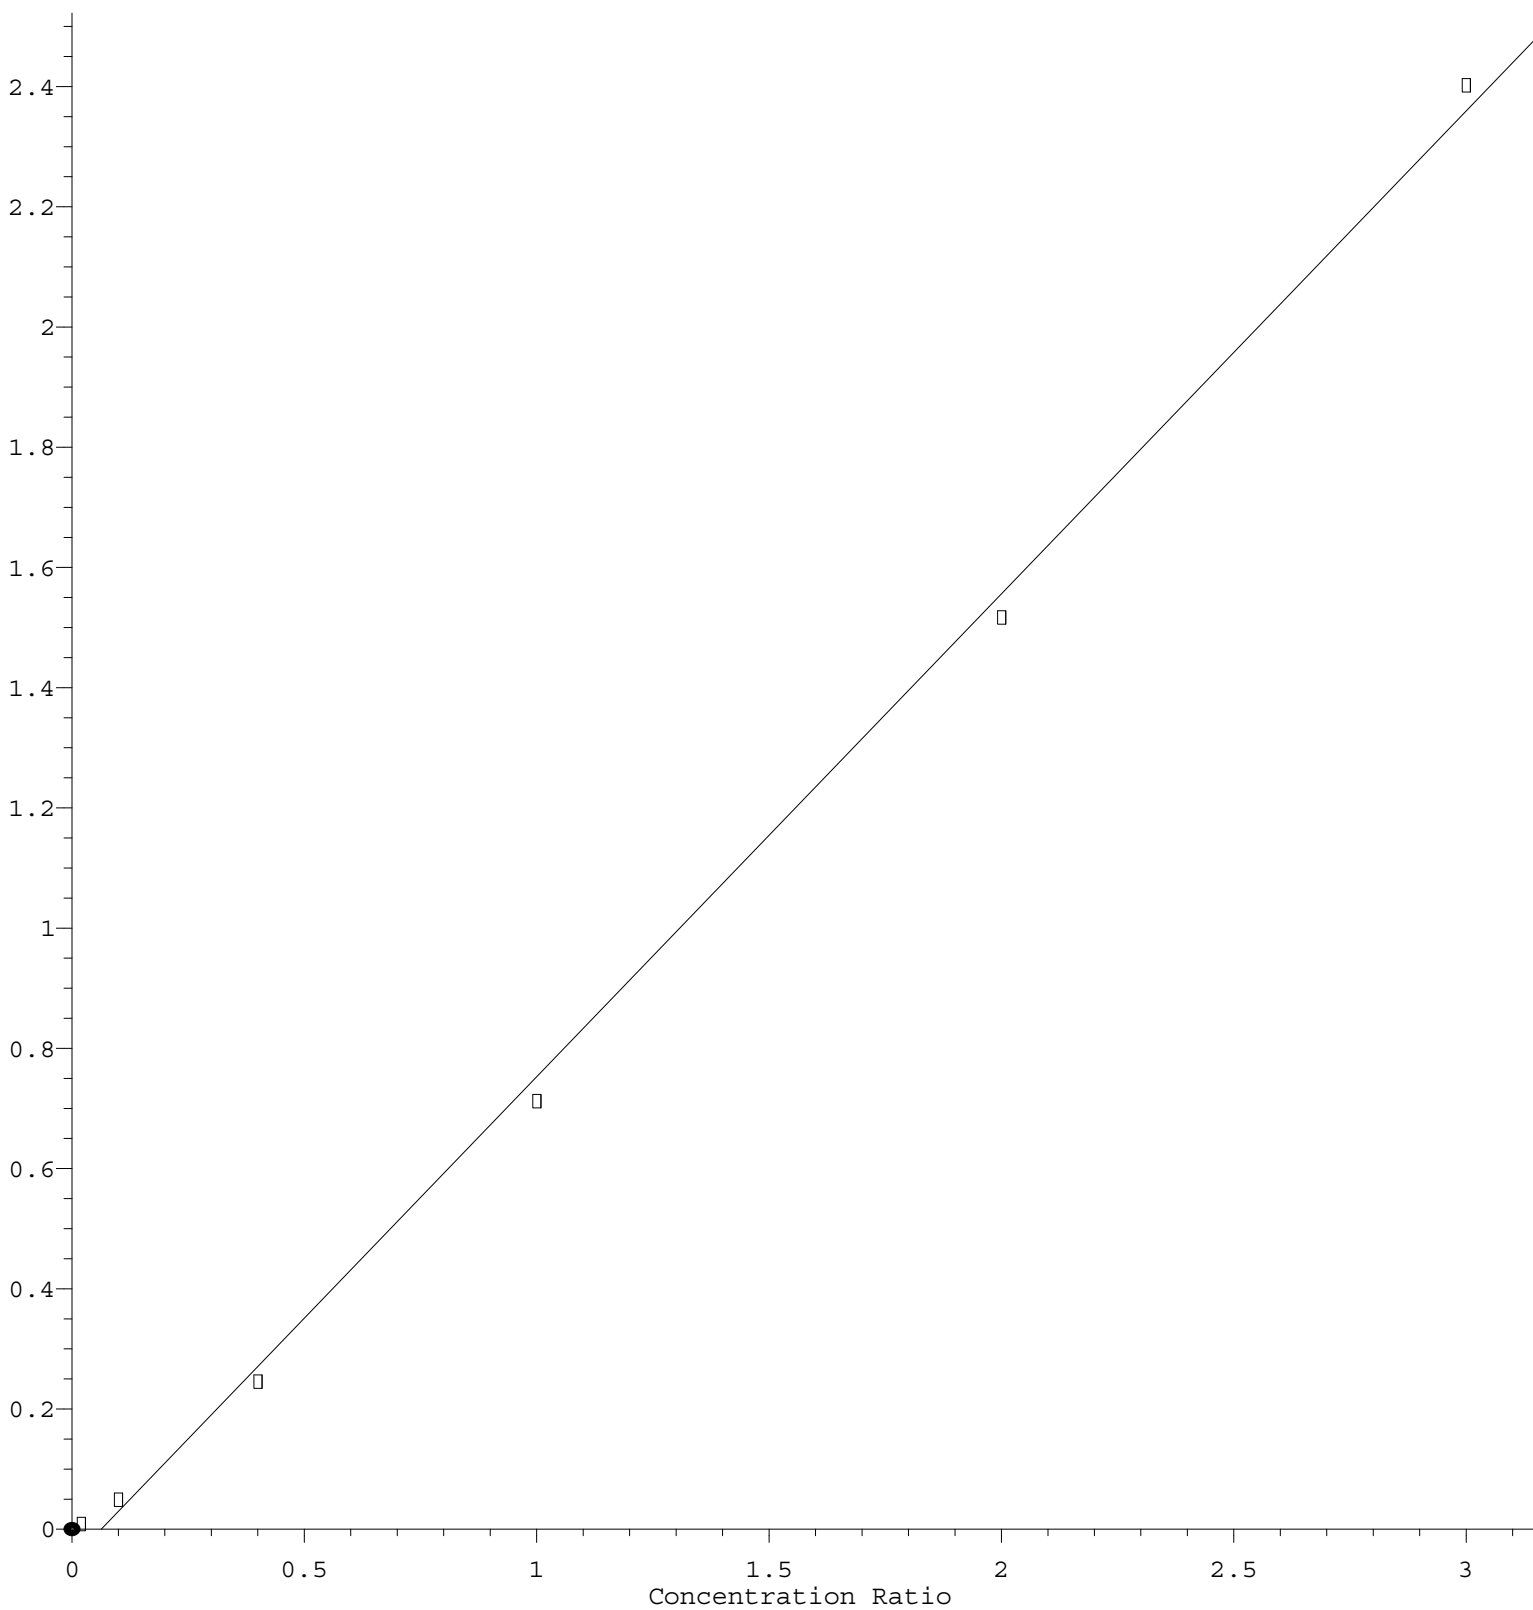

$$\text{Response} = 8.035\text{e-}001 * \text{Amt} - 5.093\text{e-}002$$


Coef of Det (r^2) = 0.998275 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M

Calibration Table Last Updated: Tue Nov 09 18:18:22 2021

Bromoform

Response Ratio

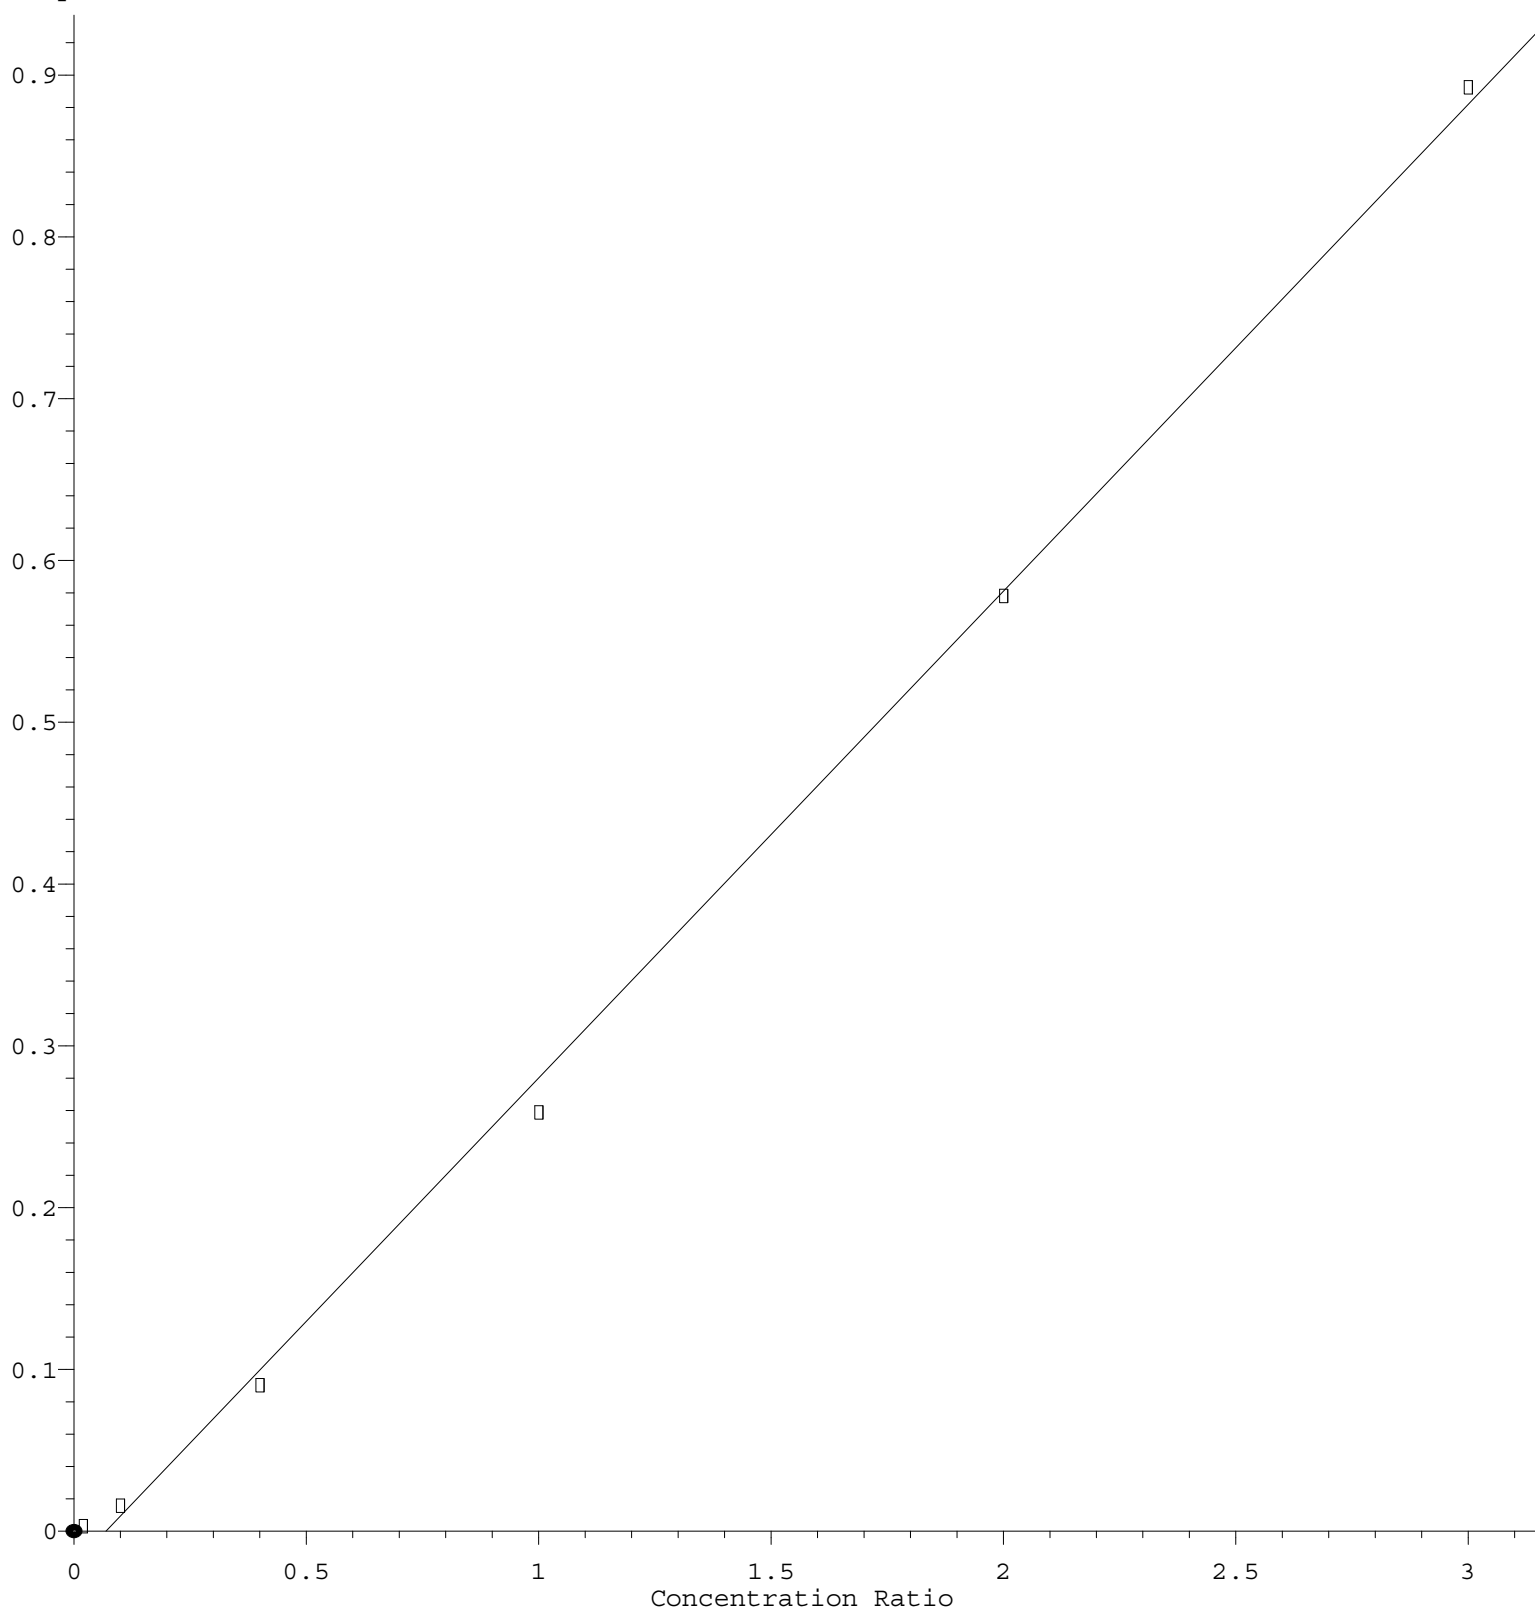

$$\text{Response} = 3.009\text{e-}001 * \text{Amt} - 2.063\text{e-}002$$


Coef of Det (r^2) = 0.998413 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M

Calibration Table Last Updated: Tue Nov 09 18:18:22 2021

2-Hexanone


Response Ratio

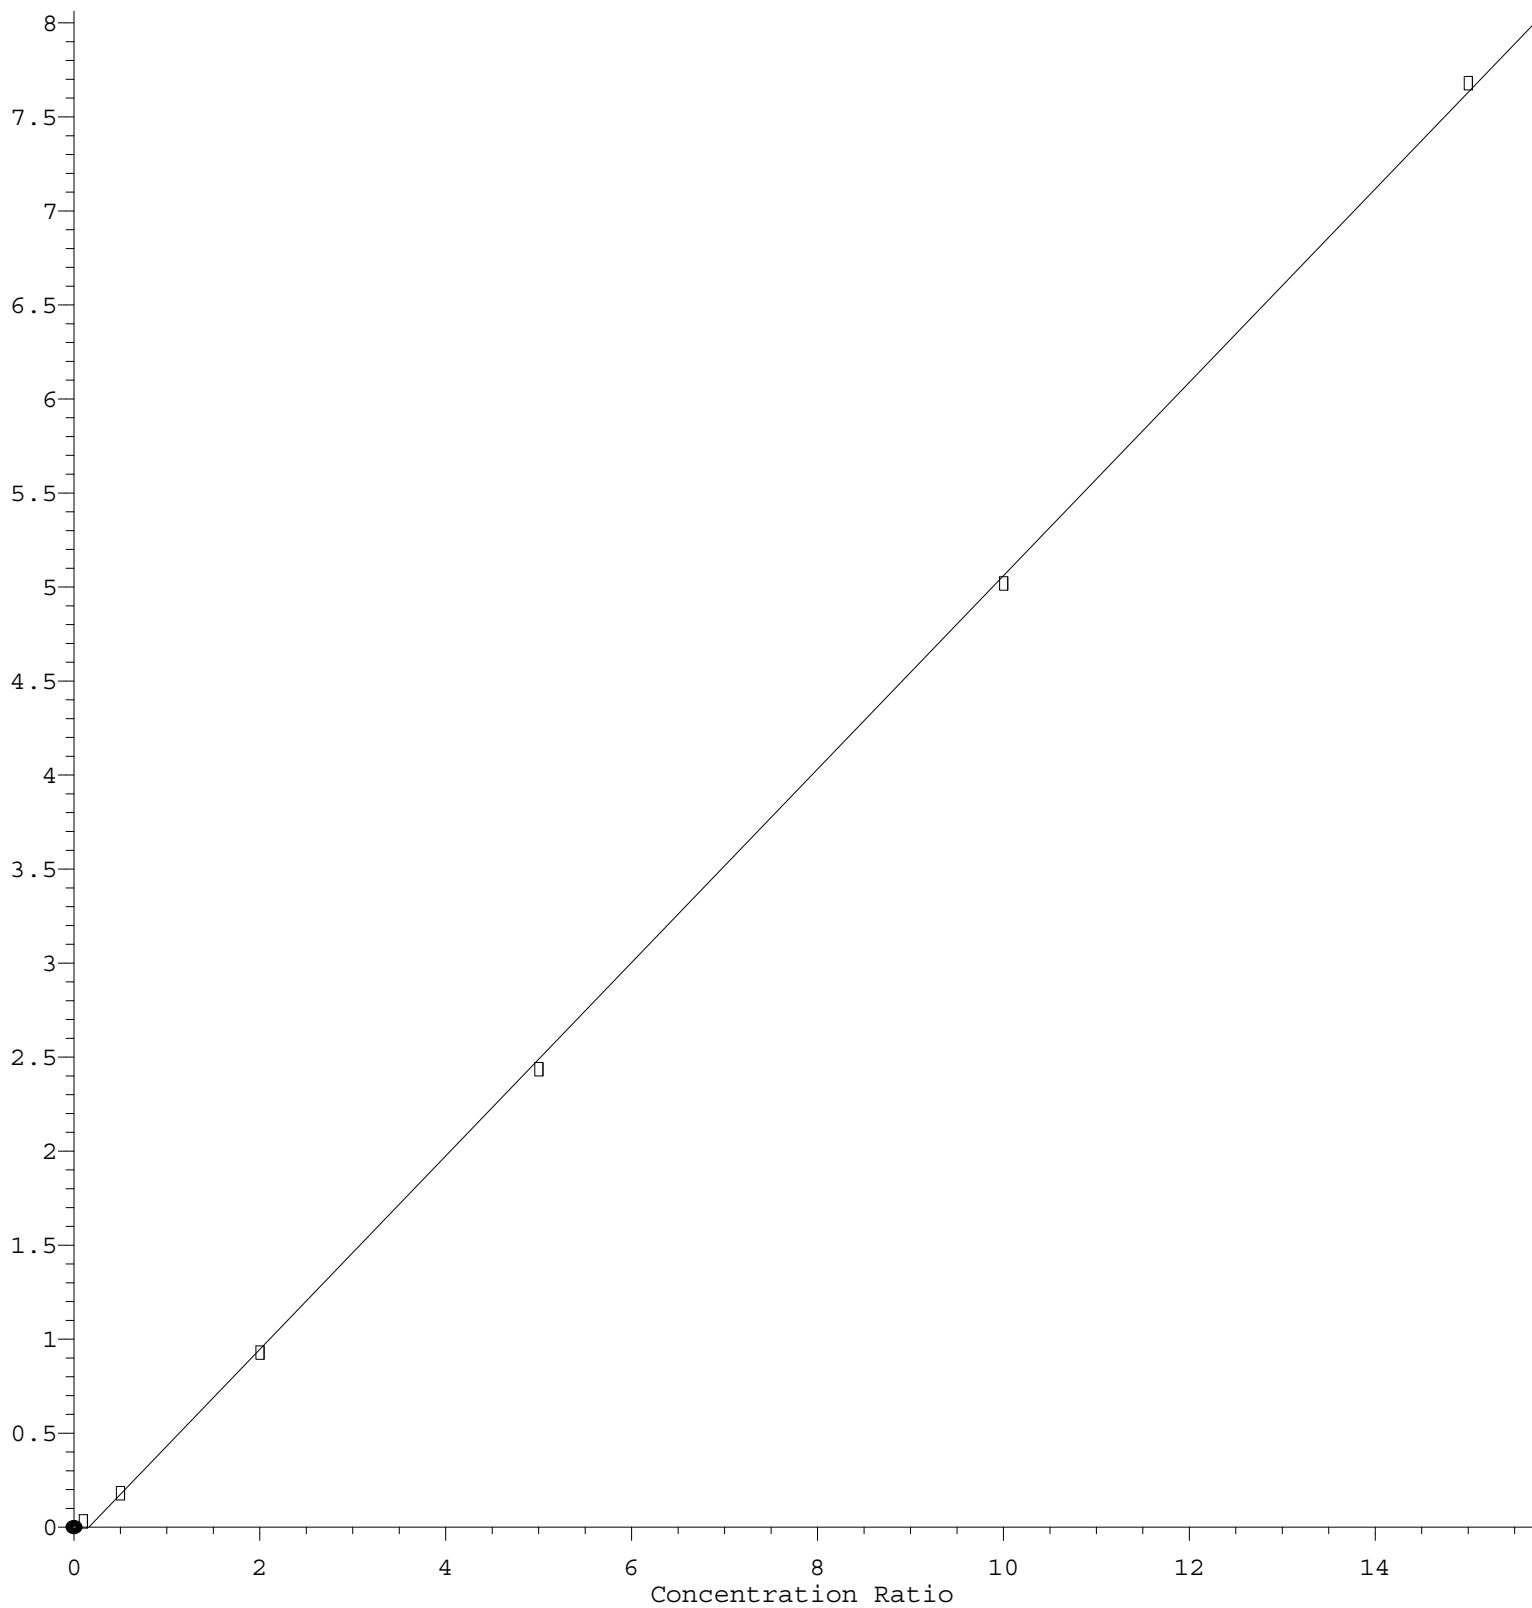

Response = 5.142e-001 * Amt - 8.167e-002
Coef of Det (r^2) = 0.999763 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M
Calibration Table Last Updated: Tue Nov 09 18:18:22 2021

2-Chloroethyl Vinyl ether

Response Ratio

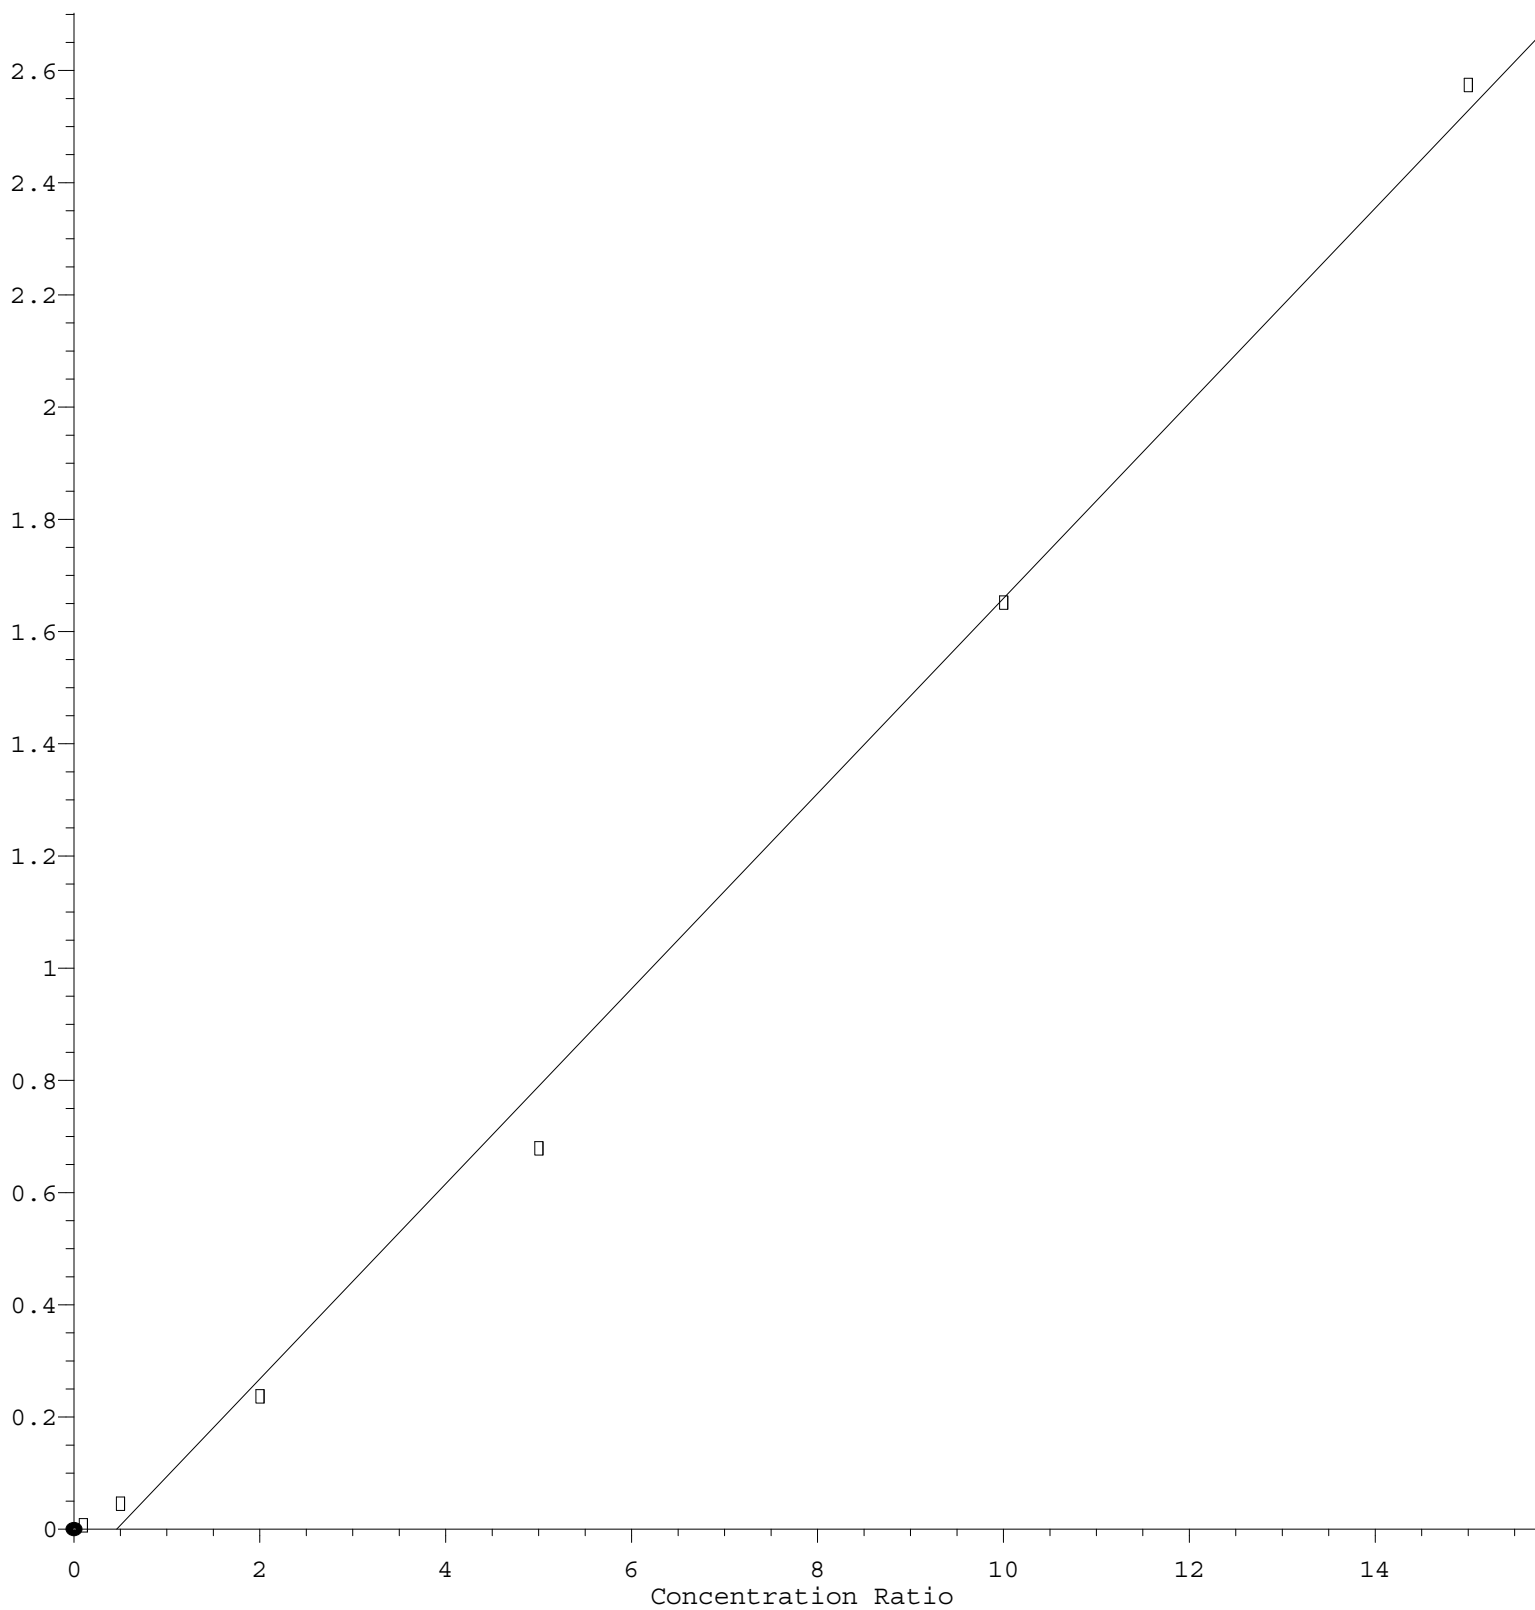

$$\text{Response} = 1.739\text{e-}001 * \text{Amt} - 7.918\text{e-}002$$


Coef of Det (r^2) = 0.995970 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M

Calibration Table Last Updated: Tue Nov 09 18:18:22 2021

Ethyl methacrylate

Response Ratio

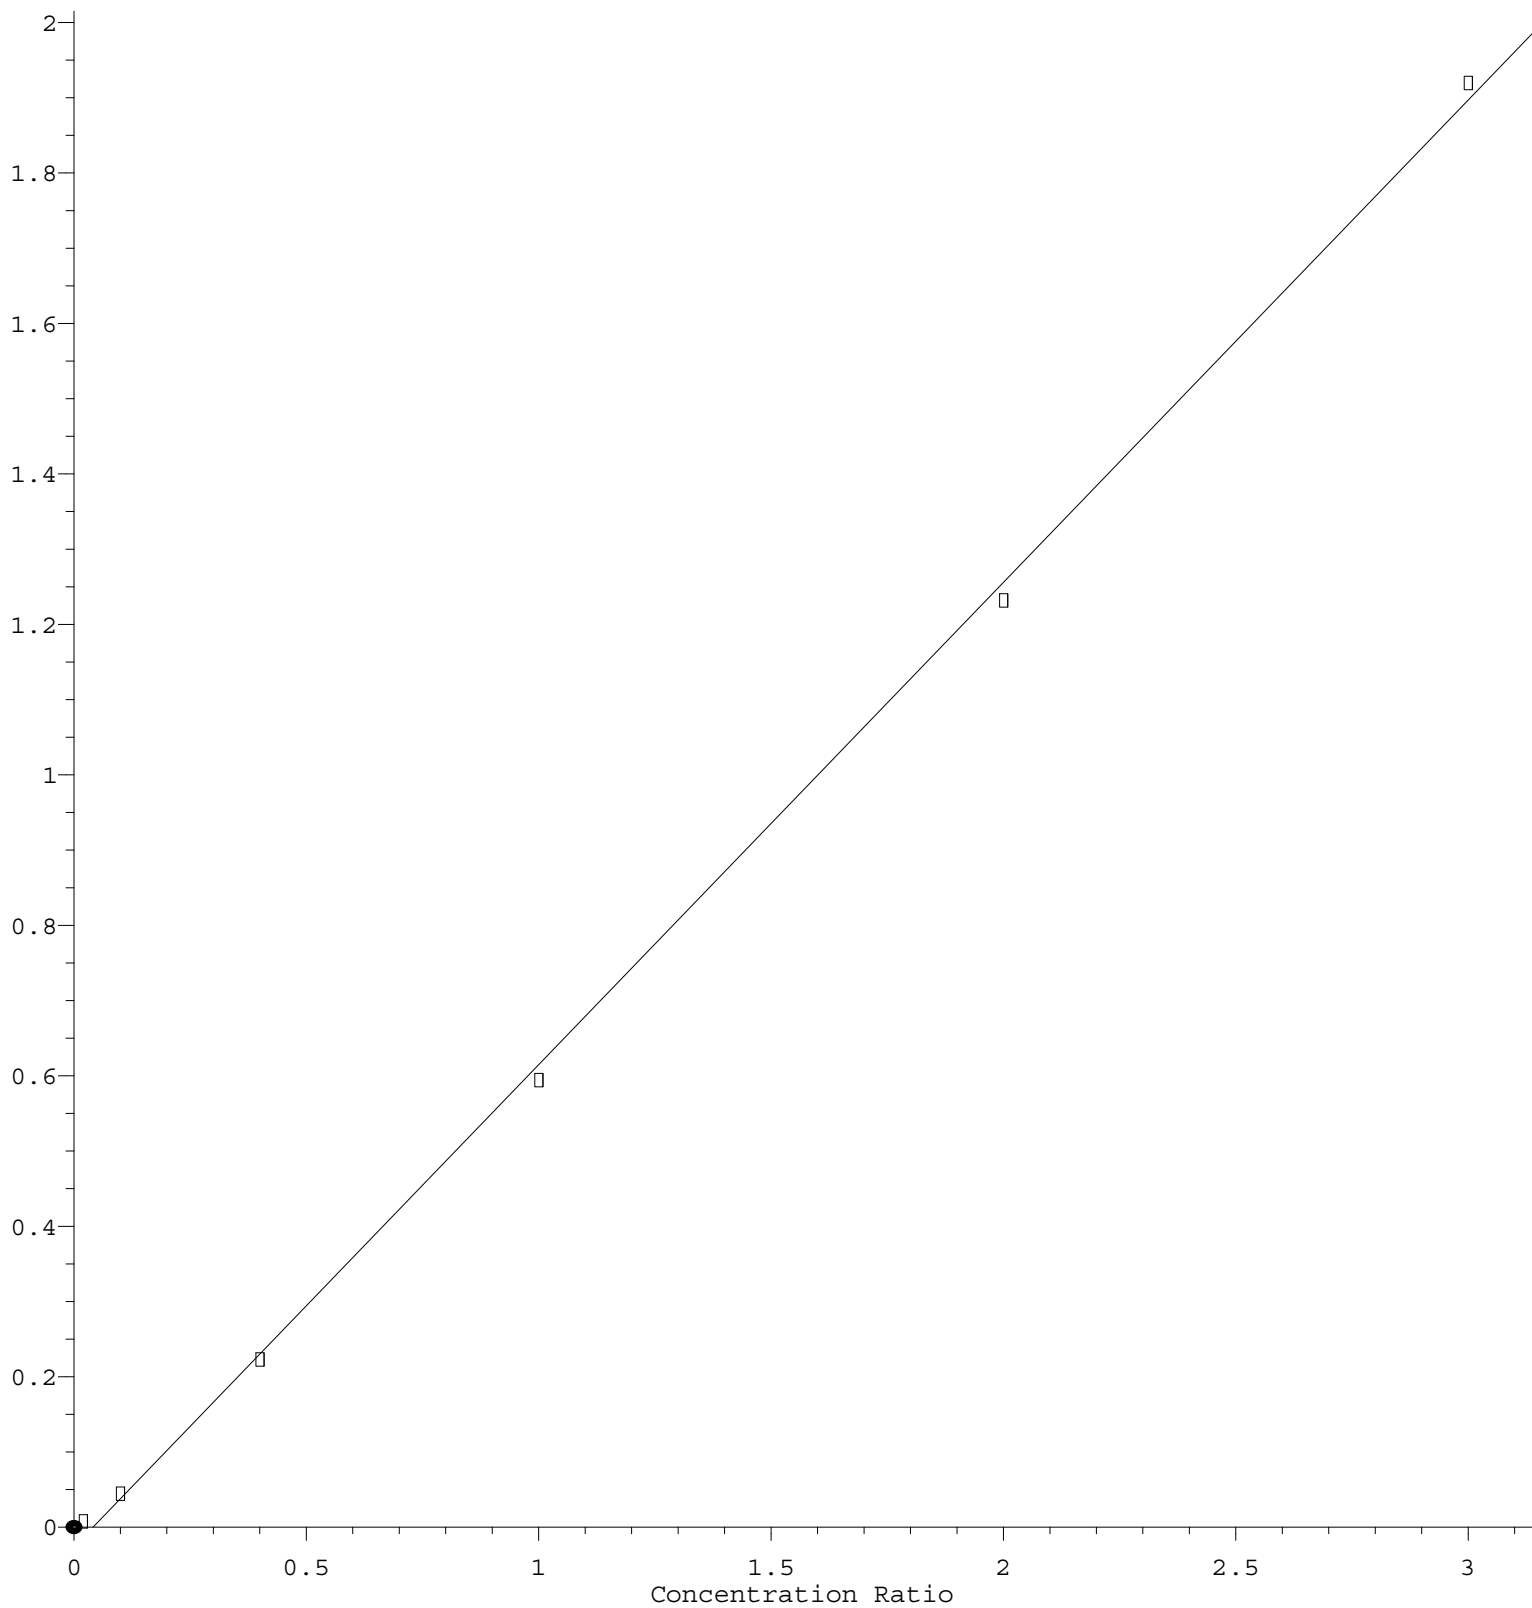

$$\text{Response} = 6.409\text{e-}001 * \text{Amt} - 2.631\text{e-}002$$


Coef of Det (r^2) = 0.999294 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M

Calibration Table Last Updated: Tue Nov 09 18:18:22 2021

t-1,3-Dichloropropene

Response Ratio

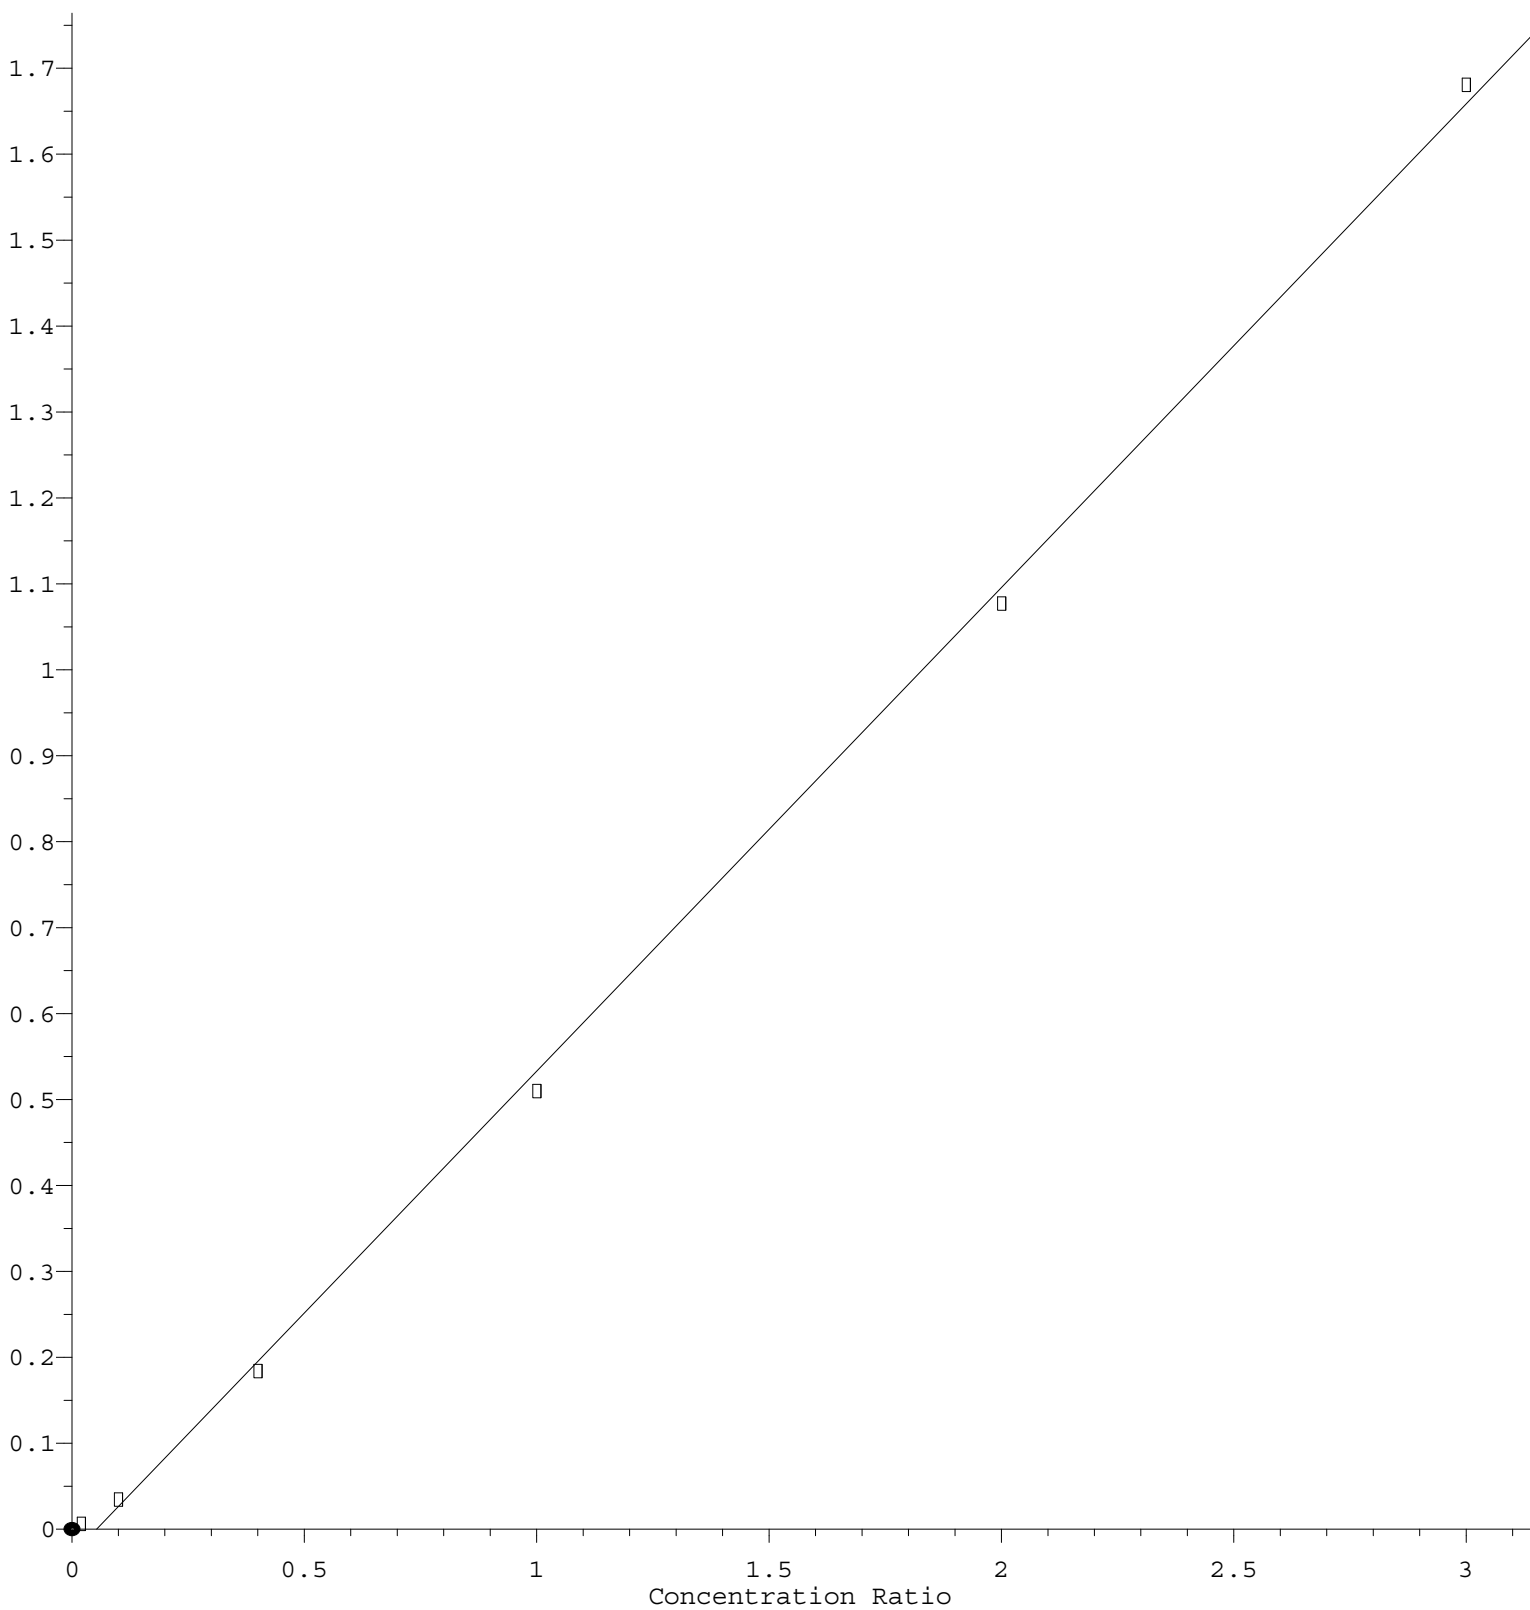


$$\text{Response} = 5.629\text{e-}001 * \text{Amt} - 2.969\text{e-}002$$

Coef of Det (r^2) = 0.999031 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M


Calibration Table Last Updated: Tue Nov 09 18:18:22 2021

1,4-Dioxane

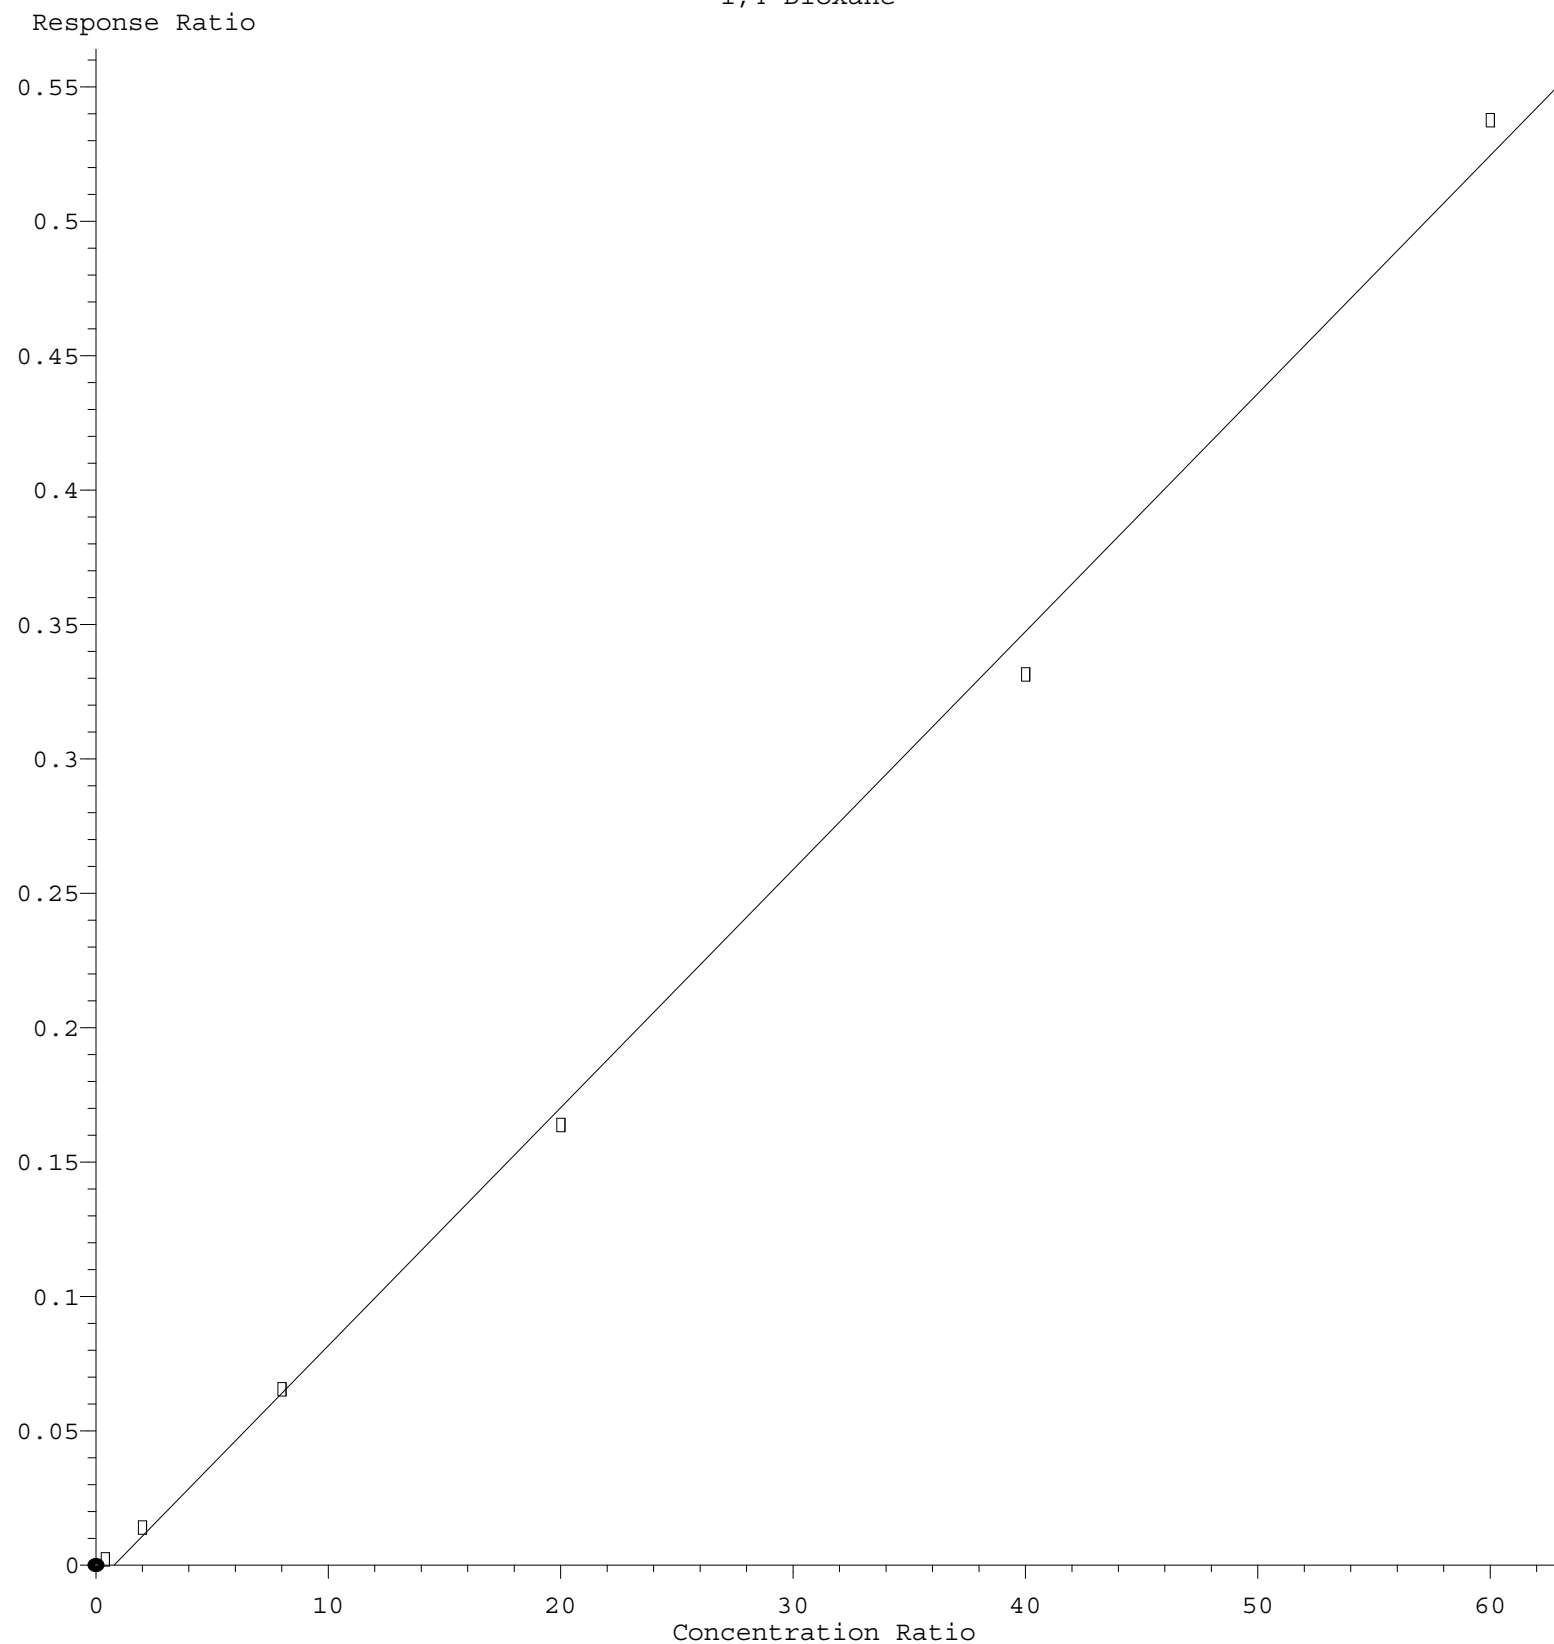

$\text{Response} = 8.863\text{e-}003 * \text{Amt} - 6.924\text{e-}003$
 Coef of Det (r^2) = 0.997714 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M
 Calibration Table Last Updated: Tue Nov 09 18:18:22 2021


Acrolein

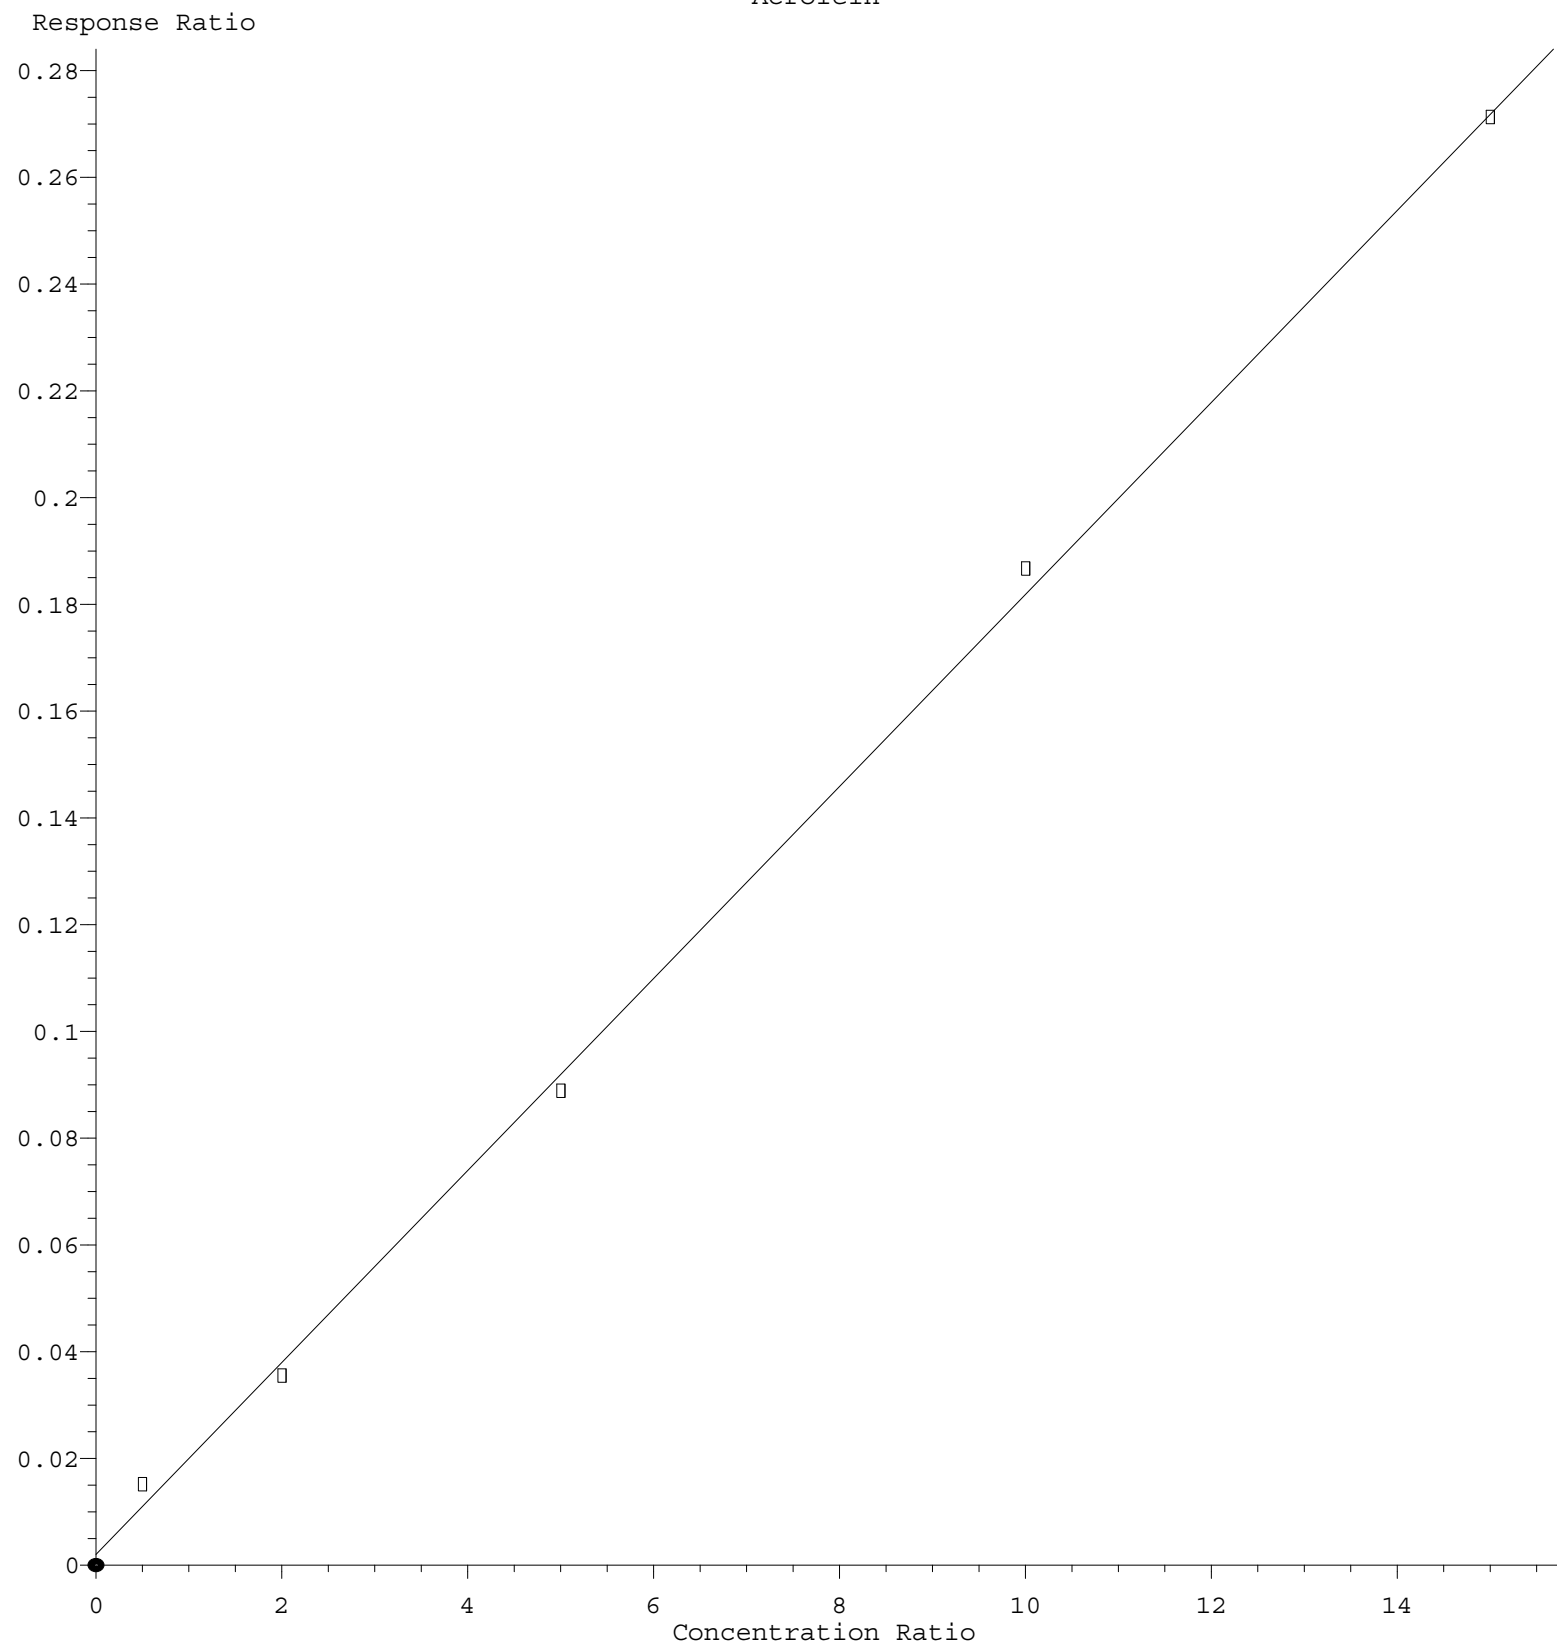

$\text{Response} = 1.801\text{e-}002 * \text{Amt} + 2.446\text{e-}003$
 Coef of Det (r^2) = 0.998823 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M
 Calibration Table Last Updated: Tue Nov 09 18:18:22 2021

1,2,4-Trichlorobenzene

Response Ratio

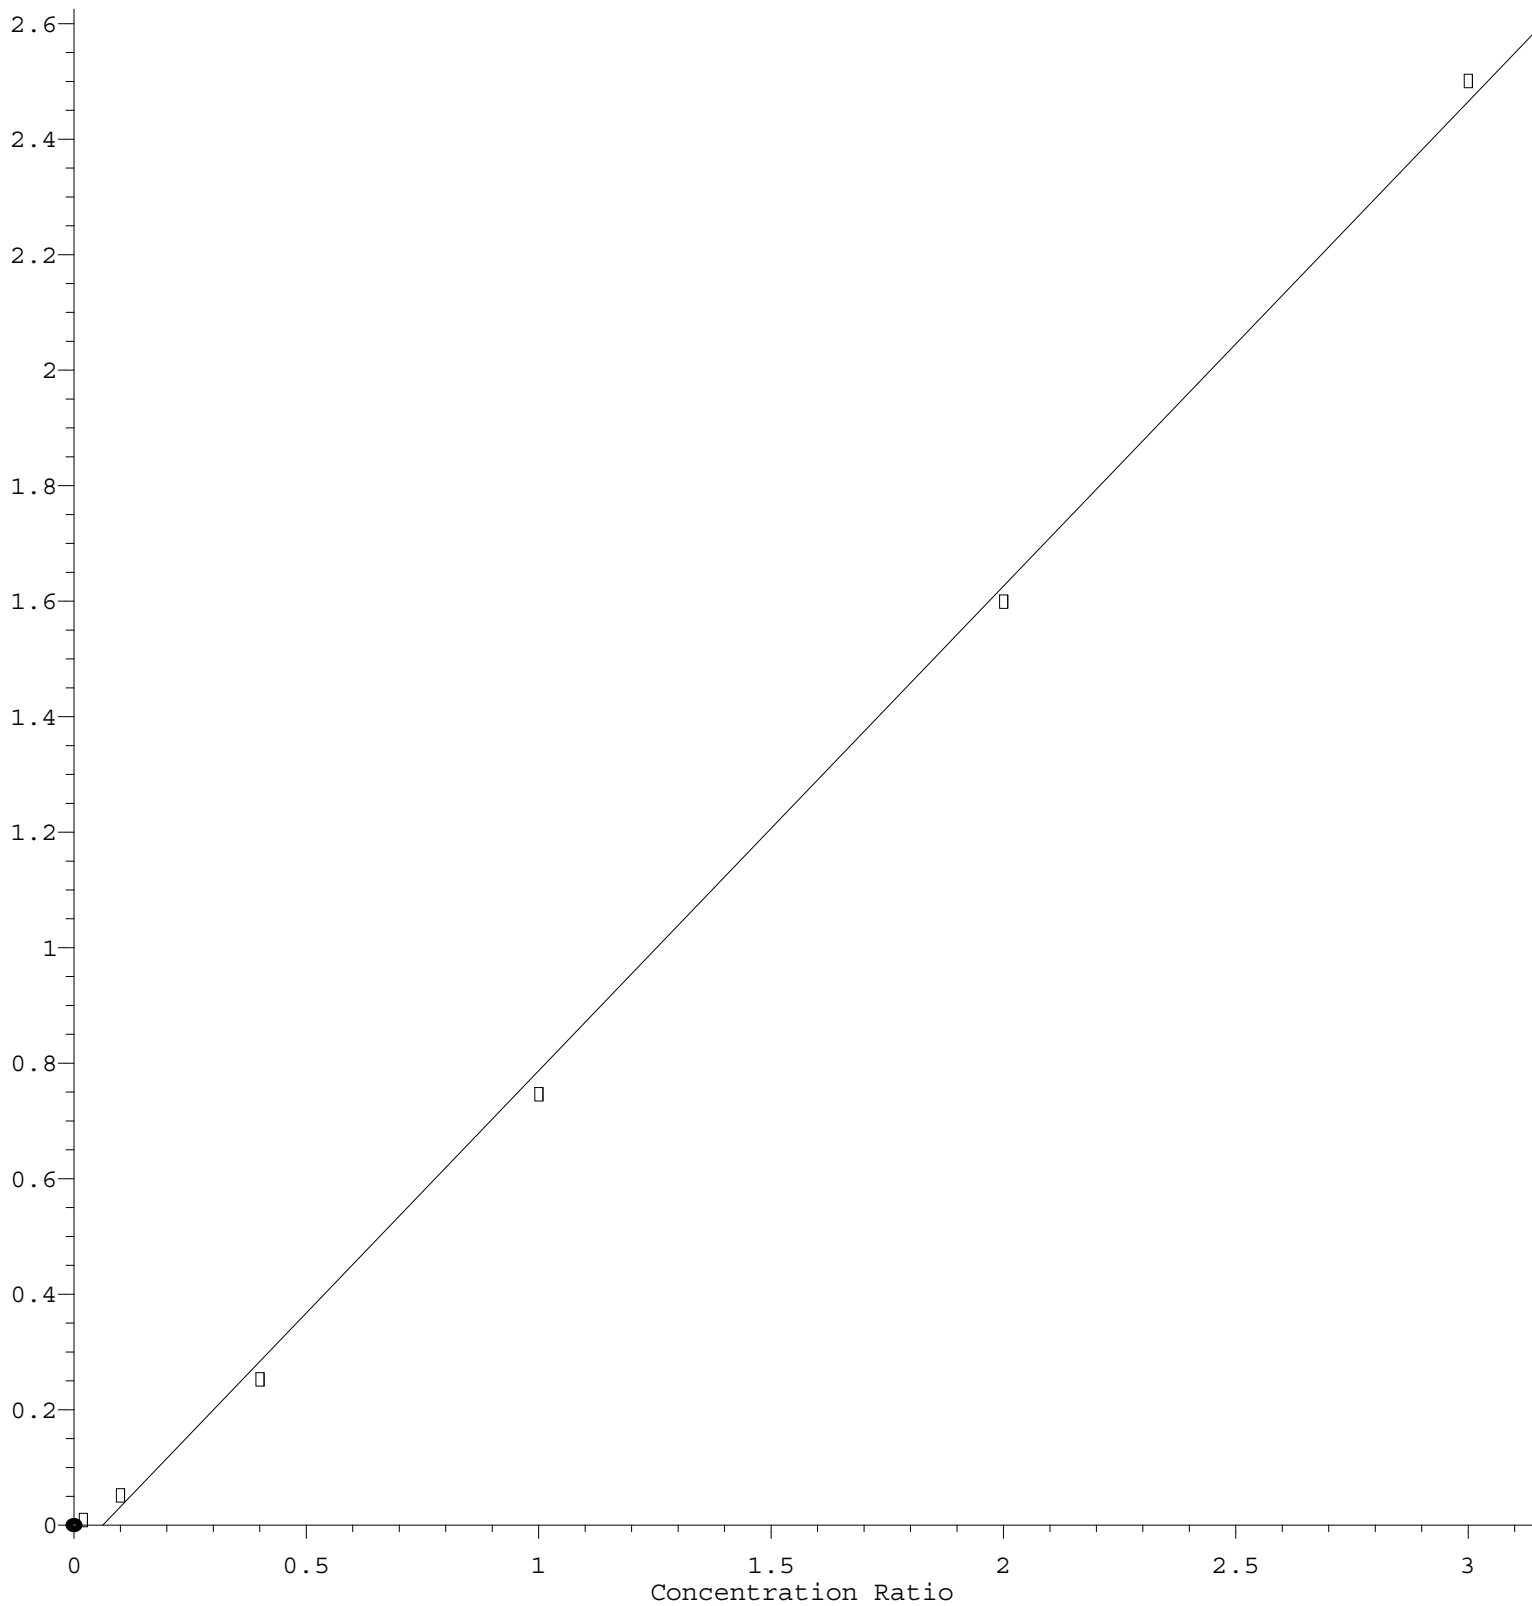

$$\text{Response} = 8.393\text{e-}001 * \text{Amt} - 5.226\text{e-}002$$

Coef of Det (r^2) = 0.998605 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N110921W.M

Calibration Table Last Updated: Tue Nov 09 18:18:22 2021