
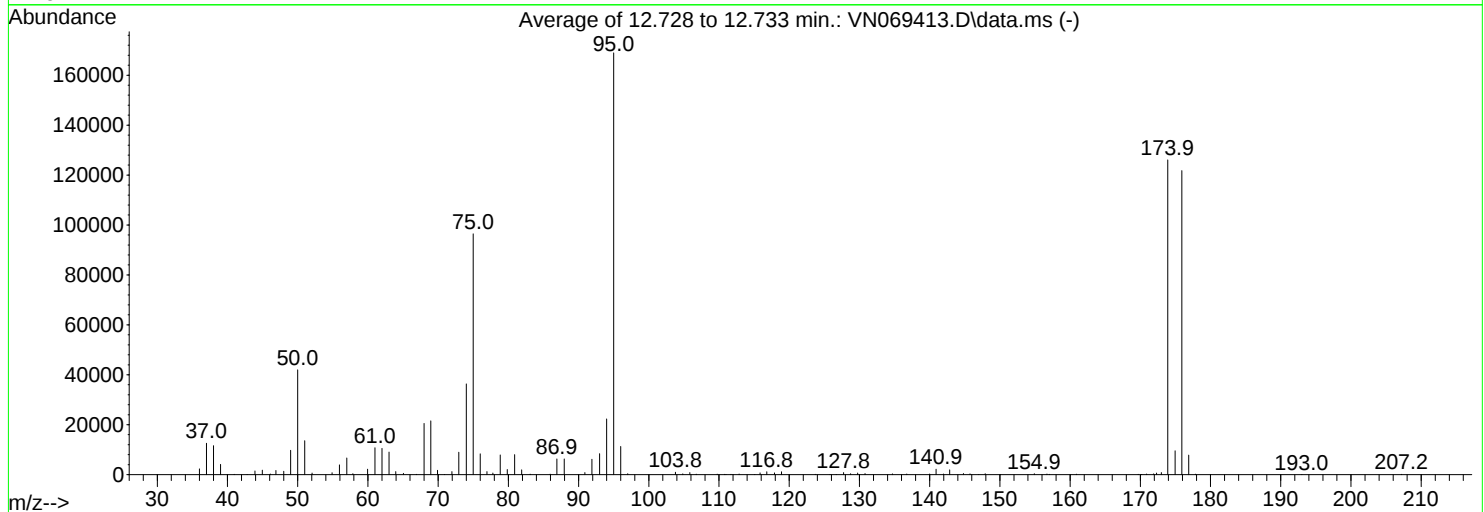


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110921\
 Data File : VN069413.D
 Acq On : 9 Nov 2021 9:12
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
 Title : SW846 8260
 Last Update : Tue Nov 09 18:18:22 2021

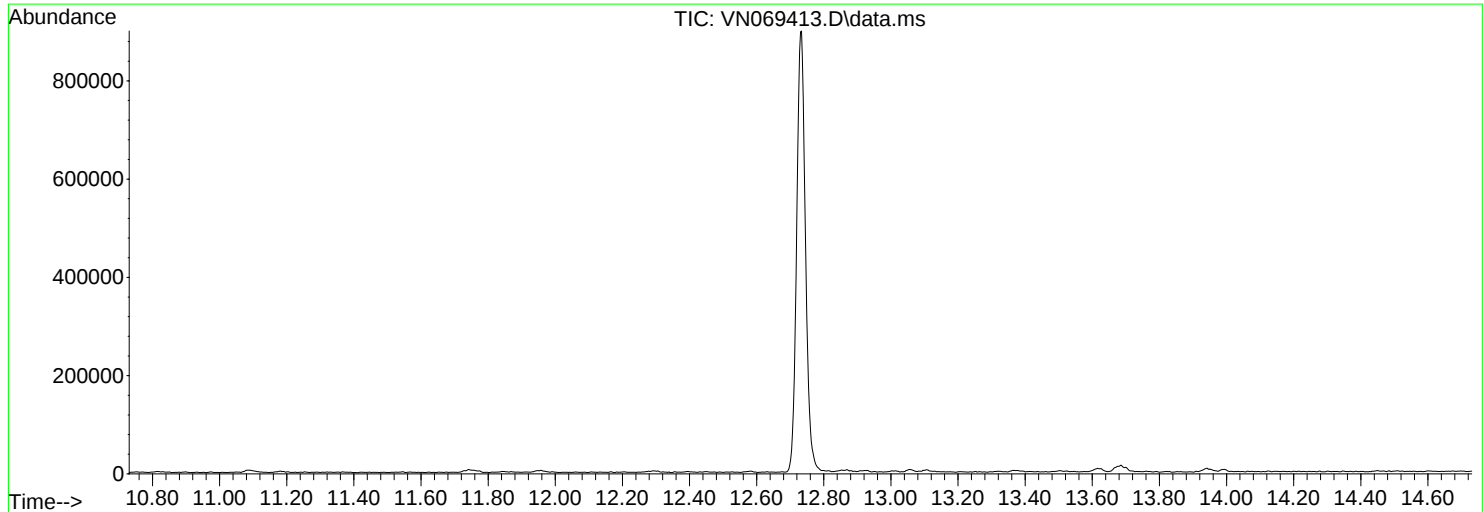

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3986

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.8	41965	PASS
75	95	30	60	57.1	96440	PASS
95	95	100	100	100.0	168960	PASS
96	95	5	9	6.7	11309	PASS
173	174	0.00	2	0.6	815	PASS
174	95	50	100	74.6	126072	PASS
175	174	5	9	7.6	9532	PASS
176	174	95	101	96.6	121765	PASS
177	176	5	9	6.4	7842	PASS