
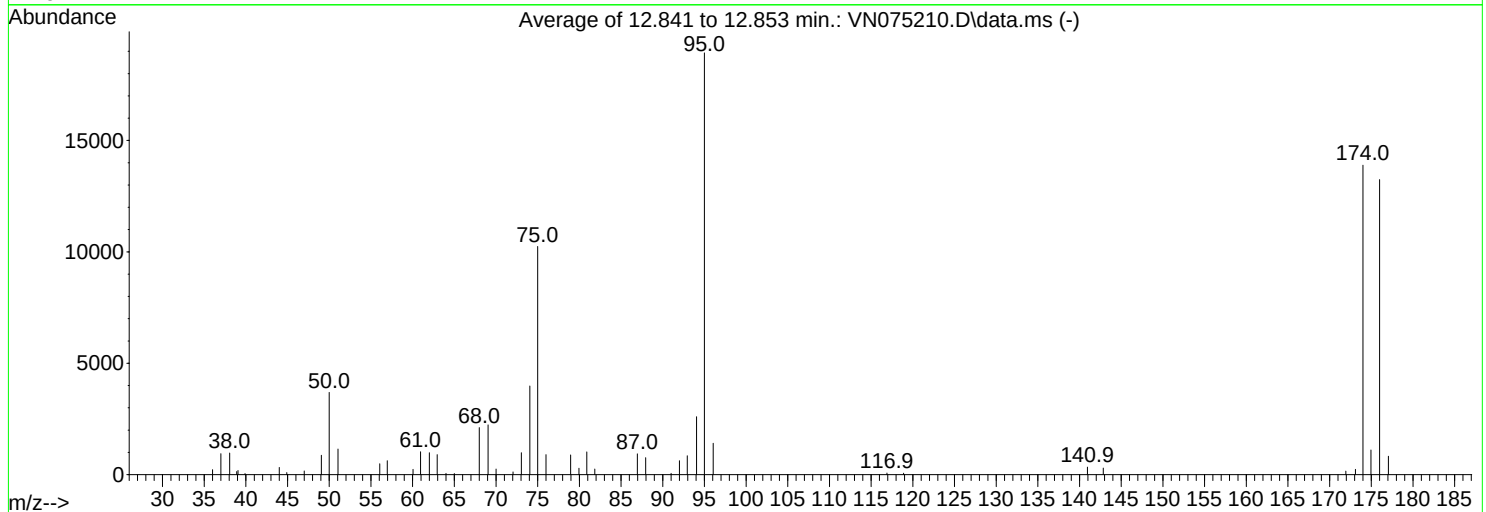


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN110922\  
Data File : VN075210.D  
Acq On : 09 Nov 2022 09:49  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N102622W.M  
Title : SW846 8260  
Last Update : Thu Oct 27 09:48:49 2022

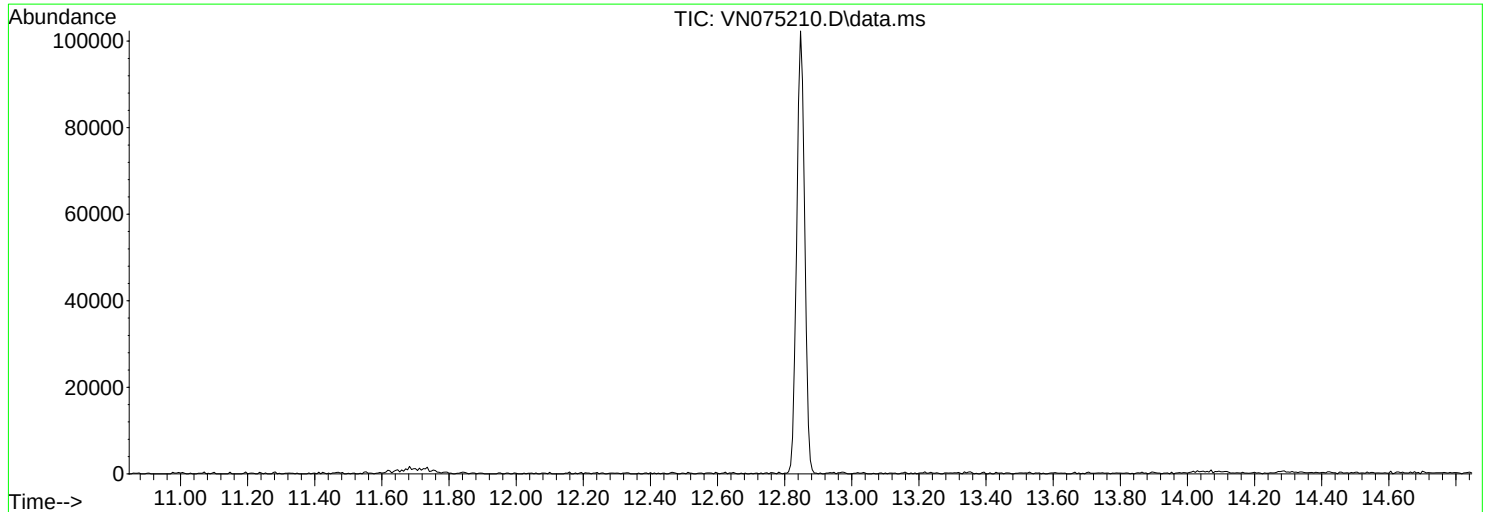

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1826

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 19.5  | 3691  | PASS      |
| 75     | 95      | 30     | 60     | 54.1  | 10243 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 18931 | PASS      |
| 96     | 95      | 5      | 9      | 7.4   | 1408  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.7   | 237   | PASS      |
| 174    | 95      | 50     | 100    | 73.4  | 13886 | PASS      |
| 175    | 174     | 5      | 9      | 8.0   | 1105  | PASS      |
| 176    | 174     | 95     | 101    | 95.4  | 13241 | PASS      |
| 177    | 176     | 5      | 9      | 6.2   | 827   | PASS      |

Average of 12.841 to 12.853 min.: VN075210.D\data.ms

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z    | abund. |
|-------|--------|-------|--------|-------|--------|--------|--------|
| 36.00 | 221    | 51.05 | 1146   | 70.00 | 255    | 87.95  | 76     |
| 37.00 | 939    | 56.05 | 492    | 72.05 | 123    | 91.00  | 5      |
| 38.05 | 973    | 56.95 | 623    | 73.05 | 983    | 92.00  | 62     |
| 38.90 | 138    | 60.05 | 235    | 74.05 | 3977   | 92.95  | 84     |
| 39.05 | 189    | 60.95 | 1027   | 75.00 | 10243  | 94.05  | 2600   |
| 39.90 | 53     | 62.00 | 982    | 76.00 | 900    | 95.00  | 18931  |
| 44.00 | 322    | 62.95 | 901    | 78.95 | 881    | 96.05  | 1408   |
| 44.90 | 90     | 64.00 | 59     | 79.95 | 288    | 116.90 | 72     |
| 47.00 | 165    | 65.00 | 54     | 80.90 | 1021   | 118.90 | 65     |
| 49.05 | 867    | 68.00 | 2115   | 81.85 | 250    | 140.95 | 335    |
| 50.00 | 3691   | 69.05 | 2235   | 86.95 | 936    | 142.85 | 298    |

Average of 12.841 to 12.853 min.: VN075210.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z | abund. | m/z | abund. | m/z | abund. |
|--------|--------|-----|--------|-----|--------|-----|--------|
| 171.95 | 157    |     |        |     |        |     |        |
| 173.10 | 237    |     |        |     |        |     |        |
| 174.00 | 13886  |     |        |     |        |     |        |
| 174.95 | 1105   |     |        |     |        |     |        |
| 176.00 | 13241  |     |        |     |        |     |        |
| 177.05 | 827    |     |        |     |        |     |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB