


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110923\
Data File : VN080021.D
Acq On : 09 Nov 2023 12:55
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Title : SW846 8260
Last Update : Thu Nov 02 05:49:08 2023

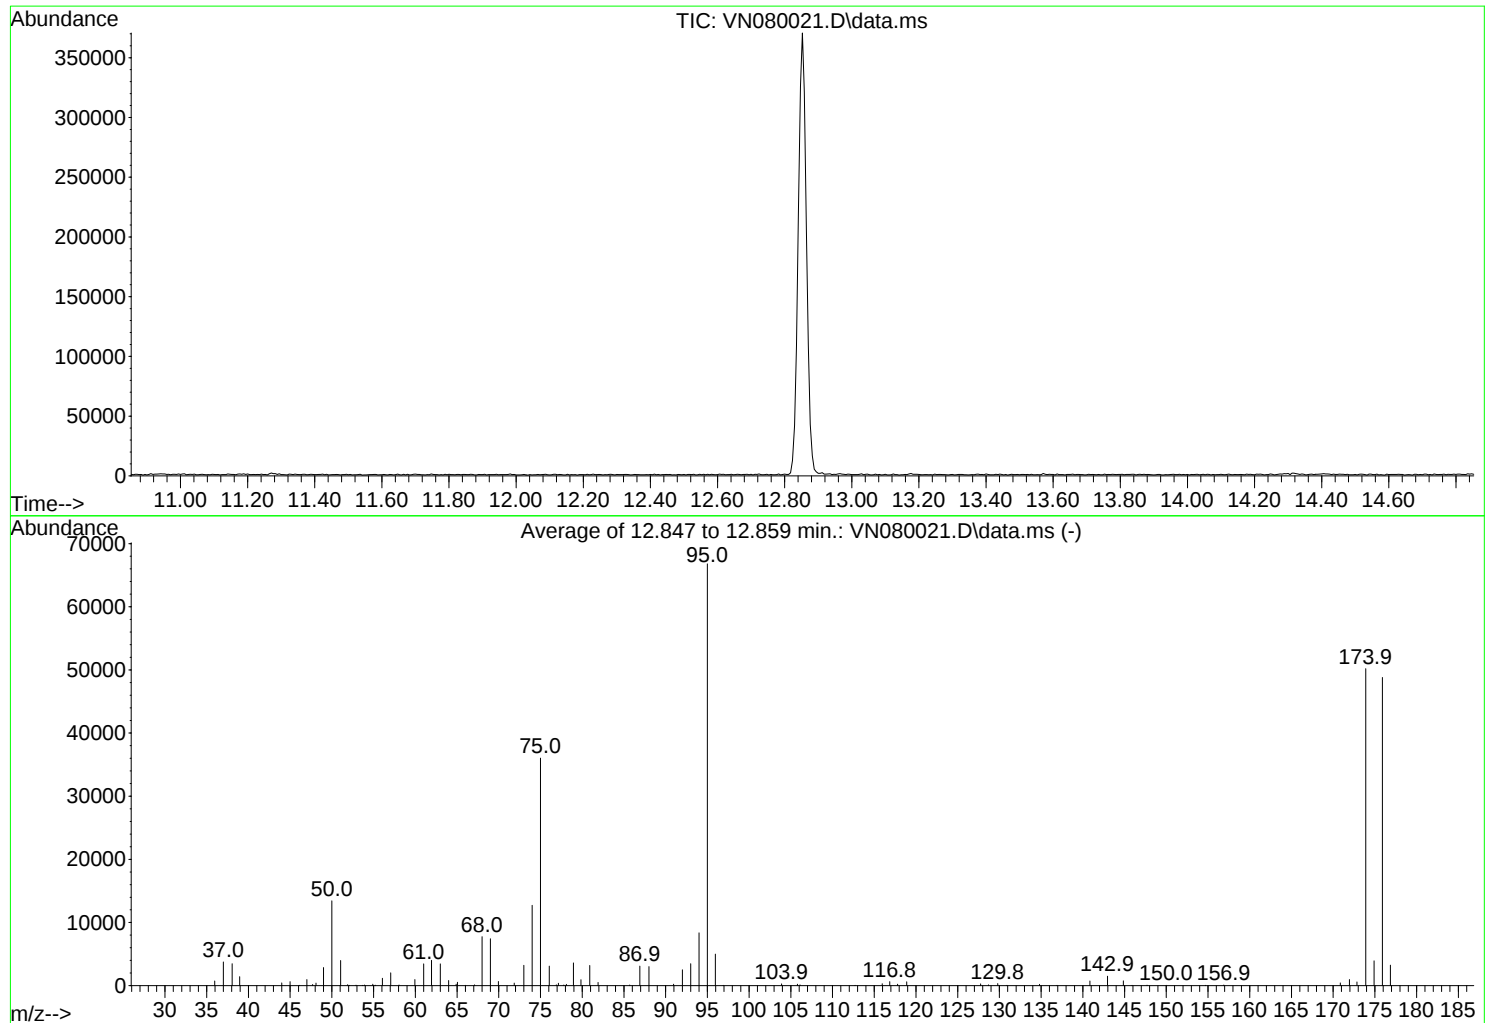

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	13434	PASS
75	95	30	60	53.9	36032	PASS
95	95	100	100	100.0	66803	PASS
96	95	5	9	7.5	4998	PASS
173	174	0.00	2	1.1	576	PASS
174	95	50	100	75.2	50208	PASS
175	174	5	9	7.8	3924	PASS
176	174	95	101	97.2	48811	PASS
177	176	5	9	6.7	3257	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	726	50.00	13434	58.05	113	69.00	742
37.00	3744	51.05	3979	59.95	954	69.95	65
38.05	3476	51.90	165	61.00	3456	71.85	41
38.95	1408	52.10	64	61.95	4001	73.00	323
44.00	426	52.90	74	63.00	3451	74.00	12712
45.00	644	53.70	53	64.00	812	75.00	36032
46.10	56	53.90	111	64.90	226	76.05	3080
47.00	963	54.90	238	65.05	524	76.90	137
47.70	172	55.20	84	66.00	56	77.15	377
48.10	400	56.05	1169	67.10	133	77.80	104
49.00	2858	57.05	2029	68.00	7746	78.10	213

Average of 12.847 to 12.859 min.: VN080021.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	3601	95.00	66803	127.75	273	150.00	59
79.85	947	95.95	4998	128.70	127	154.70	64
80.90	3207	96.90	55	129.80	325	156.90	114
81.90	506	103.90	283	130.90	63	170.85	429
85.70	93	105.80	232	134.80	215	171.95	969
86.90	3089	106.10	140	136.90	63	172.85	576
88.00	3007	112.70	52	140.85	734	173.90	50208
90.95	234	115.95	300	142.95	1502	174.90	3924
92.00	2503	116.85	647	144.85	770	175.90	48811
93.00	3464	117.80	241	145.90	54	176.85	3257
94.00	8365	118.90	617	147.70	76		

Instrument :

MSVOA_N

ClientSampleId :

BFB