

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN111020\
 Data File : VN064540.D
 Acq On : 10 Nov 2020 21:02
 Operator : JC/MD
 Sample : L4680-08
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PAV-B7-110920-19-20

Quant Time: Nov 11 01:56:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 04 12:09:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	240430	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	514439	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	566592	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	204634	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	237039	56.60	ug/l	0.00
Spiked Amount			Recovery	=	113.20%	
35) Dibromofluoromethane	7.55	113	177414	50.65	ug/l	0.00
Spiked Amount			Recovery	=	101.30%	
50) Toluene-d8	10.06	98	676058	49.94	ug/l	0.00
Spiked Amount			Recovery	=	99.88%	
62) 4-Bromofluorobenzene	12.38	95	255983	50.00	ug/l	0.00
Spiked Amount			Recovery	=	100.00%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acrolein	3.49	56	133	0.464	ug/l #	42
16) Acetone	3.79	43	9956	6.241	ug/l	99
18) Methyl Acetate	4.28	43	1003	0.320	ug/l #	69
20) Methylene Chloride	4.50	84	6903	2.181	ug/l	97
25) 2-Butanone	6.80	43	493	0.243	ug/l #	52
29) Tetrahydrofuran	7.18	42	297	0.238	ug/l #	64
31) Cyclohexane	7.63	56	7238	1.422	ug/l #	36
36) 1,1-Dichloropropene	7.62	75	23104	4.251	ug/l #	51
37) Ethyl Acetate	6.89	43	193	0.797	ug/l #	71
38) Carbon Tetrachloride	7.63	117	27940	4.810	ug/l #	18
43) Isopropyl Acetate	8.13	43	44707	5.076	ug/l	97
45) 1,2-Dichloropropane	9.24	63	2600	0.610	ug/l #	45
48) Methyl methacrylate	9.14	41	7788	1.752	ug/l #	15
49) 1,4-Dioxane	9.23	88	62	1.059	ug/l #	1
51) 4-Methyl-2-Pentanone	9.96	43	7483	1.457	ug/l	89
54) cis-1,3-Dichloropropene	9.87	75	53071	7.763	ug/l #	67
56) Ethyl methacrylate	10.51	69	1603	2.088	ug/l #	1
57) 1,3-Dichloropropane	10.74	76	33253	5.015	ug/l #	42
59) 2-Hexanone	10.74	43	513681	124.700	ug/l #	54
71) Bromoform	12.36	173	156	1.319	ug/l #	1
74) N-amyl acetate	12.03	43	888	1.324	ug/l #	53
76) 1,2,3-Trichloropropane	12.38	75	144095	29.062	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.71	105	3075	0.229	ug/l	100
81) trans-1,4-Dichloro-2-buten	12.38	75	144095	81.146	ug/l #	8
95) Naphthalene	15.12	128	61	3.628	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN111020\
Data File : VN064540.D
Acq On : 10 Nov 2020 21:02
Operator : JC/MD
Sample : L4680-08
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PAV-B7-110920-19-20

Quant Time: Nov 11 01:56:24 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 04 12:09:03 2020
Response via : Initial Calibration





#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064540.D

Acq: 10 Nov 2020 21:02

Instrument :

MSVOA_N

ClientSampleId :


PAV-B7-110920-19-20

Tot Ion:168 Resp: 240430

Ion Ratio Lower Upper




168 100

99 68.4 53.4 80.2



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO



#13

Acrolein

Concen: 0.464 ug/l

RT: 3.49 min Scan# 544

Delta R.T. -0.08 min

Lab File: VN064540.D


Acq: 10 Nov 2020 21:02

Tgt Ion: 56 Resp: 133

Ion Ratio Lower Upper



56 100


55 117.3 55.9 83.9#



Abundance Ion 56.00 (55.70 to 56.70): VNO

Ion 55.00 (54.70 to 55.70): VNO









#16
 Acetone
 Concen: 6.241 ug/l
 RT: 3.79 min Scan# 637
 Delta R.T. 0.01 min
 Lab File: VN064540.D
 Acq: 10 Nov 2020 21:02




Instrument :
 MSVOA_N
 ClientSampleId :
 PAV-B7-110920-19-20


Tot Ion: 43 Resp: 9956
 Ion Ratio Lower Upper
 43 100
 58 27.2 21.4 32.0

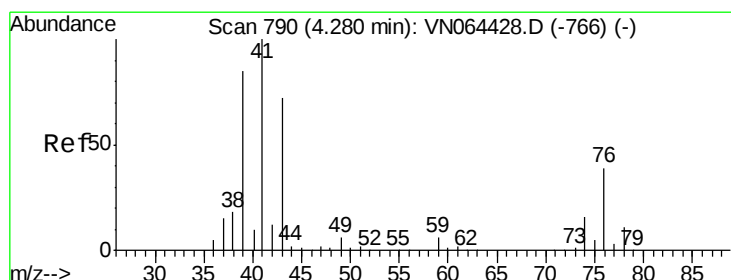

#18
 Methyl Acetate
 Concen: 0.320 ug/l
 RT: 4.28 min Scan# 790
 Delta R.T. -0.00 min
 Lab File: VN064540.D
 Acq: 10 Nov 2020 21:02

Tgt Ion: 43 Resp: 1003
 Ion Ratio Lower Upper
 43 100
 74 6.8 17.0 25.4#









#20
Methvlene Chloride
Concen: 2.181 ug/l
RT: 4.50 min Scan# 858
Delta R.T. -0.01 min
Lab File: VN064540.D
Acq: 10 Nov 2020 21:02




Instrument :
MSVOA_N
ClientSampleId :
PAV-B7-110920-19-20


Tot Ion:	84	Resp:	6903
Ion	Ratio	Lower	Upper
84	100		
49	139.2	110.1	165.1
51	49.4	33.6	50.4
86	64.6	52.1	78.1



#25
2-Butanone
Concen: 0.243 ug/l
RT: 6.80 min Scan# 1573
Delta R.T. 0.01 min
Lab File: VN064540.D
Acq: 10 Nov 2020 21:02

Tgt Ion:	43	Resp:	493
Ion	Ratio	Lower	Upper
43	100		
72	0.0	18.5	27.7#





#29

Tetrahydrofuran

Concen: 0.238 ug/l

RT: 7.18 min Scan# 1692

Delta R.T. 0.01 min

Lab File: VN064540.D

Acq: 10 Nov 2020 21:02

Instrument :

MSVOA_N

ClientSampleId :

PAV-B7-110920-19-20


Tot Ion: 42 Resp: 297

Ion Ratio Lower Upper

42 100

72 0.0 31.7 47.5#

71 34.0 29.8 44.6



Abundance Ion 42.00 (41.70 to 42.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

Ion 71.00 (70.70 to 71.70): VN0

Time-->

7.16 7.17 7.18 7.19



400

300

200

100

0



#31

Cyclohexane

Concen: 1.422 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.02 min

Lab File: VN064540.D

Acq: 10 Nov 2020 21:02


Tgt Ion: 56 Resp: 7238

Ion Ratio Lower Upper

56 100

69 145.6 25.6 38.4#

84 85.5 63.0 94.6



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0

Time-->

7.55 7.60 7.65 7.70

5000


4000


3000

2000

1000

0





#33

1,2-Dichloroethane-d4

Concen: 56.601 ug/l

RT: 7.99 min Scan# 1944

Delta R.T. 0.00 min

Lab File: VN064540.D

Acq: 10 Nov 2020 21:02

Instrument :

MSVOA_N

ClientSampleId :


PAV-B7-110920-19-20

Tot Ion: 65 Resp: 237039

Ion Ratio Lower Upper




65 100

67 49.9 0.0 101.6



Abundance Ion 64.90 (64.60 to 65.60): VN064540.D (-1850) (-)

Ion 66.90 (66.60 to 67.60): VN064540.D (-1850) (-)



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2118

Delta R.T. -0.00 min

Lab File: VN064540.D

Acq: 10 Nov 2020 21:02


Tgt Ion: 114 Resp: 514439

Ion Ratio Lower Upper

114 100

63 22.5 0.0 45.6



88 15.3 0.0 32.8




Abundance Ion 113.90 (113.60 to 114.60): VN064540.D (-2025) (-)

Ion 63.00 (62.70 to 63.70): VN064540.D (-2025) (-)

Ion 87.90 (87.60 to 88.60): VN064540.D (-2025) (-)









#35
 Dibromofluoromethane
 Concen: 50.652 ug/l
 RT: 7.55 min Scan# 1808
 Delta R.T. 0.01 min
 Lab File: VN064540.D
 Acq: 10 Nov 2020 21:02




Instrument :
 MSVOA_N
 ClientSampleId :
 PAV-B7-110920-19-20

Tot Ion:113 Resp: 177414
 Ion Ratio Lower Upper
 113 100
 111 102.1 81.1 121.7
 192 17.2 12.8 19.2



#36
 1,1-Dichloropropene
 Concen: 4.251 ug/l
 RT: 7.62 min Scan# 1829
 Delta R.T. -0.13 min
 Lab File: VN064540.D
 Acq: 10 Nov 2020 21:02

Tgt Ion: 75 Resp: 23104
 Ion Ratio Lower Upper
 75 100
 110 8.5 16.0 48.0#
 77 0.0 24.0 36.0#









#37
Ethyl Acetate
Concen: 0.797 ug/l
RT: 6.89 min Scan# 1602
Delta R.T. 0.01 min
Lab File: VN064540.D
Acq: 10 Nov 2020 21:02




Instrument :
MSVOA_N
ClientSampleId :
PAV-B7-110920-19-20


Tot Ion: 43 Resp: 193
Ion Ratio Lower Upper
43 100
61 0.0 10.0 15.0#
70 0.0 7.1 10.7#



#38
Carbon Tetrachloride
Concen: 4.810 ug/l
RT: 7.63 min Scan# 1831
Delta R.T. -0.11 min
Lab File: VN064540.D
Acq: 10 Nov 2020 21:02

Tgt Ion: 117 Resp: 27940
Ion Ratio Lower Upper
117 100
119 6.5 75.5 113.3#
121 0.0 24.4 36.6#





#43

Isopropyl Acetate

Concen: 5.076 ug/l

RT: 8.13 min Scan# 1988

Delta R.T. 0.01 min

Lab File: VN064540.D

Acq: 10 Nov 2020 21:02

Instrument :

MSVOA_N

ClientSampleId :

PAV-B7-110920-19-20


Tot Ion: 43 Resp: 44707

Ion Ratio Lower Upper

43 100

61 16.0 14.0 21.0




87 10.4 9.1 13.7



Abundance Ion 43.00 (42.70 to 43.70): VN064540.D (-1988) (-)

Ion 61.00 (60.70 to 61.70): VN064540.D (-1988) (-)

Ion 87.00 (86.70 to 87.70): VN064540.D (-1988) (-)



#45

1,2-Dichloropropane

Concen: 0.610 ug/l

RT: 9.24 min Scan# 2333

Delta R.T. 0.16 min

Lab File: VN064540.D


Acq: 10 Nov 2020 21:02

Tgt Ion: 63 Resp: 2600

Ion Ratio Lower Upper



63 100


65 0.0 23.6 35.4#



Abundance Ion 62.90 (62.60 to 63.60): VN064540.D (-2333) (-)

Ion 64.90 (64.60 to 65.60): VN064540.D (-2333) (-)







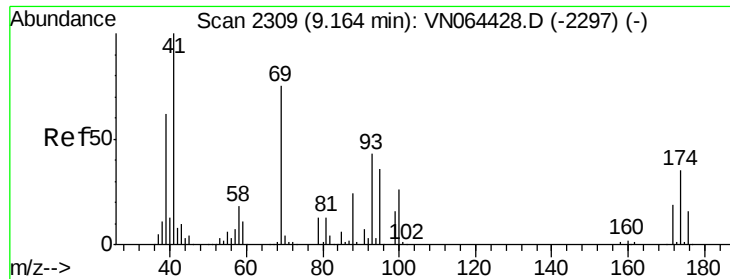

#48
Methvl methacrylate
Concen: 1.752 ug/l
RT: 9.14 min Scan# 2303
Delta R.T. -0.02 min
Lab File: VN064540.D
Acq: 10 Nov 2020 21:02




Instrument :
MSVOA_N
ClientSampleId :
PAV-B7-110920-19-20


Tot Ion: 41 Resp: 7788
Ion Ratio Lower Upper
41 100
69 0.0 60.4 90.6#
39 0.0 51.2 76.8#



#49
1,4-Dioxane
Concen: 1.059 ug/l
RT: 9.23 min Scan# 2329
Delta R.T. 0.06 min
Lab File: VN064540.D
Acq: 10 Nov 2020 21:02

Tgt Ion: 88 Resp: 62
Ion Ratio Lower Upper
88 100
43 3254687.1 31.0 46.6#
58 16514.5 58.4 87.6#





#50

Toluene-d8

Concen: 49.939 ug/l

RT: 10.06 min Scan# 2588

Delta R.T. 0.00 min

Lab File: VN064540.D

Acq: 10 Nov 2020 21:02

Instrument :

MSVOA_N

ClientSampleId :


PAV-B7-110920-19-20

Tot Ion: 98 Resp: 676058

Ion Ratio Lower Upper

98 100

100 63.7 50.7 76.1



Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN

10.06

400000



300000

200000

100000

0

Time-->



#51

4-Methyl-2-Pentanone

Concen: 1.457 ug/l

RT: 9.96 min Scan# 2555

Delta R.T. 0.00 min

Lab File: VN064540.D


Acq: 10 Nov 2020 21:02

Tgt Ion: 43 Resp: 7483

Ion Ratio Lower Upper

43 100

58 29.3 28.4 42.6



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

10000

8000


6000


4000

2000

0

Time-->









#54

cis-1,3-Dichloropropene
 Concen: 7.763 ug/l
 RT: 9.87 min Scan# 2530
 Delta R.T. 0.07 min
 Lab File: VN064540.D
 Acq: 10 Nov 2020 21:02

Instrument :
 MSVOA_N
 ClientSampleId :
 PAV-B7-110920-19-20




Tot Ion	Ratio	Lower	Upper
75	100		
77	0.0	24.9	37.3#
39	43.7	47.1	70.7#




#56

Ethyl methacrylate
 Concen: 2.088 ug/l
 RT: 10.51 min Scan# 2728
 Delta R.T. 0.11 min
 Lab File: VN064540.D
 Acq: 10 Nov 2020 21:02

Tgt Ion	Ratio	Lower	Upper
69	100		
41	2320.1	59.3	88.9#
39	1078.9	35.4	53.0#









#57
 1,3-Dichloropropane
 Concen: 5.015 ug/l
 RT: 10.74 min Scan# 2798
 Delta R.T. 0.06 min
 Lab File: VN064540.D
 Acq: 10 Nov 2020 21:02




Instrument :
 MSVOA_N
 ClientSampleId :
 PAV-B7-110920-19-20


Tot Ion: 76 Resp: 33253
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.8 38.6#



#59
 2-Hexanone
 Concen: 124.700 ug/l
 RT: 10.74 min Scan# 2798
 Delta R.T. 0.02 min
 Lab File: VN064540.D
 Acq: 10 Nov 2020 21:02

Tgt Ion: 43 Resp: 513681
 Ion Ratio Lower Upper
 43 100
 58 17.8 24.7 74.1#





#62

4-Bromofluorobenzene

Concen: 49.999 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.00 min

Lab File: VN064540.D

Acq: 10 Nov 2020 21:02

Instrument :

MSVOA_N

ClientSampleId :

PAV-B7-110920-19-20


Tot Ion: 95 Resp: 255983

Ion Ratio Lower Upper

95 100

174 70.2 0.0 132.6


176 66.9 0.0 129.2





Abundance Ion 94.90 (94.60 to 95.60): VN064428.D (-3293) (-)

Ion 173.80 (173.50 to 174.50): VN064428.D (-3293) (-)

Ion 175.80 (175.50 to 176.50): VN064428.D (-3293) (-)



Time-->



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.38 min Scan# 2998

Delta R.T. -0.00 min

Lab File: VN064540.D

Acq: 10 Nov 2020 21:02


Tgt Ion: 117 Resp: 566592

Ion Ratio Lower Upper

117 100

82 58.7 48.1 72.1


119 32.3 26.2 39.4




Abundance Ion 116.90 (116.60 to 117.60): VN064428.D (-2983) (-)


Ion 82.00 (81.70 to 82.70): VN064428.D (-2983) (-)

Ion 118.90 (118.60 to 119.60): VN064428.D (-2983) (-)



Time-->









#71
Bromoform
Concen: 1.319 ug/l
RT: 12.36 min Scan# 3302
Delta R.T. 0.26 min
Lab File: VN064540.D
Acq: 10 Nov 2020 21:02




Instrument :
MSVOA_N
ClientSampleId :
PAV-B7-110920-19-20


Tot Ion:173 Resp: 156
Ion Ratio Lower Upper
173 100
175 7123.7 23.7 71.1#
254 0.0 0.0 0.0



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN064540.D
Acq: 10 Nov 2020 21:02

Tgt Ion:152 Resp: 204634
Ion Ratio Lower Upper
152 100
115 64.4 32.0 96.0
150 157.2 0.0 353.8





#74

N-amvl acetate

Concen: 1.324 ug/l

RT: 12.03 min Scan# 3201

Delta R.T. -0.01 min

Lab File: VN064540.D

Acq: 10 Nov 2020 21:02

Instrument :

MSVOA_N

ClientSampleId :

PAV-B7-110920-19-20

Tot Ion: 43 Resp: 888


Ion Ratio Lower Upper

43 100

70 0.0 29.6 44.4#

55 12.2 18.4 27.6#

61 0.0 17.8 26.6#






Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 70.00 (69.70 to 70.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

Ion 61.00 (60.70 to 61.70): VN0



#76

1,2,3-Trichloropropane

Concen: 29.062 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.15 min

Lab File: VN064540.D


Acq: 10 Nov 2020 21:02

Tgt Ion: 75 Resp: 144095

Ion Ratio Lower Upper



75 100


77 1.1 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0









#80
 1,3,5-Trimethylbenzene
 Concen: 0.229 ug/l
 RT: 12.71 min Scan# 3411
 Delta R.T. -0.00 min
 Lab File: VN064540.D
 Acq: 10 Nov 2020 21:02




Instrument :
 MSVOA_N
 ClientSampleId :
 PAV-B7-110920-19-20


Tot Ion:105 Resp: 3075
 Ion Ratio Lower Upper
 105 100
 120 46.7 23.4 70.2



#81
 trans-1,4-Dichloro-2-butene
 Concen: 81.146 ug/l
 RT: 12.38 min Scan# 3308
 Delta R.T. 0.10 min
 Lab File: VN064540.D
 Acq: 10 Nov 2020 21:02

Tgt Ion: 75 Resp: 144095
 Ion Ratio Lower Upper
 75 100
 53 0.1 84.0 126.0#
 89 0.0 36.3 54.5#





#95

Napthalene

Concen: 3.628 ug/l

RT: 15.12 min Scan# 4160

Delta R.T. 0.02 min

Lab File: VN064540.D


Acq: 10 Nov 2020 21:02

Instrument :

MSVOA_N

ClientSampleId :

PAV-B7-110920-19-20




Tot Ion:128 Resp: 61

Ion Ratio Lower Upper

128 100

127 0.0 10.5 15.7#

129 0.0 8.8 13.2#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

