


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN111020\
 Data File : VN064516.D
 Acq On : 10 Nov 2020 10:37
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
 Title : SW846 8260
 Last Update : Wed Nov 04 12:09:03 2020

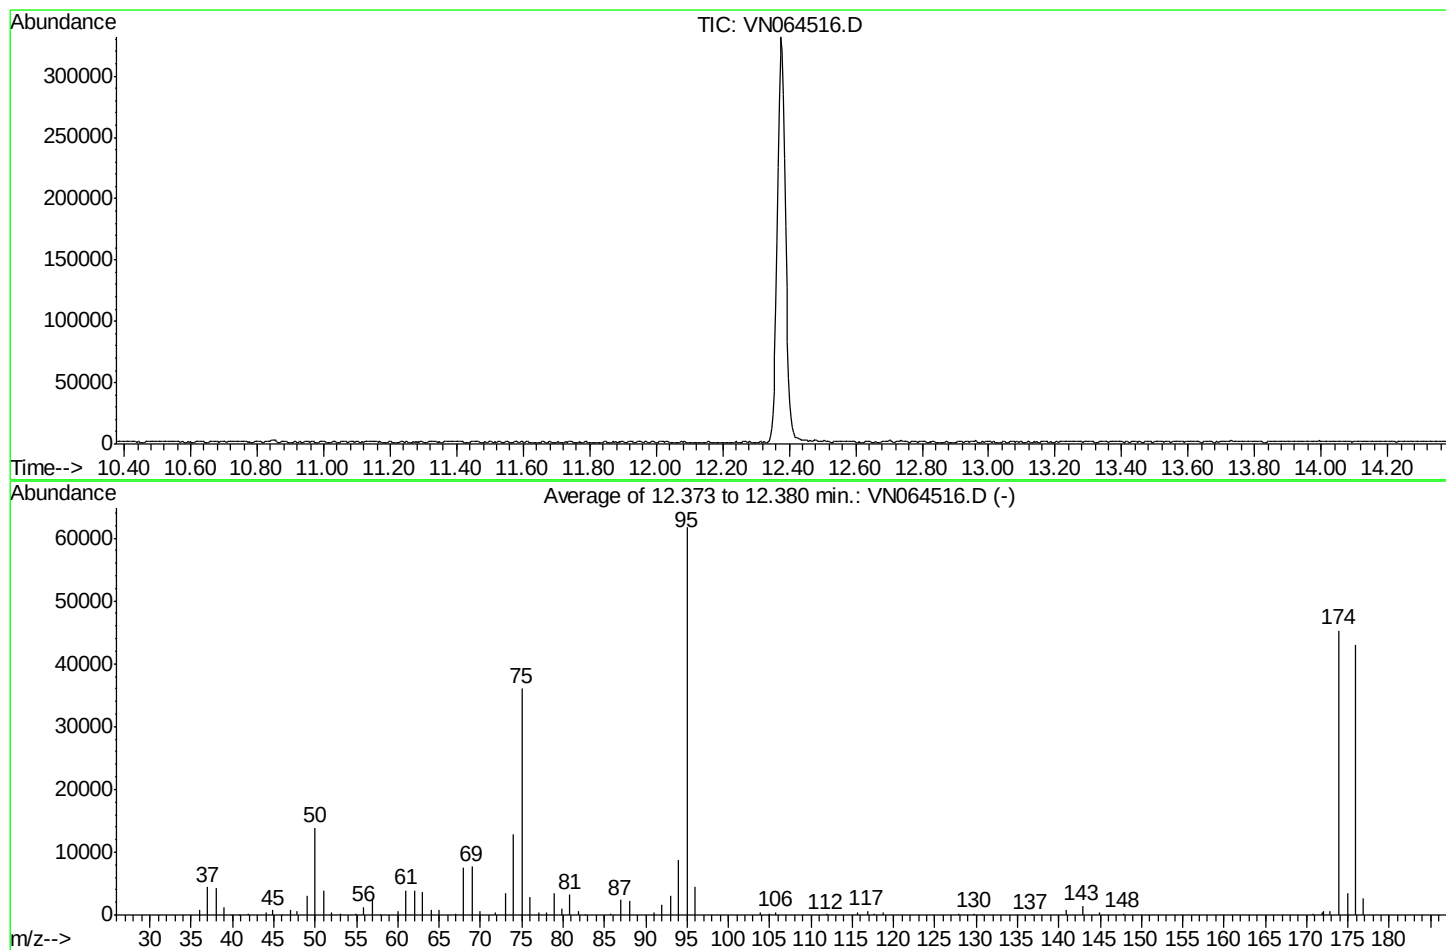

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	13892	PASS
75	95	30	60	58.4	36037	PASS
95	95	100	100	100.0	61712	PASS
96	95	5	9	7.4	4552	PASS
173	174	0.00	2	1.4	640	PASS
174	95	50	100	73.4	45296	PASS
175	174	5	9	7.7	3489	PASS
176	174	95	101	95.1	43098	PASS
177	176	5	9	6.0	2603	PASS