


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111021\
 Data File : VN069431.D
 Acq On : 10 Nov 2021 9:52
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N111021W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Nov 10 14:36:17 2021

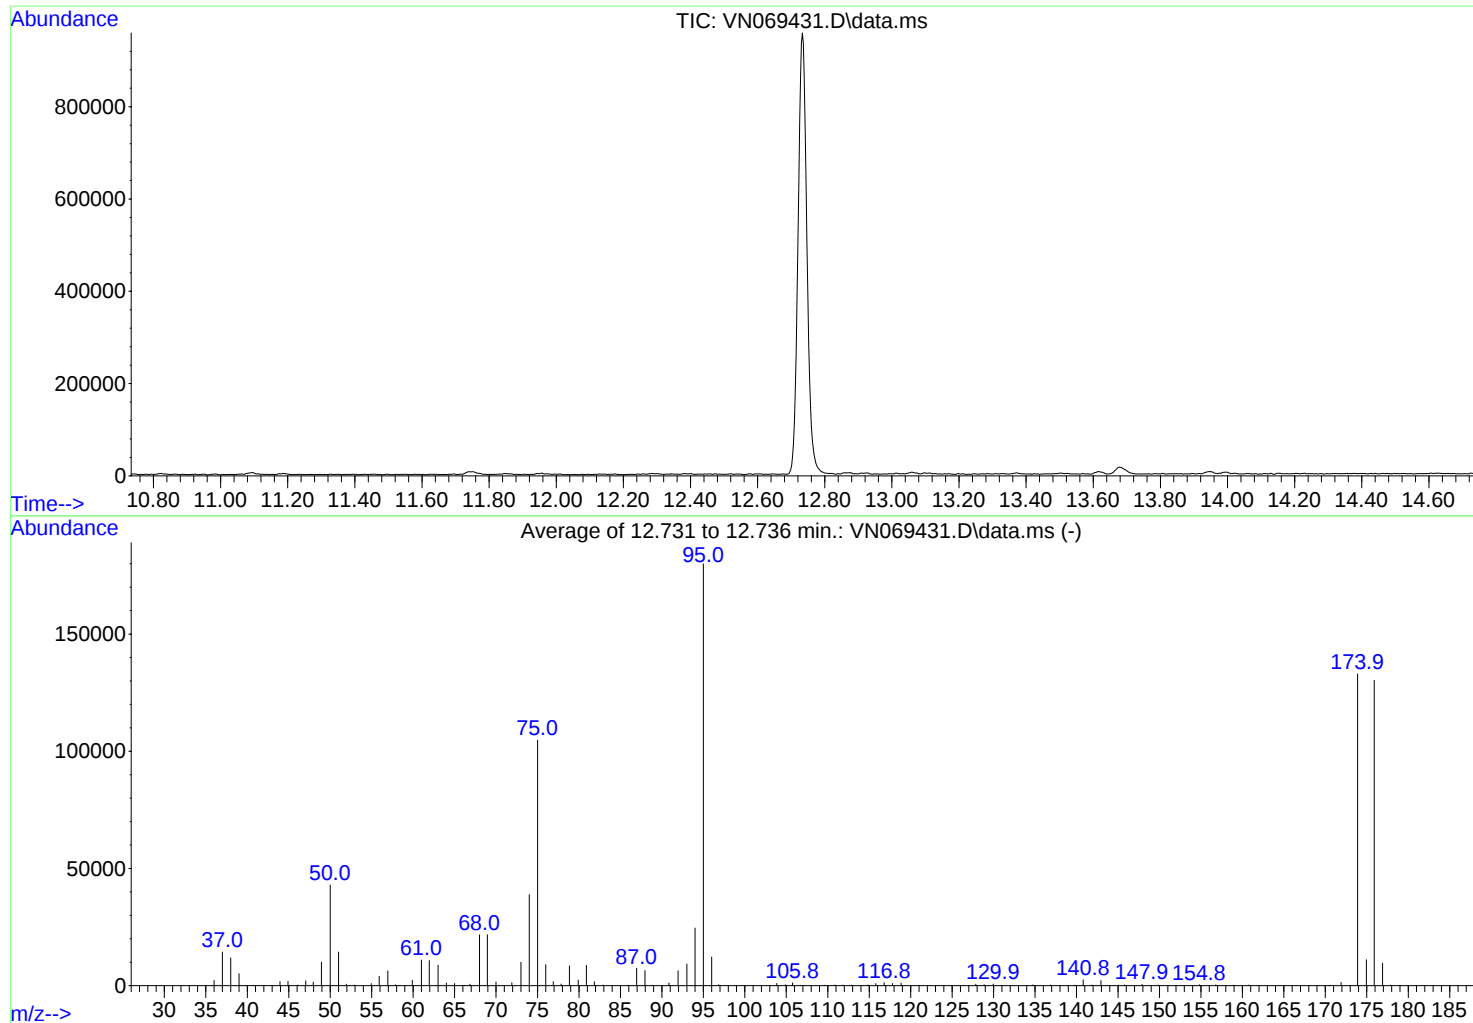

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	42912	PASS
75	95	30	60	58.2	104731	PASS
95	95	100	100	100.0	179947	PASS
96	95	5	9	6.8	12252	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.9	133005	PASS
175	174	5	9	8.3	11080	PASS
176	174	95	101	97.9	130235	PASS
177	176	5	9	7.3	9557	PASS