
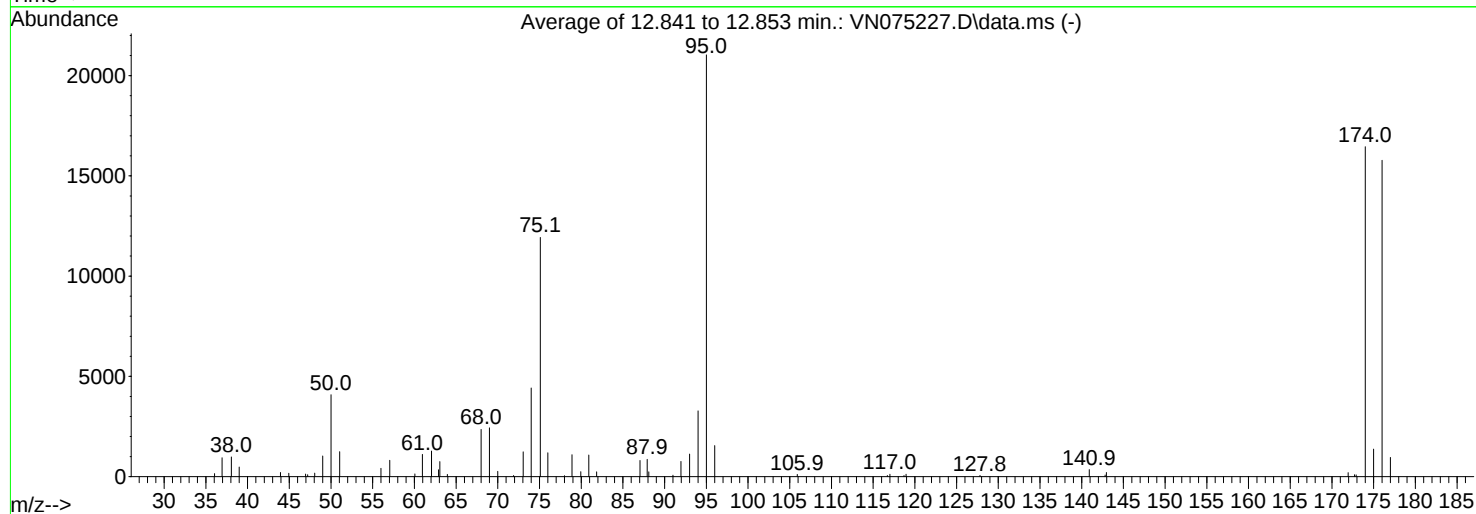


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111022\
Data File : VN075227.D
Acq On : 10 Nov 2022 09:55
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Title : SW846 8260
Last Update : Thu Oct 27 09:48:49 2022

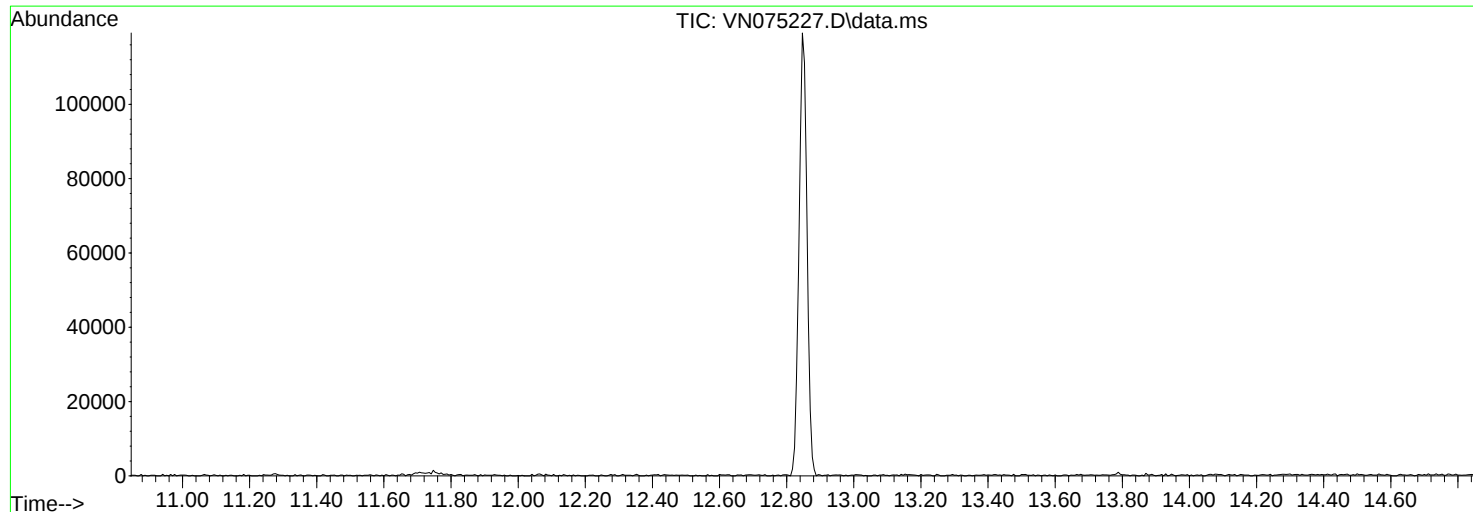

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	4082	PASS
75	95	30	60	56.7	11932	PASS
95	95	100	100	100.0	21035	PASS
96	95	5	9	7.4	1551	PASS
173	174	0.00	2	0.6	94	PASS
174	95	50	100	78.2	16453	PASS
175	174	5	9	8.4	1374	PASS
176	174	95	101	95.9	15778	PASS
177	176	5	9	6.1	957	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	150	51.05	1245	70.00	260	87.05	80
36.95	939	56.00	418	71.90	60	87.90	86
38.05	978	57.05	813	73.05	1238	88.10	24
39.00	477	60.05	138	74.00	4423	91.00	7
43.95	210	60.95	1107	75.10	11932	91.95	760
44.95	168	62.05	1274	76.00	1190	93.00	1123
46.95	126	62.90	346	78.00	51	94.00	3281
47.20	97	63.05	749	78.90	1093	95.00	21035
48.05	175	63.95	114	79.95	246	96.00	1551
49.00	1030	68.00	2355	80.90	1074	105.90	108
50.00	4082	69.00	2430	81.85	240	116.70	59

Average of 12.841 to 12.853 min.: VN075227.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.00	122	175.00	1374				
118.70	55	176.00	15778				
118.95	117	177.00	957				
127.80	61						
140.90	354						
142.80	84						
142.95	208						
171.95	198						
172.70	94						
172.90	92						
174.00	16453						

Instrument :

MSVOA_N

ClientSampleId :

BFB