

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111023\
 Data File : VN080048.D
 Acq On : 10 Nov 2023 13:12
 Operator : JC\MD
 Sample : 05325-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 10 23:56:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N110823W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Thu Nov 09 04:02:05 2023
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	7.818	128	73283	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.106	114	389277	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.870	117	362641	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.582	65	189579	30.818	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	102.733%
60) 4-Bromofluorobenzene	12.853	95	157488	27.157	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	90.533%
63) Toluene-d8	10.570	98	491376	28.597	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	95.333%
Target Compounds						
					Qvalue	
8) Diethyl Ether	3.965	74	6412	2.366	ug/l	87
15) Acetone	4.424	58	130407	166.224	ug/l	82
22) cis-1,2-Dichloroethene	7.494	96	1907	0.351	ug/l #	30
23) tert-Butyl Alcohol	5.518	59	3320008	5293.934	ug/l #	100
24) Methyl tert-Butyl Ether	5.794	73	11575	0.833	ug/l	96
30) 2-Butanone	7.482	43	321039	100.618	ug/l	95
31) 2,2-Dichloropropane	7.435	77	175890	24.358	ug/l #	53
34) Benzene	8.606	78	64010	3.225	ug/l #	71
35) Methacrylonitrile	7.841	41	539581	161.301	ug/l #	43
36) 1,2-Dichloroethane	8.676	62	2115	0.294	ug/l #	75
43) Ethyl Acetate	7.482	43	321039	53.562	ug/l #	77
44) Isopropyl Acetate	8.659	43	14821	1.518	ug/l #	54
45) 1,4-Dioxane	9.700	88	5980	79.453	ug/l #	84
47) n-amyl Acetate	12.835	43	2183	0.278	ug/l	96
56) Bromoform	12.847	173	1215	0.374	ug/l #	1
58) 4-Methyl-2-Pentanone	10.447	43	40061	6.612	ug/l #	88
59) 2-Hexanone	11.170	43	149510	32.395	ug/l #	34
62) Toluene	10.635	91	48011	2.289	ug/l	97
64) Chlorobenzene	11.900	112	11921	0.952	ug/l #	81
66) Ethyl Benzene	11.965	91	62263	2.825	ug/l	93
67) m/p-Xylenes	12.070	106	48809	5.948	ug/l	95
68) o-Xylene	12.400	106	30810	3.917	ug/l	95
69) Styrene	12.412	104	5494	0.422	ug/l #	8
70) Isopropylbenzene	12.700	105	9855	0.502	ug/l	98
76) 1,3,5-Trimethylbenzene	13.182	105	7207	0.444	ug/l	85
77) t-1,4-Dichloro-2-butene	12.753	75	421	0.207	ug/l #	34
80) 1,2,4-Trimethylbenzene	13.482	105	27964	1.757	ug/l	92
81) sec-Butylbenzene	13.823	105	19167	1.069	ug/l	61
83) 1,3-Dichlorobenzene	13.817	146	19579	2.228	ug/l	95
84) 1,4-Dichlorobenzene	13.817	146	19579	2.270	ug/l	93
85) n-Butylbenzene	14.000	91	3596	0.295	ug/l	55
87) 1,2-Dichlorobenzene	13.817	146	19579	2.332	ug/l	98
88) 1,2-Dibromo-3-Chloropr...	14.729	75	450	0.368	ug/l #	6
91) Naphthalene	15.641	128	150841	12.084	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111023\
Data File : VN080048.D
Acq On : 10 Nov 2023 13:12
Operator : JC\MD
Sample : 05325-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Nov 10 23:56:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N110823W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Thu Nov 09 04:02:05 2023
Response via : Initial Calibration




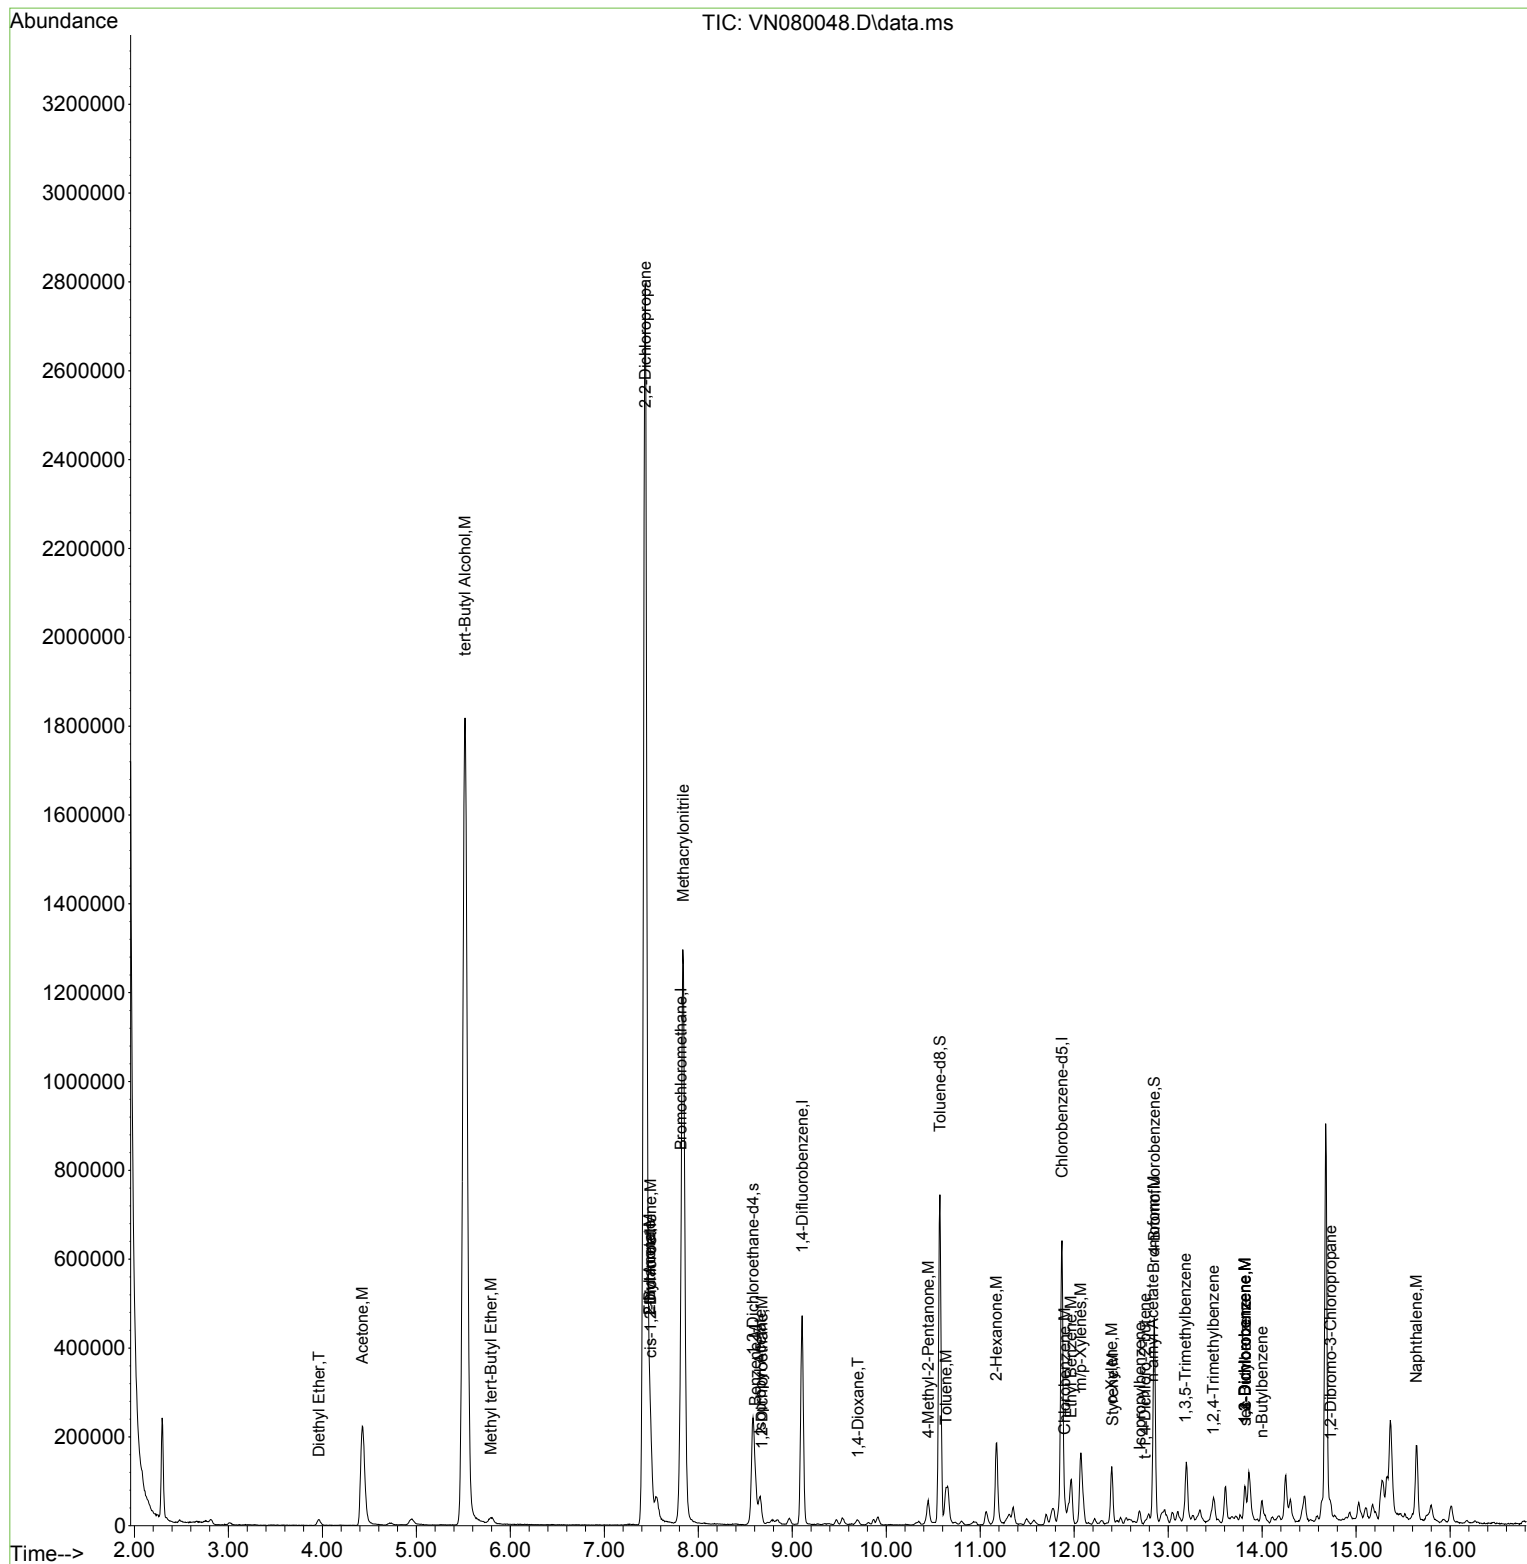


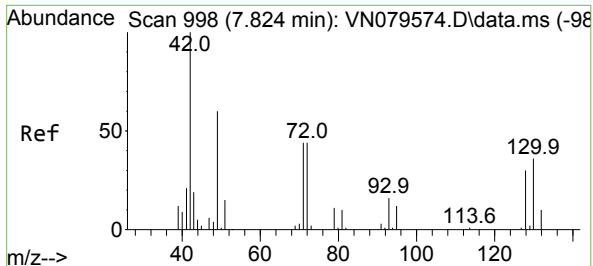

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.818 min Scan# 998
Delta R.T. -0.006 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:128 Resp: 73283
Ion Ratio Lower Upper
128 100
49 182.2 0.0 468.5
130 130.5 0.0 320.7

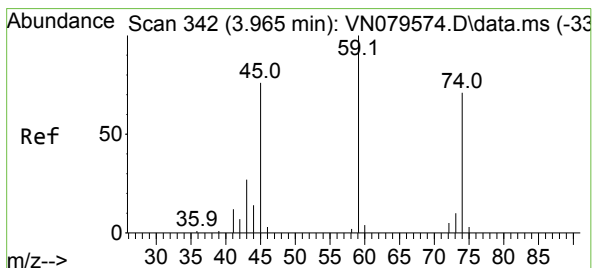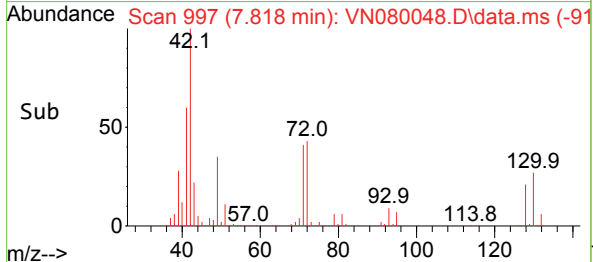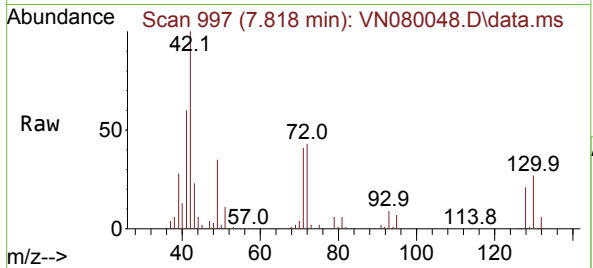

#8
Diethyl Ether
Concen: 2.366 ug/l
RT: 3.965 min Scan# 342
Delta R.T. 0.000 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Tgt Ion: 74 Resp: 6412
Ion Ratio Lower Upper
74 100
45 107.8 19.0 171.0


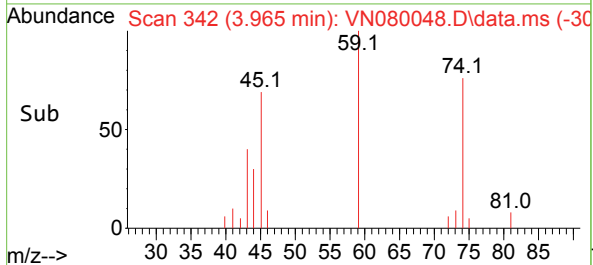

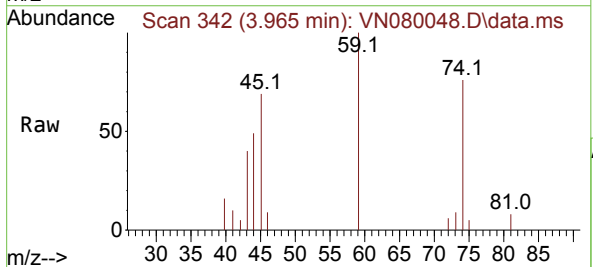




#15
Acetone
Concen: 166.224 ug/l
RT: 4.424 min Scan# 41
Delta R.T. -0.012 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 58 Resp: 130407
Ion Ratio Lower Upper
58 100
43 315.8 225.2 337.8

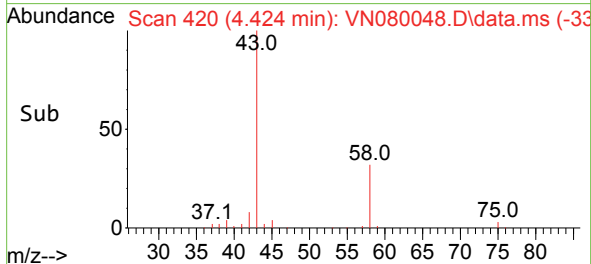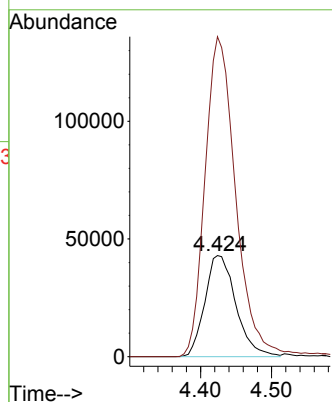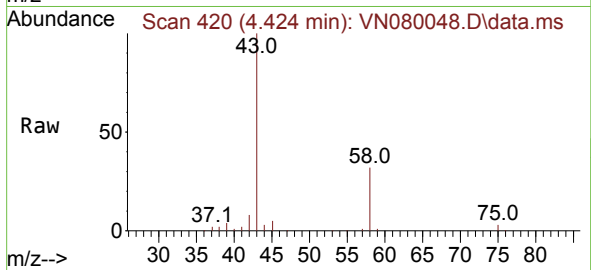

#22
cis-1,2-Dichloroethene
Concen: 0.351 ug/l
RT: 7.494 min Scan# 942
Delta R.T. 0.000 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Tgt Ion: 96 Resp: 1907
Ion Ratio Lower Upper
96 100
61 25.5 124.6 186.8#
98 67.3 54.2 81.4


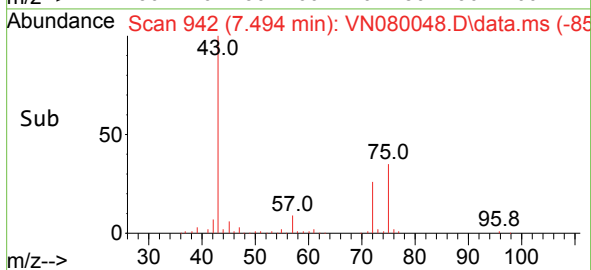
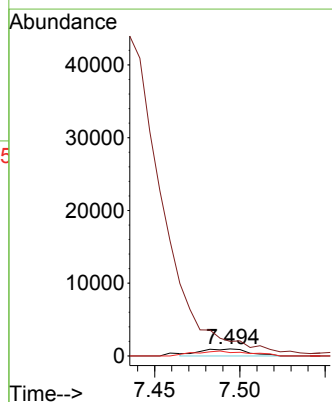
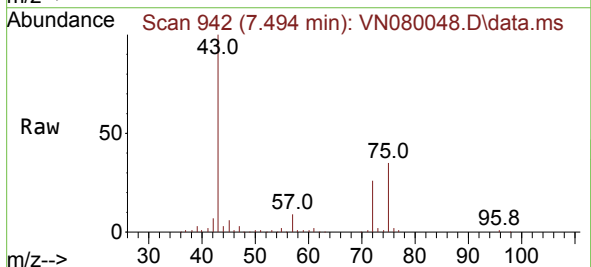




#23
tert-Butyl Alcohol
Concen: 5293.934 ug/l
RT: 5.518 min Scan# 607
Delta R.T. -0.006 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 59 Resp: 3320008
Ion Ratio Lower Upper
59 100
52 0.3 0.0 0.0#

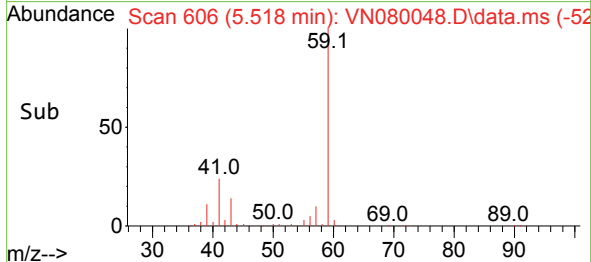

#24
Methyl tert-Butyl Ether
Concen: 0.833 ug/l
RT: 5.794 min Scan# 653
Delta R.T. -0.006 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Tgt Ion: 73 Resp: 11575
Ion Ratio Lower Upper
73 100
43 18.9 16.6 24.8


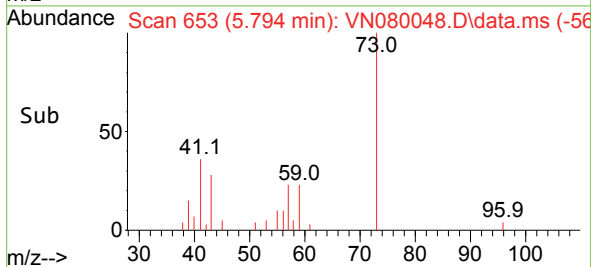

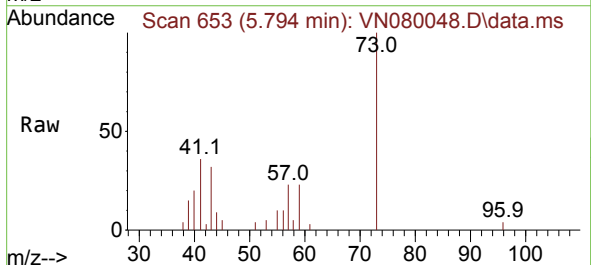




#27
1,2-Dichloroethane-d4
Concen: 30.818 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 65 Resp: 189579
Ion Ratio Lower Upper
65 100
67 51.1 42.1 63.1

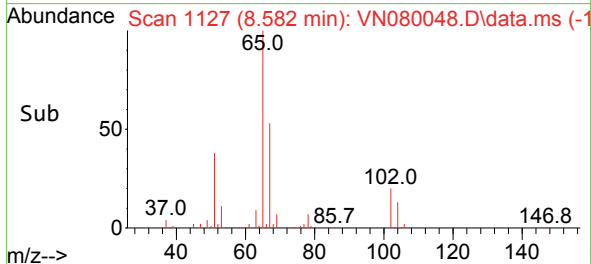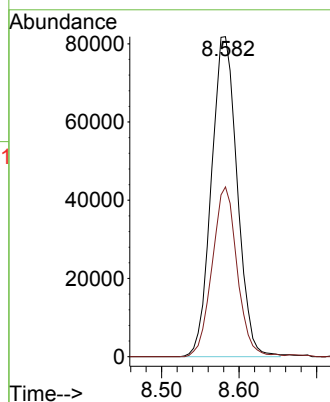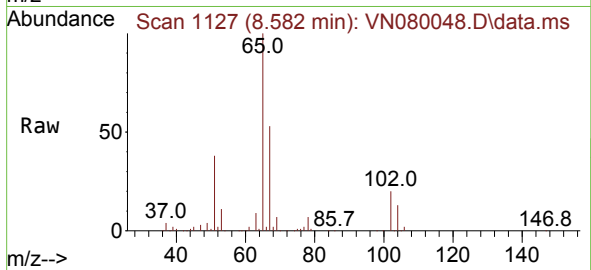

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 9.106 min Scan# 1216
Delta R.T. -0.000 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12


Tgt Ion: 114 Resp: 389277
Ion Ratio Lower Upper
114 100
63 21.4 18.1 27.1
88 16.0 12.2 18.2

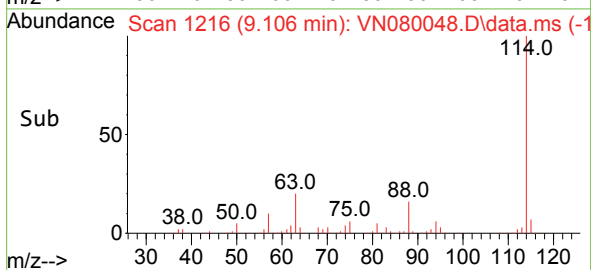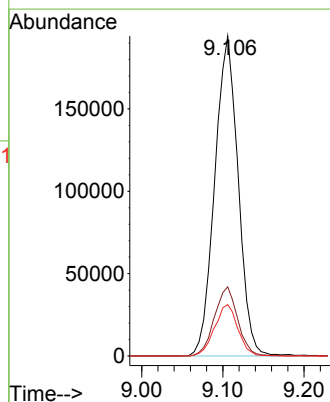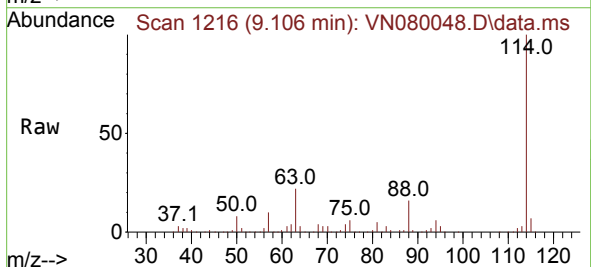






#30
2-Butanone
Concen: 100.618 ug/l
RT: 7.482 min Scan# 941
Delta R.T. -0.006 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 321039
Ion Ratio Lower Upper
43 100
57 9.0 6.4 9.6
72 28.5 20.7 31.1

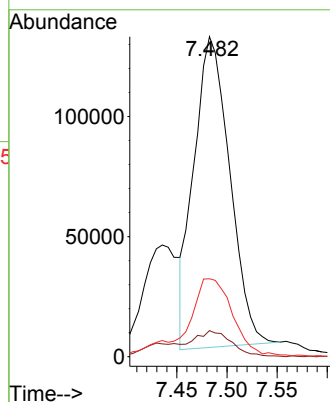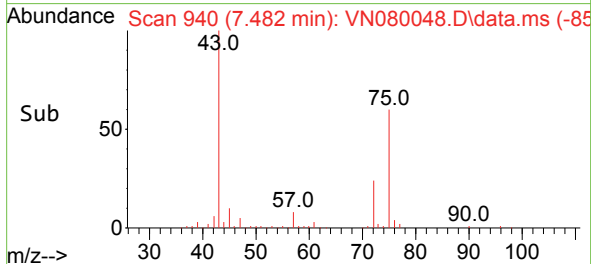

#31
2,2-Dichloropropane
Concen: 24.358 ug/l
RT: 7.435 min Scan# 932
Delta R.T. -0.059 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12


Tgt Ion: 77 Resp: 175890
Ion Ratio Lower Upper
77 100
97 0.0 17.9 26.9#

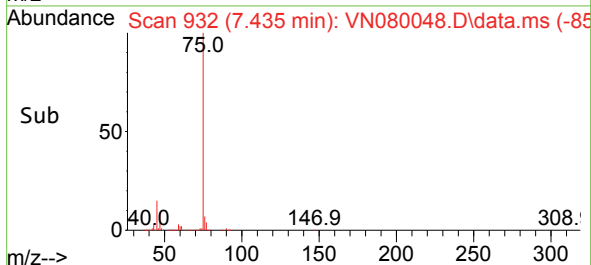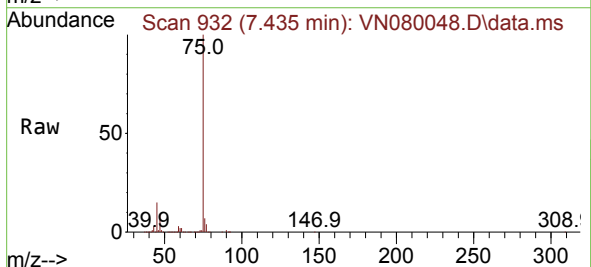






#34
Benzene
Concen: 3.225 ug/l
RT: 8.606 min Scan# 1132
Delta R.T. -0.006 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 78 Resp: 64010
Ion Ratio Lower Upper
78 100
77 18.2 19.7 29.5#
51 42.4 15.8 23.6#

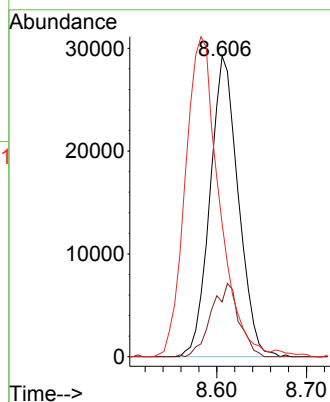

#35
Methacrylonitrile
Concen: 161.301 ug/l
RT: 7.841 min Scan# 1001
Delta R.T. 0.059 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Tgt Ion: 41 Resp: 539581
Ion Ratio Lower Upper
41 100
39 42.6 26.3 78.8
67 0.0 37.5 112.3#
52 0.2 14.4 43.4#

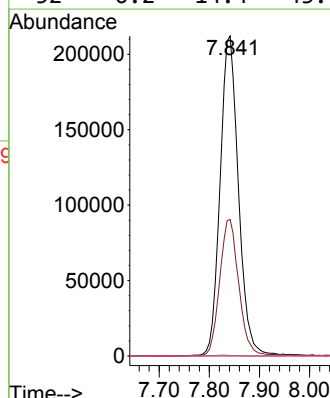



#36

1,2-Dichloroethane

Concen: 0.294 ug/l

RT: 8.676 min Scan# 1142

Delta R.T. 0.005 min

Lab File: VN080048.D

Acq: 10 Nov 2023 13:12

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 62 Resp: 2115

Ion Ratio Lower Upper

62 100

98 0.0 7.2 10.8#

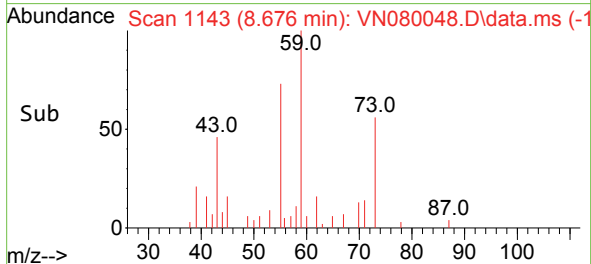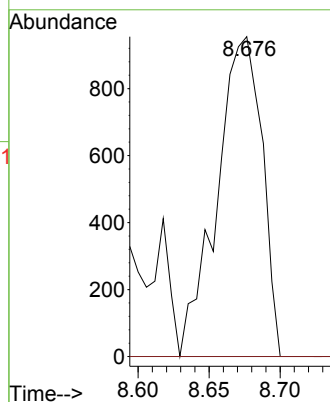

#43

Ethyl Acetate

Concen: 53.562 ug/l

RT: 7.482 min Scan# 940

Delta R.T. -0.083 min

Lab File: VN080048.D




Acq: 10 Nov 2023 13:12


Tgt Ion: 43 Resp: 321039

Ion Ratio Lower Upper

43 100

45 5.4 11.8 17.8#


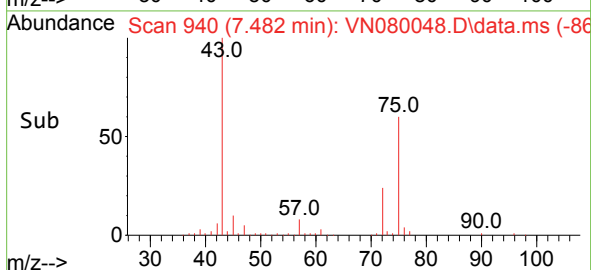






#44
Isopropyl Acetate
Concen: 1.518 ug/l
RT: 8.659 min Scan# 1140
Delta R.T. -0.035 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 14821
Ion Ratio Lower Upper
43 100
61 2.1 20.3 30.5#

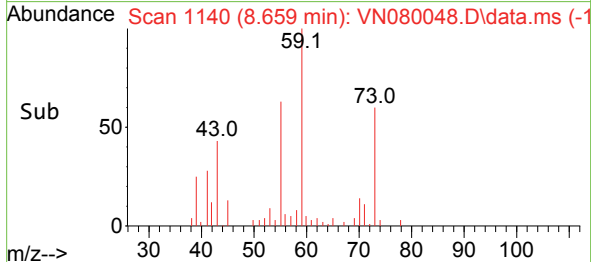

#45
1,4-Dioxane
Concen: 79.453 ug/l
RT: 9.700 min Scan# 1317
Delta R.T. -0.006 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Tgt Ion: 88 Resp: 5980
Ion Ratio Lower Upper
88 100
43 31.9 28.7 43.1
58 87.6 56.9 85.3#

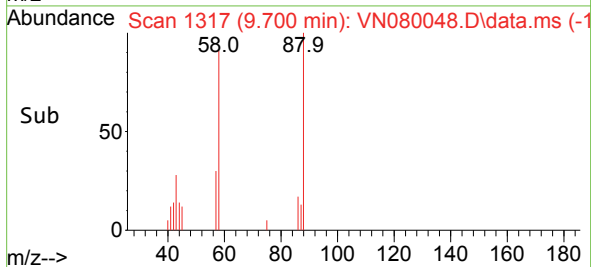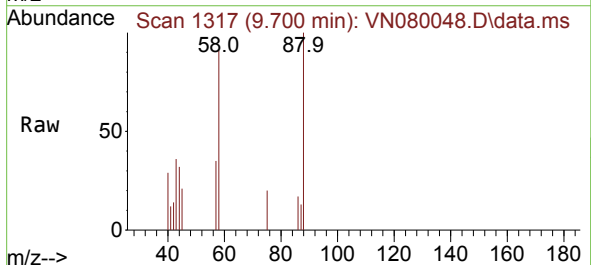



#47

n-amy1 Acetate

Concen: 0.278 ug/l

RT: 12.835 min Scan# 1850

Delta R.T. 0.335 min

Lab File: VN080048.D

Acq: 10 Nov 2023 13:12

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 2183

Ion Ratio Lower Upper

43 100

55 28.1 20.7 31.1

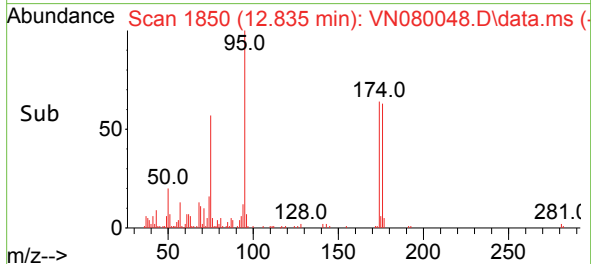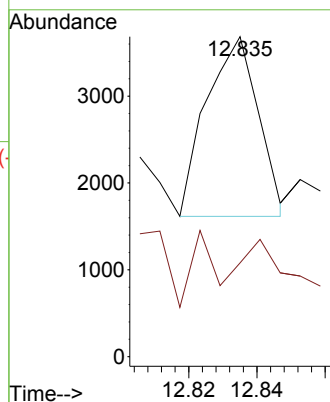

#56

Bromoform

Concen: 0.374 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. 0.265 min

Lab File: VN080048.D

Acq: 10 Nov 2023 13:12




Tgt Ion: 173 Resp: 1215


Ion Ratio Lower Upper

173 100

175 693.7 37.9 56.9#

254 0.0 7.3 10.9#


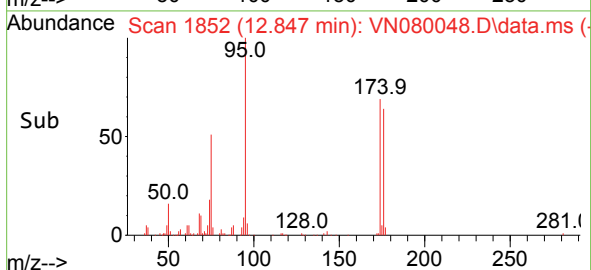




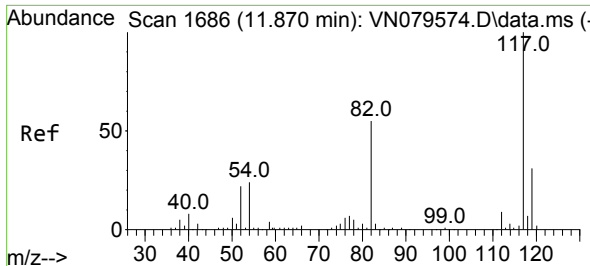

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.870 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 362641
Ion Ratio Lower Upper
117 100
82 58.2 46.2 69.2
119 31.7 25.2 37.8

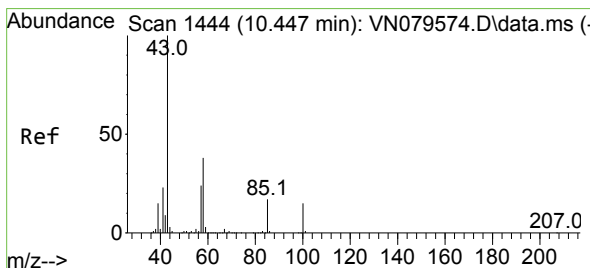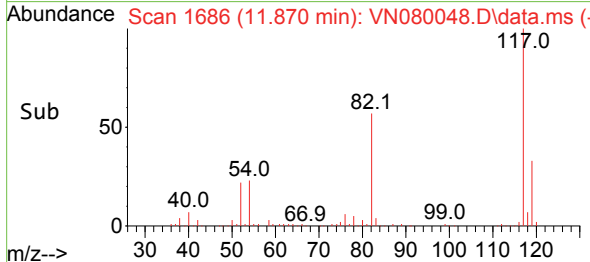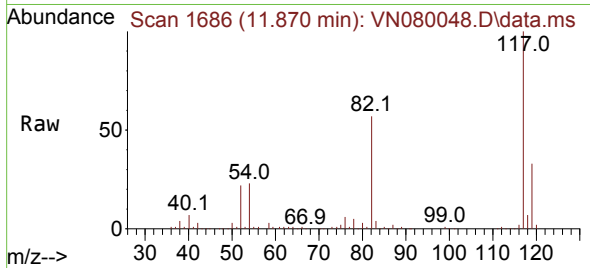

#58
4-Methyl-2-Pentanone
Concen: 6.612 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. -0.000 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12


Tgt Ion: 43 Resp: 40061
Ion Ratio Lower Upper
43 100
58 29.8 30.4 45.6#
85 12.7 13.2 19.8#

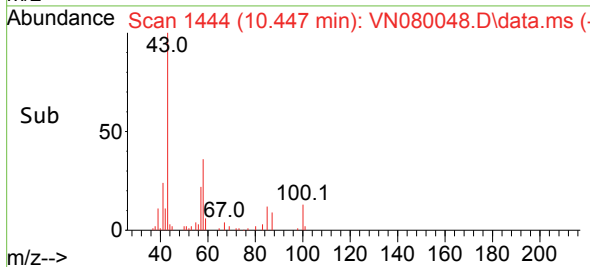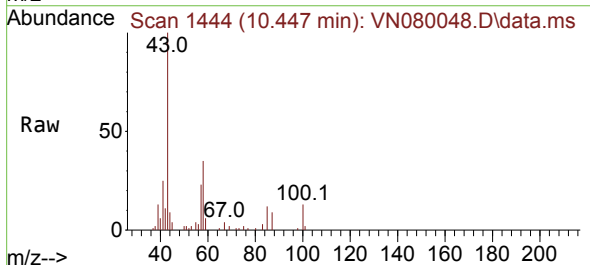



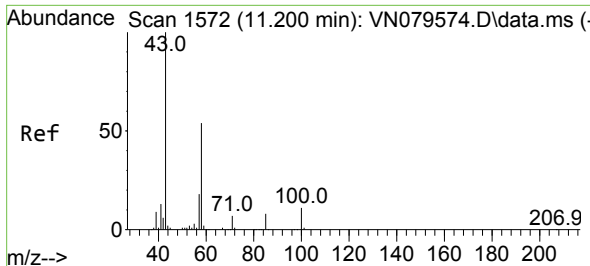


#59
2-Hexanone
Concen: 32.395 ug/l
RT: 11.170 min Scan# 11
Delta R.T. -0.030 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Instrument :
MSVOA_N
ClientSampleId :



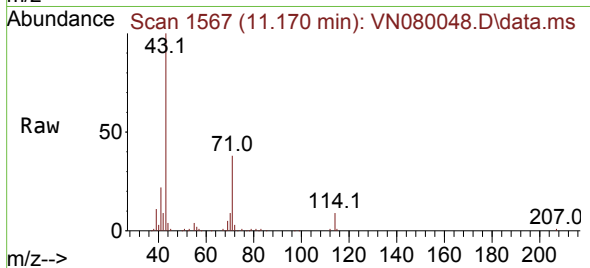



Tgt Ion: 43 Resp: 149510
Ion Ratio Lower Upper
43 100
58 0.0 42.3 63.5#
57 0.6 13.9 20.9#

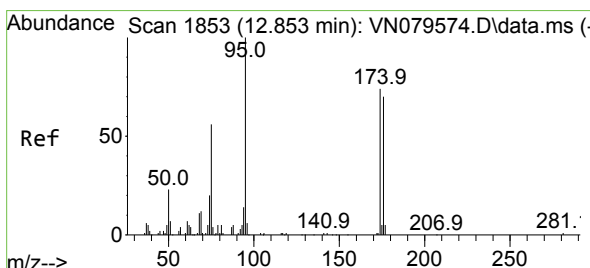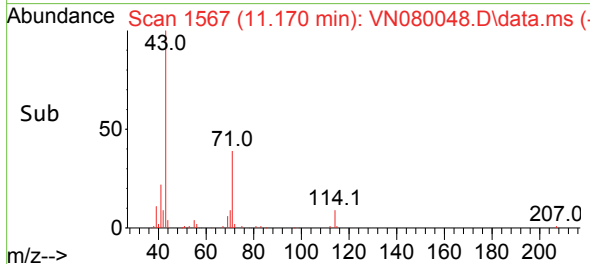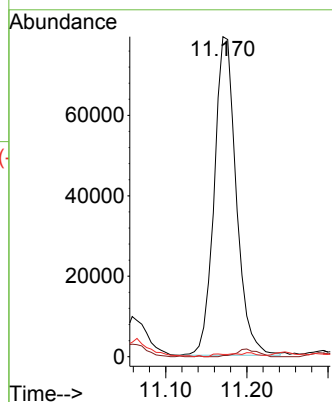

#60
4-Bromofluorobenzene
Concen: 27.157 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Tgt Ion: 95 Resp: 157488
Ion Ratio Lower Upper
95 100
174 73.7 60.5 90.7
176 69.5 57.2 85.8

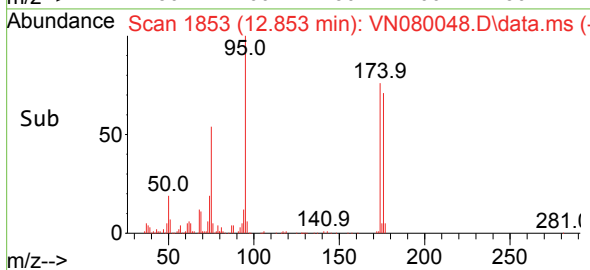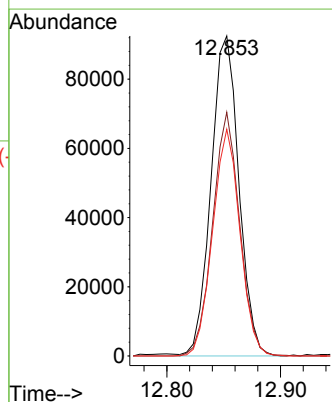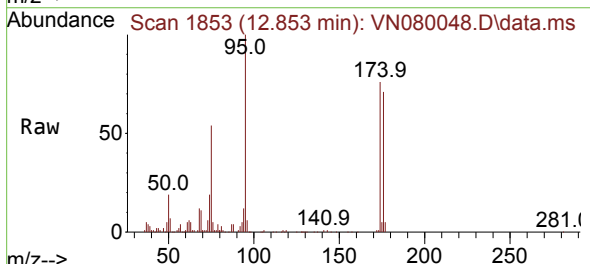

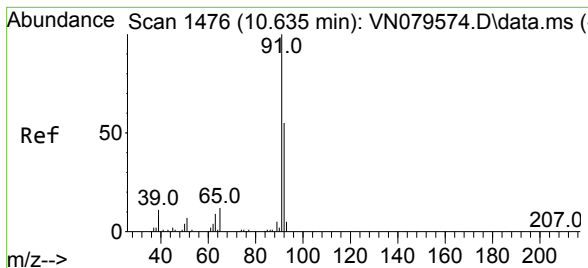

#62

Toluene

Concen: 2.289 ug/l

RT: 10.635 min Scan# 1476

Delta R.T. 0.000 min

Lab File: VN080048.D

Acq: 10 Nov 2023 13:12

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 91 Resp: 48011

Ion Ratio Lower Upper

91 100

92 58.9 45.3 67.9

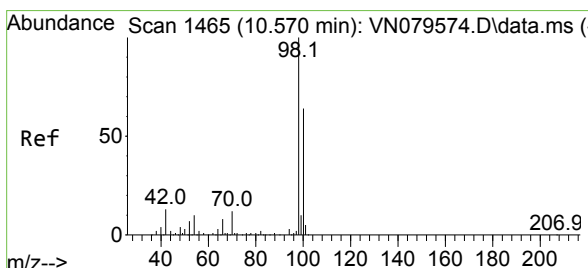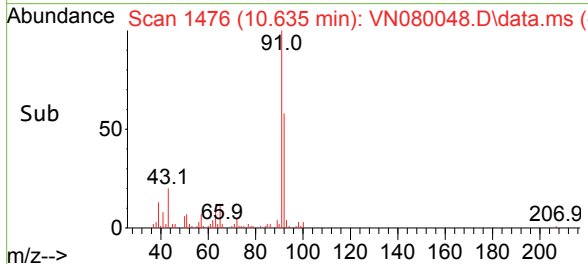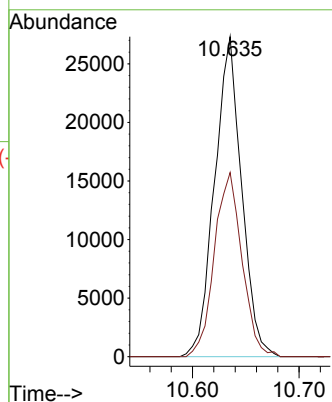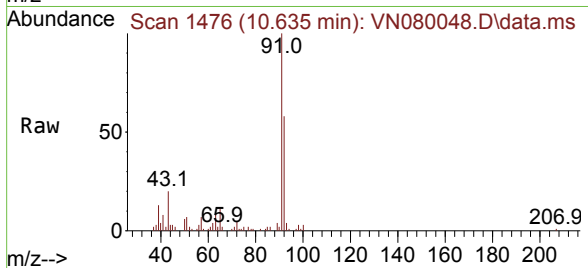

#63

Toluene-d8

Concen: 28.597 ug/l

RT: 10.570 min Scan# 1465

Delta R.T. 0.000 min

Lab File: VN080048.D




Acq: 10 Nov 2023 13:12


Tgt Ion: 98 Resp: 491376

Ion Ratio Lower Upper

98 100

100 63.9 51.6 77.4


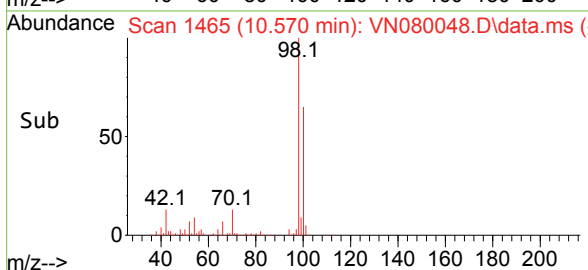

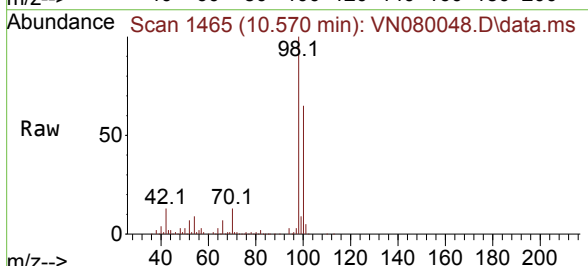


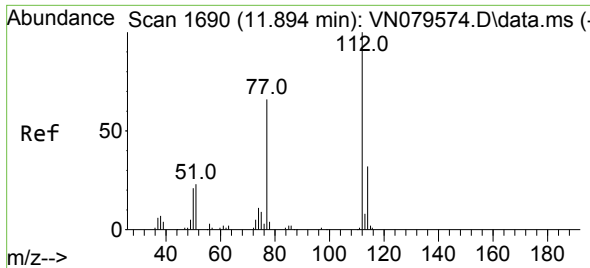

#64
Chlorobenzene
Concen: 0.952 ug/l
RT: 11.900 min Scan# 11921
Delta R.T. 0.006 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:112 Resp: 11921
Ion Ratio Lower Upper
112 100
114 24.2 28.1 42.1#

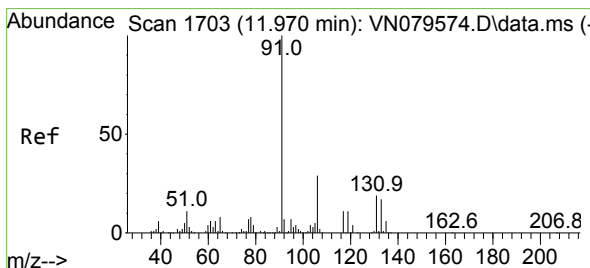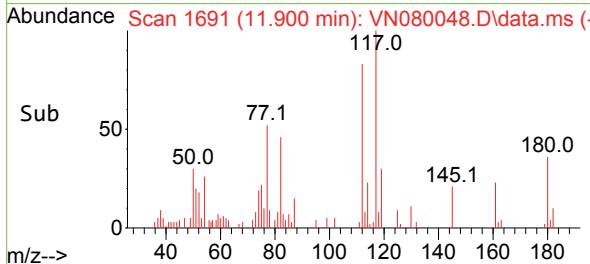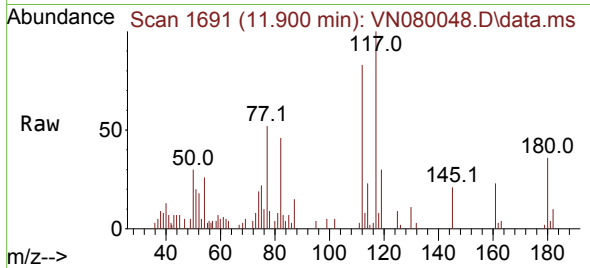

#66
Ethyl Benzene
Concen: 2.825 ug/l
RT: 11.965 min Scan# 1702
Delta R.T. -0.005 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Tgt Ion: 91 Resp: 62263
Ion Ratio Lower Upper
91 100
106 25.9 23.8 35.8


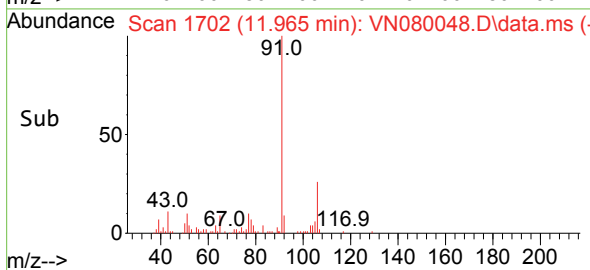

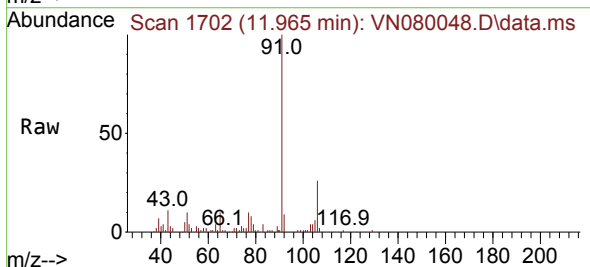




#67
m/p-Xylenes
Concen: 5.948 ug/l
RT: 12.070 min Scan# 1720
Delta R.T. -0.006 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 48809
Ion Ratio Lower Upper
106 100
91 210.4 161.8 242.6

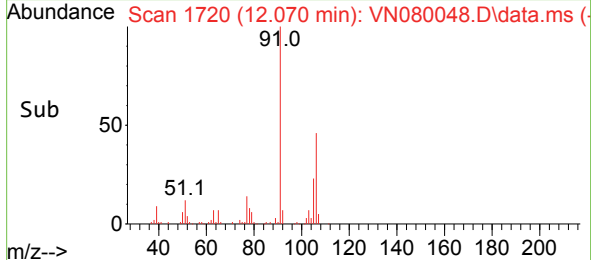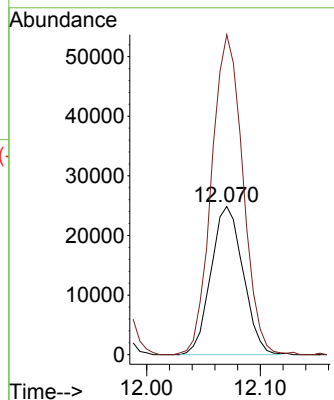

#68
o-Xylene
Concen: 3.917 ug/l
RT: 12.400 min Scan# 1776
Delta R.T. -0.000 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12


Tgt Ion:106 Resp: 30810
Ion Ratio Lower Upper
106 100
91 228.0 109.9 329.7

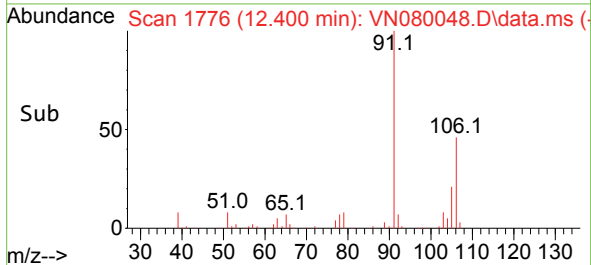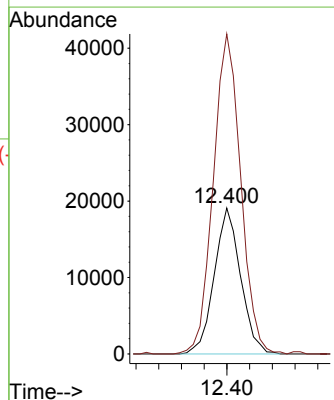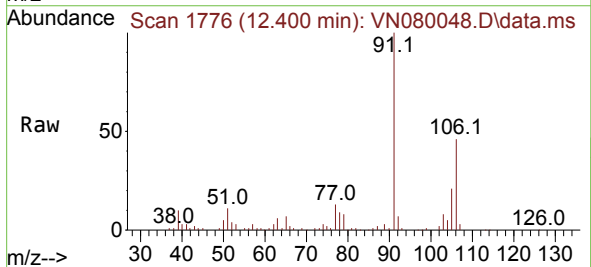






#69
Styrene
Concen: 0.422 ug/l
RT: 12.412 min Scan# 11
Delta R.T. -0.005 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Instrument :
MSVOA_N
ClientSampleId :



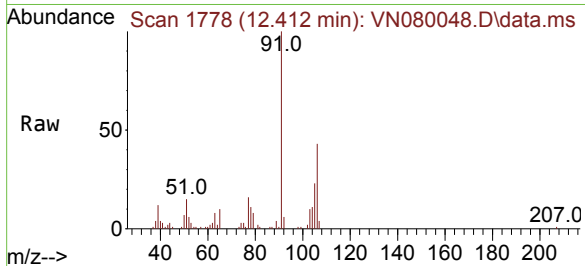



Tgt Ion:104 Resp: 5494
Ion Ratio Lower Upper
104 100
78 122.8 41.2 61.8#
103 112.6 43.1 64.7#

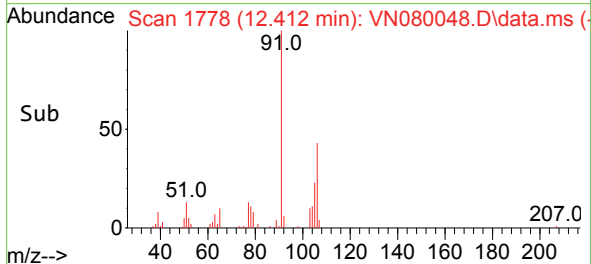

#70
Isopropylbenzene
Concen: 0.502 ug/l
RT: 12.700 min Scan# 1827
Delta R.T. -0.000 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Tgt Ion:105 Resp: 9855
Ion Ratio Lower Upper
105 100
120 24.9 18.1 33.5

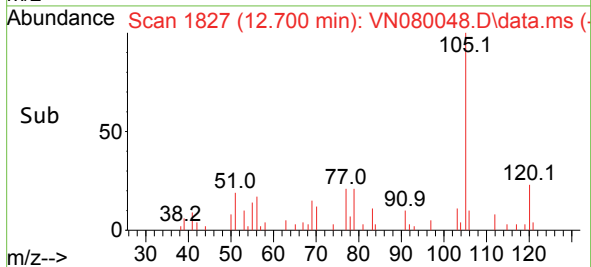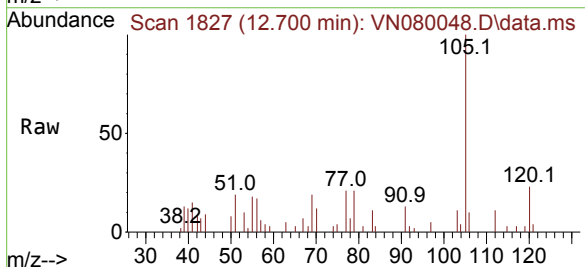

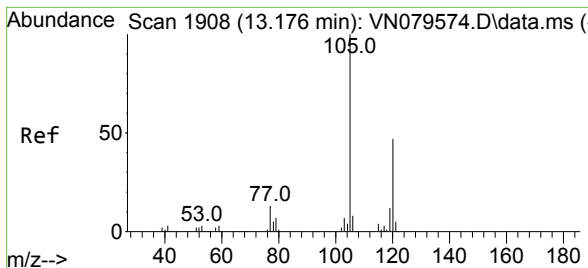

#76

1,3,5-Trimethylbenzene

Concen: 0.444 ug/l

RT: 13.182 min Scan# 1908

Delta R.T. 0.006 min

Lab File: VN080048.D

Acq: 10 Nov 2023 13:12

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:105 Resp: 7207

Ion Ratio Lower Upper

105 100

120 56.4 0.0 93.2

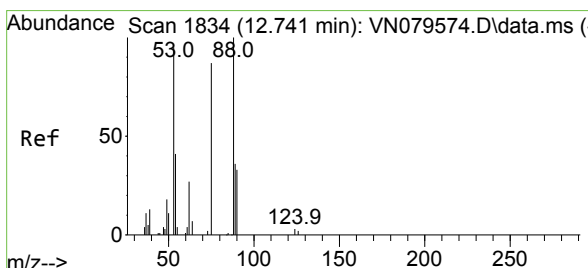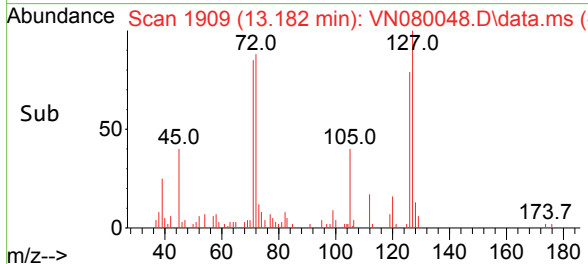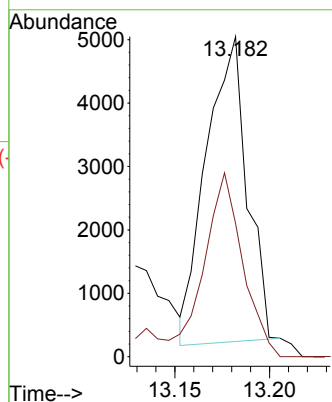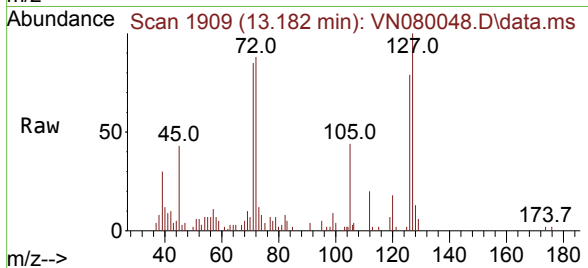

#77

t-1,4-Dichloro-2-butene

Concen: 0.207 ug/l

RT: 12.753 min Scan# 1836

Delta R.T. 0.012 min

Lab File: VN080048.D

Acq: 10 Nov 2023 13:12




Tgt Ion: 75 Resp: 421


Ion Ratio Lower Upper

75 100

53 39.8 53.0 159.1#

89 0.0 22.6 67.7#

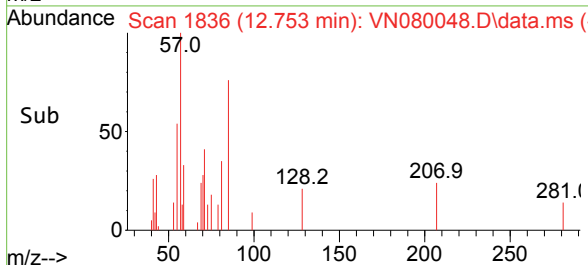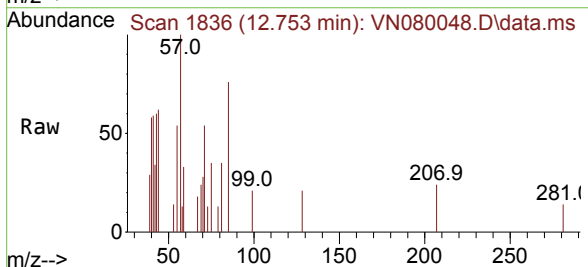



#80

1,2,4-Trimethylbenzene

Concen: 1.757 ug/l

RT: 13.482 min Scan# 1961

Delta R.T. -0.006 min

Lab File: VN080048.D

Acq: 10 Nov 2023 13:12

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:105 Resp: 27964

Ion Ratio Lower Upper

105 100

120 49.2 0.0 88.6

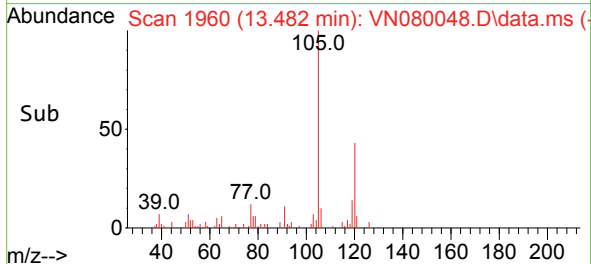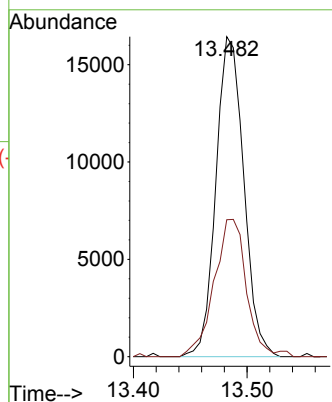

#81

sec-Butylbenzene

Concen: 1.069 ug/l

RT: 13.823 min Scan# 2018

Delta R.T. 0.206 min

Lab File: VN080048.D




Acq: 10 Nov 2023 13:12


Tgt Ion:105 Resp: 19167

Ion Ratio Lower Upper

105 100


134 1.6 0.0 38.2





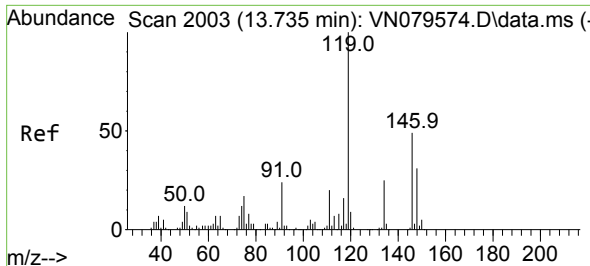


#83
1,3-Dichlorobenzene
Concen: 2.228 ug/l
RT: 13.817 min Scan# 2003
Delta R.T. 0.082 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Instrument :
MSVOA_N
ClientSampleId :



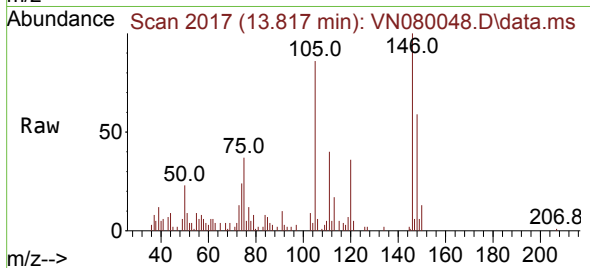



Tgt Ion:146 Resp: 19579
Ion Ratio Lower Upper
146 100
111 46.7 21.0 63.0
148 62.2 32.4 97.0

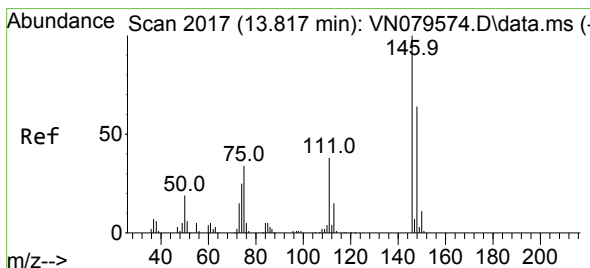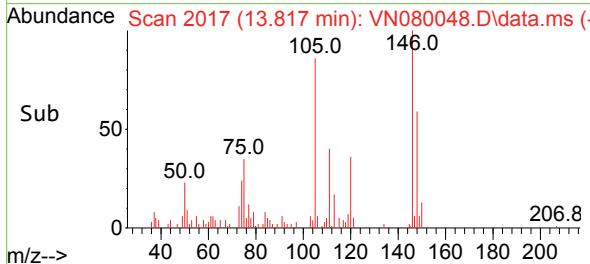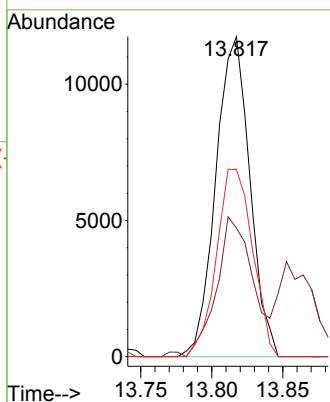

#84
1,4-Dichlorobenzene
Concen: 2.270 ug/l
RT: 13.817 min Scan# 2017
Delta R.T. 0.000 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Tgt Ion:146 Resp: 19579
Ion Ratio Lower Upper
146 100
111 46.7 19.9 59.7
148 62.2 32.6 97.7


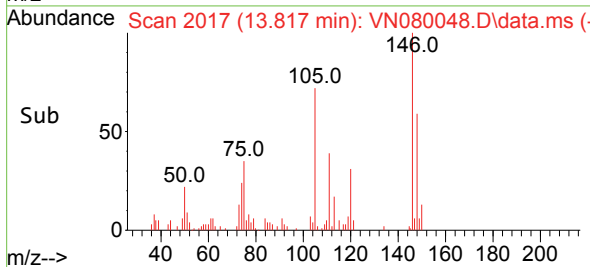

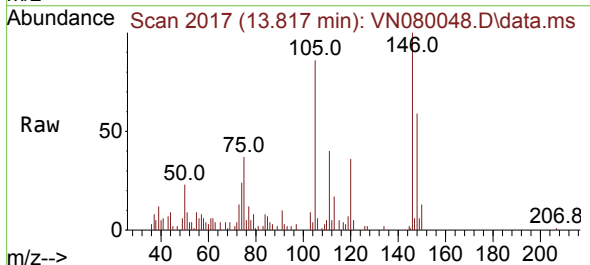




#85
n-Butylbenzene
Concen: 0.295 ug/l
RT: 14.000 min Scan# 2058
Delta R.T. -0.059 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 3596
Ion Ratio Lower Upper
91 100
92 16.8 0.0 99.6
134 4.1 0.0 46.2

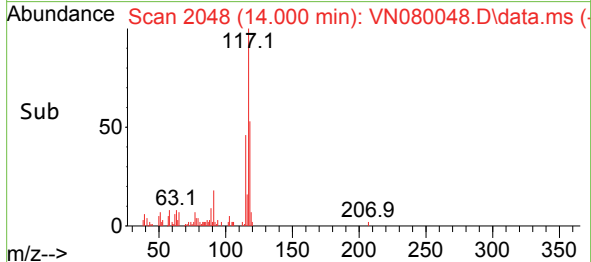

#87
1,2-Dichlorobenzene
Concen: 2.332 ug/l
RT: 13.817 min Scan# 2017
Delta R.T. -0.294 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12


Tgt Ion: 146 Resp: 19579
Ion Ratio Lower Upper
146 100
111 46.7 22.0 66.0
148 62.2 31.1 93.5

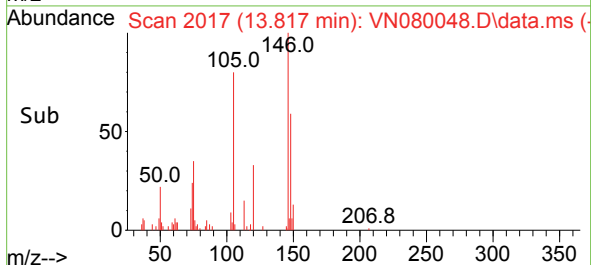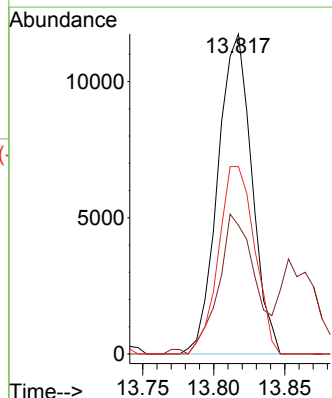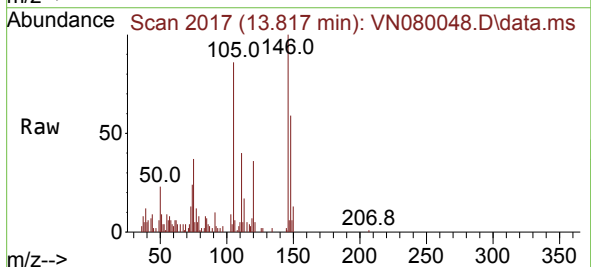






#88
1,2-Dibromo-3-Chloropropane
Concen: 0.368 ug/l
RT: 14.729 min Scan# 2171
Delta R.T. 0.006 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Instrument :
MSVOA_N
ClientSampleId :



Tgt Ion: 75 Resp: 450
Ion Ratio Lower Upper
75 100
155 0.0 60.7 91.1#
157 0.0 76.8 115.2#

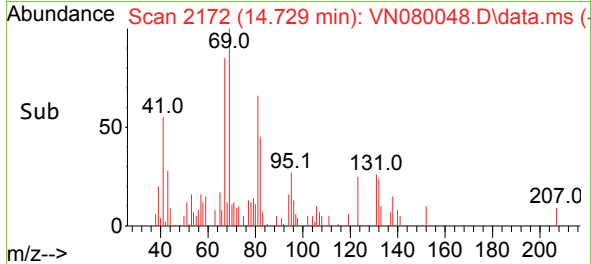

#91
Naphthalene
Concen: 12.084 ug/l
RT: 15.641 min Scan# 2327
Delta R.T. -0.000 min
Lab File: VN080048.D
Acq: 10 Nov 2023 13:12

Tgt Ion: 128 Resp: 150841
Ion Ratio Lower Upper
128 100
127 13.6 10.9 16.3
129 11.1 8.6 12.8

