

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111023\
 Data File : VN080050.D
 Acq On : 10 Nov 2023 13:59
 Operator : JC\MD
 Sample : 05310-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SEMI-ANNUAL-CONDENSATE

Quant Time: Nov 10 23:57:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N110823W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Thu Nov 09 04:02:05 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/13/2023
 Supervised By : Mahesh Dadoda 11/13/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.818	128	77133	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.106	114	425844	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.871	117	403381	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.583	65	198498	30.657	ug/l	0.00
Spiked Amount 30.000	Range 91 - 110		Recovery = 102.200%			
60) 4-Bromofluorobenzene	12.853	95	189707	29.409	ug/l	0.00
Spiked Amount 30.000	Range 63 - 112		Recovery = 98.033%			
63) Toluene-d8	10.571	98	518997	27.154	ug/l	0.00
Spiked Amount 30.000	Range 91 - 112		Recovery = 90.500%#			
Target Compounds						
					Qvalue	
8) Diethyl Ether	3.965	74	2756m	0.966	ug/l	
15) Acetone	4.436	58	28701	34.758	ug/l	97
16) Carbon Disulfide	4.712	76	10976	0.809	ug/l #	81
18) Methylene Chloride	5.271	84	8914	1.674	ug/l	92
23) tert-Butyl Alcohol	5.518	59	406120	615.257	ug/l #	100
25) Chloroform	7.965	83	272881	27.310	ug/l	97
30) 2-Butanone	7.488	43	150637	43.158	ug/l	97
34) Benzene	8.612	78	217321	10.010	ug/l	99
41) Bromodichloromethane	9.894	83	6151	0.800	ug/l #	89
45) 1,4-Dioxane	9.700	88	10612	128.888	ug/l #	76
58) 4-Methyl-2-Pentanone	10.447	43	41525	6.162	ug/l	96
62) Toluene	10.635	91	710746	30.464	ug/l	99
64) Chlorobenzene	11.894	112	60739	4.363	ug/l	93
66) Ethyl Benzene	11.965	91	310184	12.652	ug/l	98
67) m/p-Xylenes	12.071	106	144941	15.880	ug/l	95
68) o-Xylene	12.400	106	97441	11.138	ug/l	98
70) Isopropylbenzene	12.700	105	40441	1.853	ug/l	94
74) n-propylbenzene	13.041	91	23925	0.916	ug/l	95
76) 1,3,5-Trimethylbenzene	13.176	105	85111	4.715	ug/l	98
80) 1,2,4-Trimethylbenzene	13.488	105	266631	15.065	ug/l	99
81) sec-Butylbenzene	13.617	105	15871m	0.795	ug/l	
82) p-Isopropyltoluene	13.729	119	1093136	67.458	ug/l	98
83) 1,3-Dichlorobenzene	13.735	146	4093	0.419	ug/l	89
84) 1,4-Dichlorobenzene	13.817	146	318144	33.156	ug/l	98
85) n-Butylbenzene	14.053	91	3490	0.258	ug/l	63
87) 1,2-Dichlorobenzene	14.112	146	12225	1.309	ug/l	91
91) Naphthalene	15.647	128	612572	44.117	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111023\
Data File : VN080050.D
Acq On : 10 Nov 2023 13:59
Operator : JC\MD
Sample : 05310-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1


Instrument :
MSVOA_N
ClientSampleId :
SEMI-ANNUAL-CONDENSATE

Quant Time: Nov 10 23:57:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N110823W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Thu Nov 09 04:02:05 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlone 11/13/2023
Supervised By :Mahesh Dadoda 11/13/2023

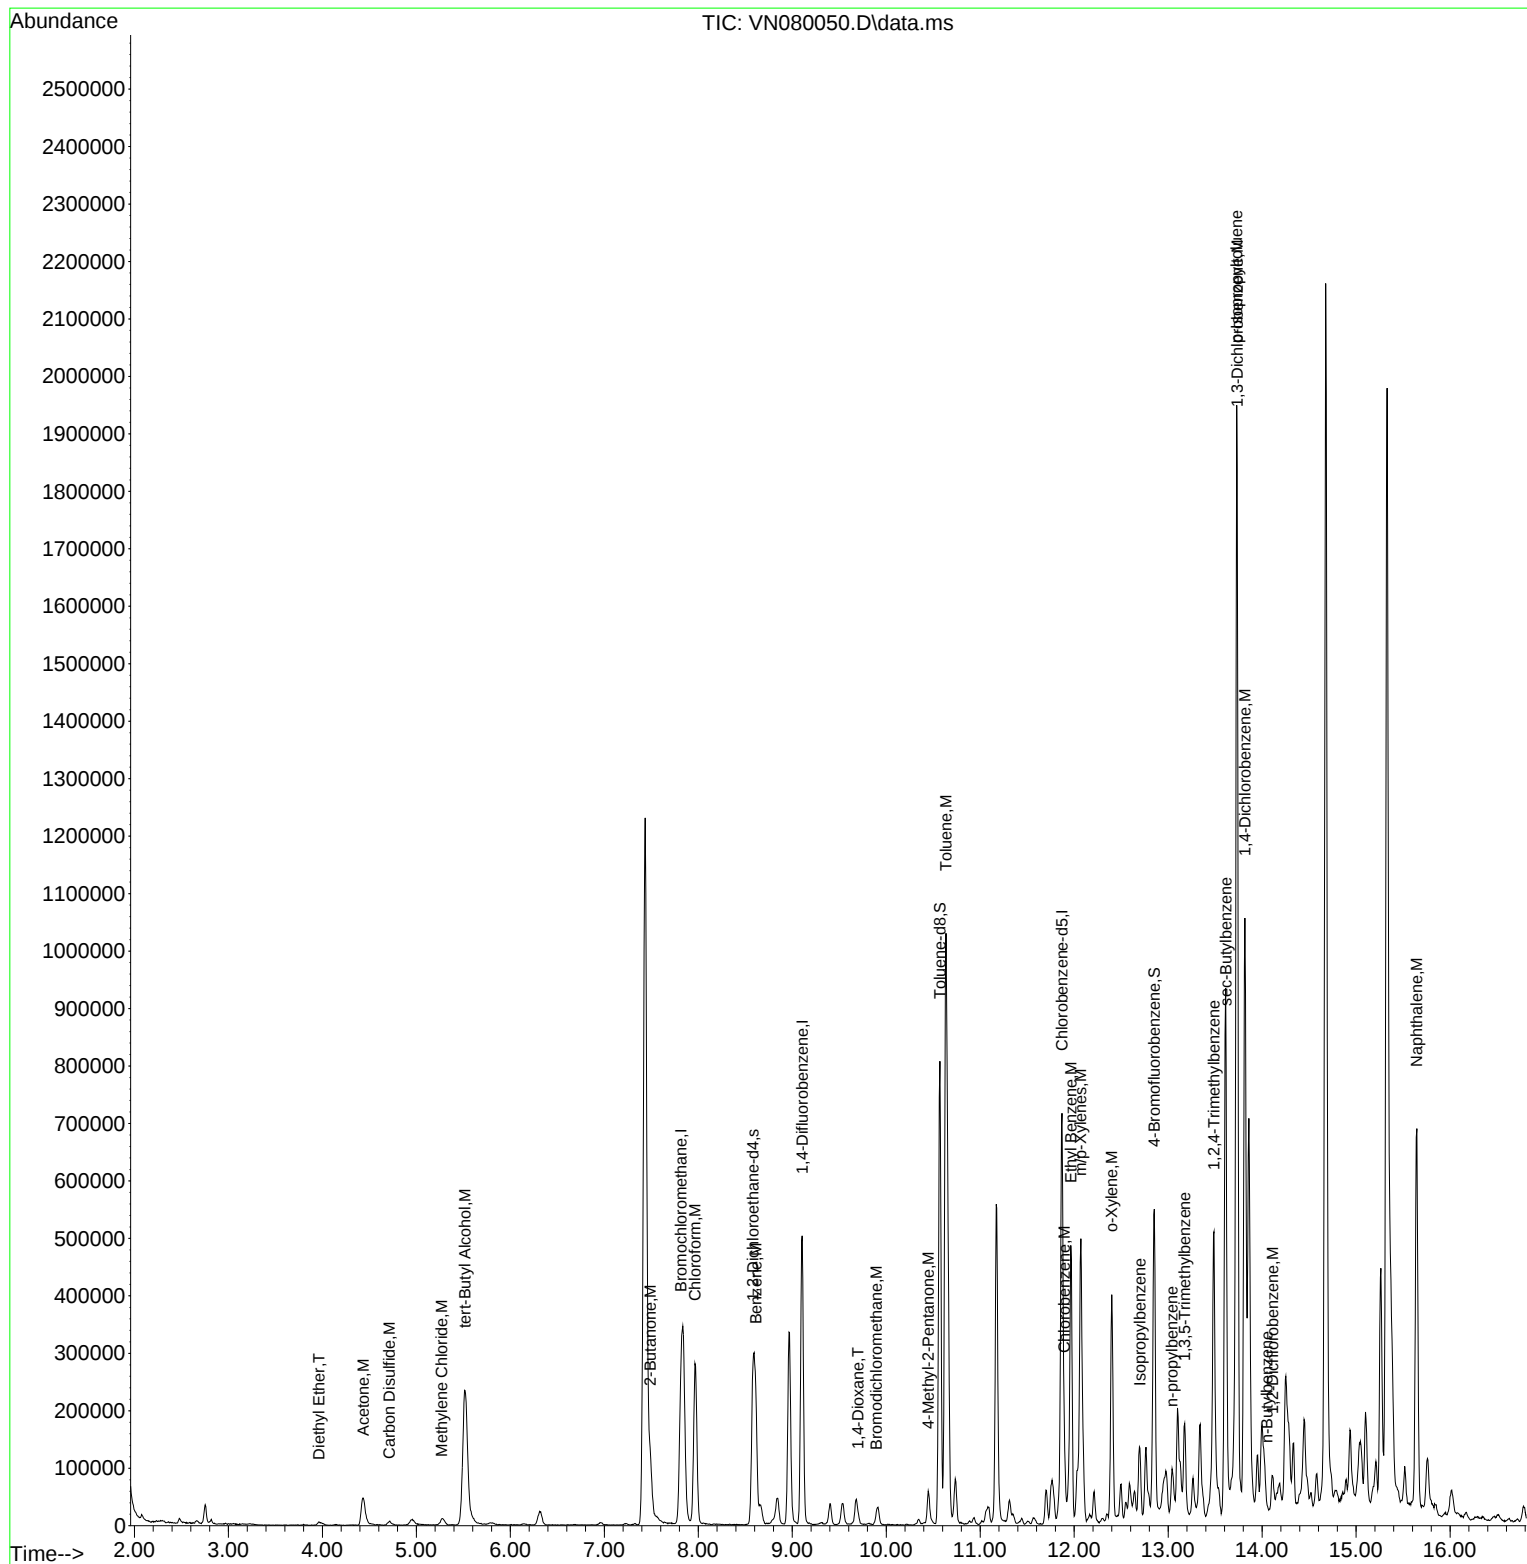

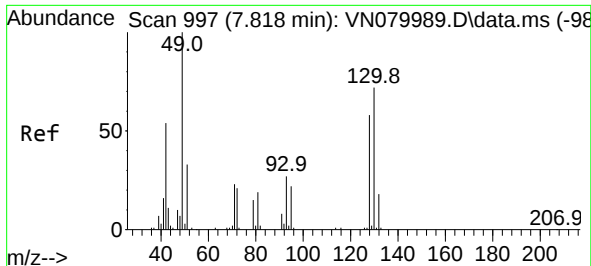





#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.818 min Scan# 91
Delta R.T. -0.006 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59

Instrument :
MSVOA_N
ClientSampleId :
SEMI-ANNUAL-CONDENSATE

Tgt Ion:128 Resp: 7713
Ion Ratio Lower Upper
128 100
49 181.0 0.0 468.5
130 129.1 0.0 320.7




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/13/2023
Supervised By :Mahesh Dadoda 11/13/2023

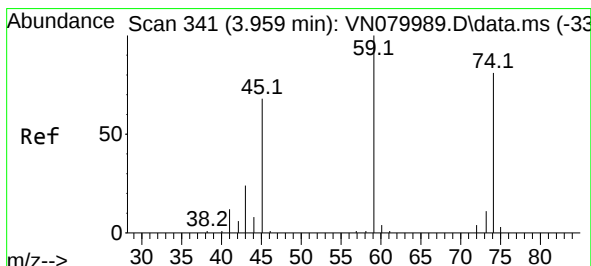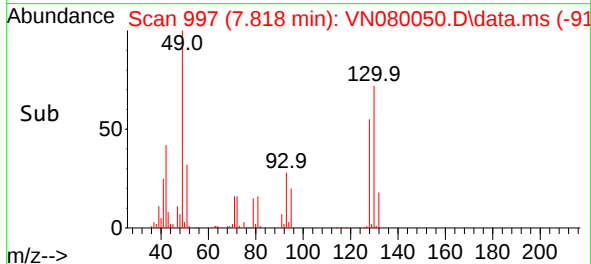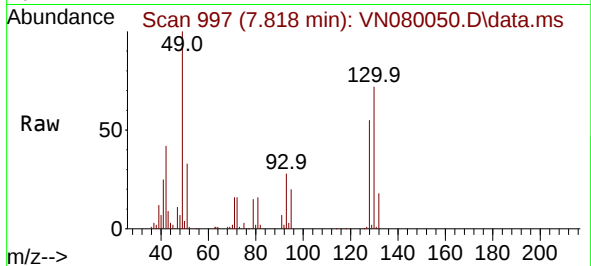

#8
Diethyl Ether
Concen: 0.966 ug/l m
RT: 3.965 min Scan# 342
Delta R.T. 0.000 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59

Tgt Ion: 74 Resp: 2756
Ion Ratio Lower Upper
74 100
45 103.7 19.0 171.0

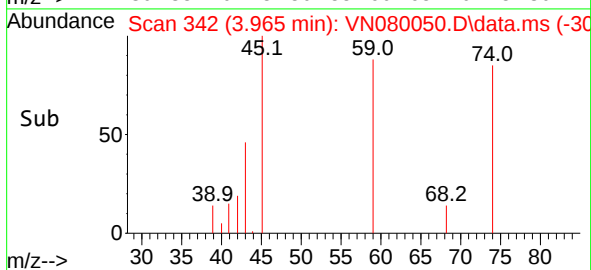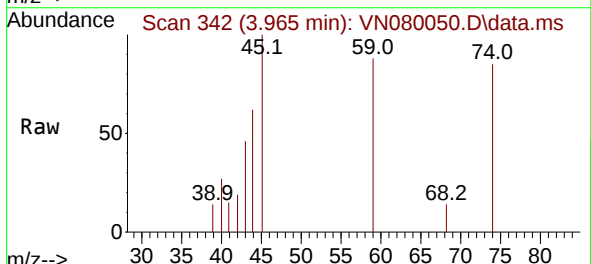

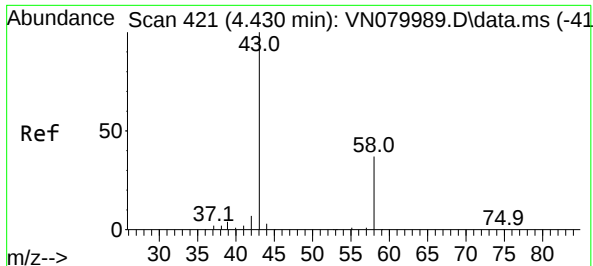

#15

Acetone

Concen: 34.758 ug/l

RT: 4.436 min Scan# 41

Delta R.T. -0.000 min

Lab File: VN080050.D

Acq: 10 Nov 2023 13:59

Instrument :

MSVOA_N

ClientSampleId :

SEMI-ANNUAL-CONDENSATE

Tgt Ion: 58 Resp: 2870

Ion Ratio Lower Upper

58 100





43 287.7 225.2 337.8

Manual Integrations

APPROVED

Reviewed By :John Carlone 11/13/2023

Supervised By :Mahesh Dadoda 11/13/2023

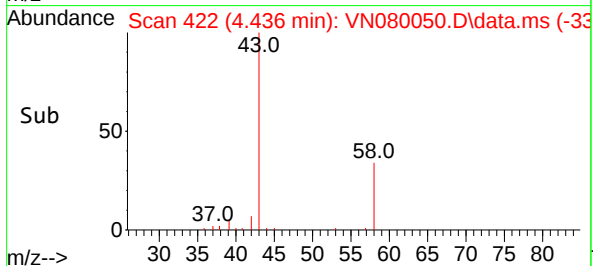

#16

Carbon Disulfide

Concen: 0.809 ug/l

RT: 4.712 min Scan# 469

Delta R.T. -0.006 min

Lab File: VN080050.D




Acq: 10 Nov 2023 13:59


Tgt Ion: 76 Resp: 10976

Ion Ratio Lower Upper

76 100


78 16.2 7.5 11.3#

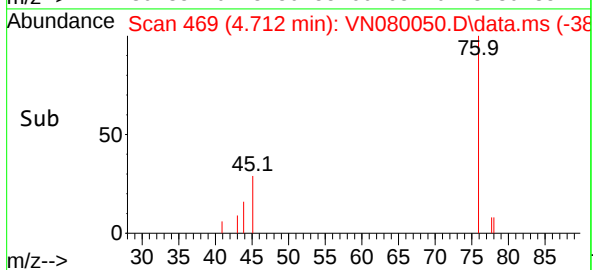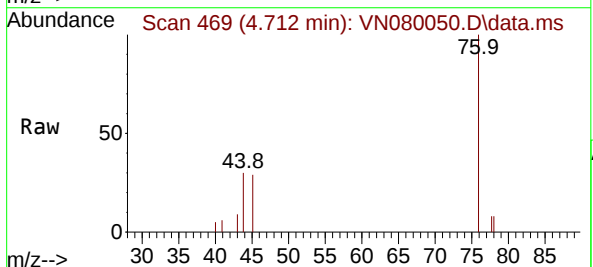

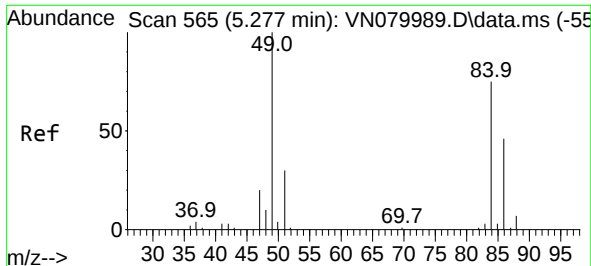

#18
Methylene Chloride
Concen: 1.674 ug/l
RT: 5.271 min Scan# 501
Delta R.T. -0.012 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59




Instrument :
MSVOA_N
ClientSampleId :
SEMI-ANNUAL-CONDENSATE

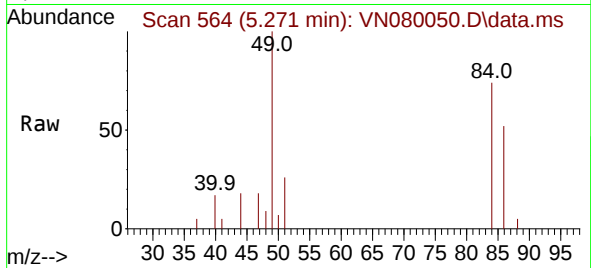

Tgt Ion: 84 Resp: 8914
Ion Ratio Lower Upper
84 100
49 135.4 100.9 151.3
51 35.8 29.4 44.2
86 70.4 48.2 72.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/13/2023
Supervised By :Mahesh Dadoda 11/13/2023

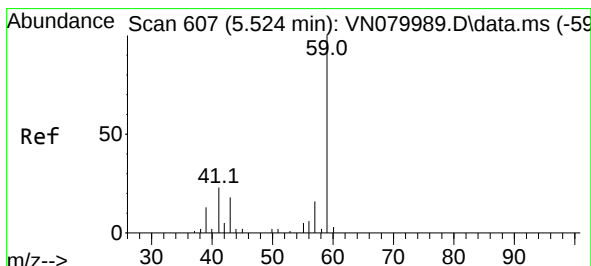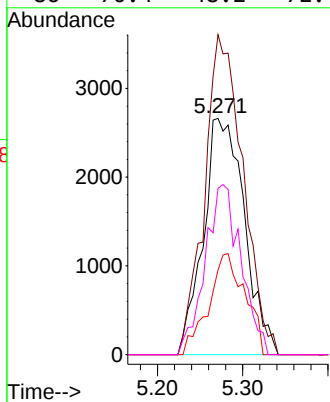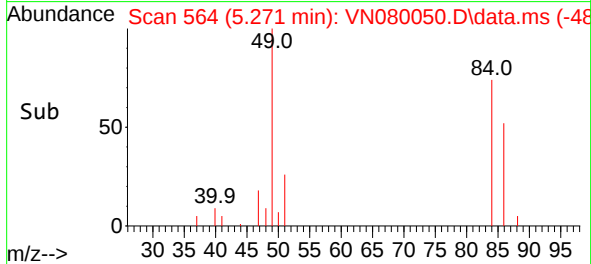

#23
tert-Butyl Alcohol
Concen: 615.257 ug/l
RT: 5.518 min Scan# 606
Delta R.T. -0.006 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59


Tgt Ion: 59 Resp: 406120
Ion Ratio Lower Upper
59 100
52 0.1 0.0 0.0#

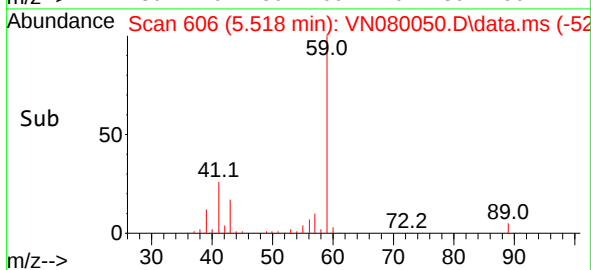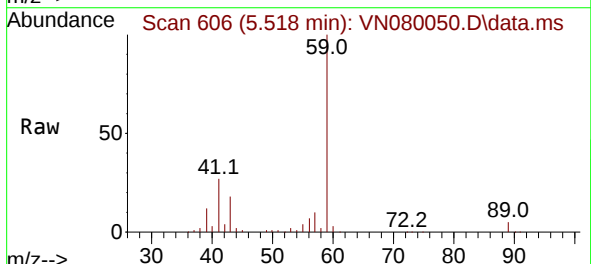



#25
Chloroform
Concen: 27.310 ug/l
RT: 7.965 min Scan# 1023
Delta R.T. -0.000 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59




Instrument :
MSVOA_N
ClientSampleId :
SEMI-ANNUAL-CONDENSATE



Tgt Ion: 83 Resp: 27288
Ion Ratio Lower Upper
83 100
85 61.9 47.4 71.2




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/13/2023
Supervised By :Mahesh Dadoda 11/13/2023

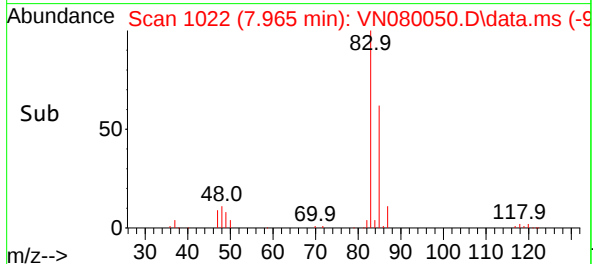

#27
1,2-Dichloroethane-d4
Concen: 30.657 ug/l
RT: 8.583 min Scan# 1127
Delta R.T. 0.001 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59

Tgt Ion: 65 Resp: 198498
Ion Ratio Lower Upper
65 100
67 51.0 42.1 63.1

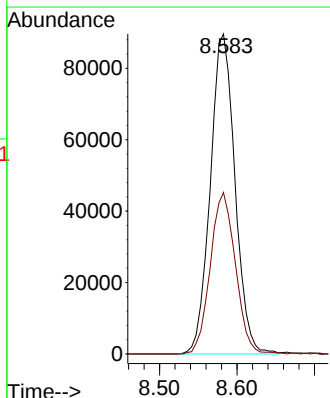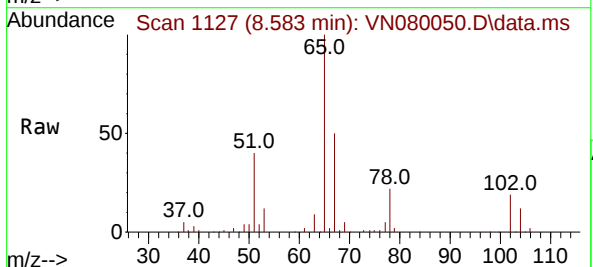

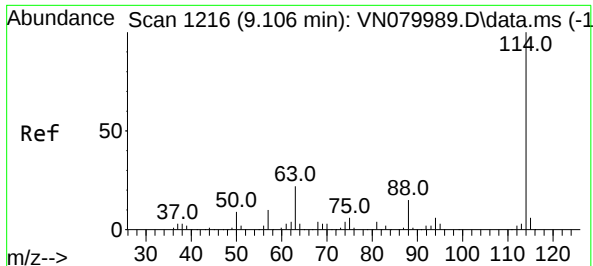

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 9.106 min Scan# 114

Delta R.T. 0.000 min

Lab File: VN080050.D

Acq: 10 Nov 2023 13:59

Instrument :

MSVOA_N

ClientSampleId :

SEMI-ANNUAL-CONDENSATE

Tgt Ion:114 Resp: 425844





Ion	Ratio	Lower	Upper
114	100		
63	21.8	18.1	27.1
88	16.2	12.2	18.2

Manual Integrations

APPROVED

Reviewed By :John Carlone 11/13/2023

Supervised By :Mahesh Dadoda 11/13/2023

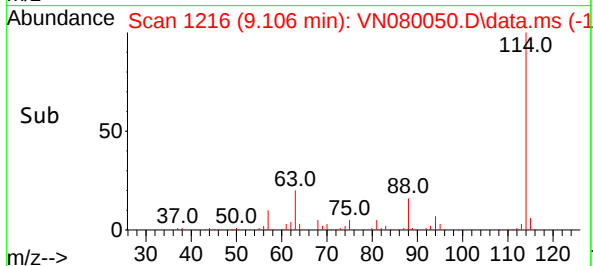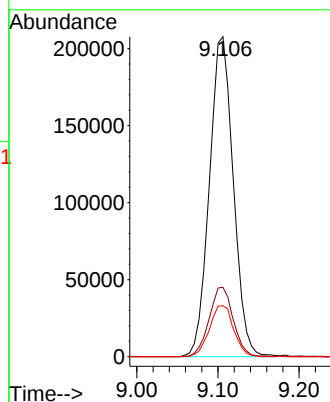

#30

2-Butanone

Concen: 43.158 ug/l

RT: 7.488 min Scan# 941




Delta R.T. 0.000 min


Lab File: VN080050.D

Acq: 10 Nov 2023 13:59

Tgt Ion: 43 Resp: 150637


Ion	Ratio	Lower	Upper
43	100		
57	7.7	6.4	9.6
72	27.9	20.7	31.1

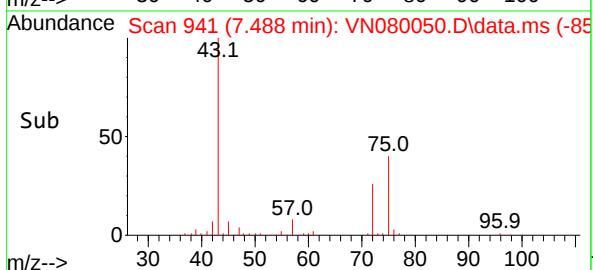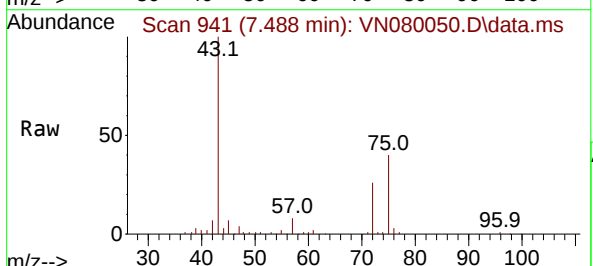

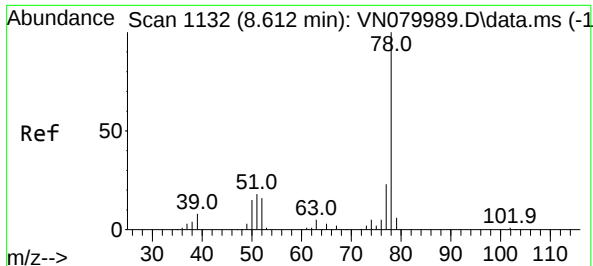

#34
Benzene
Concen: 10.010 ug/l
RT: 8.612 min Scan# 1132
Delta R.T. -0.000 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59




Instrument :
MSVOA_N
ClientSampleId :
SEMI-ANNUAL-CONDENSATE



Tgt Ion: 78 Resp: 21732
Ion Ratio Lower Upper
78 100
77 24.1 19.7 29.5
51 19.6 15.8 23.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/13/2023
Supervised By :Mahesh Dadoda 11/13/2023

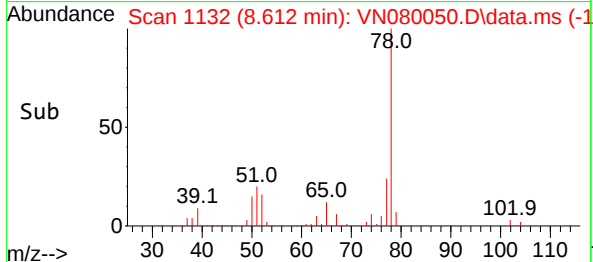

#41
Bromodichloromethane
Concen: 0.800 ug/l
RT: 9.894 min Scan# 1350
Delta R.T. 0.006 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59


Tgt Ion: 83 Resp: 6151
Ion Ratio Lower Upper
83 100
85 71.4 50.3 75.5
127 11.5 6.8 10.2#

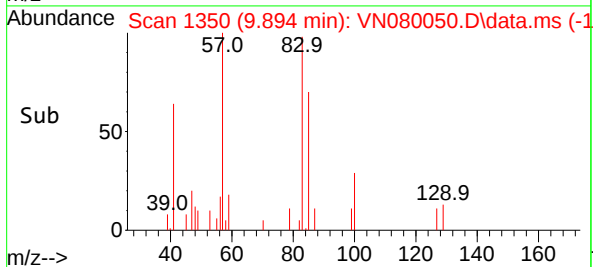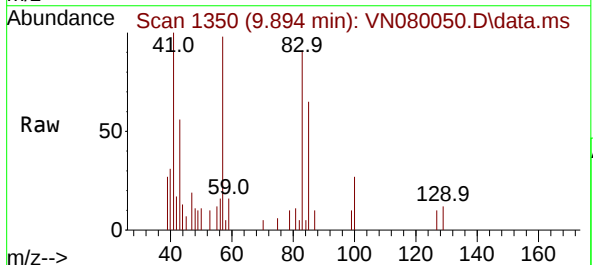

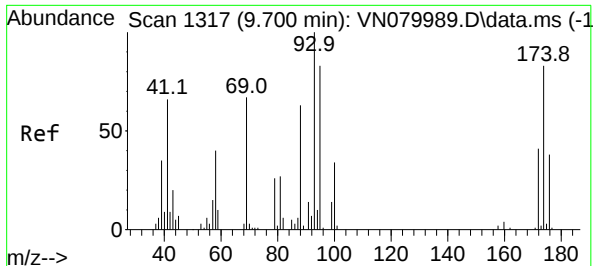

#45
1,4-Dioxane
Concen: 128.888 ug/l
RT: 9.700 min Scan# 1317
Delta R.T. -0.006 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59




Instrument :
MSVOA_N
ClientSampleId :
SEMI-ANNUAL-CONDENSATE

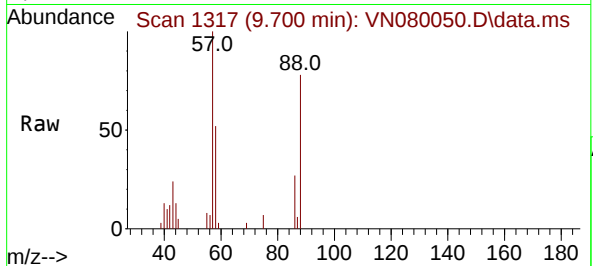


Tgt Ion: 88 Resp: 10612
Ion Ratio Lower Upper
88 100
43 9.6 28.7 43.1
58 82.0 56.9 85.3

Manual Integrations
APPROVED



Reviewed By :John Carlone 11/13/2023
Supervised By :Mahesh Dadoda 11/13/2023

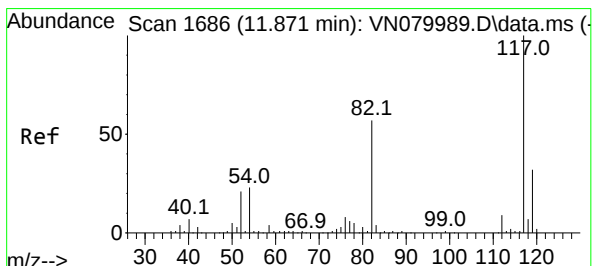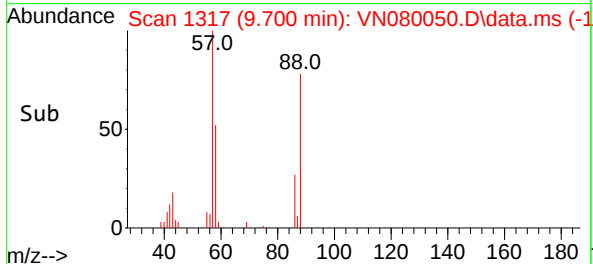


#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. 0.001 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59

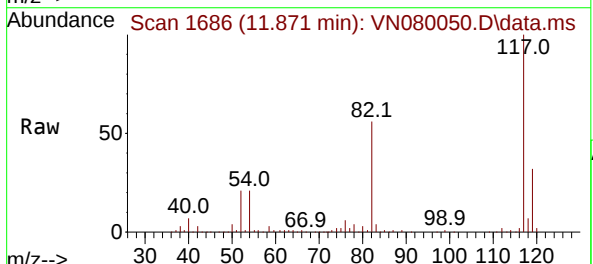

Tgt Ion:117 Resp: 403381
Ion Ratio Lower Upper
117 100
82 57.7 46.2 69.2
119 31.8 25.2 37.8

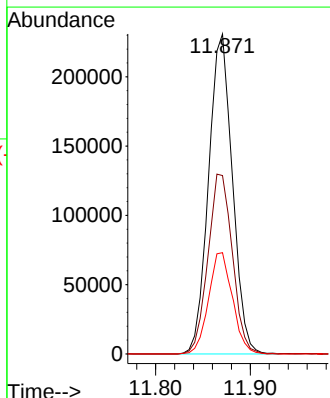







#58
4-Methyl-2-Pentanone
Concen: 6.162 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59

Instrument : MSVOA_N
ClientSampleId : SEMI-ANNUAL-CONDENSATE

Tgt Ion: 43 Resp: 41529
Ion Ratio Lower Upper
43 100
58 35.4 30.4 45.6
85 15.2 13.2 19.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/13/2023
Supervised By :Mahesh Dadoda 11/13/2023

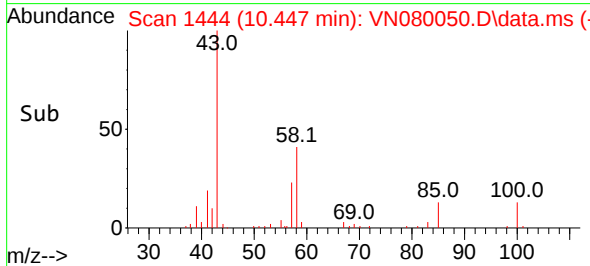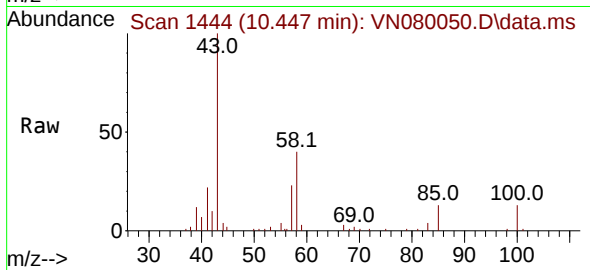

#60
4-Bromofluorobenzene
Concen: 29.409 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59

Tgt Ion: 95 Resp: 189707
Ion Ratio Lower Upper
95 100
174 70.1 60.5 90.7
176 69.9 57.2 85.8

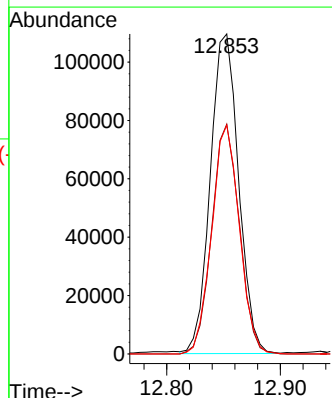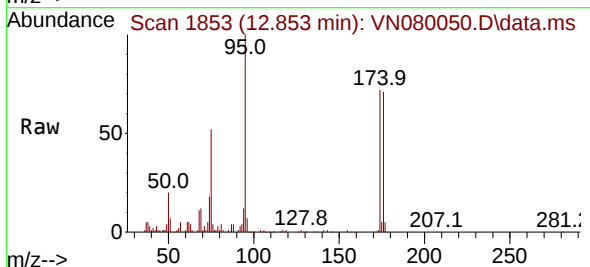

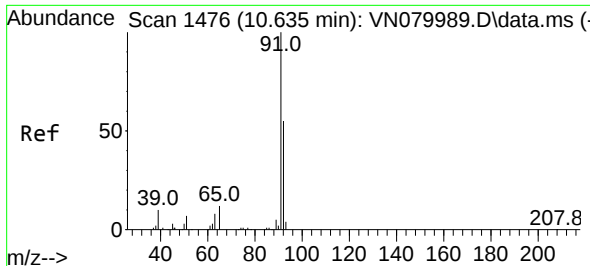





#62
Toluene
Concen: 30.464 ug/l
RT: 10.635 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59

Instrument :
MSVOA_N
ClientSampleId :
SEMI-ANNUAL-CONDENSATE

Tgt Ion: 91 Resp: 710740
Ion Ratio Lower Upper
91 100
92 57.4 45.3 67.9




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/13/2023
Supervised By :Mahesh Dadoda 11/13/2023

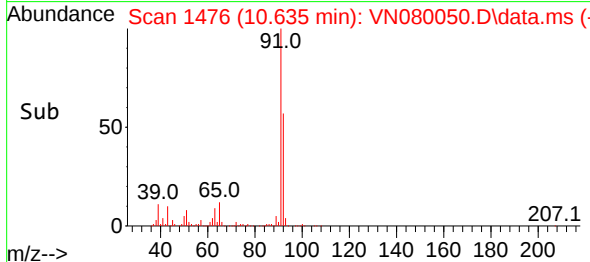

#63
Toluene-d8
Concen: 27.154 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.001 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59


Tgt Ion: 98 Resp: 518997
Ion Ratio Lower Upper
98 100
100 66.1 51.6 77.4

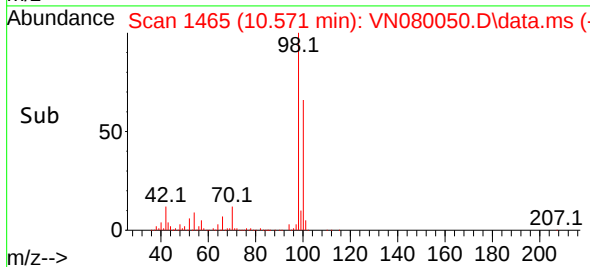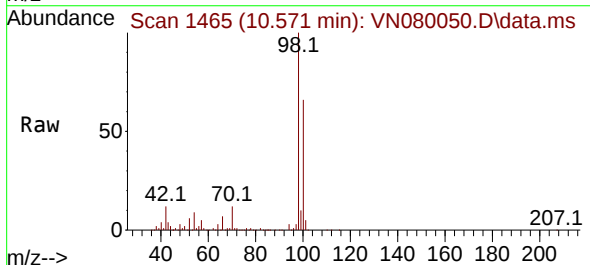



#64
Chlorobenzene
Concen: 4.363 ug/l
RT: 11.894 min Scan# 1690
Delta R.T. 0.000 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59




Instrument :
MSVOA_N
ClientSampleId :
SEMI-ANNUAL-CONDENSATE



Tgt Ion:112 Resp: 60739
Ion Ratio Lower Upper
112 100
114 31.3 28.1 42.1




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/13/2023
Supervised By :Mahesh Dadoda 11/13/2023

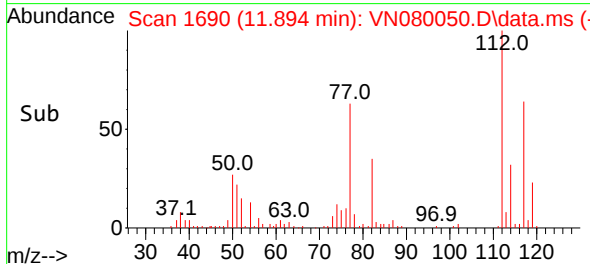

#66
Ethyl Benzene
Concen: 12.652 ug/l
RT: 11.965 min Scan# 1702
Delta R.T. -0.005 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59


Tgt Ion: 91 Resp: 310184
Ion Ratio Lower Upper
91 100
106 28.7 23.8 35.8

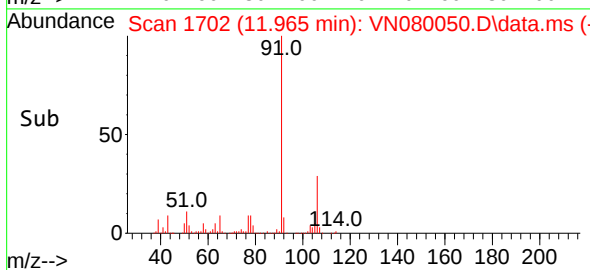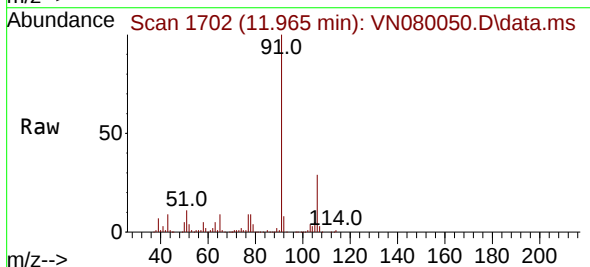

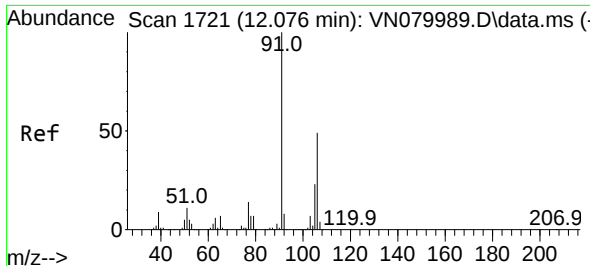

#67
m/p-Xylenes
Concen: 15.880 ug/l
RT: 12.071 min Scan# 1720
Delta R.T. -0.005 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59




Instrument :
MSVOA_N
ClientSampleId :
SEMI-ANNUAL-CONDENSATE



Tgt Ion:106 Resp: 14494
Ion Ratio Lower Upper
106 100
91 209.8 161.8 242.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/13/2023
Supervised By :Mahesh Dadoda 11/13/2023

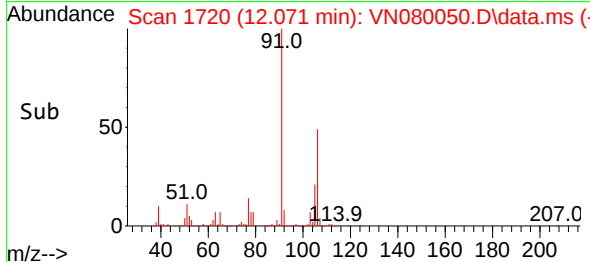

#68
o-Xylene
Concen: 11.138 ug/l
RT: 12.400 min Scan# 1776
Delta R.T. -0.000 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59

Tgt Ion:106 Resp: 97441
Ion Ratio Lower Upper
106 100
91 216.8 109.9 329.7

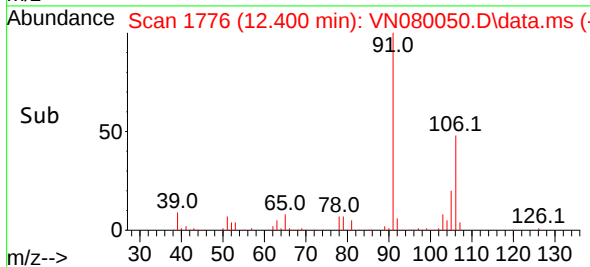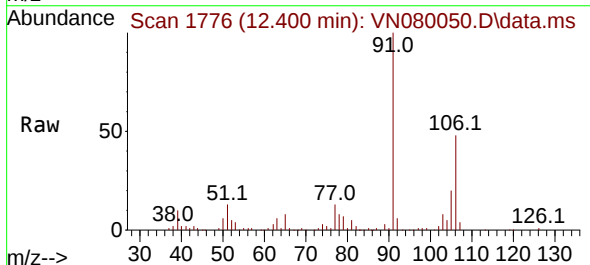

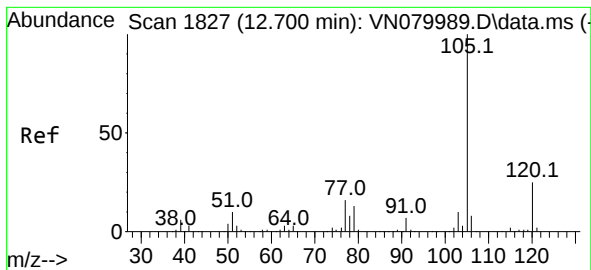

#70

Isopropylbenzene

Concen: 1.853 ug/l

RT: 12.700 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN080050.D

Acq: 10 Nov 2023 13:59

Instrument :

MSVOA_N

ClientSampleId :

SEMI-ANNUAL-CONDENSATE

Tgt Ion:105 Resp: 4044

Ion Ratio Lower Upper

105 100





120 28.7 18.1 33.5

Manual Integrations

APPROVED

Reviewed By :John Carlone 11/13/2023

Supervised By :Mahesh Dadoda 11/13/2023

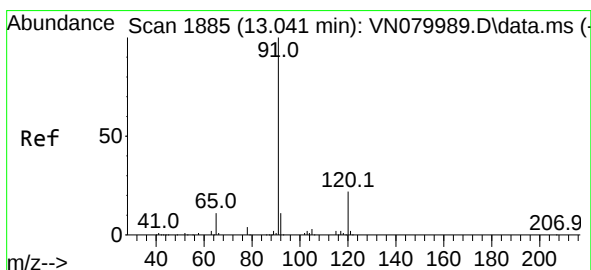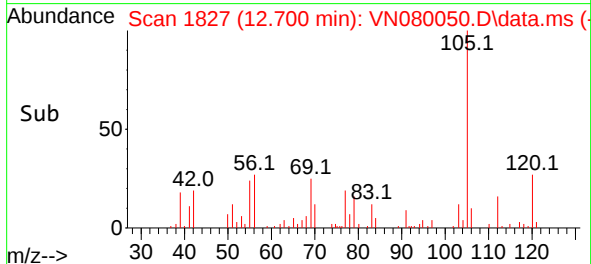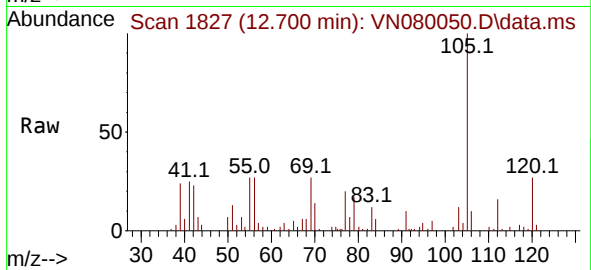

#74

n-propylbenzene

Concen: 0.916 ug/l

RT: 13.041 min Scan# 1885

Delta R.T. 0.000 min

Lab File: VN080050.D




Acq: 10 Nov 2023 13:59


Tgt Ion: 91 Resp: 23925

Ion Ratio Lower Upper

91 100

120 23.3 0.0 42.0

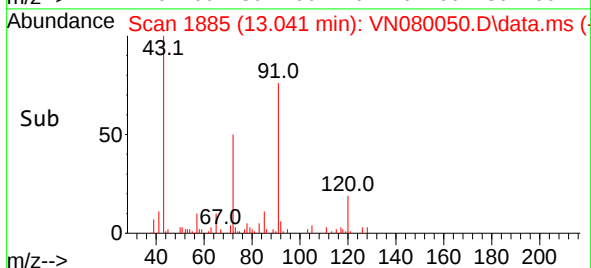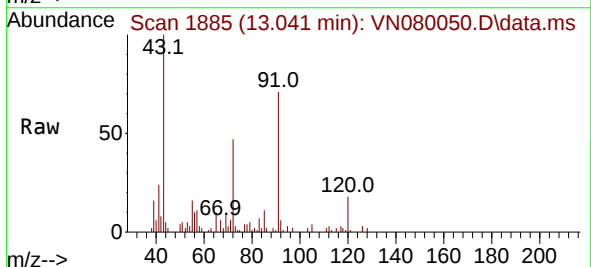

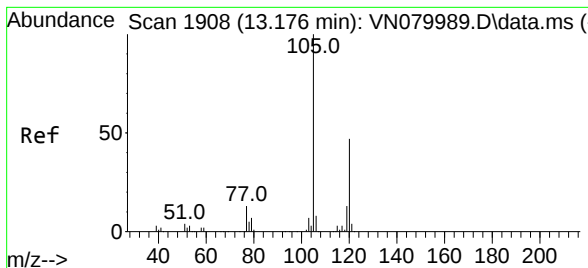





#76
1,3,5-Trimethylbenzene
Concen: 4.715 ug/l
RT: 13.176 min Scan# 1908
Delta R.T. 0.000 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59

Instrument : MSVOA_N
ClientSampleId : SEMI-ANNUAL-CONDENSATE

Tgt Ion:105 Resp: 8511
Ion Ratio Lower Upper
105 100
120 48.2 0.0 93.2




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/13/2023
Supervised By :Mahesh Dadoda 11/13/2023

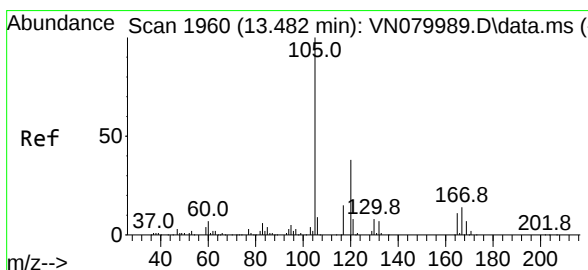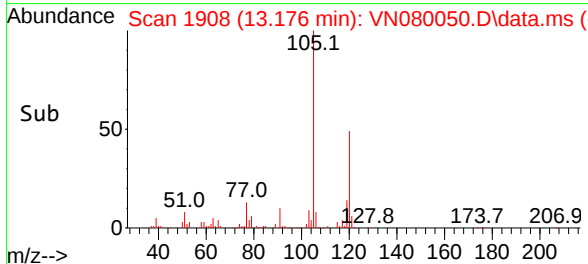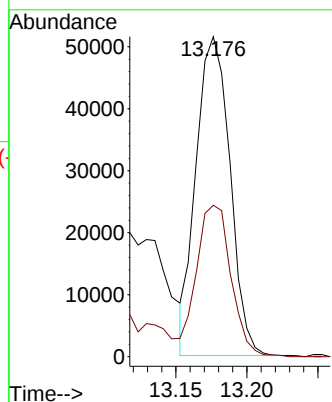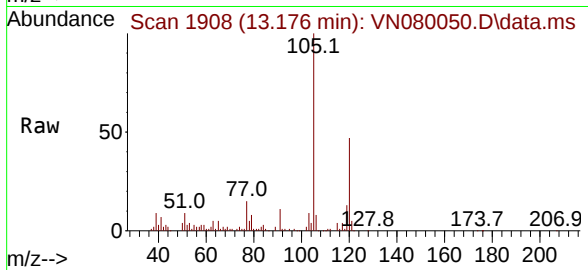

#80
1,2,4-Trimethylbenzene
Concen: 15.065 ug/l
RT: 13.488 min Scan# 1961
Delta R.T. 0.000 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59


Tgt Ion:105 Resp: 266631
Ion Ratio Lower Upper
105 100
120 43.7 0.0 88.6

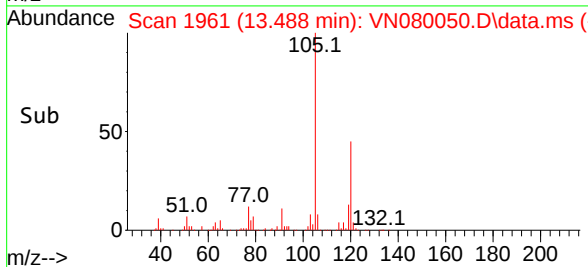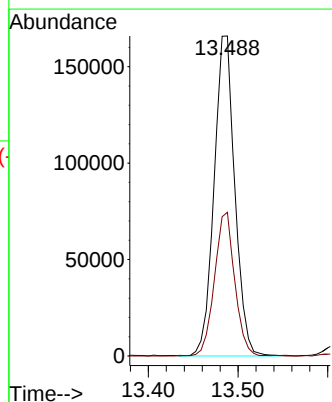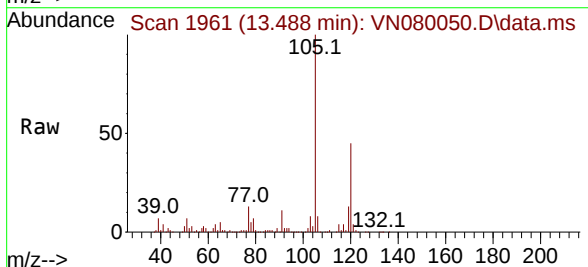

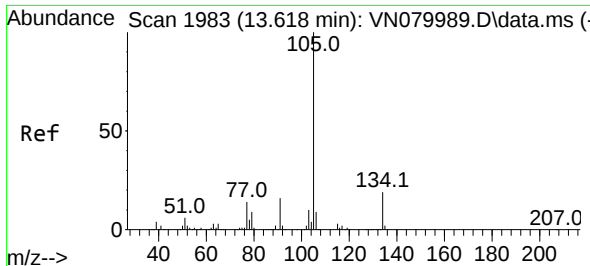

#81
 sec-Butylbenzene
 Concen: 0.795 ug/l m
 RT: 13.617 min Scan# 1983
 Delta R.T. 0.000 min
 Lab File: VN080050.D
 Acq: 10 Nov 2023 13:59




Instrument :
 MSVOA_N
 ClientSampleId :
 SEMI-ANNUAL-CONDENSATE

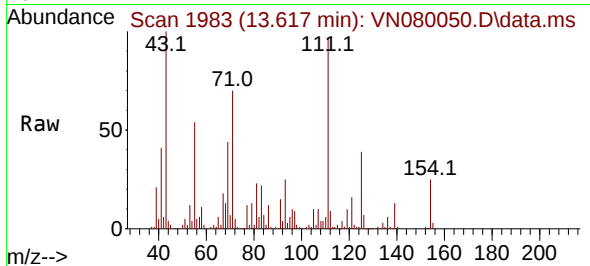


Tgt Ion:105 Resp: 1587
 Ion Ratio Lower Upper
 105 100
 134 0.0 0.0 38.2

Manual Integrations
 APPROVED



Reviewed By :John Carlone 11/13/2023
 Supervised By :Mahesh Dadoda 11/13/2023

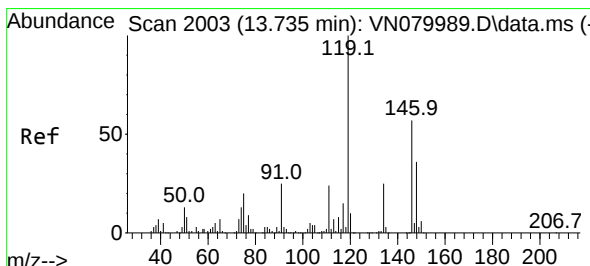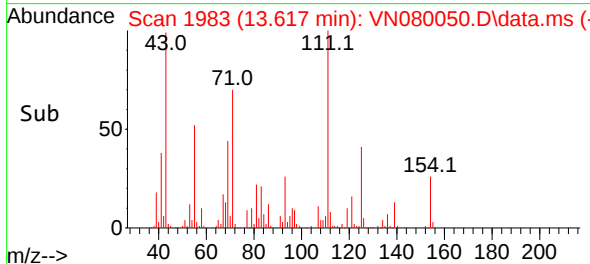


#82
 p-Isopropyltoluene
 Concen: 67.458 ug/l
 RT: 13.729 min Scan# 2002
 Delta R.T. -0.006 min
 Lab File: VN080050.D
 Acq: 10 Nov 2023 13:59

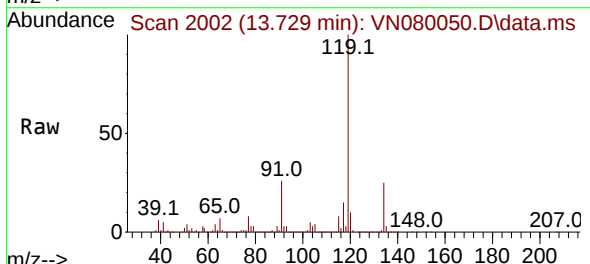


Tgt Ion:119 Resp: 1093136
 Ion Ratio Lower Upper
 119 100
 134 25.5 0.0 52.2
 91 26.1 0.0 50.0

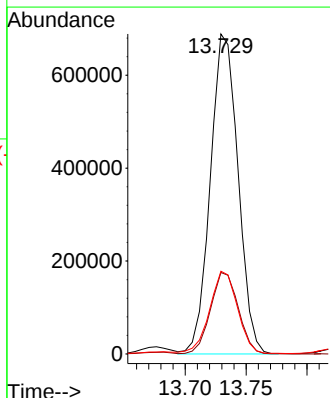



#83
1,3-Dichlorobenzene
Concen: 0.419 ug/l
RT: 13.735 min Scan# 2003
Delta R.T. 0.000 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59




Instrument :
MSVOA_N
ClientSampleId :
SEMI-ANNUAL-CONDENSATE




Tgt Ion:146 Resp: 409
Ion Ratio Lower Upper
146 100
111 56.7 21.0 63.0
148 62.5 32.4 97.0

Manual Integrations
APPROVED



Reviewed By :John Carlone 11/13/2023
Supervised By :Mahesh Dadoda 11/13/2023

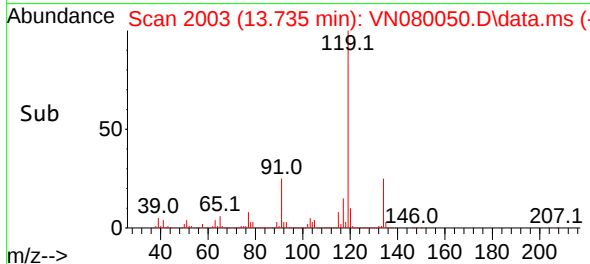


#84
1,4-Dichlorobenzene
Concen: 33.156 ug/l
RT: 13.817 min Scan# 2017
Delta R.T. 0.000 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59

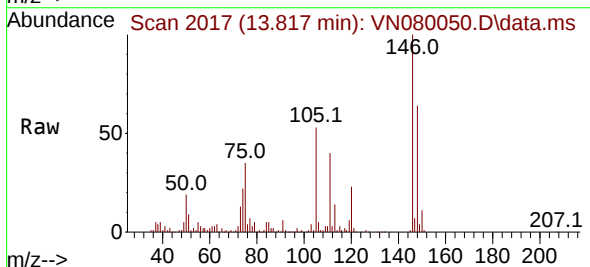

Tgt Ion:146 Resp: 318144
Ion Ratio Lower Upper
146 100
111 41.6 19.9 59.7
148 64.0 32.6 97.7

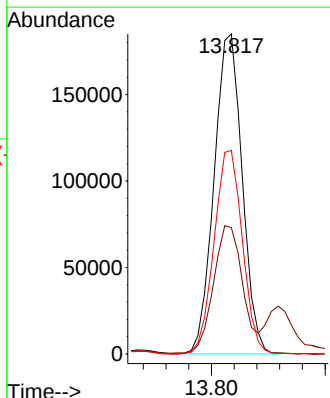

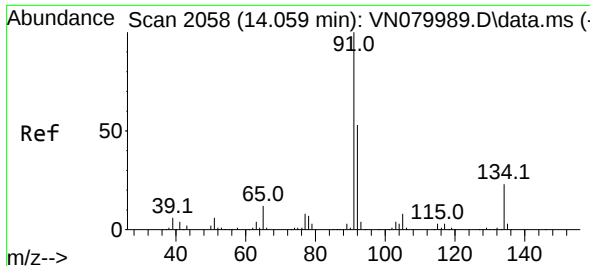





#85
n-Butylbenzene
Concen: 0.258 ug/l
RT: 14.053 min Scan# 2057
Delta R.T. -0.006 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59

Instrument :
MSVOA_N
ClientSampleId :
SEMI-ANNUAL-CONDENSATE

Tgt Ion: 91	Resp: 3490
Ion Ratio	Lower Upper
91 100	
92 26.6	0.0 99.6
134 1.8	0.0 46.2




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/13/2023
Supervised By :Mahesh Dadoda 11/13/2023

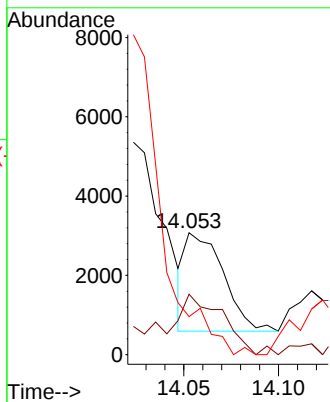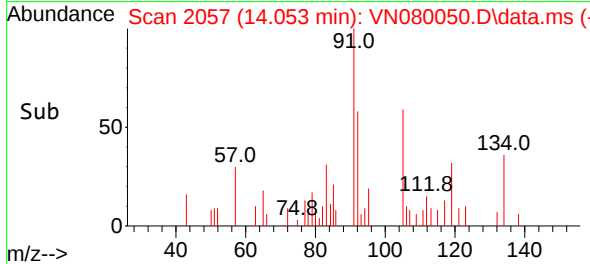

#87
1,2-Dichlorobenzene
Concen: 1.309 ug/l
RT: 14.112 min Scan# 2067
Delta R.T. 0.001 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59


Tgt Ion:146	Resp: 12225
Ion Ratio	Lower Upper
146 100	
111 48.3	22.0 66.0
148 70.1	31.1 93.5

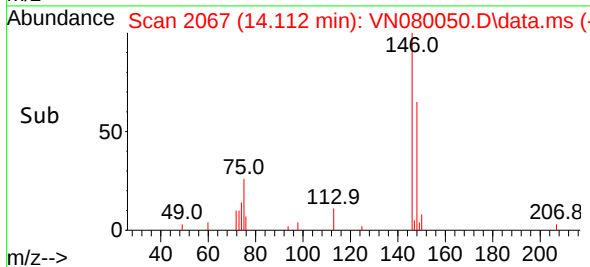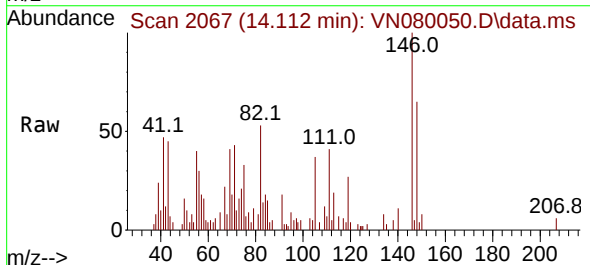

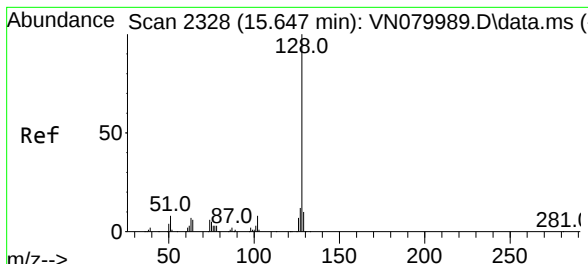

#91
Naphthalene
Concen: 44.117 ug/l
RT: 15.647 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN080050.D
Acq: 10 Nov 2023 13:59

Instrument :
MSVOA_N
ClientSampleId :
SEMI-ANNUAL-CONDENSATE

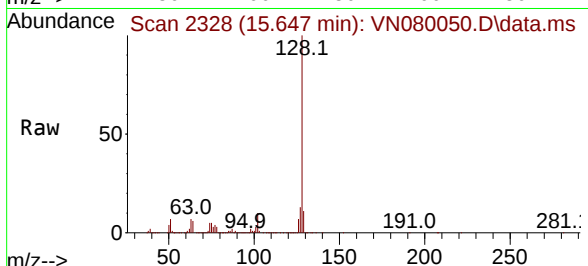

Tgt Ion:128 Resp: 612572
Ion Ratio Lower Upper
128 100
127 12.8 10.9 16.3
129 10.9 8.6 12.8

Manual Integrations
APPROVED

Reviewed By :John Carlone 11/13/2023
Supervised By :Mahesh Dadoda 11/13/2023

