
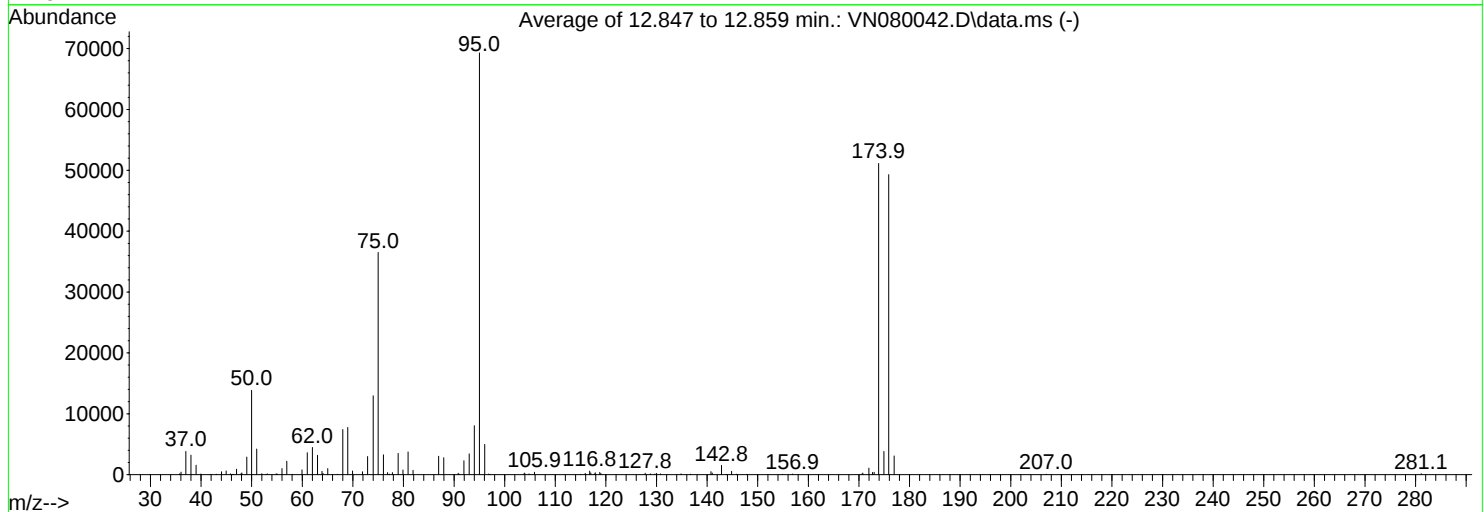


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111023\
Data File : VN080042.D
Acq On : 10 Nov 2023 09:32
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N110823W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Nov 09 04:02:05 2023

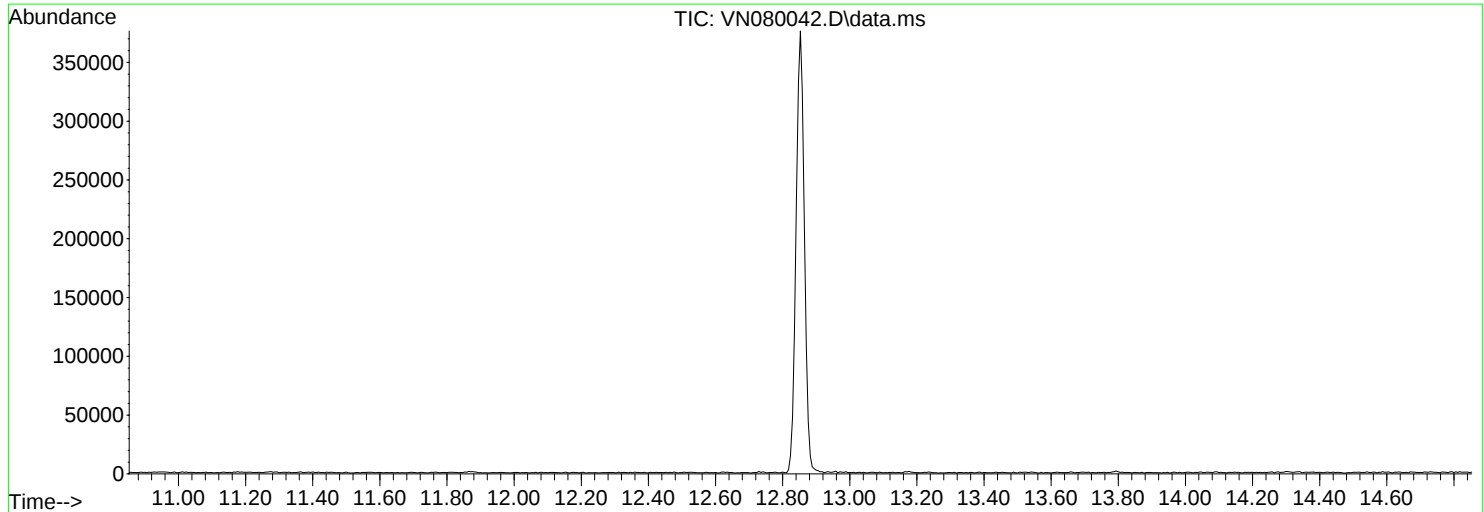

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	13859	PASS
75	95	30	60	52.7	36509	PASS
95	95	100	100	100.0	69304	PASS
96	95	5	9	7.2	4960	PASS
173	174	0.00	2	0.8	386	PASS
174	95	50	100	73.8	51136	PASS
175	174	5	9	7.5	3818	PASS
176	174	95	101	96.4	49307	PASS
177	176	5	9	6.2	3067	PASS