

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN111119\
 Data File : VN059149.D
 Acq On : 11 Nov 2019 10:50
 Operator : JC/SP
 Sample : K5775-01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 12 00:39:41 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110619W.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 07 04:00:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	497677	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.57	114	767427	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	657856	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	224124	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.00	65	309030	50.51	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.02%	
35) Dibromofluoromethane	7.57	113	234006	51.07	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.14%	
50) Toluene-d8	10.08	98	922260	51.10	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.20%	
62) 4-Bromofluorobenzene	12.40	95	286733	44.06	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.12%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	3.80	43	1678	0.527	ug/l #	44
18) Methyl Acetate	4.30	43	1940	0.257	ug/l #	53
31) Cyclohexane	7.64	56	10155	1.066	ug/l #	1
36) 1,1-Dichloropropene	7.64	75	38379	5.350	ug/l #	49
38) Carbon Tetrachloride	7.64	117	48207	6.752	ug/l #	17
76) 1,2,3-Trichloropropane	12.40	75	142082	27.845	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.40	75	142082	73.547	ug/l #	13
93) 1,2,4-Trichlorobenzene	14.91	180	223	3.096	ug/l #	40
95) Naphthalene	15.13	128	854	3.114	ug/l #	70

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN111119\
Data File : VN059149.D
Acq On : 11 Nov 2019 10:50
Operator : JC/SP
Sample : K5775-01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Nov 12 00:39:41 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N110619W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 07 04:00:41 2019
Response via : Initial Calibration

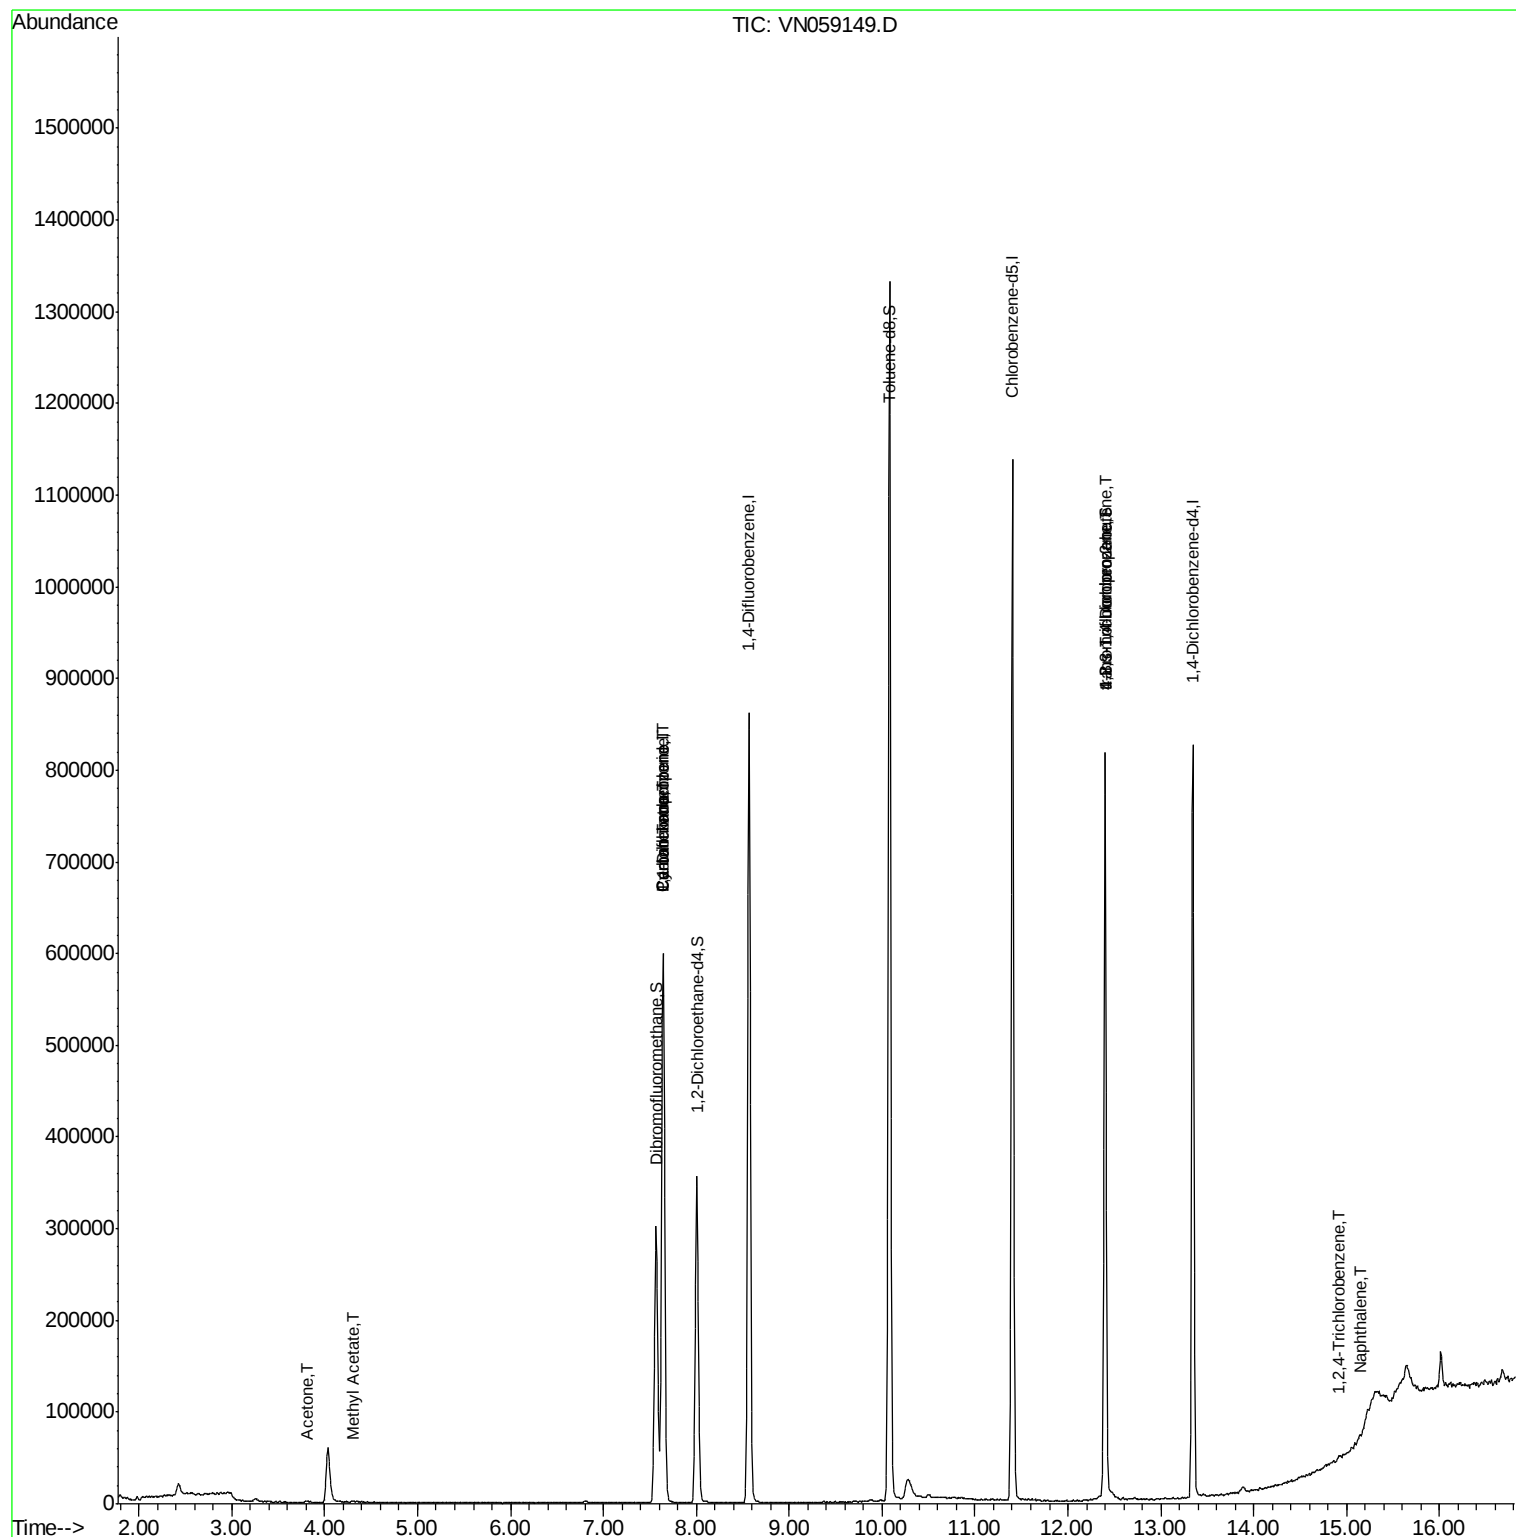



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.64 min Scan# 1826

Delta R.T. -0.00 min

Lab File: VN059149.D

Acq: 11 Nov 2019 10:50

Instrument :

MSVOA_N


ClientSampleId :

Tot Ion:168 Resp: 497677

Ion Ratio Lower Upper

168 100

99 57.8 45.7 68.5

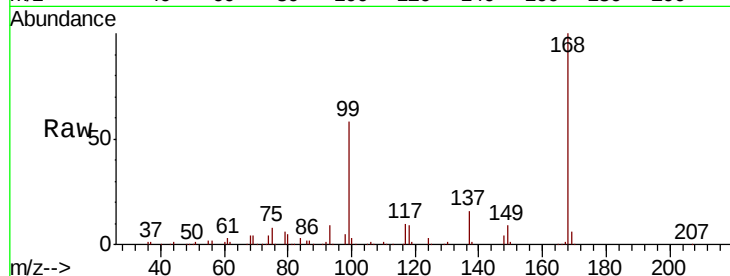

Abundance Ion 167.90 (167.60 to 168.60): VN059149.D (-1733) (-)

Ion 98.90 (98.60 to 99.60): VN059149.D (-1733) (-)

7.64

200000



150000

100000

50000

0

Time--> 7.50 7.60 7.70

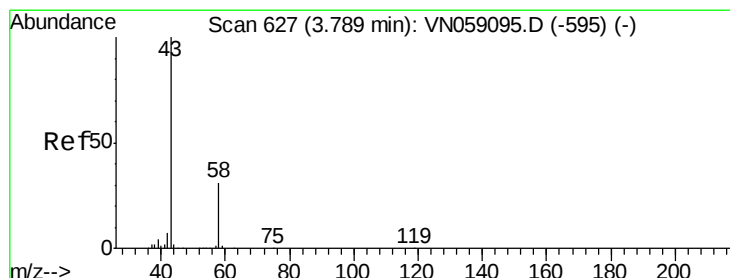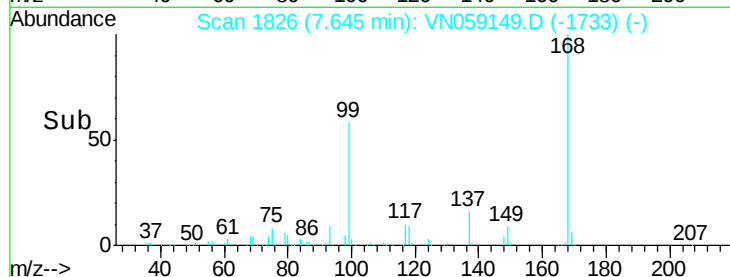

#16

Acetone

Concen: 0.527 ug/l

RT: 3.80 min Scan# 631

Delta R.T. 0.01 min

Lab File: VN059149.D


Acq: 11 Nov 2019 10:50

Tgt Ion: 43 Resp: 1678

Ion Ratio Lower Upper

43 100

58 0.0 24.9 37.3#

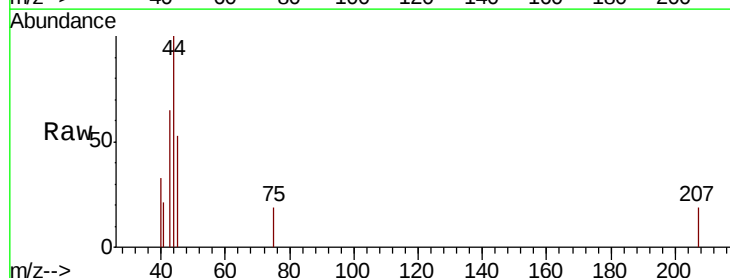

Abundance Ion 43.00 (42.70 to 43.70): VN059149.D (-534) (-)

Ion 58.00 (57.70 to 58.70): VN059149.D (-534) (-)

3.80


600


400

200

0

Time--> 3.75 3.80 3.85




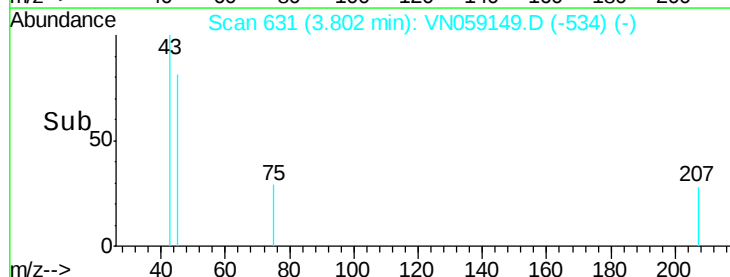




#18
Methyl Acetate
Concen: 0.257 ug/l
RT: 4.30 min Scan# 786
Delta R.T. 0.00 min
Lab File: VN059149.D
Acq: 11 Nov 2019 10:50




Instrument :
MSVOA_N
ClientSampled :


Tot Ion: 43 Resp: 1940
Ion Ratio Lower Upper
43 100
74 0.0 17.8 26.8#

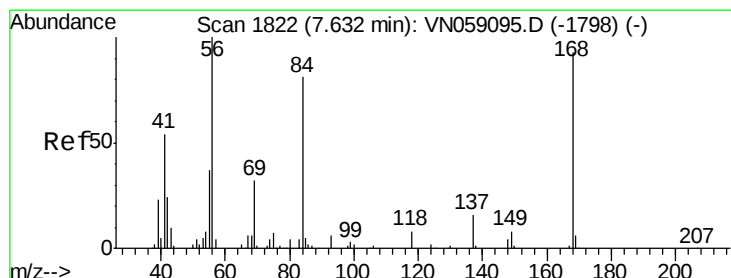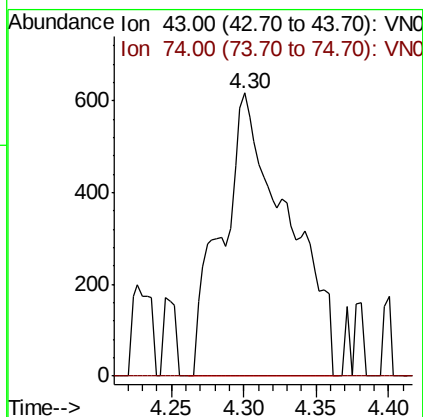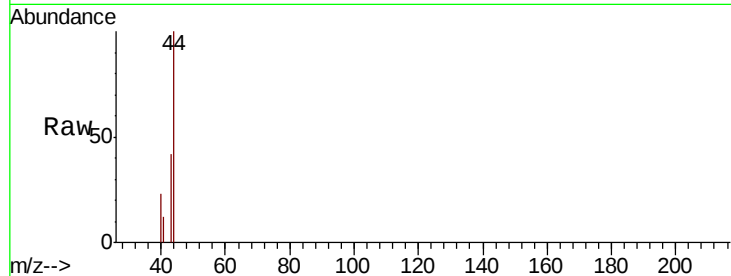

#31
Cyclohexane
Concen: 1.066 ug/l
RT: 7.64 min Scan# 1826
Delta R.T. 0.01 min
Lab File: VN059149.D
Acq: 11 Nov 2019 10:50

Tgt Ion: 56 Resp: 10155
Ion Ratio Lower Upper
56 100
69 170.9 25.8 38.8#
84 130.5 65.0 97.4#



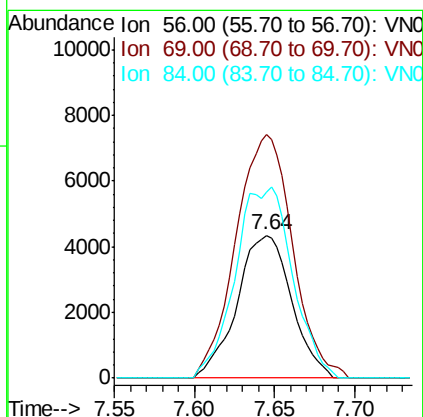
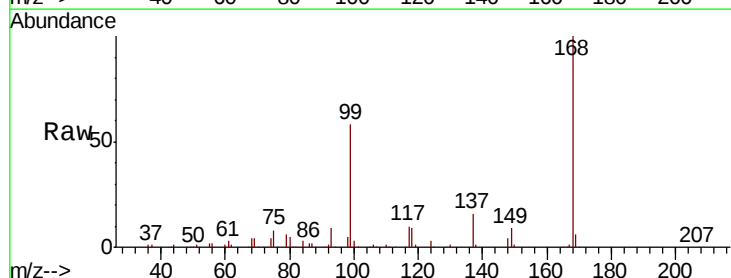


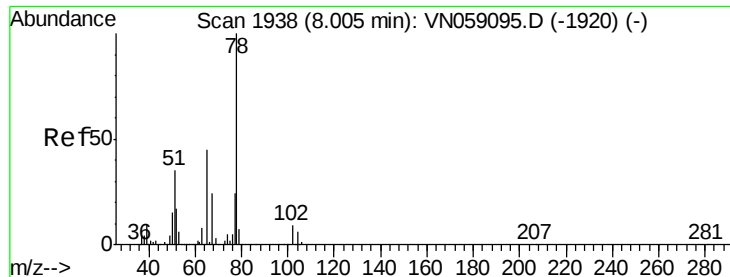

#33
 1,2-Dichloroethane-d4
 Concen: 50.514 ug/l
 RT: 8.00 min Scan# 1938
 Delta R.T. -0.00 min
 Lab File: VN059149.D
 Acq: 11 Nov 2019 10:50




Instrument :
 MSVOA_N
 ClientSampleId :


Tot Ion: 65 Resp: 309030
 Ion Ratio Lower Upper
 65 100
 67 52.5 0.0 107.4

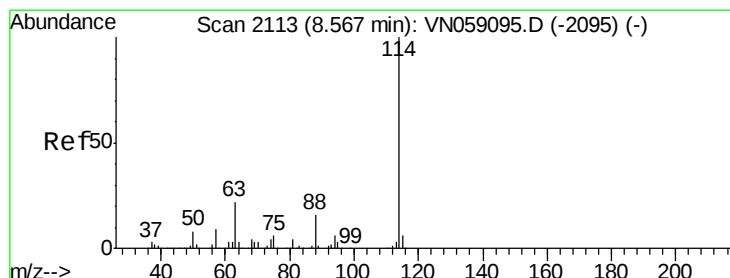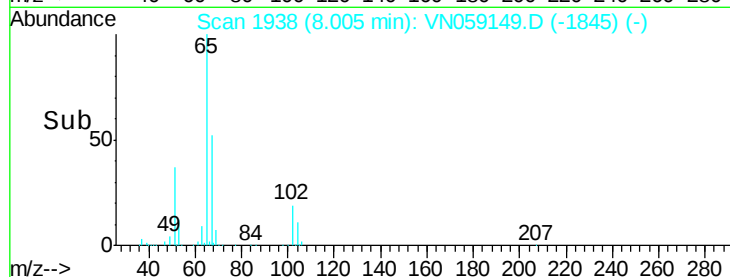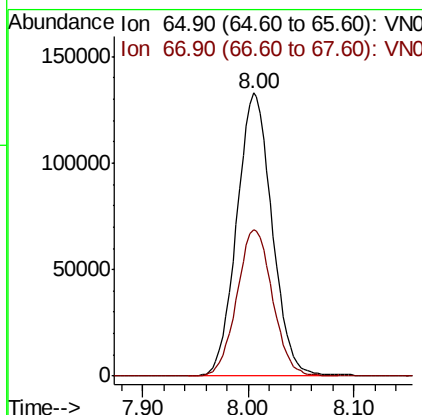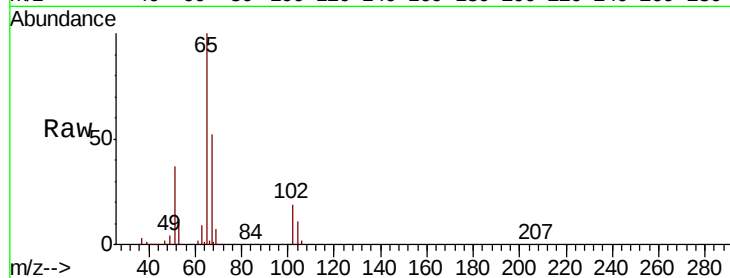

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.57 min Scan# 2113
 Delta R.T. -0.00 min
 Lab File: VN059149.D
 Acq: 11 Nov 2019 10:50

Tgt Ion: 114 Resp: 767427
 Ion Ratio Lower Upper
 114 100
 63 21.4 0.0 43.4
 88 16.5 0.0 32.2


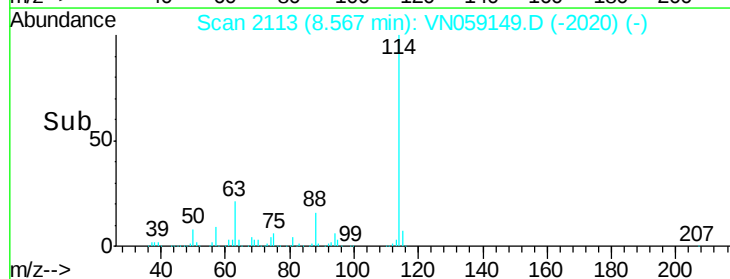
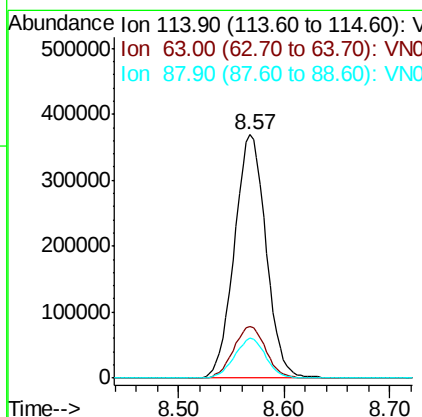
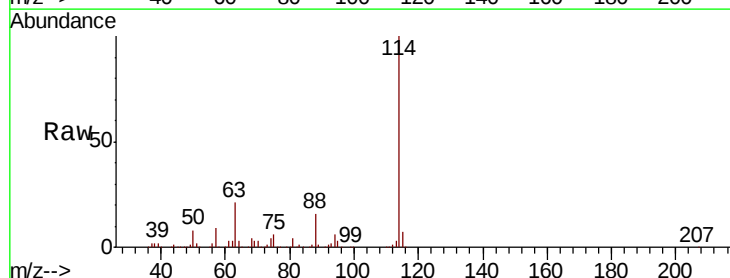




#35
Dibromofluoromethane
Concen: 51.068 ug/l
RT: 7.57 min Scan# 1802
Delta R.T. -0.00 min
Lab File: VN059149.D
Acq: 11 Nov 2019 10:50




Instrument :
MSVOA_N
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
113	100		
111	100.8	82.8	124.2
192	19.9	16.1	24.1

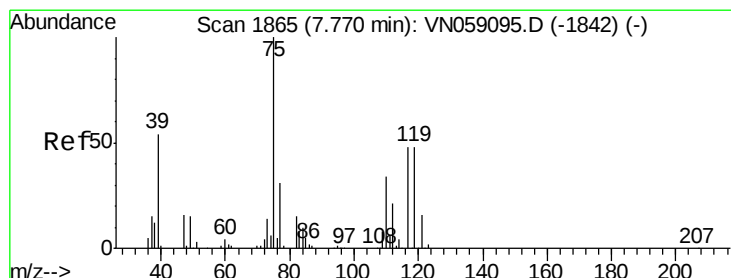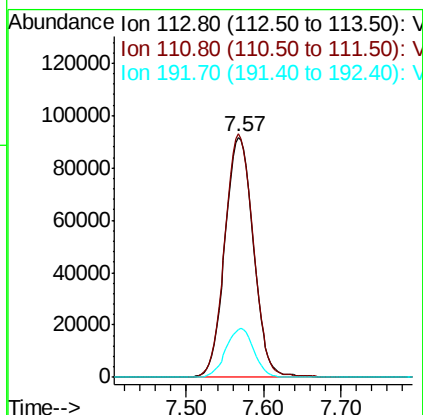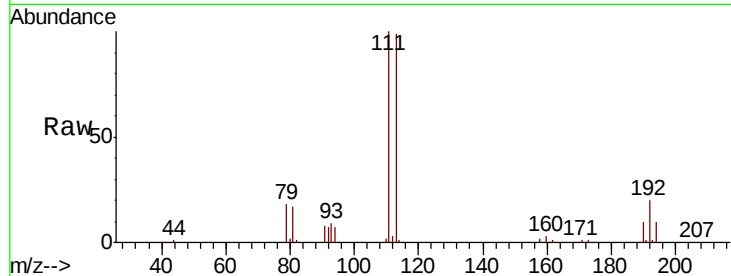

#36
1,1-Dichloropropene
Concen: 5.350 ug/l
RT: 7.64 min Scan# 1825
Delta R.T. -0.13 min
Lab File: VN059149.D
Acq: 11 Nov 2019 10:50

Tgt Ion	Ratio	Lower	Upper
75	100		
110	8.0	17.1	51.2#
77	0.0	24.8	37.2#

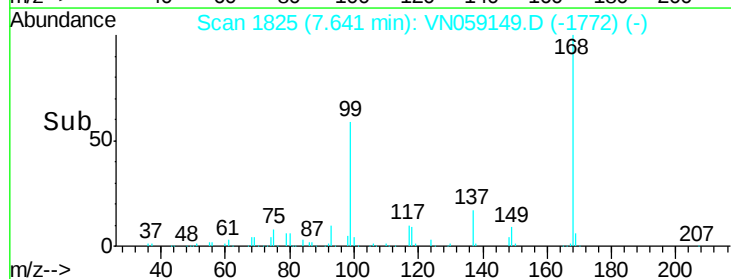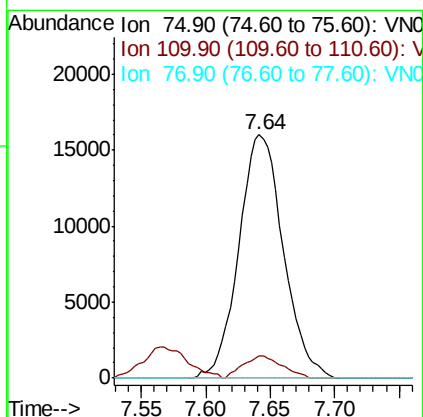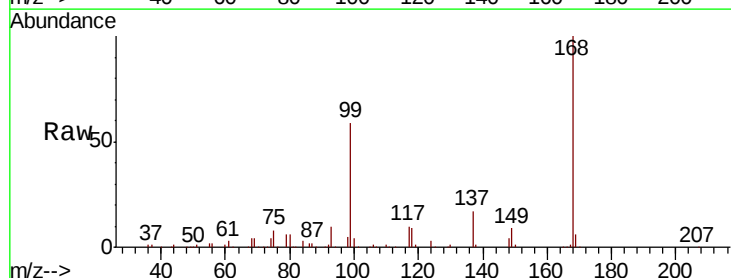



#38

Carbon Tetrachloride

Concen: 6.752 ug/l

RT: 7.64 min Scan# 1826

Delta R.T. -0.11 min

Lab File: VN059149.D

Acq: 11 Nov 2019 10:50

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion:117 Resp: 48207

Ion Ratio Lower Upper

117 100

119 6.1 75.6 113.4#




121 0.0 24.6 36.8#

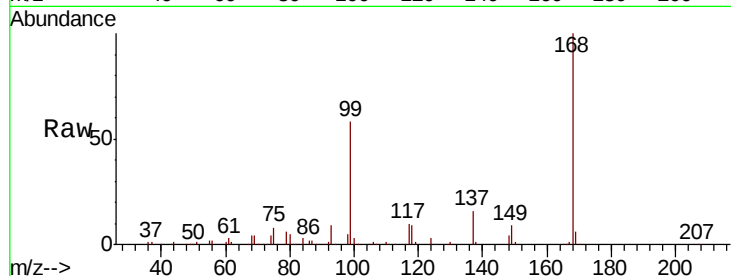

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

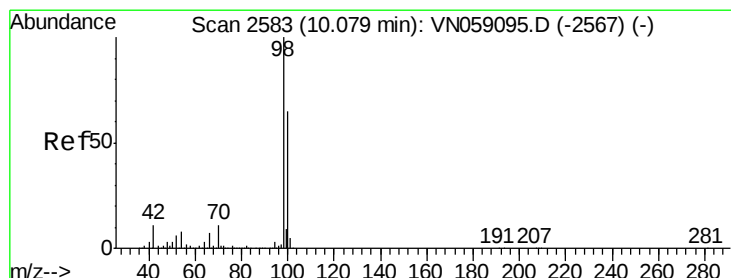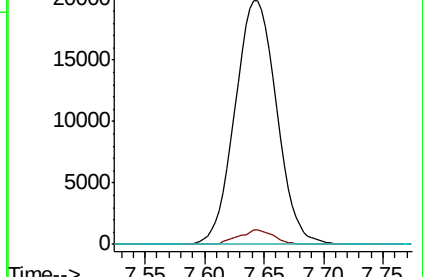

#50

Toluene-d8

Concen: 51.097 ug/l

RT: 10.08 min Scan# 2583

Delta R.T. -0.00 min

Lab File: VN059149.D


Acq: 11 Nov 2019 10:50

Tgt Ion: 98 Resp: 922260

Ion Ratio Lower Upper



98 100


100 64.2 52.2 78.2

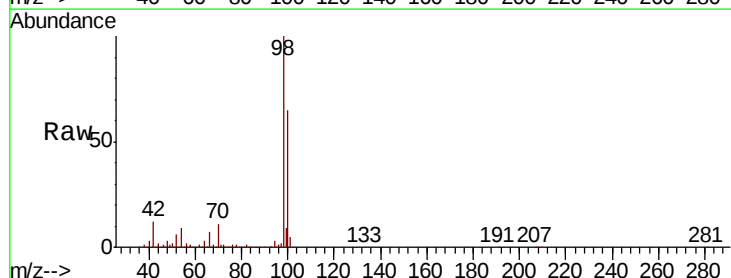

Abundance Ion 98.00 (97.70 to 98.70): V

Ion 100.00 (99.70 to 100.70): V

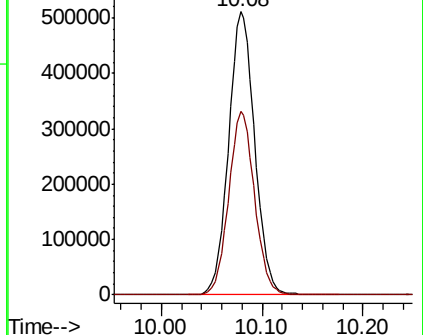

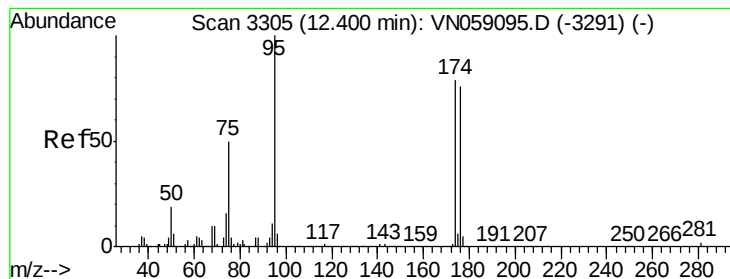

#62

4-Bromofluorobenzene

Concen: 44.059 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN059149.D

Acq: 11 Nov 2019 10:50

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion: 95 Resp: 286733

Ion Ratio Lower Upper

95 100

174 77.3 0.0 158.2




176 75.0 0.0 151.8

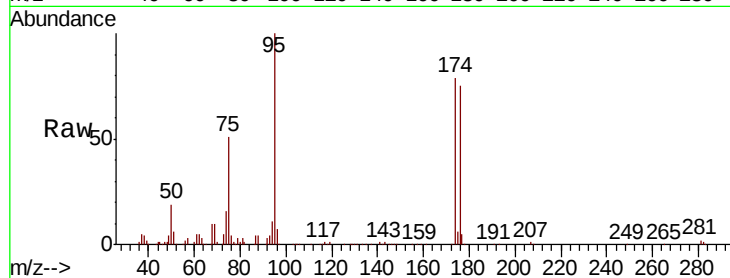

Abundance Ion 94.90 (94.60 to 95.60): VN0

Ion 173.80 (173.50 to 174.50): VN0

Ion 175.80 (175.50 to 176.50): VN0

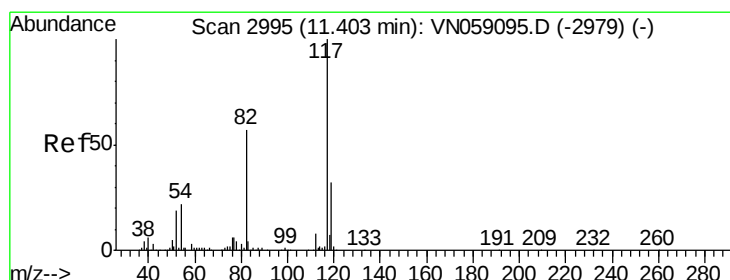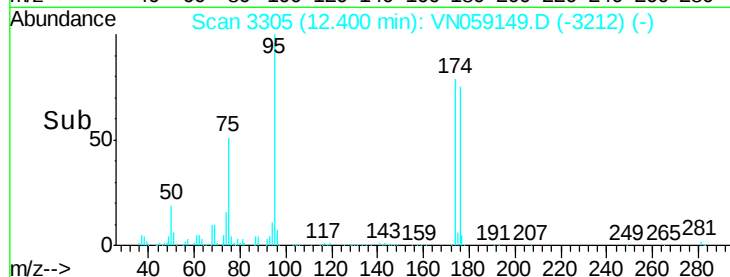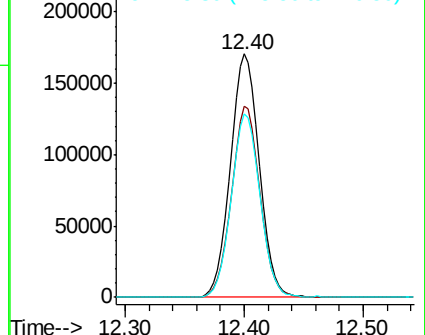

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.40 min Scan# 2995

Delta R.T. -0.00 min

Lab File: VN059149.D

Acq: 11 Nov 2019 10:50


Tgt Ion: 117 Resp: 657856

Ion Ratio Lower Upper

117 100

82 56.6 45.8 68.8



119 32.2 25.8 38.6

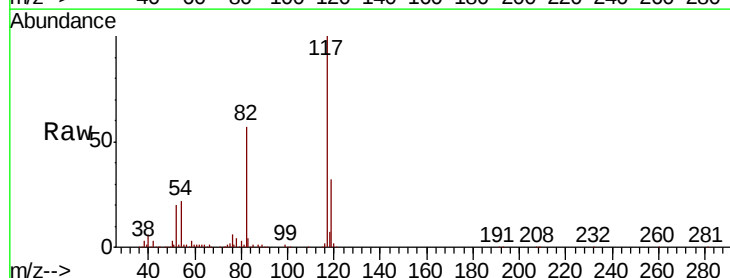


Abundance Ion 116.90 (116.60 to 117.60): VN0

Ion 82.00 (81.70 to 82.70): VN0

Ion 118.90 (118.60 to 119.60): VN0

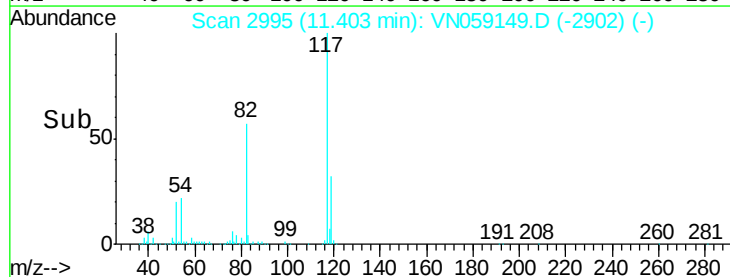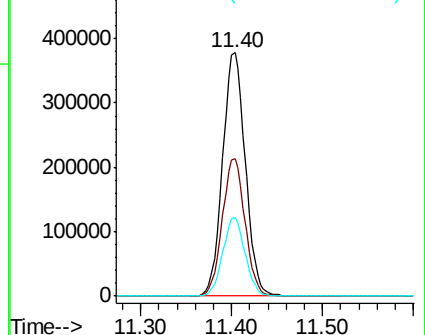







#72

1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.35 min Scan# 3599
Delta R.T. -0.00 min
Lab File: VN059149.D
Acq: 11 Nov 2019 10:50

Instrument :
MSVOA_N
ClientSampled :




Tot Ion	Ratio	Lower	Upper
152	100		
115	60.1	29.4	88.2
150	158.7	0.0	345.8

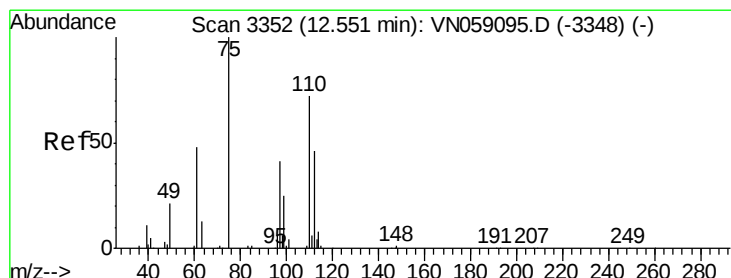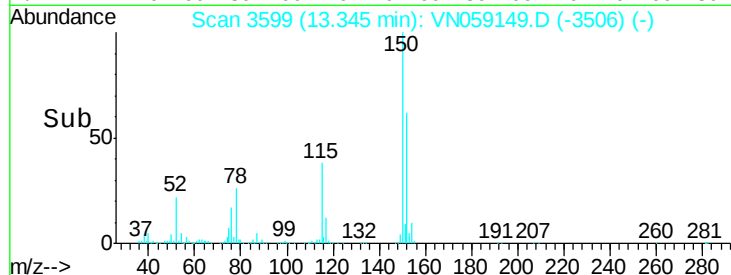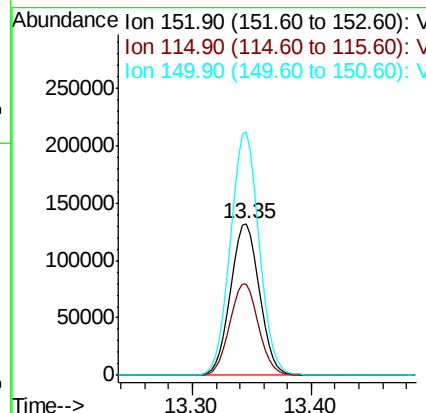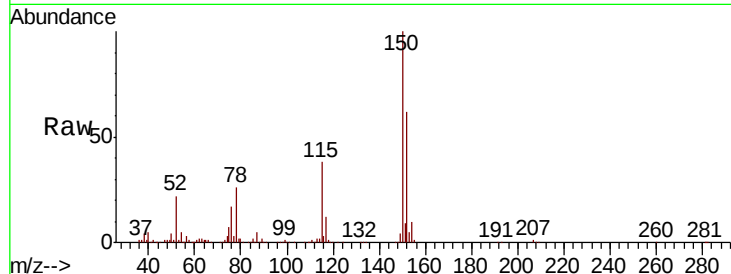


#76

1,2,3-Trichloropropane
Concen: 27.845 ug/l
RT: 12.40 min Scan# 3305
Delta R.T. -0.15 min
Lab File: VN059149.D
Acq: 11 Nov 2019 10:50

Tgt Ion	Ratio	Lower	Upper
75	100		
77	1.4	0.0	0.0#

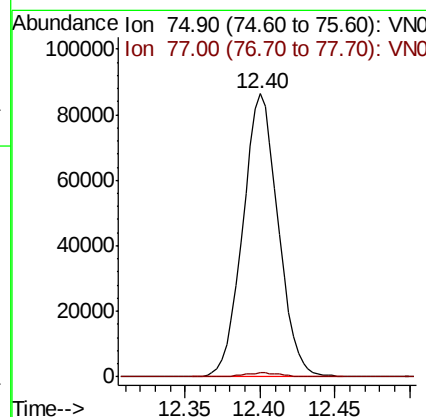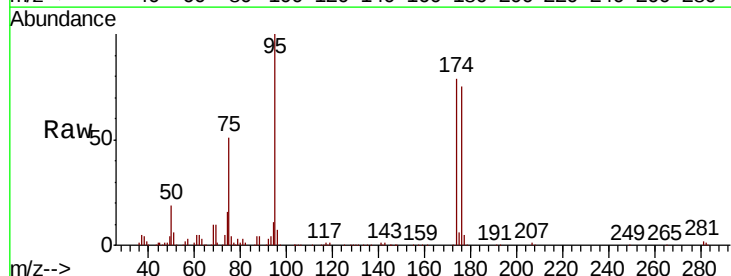

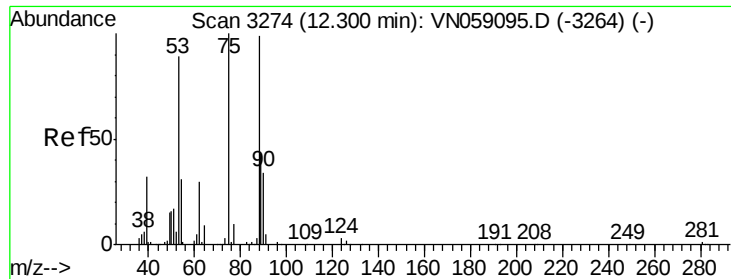

#81

trans-1,4-Dichloro-2-butene

Concen: 73.547 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. 0.10 min

Lab File: VN059149.D

Acq: 11 Nov 2019 10:50

Instrument :

MSVOA_N

ClientSampled :





Tot Ion: 75 Resp: 142082

Ion Ratio Lower Upper

75 100

53 0.0 72.2 108.2#

89 0.0 35.8 53.8#

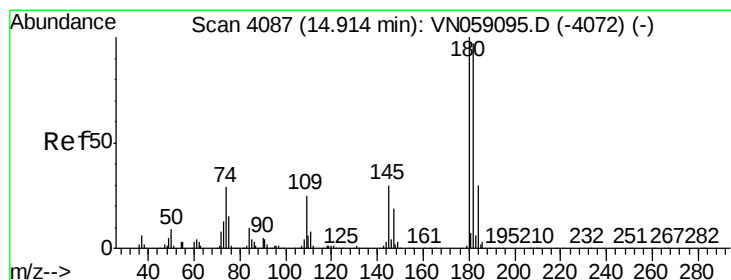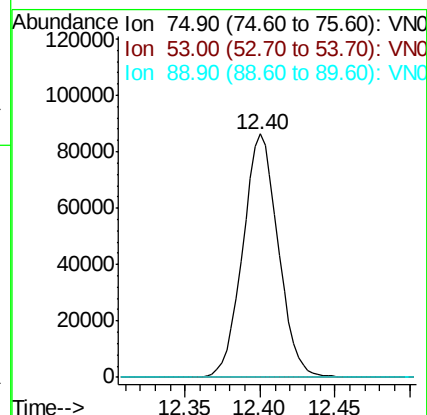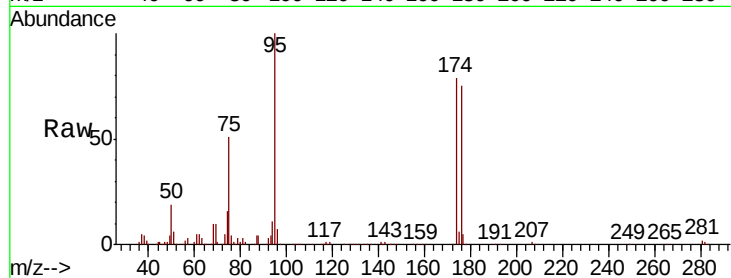

#93

1,2,4-Trichlorobenzene

Concen: 3.096 ug/l

RT: 14.91 min Scan# 4086

Delta R.T. -0.00 min

Lab File: VN059149.D

Acq: 11 Nov 2019 10:50




Tgt Ion: 180 Resp: 223


Ion Ratio Lower Upper

180 100

182 43.0 48.1 144.3#

145 73.1 15.1 45.3#

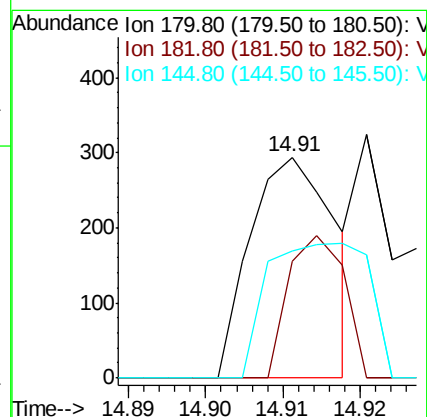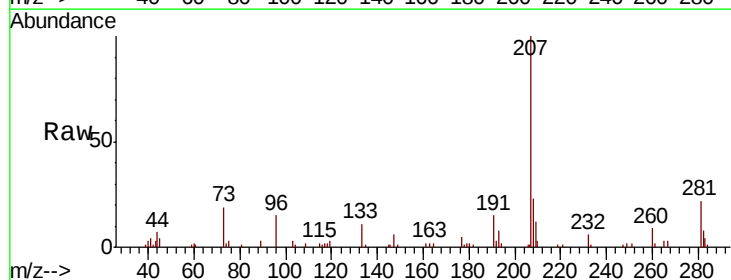



#95

Naphthalene

Concen: 3.114 ug/l

RT: 15.13 min Scan# 4155

Delta R.T. 0.00 min

Lab File: VN059149.D

Acq: 11 Nov 2019 10:50

Instrument :

MSVOA_N

ClientSampleId :



Tot Ion:128 Resp: 854

Ion Ratio Lower Upper

128 100

127 0.0 10.2 15.2#

129 0.0 8.6 12.8#

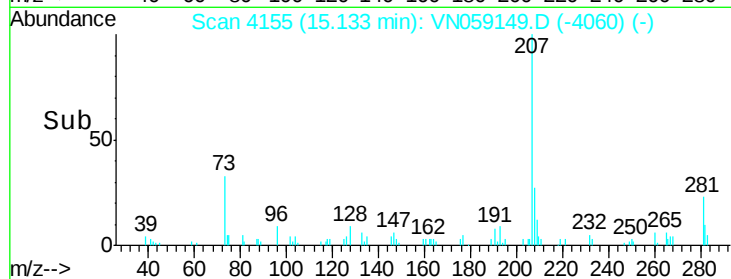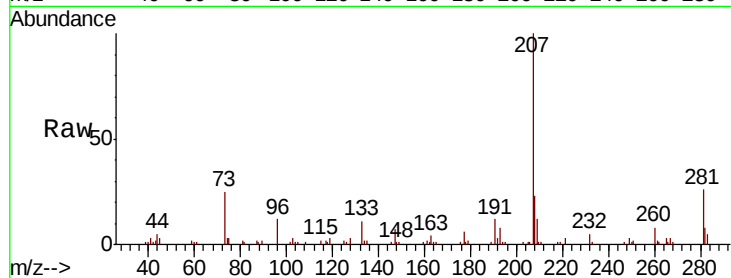

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

