

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN111120\
 Data File : VN064560.D
 Acq On : 11 Nov 2020 17:14
 Operator : JC/MD
 Sample : PB132934ZHE#04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132934ZHE#04

Quant Time: Nov 12 01:33:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 04 12:09:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	233329	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	505001	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	548512	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	186998	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	235449	57.93	ug/l	0.00
Spiked Amount			Recovery	=	115.86%	
35) Dibromofluoromethane	7.55	113	172671	50.22	ug/l	0.00
Spiked Amount			Recovery	=	100.44%	
50) Toluene-d8	10.06	98	662013	49.82	ug/l	0.00
Spiked Amount			Recovery	=	99.64%	
62) 4-Bromofluorobenzene	12.38	95	240287	47.81	ug/l	0.00
Spiked Amount			Recovery	=	95.62%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acrolein	3.48	56	184	0.662	ug/l #	10
16) Acetone	3.79	43	9986	6.450	ug/l	97
18) Methyl Acetate	4.29	43	1773	0.583	ug/l	94
20) Methylene Chloride	4.51	84	9079	2.956	ug/l #	82
25) 2-Butanone	6.80	43	1257	0.637	ug/l #	52
31) Cyclohexane	7.63	56	6727	1.362	ug/l #	29
36) 1,1-Dichloropropene	7.63	75	22333	4.186	ug/l #	52
37) Ethyl Acetate	6.89	43	108	0.782	ug/l #	71
38) Carbon Tetrachloride	7.62	117	27052	4.744	ug/l #	16
43) Isopropyl Acetate	8.13	43	46087	5.331	ug/l	99
45) 1,2-Dichloropropane	9.24	63	2372	0.567	ug/l #	45
48) Methyl methacrylate	9.15	41	9375	2.149	ug/l #	15
49) 1,4-Dioxane	9.24	88	259	4.507	ug/l #	1
51) 4-Methyl-2-Pentanone	9.95	43	7297	1.447	ug/l	99
54) cis-1,3-Dichloropropene	9.87	75	55065	8.205	ug/l #	72
56) Ethyl methacrylate	10.34	69	242	1.879	ug/l #	20
57) 1,3-Dichloropropane	10.74	76	33041	5.076	ug/l #	43
59) 2-Hexanone	10.74	43	523462	129.295	ug/l #	54
71) Bromoform	12.37	173	531	1.429	ug/l #	1
74) N-amyl acetate	12.00	43	1048	1.356	ug/l #	54
76) 1,2,3-Trichloropropane	12.38	75	136427	30.111	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.71	105	2684	0.219	ug/l	99
81) trans-1,4-Dichloro-2-buten	12.38	75	136427	84.073	ug/l #	8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN111120\
Data File : VN064560.D
Acq On : 11 Nov 2020 17:14
Operator : JC/MD
Sample : PB132934ZHE#04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB132934ZHE#04

Quant Time: Nov 12 01:33:22 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 04 12:09:03 2020
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.63 min Scan# 1831
Delta R.T. 0.00 min
Lab File: VN064560.D
Acq: 11 Nov 2020 17:14

Instrument :
MSVOA_N
ClientSampleId :
PB132934ZHE#04

Tot Ion:168 Resp: 233329
Ion Ratio Lower Upper
168 100
99 67.2 53.4 80.2




Abundance Ion 167.90 (167.60 to 168.60): V
Ion 98.90 (98.60 to 99.60): VN






#13
Acrolein
Concen: 0.662 ug/l
RT: 3.48 min Scan# 540
Delta R.T. -0.09 min
Lab File: VN064560.D
Acq: 11 Nov 2020 17:14

Tgt Ion: 56 Resp: 184
Ion Ratio Lower Upper
56 100
55 143.5 55.9 83.9#



Abundance Ion 56.00 (55.70 to 56.70): VN
Ion 55.00 (54.70 to 55.70): VN





#16

Acetone

Concen: 6.450 ug/l

RT: 3.79 min Scan# 637

Delta R.T. 0.01 min

Lab File: VN064560.D

Acq: 11 Nov 2020 17:14

Instrument :

MSVOA_N

ClientSampleId :





PB132934ZHE#04

Tot Ion: 43 Resp: 9986

Ion Ratio Lower Upper

43 100

58 28.3 21.4 32.0

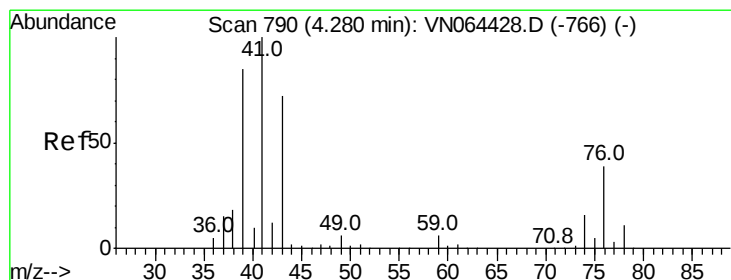

#18

Methyl Acetate

Concen: 0.583 ug/l

RT: 4.29 min Scan# 792

Delta R.T. 0.01 min

Lab File: VN064560.D




Acq: 11 Nov 2020 17:14


Tgt Ion: 43 Resp: 1773

Ion Ratio Lower Upper

43 100

74 23.9 17.0 25.4









#20
Methvlene Chloride
Concen: 2.956 ug/l
RT: 4.51 min Scan# 862
Delta R.T. 0.01 min
Lab File: VN064560.D
Acq: 11 Nov 2020 17:14

Instrument :
MSVOA_N
ClientSampleId :
PB132934ZHE#04

Tot Ion: 84 Resp: 9079
Ion Ratio Lower Upper
84 100
49 109.5 110.1 165.1#
51 42.8 33.6 50.4
86 52.4 52.1 78.1




Abundance Ion 83.90 (83.60 to 84.60): VN0
Ion 48.90 (48.60 to 49.60): VN0
Ion 50.90 (50.60 to 51.60): VN0
Ion 85.90 (85.60 to 86.60): VN0






#25
2-Butanone
Concen: 0.637 ug/l
RT: 6.80 min Scan# 1574
Delta R.T. 0.01 min
Lab File: VN064560.D
Acq: 11 Nov 2020 17:14

Tgt Ion: 43 Resp: 1257
Ion Ratio Lower Upper
43 100
72 0.0 18.5 27.7#



Abundance Ion 43.00 (42.70 to 43.70): VN0
Ion 72.00 (71.70 to 72.70): VN0









#31
Cyclohexane
Concen: 1.362 ug/l
RT: 7.63 min Scan# 1832
Delta R.T. 0.02 min
Lab File: VN064560.D
Acq: 11 Nov 2020 17:14

Instrument :
MSVOA_N
ClientSampleId :
PB132934ZHE#04

Tot Ion: 56 Resp: 6727
Ion Ratio Lower Upper
56 100
69 165.8 25.6 38.4#
84 80.3 63.0 94.6




Abundance Ion 56.00 (55.70 to 56.70): VNC
Ion 69.00 (68.70 to 69.70): VNC
Ion 84.00 (83.70 to 84.70): VNC






#33
1,2-Dichloroethane-d4
Concen: 57.932 ug/l
RT: 7.99 min Scan# 1944
Delta R.T. 0.00 min
Lab File: VN064560.D
Acq: 11 Nov 2020 17:14

Tgt Ion: 65 Resp: 235449
Ion Ratio Lower Upper
65 100
67 51.1 0.0 101.6



Abundance Ion 64.90 (64.60 to 65.60): VNC
Ion 66.90 (66.60 to 67.60): VNC









#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN064560.D
 Acq: 11 Nov 2020 17:14

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132934ZHE#04

Tot Ion:114 Resp: 505001
 Ion Ratio Lower Upper
 114 100
 63 23.0 0.0 45.6
 88 16.5 0.0 32.8




Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN






#35
 Dibromofluoromethane
 Concen: 50.219 ug/l
 RT: 7.55 min Scan# 1807
 Delta R.T. 0.00 min
 Lab File: VN064560.D
 Acq: 11 Nov 2020 17:14

Tgt Ion:113 Resp: 172671
 Ion Ratio Lower Upper
 113 100
 111 103.9 81.1 121.7
 192 15.6 12.8 19.2



Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V









#36
 1,1-Dichloropropene
 Concen: 4.186 ug/l
 RT: 7.63 min Scan# 1831
 Delta R.T. -0.13 min
 Lab File: VN064560.D
 Acq: 11 Nov 2020 17:14




Instrument :
 MSVOA_N
 ClientSampleId :
 PB132934ZHE#04


Tot Ion: 75 Resp: 22333
 Ion Ratio Lower Upper
 75 100
 110 9.3 16.0 48.0#
 77 0.0 24.0 36.0#



#37
 Ethyl Acetate
 Concen: 0.782 ug/l
 RT: 6.89 min Scan# 1601
 Delta R.T. 0.00 min
 Lab File: VN064560.D
 Acq: 11 Nov 2020 17:14

Tgt Ion: 43 Resp: 108
 Ion Ratio Lower Upper
 43 100
 61 0.0 10.0 15.0#
 70 0.0 7.1 10.7#





#38

Carbon Tetrachloride

Concen: 4.744 ug/l

RT: 7.62 min Scan# 1830

Delta R.T. -0.11 min

Lab File: VN064560.D

Acq: 11 Nov 2020 17:14

Instrument :

MSVOA_N

ClientSampleId :

PB132934ZHE#04


Tot Ion:117 Resp: 27052

Ion Ratio Lower Upper

117 100

119 4.4 75.5 113.3#




121 0.0 24.4 36.6#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V



#43

Isopropyl Acetate

Concen: 5.331 ug/l

RT: 8.13 min Scan# 1988

Delta R.T. 0.01 min

Lab File: VN064560.D

Acq: 11 Nov 2020 17:14


Tgt Ion: 43 Resp: 46087

Ion Ratio Lower Upper

43 100

61 17.1 14.0 21.0



87 12.0 9.1 13.7




Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0





#45

1,2-Dichloropropane

Concen: 0.567 ug/l

RT: 9.24 min Scan# 2332

Delta R.T. 0.15 min

Lab File: VN064560.D

Acq: 11 Nov 2020 17:14

Instrument :

MSVOA_N

ClientSampleId :


PB132934ZHE#04

Tot Ion: 63 Resp: 2372

Ion Ratio Lower Upper




63 100

65 0.0 23.6 35.4#



Abundance Ion 62.90 (62.60 to 63.60): VNC

Ion 64.90 (64.60 to 65.60): VNC



#48

Methyl methacrylate

Concen: 2.149 ug/l

RT: 9.15 min Scan# 2304

Delta R.T. -0.02 min

Lab File: VN064560.D

Acq: 11 Nov 2020 17:14


Tgt Ion: 41 Resp: 9375

Ion Ratio Lower Upper

41 100

69 0.0 60.4 90.6#



39 0.0 51.2 76.8#




Abundance Ion 41.00 (40.70 to 41.70): VNC

Ion 69.00 (68.70 to 69.70): VNC

Ion 39.00 (38.70 to 39.70): VNC





#49

1,4-Dioxane

Concen: 4.507 ug/l

RT: 9.24 min Scan# 2332

Delta R.T. 0.07 min

Lab File: VN064560.D

Acq: 11 Nov 2020 17:14

Instrument :

MSVOA_N

ClientSampleId :

PB132934ZHE#04


Tot Ion: 88 Resp: 259

Ion Ratio Lower Upper

88 100

43 828980.3 31.0 46.6#




58 4322.0 58.4 87.6#



Abundance Ion 88.00 (87.70 to 88.70): VN0

Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0



#50

Toluene-d8

Concen: 49.816 ug/l

RT: 10.06 min Scan# 2588

Delta R.T. 0.00 min

Lab File: VN064560.D


Acq: 11 Nov 2020 17:14

Tgt Ion: 98 Resp: 662013

Ion Ratio Lower Upper



98 100


100 63.7 50.7 76.1



Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN0





#51

4-Methyl-2-Pentanone

Concen: 1.447 ug/l

RT: 9.95 min Scan# 2554

Delta R.T. -0.00 min

Lab File: VN064560.D

Acq: 11 Nov 2020 17:14

Instrument :

MSVOA_N

ClientSampleId :


PB132934ZHE#04

Tot Ion: 43 Resp: 7297

Ion Ratio Lower Upper




43 100

58 34.7 28.4 42.6



Abundance Ion 43.00 (42.70 to 43.70): VN064428.D (-2535) (-)

Ion 58.00 (57.70 to 58.70): VN064428.D (-2535) (-)



#54

cis-1,3-Dichloropropene

Concen: 8.205 ug/l

RT: 9.87 min Scan# 2530

Delta R.T. 0.07 min

Lab File: VN064560.D

Acq: 11 Nov 2020 17:14


Tgt Ion: 75 Resp: 55065

Ion Ratio Lower Upper

75 100

77 0.8 24.9 37.3#



39 48.8 47.1 70.7




Abundance Ion 74.90 (74.60 to 75.60): VN064428.D (-2493) (-)

Ion 76.90 (76.60 to 77.60): VN064428.D (-2493) (-)

Ion 39.00 (38.70 to 39.70): VN064428.D (-2493) (-)





#56

Ethyl methacrylate

Concen: 1.879 ug/l

RT: 10.34 min Scan# 2675

Delta R.T. -0.06 min

Lab File: VN064560.D

Acq: 11 Nov 2020 17:14

Instrument :

MSVOA_N

ClientSampleId :

PB132934ZHE#04





Tot Ion: 69 Resp: 242

Ion Ratio Lower Upper

69 100

41 0.0 59.3 88.9#

39 0.0 35.4 53.0#



#57

1,3-Dichloropropane

Concen: 5.076 ug/l

RT: 10.74 min Scan# 2798

Delta R.T. 0.06 min

Lab File: VN064560.D




Acq: 11 Nov 2020 17:14


Tgt Ion: 76 Resp: 33041

Ion Ratio Lower Upper

76 100

78 0.1 25.8 38.6#









#59
2-Hexanone
Concen: 129.295 ug/l
RT: 10.74 min Scan# 2798
Delta R.T. 0.02 min
Lab File: VN064560.D
Acq: 11 Nov 2020 17:14




Instrument :
MSVOA_N
ClientSampleId :
PB132934ZHE#04


Tot Ion: 43 Resp: 523462
Ion Ratio Lower Upper
43 100
58 17.7 24.7 74.1#



#62
4-Bromofluorobenzene
Concen: 47.810 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. 0.00 min
Lab File: VN064560.D
Acq: 11 Nov 2020 17:14

Tgt Ion: 95 Resp: 240287
Ion Ratio Lower Upper
95 100
174 71.9 0.0 132.6
176 67.3 0.0 129.2









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. -0.00 min
Lab File: VN064560.D
Acq: 11 Nov 2020 17:14

Instrument :
MSVOA_N
ClientSampleId :
PB132934ZHE#04

Tot Ion:117 Resp: 548512
Ion Ratio Lower Upper
117 100
82 57.4 48.1 72.1
119 31.5 26.2 39.4




Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V






#71
Bromoform
Concen: 1.429 ug/l
RT: 12.37 min Scan# 3307
Delta R.T. 0.27 min
Lab File: VN064560.D
Acq: 11 Nov 2020 17:14

Tgt Ion:173 Resp: 531
Ion Ratio Lower Upper
173 100
175 2019.2 23.7 71.1#
254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V





#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3601

Delta R.T. 0.00 min

Lab File: VN064560.D

Acq: 11 Nov 2020 17:14

Instrument :

MSVOA_N

ClientSampleId :

PB132934ZHE#04


Tot Ion:152 Resp: 186998

Ion Ratio Lower Upper

152 100

115 66.2 32.0 96.0




150 157.8 0.0 353.8



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V



#74

N-ethyl acetate

Concen: 1.356 ug/l

RT: 12.00 min Scan# 3192

Delta R.T. -0.04 min

Lab File: VN064560.D

Acq: 11 Nov 2020 17:14

Tgt Ion: 43 Resp: 1048


Ion Ratio Lower Upper

43 100

70 0.0 29.6 44.4#

55 13.9 18.4 27.6#

61 0.0 17.8 26.6#






Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 70.00 (69.70 to 70.70): VNO

Ion 55.00 (54.70 to 55.70): VNO

Ion 61.00 (60.70 to 61.70): VNO





#76

1,2,3-Trichloropropane

Concen: 30.111 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.15 min

Lab File: VN064560.D

Acq: 11 Nov 2020 17:14

Instrument :

MSVOA_N

ClientSampleId :


PB132934ZHE#04

Tot Ion: 75 Resp: 136427

Ion Ratio Lower Upper




75 100

77 0.6 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0



#80

1,3,5-Trimethylbenzene

Concen: 0.219 ug/l

RT: 12.71 min Scan# 3411

Delta R.T. -0.00 min

Lab File: VN064560.D


Acq: 11 Nov 2020 17:14

Tgt Ion: 105 Resp: 2684

Ion Ratio Lower Upper



105 100


120 47.7 23.4 70.2



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V





#81

trans-1,4-Dichloro-2-butene

Concen: 84.073 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.10 min

Lab File: VN064560.D

Acq: 11 Nov 2020 17:14

Instrument :

MSVOA_N

ClientSampleId :

PB132934ZHE#04

Tot Ion: 75 Resp: 136427

Ion Ratio Lower Upper

75 100

53 0.1 84.0 126.0#

89 0.0 36.3 54.5#

