

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111121\
 Data File : VN069451.D
 Acq On : 11 Nov 2021 11:04
 Operator : JC/MD
 Sample : VN1111MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 12 05:15:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 09 18:18:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	1260115	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2226117	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	2131654	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	767715	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	925192	50.637	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 101.280%			
35) Dibromofluoromethane	8.024	113	654588	49.028	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 98.060%			
50) Toluene-d8	10.443	98	2795909	53.245	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 106.480%			
62) 4-Bromofluorobenzene	12.733	95	941573	48.810	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 97.620%			
Target Compounds						Qvalue
13) Acrolein	4.047	56	1019	Below Cal	#	49
16) Acetone	4.296	43	6467	0.656	ug/l #	86
20) Methylene Chloride	5.095	84	2876	0.206	ug/l #	89
31) Cyclohexane	8.086	56	32663	1.309	ug/l #	31
36) 1,1-Dichloropropene	8.086	75	110286	5.888	ug/l #	48
38) Carbon Tetrachloride	8.086	117	132194	7.310	ug/l #	16
49) 1,4-Dioxane	9.566	88	619	40.627	ug/l	95
51) 4-Methyl-2-Pentanone	10.333	43	12465	0.475	ug/l	90
53) t-1,3-Dichloropropene	10.722	75	526	2.658	ug/l #	43
54) cis-1,3-Dichloropropene	10.186	75	277	1.744	ug/l #	67
56) Ethyl methacrylate	10.770	69	1200	2.095	ug/l #	4
58) 2-Chloroethyl Vinyl ether	10.038	63	89	22.782	ug/l #	45
59) 2-Hexanone	11.092	43	24608	9.017	ug/l	88
60) Dibromochloromethane	11.245	129	113	2.424	ug/l #	11
61) 1,2-Dibromoethane	11.339	107	142	1.080	ug/l	88
70) Styrene	12.296	104	3378	1.588	ug/l #	90
71) Bromoform	12.457	173	224	3.445	ug/l #	29
74) N-amyl acetate	12.398	43	12552	0.485	ug/l #	86
76) 1,2,3-Trichloropropane	12.731	75	538707	30.406	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.731	75	538707	85.820	ug/l #	5
87) 1,3-Dichlorobenzene	13.621	146	5080	0.210	ug/l	71
88) 1,4-Dichlorobenzene	13.621	146	5080	0.214	ug/l	70
89) n-Butylbenzene	13.943	91	13415	0.335	ug/l #	85
90) Hexachloroethane	14.211	117	62	2.169	ug/l #	6
91) 1,2-Dichlorobenzene	13.994	146	6206	0.269	ug/l	93
92) 1,2-Dibromo-3-Chloropr...	14.605	75	706	1.974	ug/l #	59
93) 1,2,4-Trichlorobenzene	15.265	180	11429	4.000	ug/l	97
95) Naphthalene	15.509	128	48861	5.757	ug/l #	93
96) 1,2,3-Trichlorobenzene	15.700	180	13719	4.281	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111121\
Data File : VN069451.D
Acq On : 11 Nov 2021 11:04
Operator : JC/MD
Sample : VN1111MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Nov 12 05:15:15 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 09 18:18:22 2021
Response via : Initial Calibration




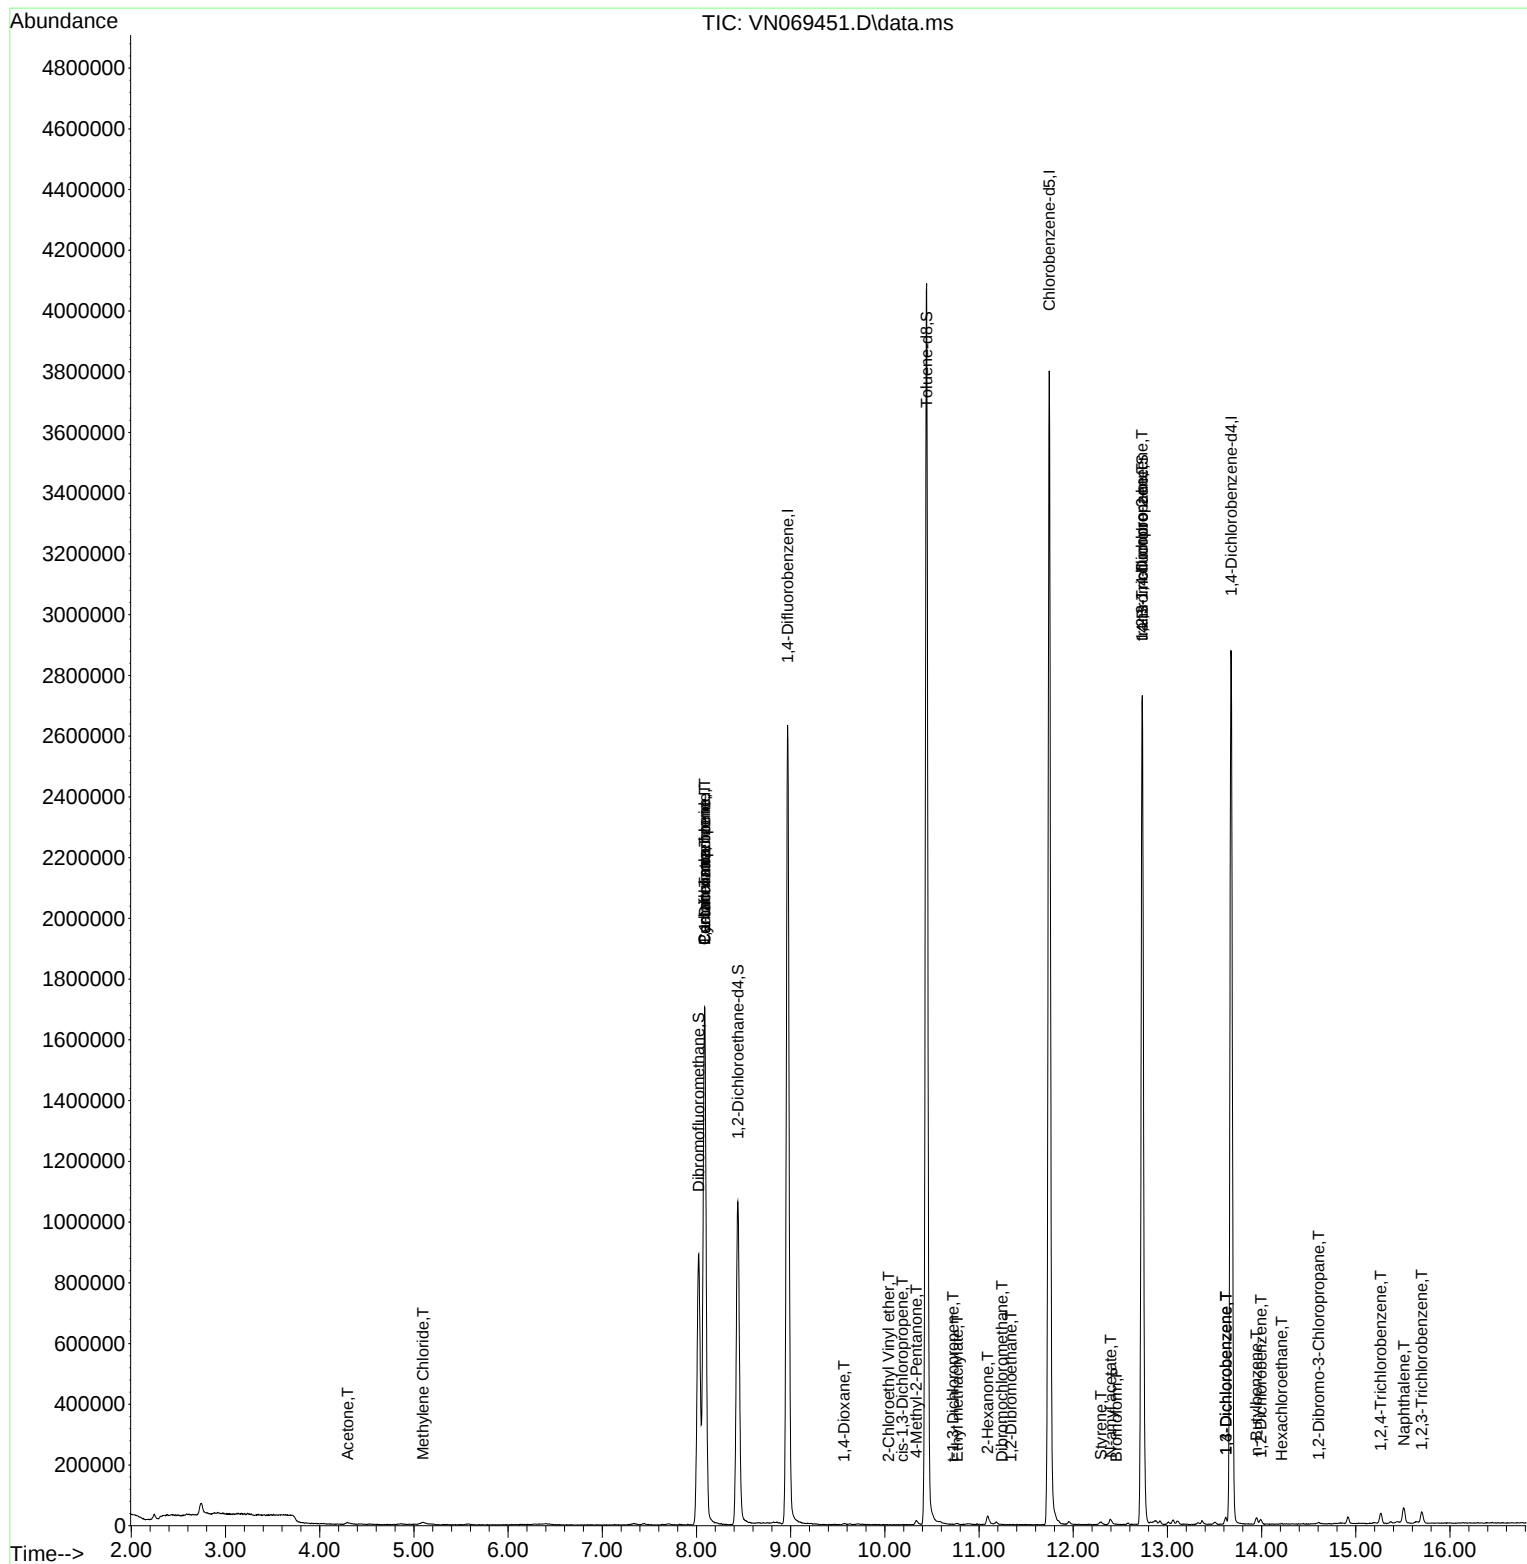


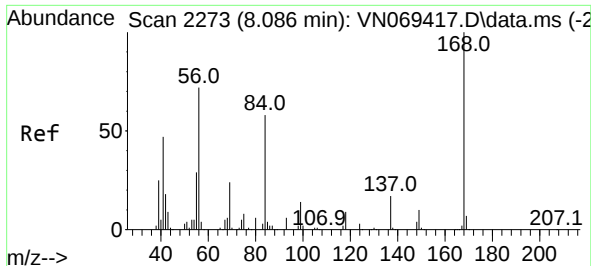

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 1260115
Ion Ratio Lower Upper
168 100
99 61.0 41.3 61.9

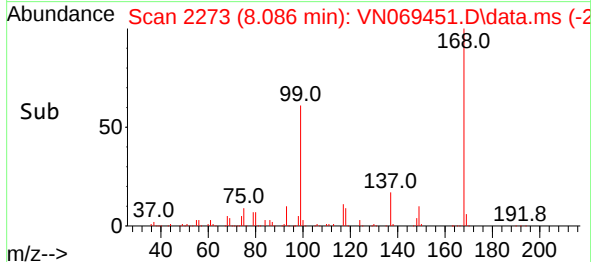

#13
Acrolein
Concen: Below Cal
RT: 4.047 min Scan# 767
Delta R.T. 0.006 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04

Tgt Ion: 56 Resp: 1019
Ion Ratio Lower Upper
56 100
55 28.6 56.6 85.0#


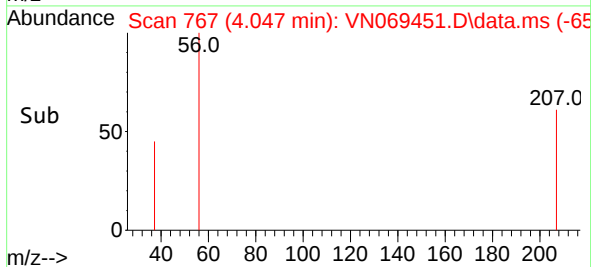

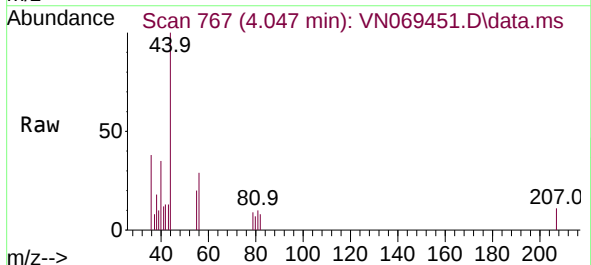




#16
Acetone
Concen: 0.656 ug/l
RT: 4.296 min Scan# 80
Delta R.T. 0.008 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 6467
Ion Ratio Lower Upper
43 100
58 21.4 23.1 34.7#

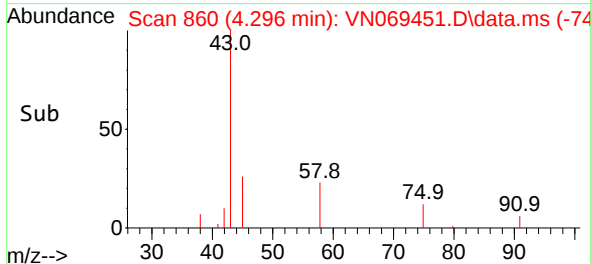

#20
Methylene Chloride
Concen: 0.206 ug/l
RT: 5.095 min Scan# 1158
Delta R.T. 0.002 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04


Tgt Ion: 84 Resp: 2876
Ion Ratio Lower Upper
84 100
49 108.0 93.5 140.3
51 38.3 29.4 44.2
86 48.6 53.0 79.4#

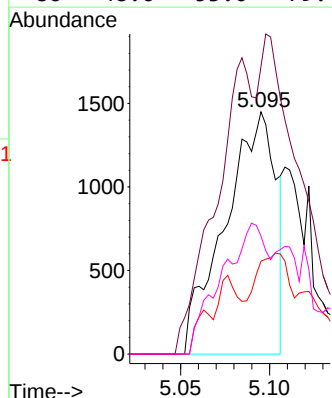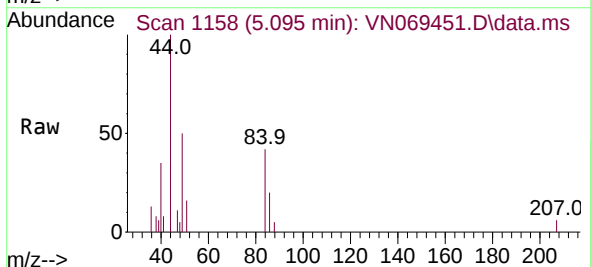



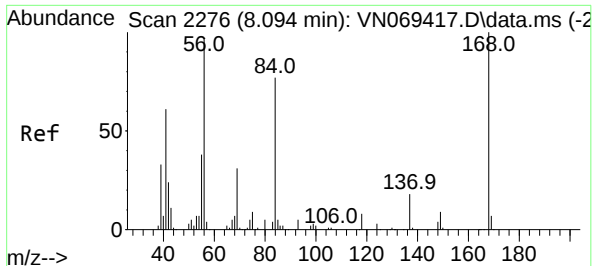


#31
Cyclohexane
Concen: 1.309 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.008 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04

Instrument :
MSVOA_N
ClientSampleId :



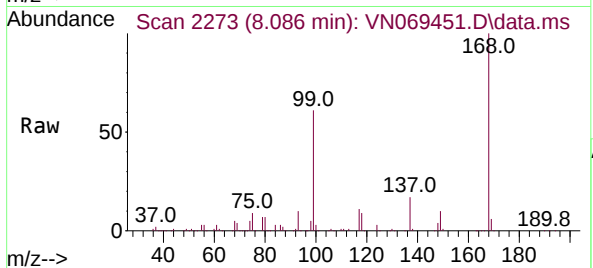



Tgt Ion: 56 Resp: 32663
Ion Ratio Lower Upper
56 100
69 145.2 27.1 40.7#
84 113.3 73.4 110.0#

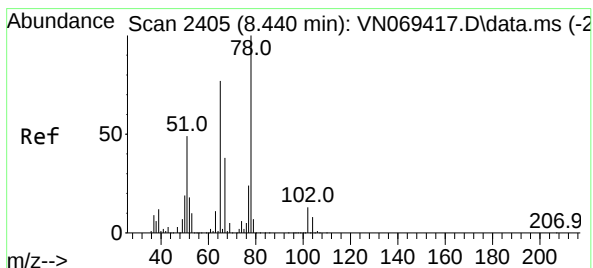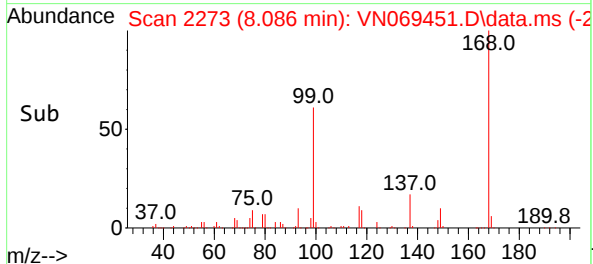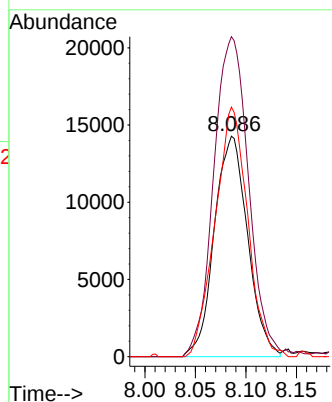

#33
1,2-Dichloroethane-d4
Concen: 50.637 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04


Tgt Ion: 65 Resp: 925192
Ion Ratio Lower Upper
65 100
67 50.8 0.0 103.0

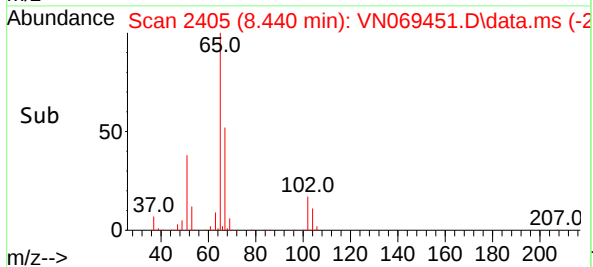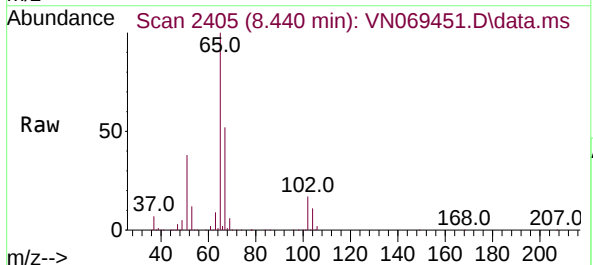



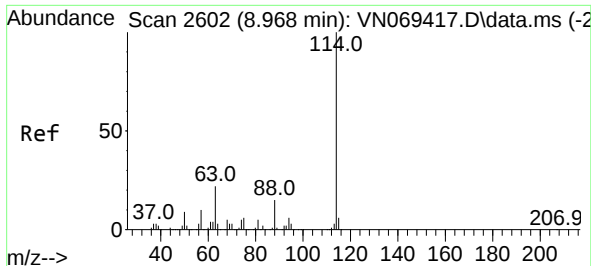


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:114 Resp: 2226117
Ion Ratio Lower Upper
114 100
63 22.9 0.0 37.8
88 15.6 0.0 27.4

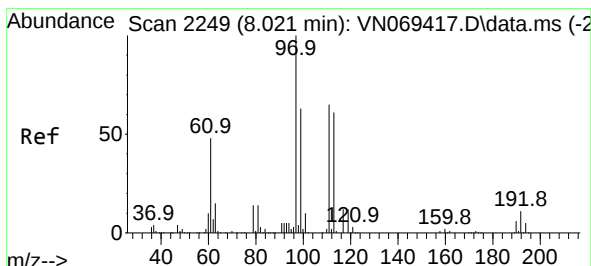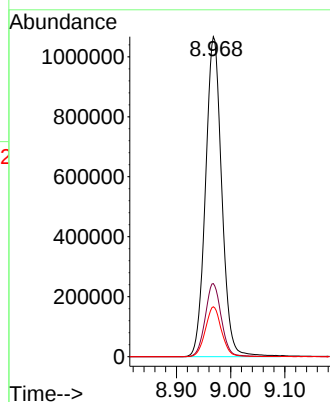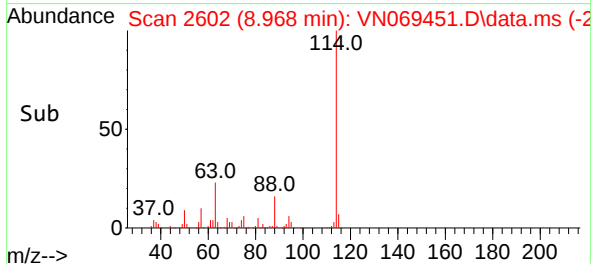

#35
Dibromofluoromethane
Concen: 49.028 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04


Tgt Ion:113 Resp: 654588
Ion Ratio Lower Upper
113 100
111 102.3 82.2 123.2
192 17.8 16.9 25.3

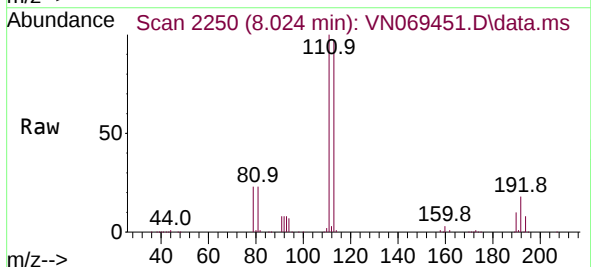



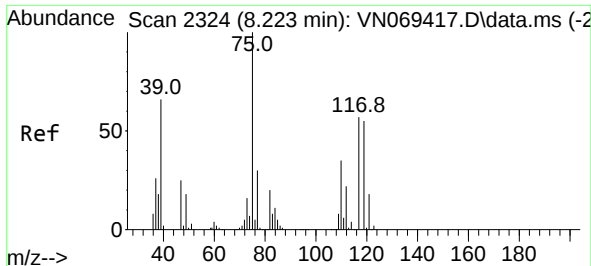


#36
 1,1-Dichloropropene
 Concen: 5.888 ug/l
 RT: 8.086 min Scan# 2273
 Delta R.T. -0.137 min
 Lab File: VN069451.D
 Acq: 11 Nov 2021 11:04


Instrument :
 MSVOA_N
 ClientSampleId :





Tgt Ion: 75 Resp: 110286
 Ion Ratio Lower Upper
 75 100
 110 8.3 18.4 55.2#
 77 0.0 24.4 36.6#

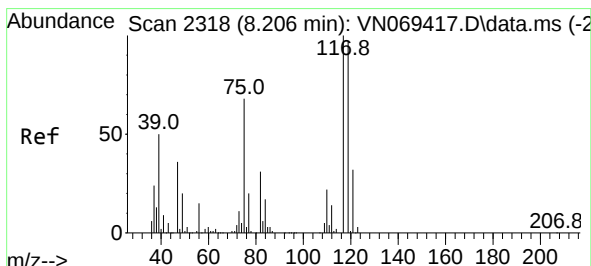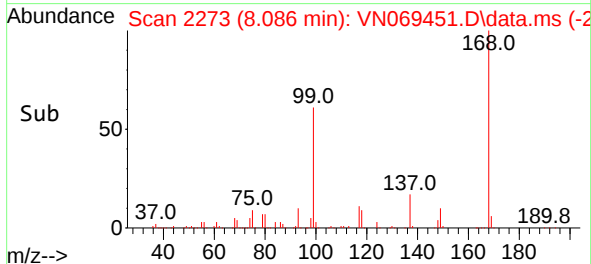


#38
 Carbon Tetrachloride
 Concen: 7.310 ug/l
 RT: 8.086 min Scan# 2273
 Delta R.T. -0.120 min
 Lab File: VN069451.D
 Acq: 11 Nov 2021 11:04

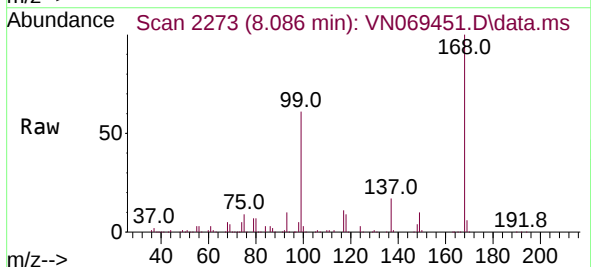

Tgt Ion: 117 Resp: 132194
 Ion Ratio Lower Upper
 117 100
 119 4.7 76.1 114.1#
 121 0.0 24.2 36.2#

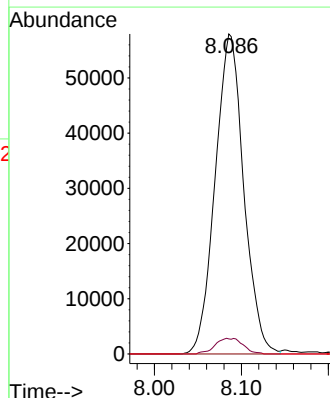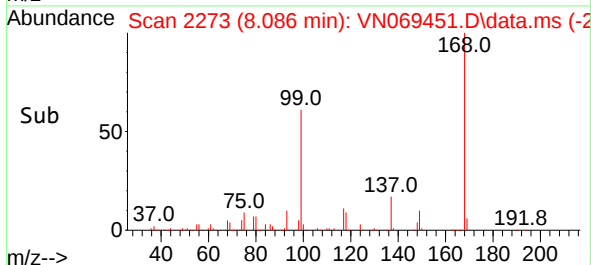

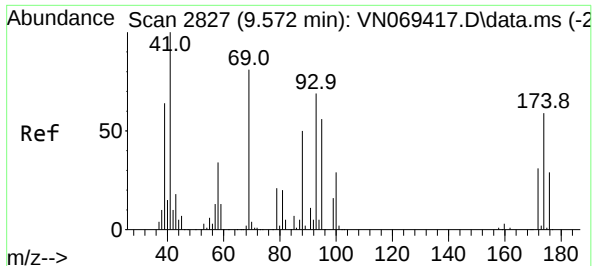

#49

1,4-Dioxane

Concen: 40.627 ug/l

RT: 9.566 min Scan# 21

Delta R.T. -0.006 min

Lab File: VN069451.D

Acq: 11 Nov 2021 11:04

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 88 Resp: 619

Ion Ratio Lower Upper

88 100

43 28.9 23.4 35.2

58 68.5 50.6 75.8

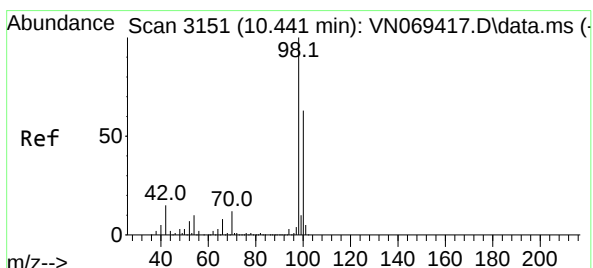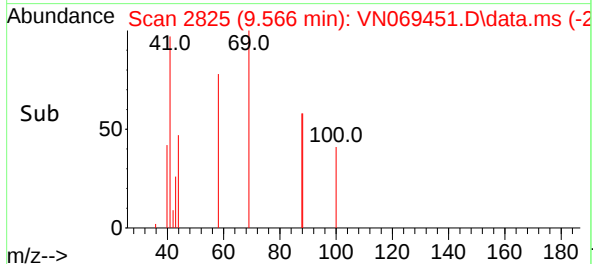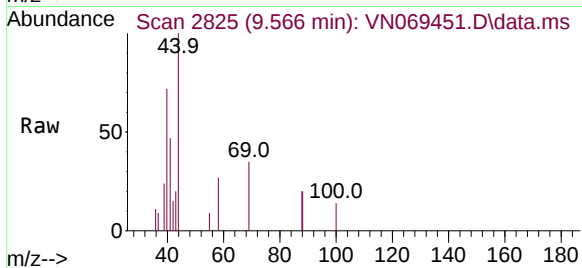

#50

Toluene-d8

Concen: 53.245 ug/l

RT: 10.443 min Scan# 3152

Delta R.T. 0.002 min

Lab File: VN069451.D




Acq: 11 Nov 2021 11:04


Tgt Ion: 98 Resp: 2795909

Ion Ratio Lower Upper

98 100


100 63.9 50.4 75.6

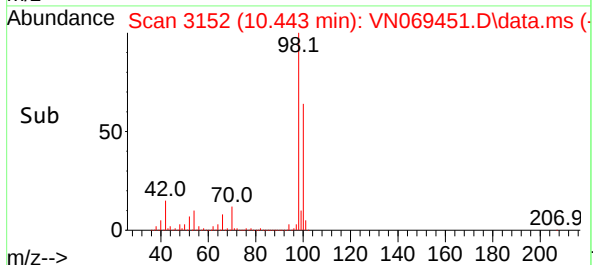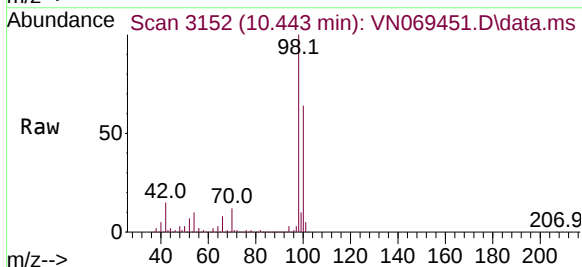






#51
4-Methyl-2-Pentanone
Concen: 0.475 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. 0.002 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 12465
Ion Ratio Lower Upper
43 100
58 32.2 30.4 45.6

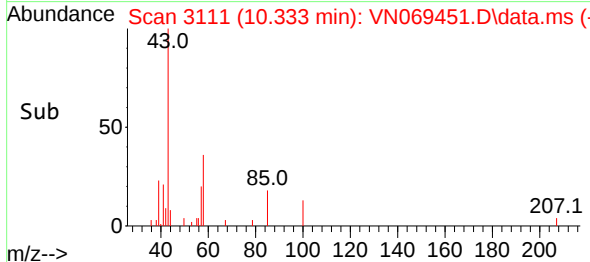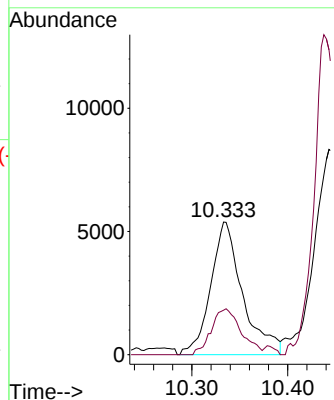

#53
t-1,3-Dichloropropene
Concen: 2.658 ug/l
RT: 10.722 min Scan# 3256
Delta R.T. 0.003 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04


Tgt Ion: 75 Resp: 526
Ion Ratio Lower Upper
75 100
77 0.0 25.6 38.4#

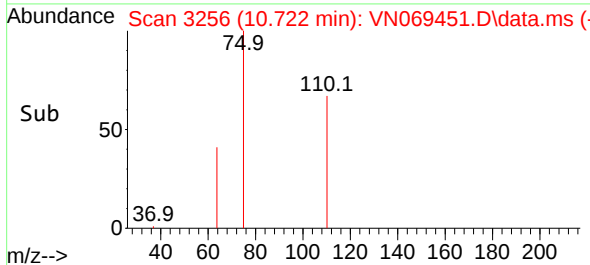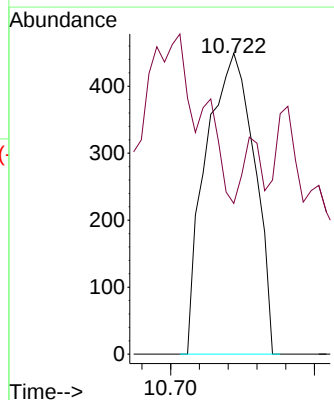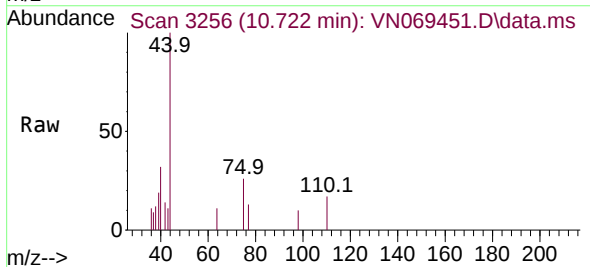



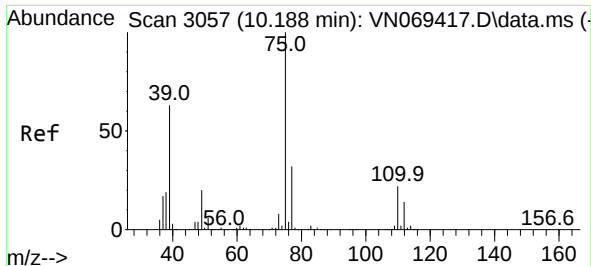


#54
 cis-1,3-Dichloropropene
 Concen: 1.744 ug/l
 RT: 10.186 min Scan# 3057
 Delta R.T. -0.002 min
 Lab File: VN069451.D
 Acq: 11 Nov 2021 11:04

Instrument :
 MSVOA_N
 ClientSampleId :







Tgt Ion: 75 Resp: 277
 Ion Ratio Lower Upper
 75 100
 77 0.0 26.4 39.6#
 39 64.9 42.5 63.7#

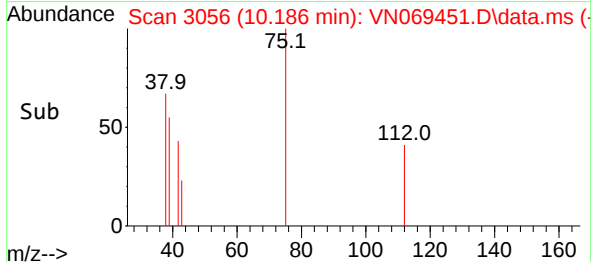

#56
 Ethyl methacrylate
 Concen: 2.095 ug/l
 RT: 10.770 min Scan# 3274
 Delta R.T. 0.008 min
 Lab File: VN069451.D
 Acq: 11 Nov 2021 11:04

Tgt Ion: 69 Resp: 1200
 Ion Ratio Lower Upper
 69 100
 41 139.0 51.4 77.0#
 39 105.3 34.6 52.0#


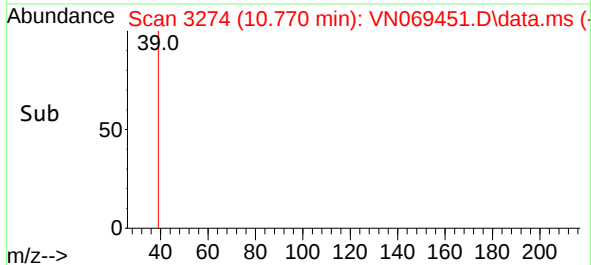

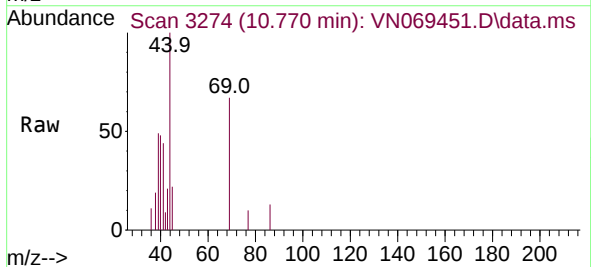


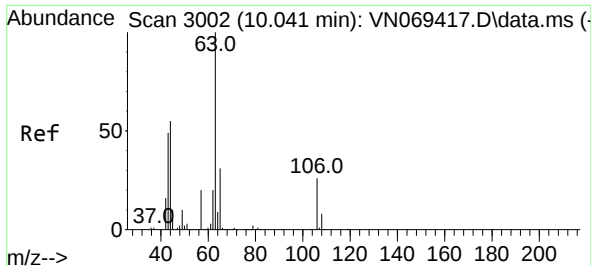

#58
2-Chloroethyl Vinyl ether
Concen: 22.782 ug/l
RT: 10.038 min Scan# 3002
Delta R.T. -0.003 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 63 Resp: 89
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#

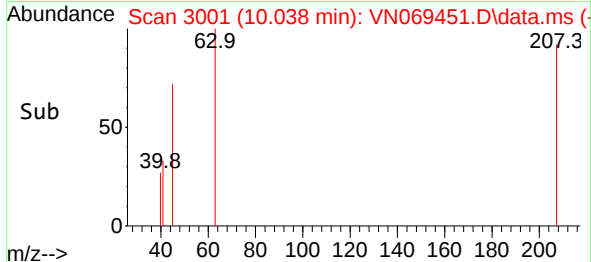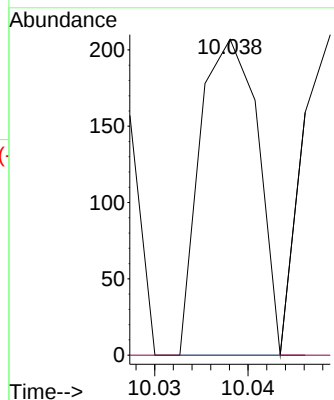

#59
2-Hexanone
Concen: 9.017 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.005 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04


Tgt Ion: 43 Resp: 24608
Ion Ratio Lower Upper
43 100
58 45.1 26.9 80.7

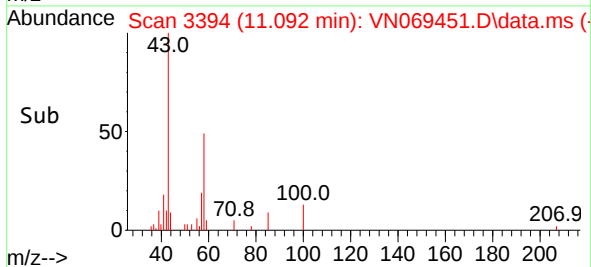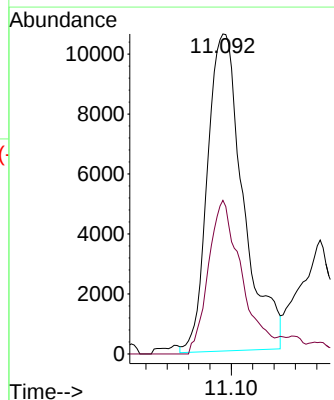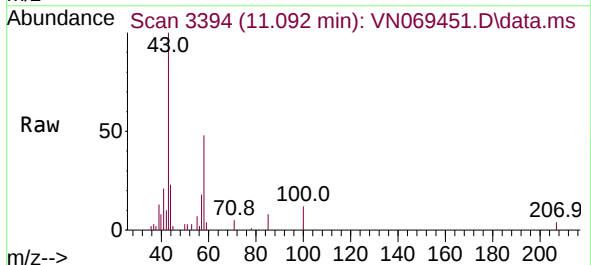



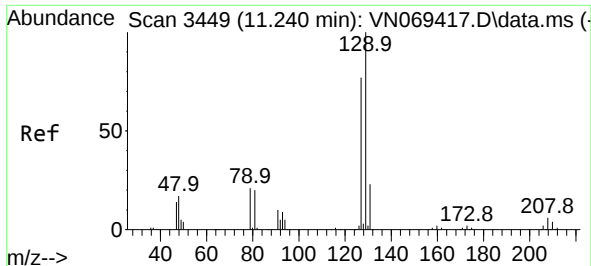


#60
Dibromochloromethane
Concen: 2.424 ug/l
RT: 11.245 min Scan# 3449
Delta R.T. 0.005 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:129 Resp: 113
Ion Ratio Lower Upper
129 100
127 0.0 38.6 116.0#

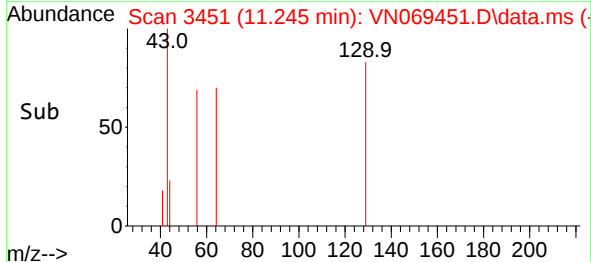

#61
1,2-Dibromoethane
Concen: 1.080 ug/l
RT: 11.339 min Scan# 3486
Delta R.T. -0.008 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04

Tgt Ion:107 Resp: 142
Ion Ratio Lower Upper
107 100
109 83.1 75.7 113.5


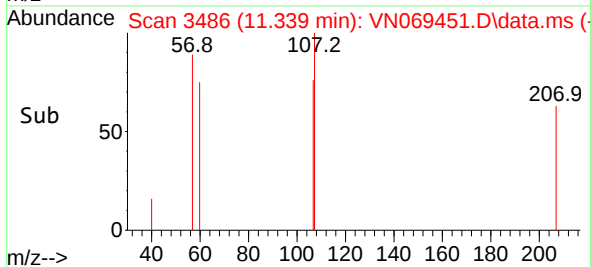

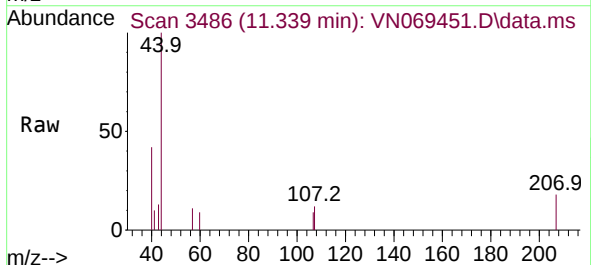




#62
4-Bromofluorobenzene
Concen: 48.810 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.001 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 941573
Ion Ratio Lower Upper
95 100
174 75.7 0.0 187.2
176 73.6 0.0 181.4

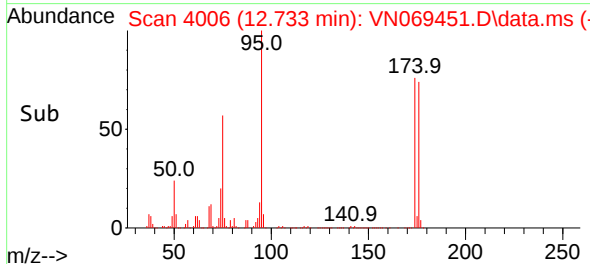

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. -0.001 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04


Tgt Ion: 117 Resp: 2131654
Ion Ratio Lower Upper
117 100
82 57.6 42.4 63.6
119 32.0 25.4 38.2

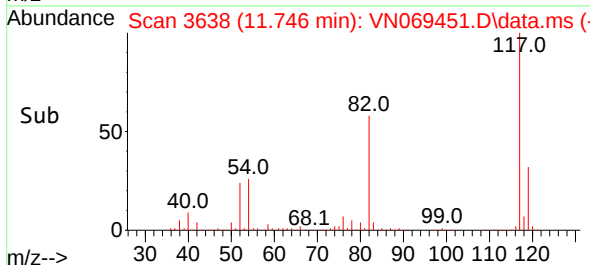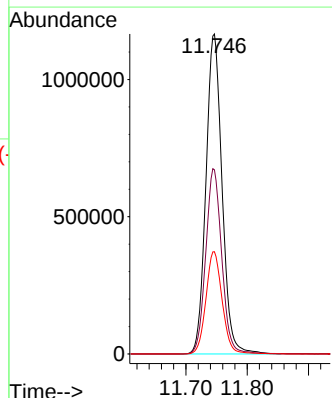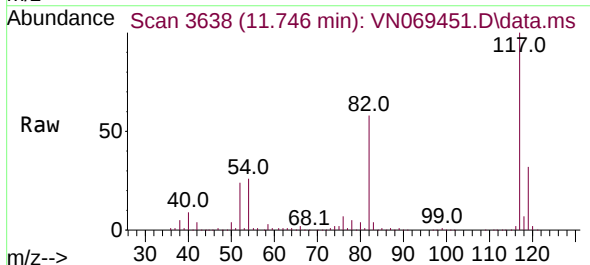






#70
Styrene
Concen: 1.588 ug/l
RT: 12.296 min Scan# 3842
Delta R.T. 0.002 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:104 Resp: 3378
Ion Ratio Lower Upper
104 100
78 59.5 38.7 58.1#
103 53.5 45.0 67.6

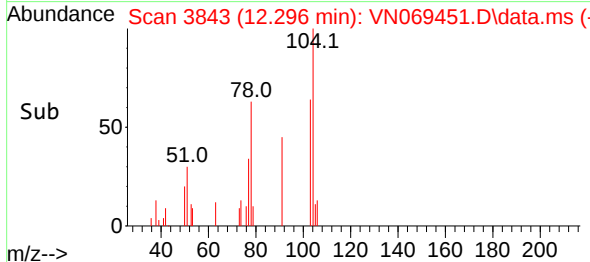

#71
Bromoform
Concen: 3.445 ug/l
RT: 12.457 min Scan# 3903
Delta R.T. -0.003 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04


Tgt Ion:173 Resp: 224
Ion Ratio Lower Upper
173 100
175 0.0 24.2 72.6#
254 0.0 0.0 0.0

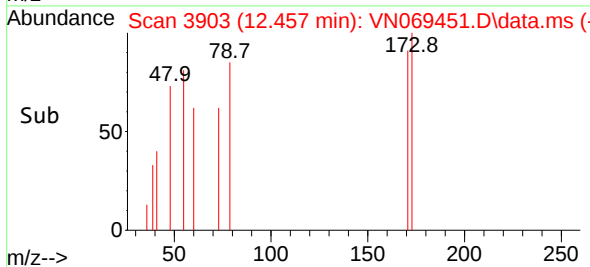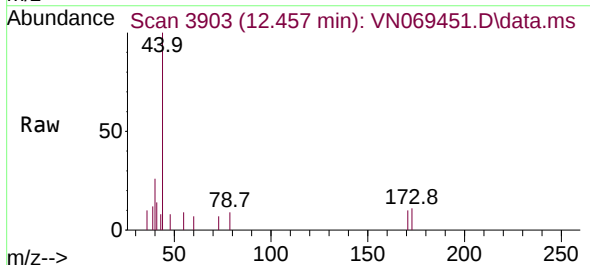






#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.678 min Scan# 41
 Delta R.T. 0.002 min
 Lab File: VN069451.D
 Acq: 11 Nov 2021 11:04


Instrument :
 MSVOA_N
 ClientSampleId :





Tgt Ion:152 Resp: 767715
 Ion Ratio Lower Upper
 152 100
 115 60.3 27.5 82.5
 150 157.3 0.0 344.4

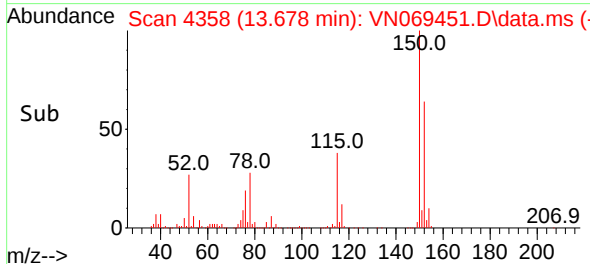


#74
 N-ethyl acetate
 Concen: 0.485 ug/l
 RT: 12.398 min Scan# 3881
 Delta R.T. 0.010 min
 Lab File: VN069451.D
 Acq: 11 Nov 2021 11:04

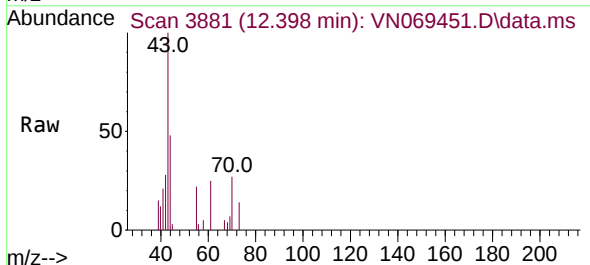

Tgt Ion: 43 Resp: 12552
 Ion Ratio Lower Upper
 43 100
 70 23.8 33.4 50.0#
 55 22.7 19.3 28.9
 61 22.5 18.5 27.7



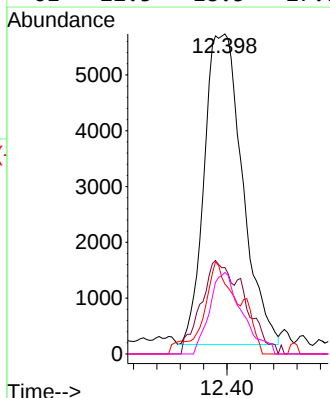
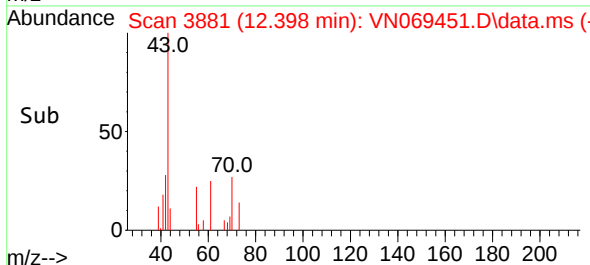




#76
1,2,3-Trichloropropane
Concen: 30.406 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.150 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 538707
Ion Ratio Lower Upper
75 100
77 1.1 82.6 247.8#

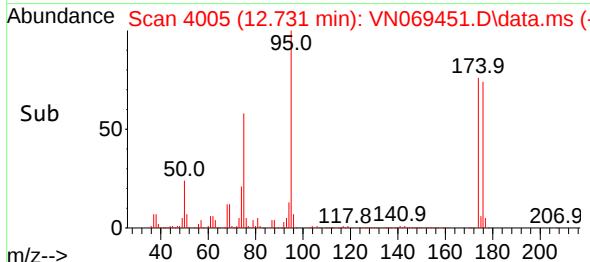

#81
trans-1,4-Dichloro-2-butene
Concen: 85.820 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.105 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04


Tgt Ion: 75 Resp: 538707
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#

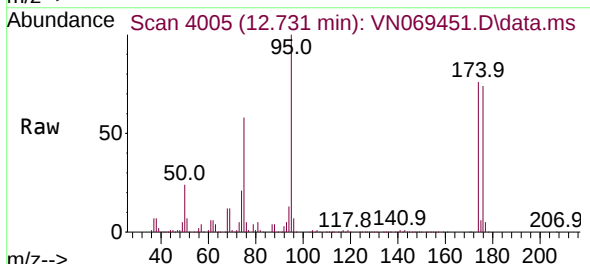






#87
1,3-Dichlorobenzene
Concen: 0.210 ug/l
RT: 13.621 min Scan# 4337
Delta R.T. 0.005 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:146 Resp: 5080
Ion Ratio Lower Upper
146 100
111 45.8 18.6 55.6
148 34.2 31.6 95.0

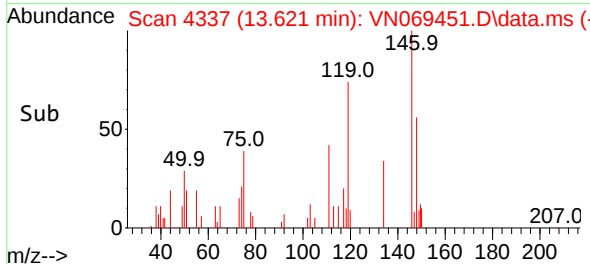

#88
1,4-Dichlorobenzene
Concen: 0.214 ug/l
RT: 13.621 min Scan# 4337
Delta R.T. -0.075 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04

Tgt Ion:146 Resp: 5080
Ion Ratio Lower Upper
146 100
111 45.8 18.3 54.8
148 34.2 31.8 95.4


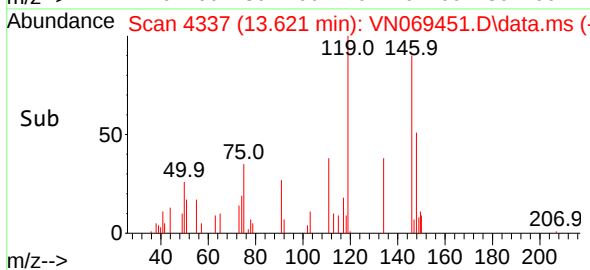

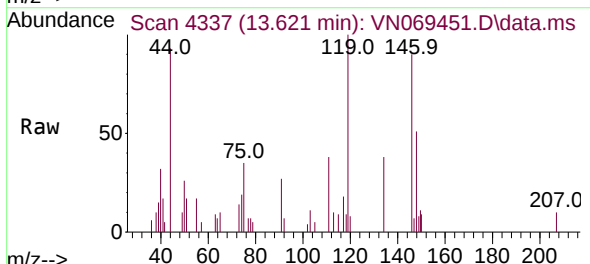




#89
n-Butylbenzene
Concen: 0.335 ug/l
RT: 13.943 min Scan# 4457
Delta R.T. 0.000 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion	Ratio	Lower	Upper
91	100		
92	47.1	25.4	76.0
134	10.2	13.6	40.8

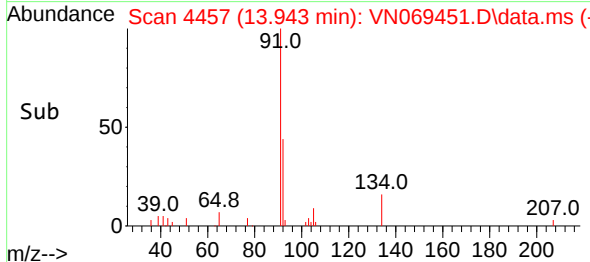

#90
Hexachloroethane
Concen: 2.169 ug/l
RT: 14.211 min Scan# 4557
Delta R.T. 0.000 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04


Tgt Ion	Ratio	Lower	Upper
117	100		
201	0.0	43.9	131.6

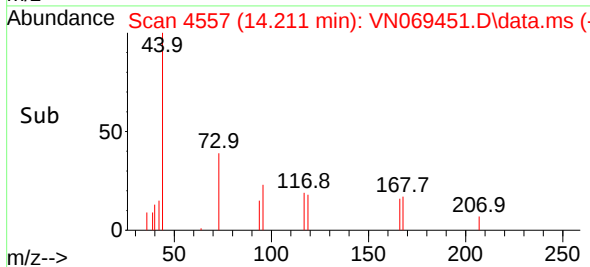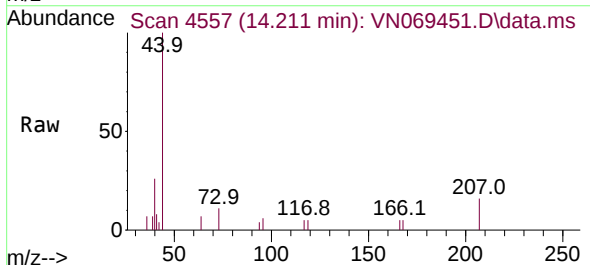






#91
1,2-Dichlorobenzene
Concen: 0.269 ug/l
RT: 13.994 min Scan# 4474
Delta R.T. 0.005 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:146 Resp: 6206
Ion Ratio Lower Upper
146 100
111 27.5 19.1 57.3
148 63.3 32.1 96.3

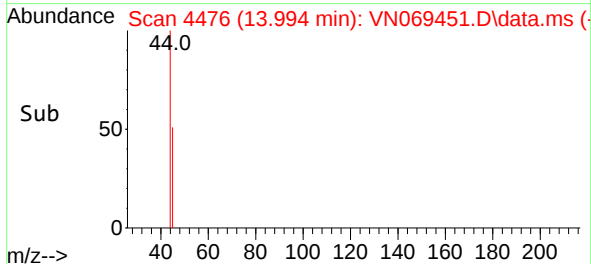


#92
1,2-Dibromo-3-Chloropropane
Concen: 1.974 ug/l
RT: 14.605 min Scan# 4704
Delta R.T. -0.001 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04

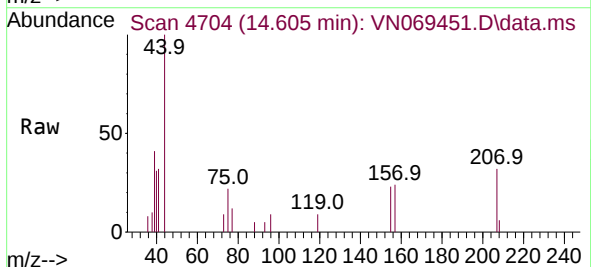

Tgt Ion: 75 Resp: 706
Ion Ratio Lower Upper
75 100
155 151.7 46.9 140.7#
157 151.0 60.6 181.7



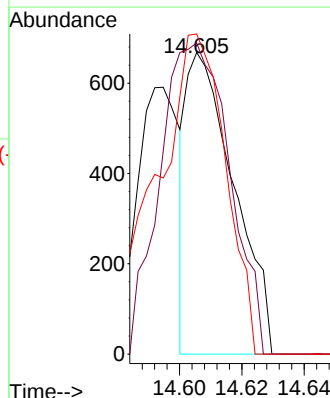





#93
1,2,4-Trichlorobenzene
Concen: 4.000 ug/l
RT: 15.265 min Scan# 4950
Delta R.T. 0.000 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:180 Resp: 11429
Ion Ratio Lower Upper
180 100
182 93.8 48.3 144.9
145 30.7 14.5 43.5

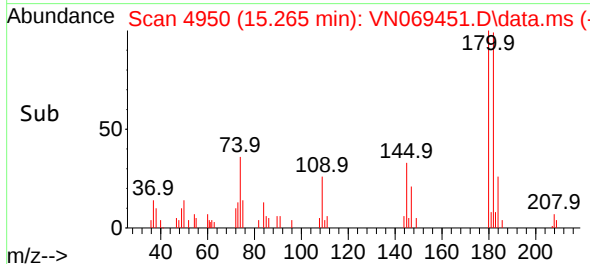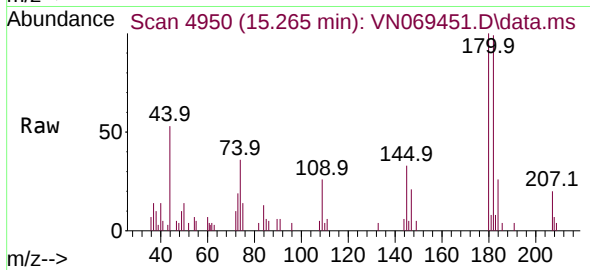

#95
Naphthalene
Concen: 5.757 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.002 min
Lab File: VN069451.D
Acq: 11 Nov 2021 11:04


Tgt Ion:128 Resp: 48861
Ion Ratio Lower Upper
128 100
127 7.9 10.5 15.7#
129 10.9 8.7 13.1

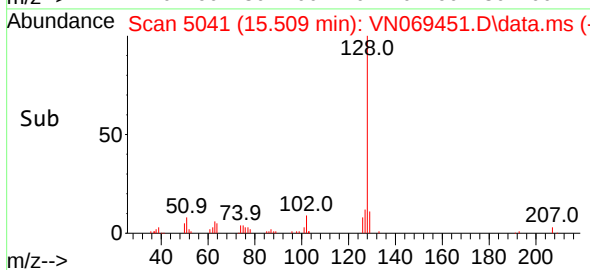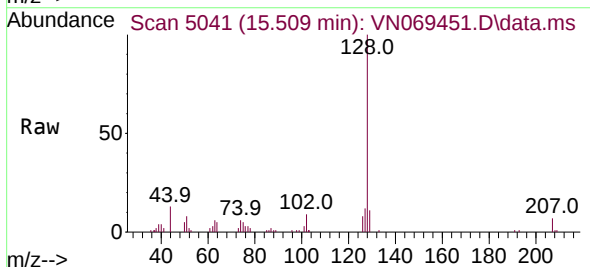



#96
 1,2,3-Trichlorobenzene
 Concen: 4.281 ug/l
 RT: 15.700 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: VN069451.D
 Acq: 11 Nov 2021 11:04

Instrument :
 MSVOA_N
 ClientSampleId :

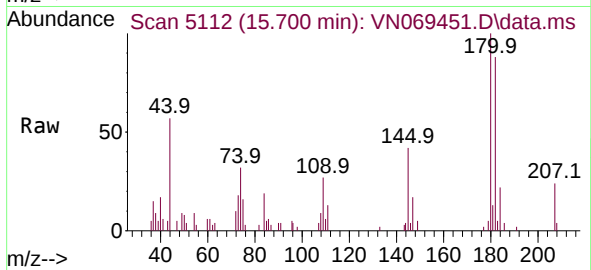

Tgt Ion:180	Resp:	13719
Ion	Ratio	Lower Upper
180	100	
182	86.8	47.4 142.2
145	35.0	15.0 45.1

