
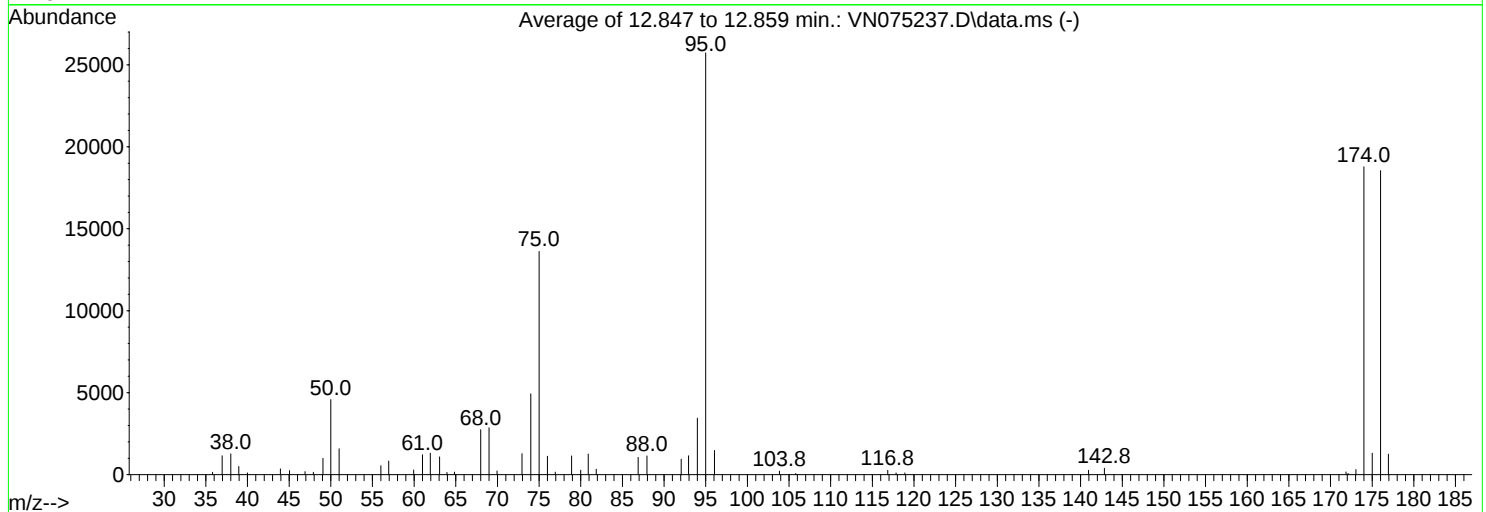


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111122\
Data File : VN075237.D
Acq On : 11 Nov 2022 09:31
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Title : SW846 8260
Last Update : Thu Oct 27 09:48:49 2022

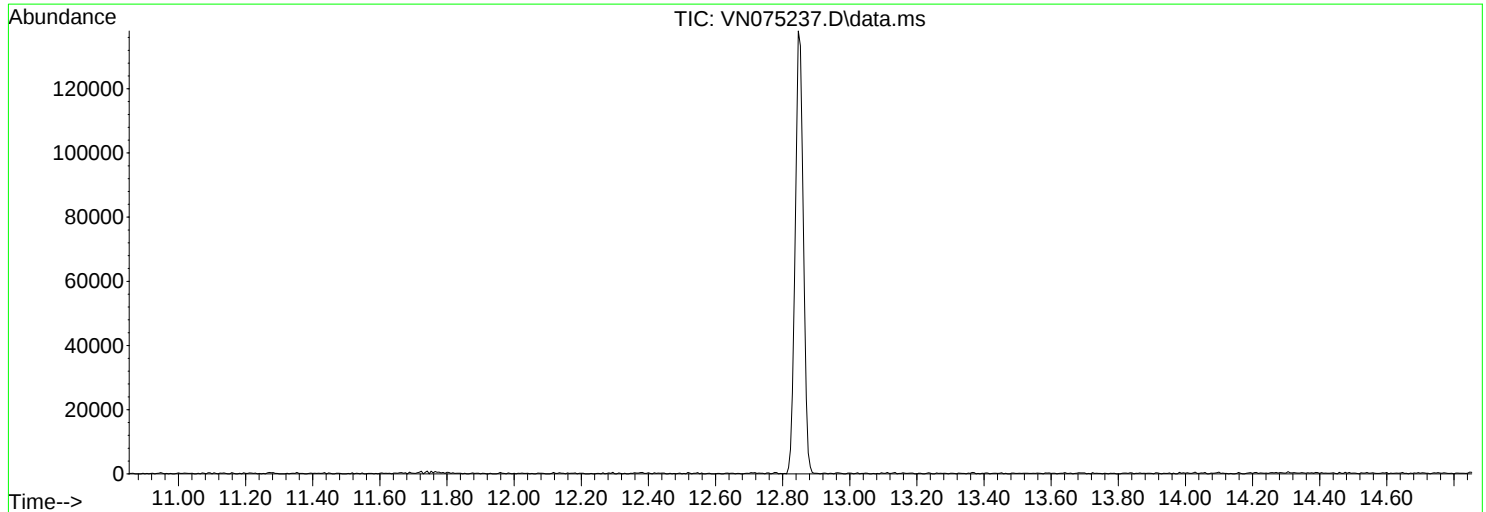

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	4583	PASS
75	95	30	60	52.9	13618	PASS
95	95	100	100	100.0	25733	PASS
96	95	5	9	5.7	1474	PASS
173	174	0.00	2	1.6	308	PASS
174	95	50	100	73.0	18778	PASS
175	174	5	9	7.0	1311	PASS
176	174	95	101	98.8	18550	PASS
177	176	5	9	6.8	1254	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	143	51.00	1577	69.95	229	87.95	1144
36.95	1154	56.00	549	72.95	1280	92.05	941
38.00	1273	56.95	829	74.00	4927	92.95	1150
38.95	494	59.95	285	75.00	13618	94.00	3450
40.00	110	61.00	1210	76.00	1124	95.00	25733
43.95	354	61.95	1305	76.95	157	96.05	1474
45.05	241	63.05	1081	78.90	1144	103.85	212
46.90	187	63.95	140	80.00	272	105.80	65
47.90	143	64.85	153	80.90	1256	116.85	267
49.05	995	68.00	2741	81.85	329	117.85	110
50.00	4583	69.00	2864	86.90	1055	118.90	109

Average of 12.847 to 12.859 min.: VN075237.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
140.95	260						
142.85	386						
171.85	164						
172.10	82						
173.05	308						
174.00	18778						
175.00	1311						
176.00	18550						
176.95	1254						

Instrument :

MSVOA_N

ClientSampleId :

BFB