

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111125\
 Data File : VN088244.D
 Acq On : 11 Nov 2025 10:26
 Operator : JC\MD
 Sample : VN1111MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1111MBL01

Quant Time: Nov 12 01:10:22 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 03 01:16:06 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.206	168	202654	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.082	114	454207	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.841	117	437617	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	213641	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.559	65	213865	61.029	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	122.060%
35) Dibromofluoromethane	8.147	113	164080	53.772	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	107.540%
50) Toluene-d8	10.541	98	602047	51.205	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.420%
62) 4-Bromofluorobenzene	12.829	95	222397	53.560	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	107.120%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111125\
Data File : VN088244.D
Acq On : 11 Nov 2025 10:26
Operator : JC\MD
Sample : VN1111MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1111MBL01

Quant Time: Nov 12 01:10:22 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Quant Title : SW846 8260
QLast Update : Mon Nov 03 01:16:06 2025
Response via : Initial Calibration




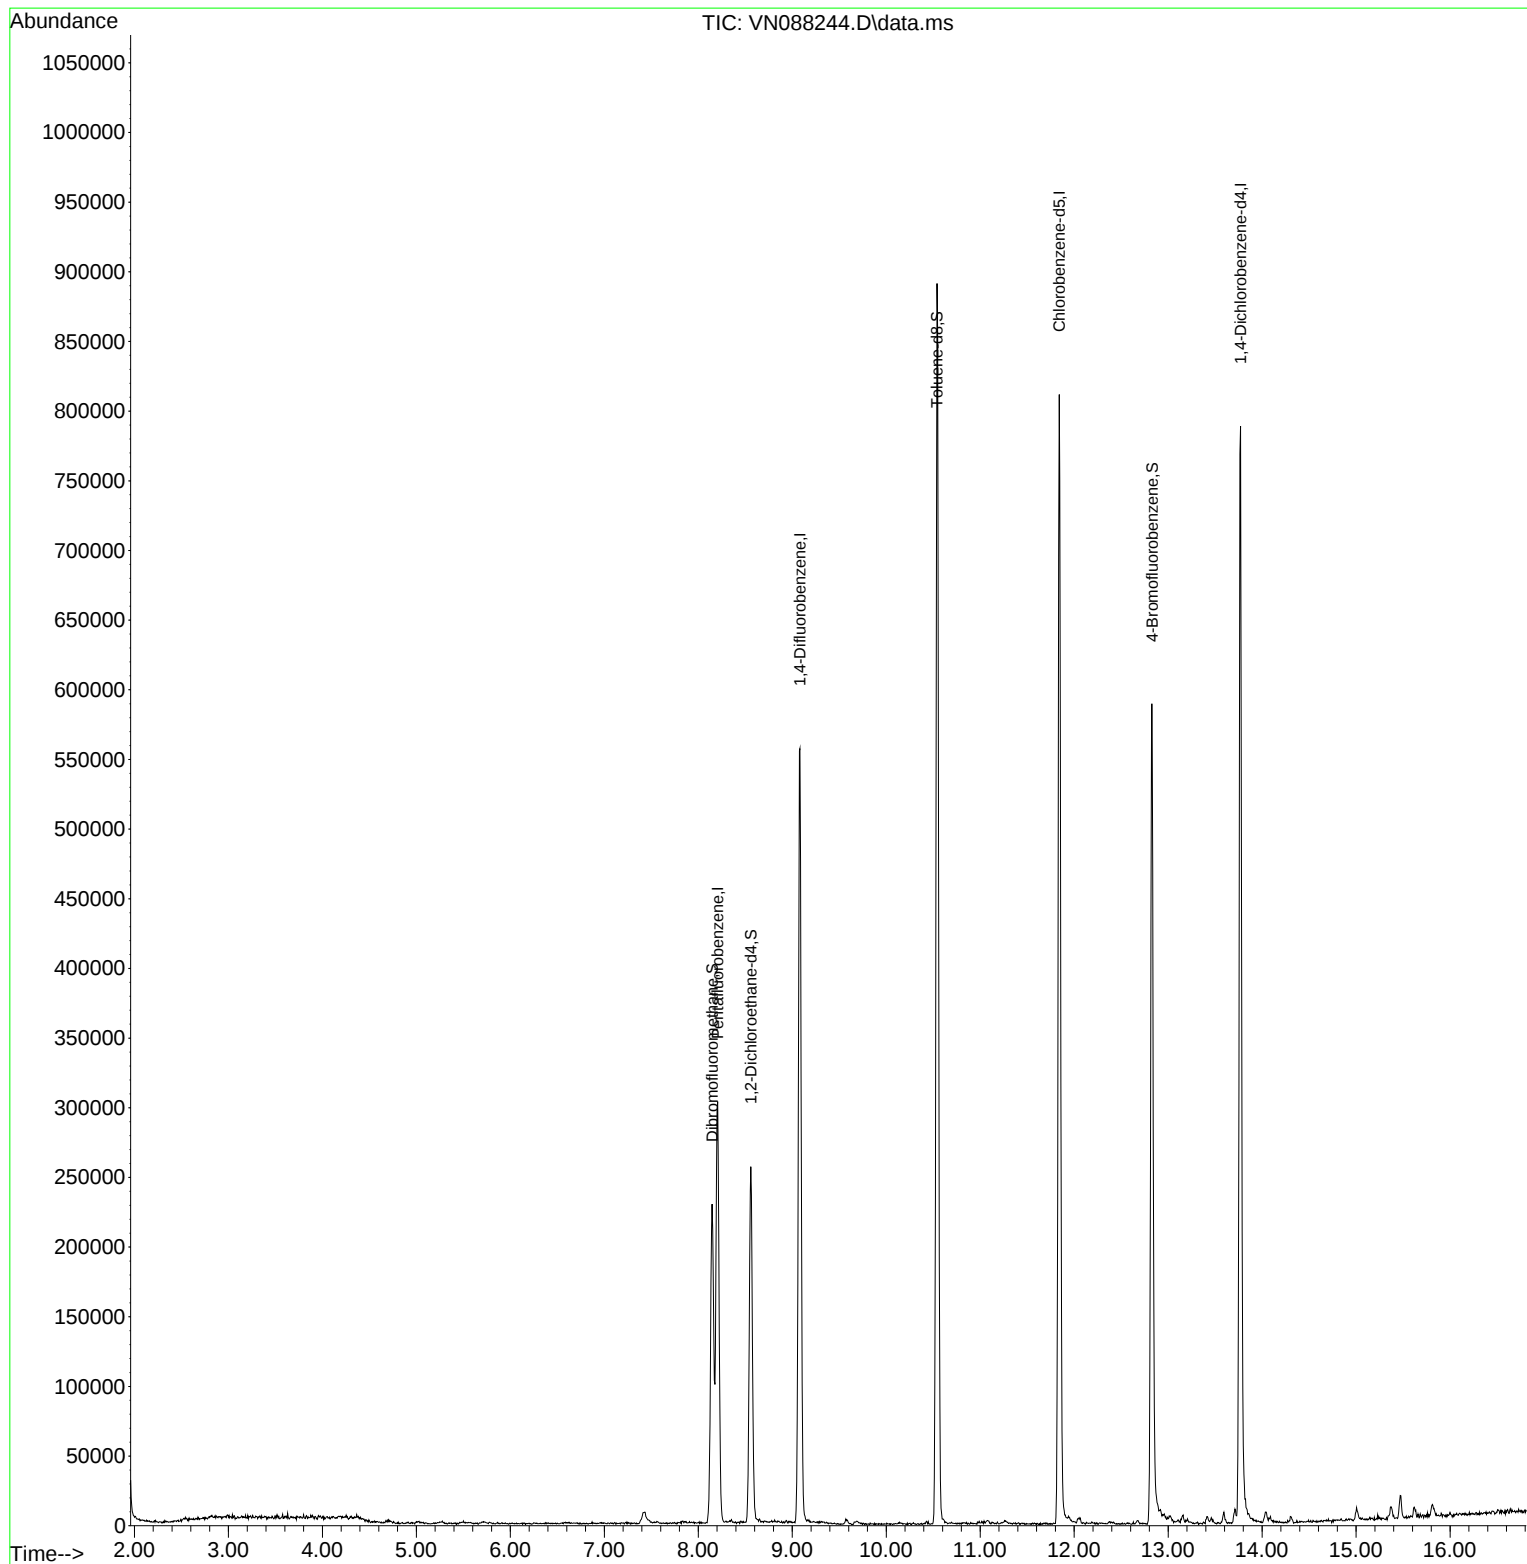


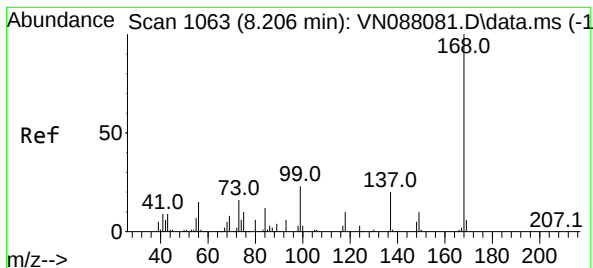

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.206 min Scan# 1103
Delta R.T. 0.000 min
Lab File: VN088244.D
Acq: 11 Nov 2025 10:26




Instrument :
MSVOA_N
ClientSampleId :
VN1111MBL01


Tgt Ion:168 Resp: 202654
Ion Ratio Lower Upper
168 100
99 72.3 57.2 85.8

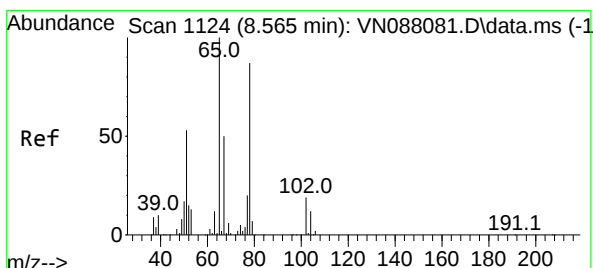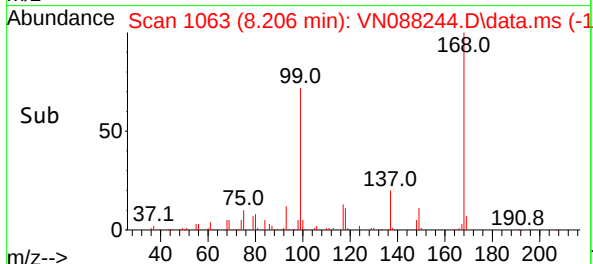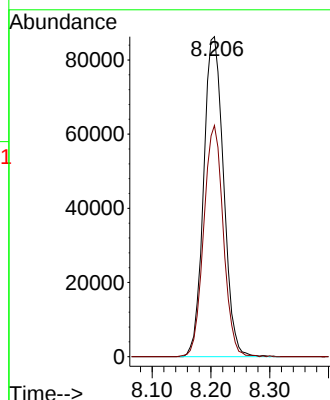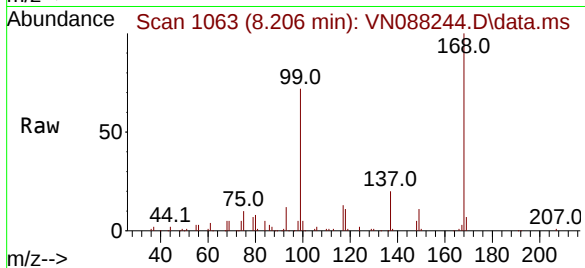

#33
1,2-Dichloroethane-d4
Concen: 61.029 ug/l
RT: 8.559 min Scan# 1123
Delta R.T. -0.000 min
Lab File: VN088244.D
Acq: 11 Nov 2025 10:26

Tgt Ion: 65 Resp: 213865
Ion Ratio Lower Upper
65 100
67 51.6 0.0 100.0


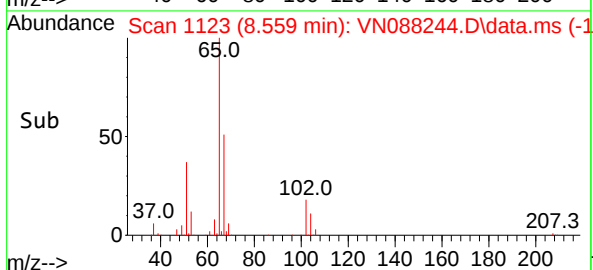
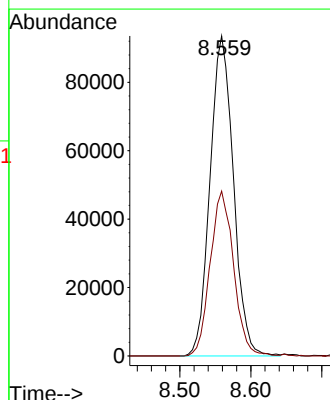
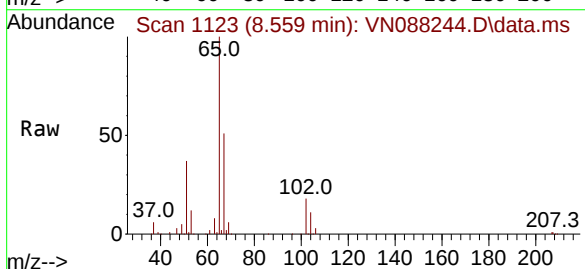


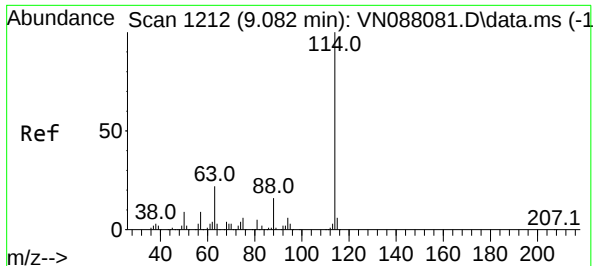

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.082 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN088244.D
Acq: 11 Nov 2025 10:26




Instrument :
MSVOA_N
ClientSampleId :
VN1111MBL01


Tgt Ion:114 Resp: 454207
Ion Ratio Lower Upper
114 100
63 22.7 0.0 45.2
88 16.8 0.0 33.4

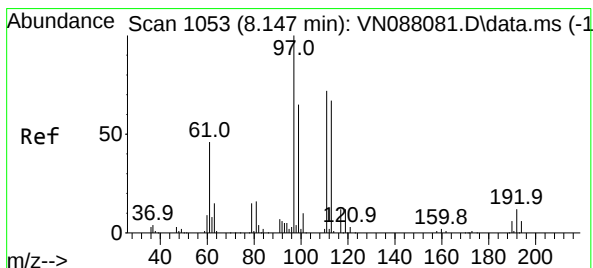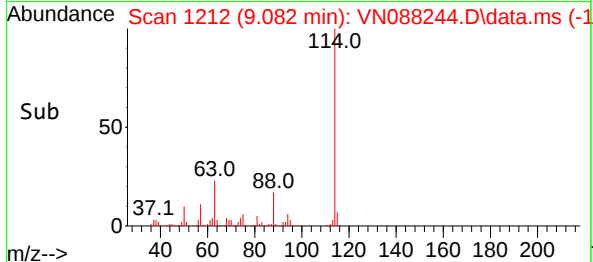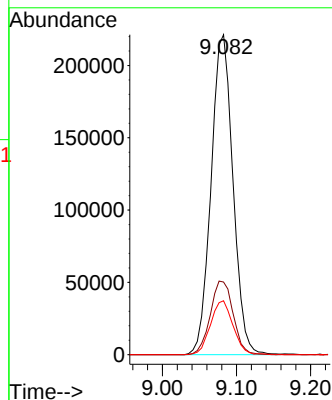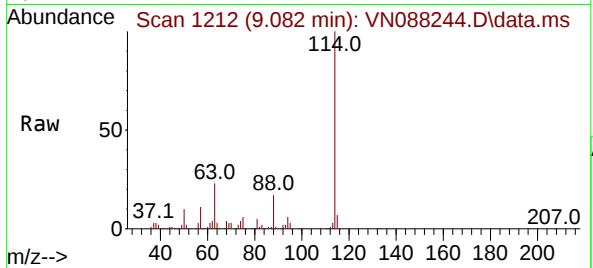

#35
Dibromofluoromethane
Concen: 53.772 ug/l
RT: 8.147 min Scan# 1053
Delta R.T. -0.006 min
Lab File: VN088244.D
Acq: 11 Nov 2025 10:26

Tgt Ion:113 Resp: 164080
Ion Ratio Lower Upper
113 100
111 103.2 82.8 124.2
192 15.9 12.8 19.2


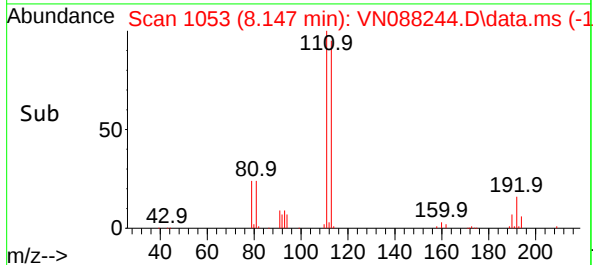
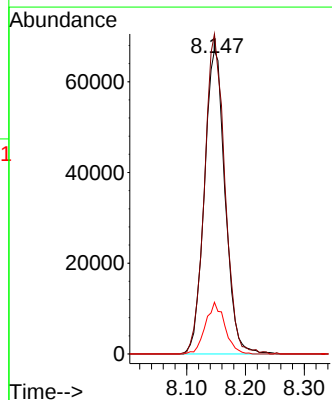
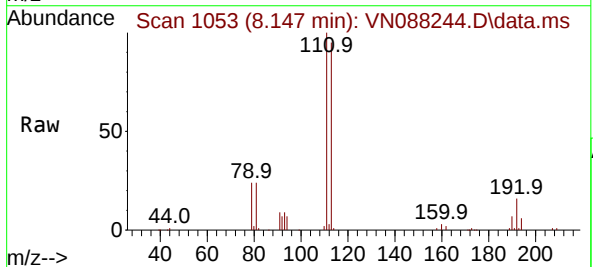


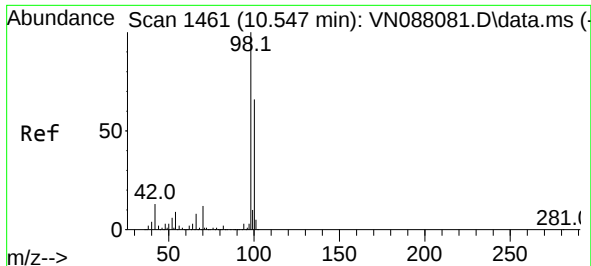

#50
Toluene-d8
Concen: 51.205 ug/l
RT: 10.541 min Scan# 1461
Delta R.T. -0.006 min
Lab File: VN088244.D
Acq: 11 Nov 2025 10:26




Instrument :
MSVOA_N
ClientSampleId :
VN1111MBL01


Tgt Ion: 98 Resp: 602047
Ion Ratio Lower Upper
98 100
100 63.7 52.8 79.2

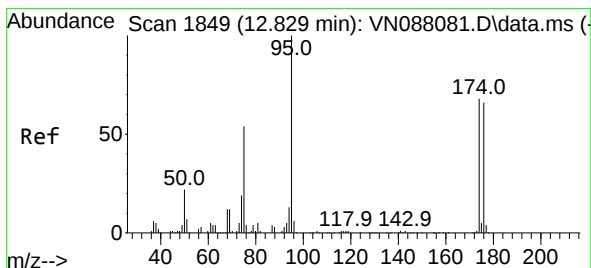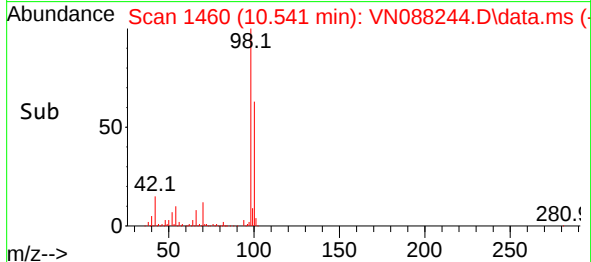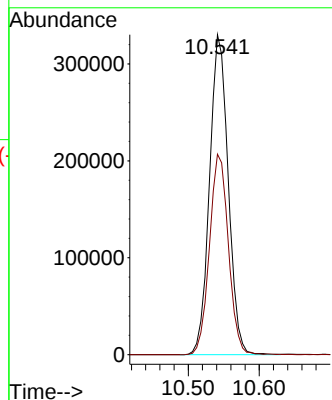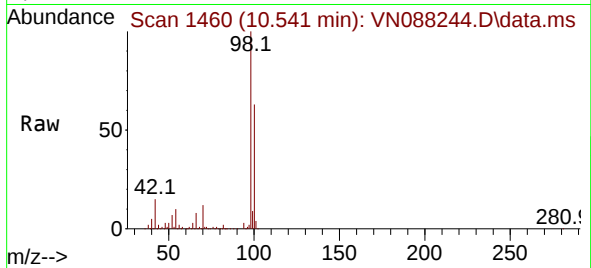

#62
4-Bromofluorobenzene
Concen: 53.560 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.006 min
Lab File: VN088244.D
Acq: 11 Nov 2025 10:26

Tgt Ion: 95 Resp: 222397
Ion Ratio Lower Upper
95 100
174 67.7 0.0 138.4
176 64.9 0.0 132.6


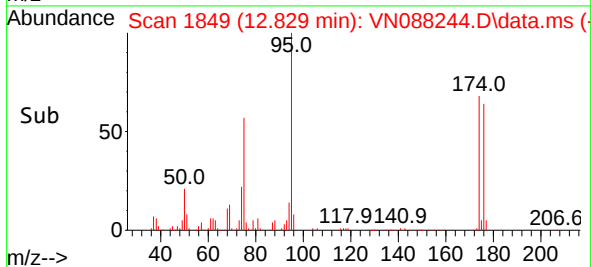
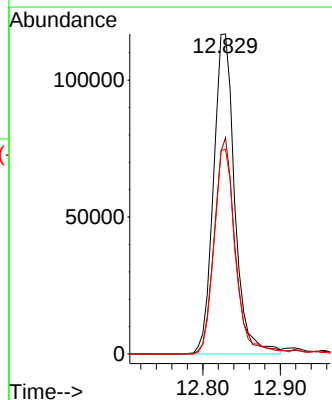
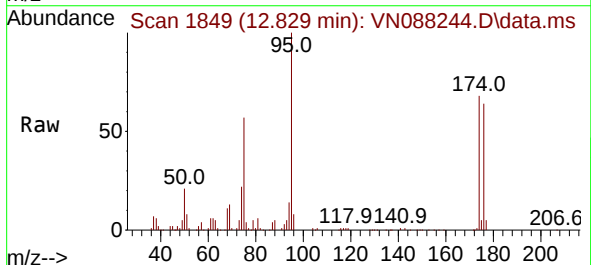


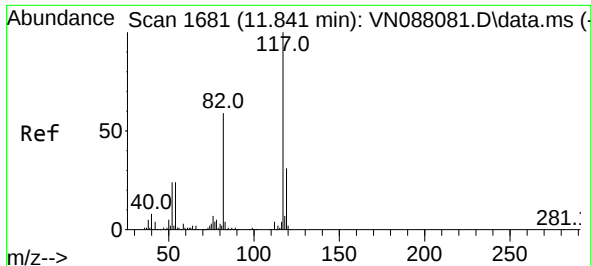

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.841 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN088244.D
Acq: 11 Nov 2025 10:26

Instrument :
MSVOA_N
ClientSampleId :
VN1111MBL01

Tgt Ion:117 Resp: 437617
Ion Ratio Lower Upper
117 100
82 61.9 47.4 71.2
119 32.8 24.3 36.5

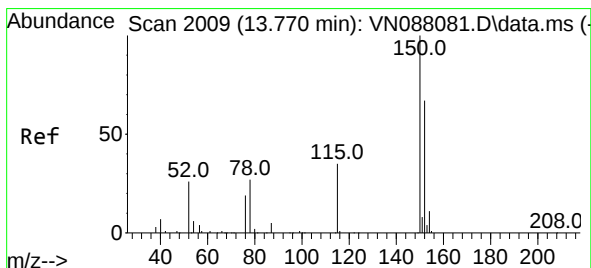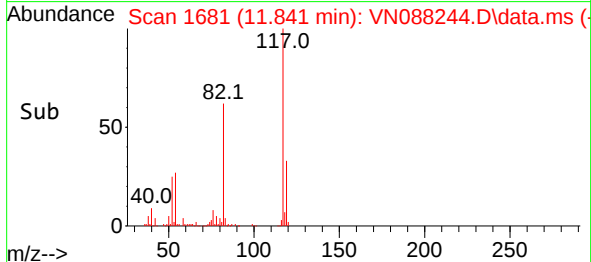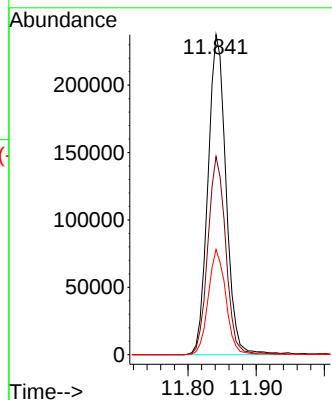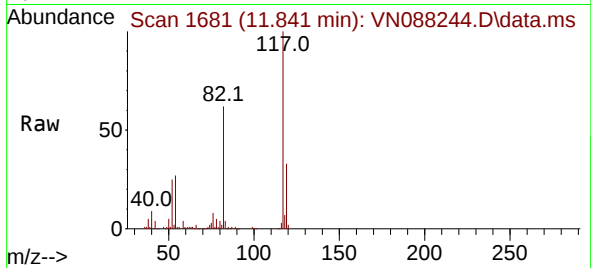

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.770 min Scan# 2009
Delta R.T. 0.006 min
Lab File: VN088244.D
Acq: 11 Nov 2025 10:26

Tgt Ion:152 Resp: 213641
Ion Ratio Lower Upper
152 100
115 63.0 32.3 96.8
150 156.4 0.0 351.0

