

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN111218\
 Data File : VN052274.D
 Acq On : 12 Nov 2018 20:31
 Operator : MD\SY
 Sample : PB114678ZHE#18
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 25 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 PB114678ZHE#18

Quant Time: Nov 13 01:36:37 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110918W.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 12 00:34:27 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	322066	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	546253	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	467952	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	163053	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	216608	49.18	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.36%	
35) Dibromofluoromethane	7.59	113	170909	48.30	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.60%	
50) Toluene-d8	10.09	98	680932	49.17	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.34%	
62) 4-Bromofluorobenzene	12.40	95	196947	43.98	ug/l	0.00
Spiked Amount 50.000			Recovery	=	87.96%	
Target Compounds						
20) Methylene Chloride	4.55	84	5717	1.424	ug/l	87
43) Isopropyl Acetate	8.17	43	25057	3.467	ug/l #	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN111218\
Data File : VN052274.D
Acq On : 12 Nov 2018 20:31
Operator : MD\SY
Sample : PB114678ZHE#18
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 25 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
PB114678ZHE#18

Quant Time: Nov 13 01:36:37 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N110918W.M
Quant Title : SW846 8260
QLast Update : Mon Nov 12 00:34:27 2018
Response via : Initial Calibration

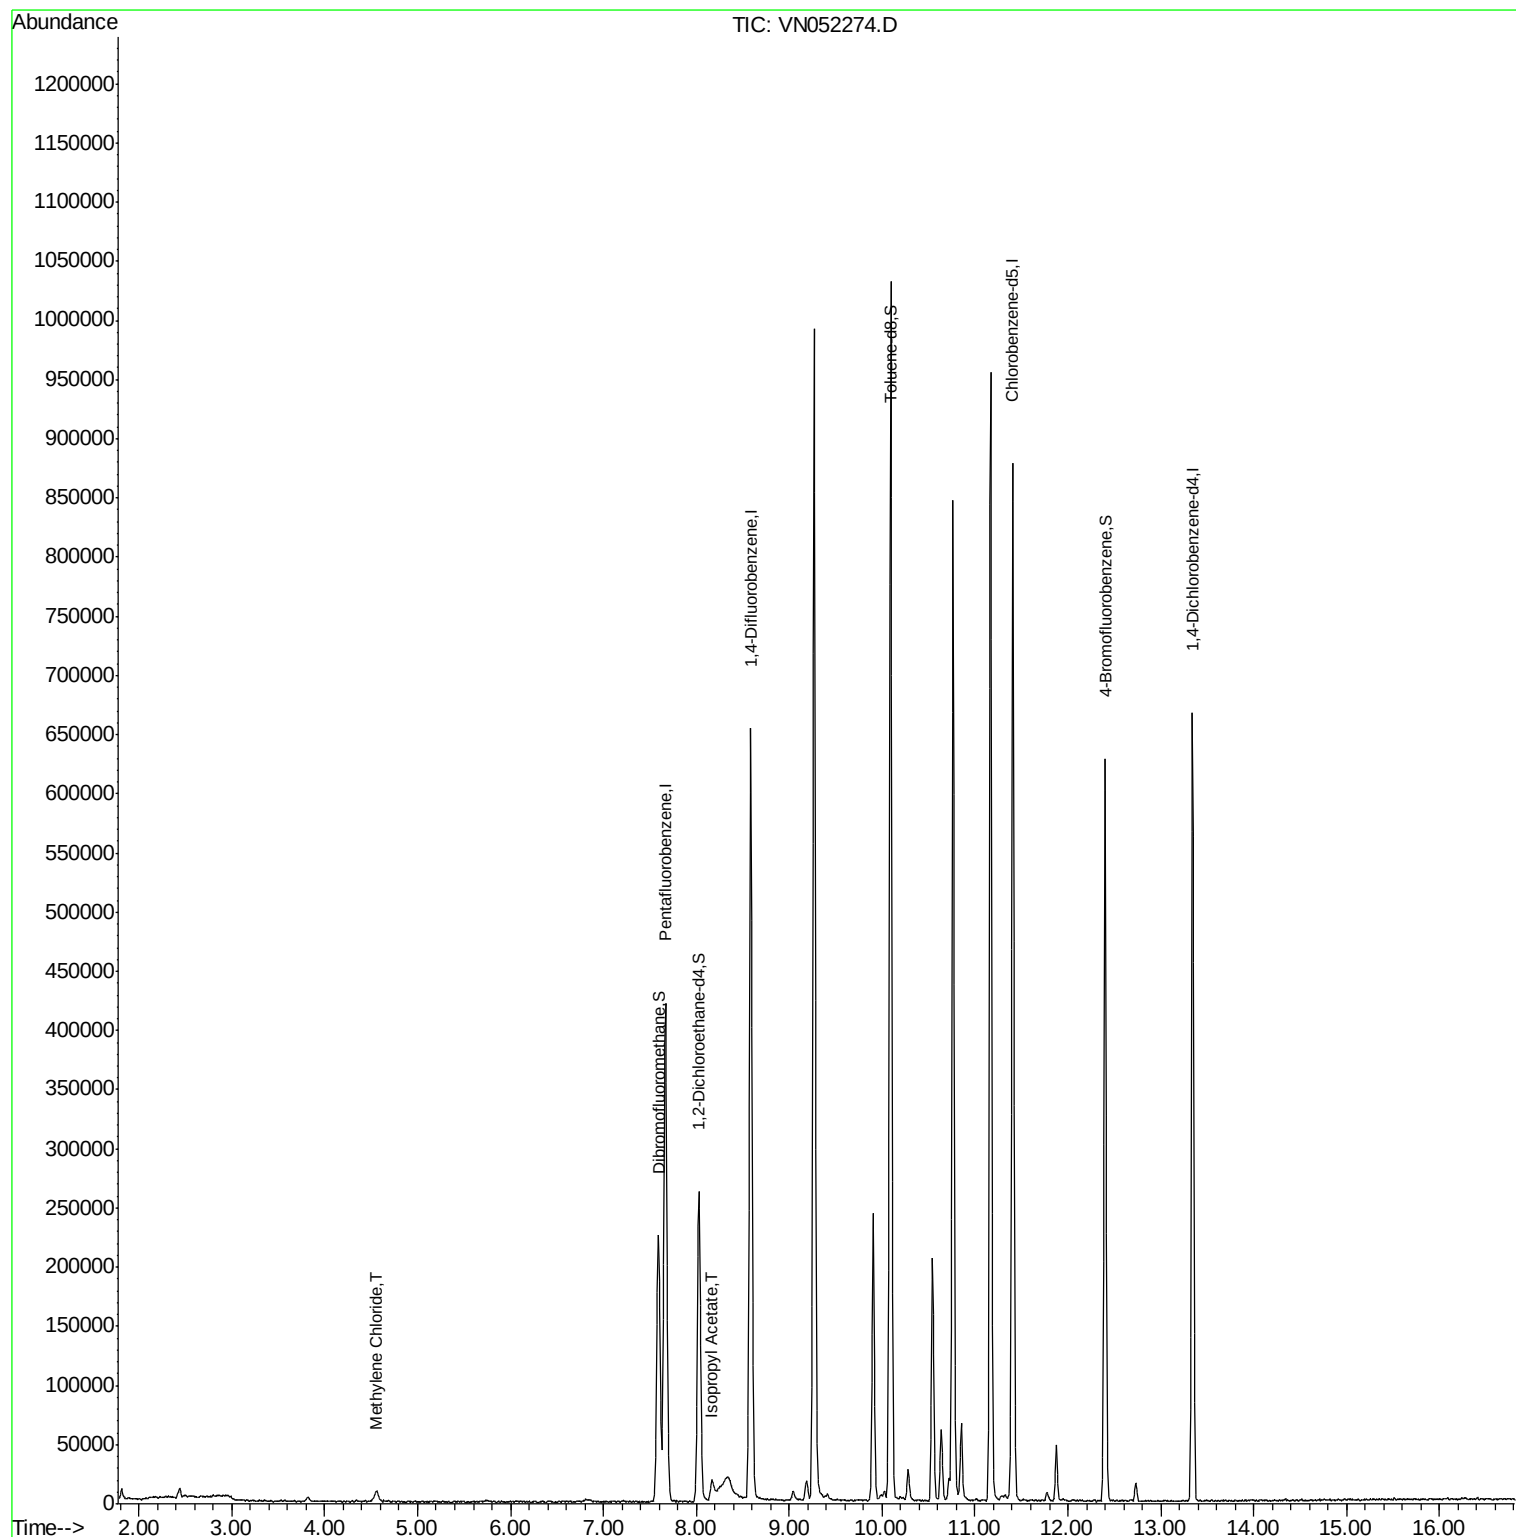

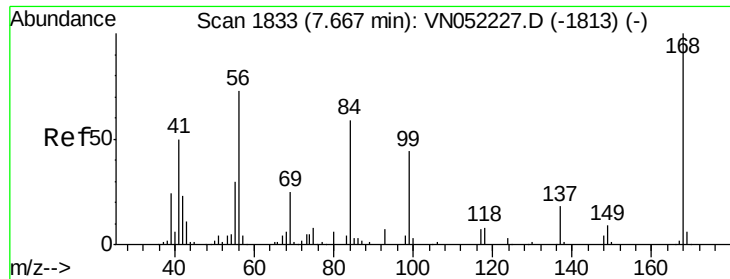

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.00 min

Lab File: VN052274.D

Acq: 12 Nov 2018 20:31

Instrument :

MSVOA_N

ClientSampleId :


PB114678ZHE#18

Tot Ion:168 Resp: 322066

Ion Ratio Lower Upper

168 100

99 58.5 44.7 67.1

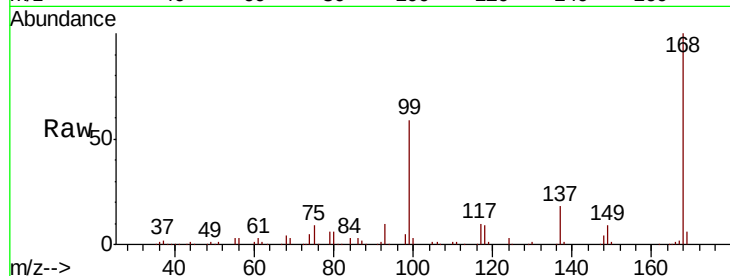

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.67

150000



100000

50000

0

Time-->

7.60 7.70 7.80

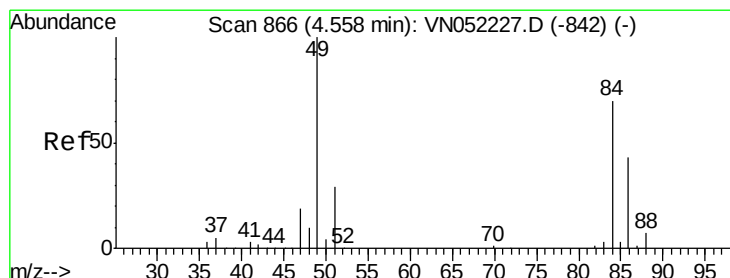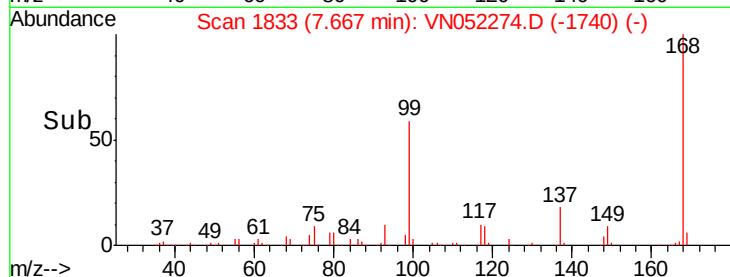

#20

Methylene Chloride

Concen: 1.424 ug/l

RT: 4.55 min Scan# 865

Delta R.T. -0.00 min

Lab File: VN052274.D

Acq: 12 Nov 2018 20:31

Tgt Ion: 84 Resp: 5717


Ion Ratio Lower Upper

84 100

49 120.5 114.8 172.2

51 40.7 33.1 49.7

86 55.3 49.7 74.5

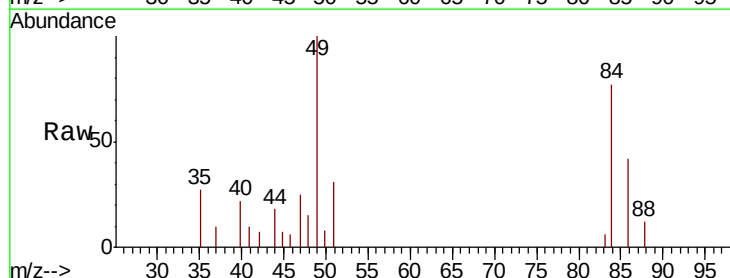

Abundance Ion 83.90 (83.60 to 84.60): VNO

Ion 48.90 (48.60 to 49.60): VNO

Ion 50.90 (50.60 to 51.60): VNO

Ion 85.90 (85.60 to 86.60): VNO

4000

3000


2000


1000

0

Time-->

4.45 4.50 4.55 4.60 4.65




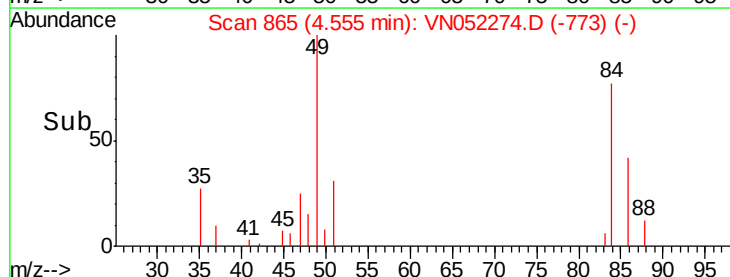


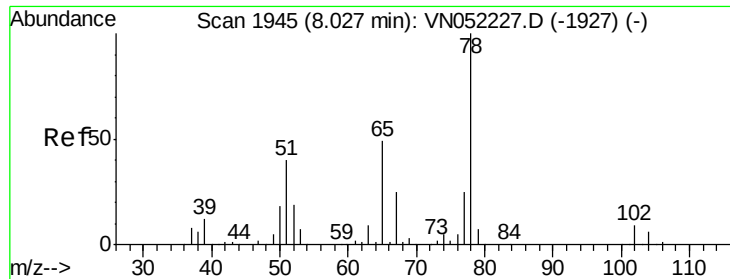

#33
 1,2-Dichloroethane-d4
 Concen: Below ug/l
 RT: 8.03 min Scan# 1945
 Delta R.T. 0.00 min
 Lab File: VN052274.D
 Acq: 12 Nov 2018 20:31




Instrument :
 MSVOA_N
 ClientSampleId :
 PB114678ZHE#18


Tot Ion: 65 Resp: 216608
 Ion Ratio Lower Upper
 65 100
 67 52.2 0.0 106.6

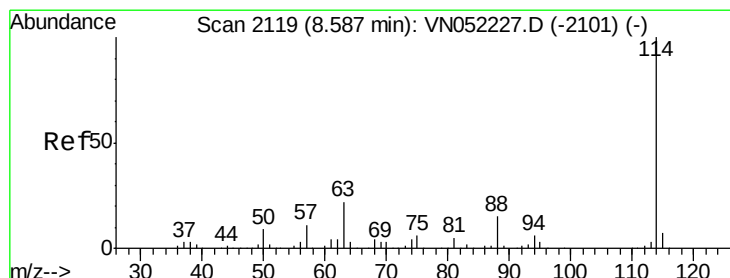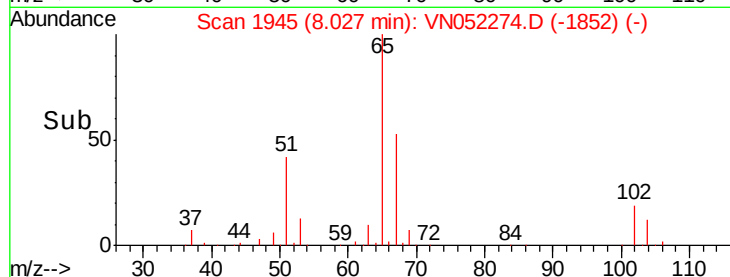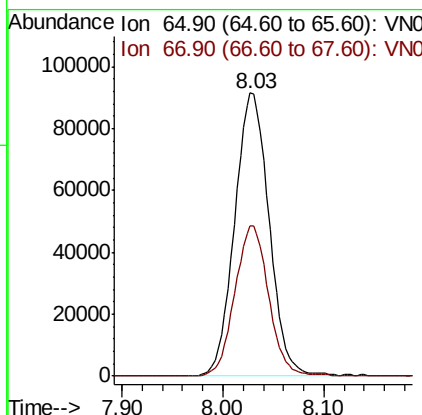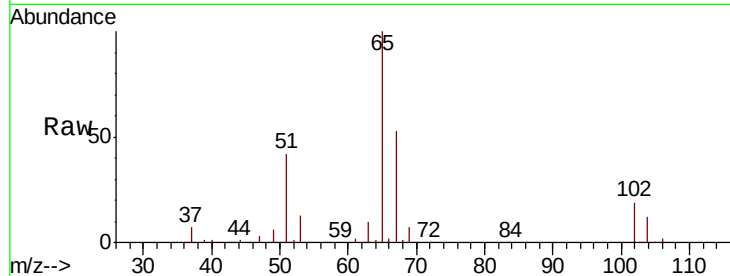

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN052274.D
 Acq: 12 Nov 2018 20:31

Tgt Ion: 114 Resp: 546253
 Ion Ratio Lower Upper
 114 100
 63 22.0 0.0 43.4
 88 15.5 0.0 30.2


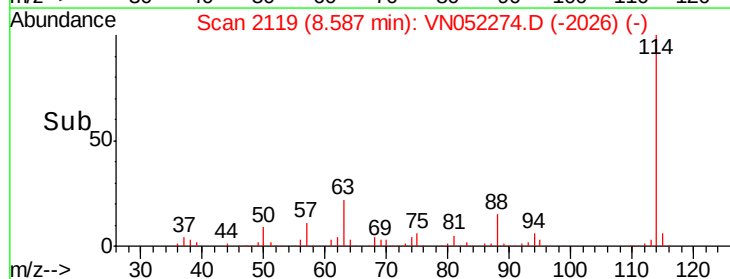
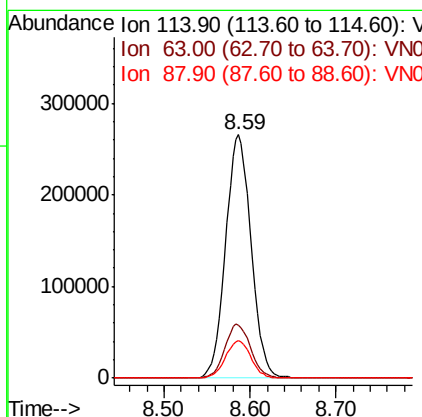
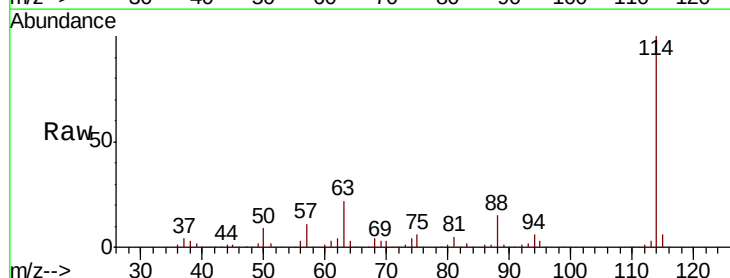


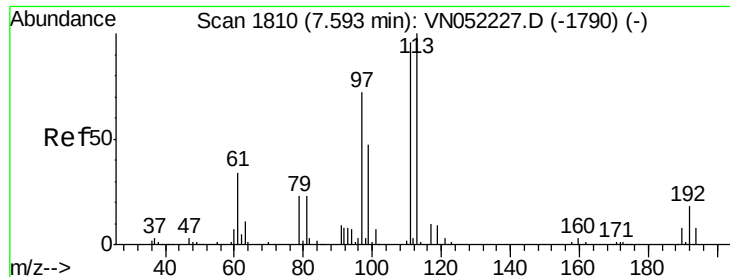

#35
 Dibromofluoromethane
 Concen: 50.000 ug/l
 RT: 7.59 min Scan# 1810
 Delta R.T. 0.00 min
 Lab File: VN052274.D
 Acq: 12 Nov 2018 20:31




Instrument :
 MSVOA_N
 ClientSampleId :
 PB114678ZHE#18


Tot Ion	Ratio	Lower	Upper
113	100		
111	102.7	80.2	120.4
192	17.2	14.1	21.1

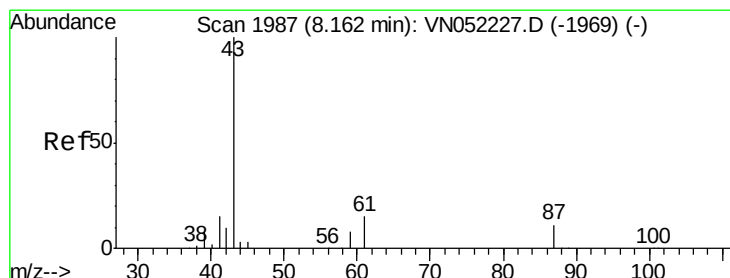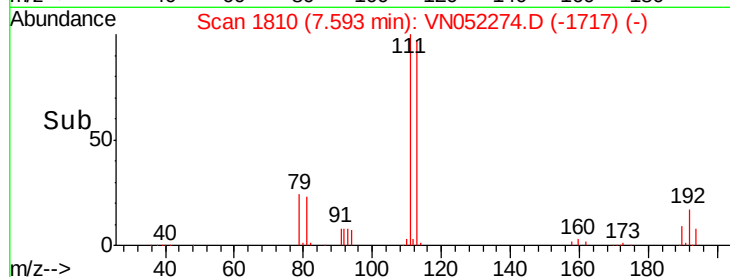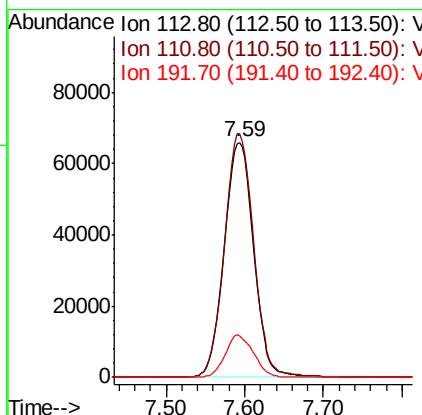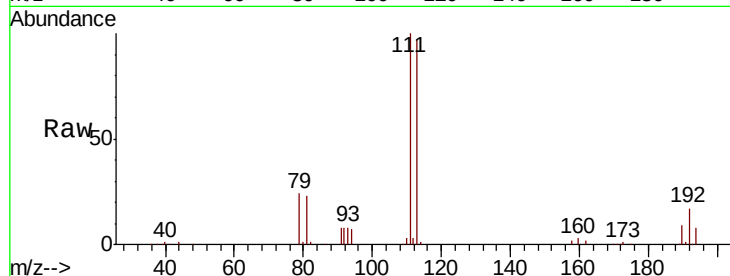

#43
 Isopropyl Acetate
 Concen: 3.467 ug/l
 RT: 8.17 min Scan# 1988
 Delta R.T. 0.00 min
 Lab File: VN052274.D
 Acq: 12 Nov 2018 20:31

Tgt Ion	Ratio	Lower	Upper
43	100		
61	12.8	14.2	21.4#
87	8.2	8.4	12.6#

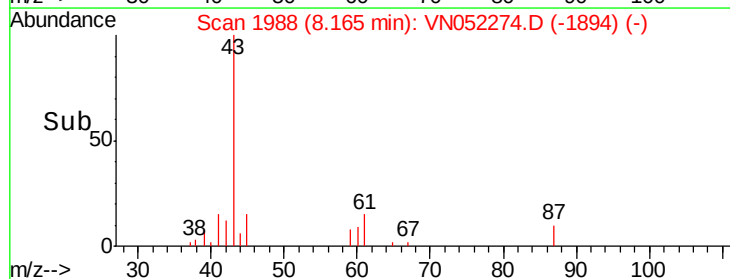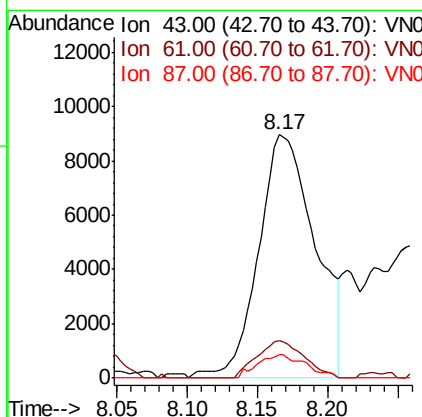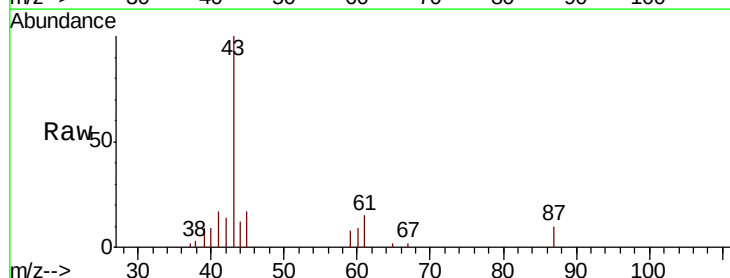


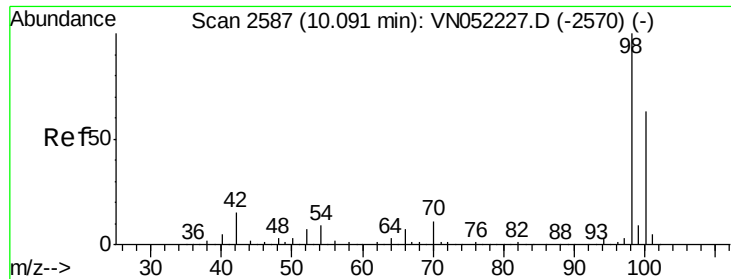


#50
Toluene-d8
Concen: N.D. ug/l
RT: 10.09 min Scan# 2587
Delta R.T. 0.00 min
Lab File: VN052274.D
Acq: 12 Nov 2018 20:31

Instrument :
MSVOA_N
ClientSampleId :
PB114678ZHE#18



Tot Ion: 98 Resp: 680932
Ion Ratio Lower Upper
98 100
100 62.3 50.2 75.2

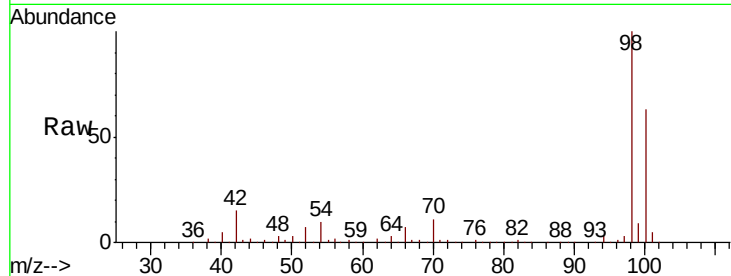

Abundance Ion 98.00 (97.70 to 98.70): VN0
Ion 100.00 (99.70 to 100.70): VN

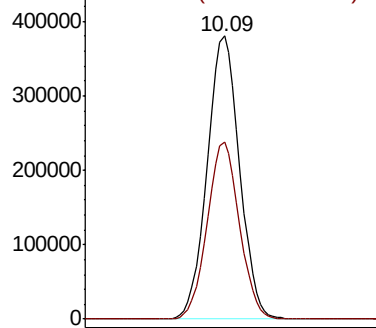


Time-->

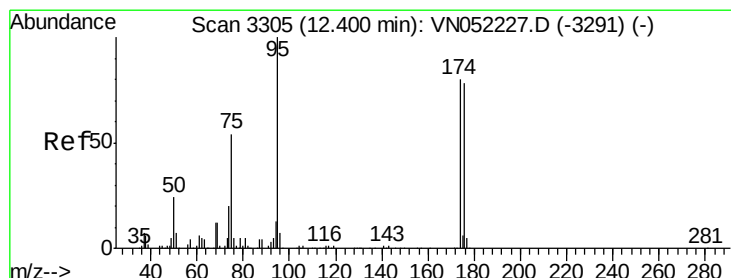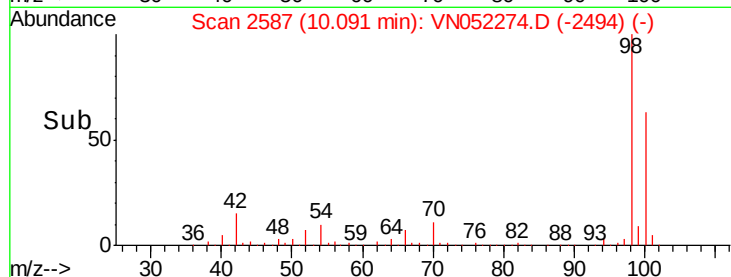


#62
4-Bromofluorobenzene
Concen: N.D. ug/l
RT: 12.40 min Scan# 3305
Delta R.T. 0.00 min
Lab File: VN052274.D
Acq: 12 Nov 2018 20:31


Tgt Ion: 95 Resp: 196947
Ion Ratio Lower Upper
95 100
174 78.0 0.0 159.4
176 74.2 0.0 157.8

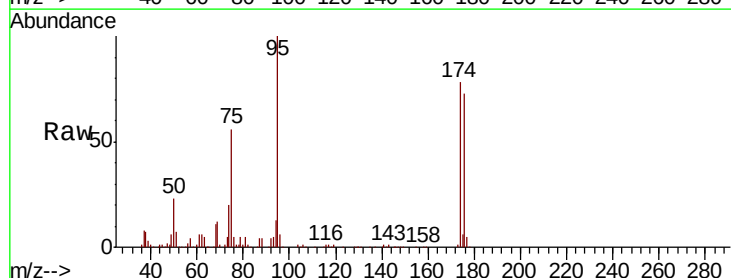


Abundance Ion 94.90 (94.60 to 95.60): VN0
Ion 173.80 (173.50 to 174.50): V
Ion 175.80 (175.50 to 176.50): V

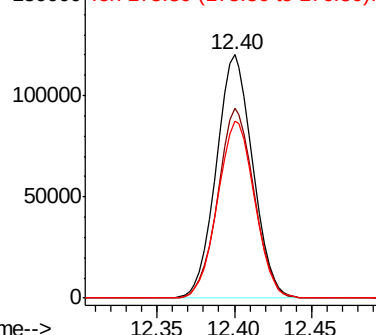

Time-->

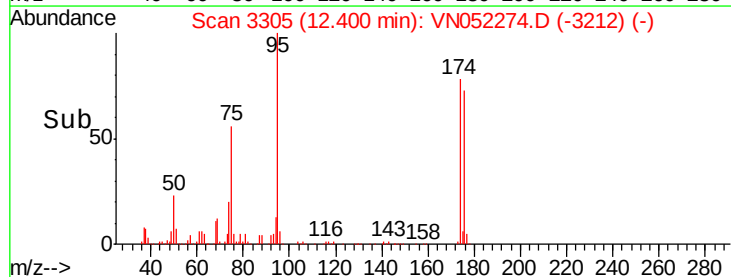


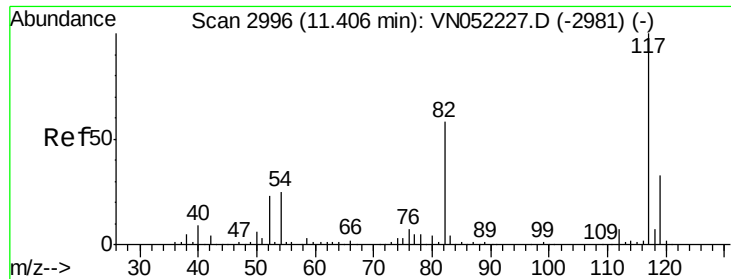




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. 0.00 min
Lab File: VN052274.D
Acq: 12 Nov 2018 20:31

Instrument :
MSVOA_N
ClientSampleId :
PB114678ZHE#18

Tot Ion:117 Resp: 467952
Ion Ratio Lower Upper
117 100
82 57.3 46.2 69.2
119 31.4 26.2 39.4

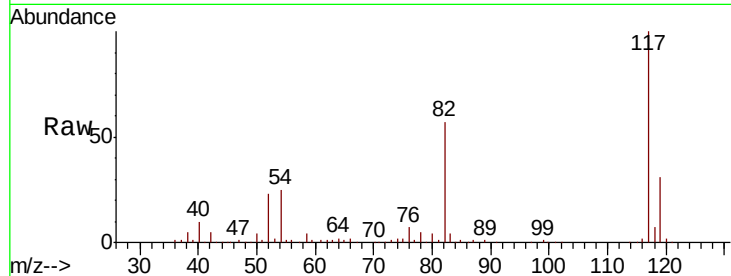


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

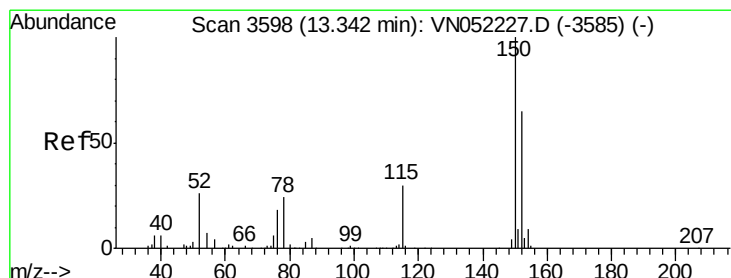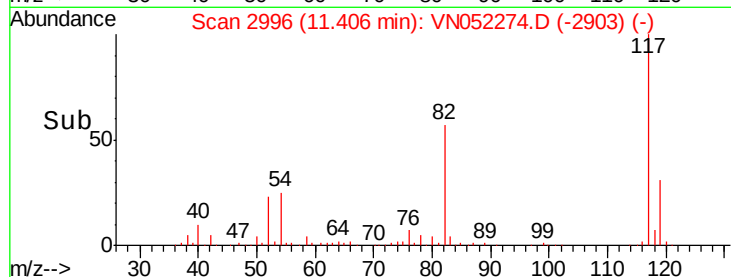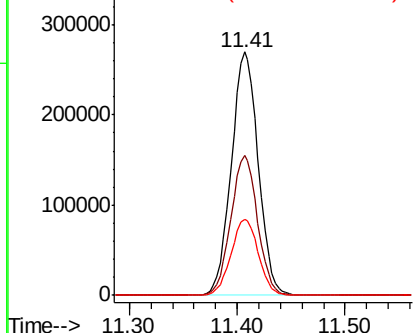

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. 0.00 min
Lab File: VN052274.D
Acq: 12 Nov 2018 20:31

Tgt Ion:152 Resp: 163053
Ion Ratio Lower Upper
152 100
115 60.4 29.8 89.5
150 157.6 0.0 350.2

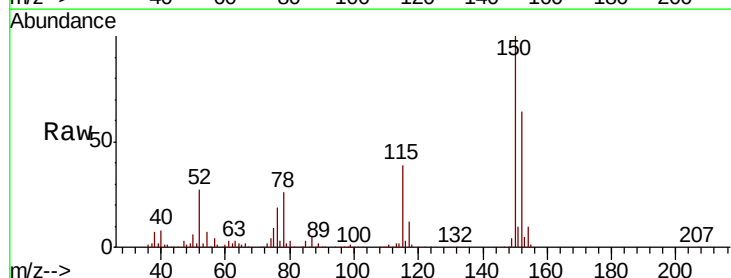

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

